

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031920\
 Data File : PS009370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2020 19:22
 Operator : DD\AJ
 Sample : L1949-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 03:47:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	208.0E6	190.8E6	376.086	347.368
Target Compounds							
1) T	Dalapon	3.007	2.589	21740712	78143174	27.879	99.247 #
2) T	3,5-DICHL...	0.000	6.109	0	79387116	N.D.	97.610
3) T	4-Nitroph...	7.141	0.000	9778207	0	40.962	N.D. #
7) T	MCPA	7.734	7.400	7870794	48117840	2.584	17.831 #
8) T	DICHLORPROP	0.000	7.752	0	29636841	N.D.	53.417
10) T	Pentachlo...	8.668	8.455	10447502	12059615	1.486	1.589
12) T	2,4,5-T	9.448	0.000	45560293	0	17.910	N.D. #
14) T	DINOSEB	11.187	10.047	29250824	36373109	14.310	16.560
15) T	Picloram	0.000	11.020	0	10239679	N.D.	2.515
16) T	DCPA	11.497	10.972	3031357	11637516	<MDL	3.005 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031920\
Data File : PS009370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2020 19:22
Operator : DD\AJ
Sample : L1949-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 03:47:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

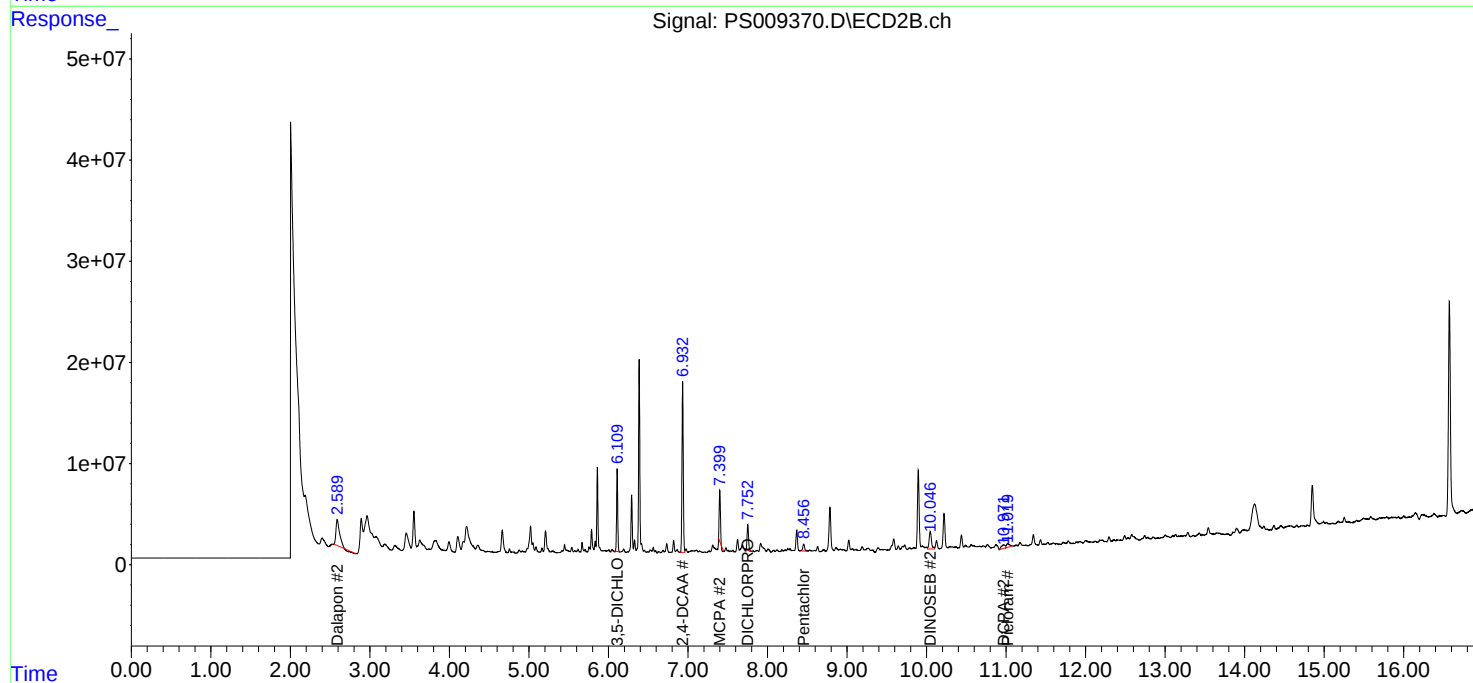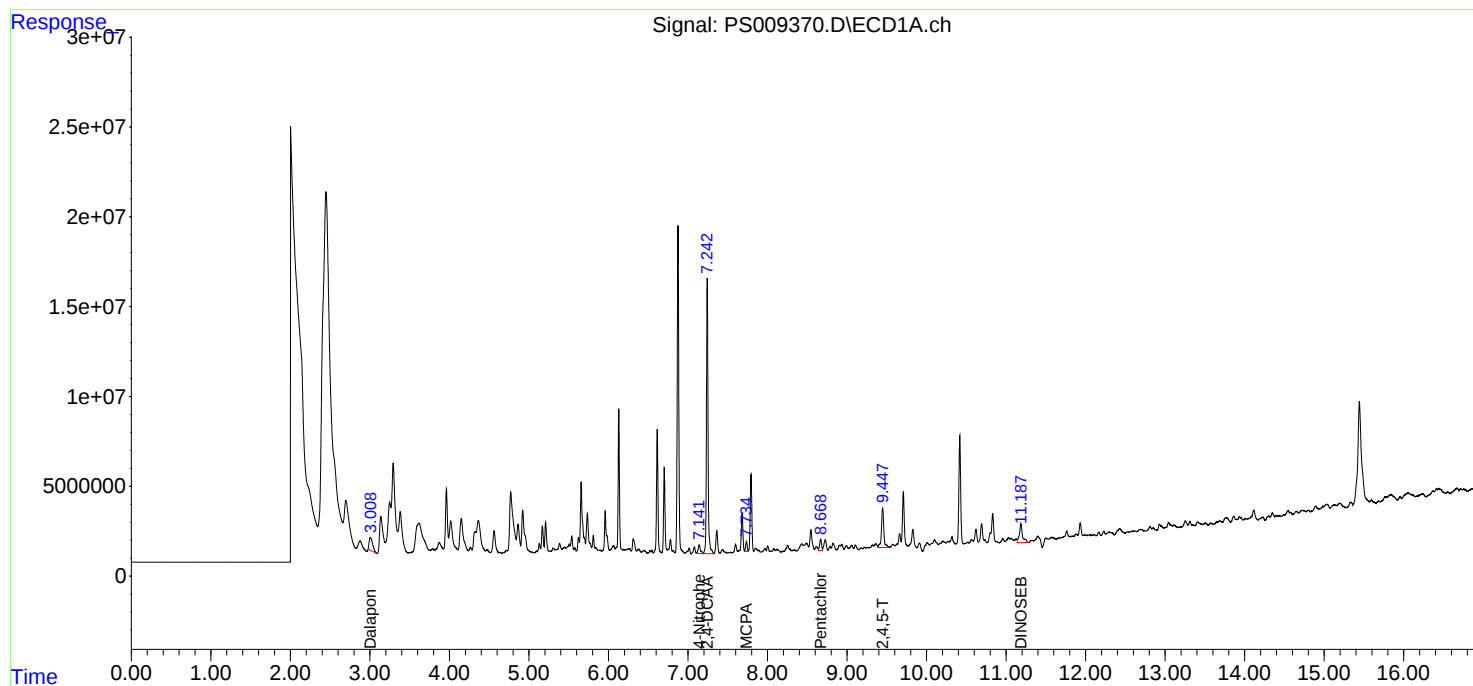


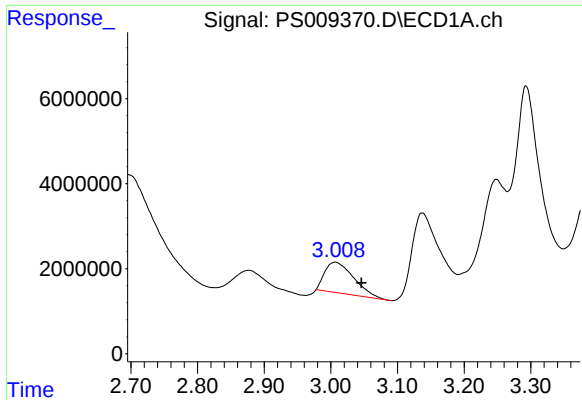

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 21740712
Conc: 27.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

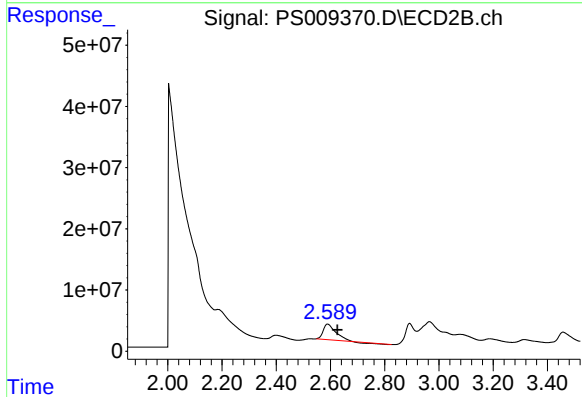


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 78143174
Conc: 99.25 ng/ml

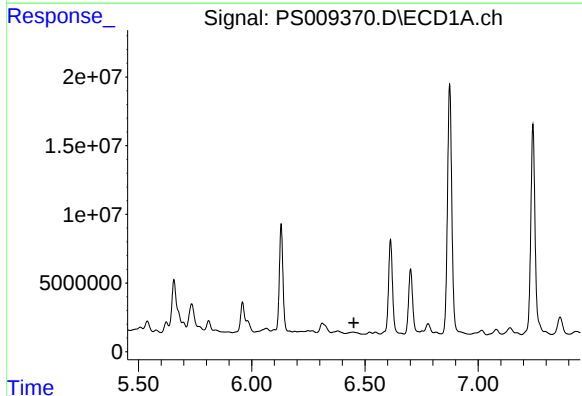


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

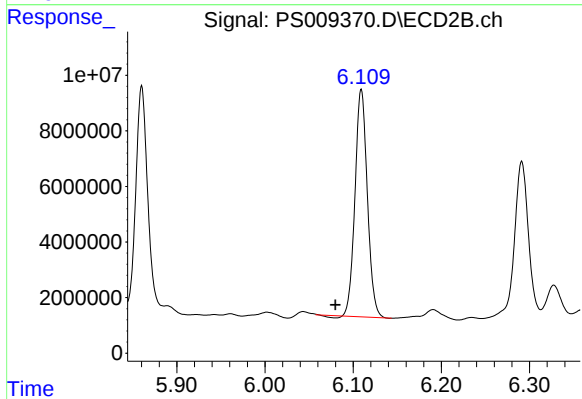

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.030 min
Response: 79387116
Conc: 97.61 ng/ml

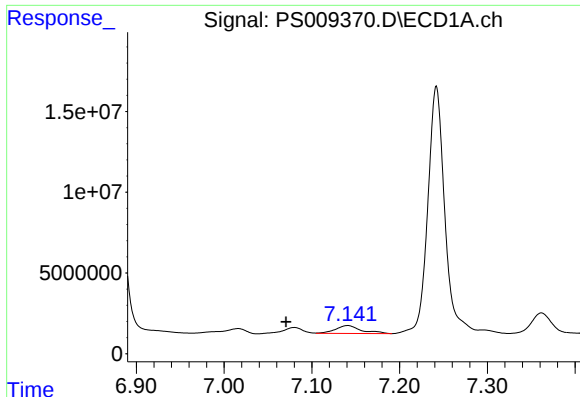

#3 4-Nitrophenol


R.T.: 7.141 min
Delta R.T.: 0.070 min
Response: 9778207
Conc: 40.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

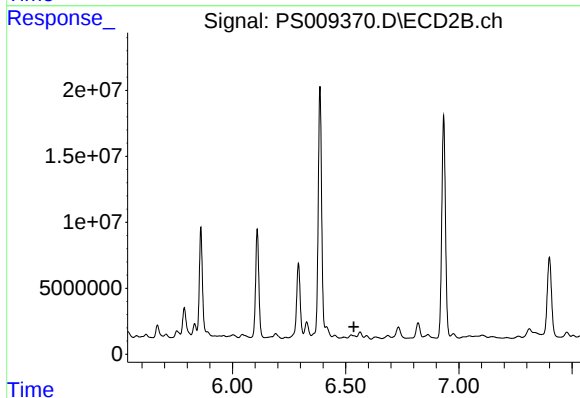


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.536 min
Response: 0
Conc: N.D.

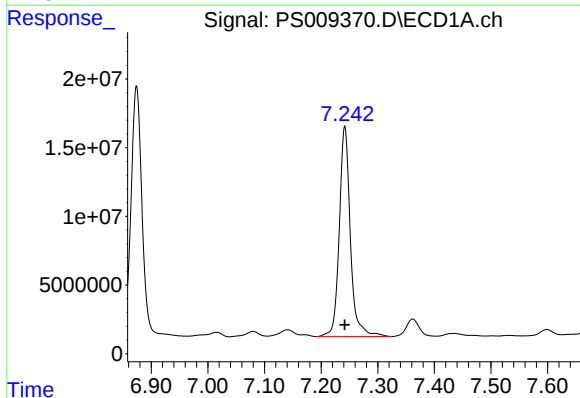


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 208039650
Conc: 376.09 ng/ml

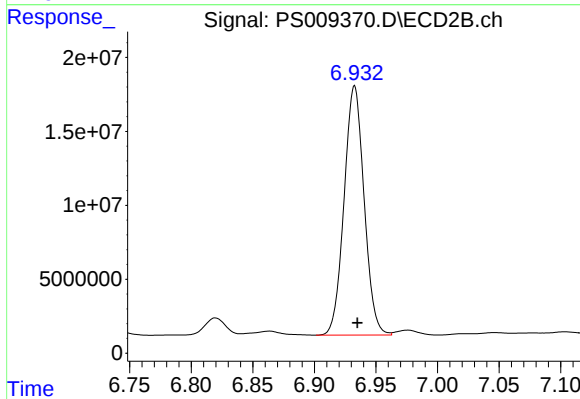

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 190773899
Conc: 347.37 ng/ml

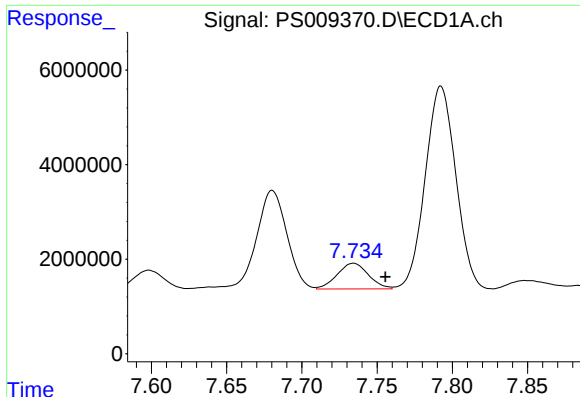

#7 MCPA


R.T.: 7.734 min
Delta R.T.: -0.021 min
Response: 7870794
Conc: 2.58 ug/ml

Instrument :
ECD_S
ClientSampleId :

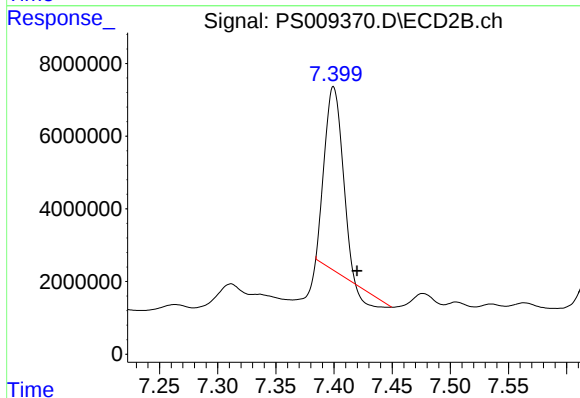


#7 MCPA

R.T.: 7.400 min
Delta R.T.: -0.020 min
Response: 48117840
Conc: 17.83 ug/ml

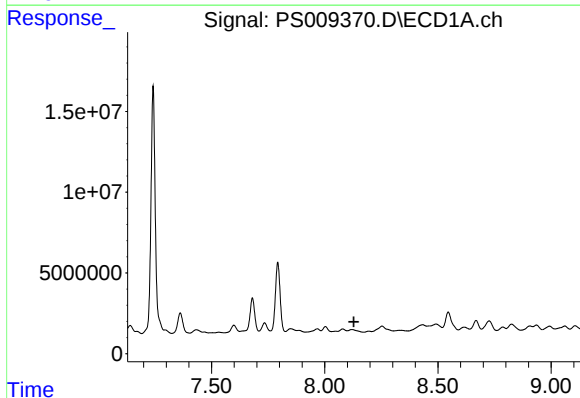


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

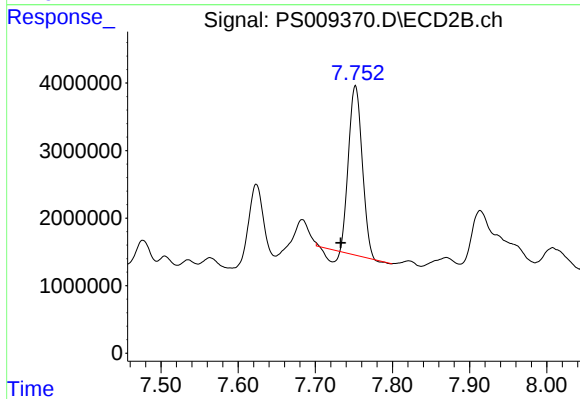

#8 DICHLORPROP


R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 29636841
Conc: 53.42 ng/ml

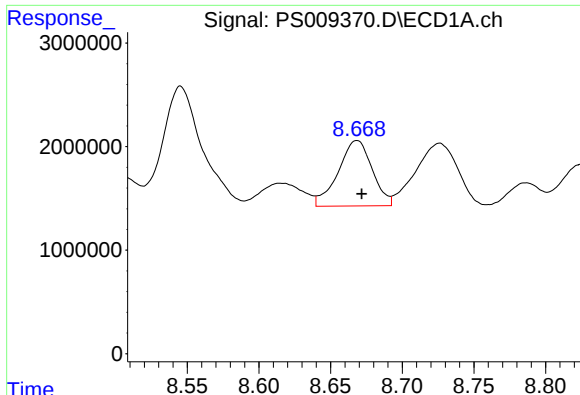

#10 Pentachlorophenol


R.T.: 8.668 min
Delta R.T.: -0.004 min
Response: 10447502
Conc: 1.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

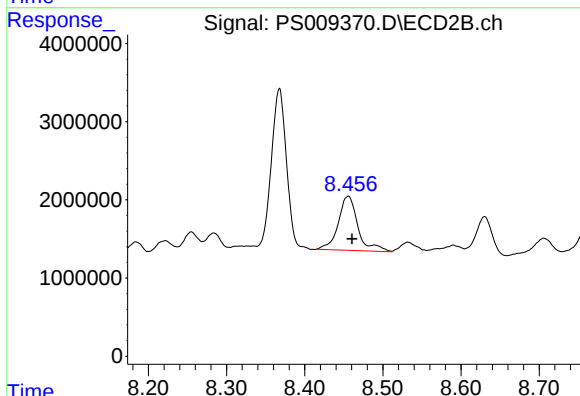


#10 Pentachlorophenol

R.T.: 8.455 min
Delta R.T.: -0.005 min
Response: 12059615
Conc: 1.59 ng/ml

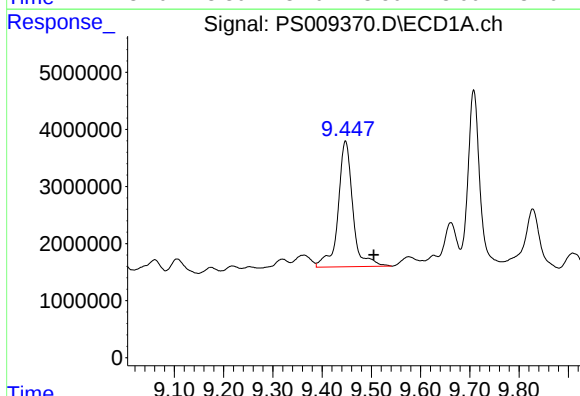


#12 2,4,5-T

R.T.: 9.448 min
Delta R.T.: -0.057 min
Response: 45560293
Conc: 17.91 ng/ml

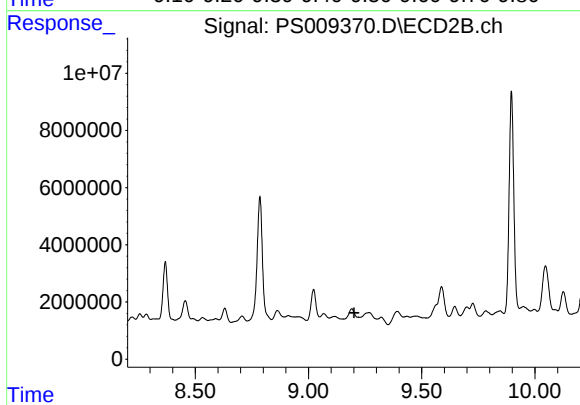

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

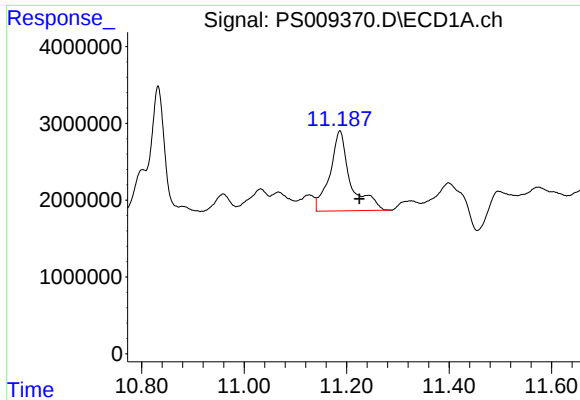

#14 DINOSEB


R.T.: 11.187 min
Delta R.T.: -0.038 min
Response: 29250824
Conc: 14.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

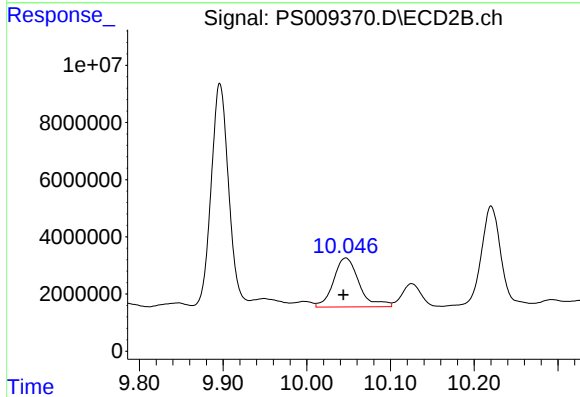


#14 DINOSEB

R.T.: 10.047 min
Delta R.T.: 0.003 min
Response: 36373109
Conc: 16.56 ng/ml

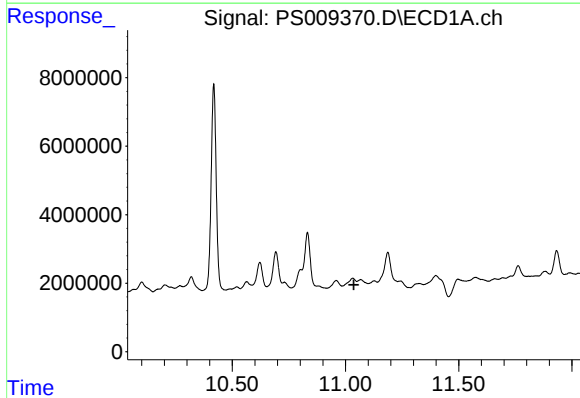


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

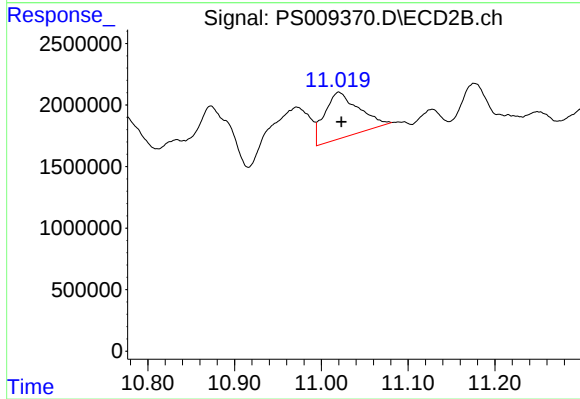

#15 Picloram


R.T.: 11.020 min
Delta R.T.: -0.003 min
Response: 10239679
Conc: 2.51 ng/ml

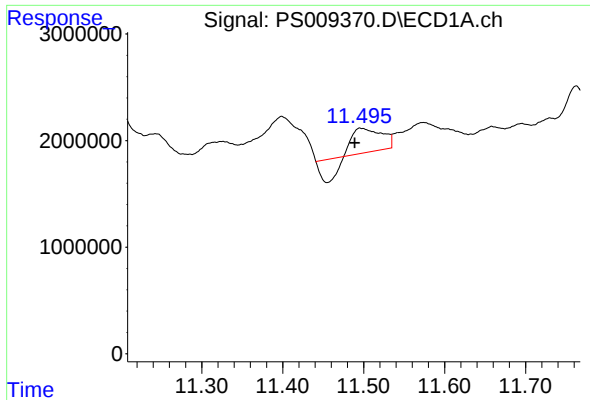

#16 DCPA

R.T.: 11.497 min
Delta R.T.: 0.008 min
Response: 3031357
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

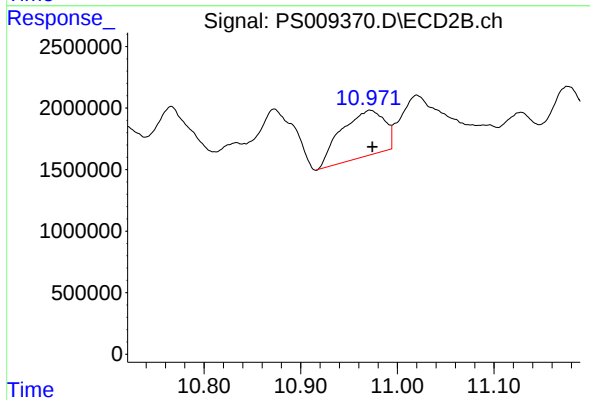

#16 DCPA

R.T.: 10.972 min
Delta R.T.: -0.002 min
Response: 11637516
Conc: 3.00 ng/ml