

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031920\
 Data File : PS009371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2020 19:45
 Operator : DD\AJ
 Sample : L1957-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 03:47:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.932	225.6E6	202.7E6	407.772	369.162
Target Compounds							
1) T	Dalapon	3.006	2.588	21420341	51379678	27.468	65.255 #
2) T	3,5-DICHL...	0.000	6.109	0	73960650	N.D.	90.938
6) T	MCP	7.596	0.000	7381441	0	3.000	N.D. #
7) T	MCPA	7.734	7.399	13822038	47457143	4.538	17.586 #
8) T	DICHLORPROP	0.000	7.751	0	27885700	N.D.	50.261
10) T	Pentachlo...	8.720	0.000	15522131	0	2.208	N.D. #
11) T	2,4,5-TP ...	0.000	8.785	0	31936124	N.D.	10.713
12) T	2,4,5-T	9.450	0.000	24924476	0	9.798	N.D. #
13) T	2,4-DB	0.000	9.645	0	11051744	N.D.	29.113
14) T	DINOSEB	11.186	10.046	28325008	31882252	13.857	14.515
15) T	Picloram	0.000	11.019	0	23941830	N.D.	5.879
16) T	DCPA	0.000	11.019	0	23941830	N.D.	6.182



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031920\
Data File : PS009371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2020 19:45
Operator : DD\AJ
Sample : L1957-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 03:47:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

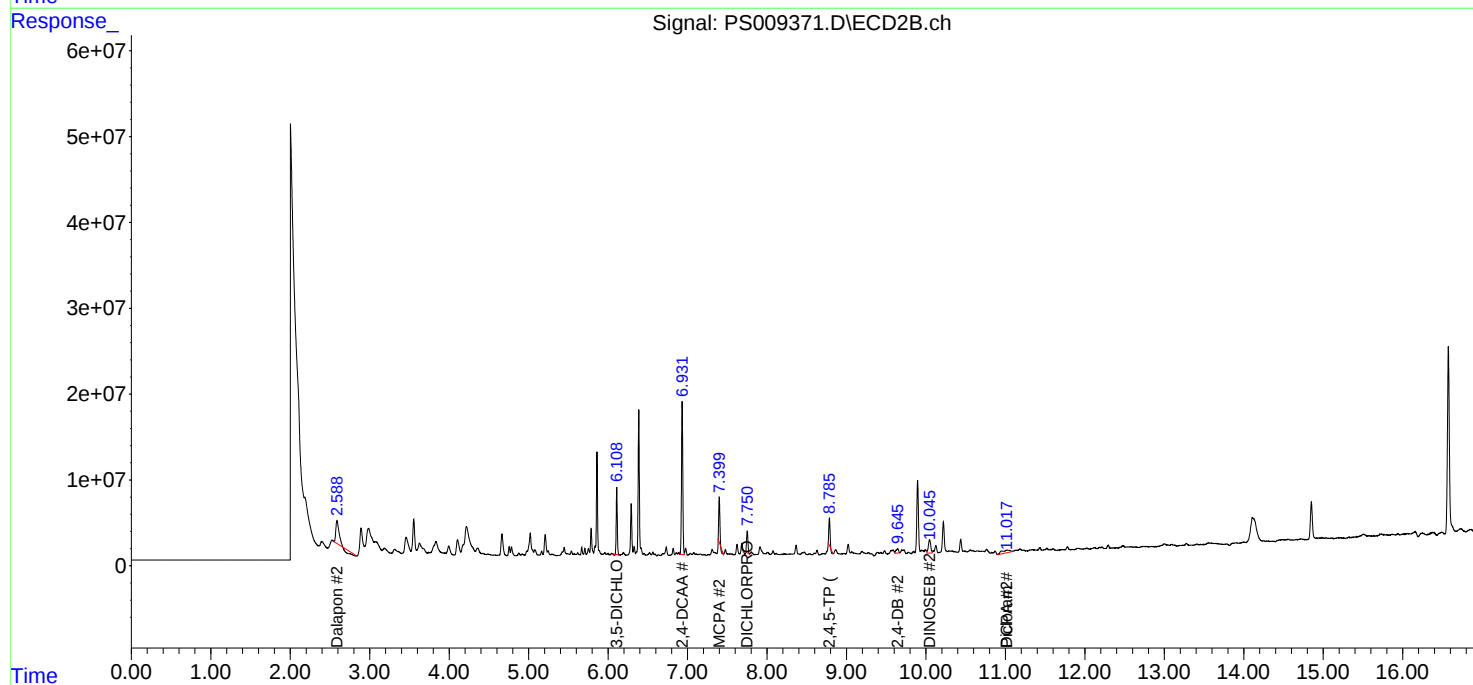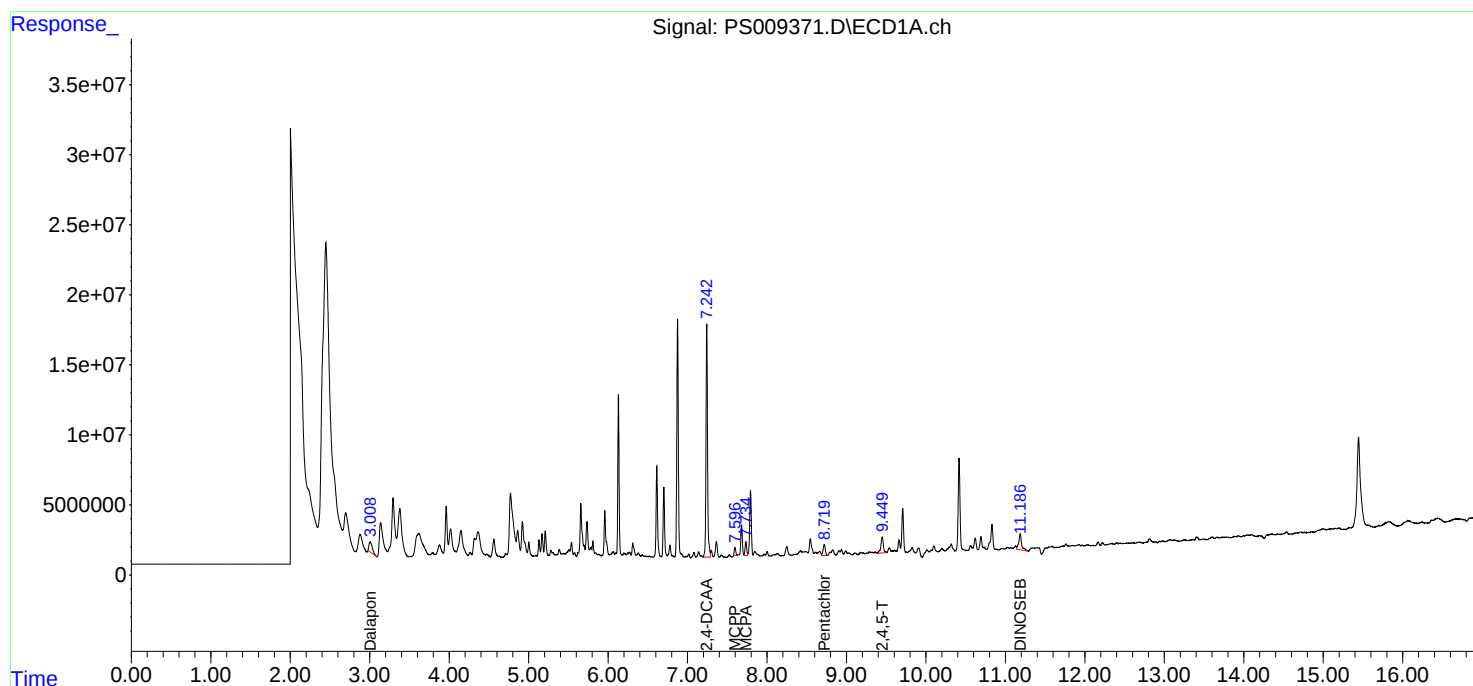


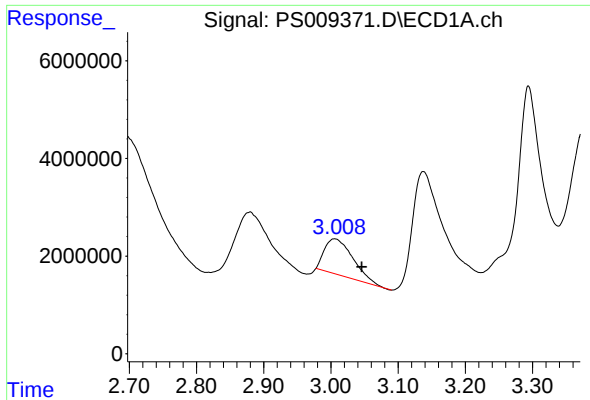

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 21420341
Conc: 27.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

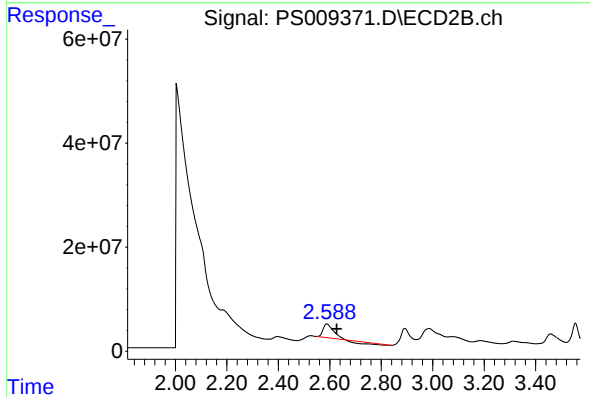


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 51379678
Conc: 65.26 ng/ml

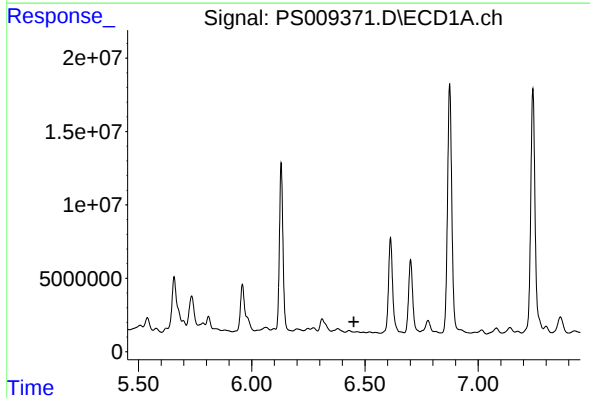


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

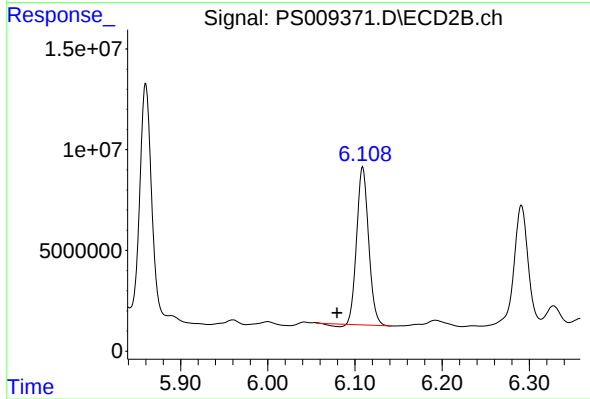

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.029 min
Response: 73960650
Conc: 90.94 ng/ml

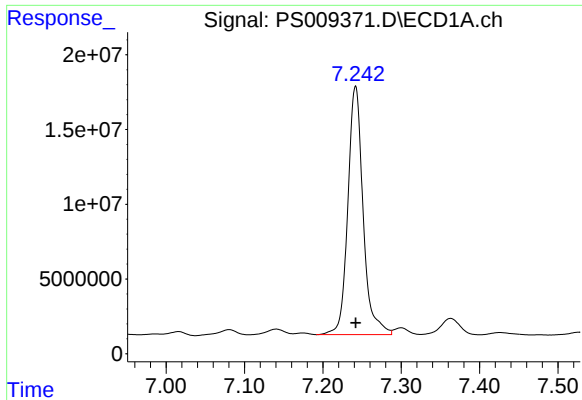

#4 2,4-DCAA


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 225567108
Conc: 407.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

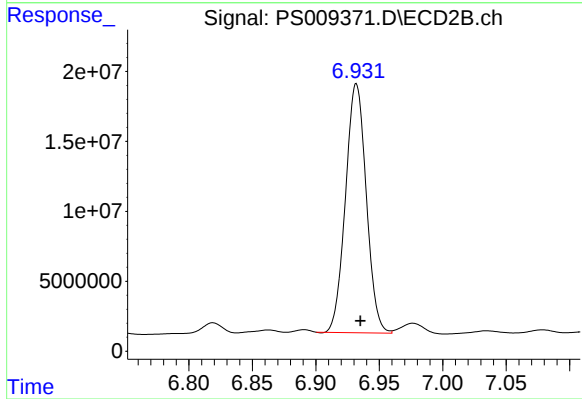


#4 2,4-DCAA

R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 202743063
Conc: 369.16 ng/ml

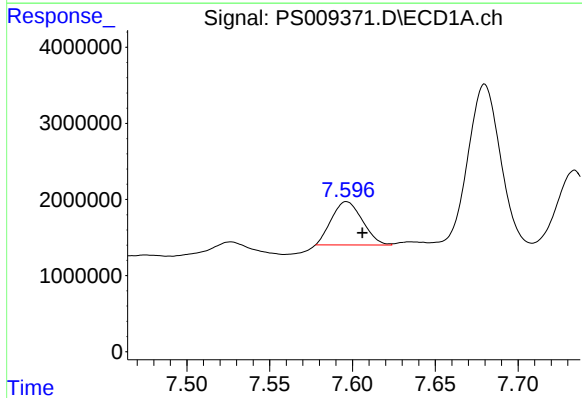


#6 MCP

R.T.: 7.596 min
Delta R.T.: -0.010 min
Response: 7381441
Conc: 3.00 ug/ml

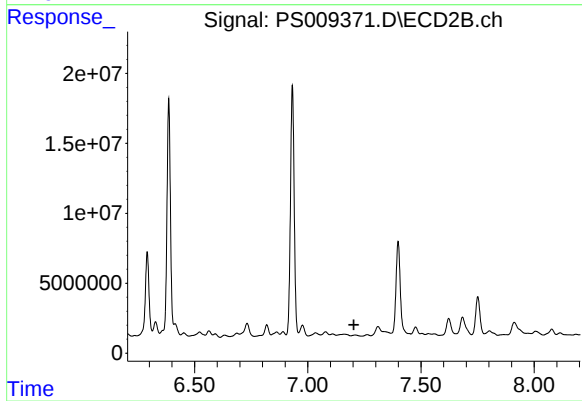

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

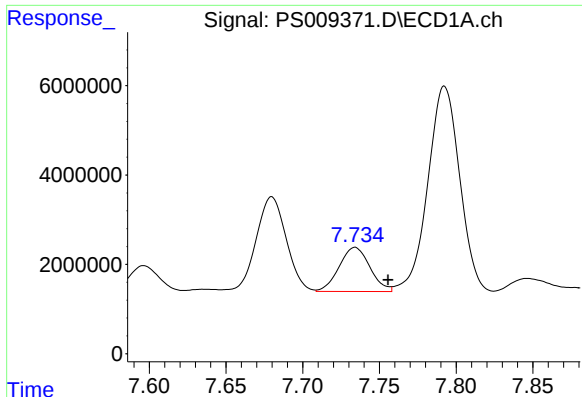

#7 MCPA


R.T.: 7.734 min
Delta R.T.: -0.022 min
Response: 13822038
Conc: 4.54 ug/ml

Instrument :
ECD_S
ClientSampleId :

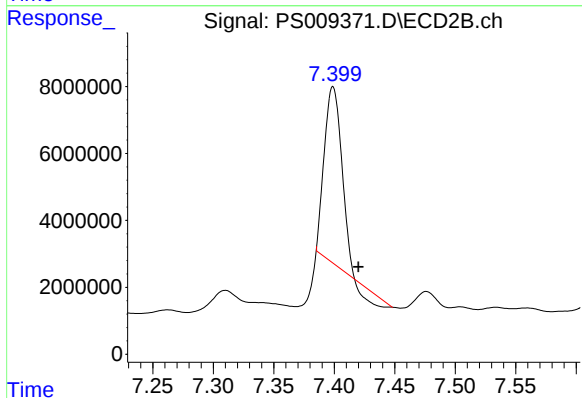


#7 MCPA

R.T.: 7.399 min
Delta R.T.: -0.021 min
Response: 47457143
Conc: 17.59 ug/ml

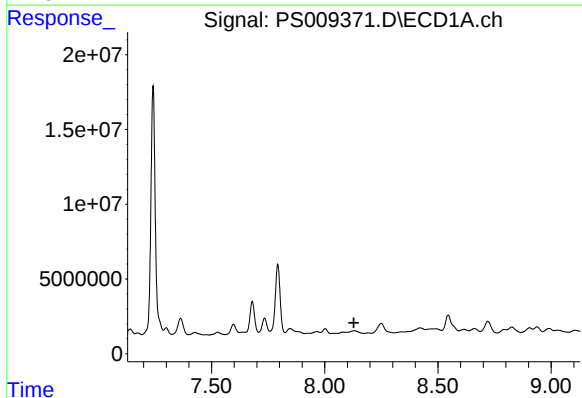


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

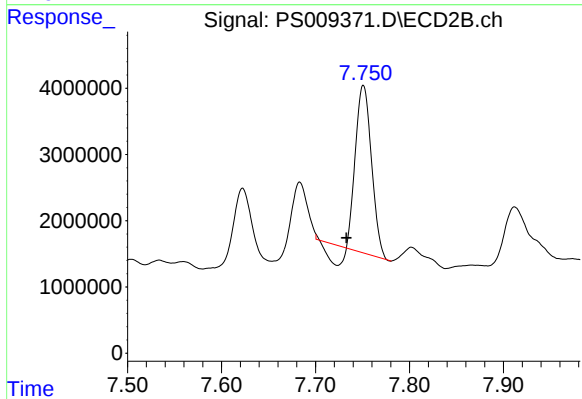

#8 DICHLORPROP


R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 27885700
Conc: 50.26 ng/ml

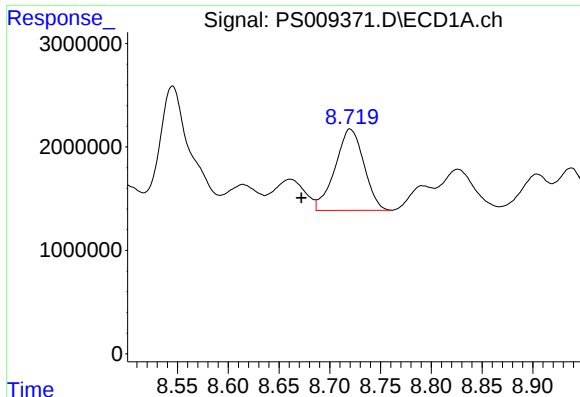

#10 Pentachlorophenol


R.T.: 8.720 min
Delta R.T.: 0.048 min
Response: 15522131
Conc: 2.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

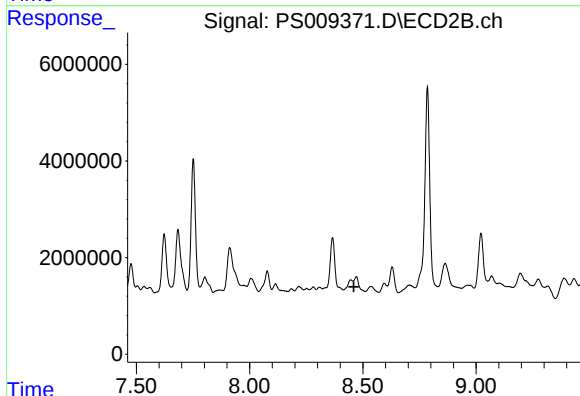


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.461 min
Response: 0
Conc: N.D.

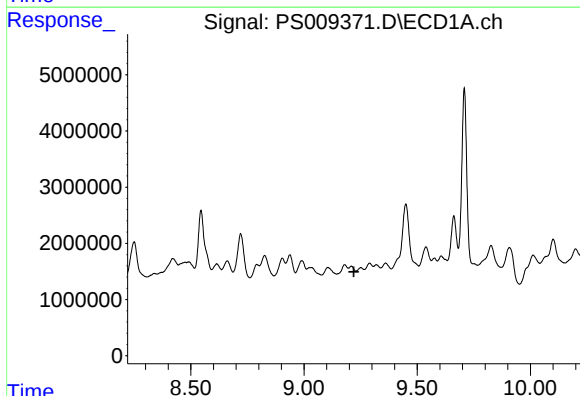


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.221 min
Response: 0
Conc: N.D.

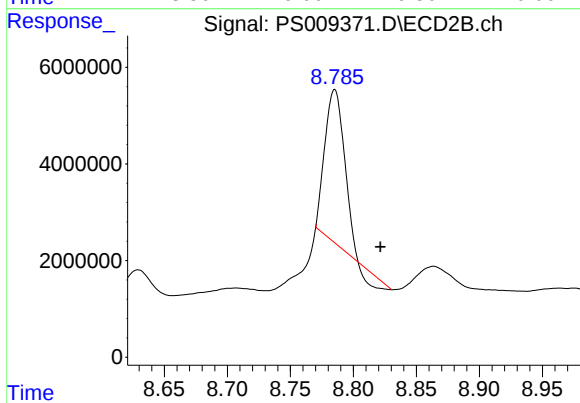

#11 2,4,5-TP (SILVEX)


R.T.: 8.785 min
Delta R.T.: -0.036 min
Response: 31936124
Conc: 10.71 ng/ml

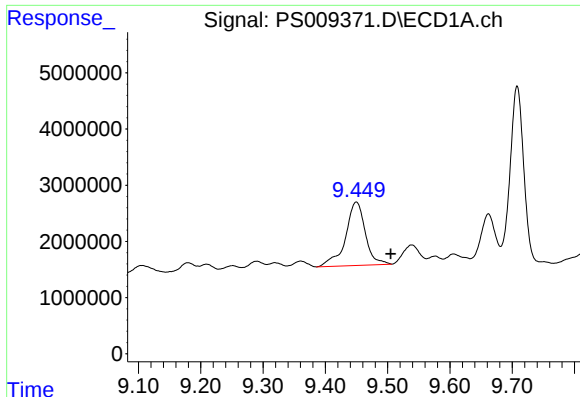

#12 2,4,5-T


R.T.: 9.450 min
Delta R.T.: -0.055 min
Response: 24924476
Conc: 9.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

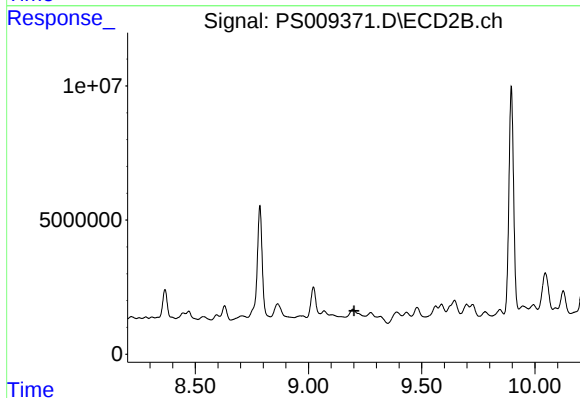


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

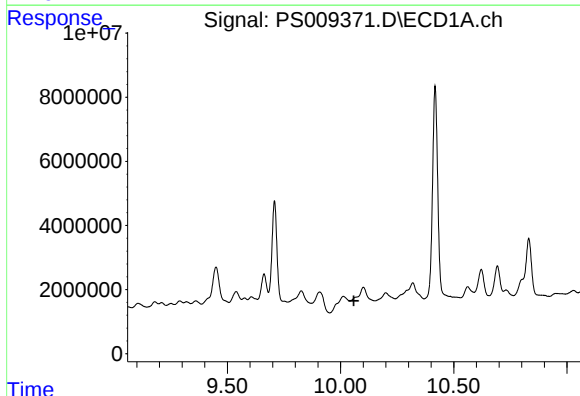


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.059 min
Response: 0
Conc: N.D.

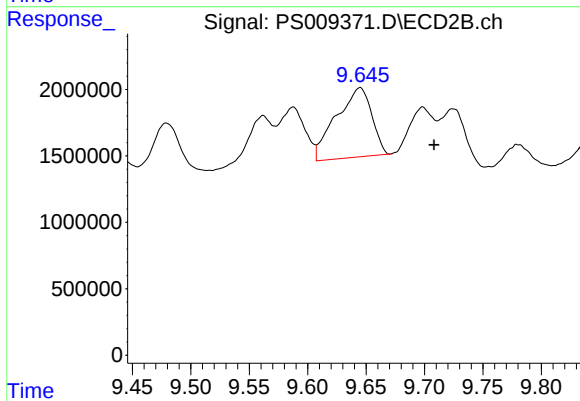

#13 2,4-DB


R.T.: 9.645 min
Delta R.T.: -0.064 min
Response: 11051744
Conc: 29.11 ng/ml

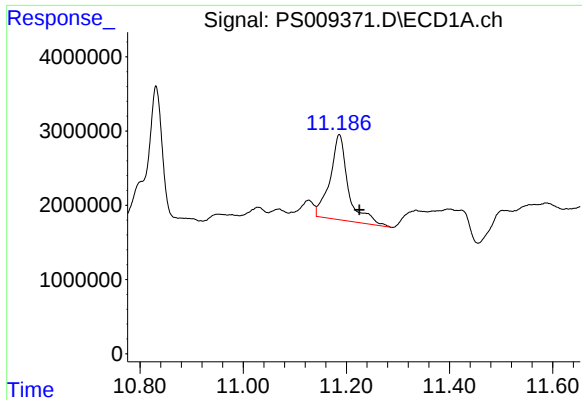

#14 DINOSEB


R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 28325008
Conc: 13.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

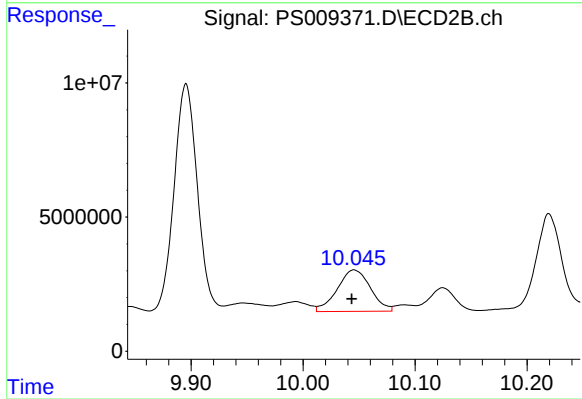


#14 DINOSEB

R.T.: 10.046 min
Delta R.T.: 0.002 min
Response: 31882252
Conc: 14.52 ng/ml

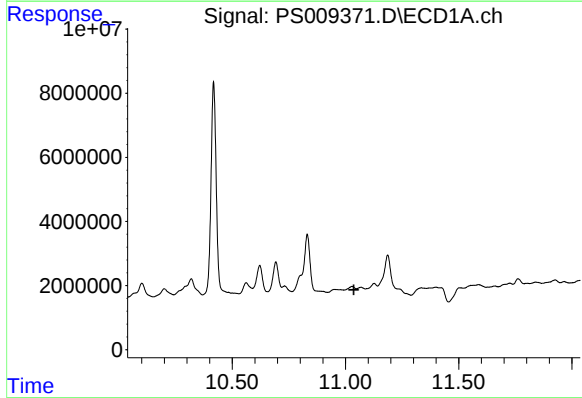


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

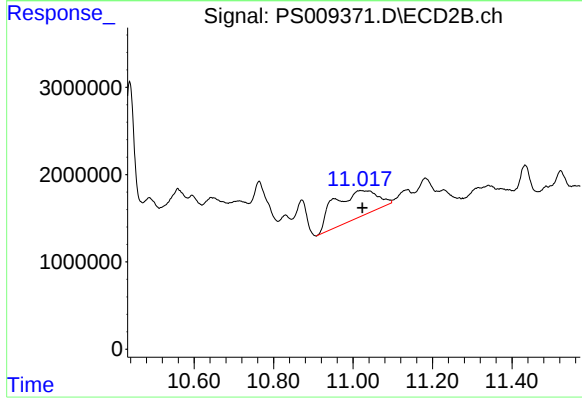

#15 Picloram


R.T.: 11.019 min
Delta R.T.: -0.004 min
Response: 23941830
Conc: 5.88 ng/ml

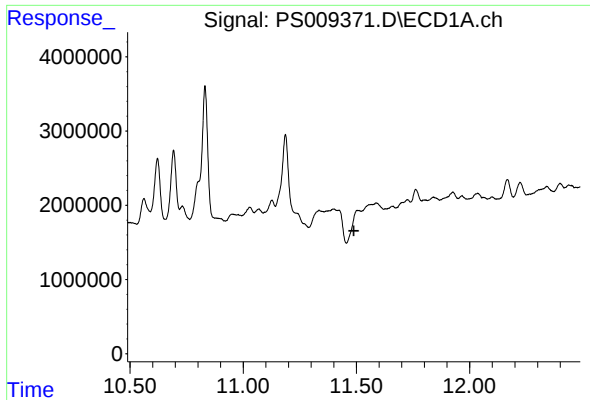

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

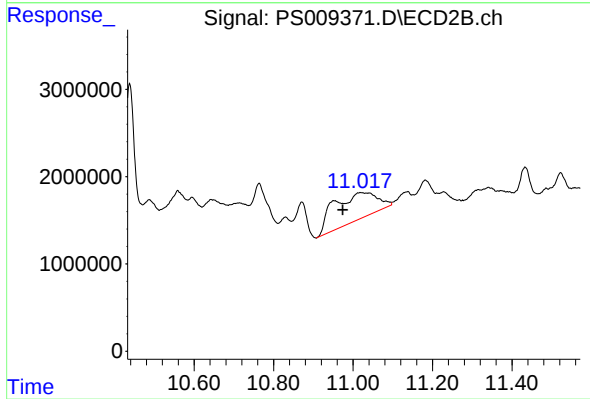

#16 DCPA

R.T.: 11.019 min
Delta R.T.: 0.045 min
Response: 23941830
Conc: 6.18 ng/ml