

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031924\
 Data File : PS026201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2024 21:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 07:02:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031924.M
 Quant Title : 8080.M
 QLast Update : Tue Mar 19 15:58:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.191	7.712	1565.0E6	460.3E6	487.415	489.145
Target Compounds							
1) T	Dalapon	2.676	2.713	64198745	7661998	12.415	4.031 #
2) T	3,5-DICHL...	6.386	0.000	96640	0	<MDL	N.D. #
3) T	4-Nitroph...	6.988	0.000	8142576	0	4.669	N.D. #
5) T	DICAMBA	0.000	7.891	0	839441	N.D.	<MDL
6) T	MCP	7.612f	8.043	25657246	389462	2.641	<MDL #
8) T	DICHLORPROP	8.051	8.604	1007951	1644367	<MDL	1.518 #
9) T	2,4-D	0.000	8.894f	0	1690632	N.D.	1.642
11) T	2,4,5-TP ...	9.210	9.875	102.9E6	666166	5.404	<MDL #
12) T	2,4,5-T	9.488	0.000	1444.9E6	0	77.678	N.D. #
13) T	2,4-DB	10.048	0.000	402.2E6	0	160.754	N.D. #
15) T	Picloram	11.044	0.000	8997702	0	<MDL	N.D. #
16) T	DCPA	11.533	0.000	2067040	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031924\
Data File : PS026201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2024 21:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 07:02:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031924.M
Quant Title : 8080.M
QLast Update : Tue Mar 19 15:58:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

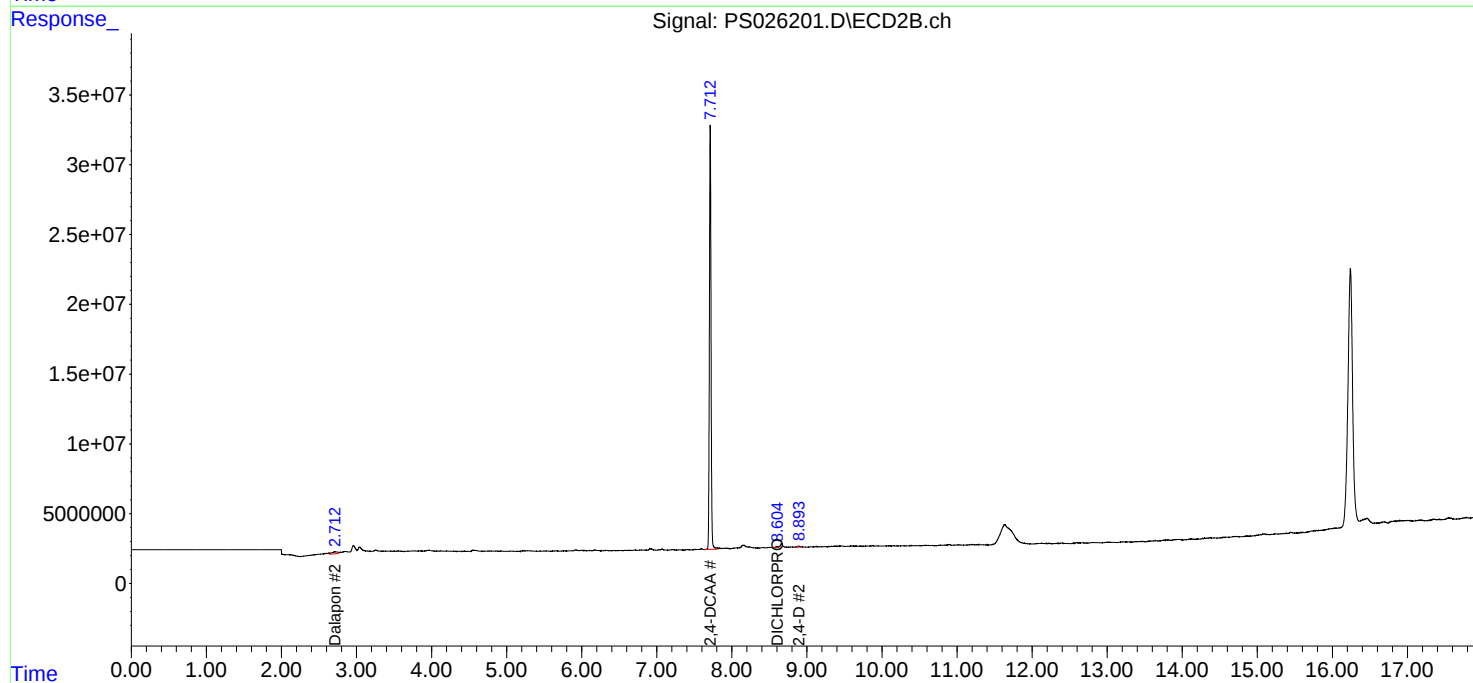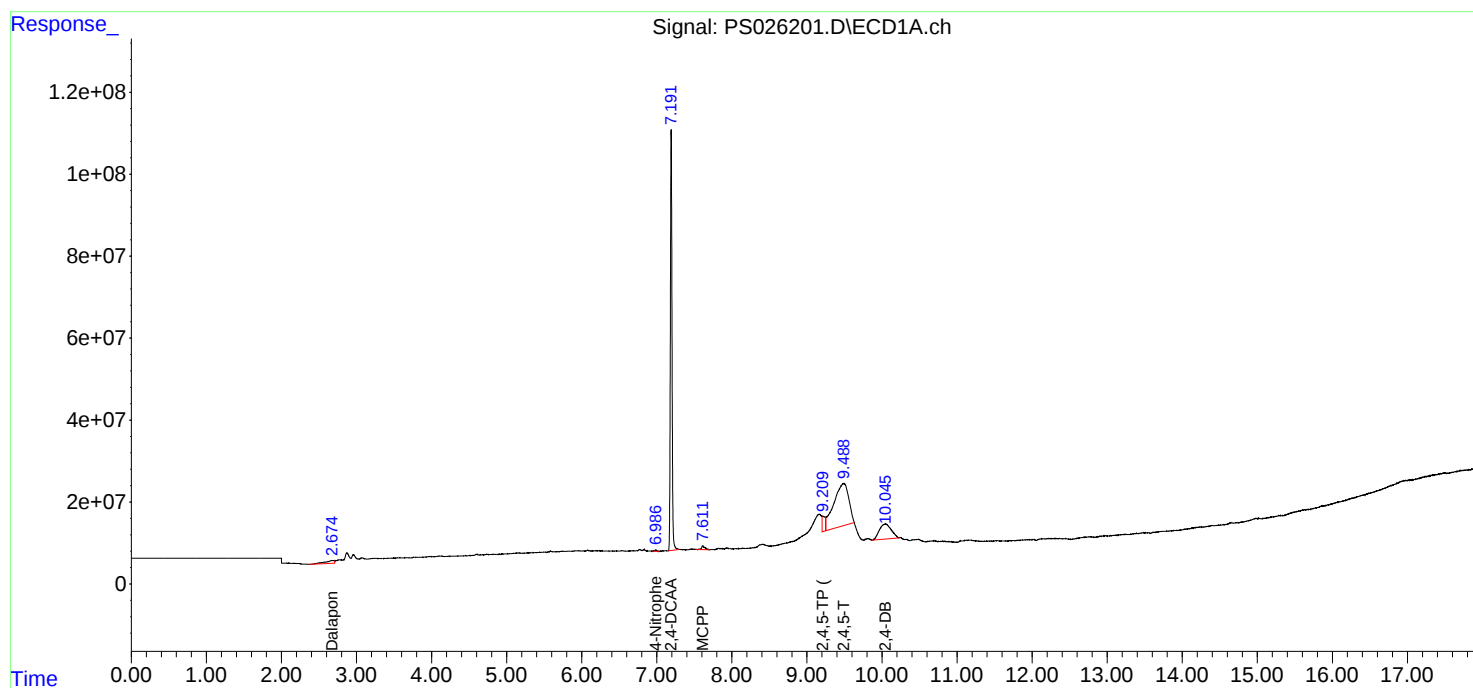


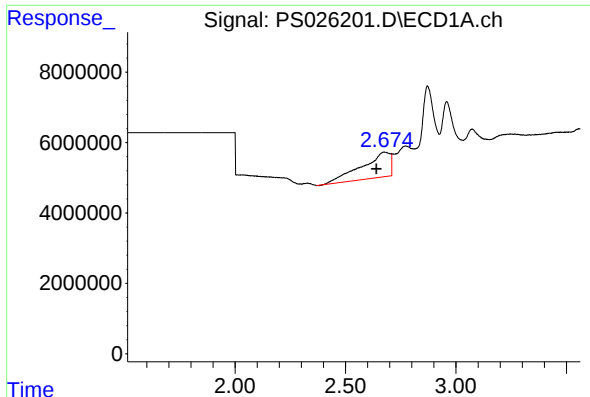

#1 Dalapon


R.T.: 2.676 min
Delta R.T.: 0.036 min
Response: 64198745
Conc: 12.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

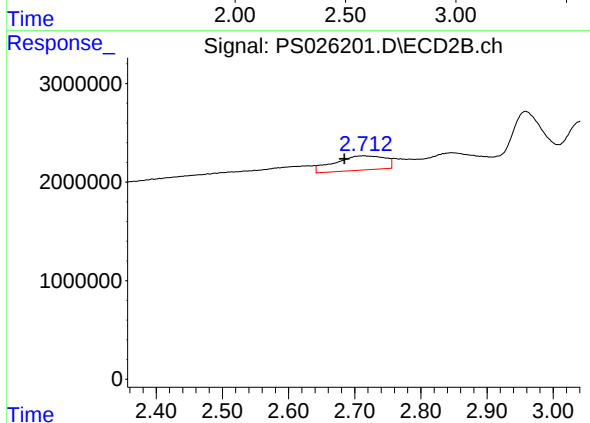


#1 Dalapon

R.T.: 2.713 min
Delta R.T.: 0.029 min
Response: 7661998
Conc: 4.03 ng/ml

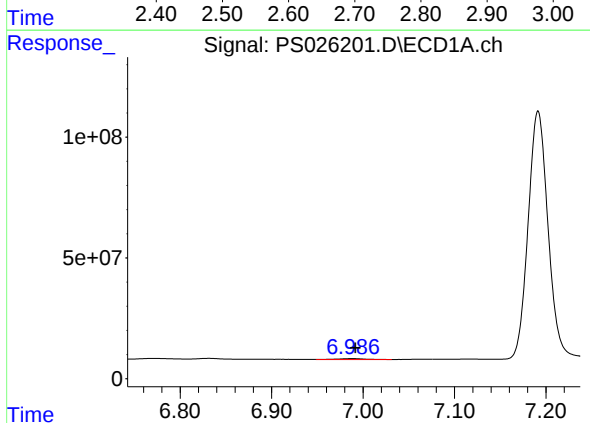


#3 4-Nitrophenol

R.T.: 6.988 min
Delta R.T.: -0.003 min
Response: 8142576
Conc: 4.67 ng/ml

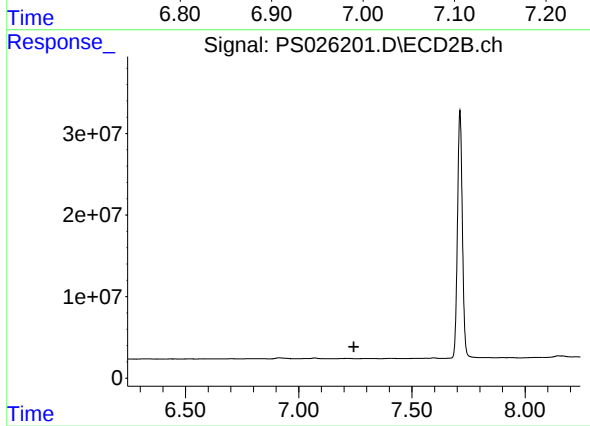

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.244 min
Response: 0
Conc: N.D.

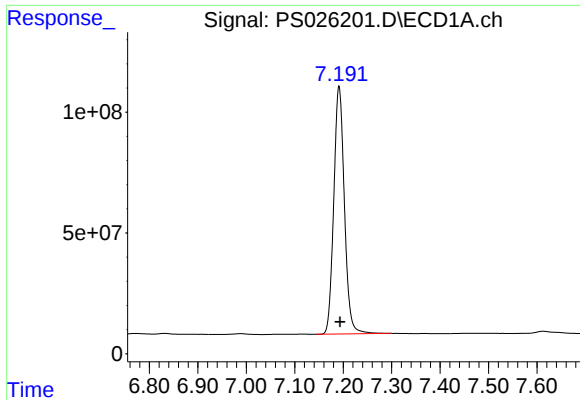

#4 2,4-DCAA


R.T.: 7.191 min
Delta R.T.: -0.002 min
Response: 1564967106
Conc: 487.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

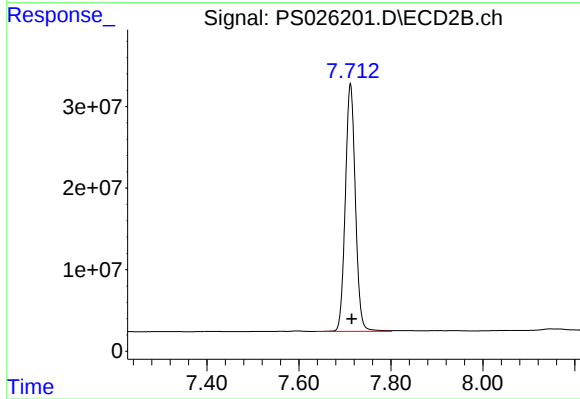


#4 2,4-DCAA

R.T.: 7.712 min
Delta R.T.: -0.003 min
Response: 460265635
Conc: 489.14 ng/ml

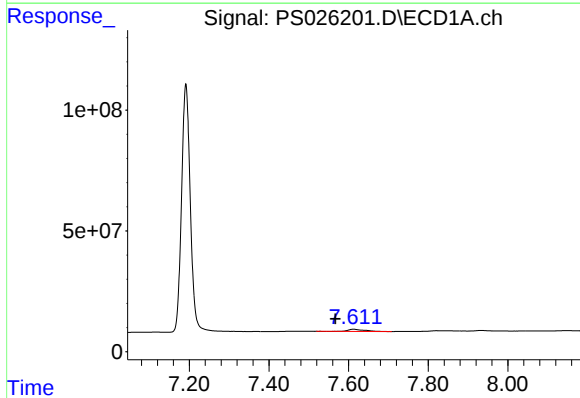


#6 MCP

R.T.: 7.612 min
Delta R.T.: 0.046 min
Response: 25657246
Conc: 2.64 ug/ml

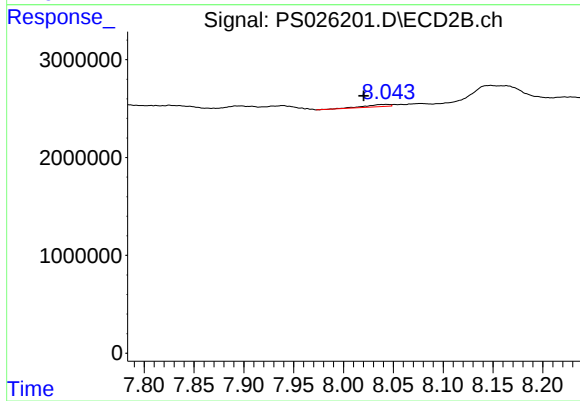

#6 MCP


R.T.: 8.043 min
Delta R.T.: 0.023 min
Response: 389462
Conc: N.D.

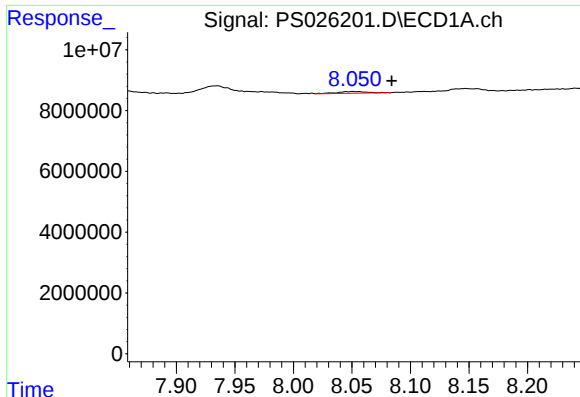

#8 DICHLORPROP


R.T.: 8.051 min
Delta R.T.: -0.033 min
Response: 1007951
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

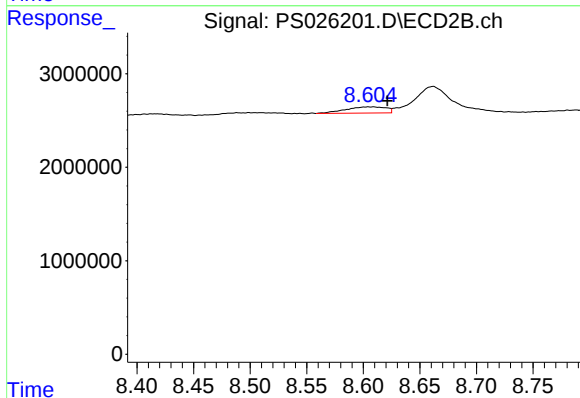


#8 DICHLORPROP

R.T.: 8.604 min
Delta R.T.: -0.017 min
Response: 1644367
Conc: 1.52 ng/ml

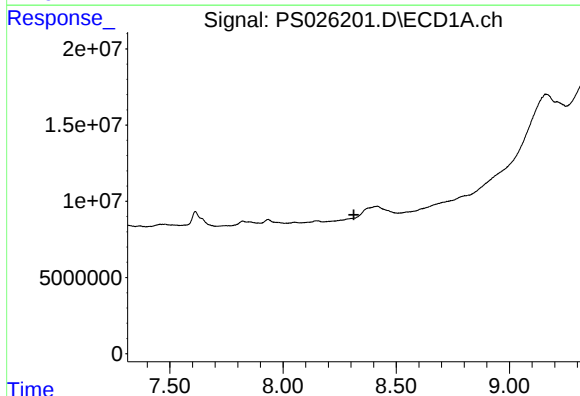


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.313 min
Response: 0
Conc: N.D.

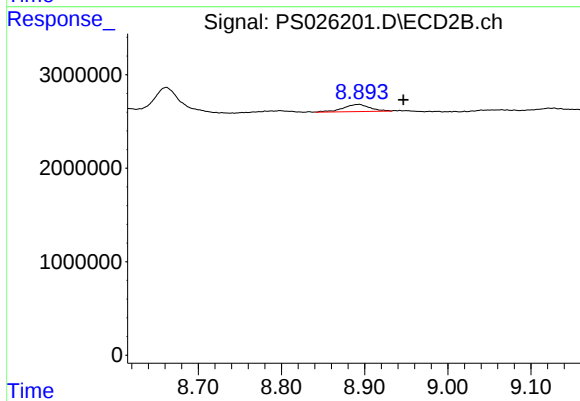

#9 2,4-D


R.T.: 8.894 min
Delta R.T.: -0.053 min
Response: 1690632
Conc: 1.64 ng/ml

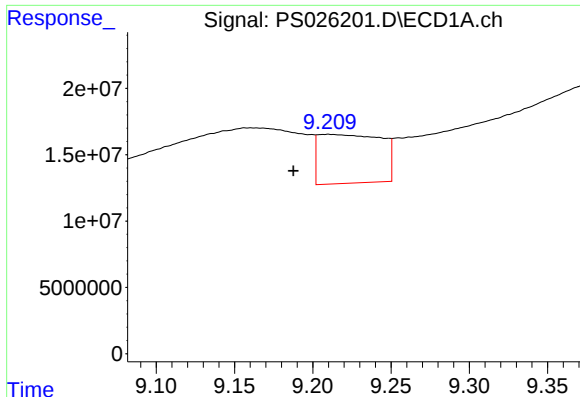

#11 2,4,5-TP (SILVEX)


R.T.: 9.210 min
Delta R.T.: 0.022 min
Response: 102884360
Conc: 5.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

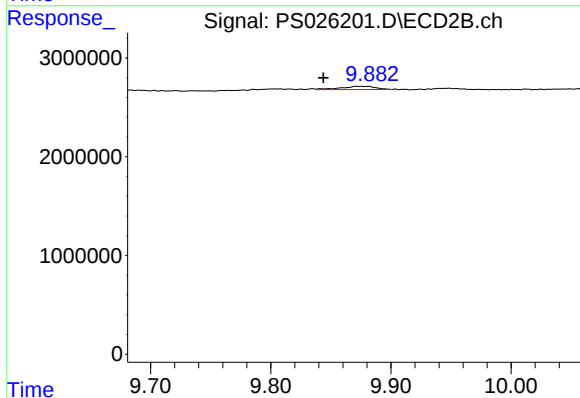


#11 2,4,5-TP (SILVEX)

R.T.: 9.875 min
Delta R.T.: 0.031 min
Response: 666166
Conc: N.D.

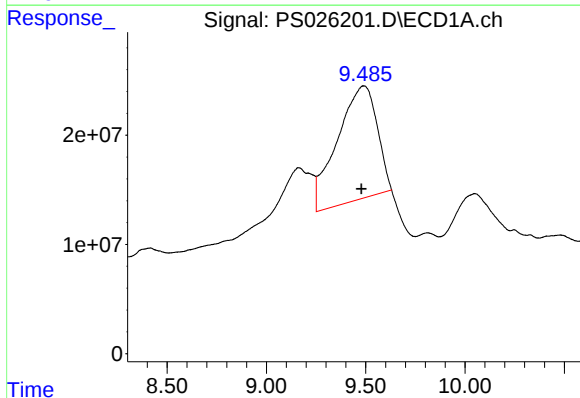


#12 2,4,5-T

R.T.: 9.488 min
Delta R.T.: 0.010 min
Response: 1444922887
Conc: 77.68 ng/ml

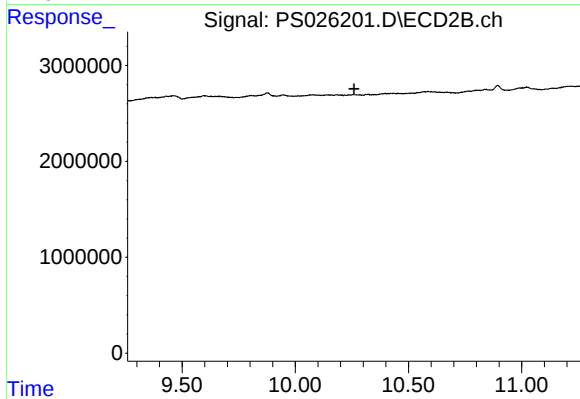

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 10.259 min
Response: 0
Conc: N.D.

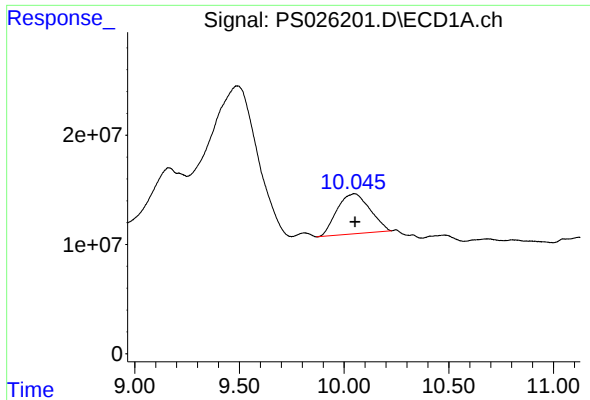

#13 2,4-DB

R.T.: 10.048 min
Delta R.T.: -0.004 min
Response: 402179112
Conc: 160.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

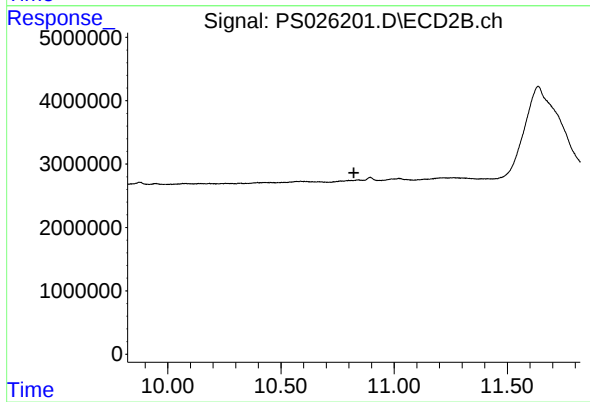

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.822 min
Response: 0
Conc: N.D.