

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031925\
 Data File : PS029452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2025 09:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 01:35:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.166	7.624	1971.5E6	449.8E6	478.448	478.294
Target Compounds							
1) T	Dalapon	2.648f	2.680f	44698831	15812790	8.097	7.469
2) T	3,5-DICHL...	6.350	0.000	3423855	0	<MDL	N.D. #
3) T	4-Nitroph...	6.960	0.000	15521339	0	6.633	N.D. #
7) T	MCPA	7.634f	0.000	7640053	0	<MDL	N.D. #
8) T	DICHLORPROP	8.076f	8.583f	1820759	3002457	<MDL	2.348 #
10) T	Pentachlo...	8.573	0.000	8538490	0	<MDL	N.D. #
12) T	2,4,5-T	9.408	0.000	16182986	0	<MDL	N.D. #
13) T	2,4-DB	9.994	0.000	233266	0	<MDL	N.D. #
14) T	DINOSEB	11.199	0.000	3683548	0	<MDL	N.D. #
15) T	Picloram	0.000	12.214f	0	15372656	N.D.	1.330
16) T	DCPA	11.499	0.000	8322475	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031925\
Data File : PS029452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2025 09:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 01:35:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

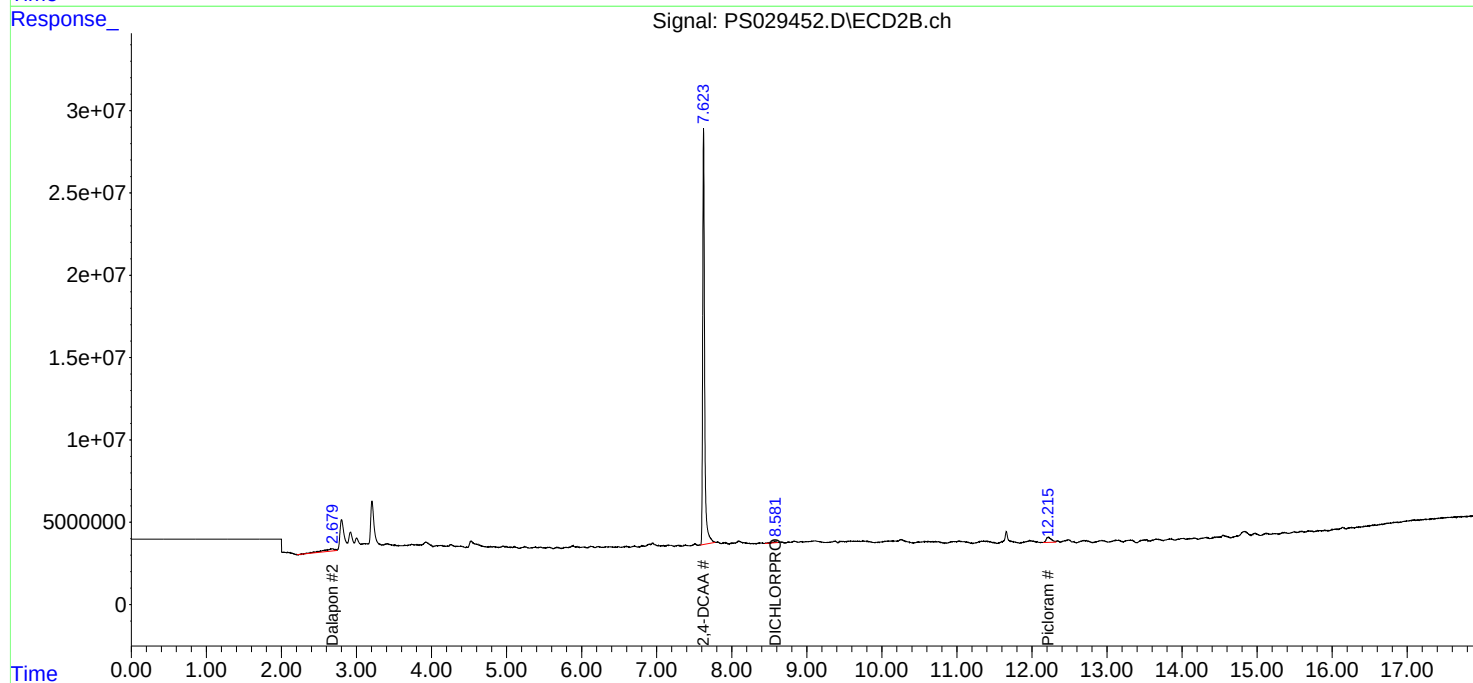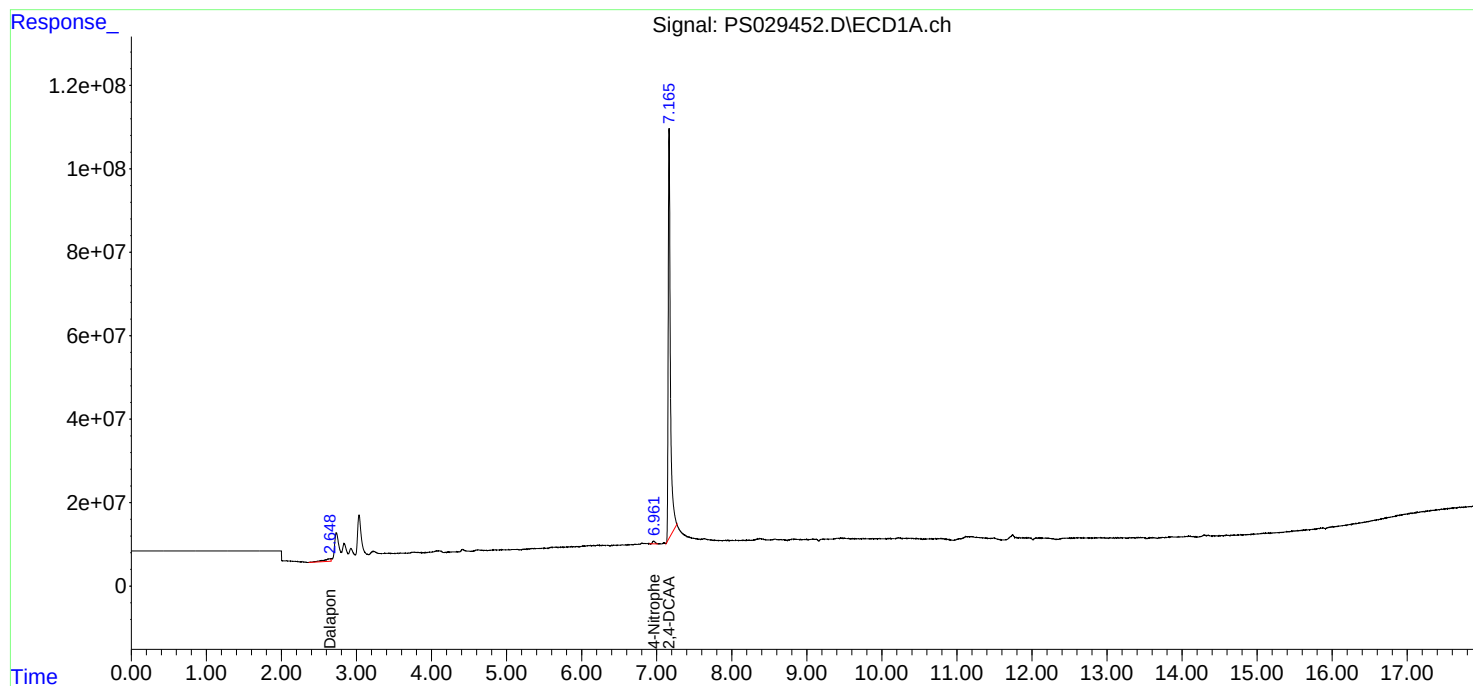


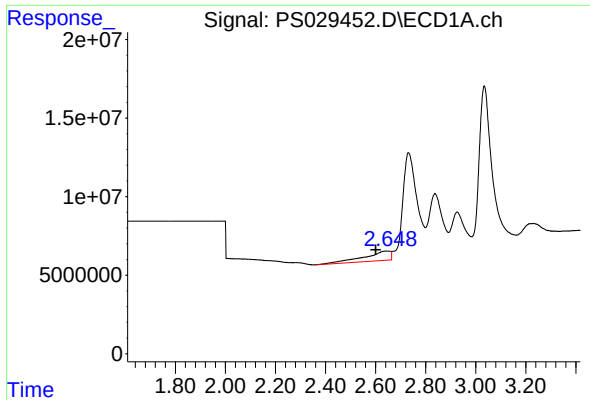

#1 Dalapon


R.T.: 2.648 min
Delta R.T.: 0.048 min
Response: 44698831
Conc: 8.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

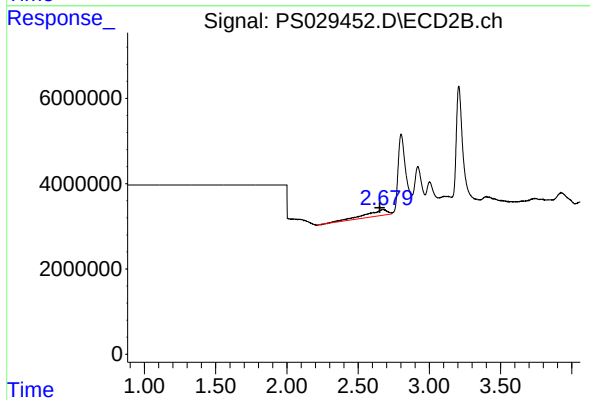


#1 Dalapon

R.T.: 2.680 min
Delta R.T.: 0.029 min
Response: 15812790
Conc: 7.47 ng/ml

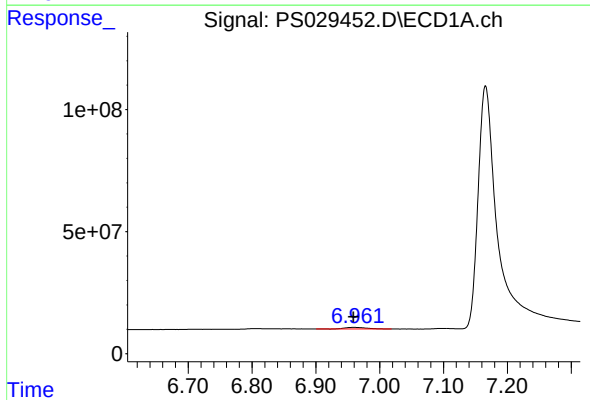


#3 4-Nitrophenol

R.T.: 6.960 min
Delta R.T.: 0.001 min
Response: 15521339
Conc: 6.63 ng/ml

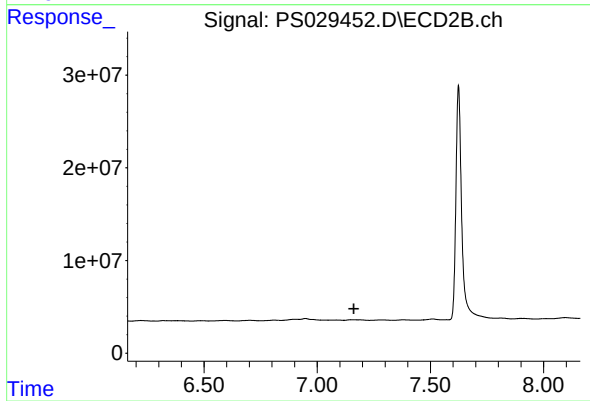

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.162 min
Response: 0
Conc: N.D.

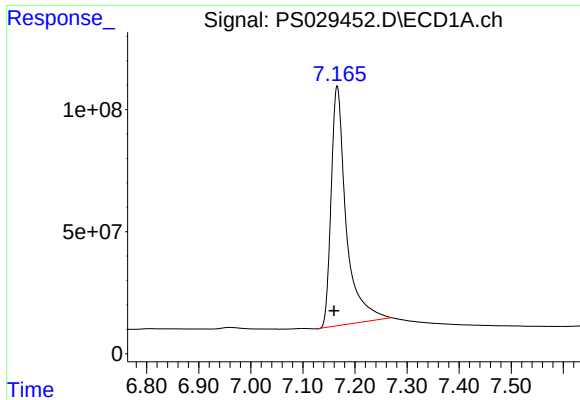

#4 2,4-DCAA


R.T.: 7.166 min
Delta R.T.: 0.006 min
Response: 1971481977
Conc: 478.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

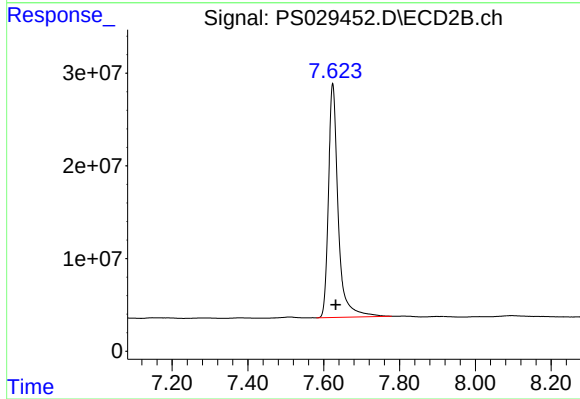


#4 2,4-DCAA

R.T.: 7.624 min
Delta R.T.: -0.008 min
Response: 449755338
Conc: 478.29 ng/ml

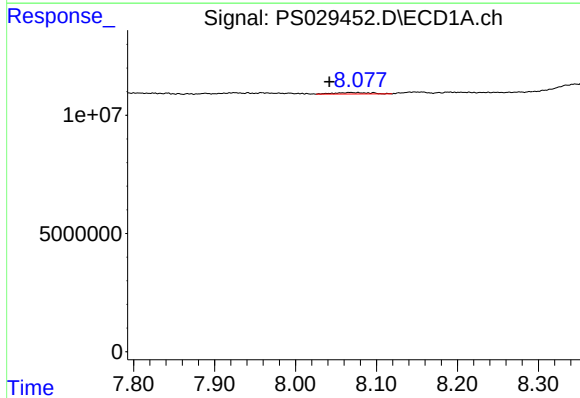


#8 DICHLORPROP

R.T.: 8.076 min
Delta R.T.: 0.034 min
Response: 1820759
Conc: N.D.

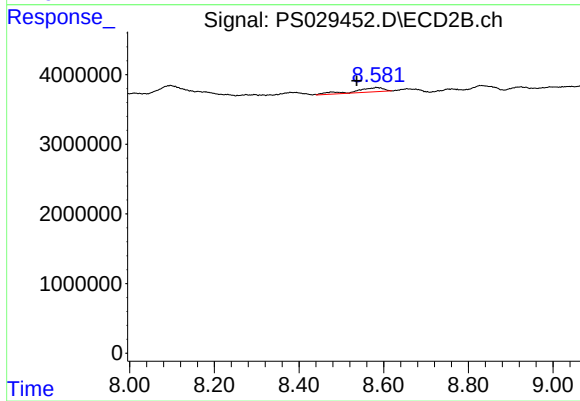

#8 DICHLORPROP


R.T.: 8.583 min
Delta R.T.: 0.047 min
Response: 3002457
Conc: 2.35 ng/ml

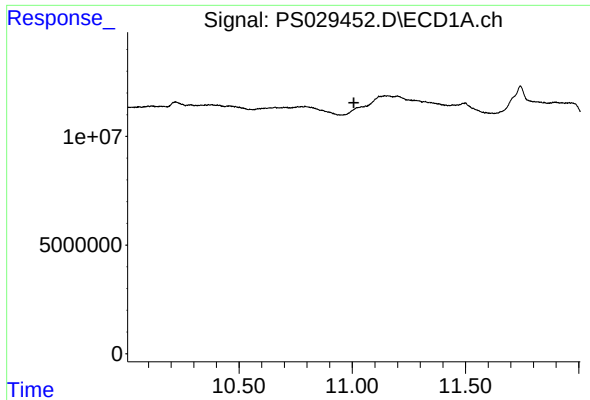

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.007 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

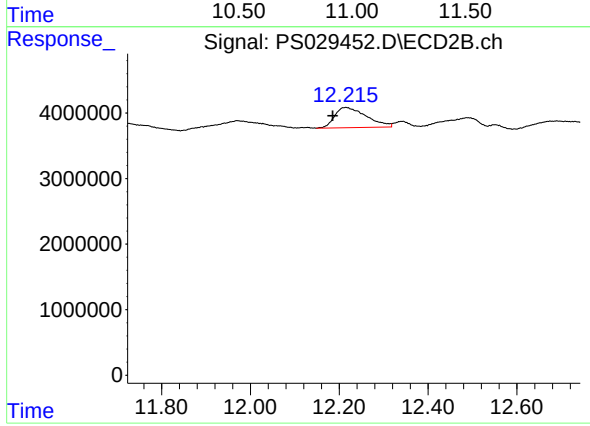

#15 Picloram

R.T.: 12.214 min
Delta R.T.: 0.029 min
Response: 15372656
Conc: 1.33 ng/ml