

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
 Data File : PS003623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 12:31
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:42:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.807	0	879387	N.D.	1.873 #
Target Compounds							
2) T	3,5-DICHL...	0.000	8.968	0	477278	N.D.	0.773 #
3) T	4-Nitroph...	0.000	9.966	0	41772	N.D.	0.186 #
5) T	DICAMBA	0.000	11.069	0	2906062	N.D.	1.739 #
6) T	MCP	0.000	11.247	0	67702	N.D.	0.057 #
10) T	Pentachlo...	13.521	13.197	5669931	4986960	0.803	0.757
11) T	2,4,5-TP ...	14.410	13.831	3266237	4420095	1.216	1.736 #
12) T	2,4,5-T	0.000	14.428	0	7393184	N.D.	3.666 #
13) T	2,4-DB	0.000	15.088	0	3294918	N.D.	12.903 #
14) T	DINOSEB	17.006	15.463	6561637	7098372	2.922	3.977 #
15) T	Picloram	16.761	16.729	64926119	10461265	26.379	4.122 #
16) T	DCPA	17.351	16.637	3748068	6772307	1.137	2.177 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
Data File : PS003623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 12:31
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:42:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

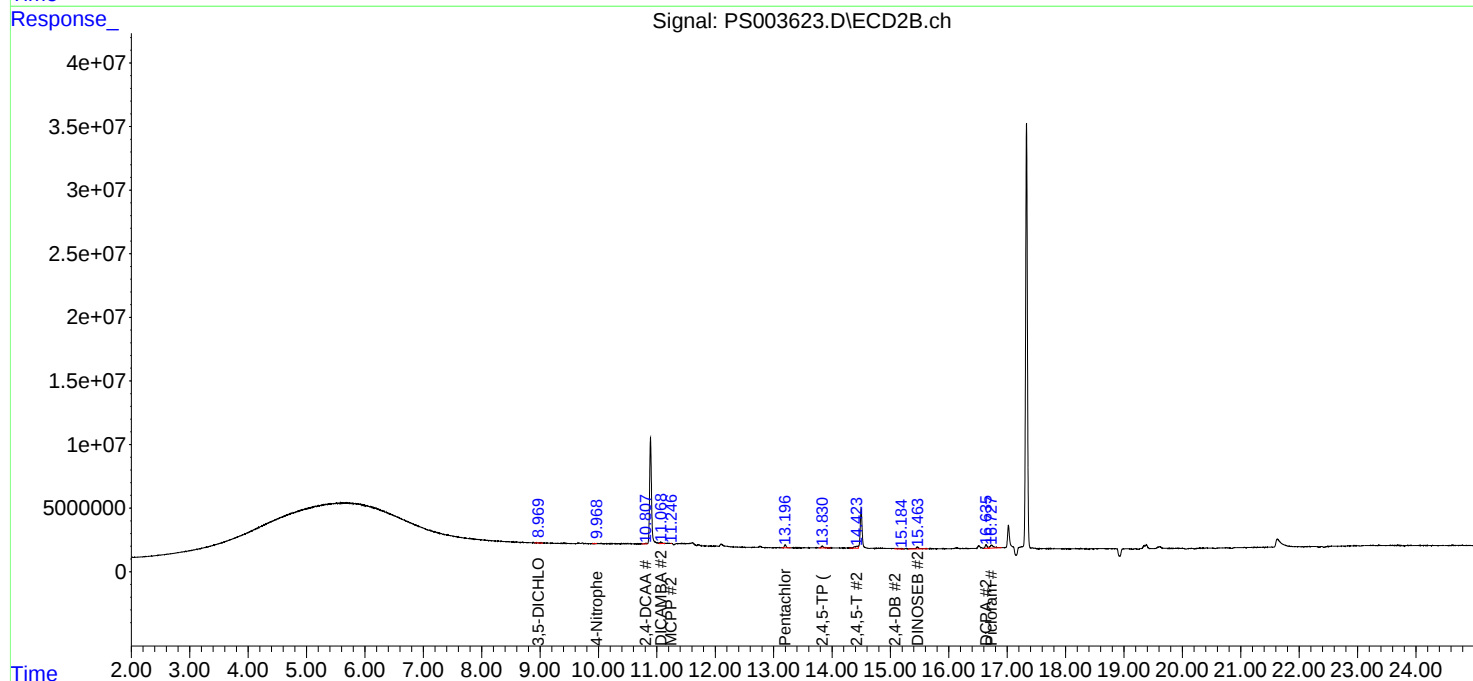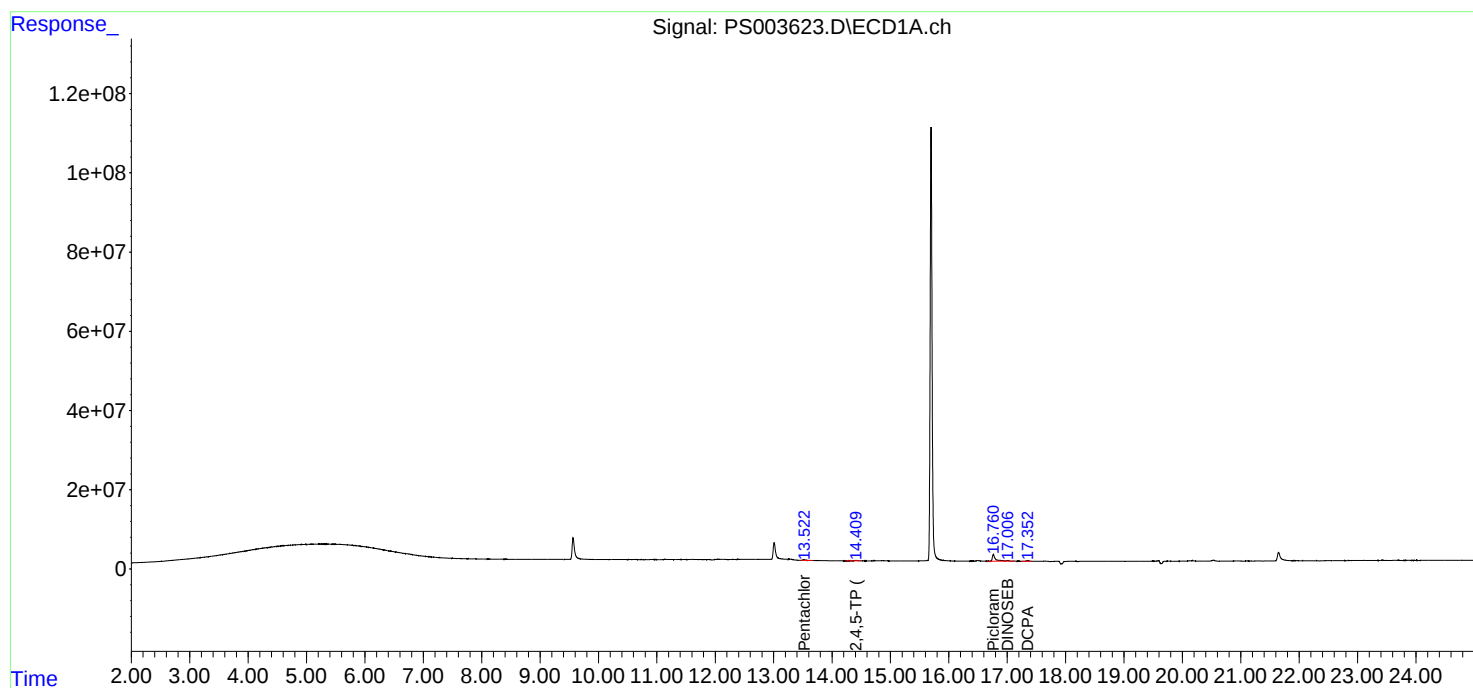


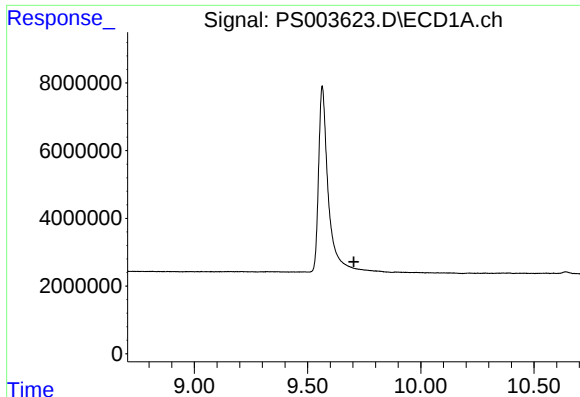

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

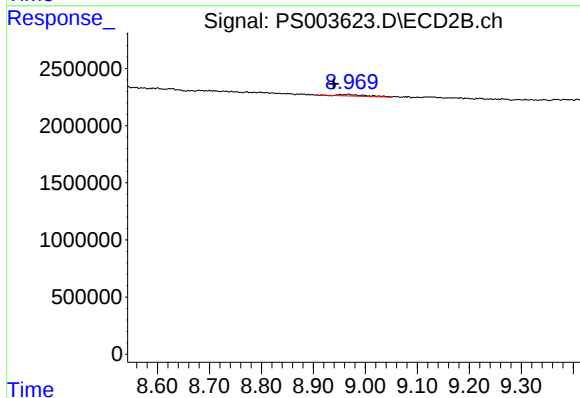


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.968 min
Delta R.T.: 0.028 min
Response: 477278
Conc: 0.77 ng/ml

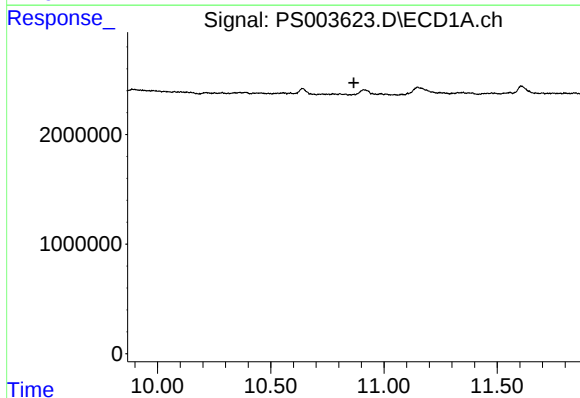


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.867 min
Response: 0
Conc: N.D.

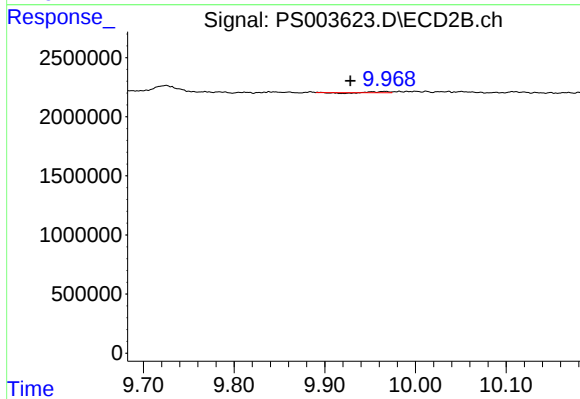

#3 4-Nitrophenol


R.T.: 9.966 min
Delta R.T.: 0.038 min
Response: 41772
Conc: 0.19 ng/ml

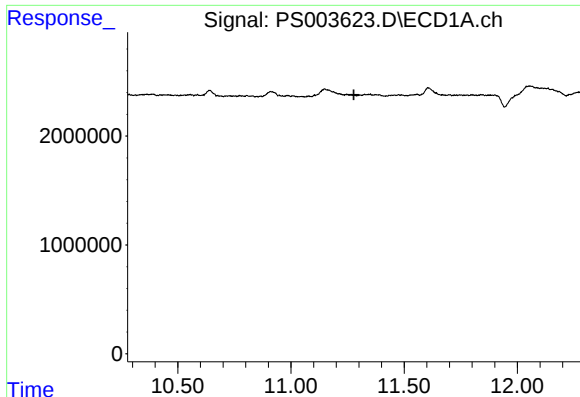

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

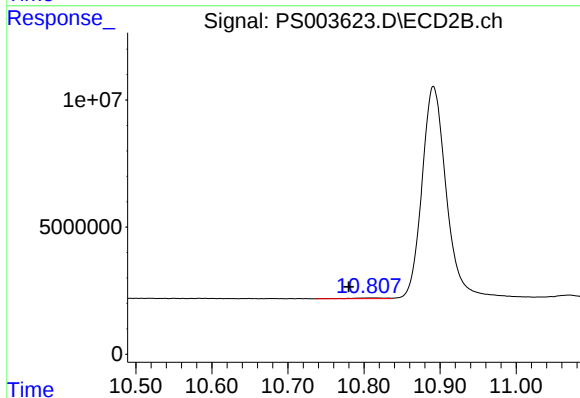


#4 2,4-DCAA

R.T.: 10.807 min
Delta R.T.: 0.028 min
Response: 879387
Conc: 1.87 ng/ml

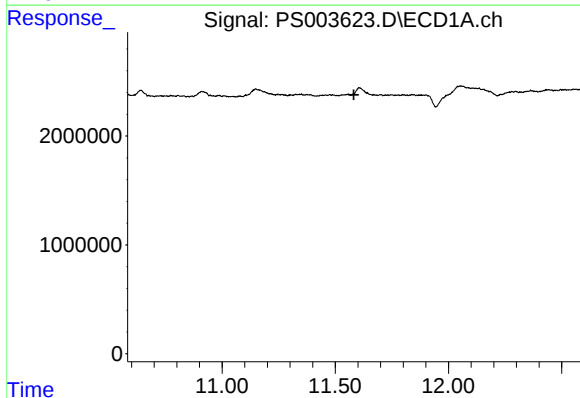


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

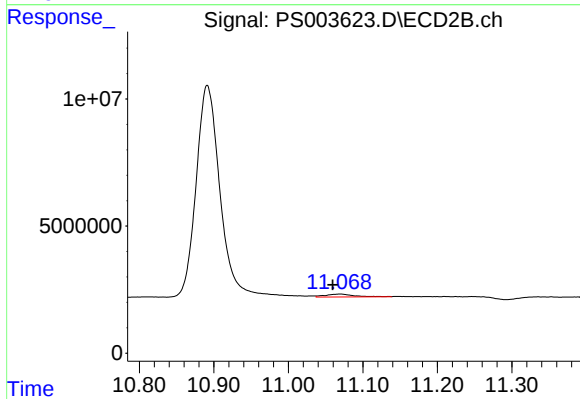

#5 DICAMBA


R.T.: 11.069 min
Delta R.T.: 0.010 min
Response: 2906062
Conc: 1.74 ng/ml

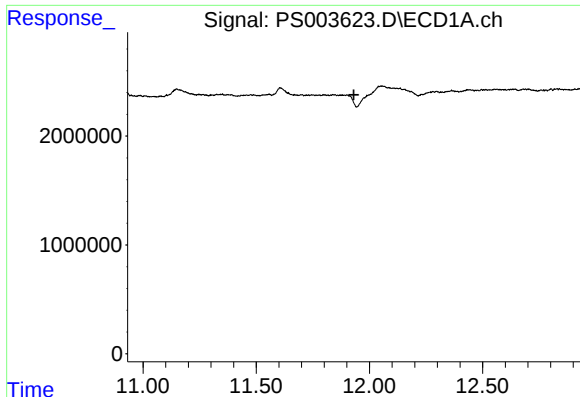

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

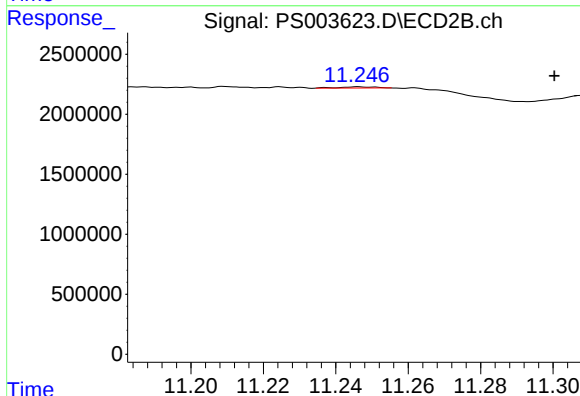


#6 MCP

R.T.: 11.247 min
Delta R.T.: -0.053 min
Response: 67702
Conc: 0.06 ug/ml

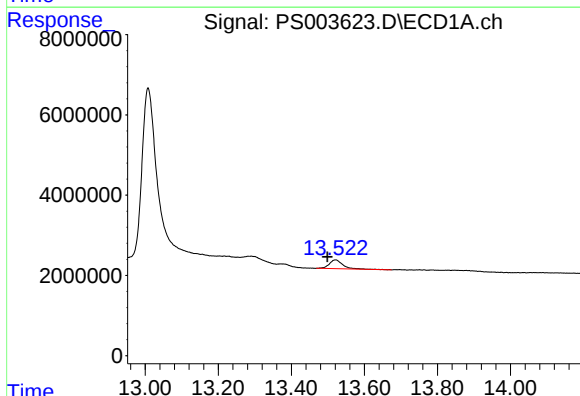


#10 Pentachlorophenol

R.T.: 13.521 min
Delta R.T.: 0.022 min
Response: 5669931
Conc: 0.80 ng/ml

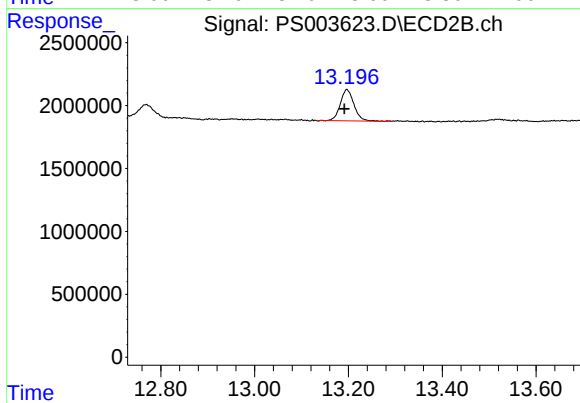

#10 Pentachlorophenol


R.T.: 13.197 min
Delta R.T.: 0.005 min
Response: 4986960
Conc: 0.76 ng/ml

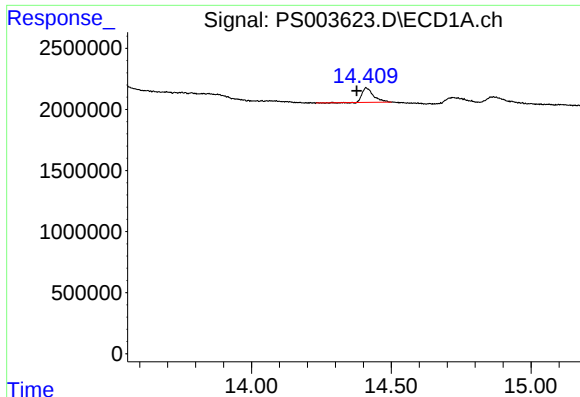

#11 2,4,5-TP (SILVEX)


R.T.: 14.410 min
Delta R.T.: 0.033 min
Response: 3266237
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

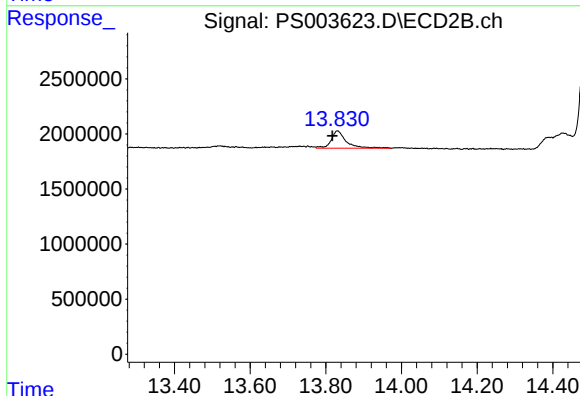


#11 2,4,5-TP (SILVEX)

R.T.: 13.831 min
Delta R.T.: 0.014 min
Response: 4420095
Conc: 1.74 ng/ml

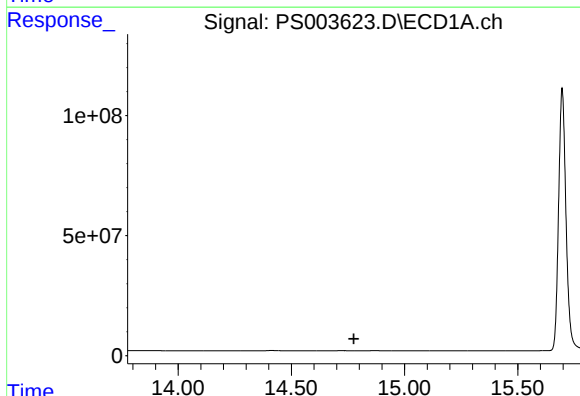


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

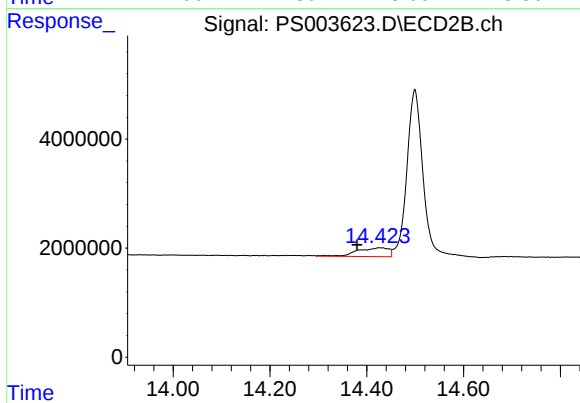

#12 2,4,5-T


R.T.: 14.428 min
Delta R.T.: 0.048 min
Response: 7393184
Conc: 3.67 ng/ml

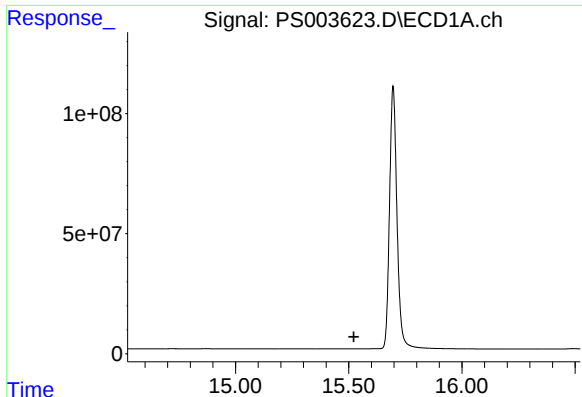

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

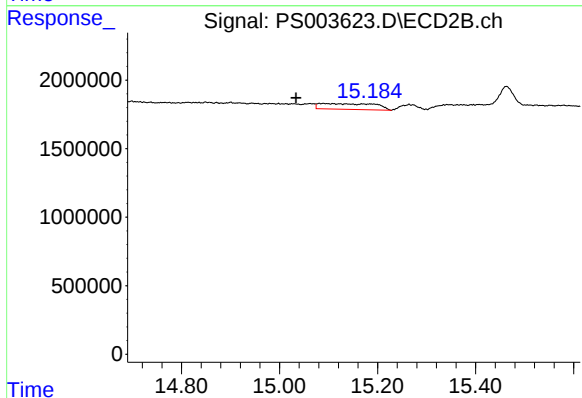


#13 2,4-DB

R.T.: 15.088 min
Delta R.T.: 0.055 min
Response: 3294918
Conc: 12.90 ng/ml

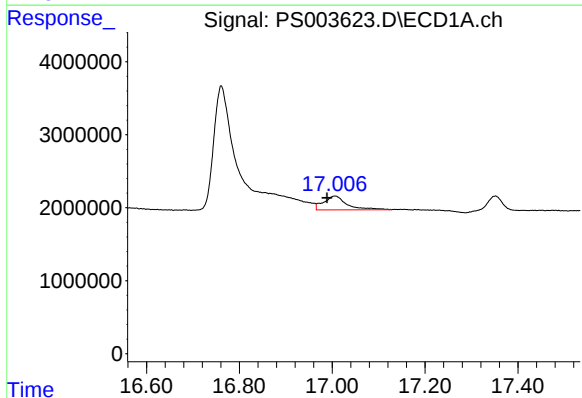


#14 DINOSEB

R.T.: 17.006 min
Delta R.T.: 0.017 min
Response: 6561637
Conc: 2.92 ng/ml

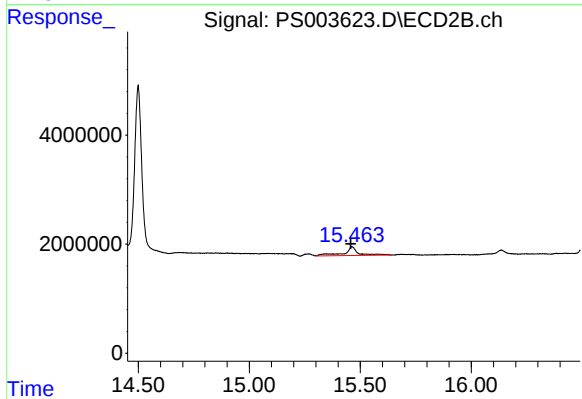

#14 DINOSEB


R.T.: 15.463 min
Delta R.T.: 0.006 min
Response: 7098372
Conc: 3.98 ng/ml

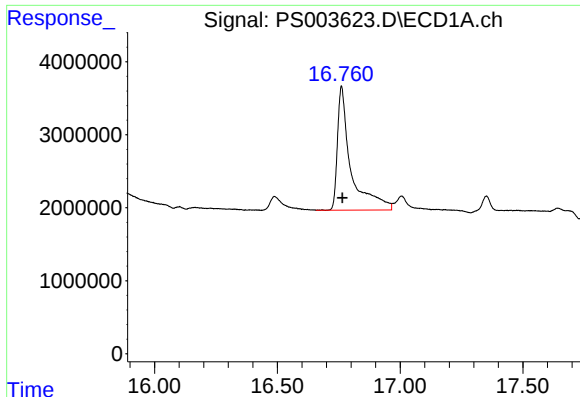

#15 Picloram


R.T.: 16.761 min
Delta R.T.: -0.004 min
Response: 64926119
Conc: 26.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

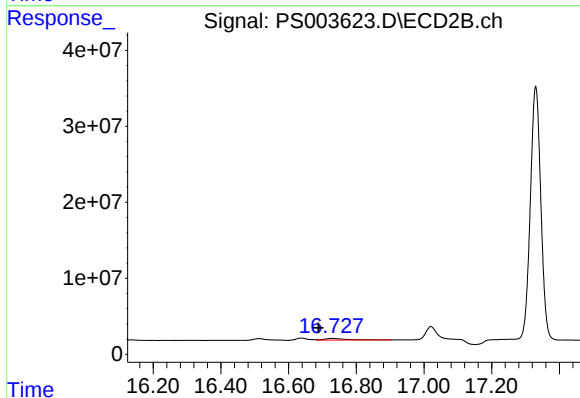


#15 Picloram

R.T.: 16.729 min
Delta R.T.: 0.040 min
Response: 10461265
Conc: 4.12 ng/ml

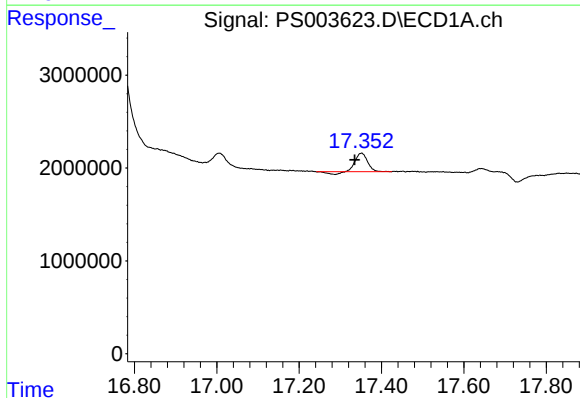

#16 DCPA

R.T.: 17.351 min
Delta R.T.: 0.016 min
Response: 3748068
Conc: 1.14 ng/ml

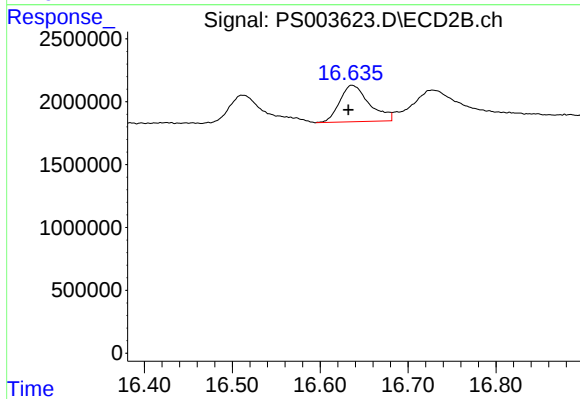

#16 DCPA

R.T.: 16.637 min
Delta R.T.: 0.005 min
Response: 6772307
Conc: 2.18 ng/ml