

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
 Data File : PS003624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 13:02
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:42:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.281	10.776	246.2E6	216.1E6	560.846	460.133
Target Compounds							
3) T	4-Nitroph...	0.000	9.966	0	62429	N.D.	0.278 #
7) T	MCPA	0.000	11.667	0	782216	N.D.	0.453 #
8) T	DICHLORPROP	0.000	12.187	0	270312	N.D.	0.654 #
10) T	Pentachlo...	0.000	13.193	0	1330330	N.D.	0.202 #
11) T	2,4,5-TP ...	0.000	13.848	0	232831	N.D.	0.091 #
13) T	2,4-DB	0.000	15.089	0	254921	N.D.	0.998 #
14) T	DINOSEB	0.000	15.463	0	642213	N.D.	0.360 #
15) T	Picloram	0.000	16.709	0	309751	N.D.	0.122 #
16) T	DCPA	0.000	16.625	0	1951562	N.D.	0.627 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
Data File : PS003624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 13:02
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:42:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

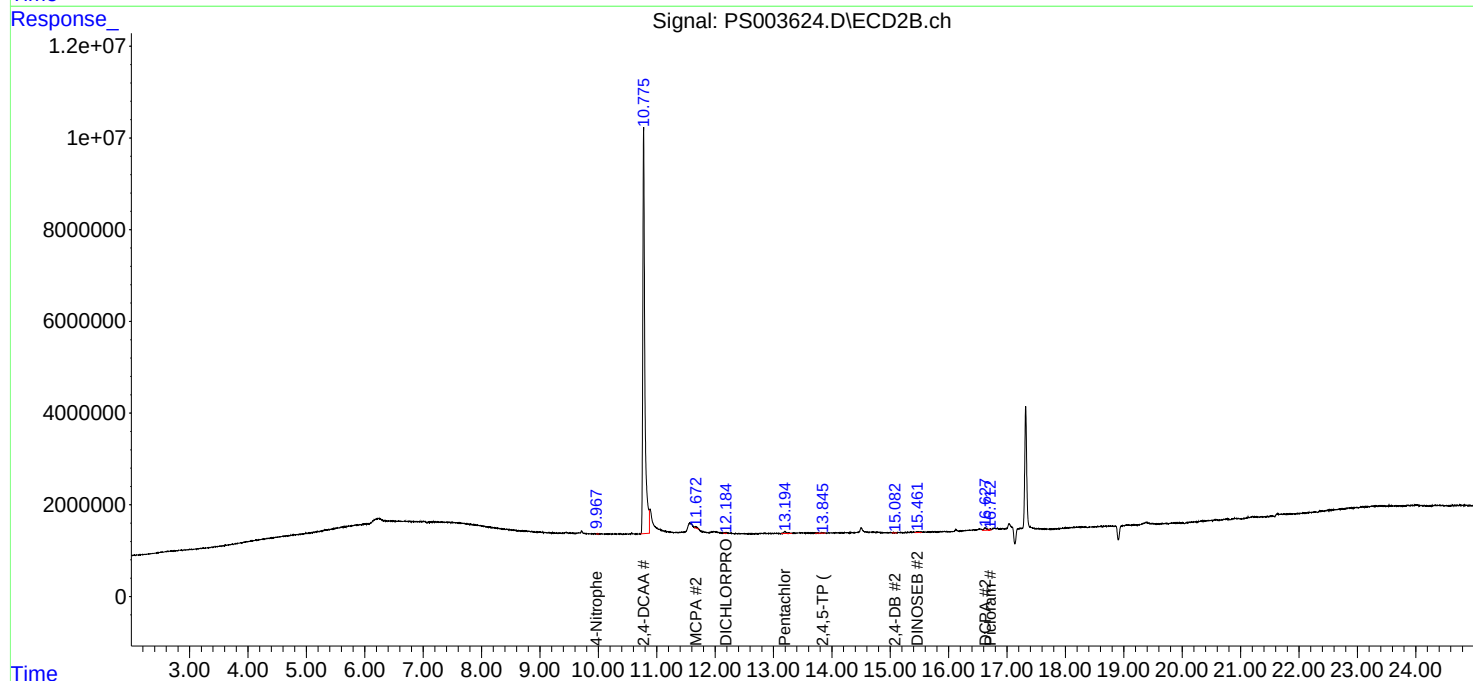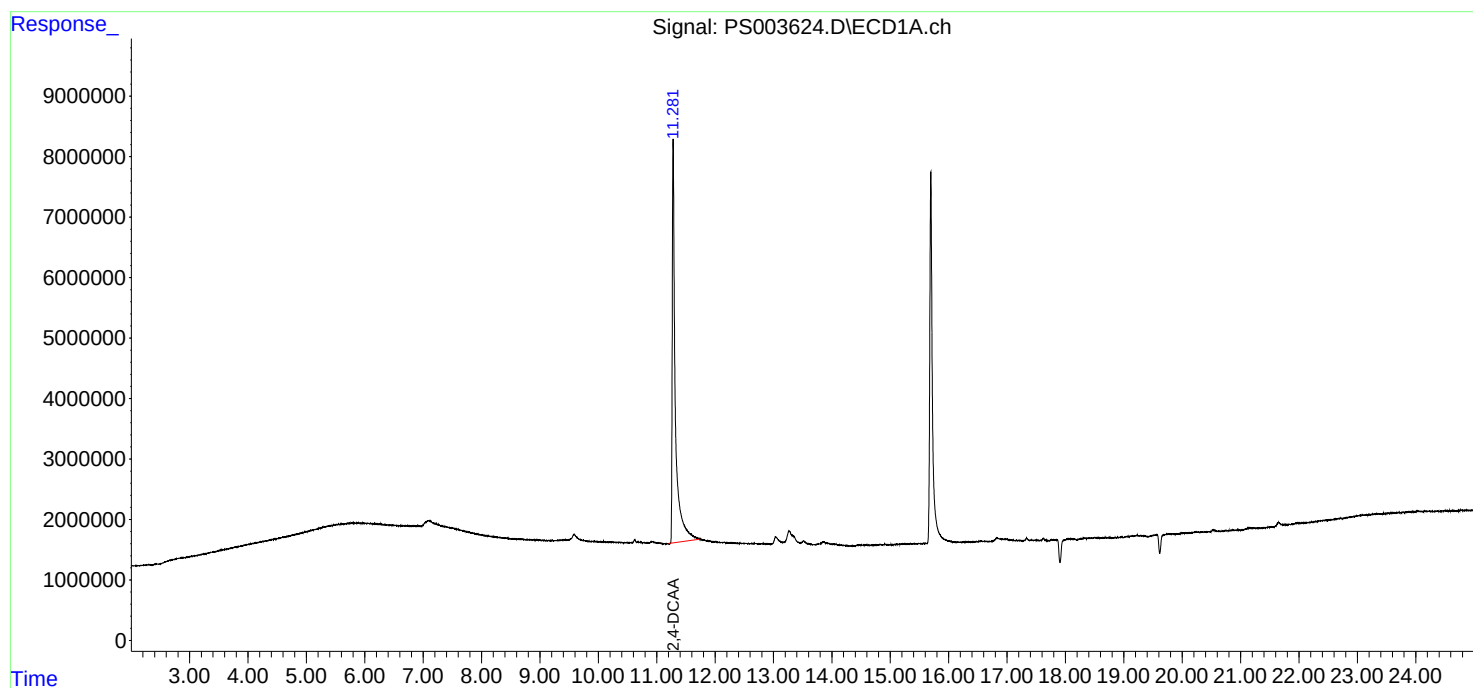


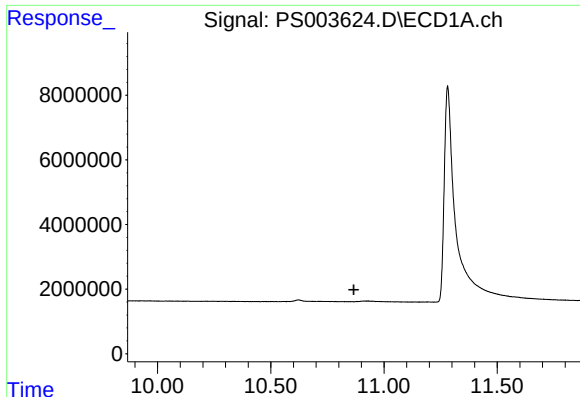

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

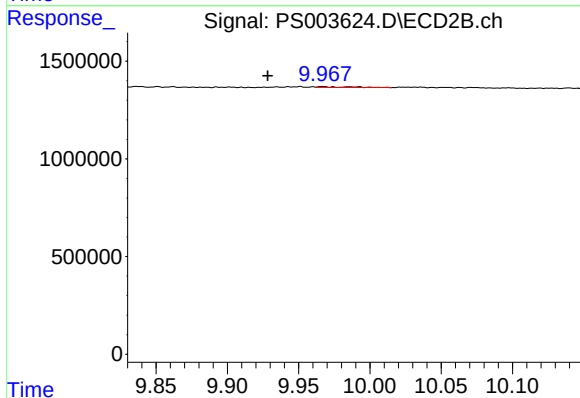


#3 4-Nitrophenol

R.T.: 9.966 min
Delta R.T.: 0.038 min
Response: 62429
Conc: 0.28 ng/ml

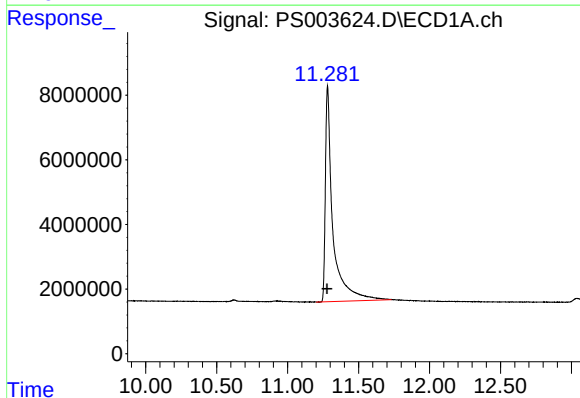


#4 2,4-DCAA

R.T.: 11.281 min
Delta R.T.: 0.004 min
Response: 246224948
Conc: 560.85 ng/ml

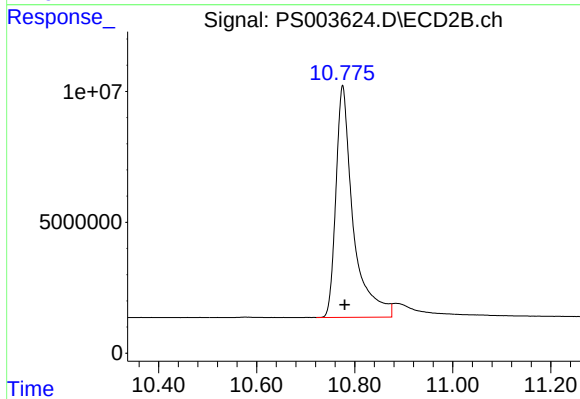

#4 2,4-DCAA


R.T.: 10.776 min
Delta R.T.: -0.004 min
Response: 216064251
Conc: 460.13 ng/ml

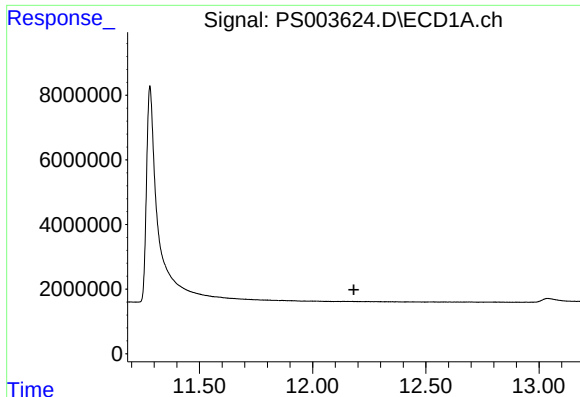

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

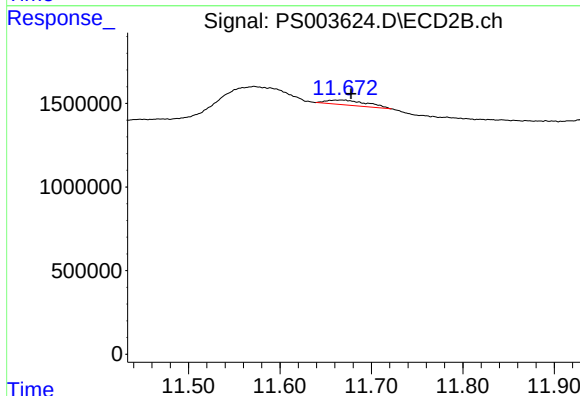


#7 MCPA

R.T.: 11.667 min
Delta R.T.: -0.010 min
Response: 782216
Conc: 0.45 ug/ml

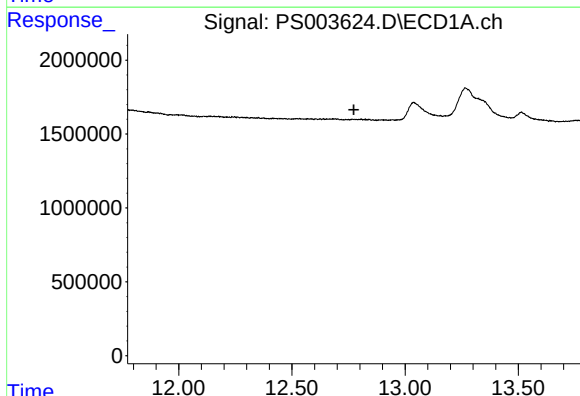


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

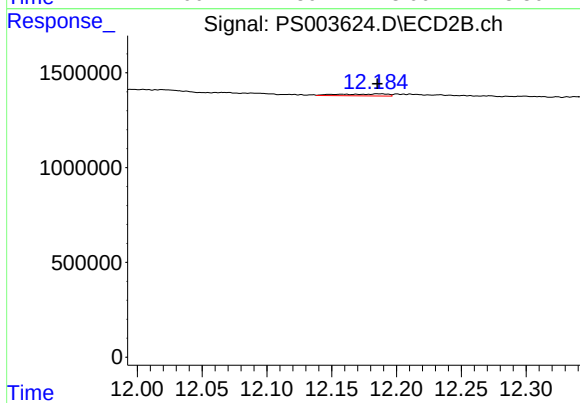

#8 DICHLORPROP


R.T.: 12.187 min
Delta R.T.: 0.002 min
Response: 270312
Conc: 0.65 ng/ml

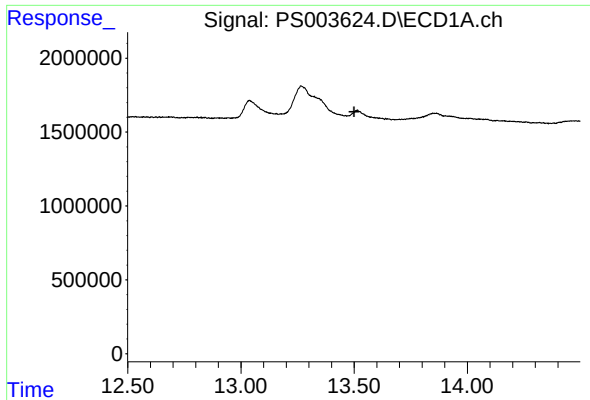

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

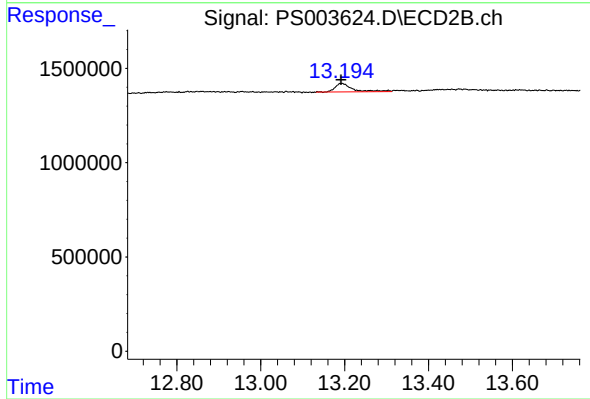


#10 Pentachlorophenol

R.T.: 13.193 min
Delta R.T.: 0.002 min
Response: 1330330
Conc: 0.20 ng/ml

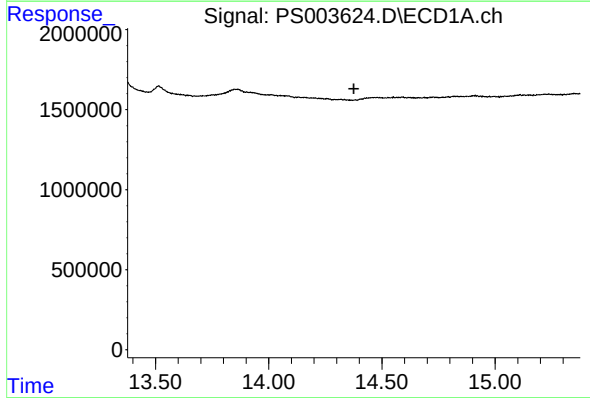


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

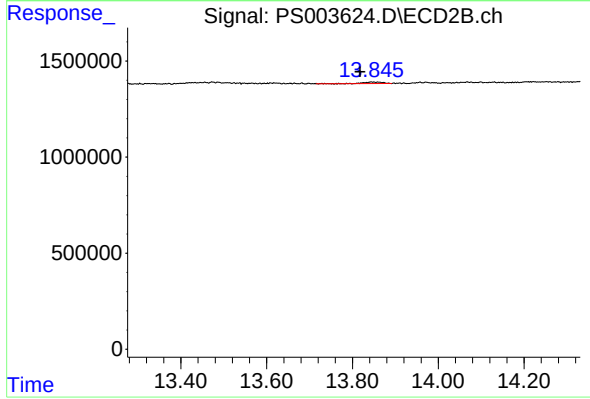

#11 2,4,5-TP (SILVEX)


R.T.: 13.848 min
Delta R.T.: 0.030 min
Response: 232831
Conc: 0.09 ng/ml

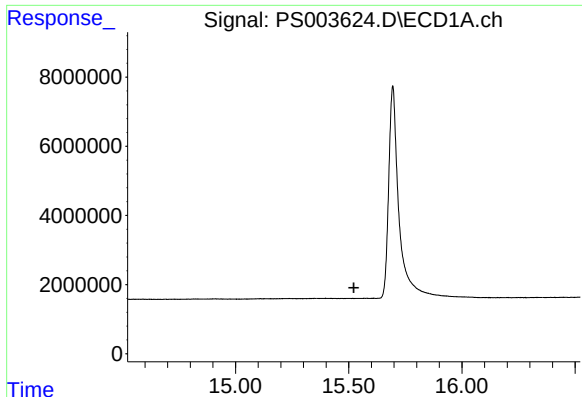

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

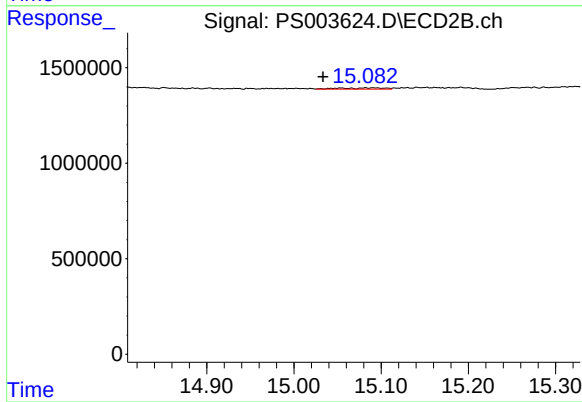


#13 2,4-DB

R.T.: 15.089 min
Delta R.T.: 0.056 min
Response: 254921
Conc: 1.00 ng/ml

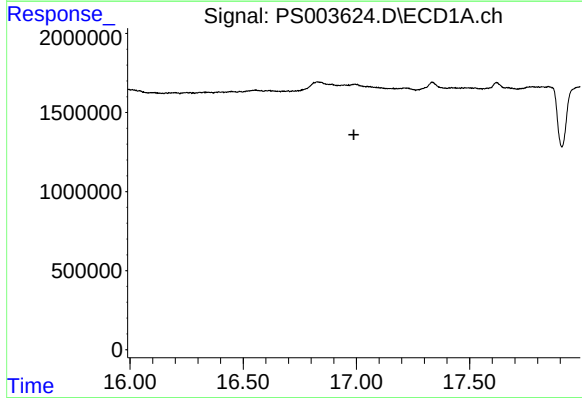


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

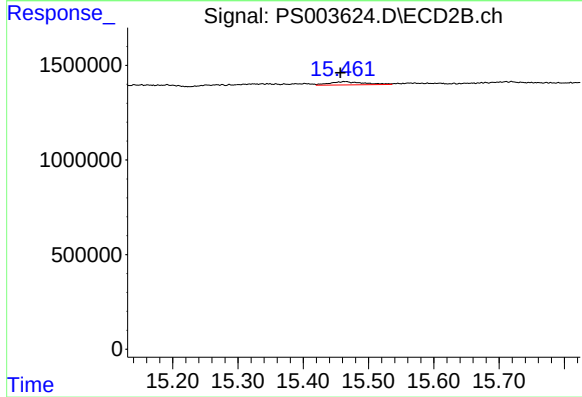

#14 DINOSEB


R.T.: 15.463 min
Delta R.T.: 0.006 min
Response: 642213
Conc: 0.36 ng/ml

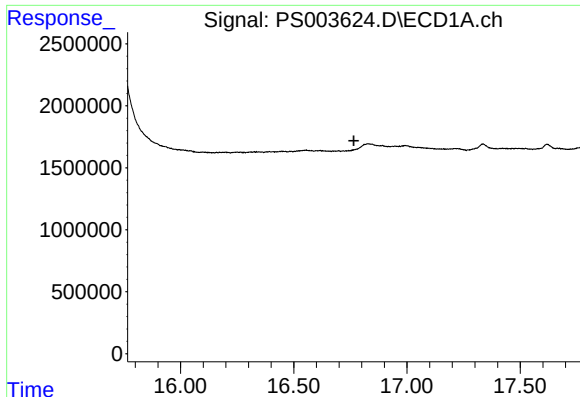

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

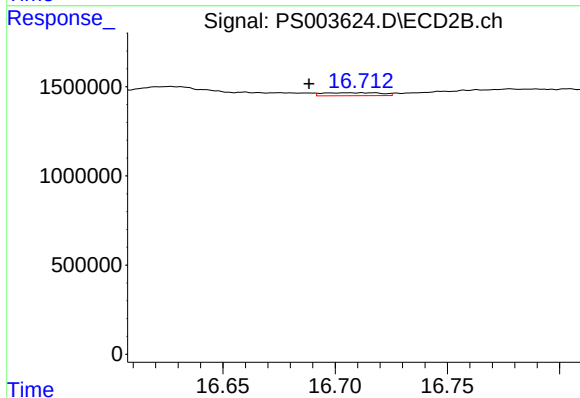


#15 Picloram

R.T.: 16.709 min
Delta R.T.: 0.020 min
Response: 309751
Conc: 0.12 ng/ml

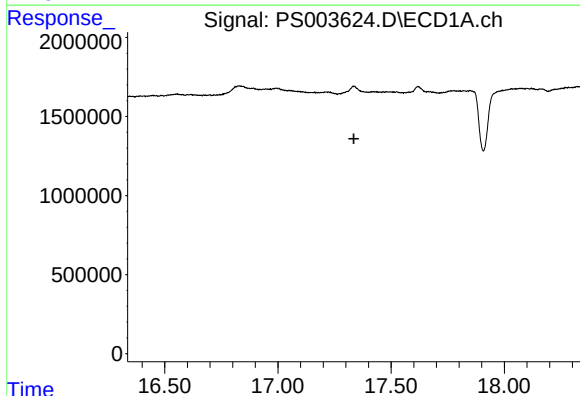

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

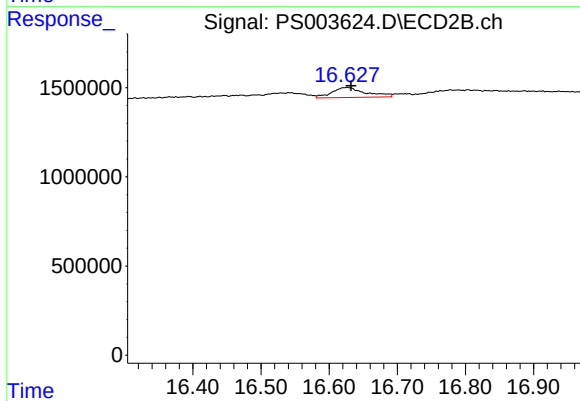

#16 DCPA

R.T.: 16.625 min
Delta R.T.: -0.006 min
Response: 1951562
Conc: 0.63 ng/ml