

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
 Data File : PS003630.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 19:44
 Operator : EI\SJ
 Sample : K1688-32
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:45:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.279	10.775	123.4E6	125.2E6	281.147	266.704
Target Compounds							
1) T	Dalapon	2.791	2.279	35819227	66990751	55.111	105.800 #
2) T	3,5-DICHL...	0.000	8.939	0	7075117	N.D.	11.458 #
3) T	4-Nitroph...	0.000	9.948	0	2786802	N.D.	12.395 #
5) T	DICAMBA	0.000	11.014	0	6621988	N.D.	3.964 #
6) T	MCPD	11.987	0.000	24178040	0	18.416	N.D. #
7) T	MCPA	12.200	0.000	62828728	0	31.675	N.D. #
9) T	2,4-D	0.000	12.631	0	1422914	N.D.	2.711 #
11) T	2,4,5-TP ...	0.000	13.783	0	2085450	N.D.	0.819 #
12) T	2,4,5-T	0.000	14.439	0	9669886	N.D.	4.795 #
13) T	2,4-DB	0.000	15.002	0	3673133	N.D.	14.384 #
14) T	DINOSEB	0.000	15.420	0	3761227	N.D.	2.107 #
15) T	Picloram	0.000	16.731	0	19557539	N.D.	7.705 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
Data File : PS003630.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 19:44
Operator : EI\SJ
Sample : K1688-32
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:45:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

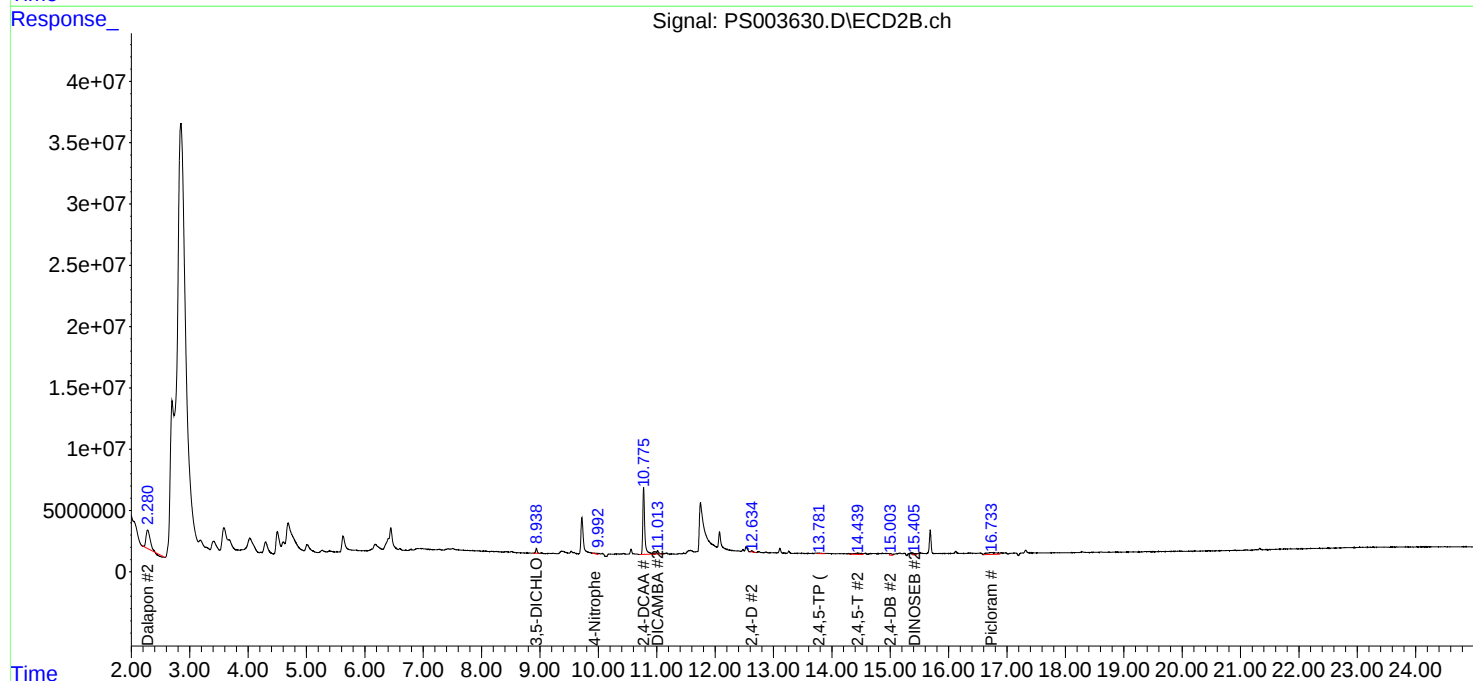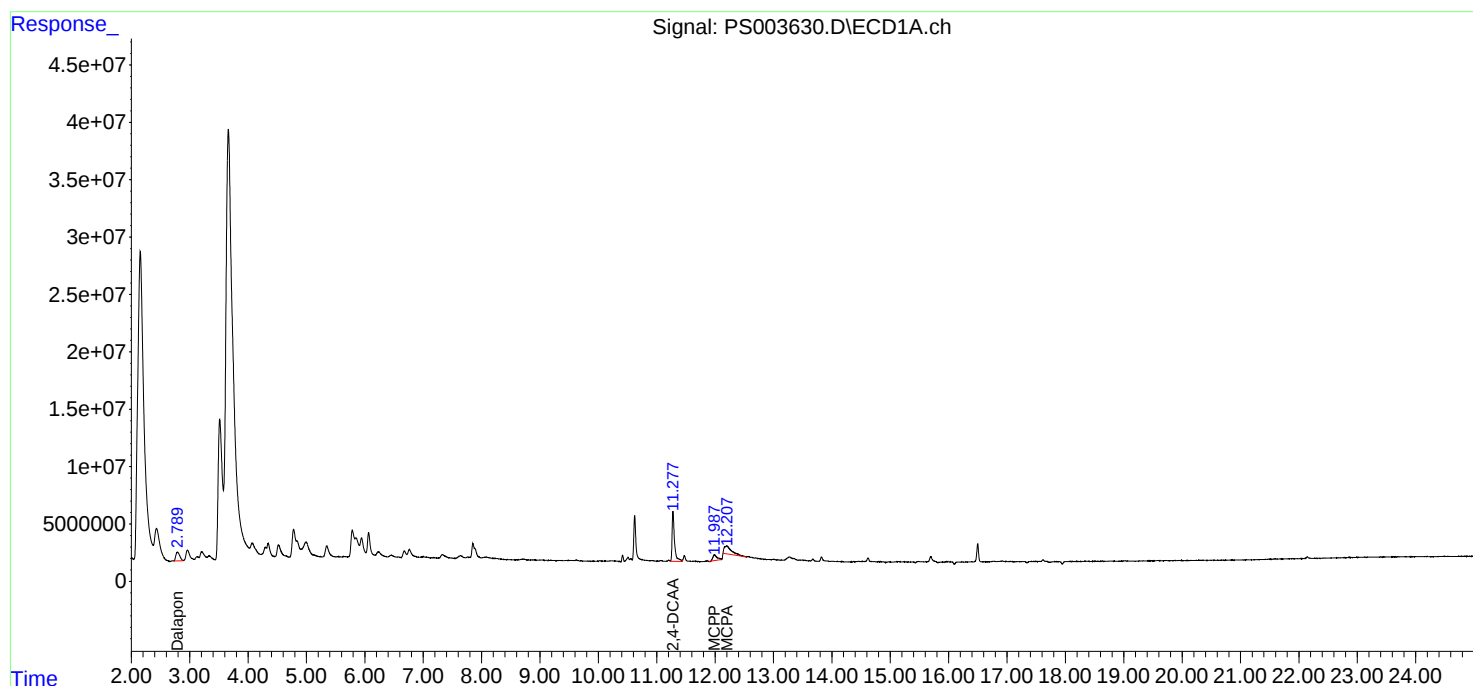


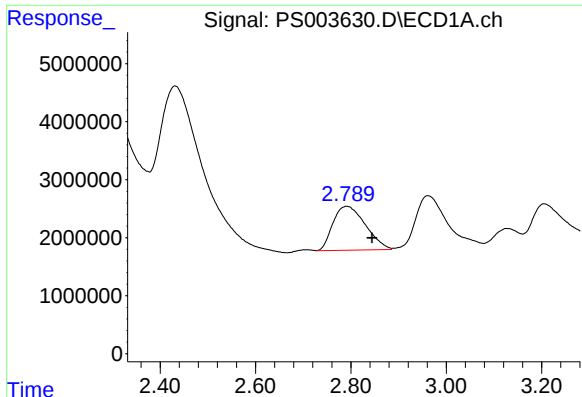

#1 Dalapon


R.T.: 2.791 min
Delta R.T.: -0.053 min
Response: 35819227
Conc: 55.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

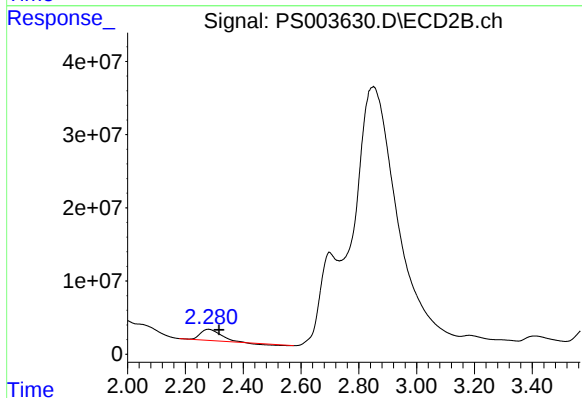


#1 Dalapon

R.T.: 2.279 min
Delta R.T.: -0.037 min
Response: 66990751
Conc: 105.80 ng/ml

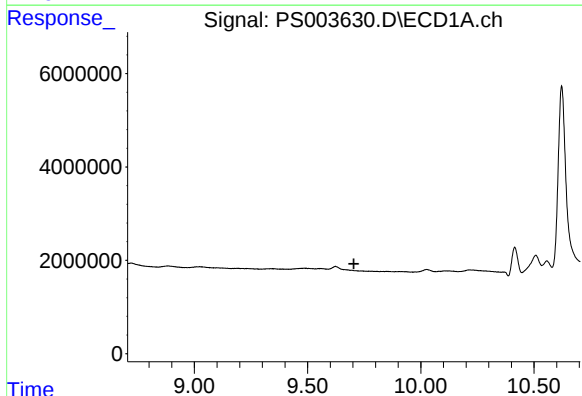


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

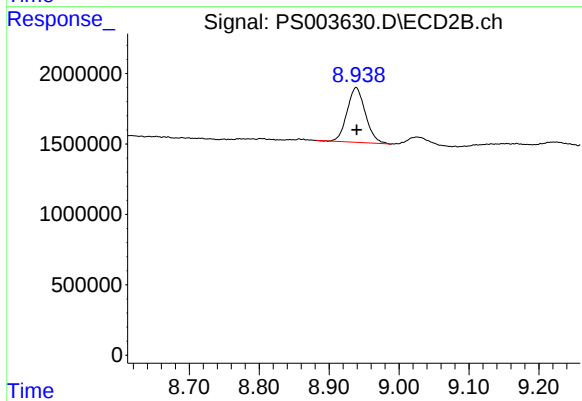

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.939 min
Delta R.T.: 0.000 min
Response: 7075117
Conc: 11.46 ng/ml

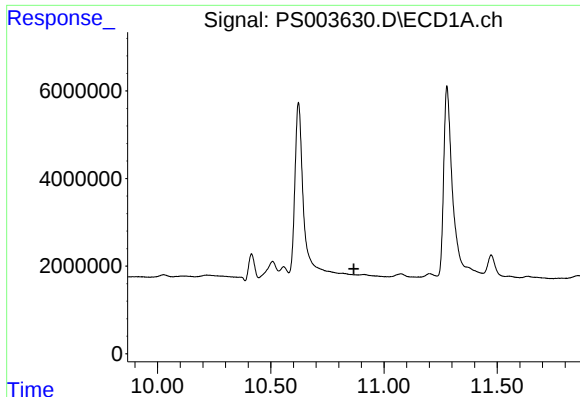

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

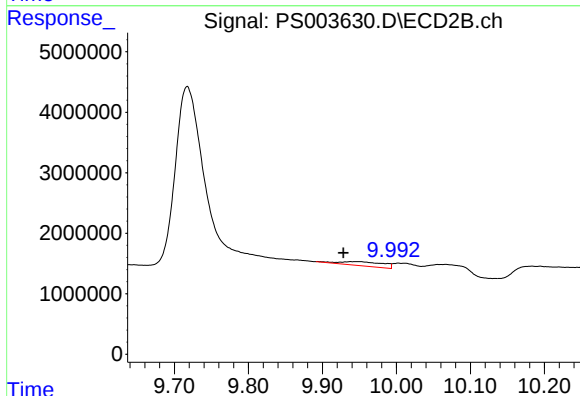


#3 4-Nitrophenol

R.T.: 9.948 min
Delta R.T.: 0.019 min
Response: 2786802
Conc: 12.40 ng/ml

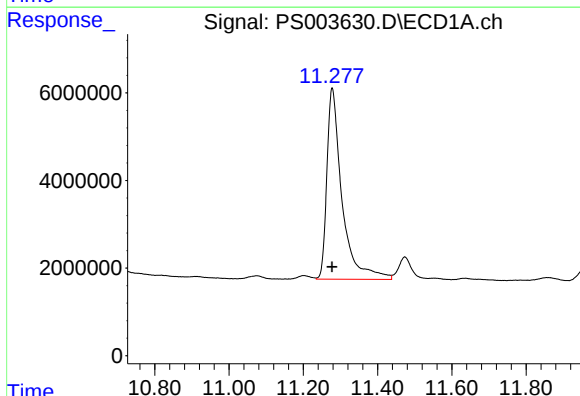


#4 2,4-DCAA

R.T.: 11.279 min
Delta R.T.: 0.001 min
Response: 123430491
Conc: 281.15 ng/ml

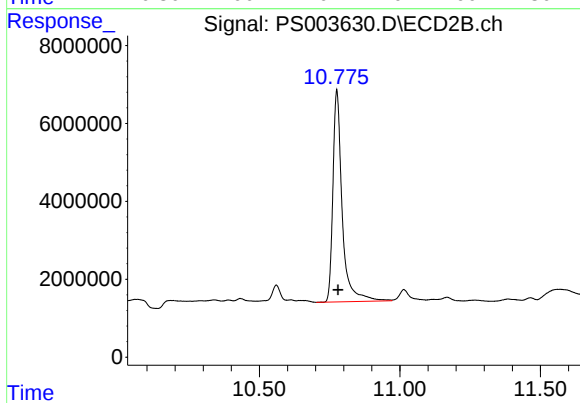

#4 2,4-DCAA


R.T.: 10.775 min
Delta R.T.: -0.004 min
Response: 125235863
Conc: 266.70 ng/ml

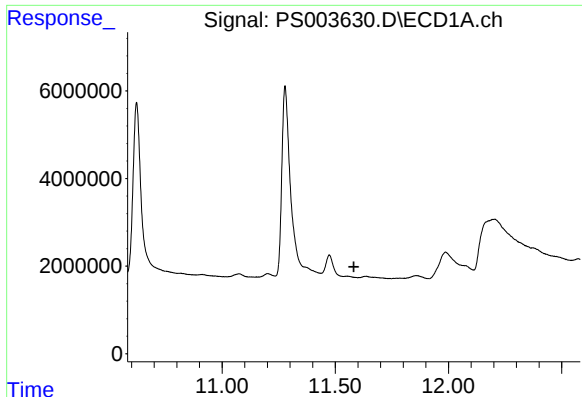

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

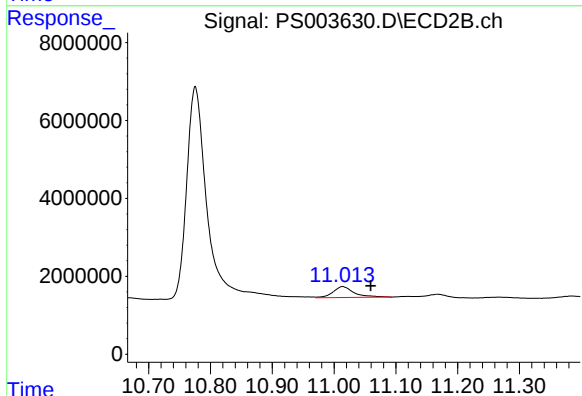


#5 DICAMBA

R.T.: 11.014 min
Delta R.T.: -0.046 min
Response: 6621988
Conc: 3.96 ng/ml

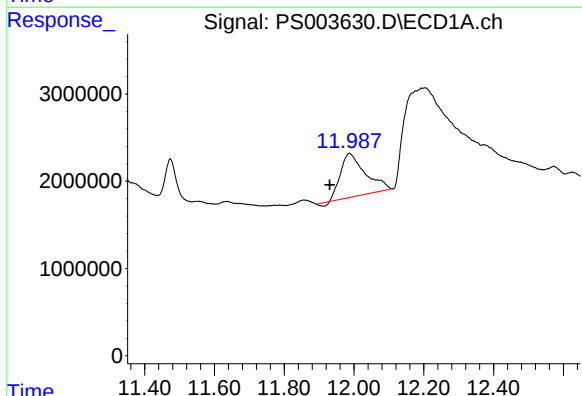


#6 MCP

R.T.: 11.987 min
Delta R.T.: 0.057 min
Response: 24178040
Conc: 18.42 ug/ml

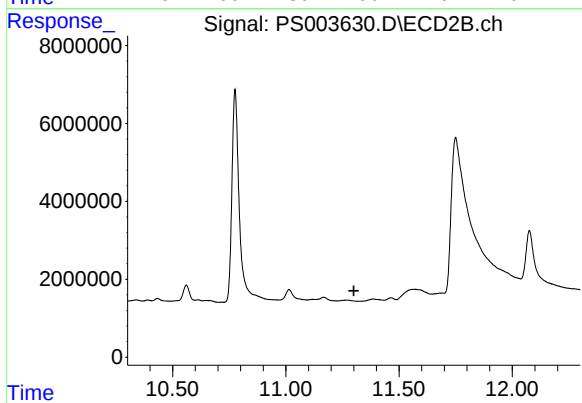

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.300 min
Response: 0
Conc: N.D.

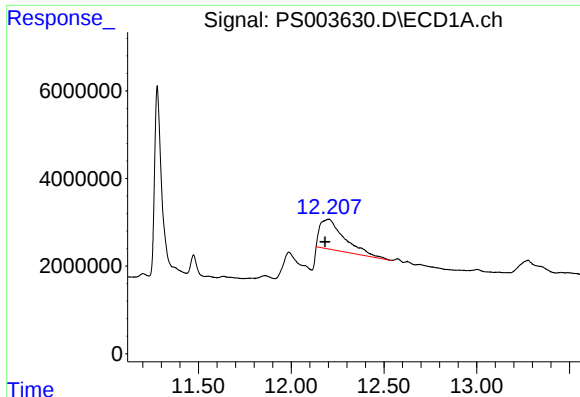

#7 MCPA


R.T.: 12.200 min
Delta R.T.: 0.018 min
Response: 62828728
Conc: 31.67 ug/ml

Instrument :
ECD_S
ClientSampleId :

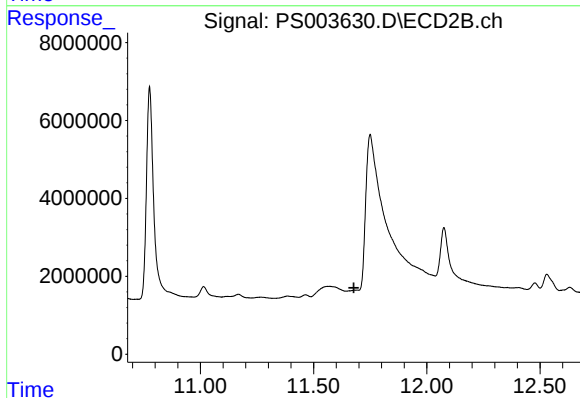


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.678 min
Response: 0
Conc: N.D.

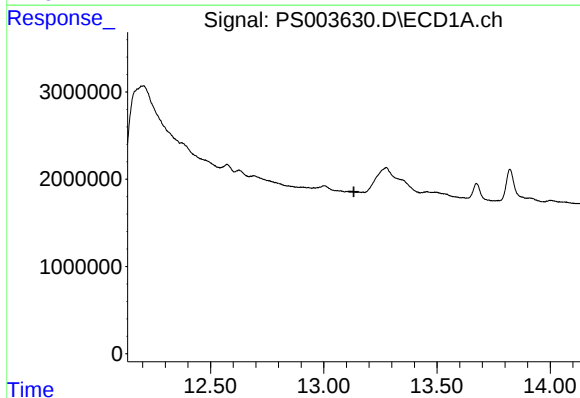


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

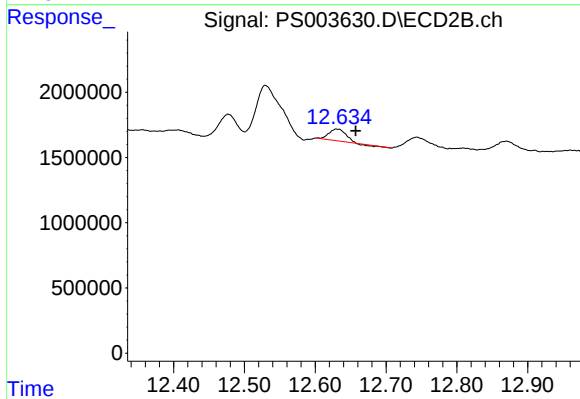

#9 2,4-D


R.T.: 12.631 min
Delta R.T.: -0.026 min
Response: 1422914
Conc: 2.71 ng/ml

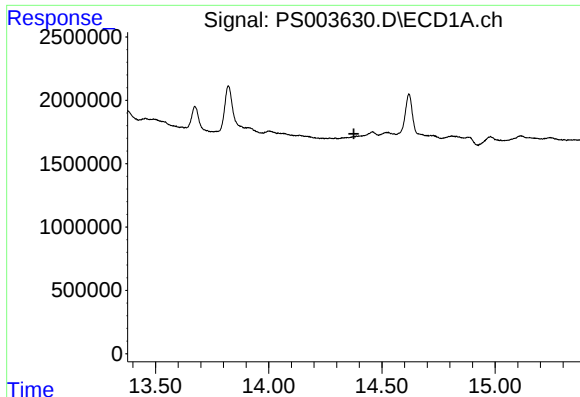

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

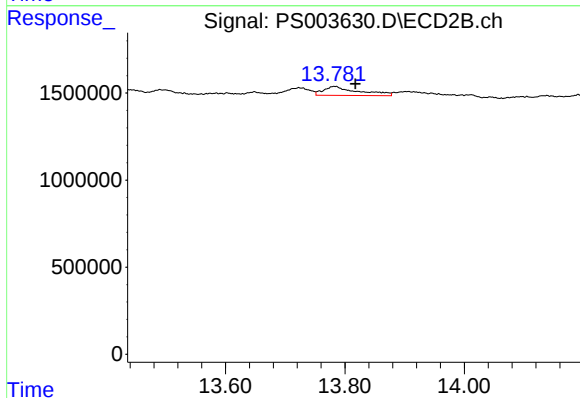


#11 2,4,5-TP (SILVEX)

R.T.: 13.783 min
Delta R.T.: -0.035 min
Response: 2085450
Conc: 0.82 ng/ml

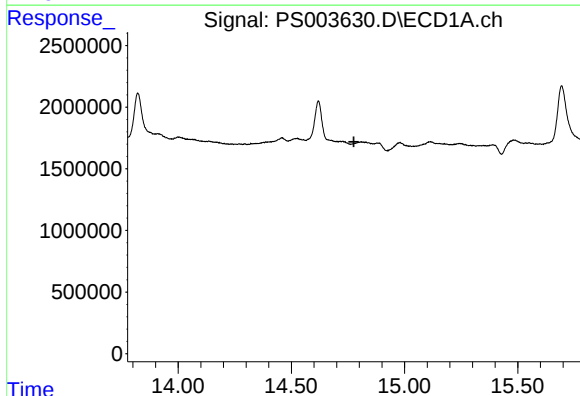


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

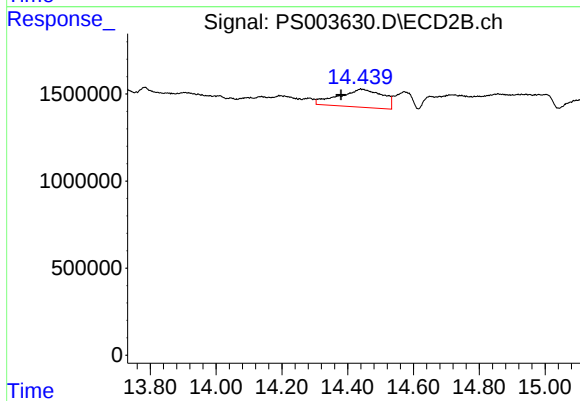

#12 2,4,5-T


R.T.: 14.439 min
Delta R.T.: 0.059 min
Response: 9669886
Conc: 4.79 ng/ml

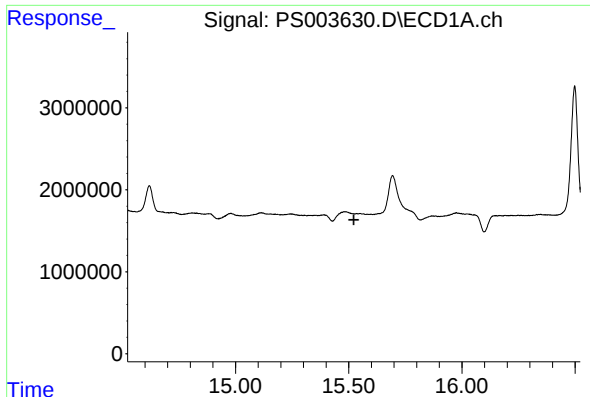

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

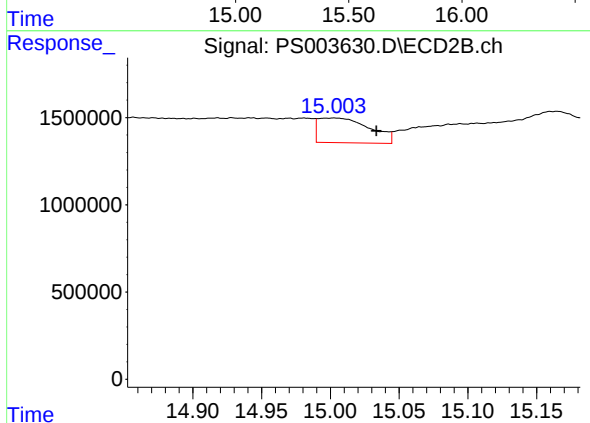


#13 2,4-DB

R.T.: 15.002 min
Delta R.T.: -0.032 min
Response: 3673133
Conc: 14.38 ng/ml

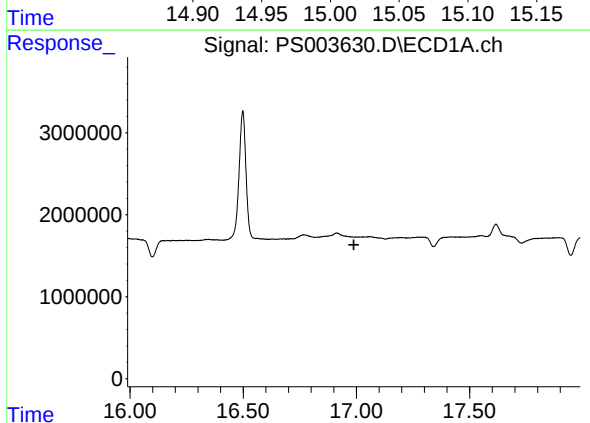


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

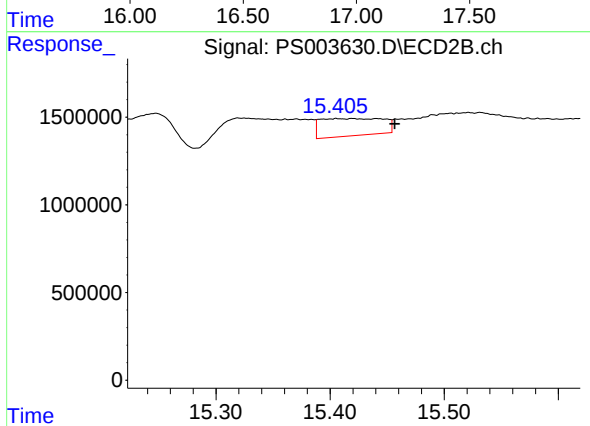

#14 DINOSEB


R.T.: 15.420 min
Delta R.T.: -0.037 min
Response: 3761227
Conc: 2.11 ng/ml

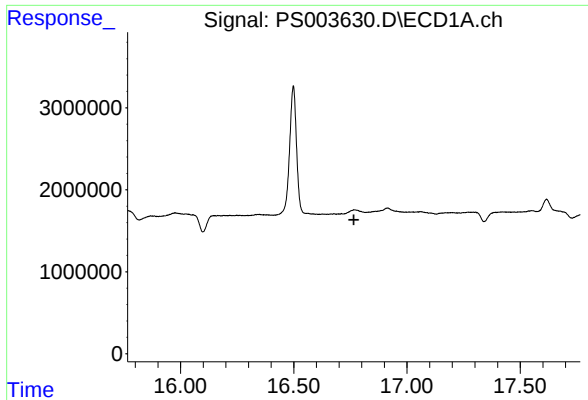

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

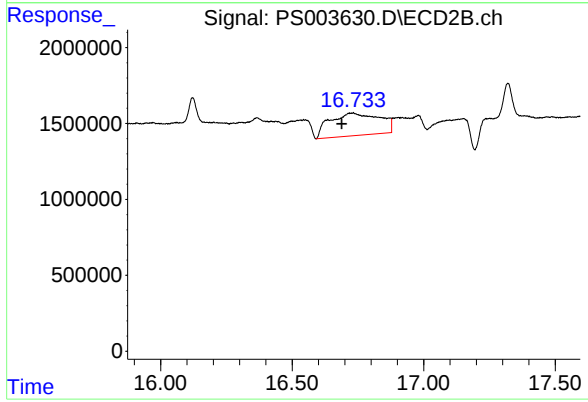

#15 Picloram

R.T.: 16.731 min
Delta R.T.: 0.043 min
Response: 19557539
Conc: 7.71 ng/ml