

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
 Data File : PS003633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 21:18
 Operator : EI\SJ
 Sample : K1688-34
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:46:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.305	10.803	109.6E6	111.8E6	249.646	238.042
Target Compounds							
1) T	Dalapon	2.816	2.310	33659817	60392540	51.789	95.379 #
2) T	3,5-DICHL...	0.000	8.967	0	6292540	N.D.	10.191 #
5) T	DICAMBA	0.000	11.040	0	7377960	N.D.	4.416 #
6) T	MCP	11.986	11.288	46531411	142486	35.441	0.121 #
9) T	2,4-D	0.000	12.661	0	206772	N.D.	0.394 #
11) T	2,4,5-TP ...	0.000	13.804	0	2029472	N.D.	0.797 #
12) T	2,4,5-T	0.000	14.427	0	8014894	N.D.	3.974 #
13) T	2,4-DB	0.000	14.981	0	8283053	N.D.	32.437 #
14) T	DINOSEB	0.000	15.432	0	4122853	N.D.	2.310 #
15) T	Picloram	0.000	16.733	0	14280202	N.D.	5.626 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
Data File : PS003633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 21:18
Operator : EI\SJ
Sample : K1688-34
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:46:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

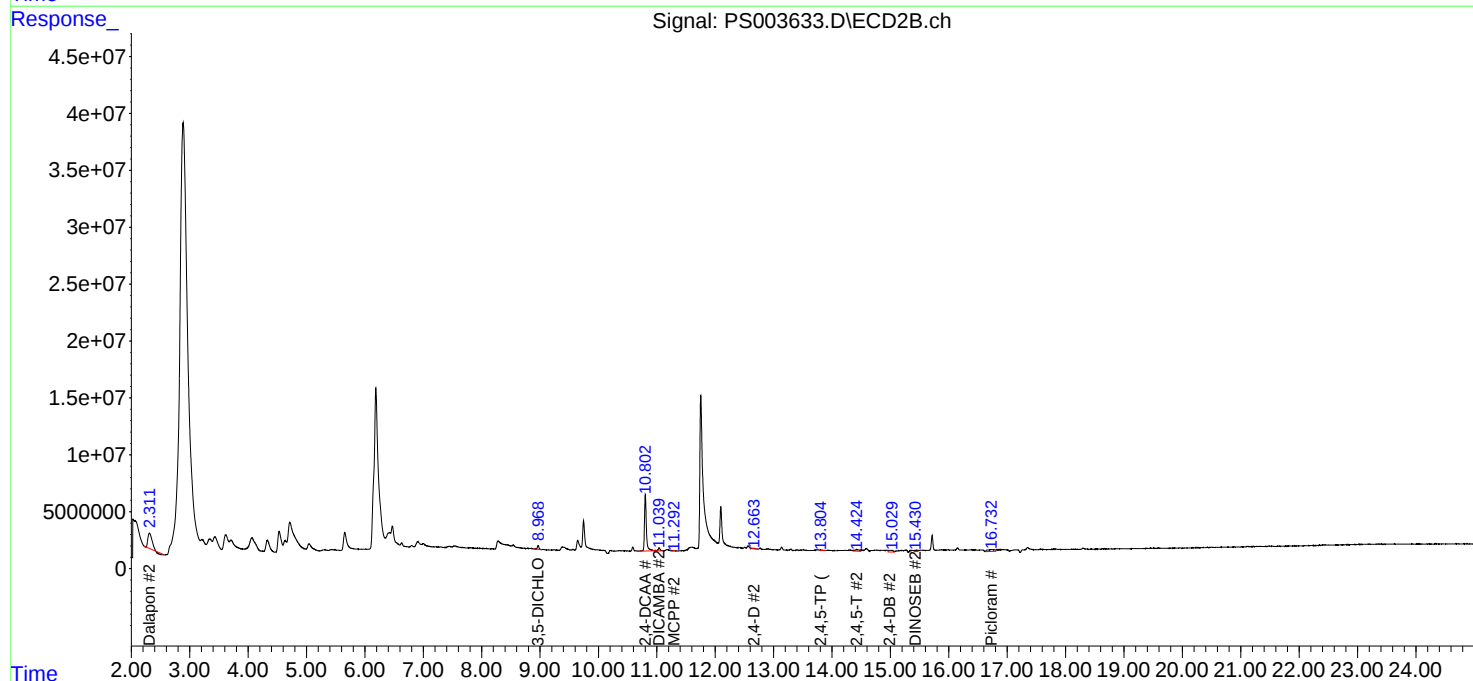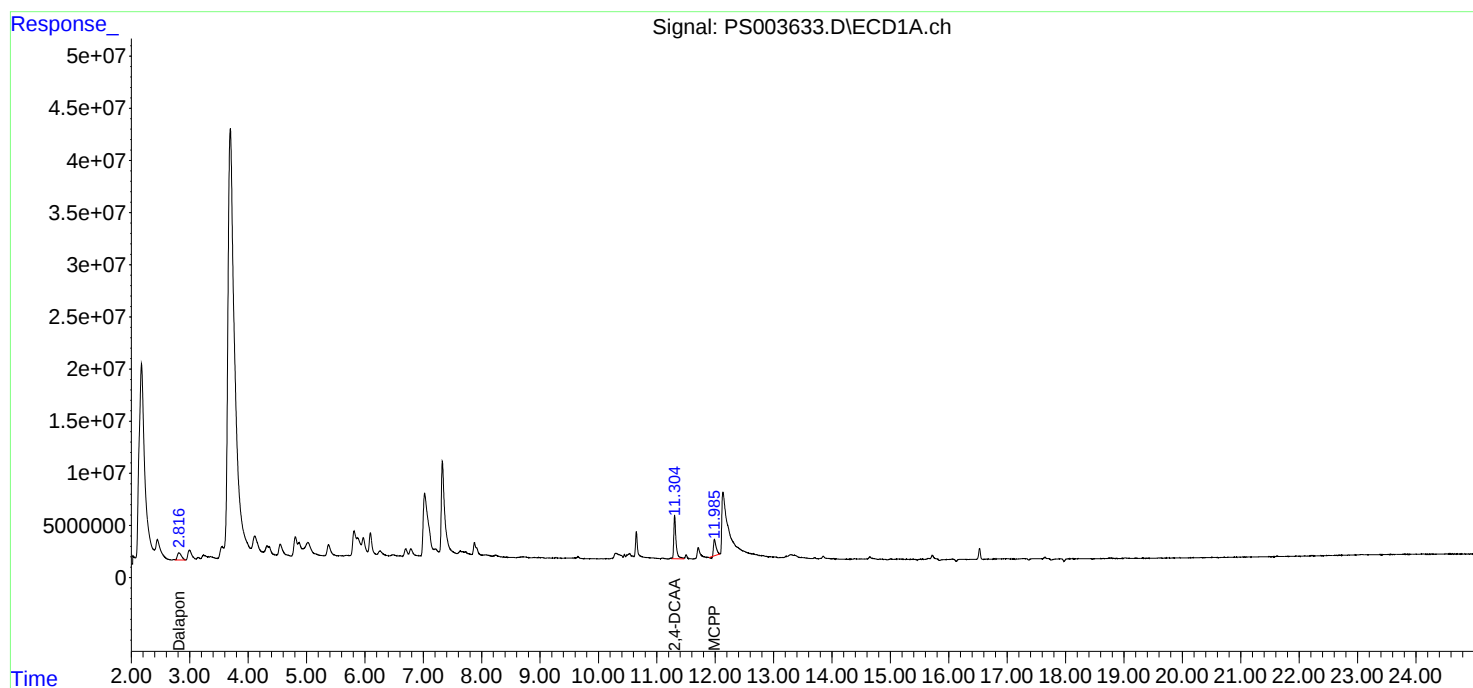


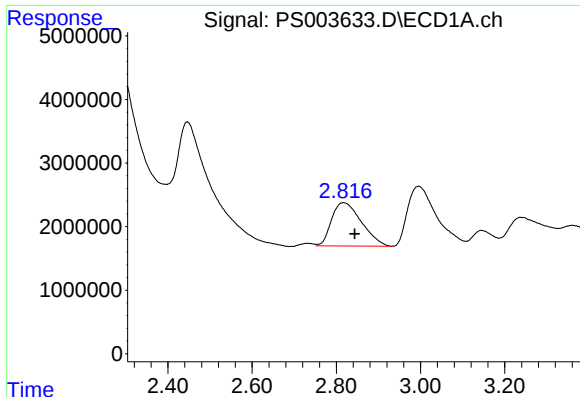

#1 Dalapon


R.T.: 2.816 min
Delta R.T.: -0.028 min
Response: 33659817
Conc: 51.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

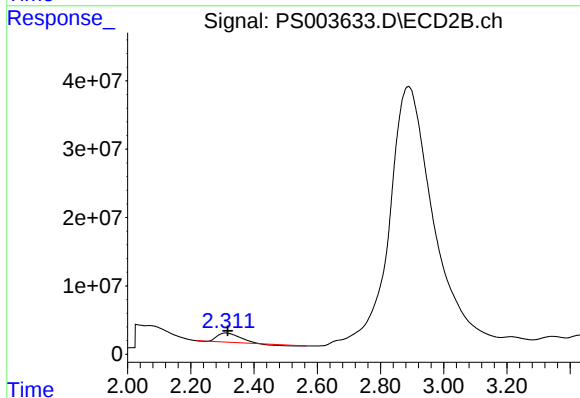


#1 Dalapon

R.T.: 2.310 min
Delta R.T.: -0.007 min
Response: 60392540
Conc: 95.38 ng/ml

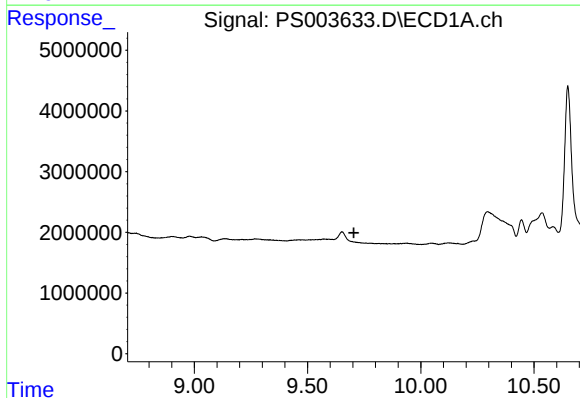


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

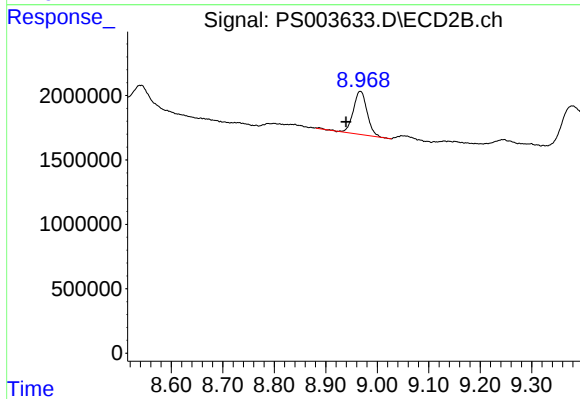

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.967 min
Delta R.T.: 0.028 min
Response: 6292540
Conc: 10.19 ng/ml

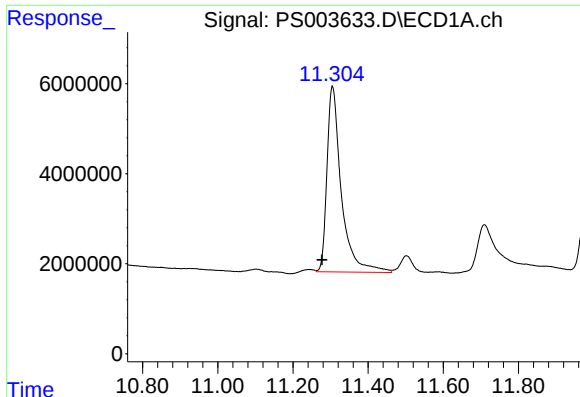

#4 2,4-DCAA


R.T.: 11.305 min
Delta R.T.: 0.028 min
Response: 109600682
Conc: 249.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

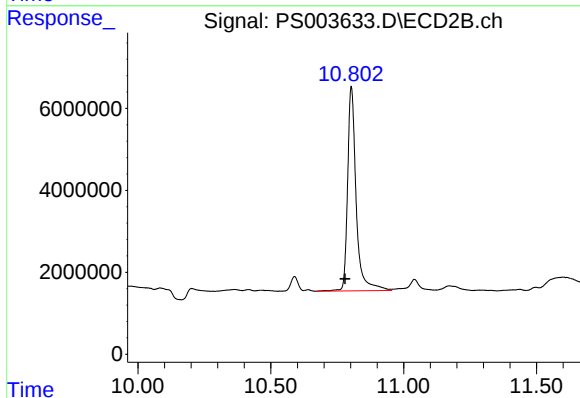


#4 2,4-DCAA

R.T.: 10.803 min
Delta R.T.: 0.023 min
Response: 111777327
Conc: 238.04 ng/ml

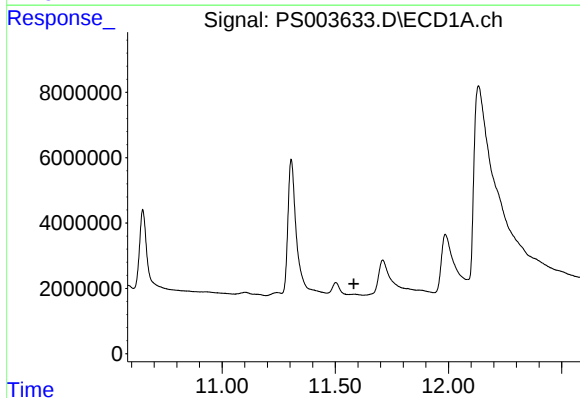


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

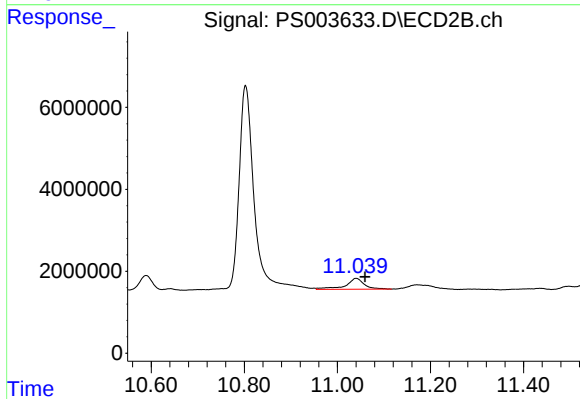

#5 DICAMBA


R.T.: 11.040 min
Delta R.T.: -0.019 min
Response: 7377960
Conc: 4.42 ng/ml

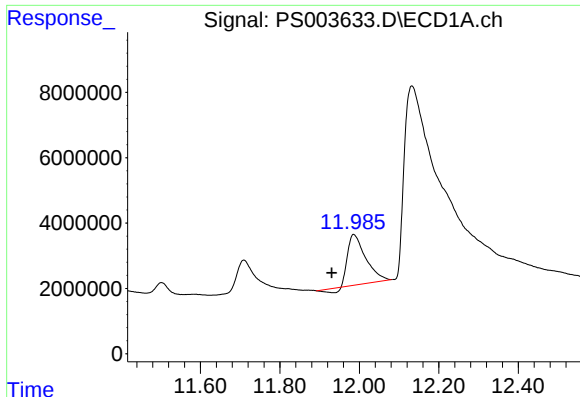

#6 MCP


R.T.: 11.986 min
Delta R.T.: 0.055 min
Response: 46531411
Conc: 35.44 ug/ml

Instrument :
ECD_S
ClientSampleId :

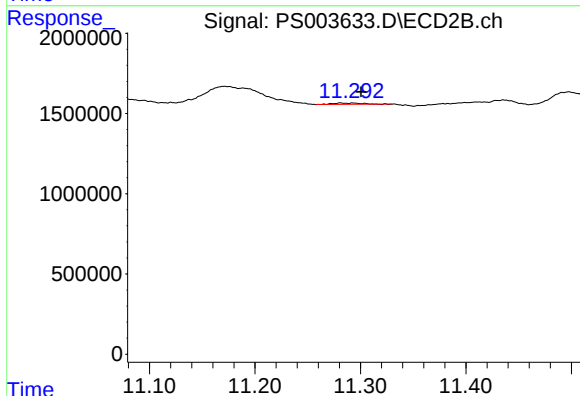


#6 MCP

R.T.: 11.288 min
Delta R.T.: -0.012 min
Response: 142486
Conc: 0.12 ug/ml

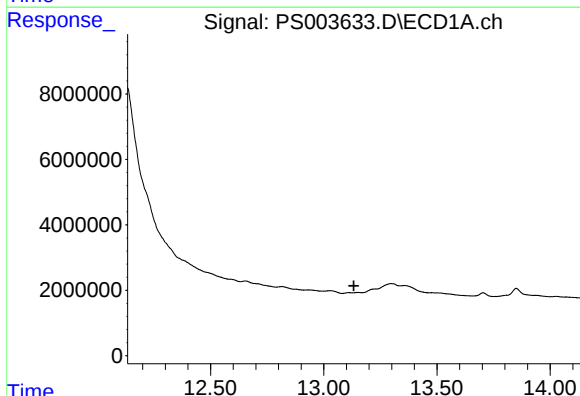


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

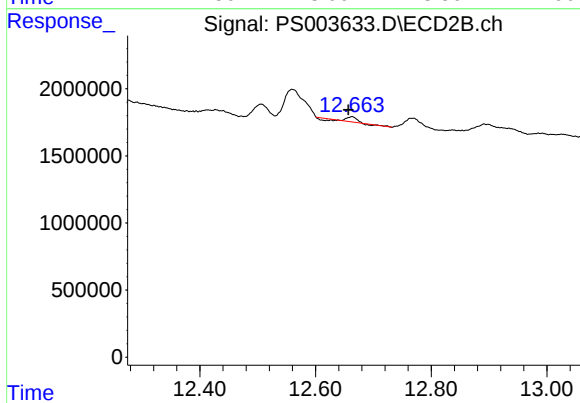

#9 2,4-D


R.T.: 12.661 min
Delta R.T.: 0.004 min
Response: 206772
Conc: 0.39 ng/ml

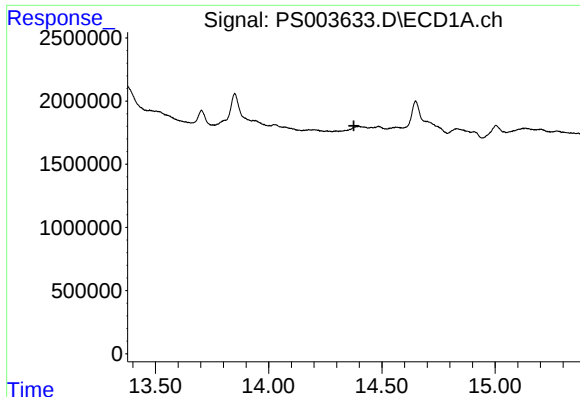

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

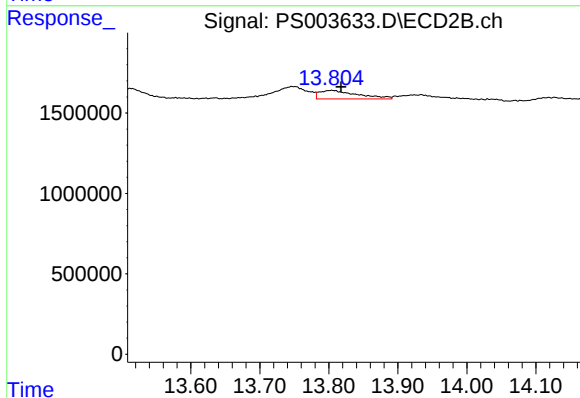


#11 2,4,5-TP (SILVEX)

R.T.: 13.804 min
Delta R.T.: -0.014 min
Response: 2029472
Conc: 0.80 ng/ml

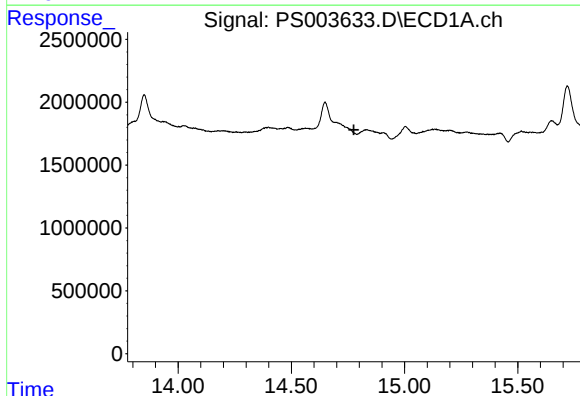


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

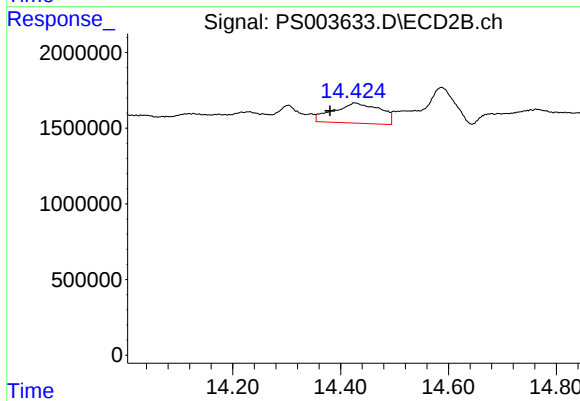

#12 2,4,5-T


R.T.: 14.427 min
Delta R.T.: 0.047 min
Response: 8014894
Conc: 3.97 ng/ml

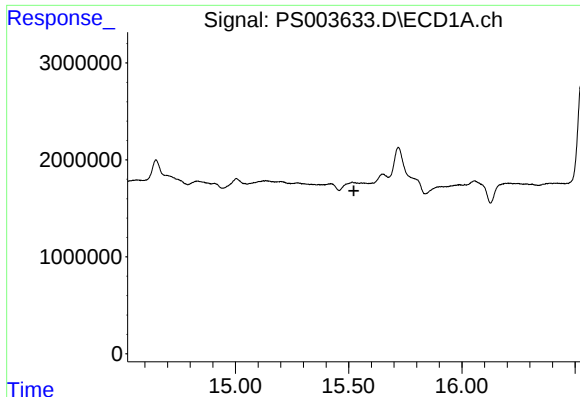

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

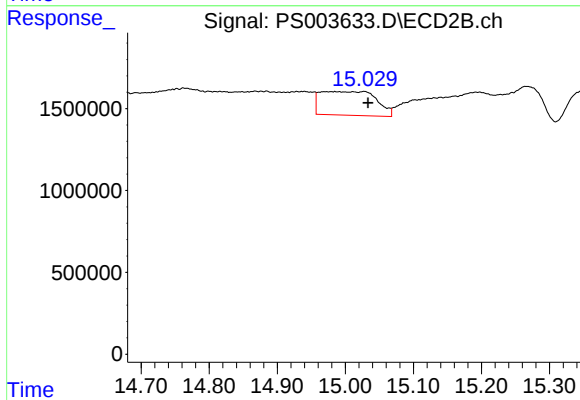


#13 2,4-DB

R.T.: 14.981 min
Delta R.T.: -0.053 min
Response: 8283053
Conc: 32.44 ng/ml

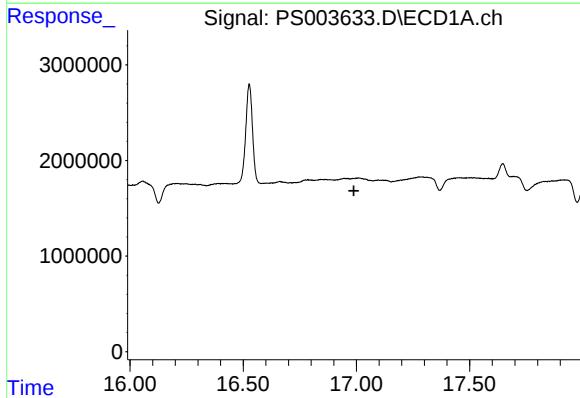


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

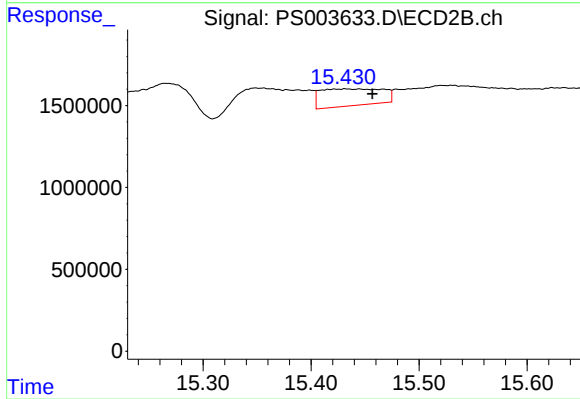

#14 DINOSEB


R.T.: 15.432 min
Delta R.T.: -0.024 min
Response: 4122853
Conc: 2.31 ng/ml

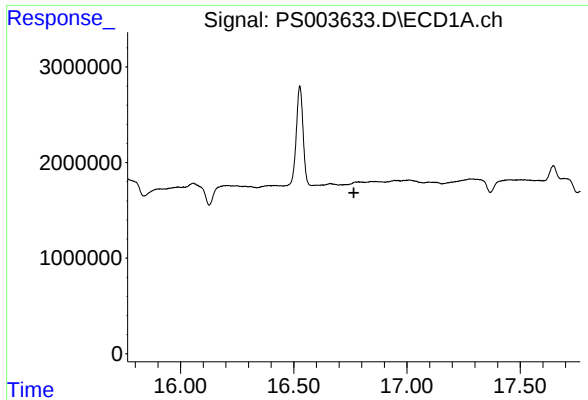

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

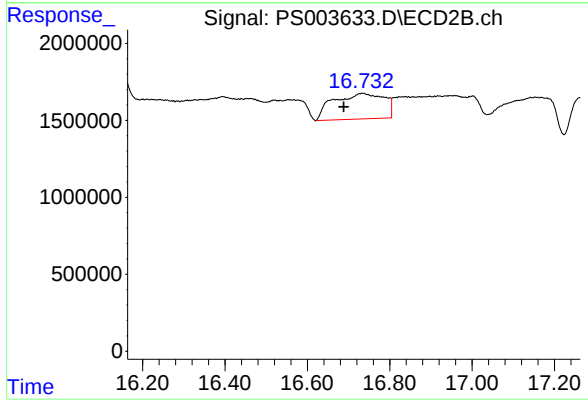

#15 Picloram

R.T.: 16.733 min
Delta R.T.: 0.045 min
Response: 14280202
Conc: 5.63 ng/ml