

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
 Data File : PS003634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 21:49
 Operator : EI\SJ
 Sample : K1688-36
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:46:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.291	10.790	132.2E6	133.3E6	301.020	283.878
Target Compounds							
1) T	Dalapon	2.805	2.295	36255749	67740876	55.783	106.984 #
2) T	3,5-DICHL...	0.000	8.953	0	5534951	N.D.	8.964 #
3) T	4-Nitroph...	0.000	9.959	0	5909448	N.D.	26.284 #
5) T	DICAMBA	0.000	11.028	0	7835193	N.D.	4.690 #
6) T	MCP	0.000	11.271	0	190116	N.D.	0.161 #
9) T	2,4-D	0.000	12.639	0	3185590	N.D.	6.069 #
11) T	2,4,5-TP ...	0.000	13.798	0	1513037	N.D.	0.594 #
13) T	2,4-DB	0.000	15.015	0	4957422	N.D.	19.414 #
14) T	DINOSEB	0.000	15.432	0	3797621	N.D.	2.128 #
15) T	Picloram	0.000	16.743	0	10139105	N.D.	3.995 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
Data File : PS003634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 21:49
Operator : EI\SJ
Sample : K1688-36
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:46:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

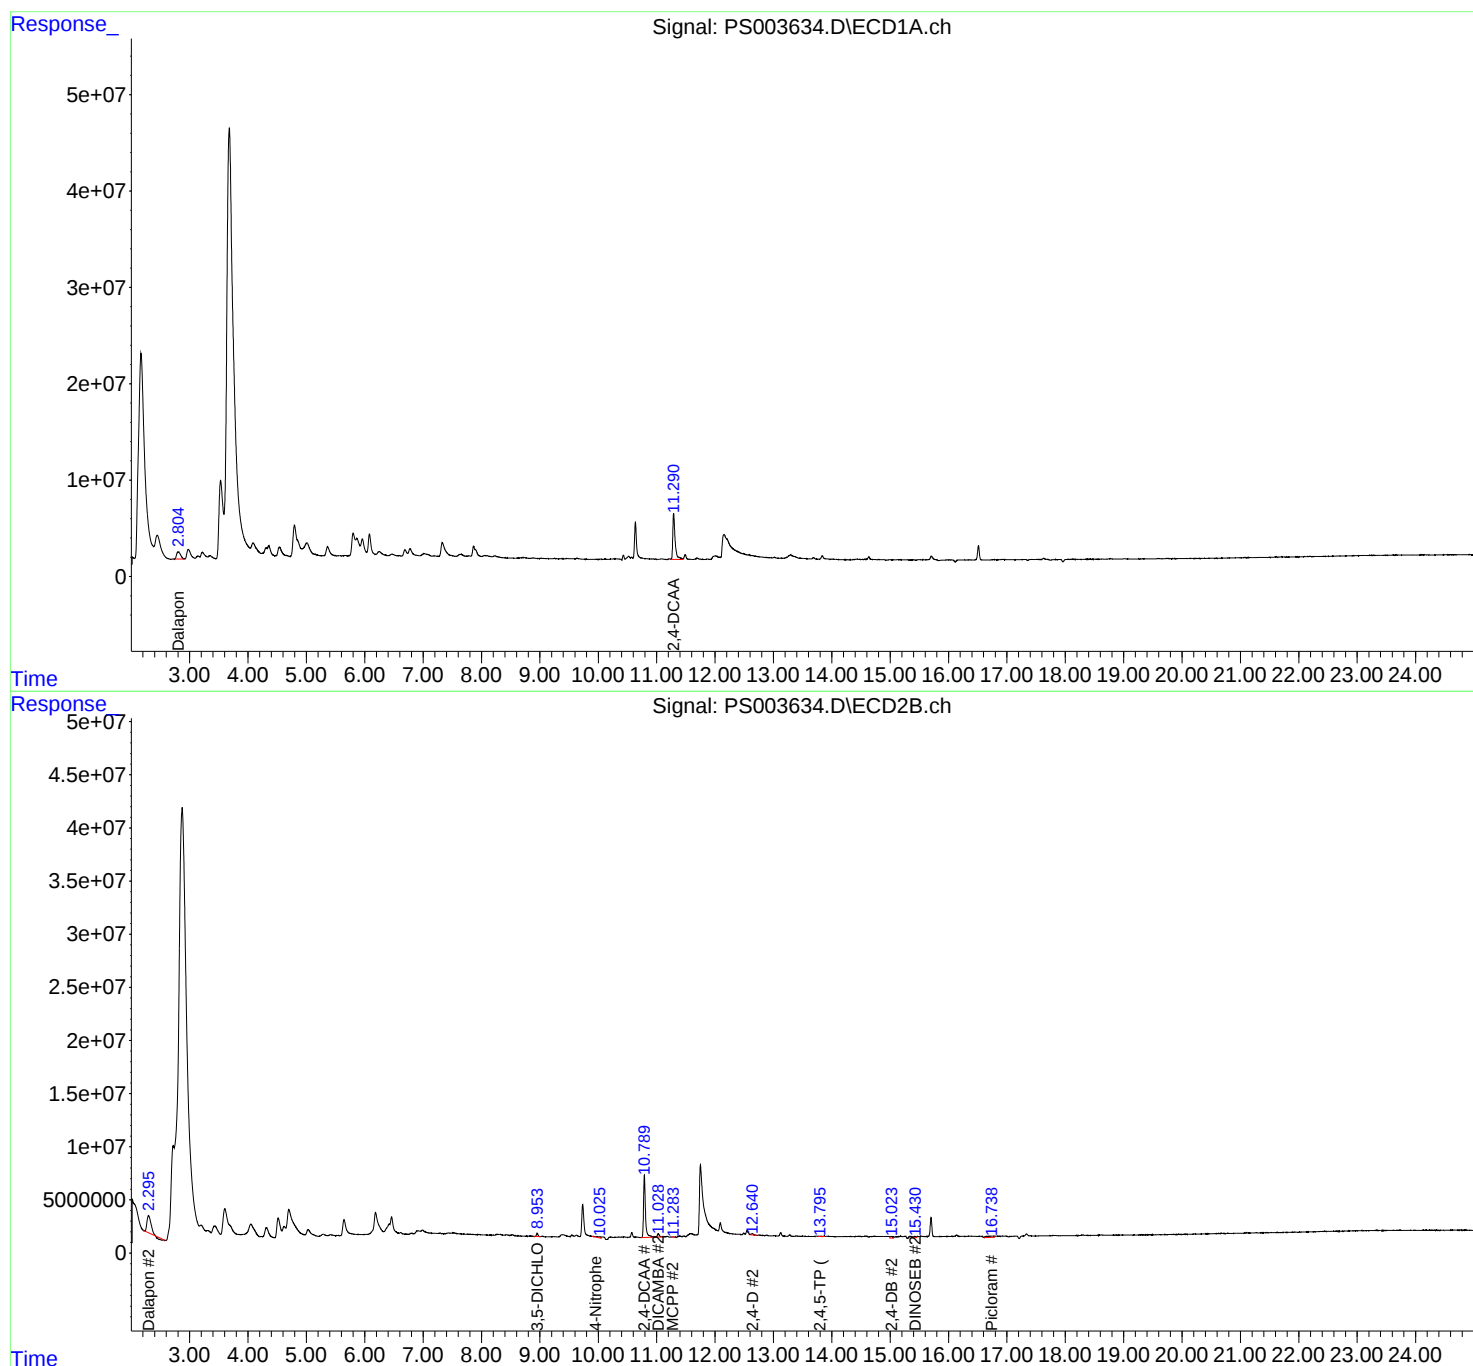


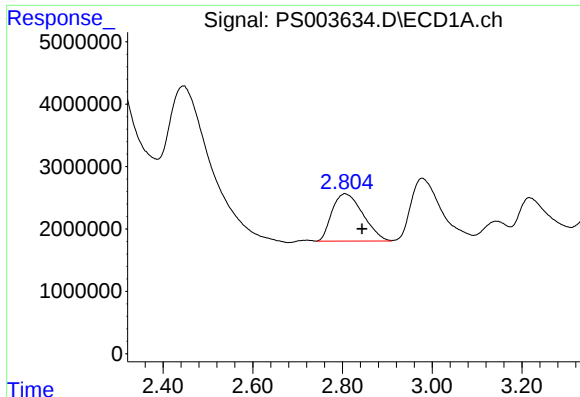

#1 Dalapon


R.T.: 2.805 min
Delta R.T.: -0.039 min
Response: 36255749
Conc: 55.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

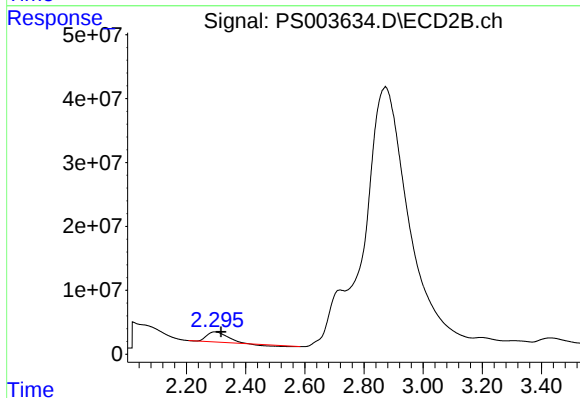


#1 Dalapon

R.T.: 2.295 min
Delta R.T.: -0.021 min
Response: 67740876
Conc: 106.98 ng/ml

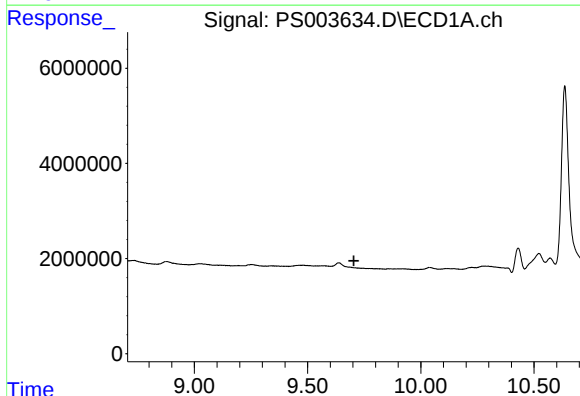


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

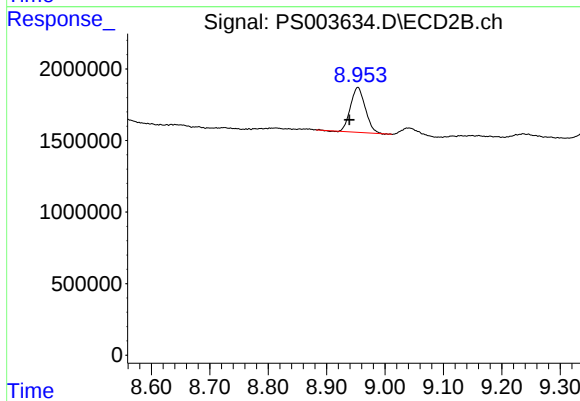

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.953 min
Delta R.T.: 0.014 min
Response: 5534951
Conc: 8.96 ng/ml

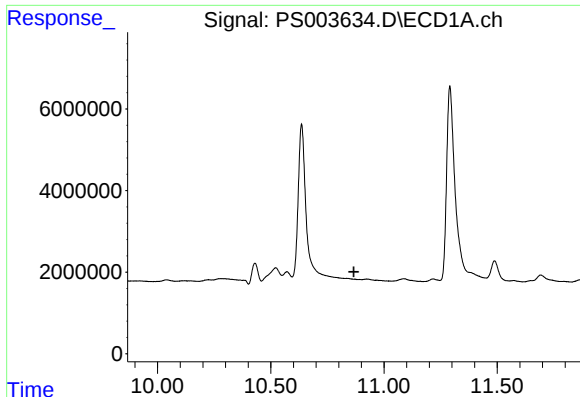

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

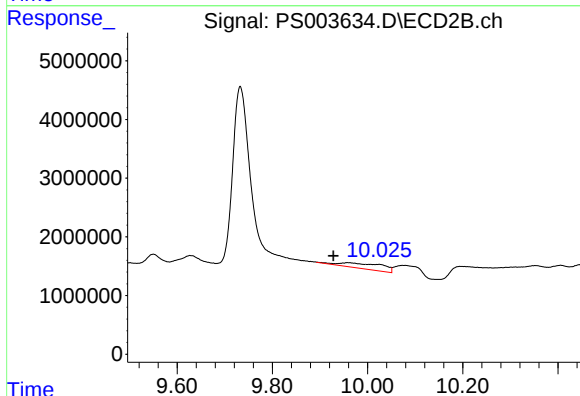


#3 4-Nitrophenol

R.T.: 9.959 min
Delta R.T.: 0.030 min
Response: 5909448
Conc: 26.28 ng/ml

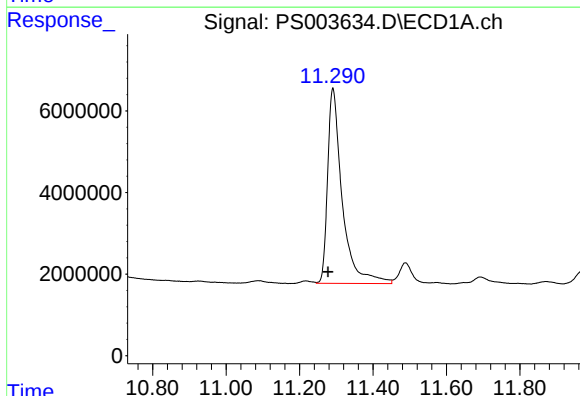


#4 2,4-DCAA

R.T.: 11.291 min
Delta R.T.: 0.013 min
Response: 132155275
Conc: 301.02 ng/ml

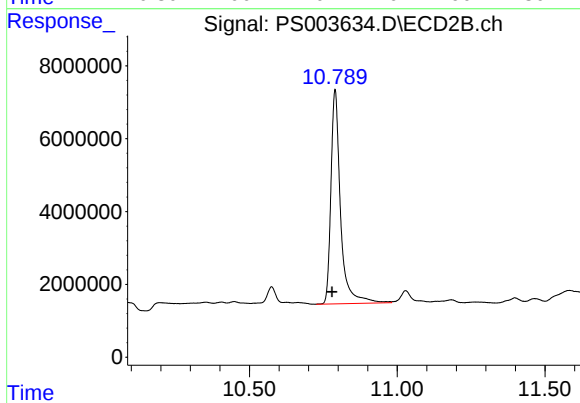

#4 2,4-DCAA


R.T.: 10.790 min
Delta R.T.: 0.010 min
Response: 133300527
Conc: 283.88 ng/ml

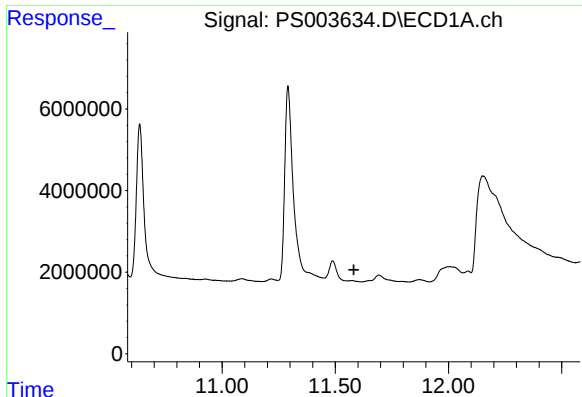

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

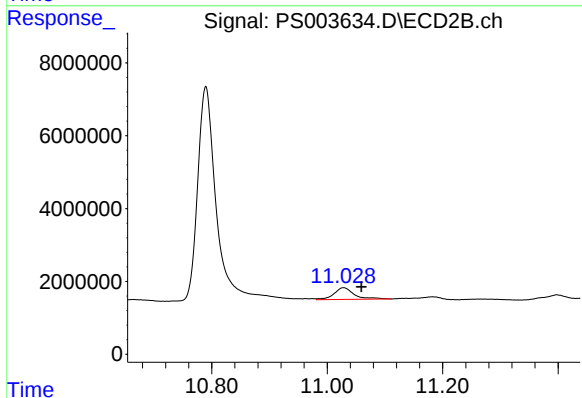


#5 DICAMBA

R.T.: 11.028 min
Delta R.T.: -0.031 min
Response: 7835193
Conc: 4.69 ng/ml

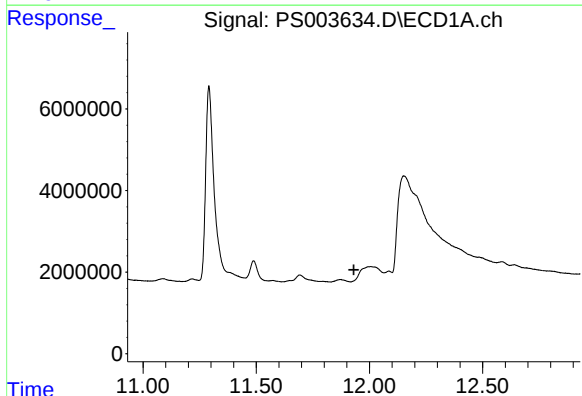


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.931 min
Response: 0
Conc: N.D.

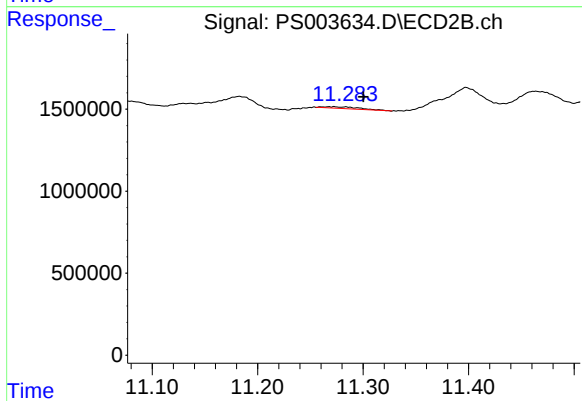

#6 MCP


R.T.: 11.271 min
Delta R.T.: -0.029 min
Response: 190116
Conc: 0.16 ug/ml

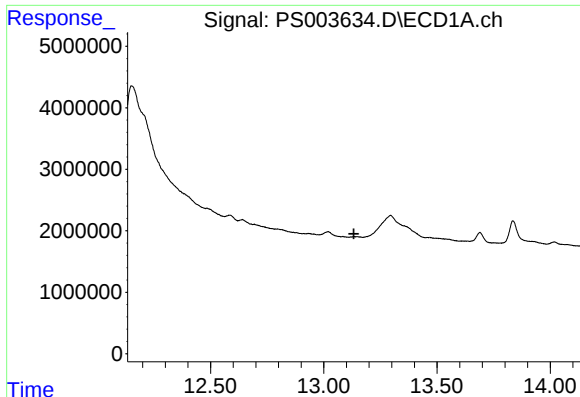

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

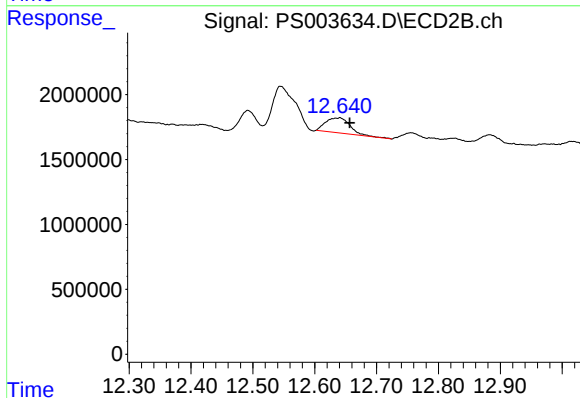


#9 2,4-D

R.T.: 12.639 min
Delta R.T.: -0.018 min
Response: 3185590
Conc: 6.07 ng/ml

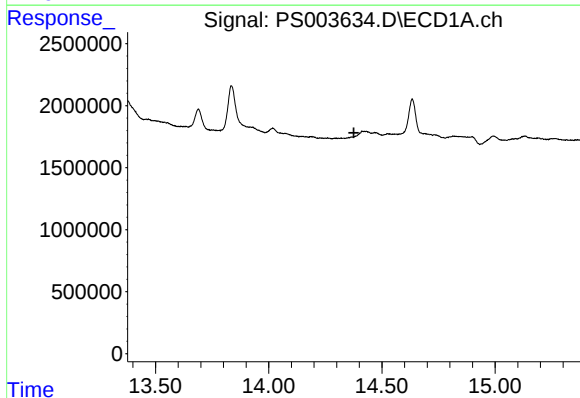


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

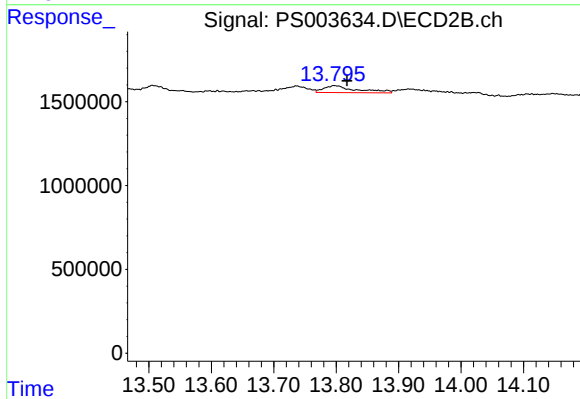

#11 2,4,5-TP (SILVEX)


R.T.: 13.798 min
Delta R.T.: -0.020 min
Response: 1513037
Conc: 0.59 ng/ml

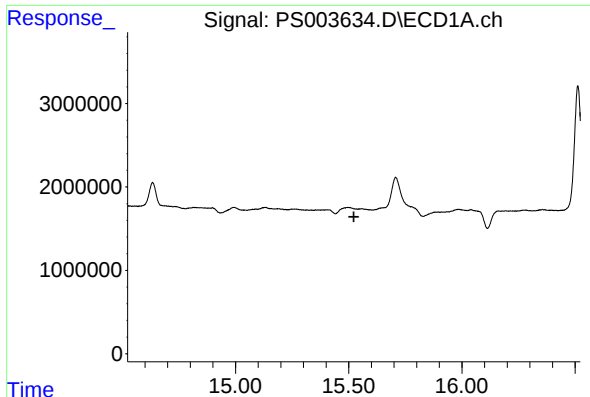

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

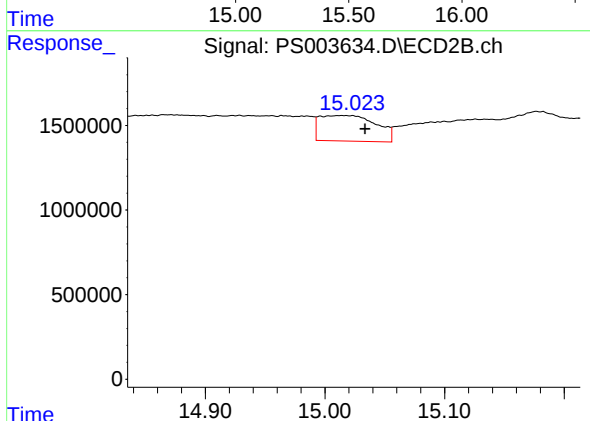


#13 2,4-DB

R.T.: 15.015 min
Delta R.T.: -0.019 min
Response: 4957422
Conc: 19.41 ng/ml

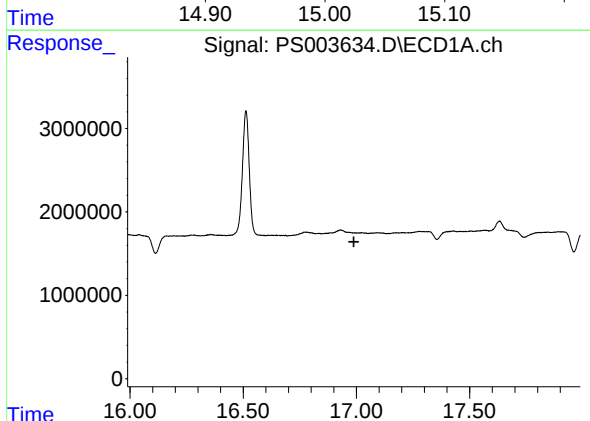


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

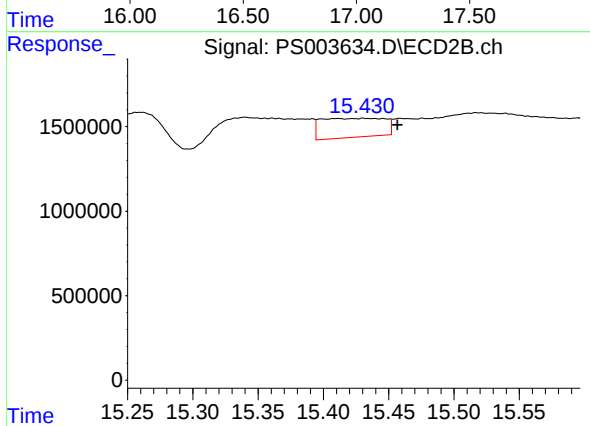

#14 DINOSEB


R.T.: 15.432 min
Delta R.T.: -0.025 min
Response: 3797621
Conc: 2.13 ng/ml

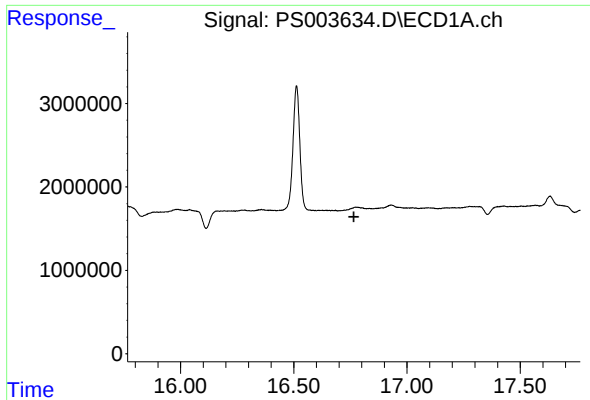

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

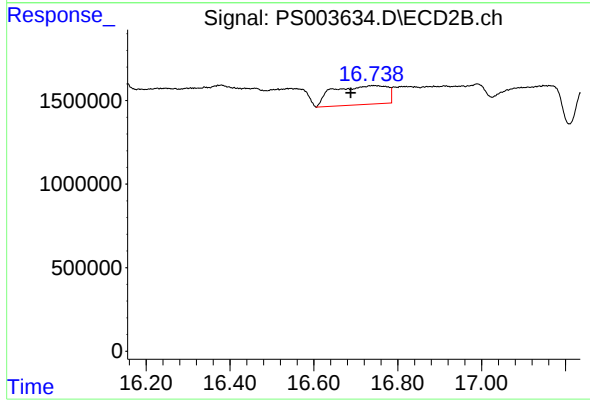

#15 Picloram

R.T.: 16.743 min
Delta R.T.: 0.055 min
Response: 10139105
Conc: 3.99 ng/ml