

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
 Data File : PS003635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 22:20
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:47:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.288	10.784	253.3E6	242.7E6	577.027	516.837
Target Compounds							
2) T	3,5-DICHL...	0.000	8.999	0	51467	N.D.	0.083 #
3) T	4-Nitroph...	0.000	9.968	0	168972	N.D.	0.752 #
7) T	MCPA	0.000	11.675	0	637669	N.D.	0.370 #
8) T	DICHLORPROP	0.000	12.178	0	1791580	N.D.	4.335 #
10) T	Pentachlo...	0.000	13.201	0	1150599	N.D.	0.175 #
11) T	2,4,5-TP ...	0.000	13.859	0	173378	N.D.	0.068 #
13) T	2,4-DB	0.000	15.043	0	270503	N.D.	1.059 #
14) T	DINOSEB	0.000	15.461	0	1283236	N.D.	0.719 #
15) T	Picloram	0.000	16.634	0	772037	N.D.	0.304 #
16) T	DCPA	0.000	16.634	0	772037	N.D.	0.248 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
Data File : PS003635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 22:20
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:47:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

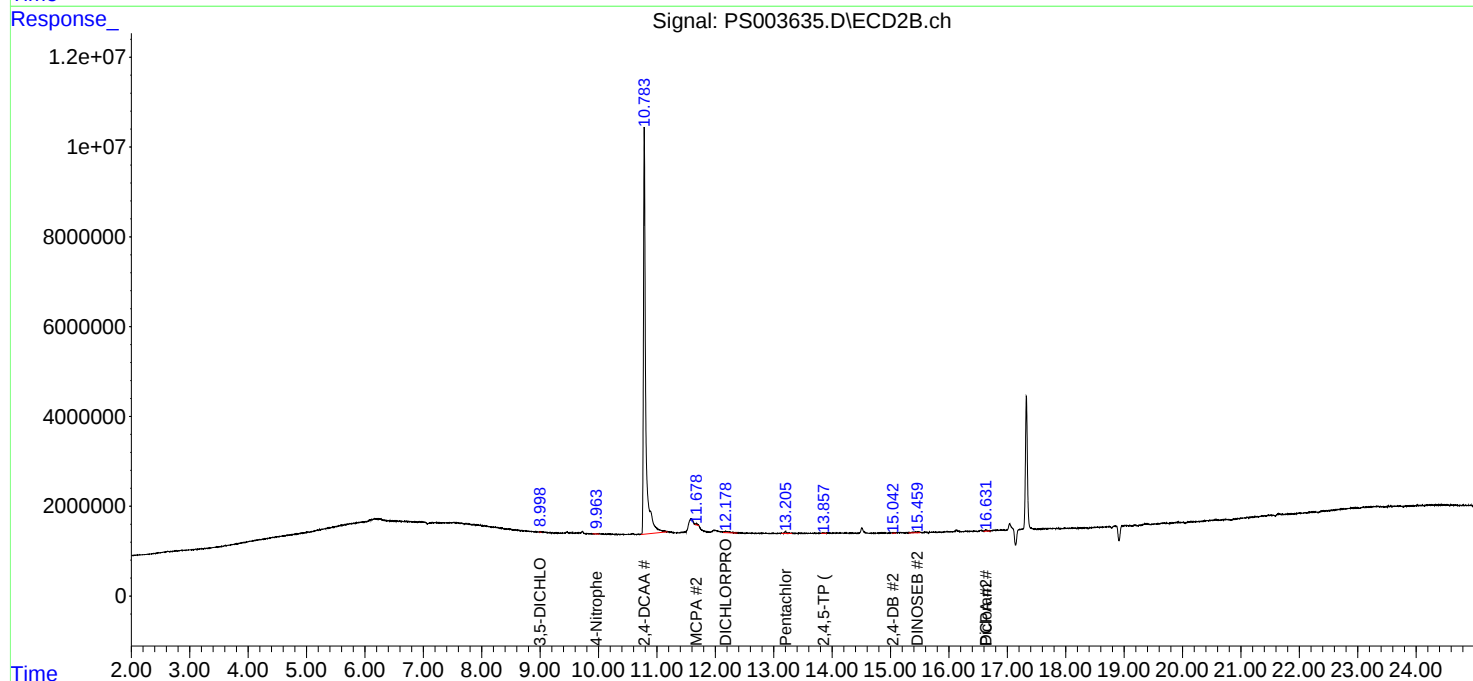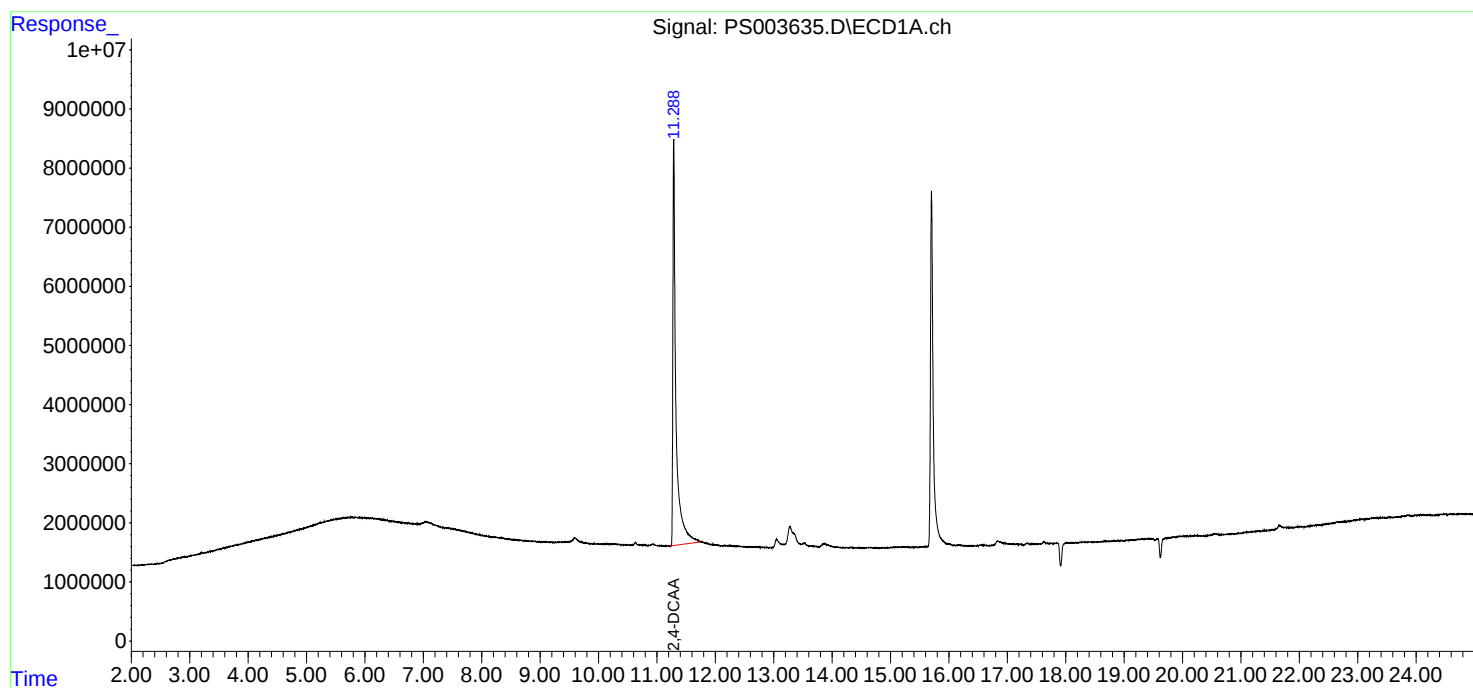


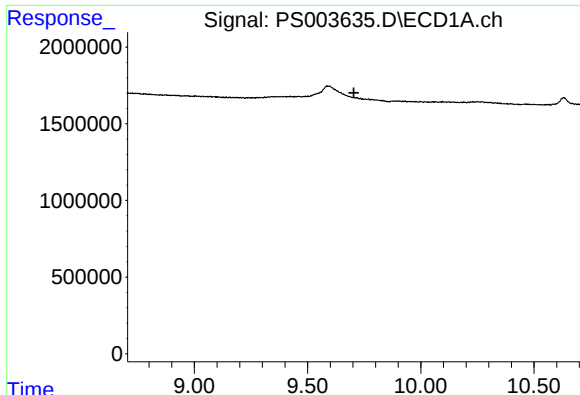

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

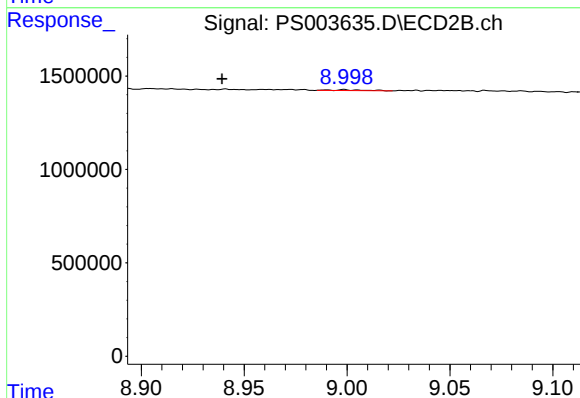


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.999 min
Delta R.T.: 0.060 min
Response: 51467
Conc: 0.08 ng/ml

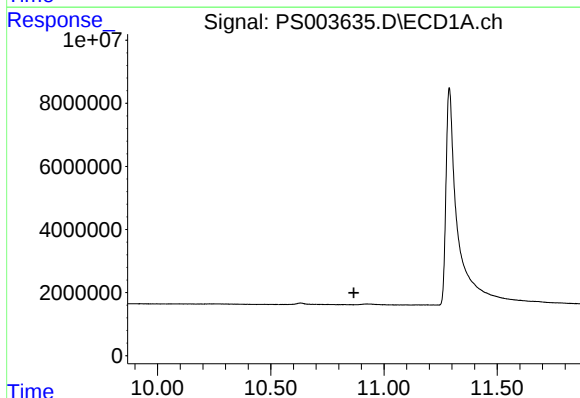


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

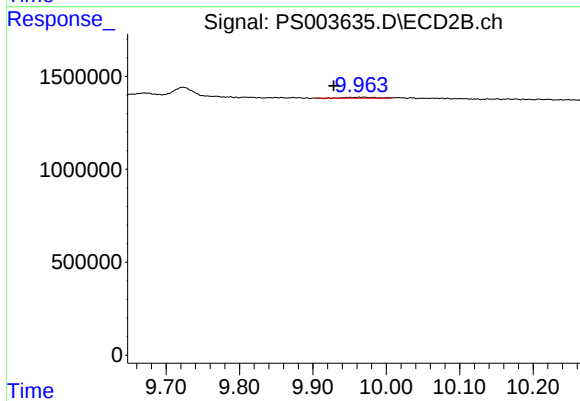

#3 4-Nitrophenol


R.T.: 9.968 min
Delta R.T.: 0.040 min
Response: 168972
Conc: 0.75 ng/ml

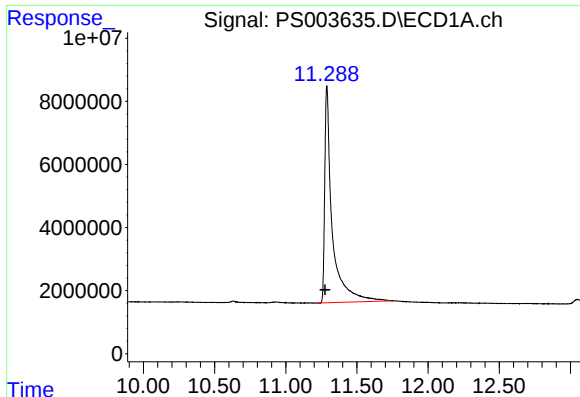

#4 2,4-DCAA


R.T.: 11.288 min
Delta R.T.: 0.011 min
Response: 253328913
Conc: 577.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

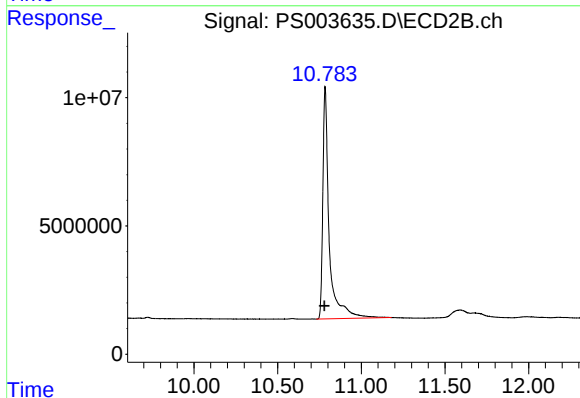


#4 2,4-DCAA

R.T.: 10.784 min
Delta R.T.: 0.004 min
Response: 242690621
Conc: 516.84 ng/ml

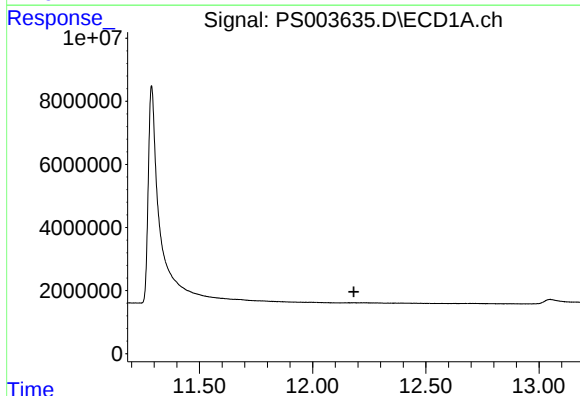


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

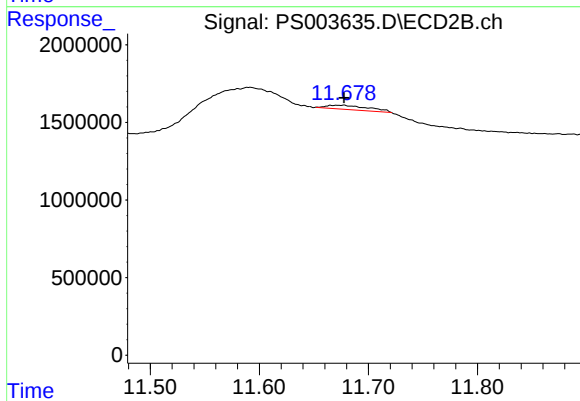

#7 MCPA


R.T.: 11.675 min
Delta R.T.: -0.003 min
Response: 637669
Conc: 0.37 ug/ml

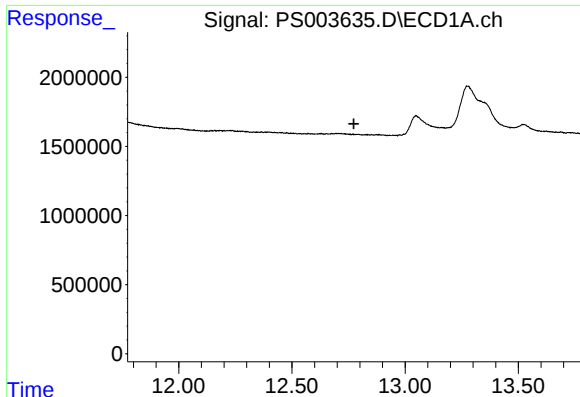

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

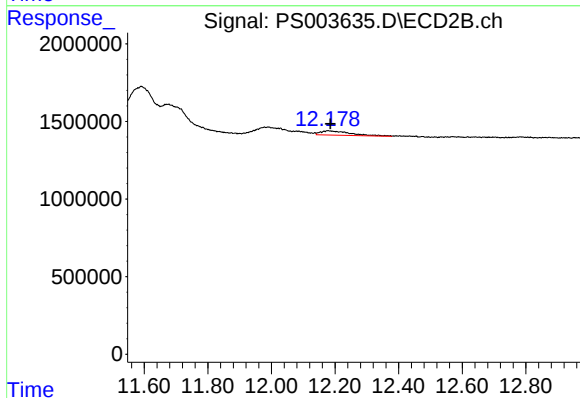


#8 DICHLORPROP

R.T.: 12.178 min
Delta R.T.: -0.007 min
Response: 1791580
Conc: 4.34 ng/ml

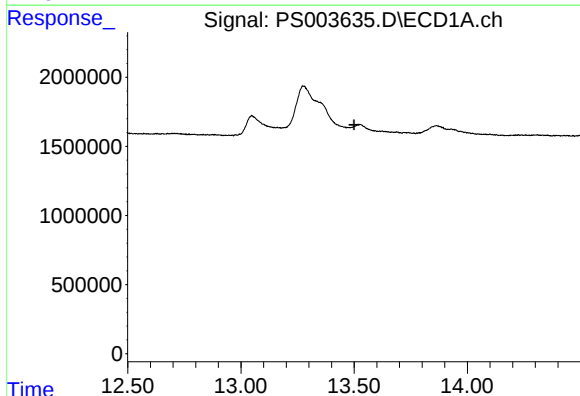


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

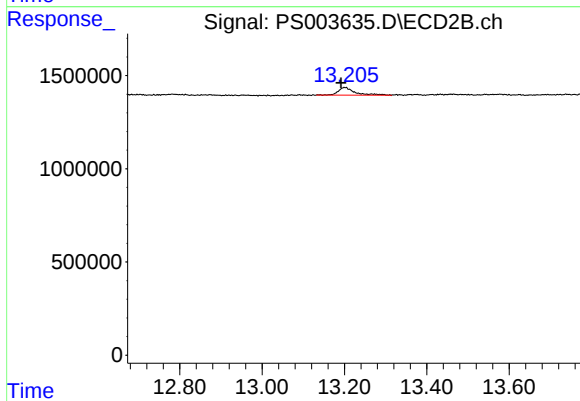

#10 Pentachlorophenol


R.T.: 13.201 min
Delta R.T.: 0.009 min
Response: 1150599
Conc: 0.17 ng/ml

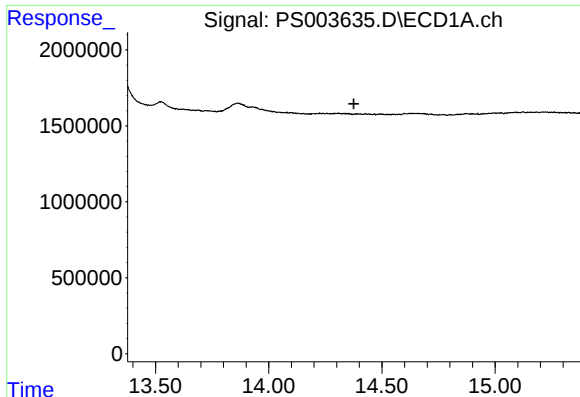

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

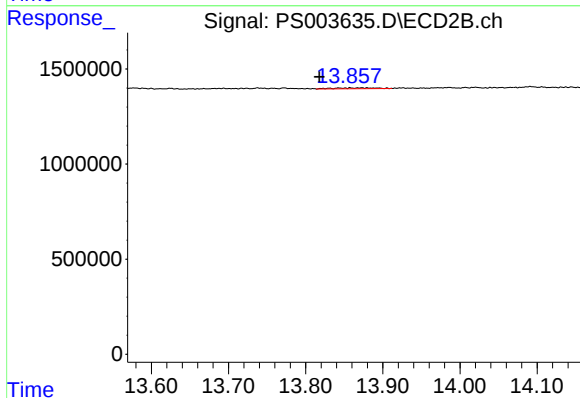


#11 2,4,5-TP (SILVEX)

R.T.: 13.859 min
Delta R.T.: 0.041 min
Response: 173378
Conc: 0.07 ng/ml

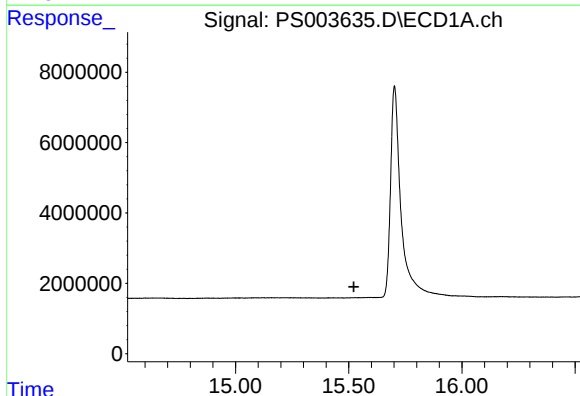


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

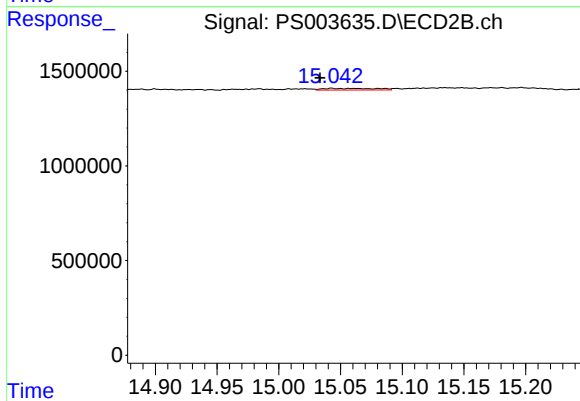

#13 2,4-DB


R.T.: 15.043 min
Delta R.T.: 0.009 min
Response: 270503
Conc: 1.06 ng/ml

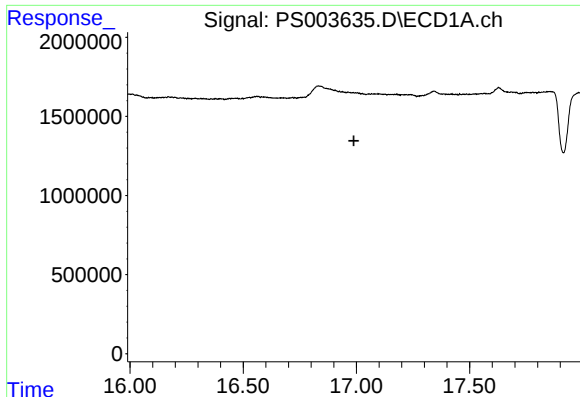

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

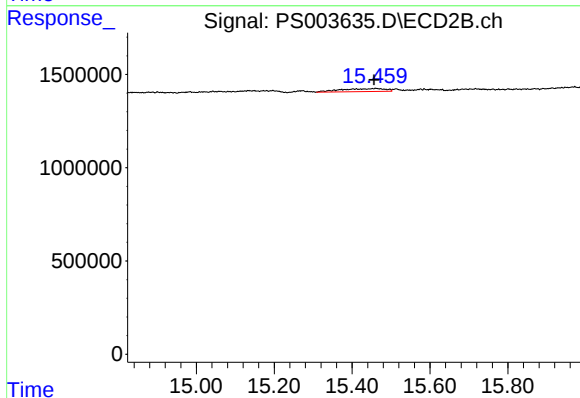


#14 DINOSEB

R.T.: 15.461 min
Delta R.T.: 0.005 min
Response: 1283236
Conc: 0.72 ng/ml

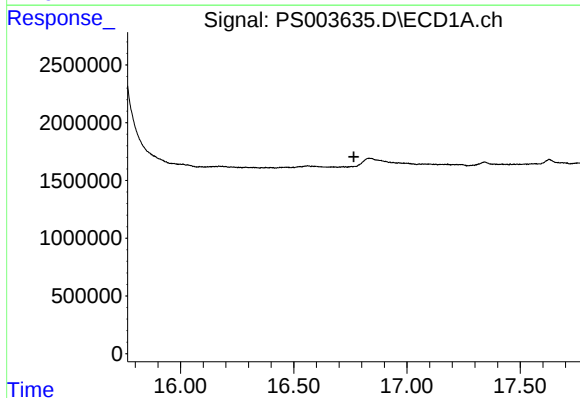


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

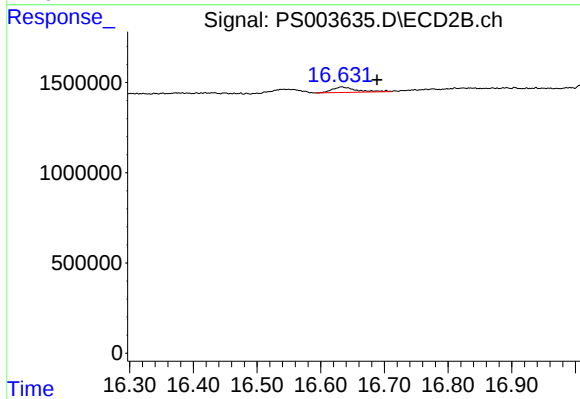

#15 Picloram


R.T.: 16.634 min
Delta R.T.: -0.054 min
Response: 772037
Conc: 0.30 ng/ml

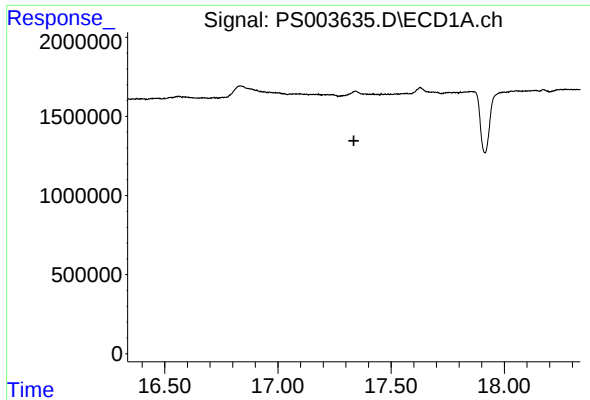

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

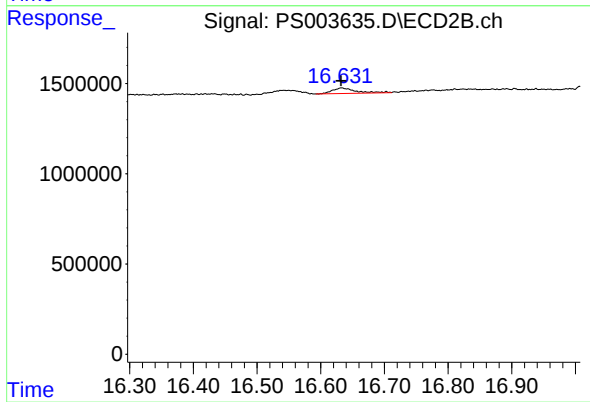

#16 DCPA

R.T.: 16.634 min
Delta R.T.: 0.002 min
Response: 772037
Conc: 0.25 ng/ml