

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
 Data File : PS003637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 23:23
 Operator : EI\SJ
 Sample : K1943-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:47:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.287	10.782	95325335	98214349	217.130	209.158
Target Compounds							
1) T	Dalapon	2.796	2.283	29421177	27167189	45.267	42.906
2) T	3,5-DICHL...	0.000	8.943	0	4392065	N.D.	7.113 #
3) T	4-Nitroph...	0.000	9.949	0	3036414	N.D.	13.505 #
5) T	DICAMBA	0.000	11.019	0	6844555	N.D.	4.097 #
6) T	MCPD	11.996	0.000	32560155	0	24.800	N.D. #
7) T	MCPA	12.176	0.000	105.5E6	0	53.202	N.D. #
9) T	2,4-D	0.000	12.637	0	1150488	N.D.	2.192 #
11) T	2,4,5-TP ...	0.000	13.822	0	757289	N.D.	0.297 #
12) T	2,4,5-T	0.000	14.434	0	13842163	N.D.	6.864 #
13) T	2,4-DB	0.000	15.011	0	4816532	N.D.	18.862 #
14) T	DINOSEB	0.000	15.450	0	5916266	N.D.	3.315 #
15) T	Picloram	0.000	16.727	0	16716048	N.D.	6.586 #
16) T	DCPA	0.000	16.631	0	2683398	N.D.	0.863 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
Data File : PS003637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 23:23
Operator : EI\SJ
Sample : K1943-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:47:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

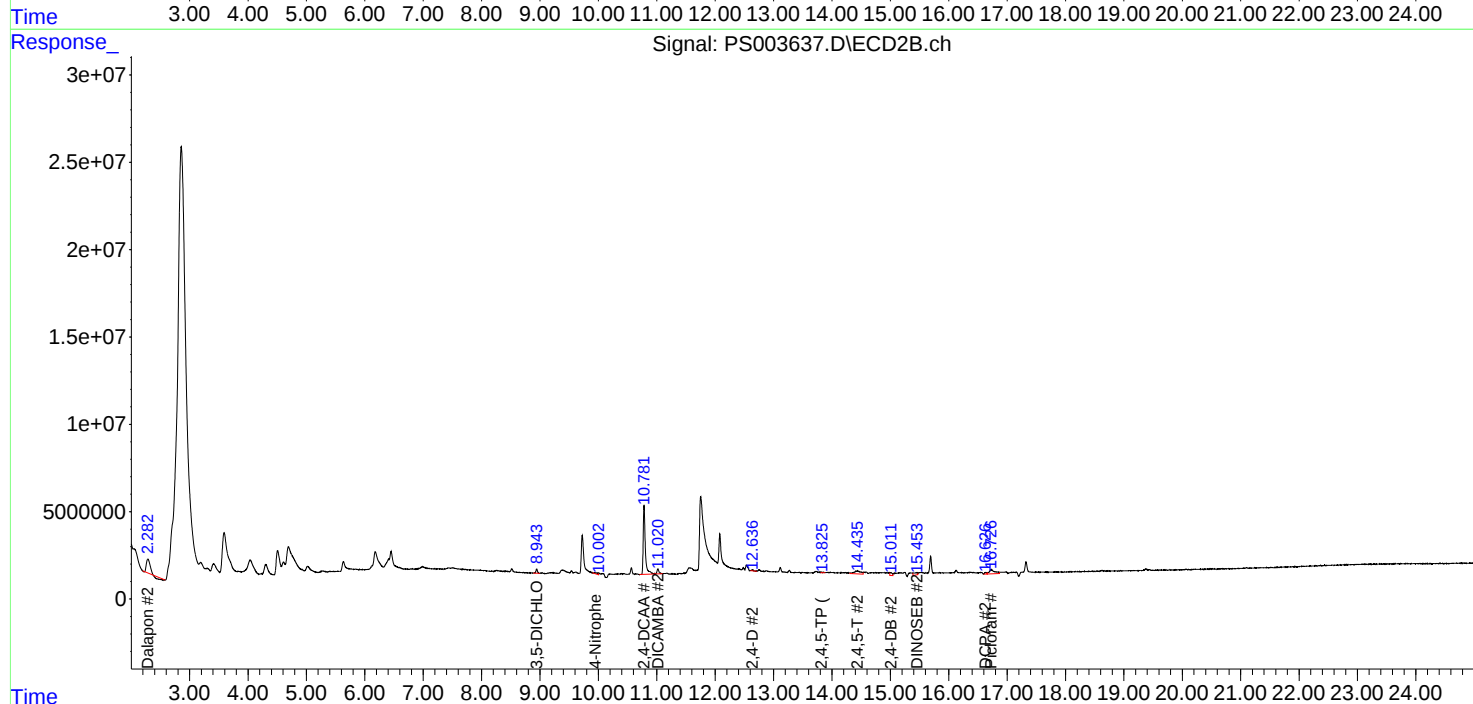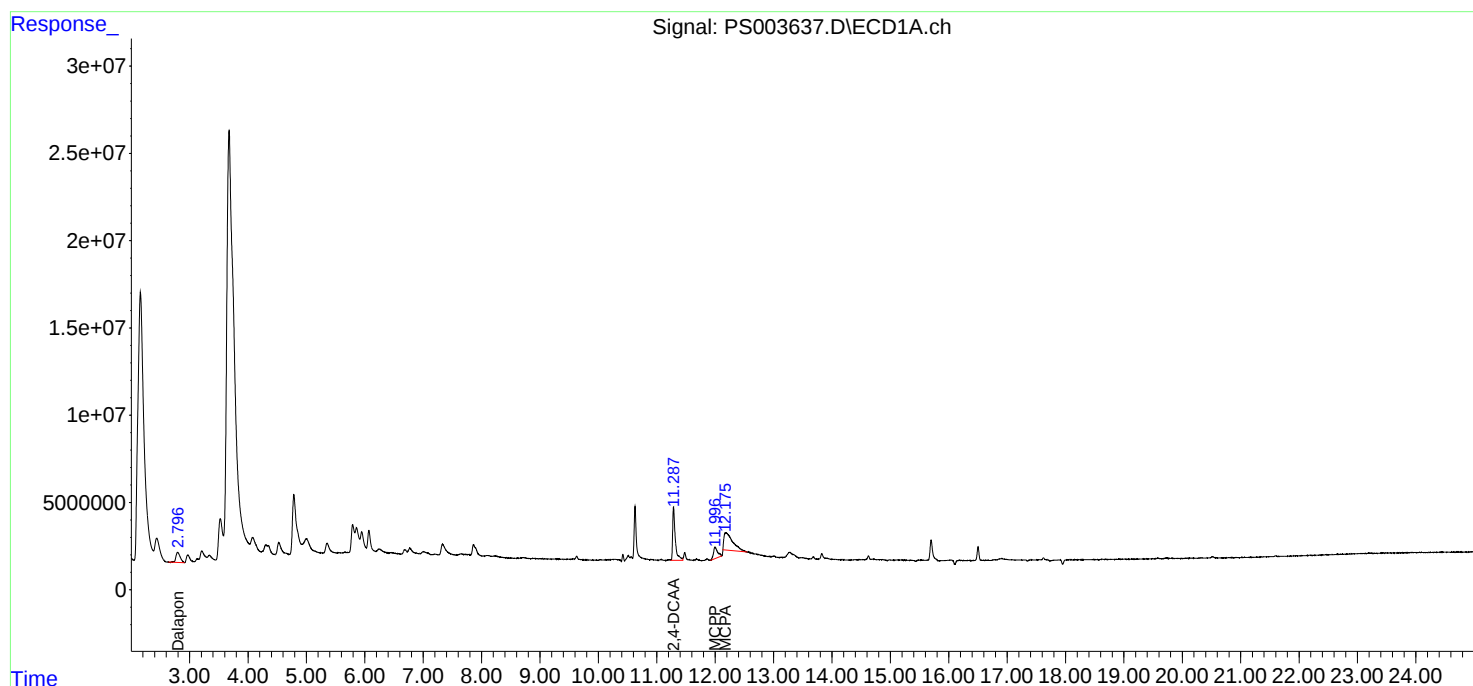


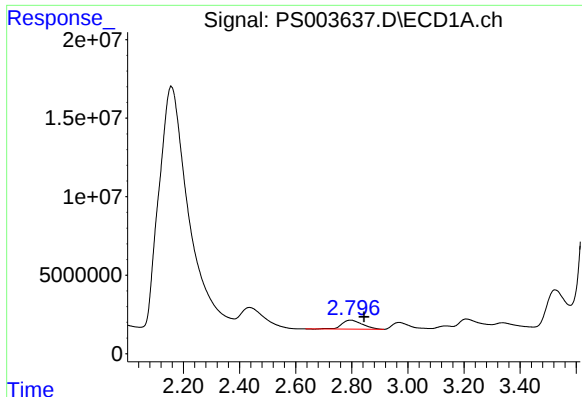

#1 Dalapon


R.T.: 2.796 min
Delta R.T.: -0.048 min
Response: 29421177
Conc: 45.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

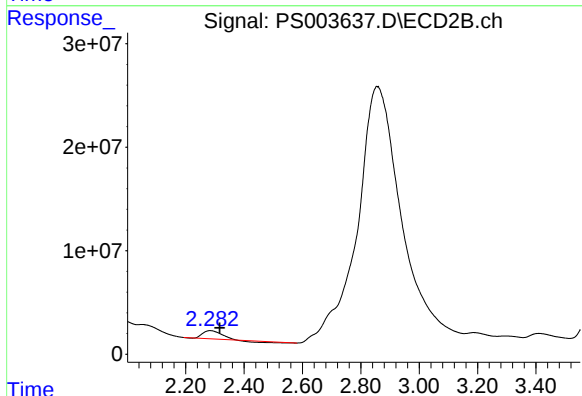


#1 Dalapon

R.T.: 2.283 min
Delta R.T.: -0.033 min
Response: 27167189
Conc: 42.91 ng/ml

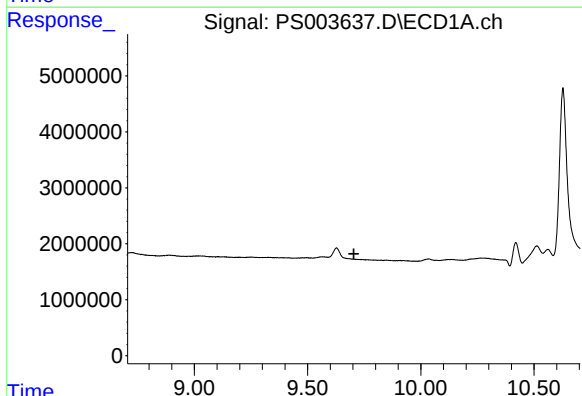


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

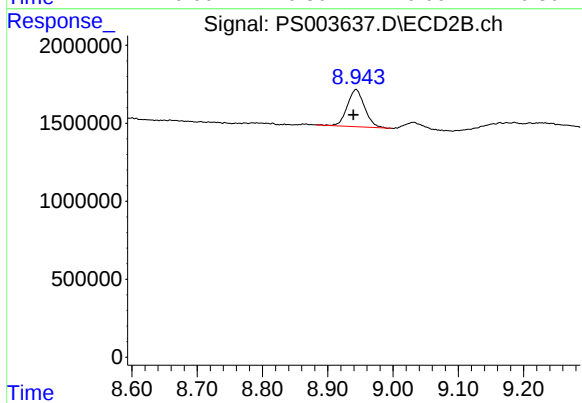

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.943 min
Delta R.T.: 0.004 min
Response: 4392065
Conc: 7.11 ng/ml

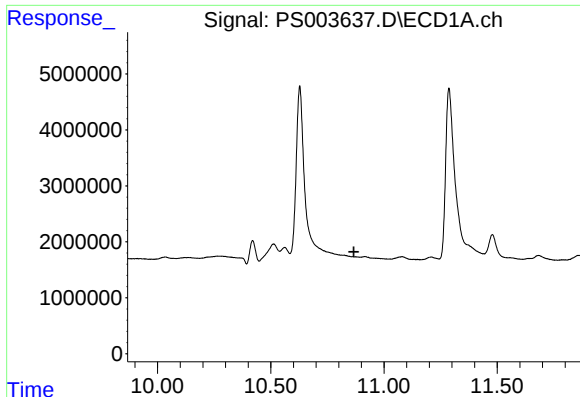

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

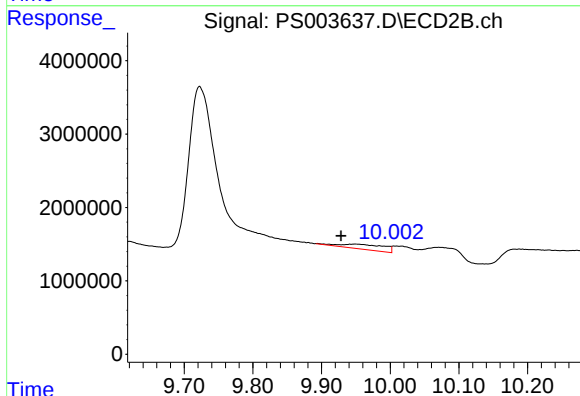


#3 4-Nitrophenol

R.T.: 9.949 min
Delta R.T.: 0.020 min
Response: 3036414
Conc: 13.51 ng/ml

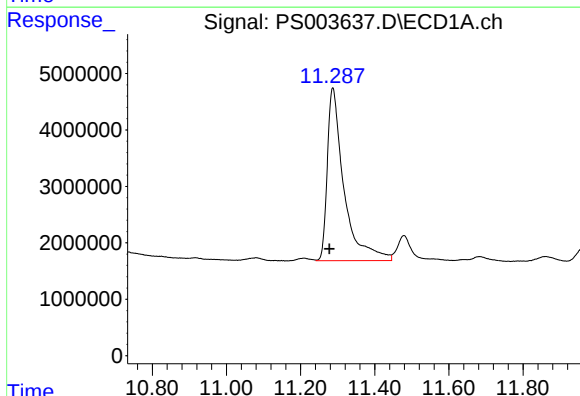


#4 2,4-DCAA

R.T.: 11.287 min
Delta R.T.: 0.009 min
Response: 9532535
Conc: 217.13 ng/ml

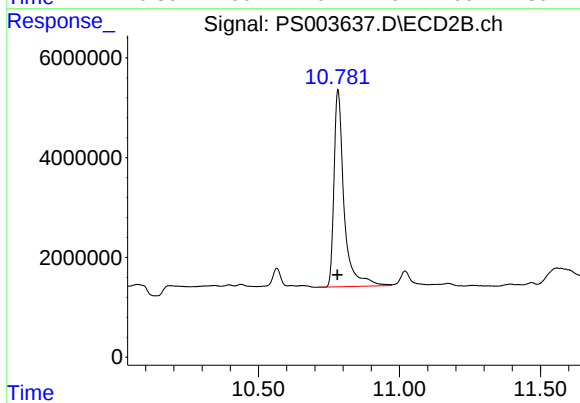

#4 2,4-DCAA


R.T.: 10.782 min
Delta R.T.: 0.002 min
Response: 98214349
Conc: 209.16 ng/ml

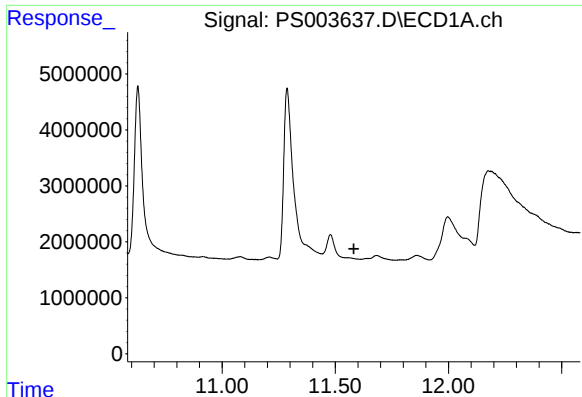

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

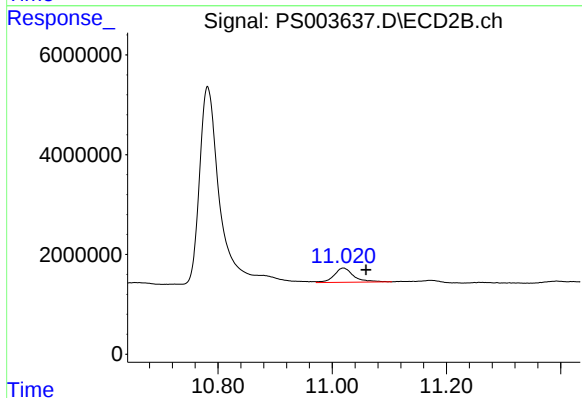


#5 DICAMBA

R.T.: 11.019 min
Delta R.T.: -0.040 min
Response: 6844555
Conc: 4.10 ng/ml

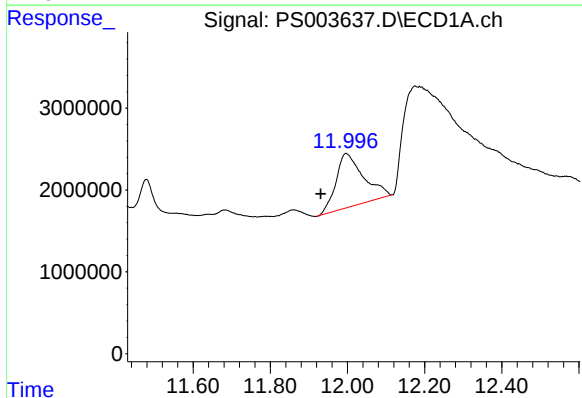


#6 MCP

R.T.: 11.996 min
Delta R.T.: 0.066 min
Response: 32560155
Conc: 24.80 ug/ml

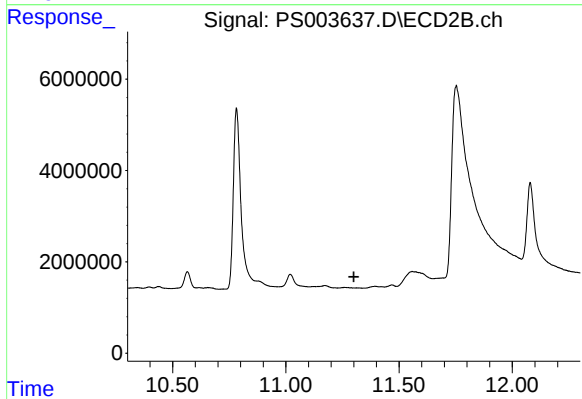

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.300 min
Response: 0
Conc: N.D.

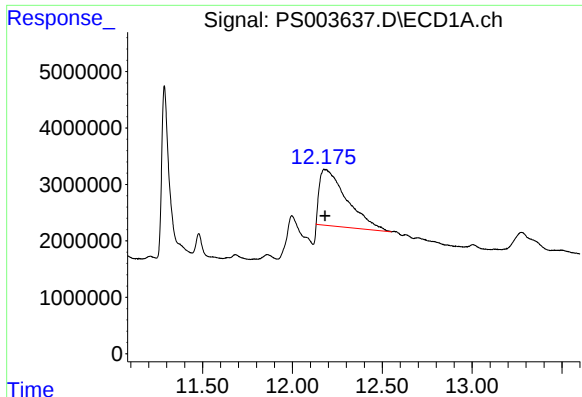

#7 MCPA


R.T.: 12.176 min
Delta R.T.: -0.007 min
Response: 105529352
Conc: 53.20 ug/ml

Instrument :
ECD_S
ClientSampleId :

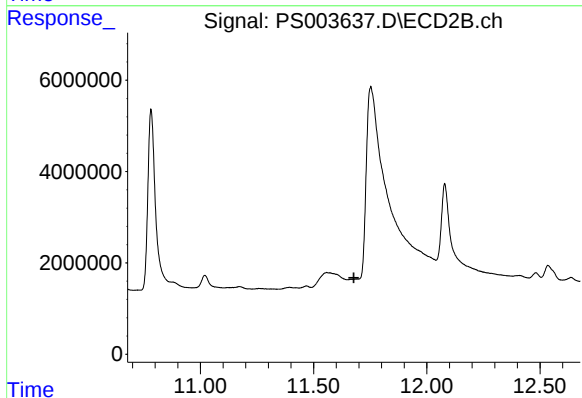


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.678 min
Response: 0
Conc: N.D.

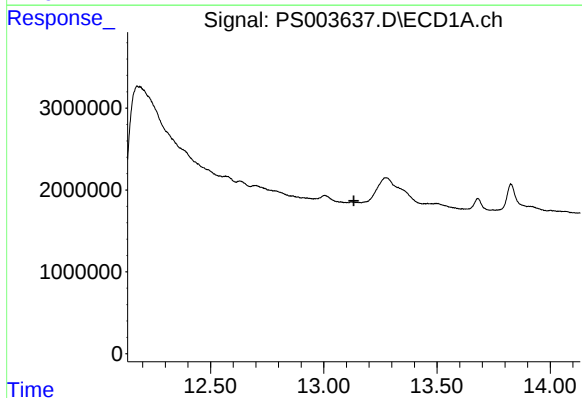


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

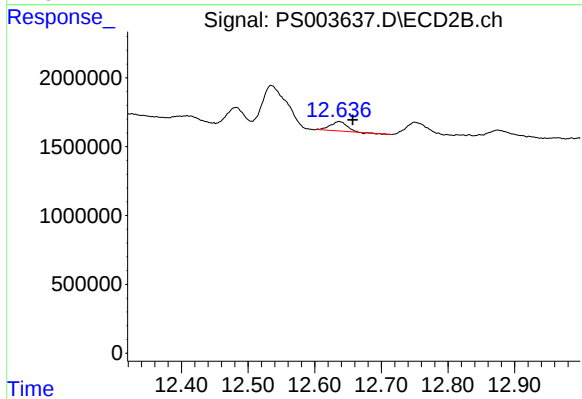

#9 2,4-D


R.T.: 12.637 min
Delta R.T.: -0.020 min
Response: 1150488
Conc: 2.19 ng/ml

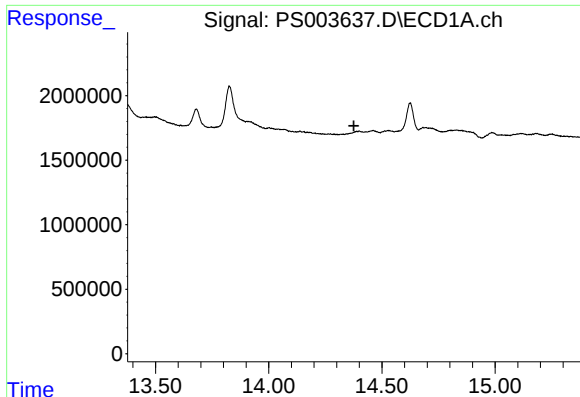

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

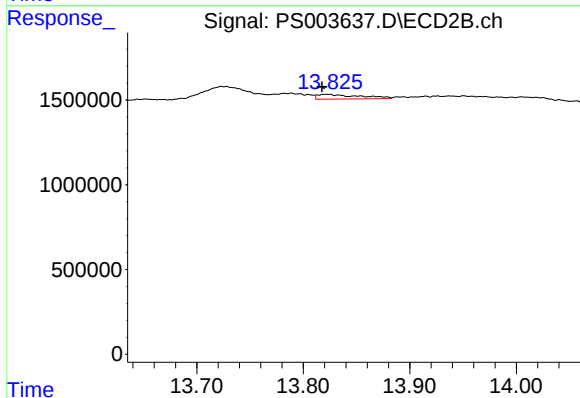


#11 2,4,5-TP (SILVEX)

R.T.: 13.822 min
Delta R.T.: 0.004 min
Response: 757289
Conc: 0.30 ng/ml

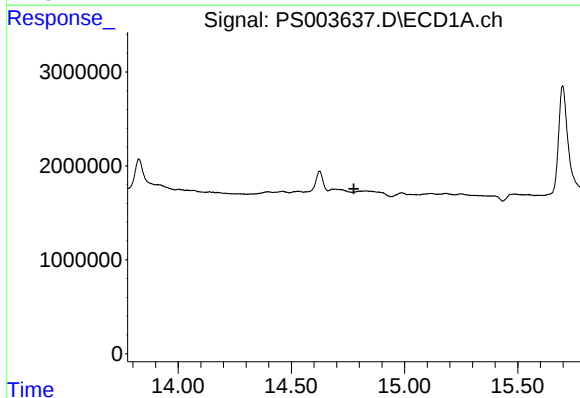


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

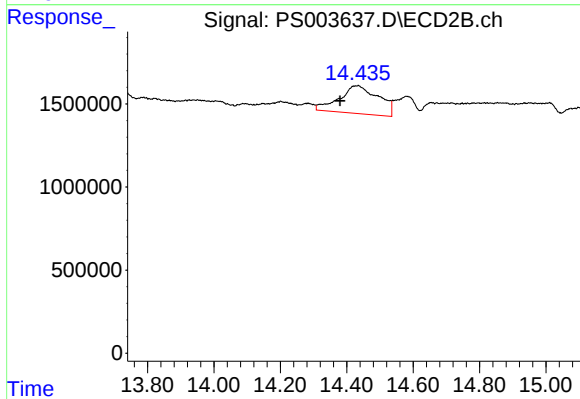

#12 2,4,5-T


R.T.: 14.434 min
Delta R.T.: 0.054 min
Response: 13842163
Conc: 6.86 ng/ml

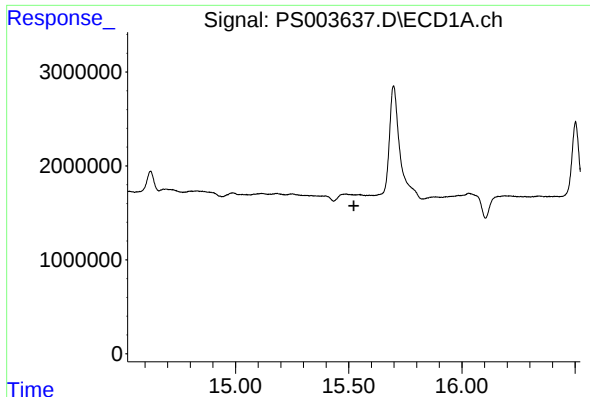

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

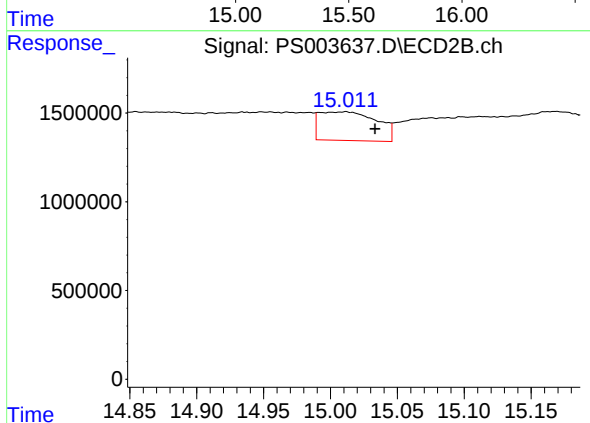


#13 2,4-DB

R.T.: 15.011 min
Delta R.T.: -0.022 min
Response: 4816532
Conc: 18.86 ng/ml

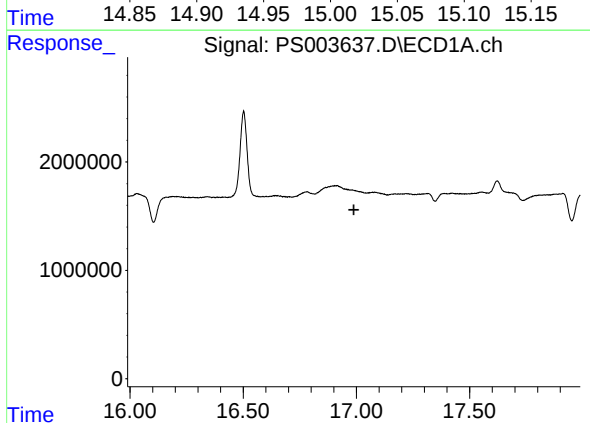


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

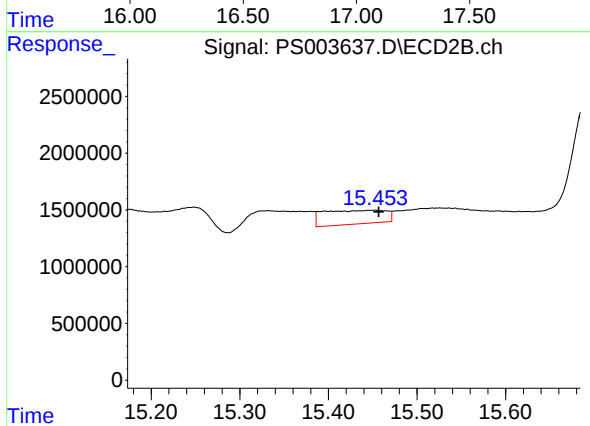

#14 DINOSEB


R.T.: 15.450 min
Delta R.T.: -0.006 min
Response: 5916266
Conc: 3.31 ng/ml

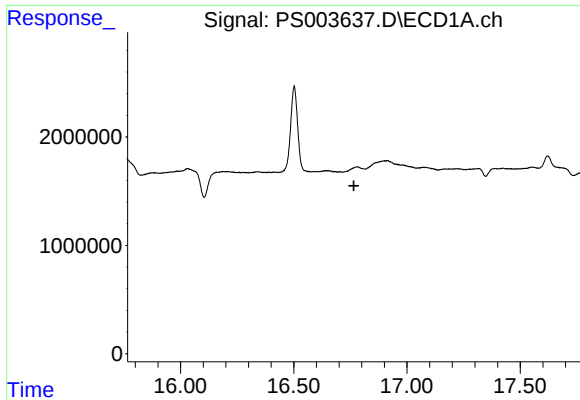

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

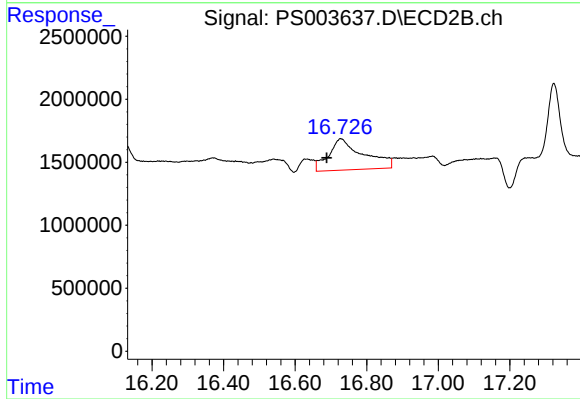


#15 Picloram

R.T.: 16.727 min
Delta R.T.: 0.039 min
Response: 16716048
Conc: 6.59 ng/ml

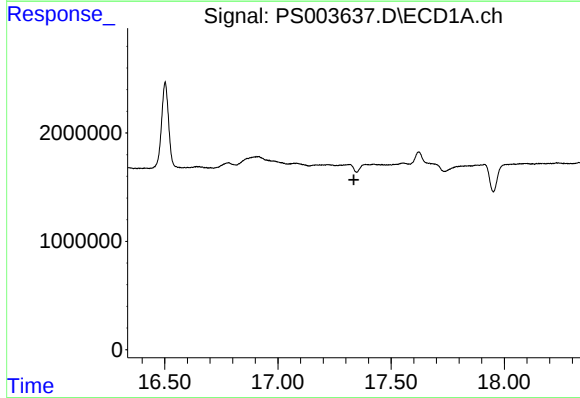

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

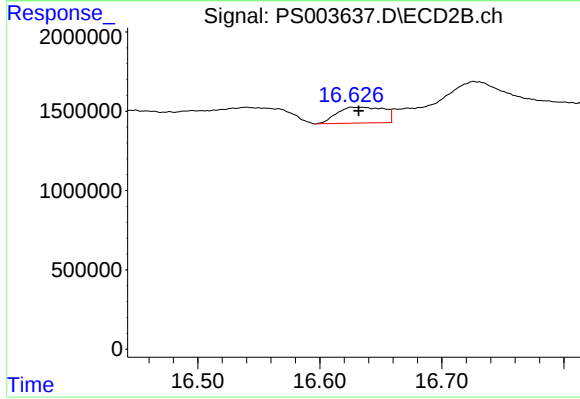

#16 DCPA

R.T.: 16.631 min
Delta R.T.: 0.000 min
Response: 2683398
Conc: 0.86 ng/ml