

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
 Data File : PS003638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 23:54
 Operator : EI\SJ
 Sample : K1943-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:48:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.302	10.796	83751486	87660256	190.767	186.682
Target Compounds							
1) T	Dalapon	2.808	2.297	32007715	21235619	49.247	33.538 #
2) T	3,5-DICHL...	0.000	8.955	0	5681992	N.D.	9.202 #
5) T	DICAMBA	0.000	11.031	0	6402175	N.D.	3.832 #
6) T	MCP	0.000	11.286	0	232032	N.D.	0.197 #
9) T	2,4-D	0.000	12.650	0	1055830	N.D.	2.012 #
11) T	2,4,5-TP ...	0.000	13.798	0	862195	N.D.	0.339 #
12) T	2,4,5-T	0.000	14.385	0	1754357	N.D.	0.870 #
13) T	2,4-DB	0.000	15.015	0	5700868	N.D.	22.325 #
14) T	DINOSEB	0.000	15.469	0	1527171	N.D.	0.856 #
15) T	Picloram	0.000	16.670	0	3637975	N.D.	1.433 #
16) T	DCPA	0.000	16.670	0	3637975	N.D.	1.170 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
Data File : PS003638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 23:54
Operator : EI\SJ
Sample : K1943-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:48:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

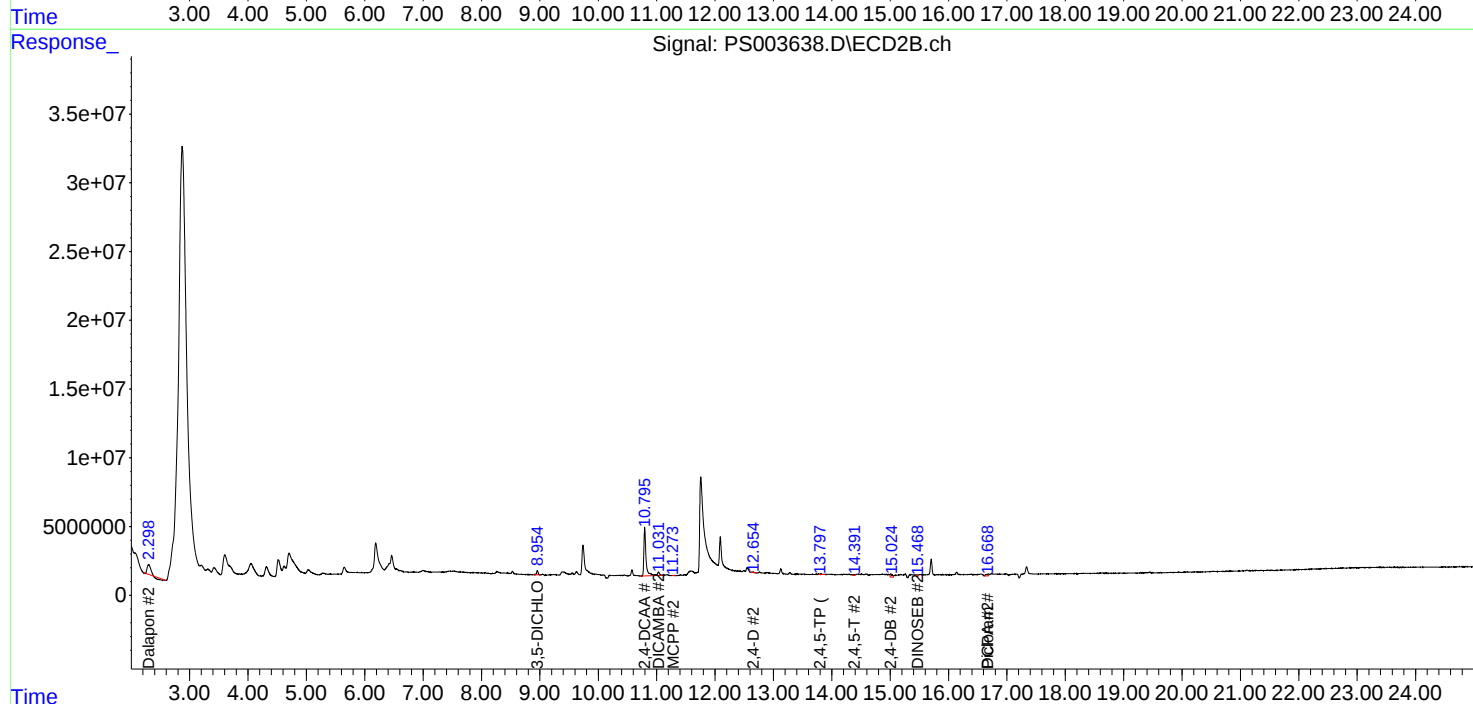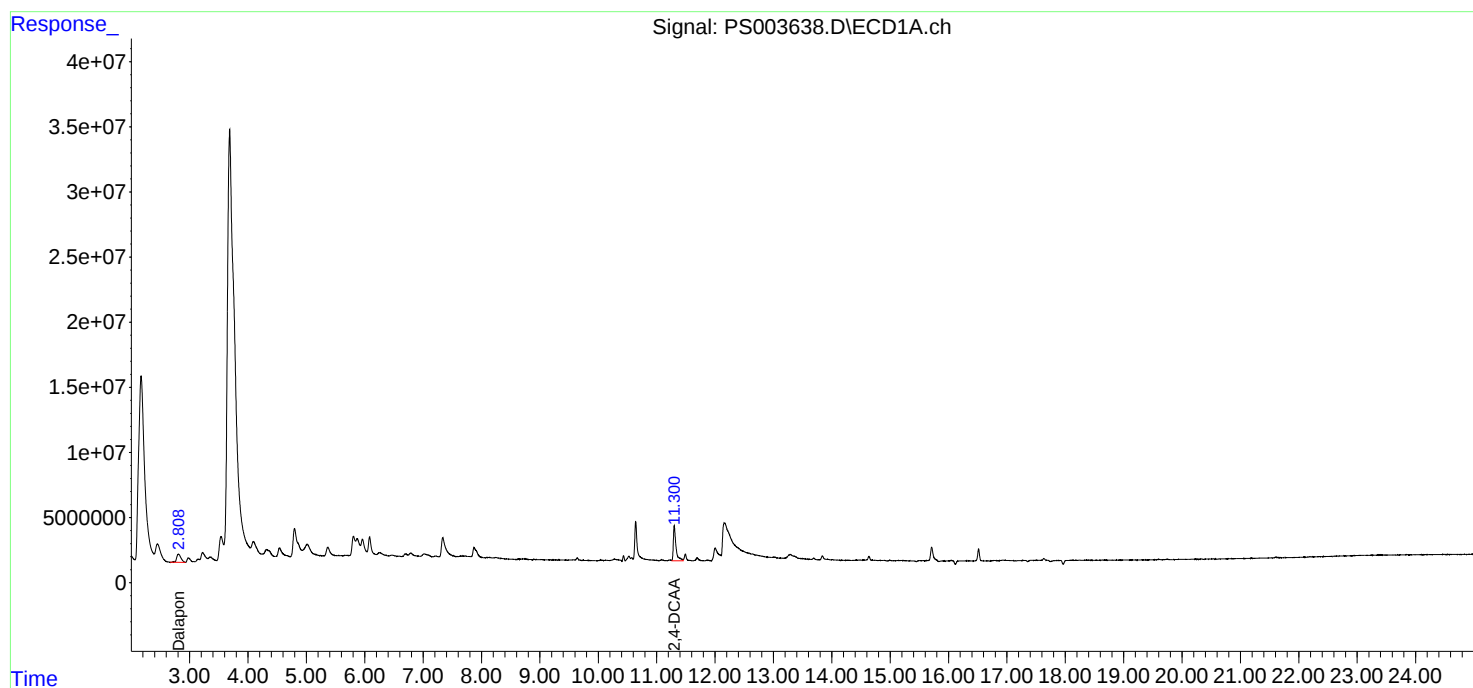


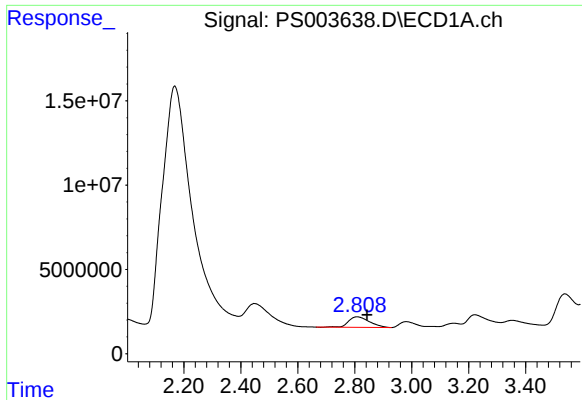

#1 Dalapon


R.T.: 2.808 min
Delta R.T.: -0.036 min
Response: 32007715
Conc: 49.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

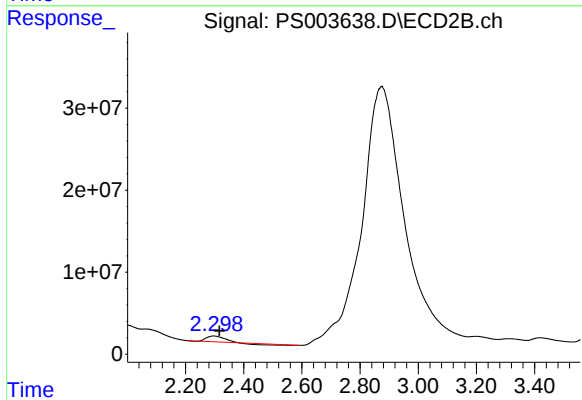


#1 Dalapon

R.T.: 2.297 min
Delta R.T.: -0.020 min
Response: 21235619
Conc: 33.54 ng/ml

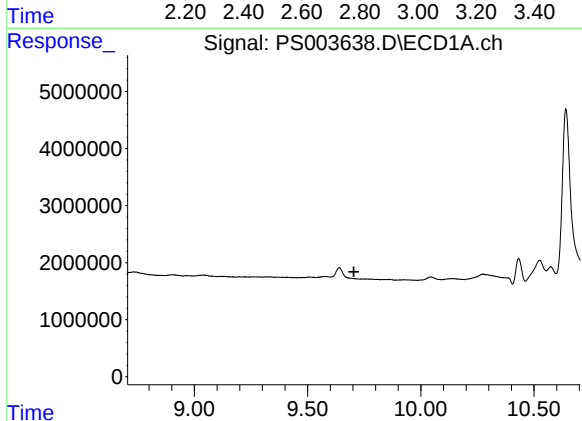


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

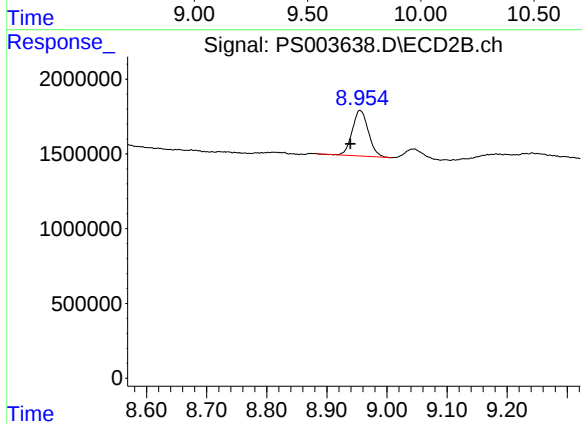

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.955 min
Delta R.T.: 0.016 min
Response: 5681992
Conc: 9.20 ng/ml

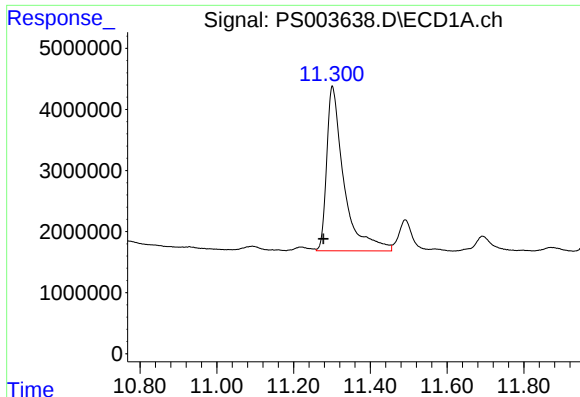

#4 2,4-DCAA


R.T.: 11.302 min
Delta R.T.: 0.024 min
Response: 83751486
Conc: 190.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

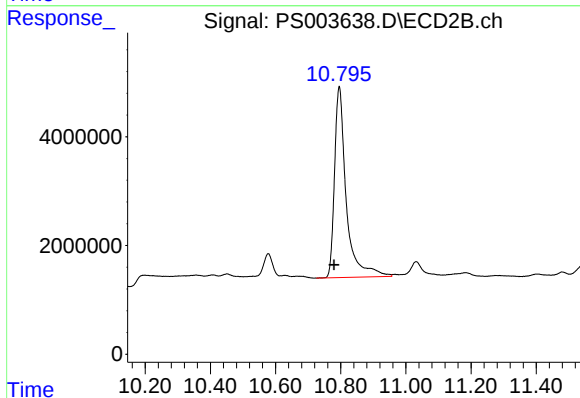


#4 2,4-DCAA

R.T.: 10.796 min
Delta R.T.: 0.016 min
Response: 87660256
Conc: 186.68 ng/ml

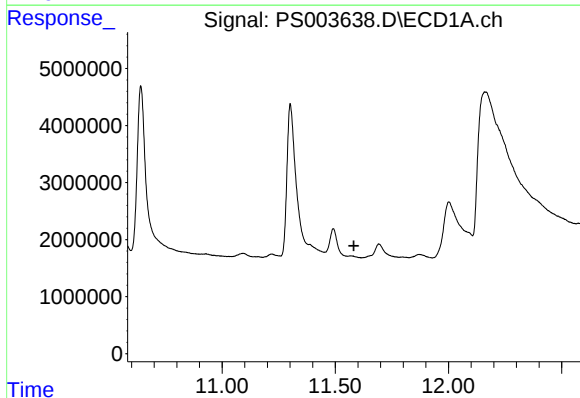


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

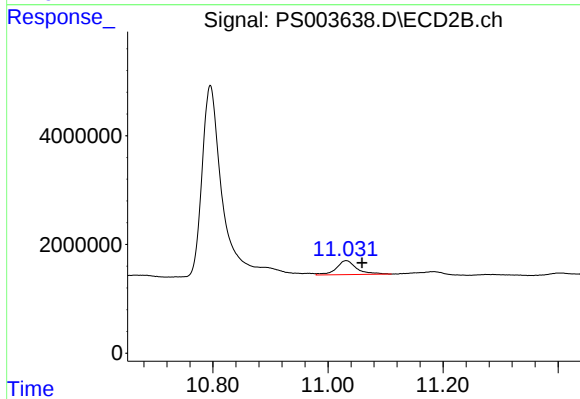

#5 DICAMBA


R.T.: 11.031 min
Delta R.T.: -0.028 min
Response: 6402175
Conc: 3.83 ng/ml

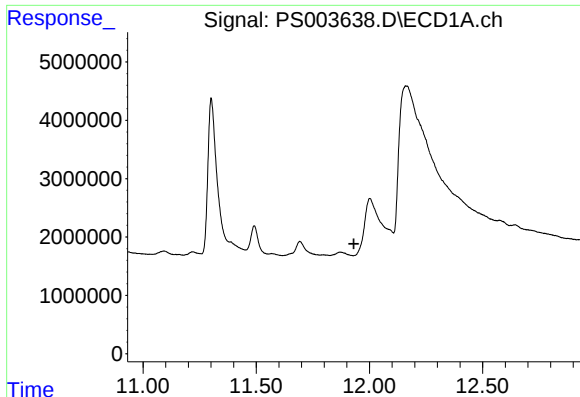

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

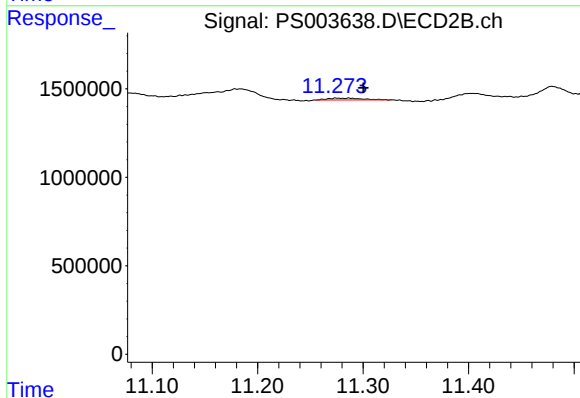


#6 MCP

R.T.: 11.286 min
Delta R.T.: -0.015 min
Response: 232032
Conc: 0.20 ug/ml

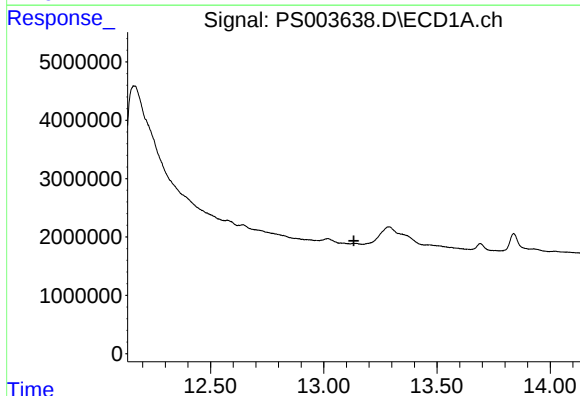


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

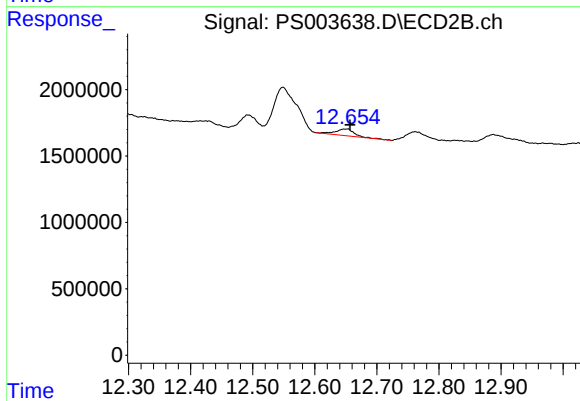

#9 2,4-D


R.T.: 12.650 min
Delta R.T.: -0.007 min
Response: 1055830
Conc: 2.01 ng/ml

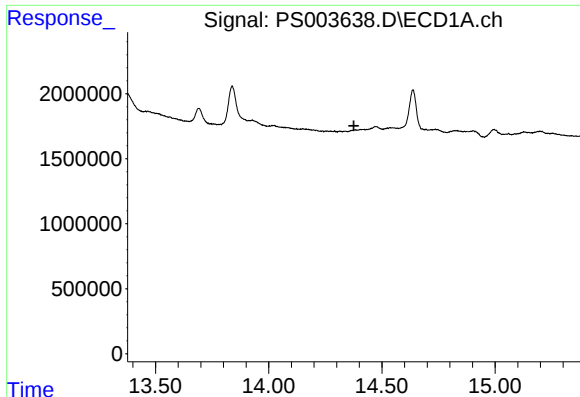

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

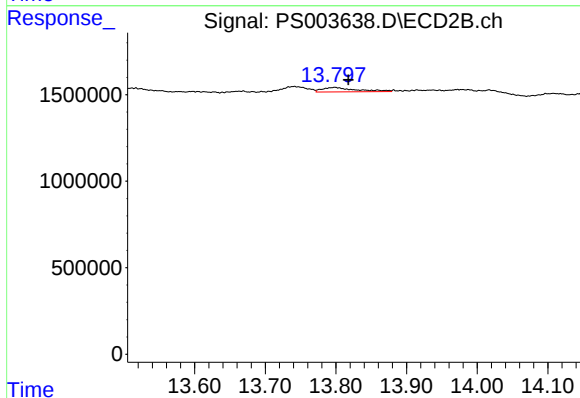


#11 2,4,5-TP (SILVEX)

R.T.: 13.798 min
Delta R.T.: -0.020 min
Response: 862195
Conc: 0.34 ng/ml

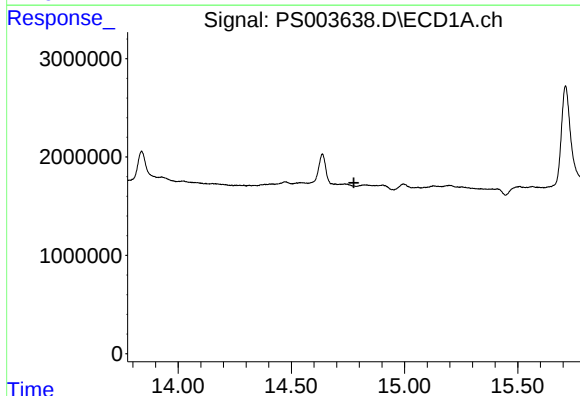


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

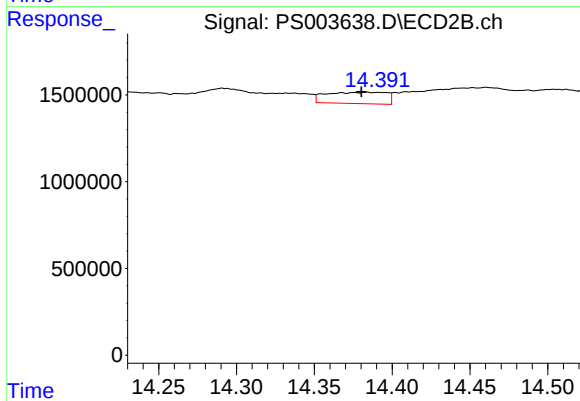

#12 2,4,5-T


R.T.: 14.385 min
Delta R.T.: 0.005 min
Response: 1754357
Conc: 0.87 ng/ml

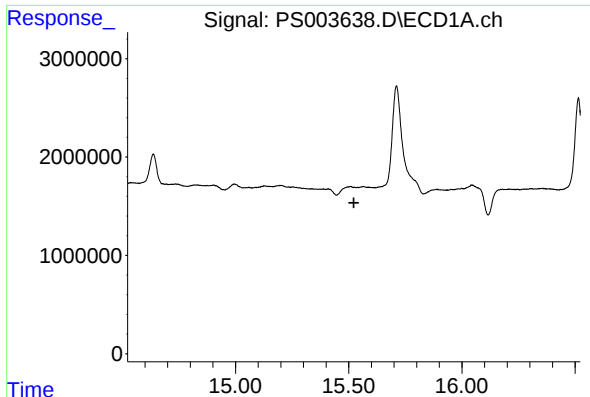

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

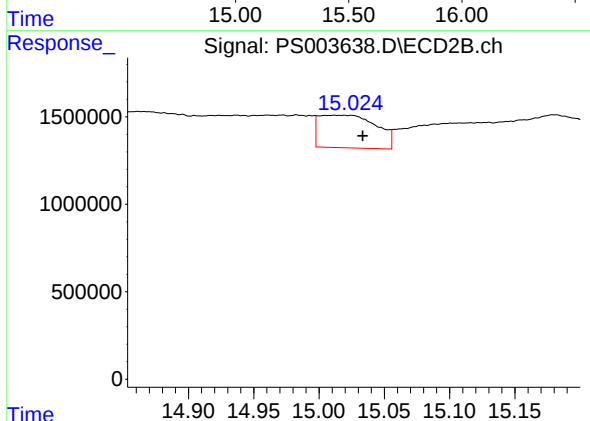


#13 2,4-DB

R.T.: 15.015 min
Delta R.T.: -0.018 min
Response: 5700868
Conc: 22.33 ng/ml

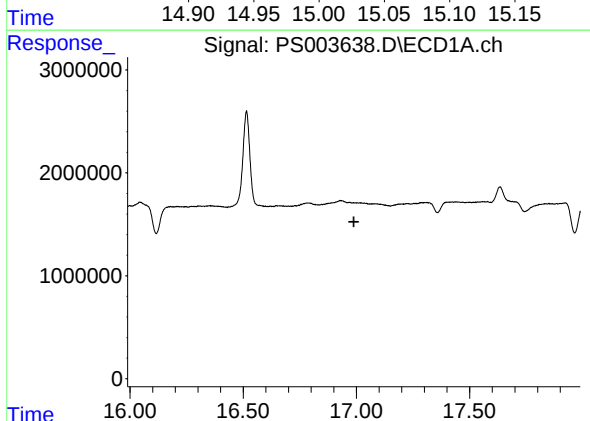


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

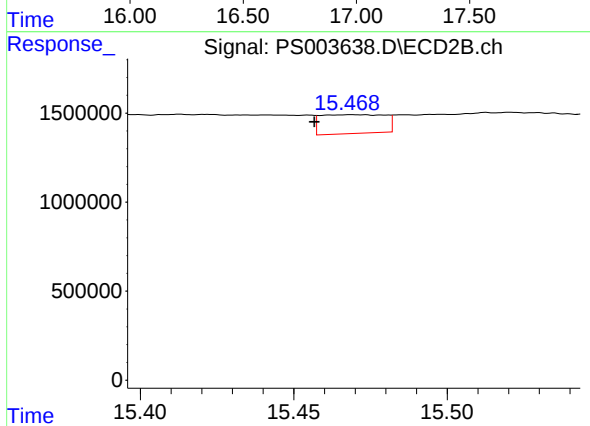

#14 DINOSEB


R.T.: 15.469 min
Delta R.T.: 0.012 min
Response: 1527171
Conc: 0.86 ng/ml

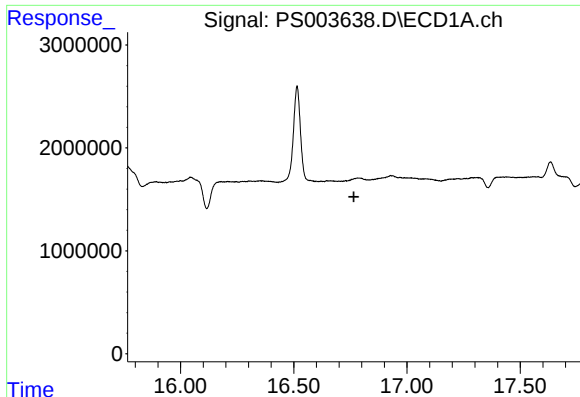

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

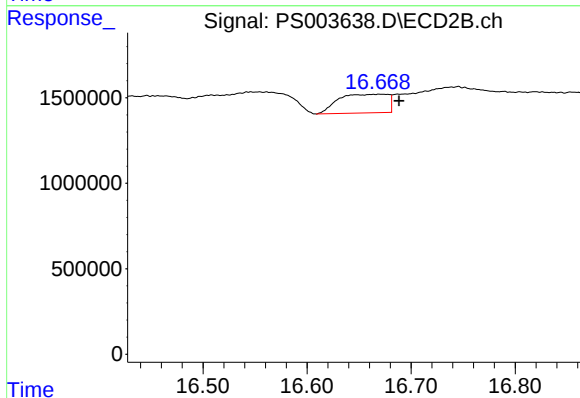


#15 Picloram

R.T.: 16.670 min
Delta R.T.: -0.018 min
Response: 3637975
Conc: 1.43 ng/ml

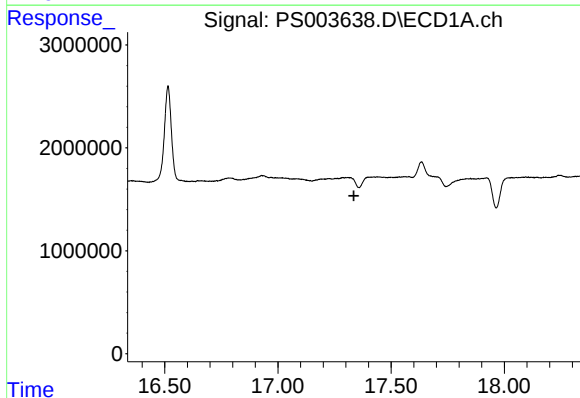

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

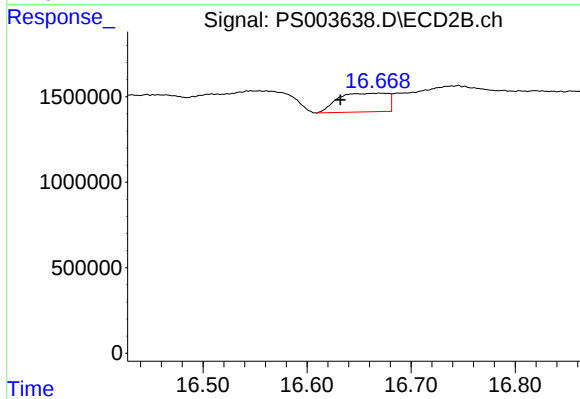

#16 DCPA

R.T.: 16.670 min
Delta R.T.: 0.038 min
Response: 3637975
Conc: 1.17 ng/ml