

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
 Data File : PS003645.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2019 03:33
 Operator : EI\SJ
 Sample : K1943-19
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:50:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.773	109.0E6	104.9E6	248.291	223.387
Target Compounds							
1) T	Dalapon	2.786	2.274	29980251	40082868	46.128	63.304 #
2) T	3,5-DICHL...	0.000	8.935	0	4900363	N.D.	7.936 #
5) T	DICAMBA	0.000	11.010	0	7880974	N.D.	4.717 #
6) T	MCP	11.945	11.304	4896871	109547	3.730	0.093 #
9) T	2,4-D	0.000	12.629	0	752223	N.D.	1.433 #
11) T	2,4,5-TP ...	0.000	13.845	0	134.8E6	N.D.	52.929 #
12) T	2,4,5-T	0.000	14.313	0	2347860	N.D.	1.164 #
13) T	2,4-DB	15.486	14.995	18599076	7614484	78.545	29.819 #
14) T	DINOSEB	0.000	15.398	0	6594057	N.D.	3.694 #
15) T	Picloram	0.000	16.736	0	8006065	N.D.	3.154 #
16) T	DCPA	0.000	16.639	0	2587208	N.D.	0.832 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
Data File : PS003645.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2019 03:33
Operator : EI\SJ
Sample : K1943-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:50:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

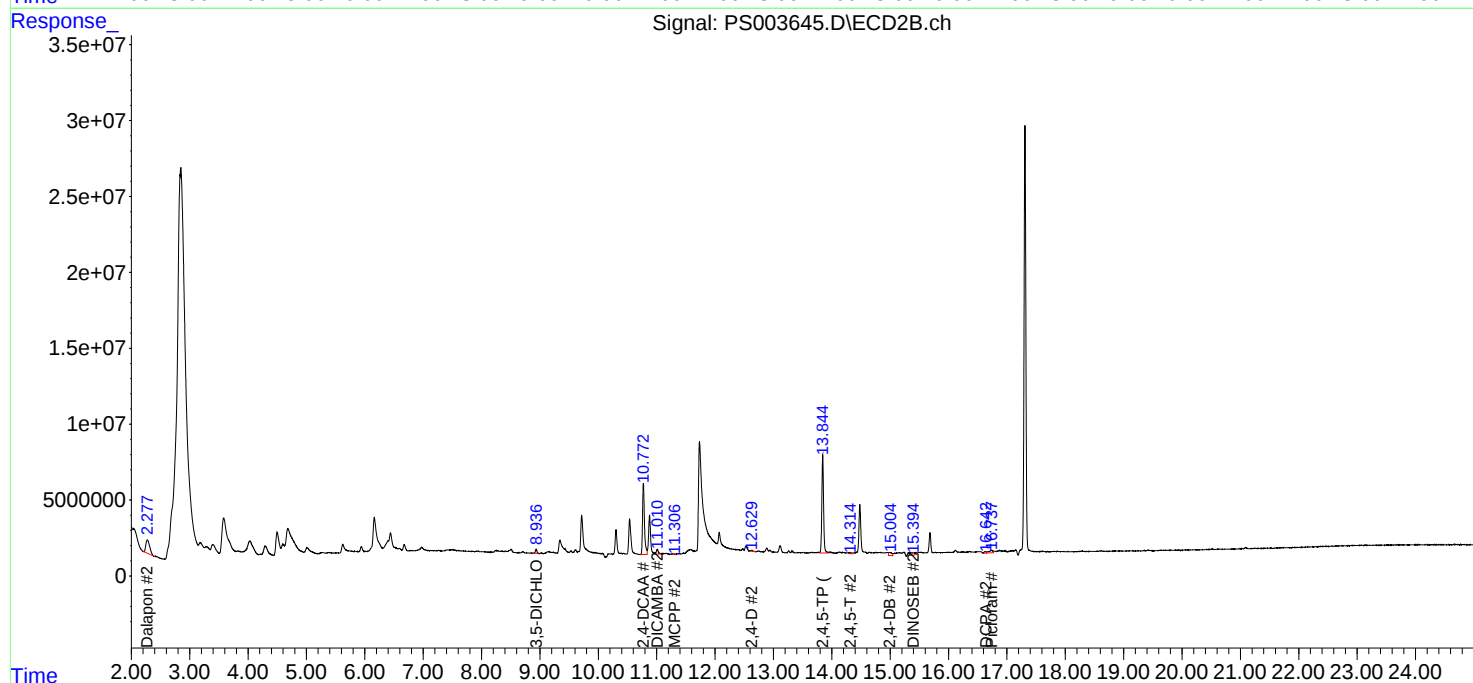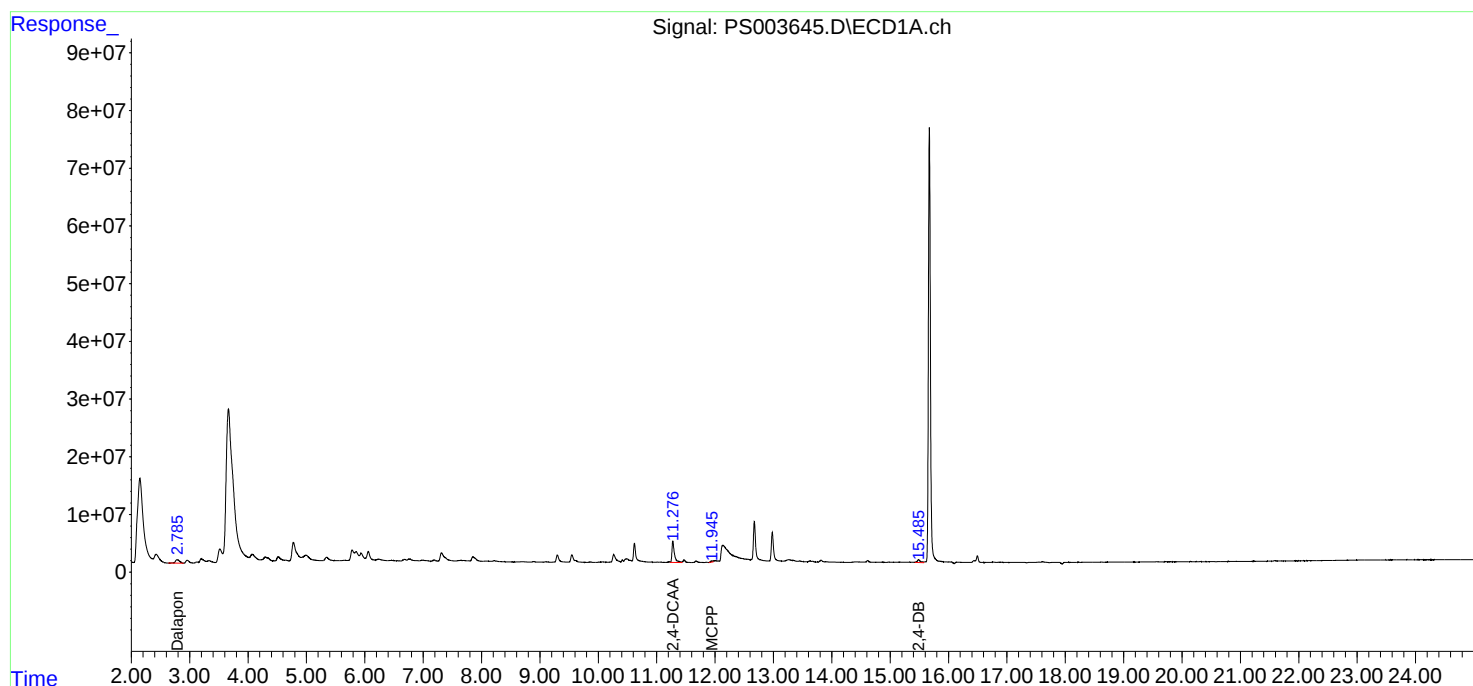


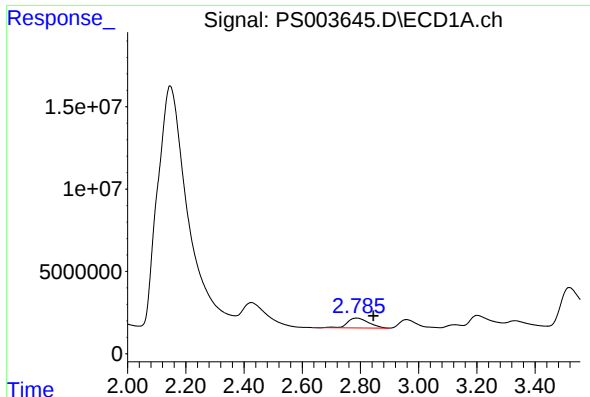

#1 Dalapon


R.T.: 2.786 min
Delta R.T.: -0.058 min
Response: 29980251
Conc: 46.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

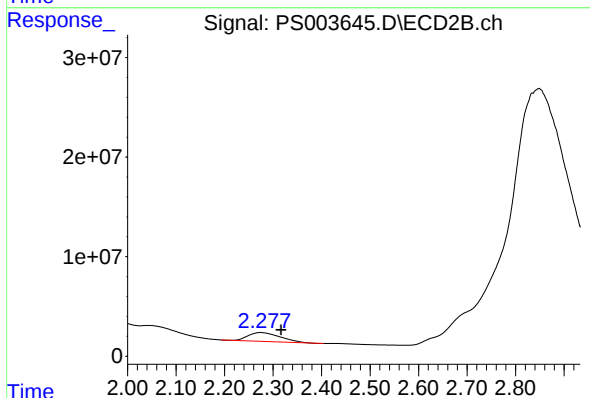


#1 Dalapon

R.T.: 2.274 min
Delta R.T.: -0.042 min
Response: 40082868
Conc: 63.30 ng/ml

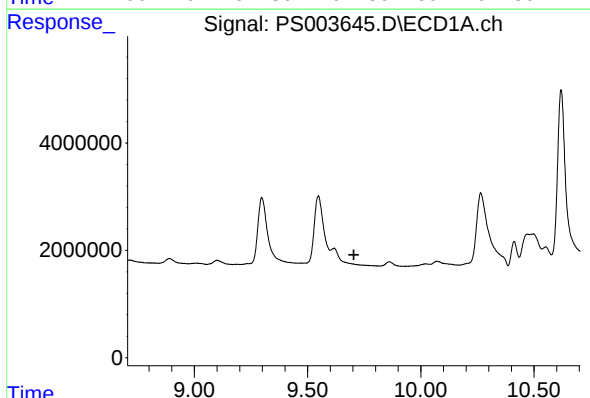


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

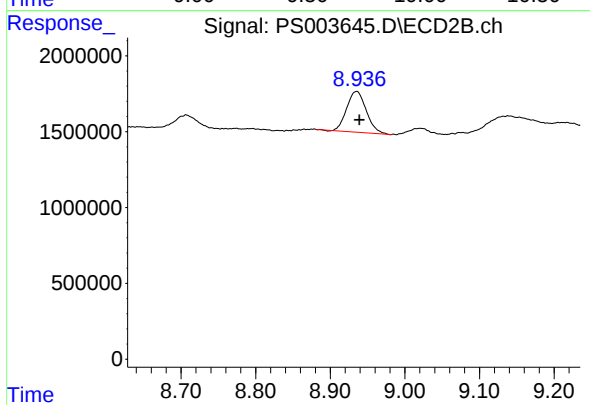

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.935 min
Delta R.T.: -0.004 min
Response: 4900363
Conc: 7.94 ng/ml

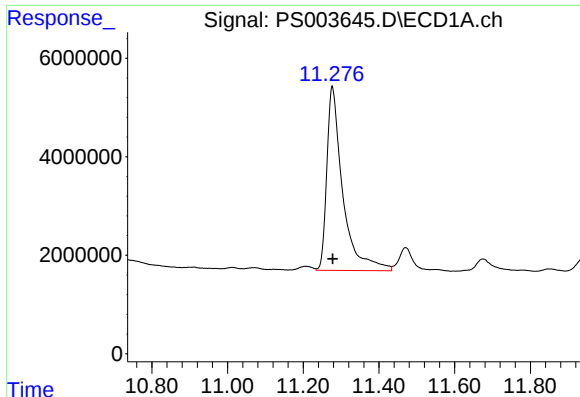

#4 2,4-DCAA


R.T.: 11.277 min
Delta R.T.: 0.000 min
Response: 109005811
Conc: 248.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

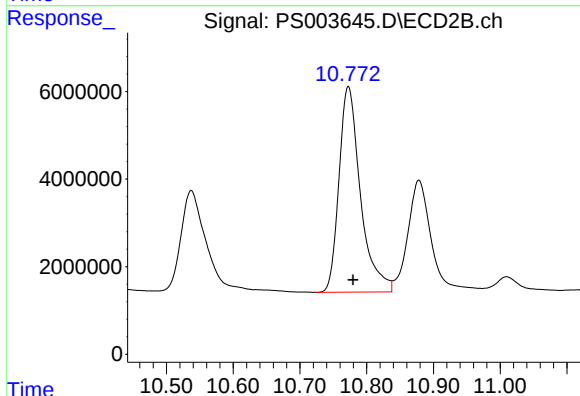


#4 2,4-DCAA

R.T.: 10.773 min
Delta R.T.: -0.007 min
Response: 104895840
Conc: 223.39 ng/ml

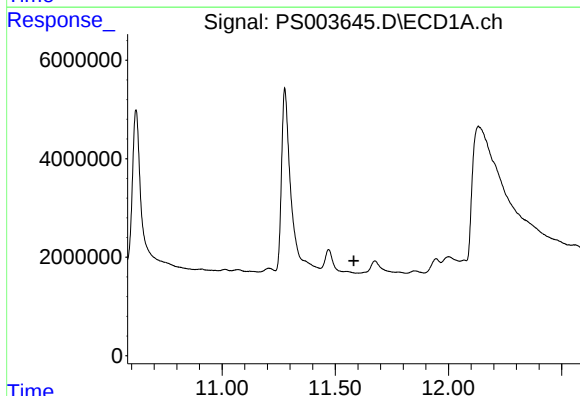


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

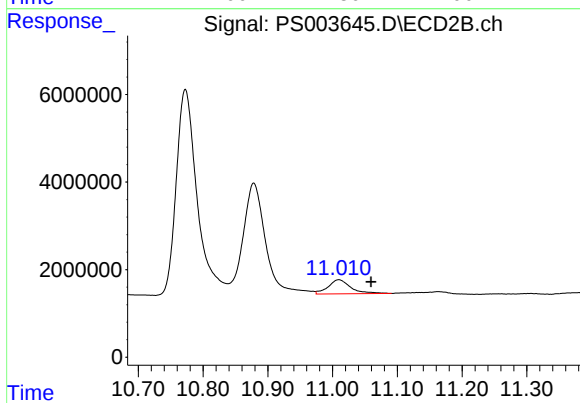

#5 DICAMBA


R.T.: 11.010 min
Delta R.T.: -0.050 min
Response: 7880974
Conc: 4.72 ng/ml

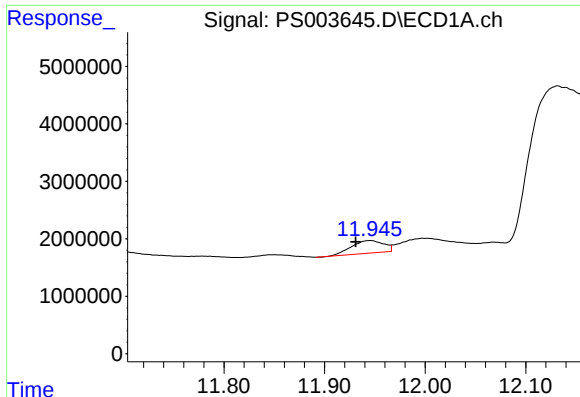

#6 MCP


R.T.: 11.945 min
Delta R.T.: 0.014 min
Response: 4896871
Conc: 3.73 ug/ml

Instrument :
ECD_S
ClientSampleId :

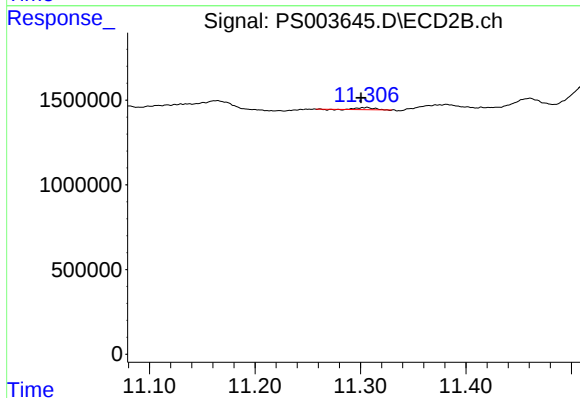


#6 MCP

R.T.: 11.304 min
Delta R.T.: 0.004 min
Response: 109547
Conc: 0.09 ug/ml

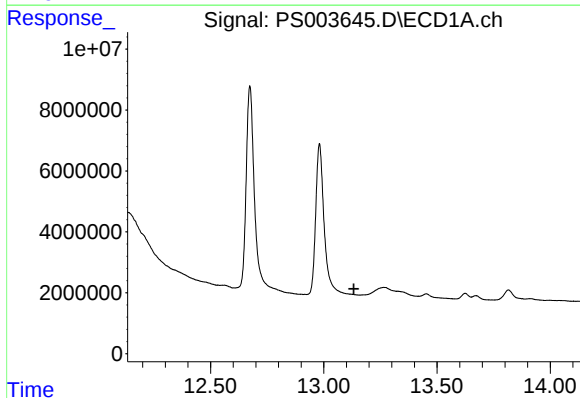


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

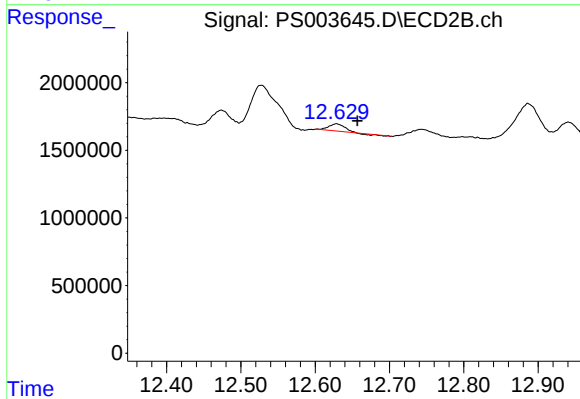

#9 2,4-D


R.T.: 12.629 min
Delta R.T.: -0.028 min
Response: 752223
Conc: 1.43 ng/ml

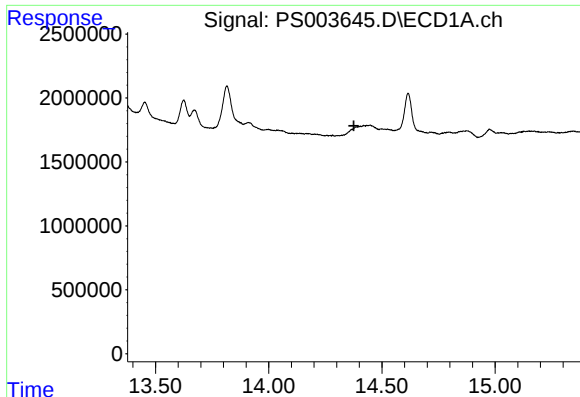

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

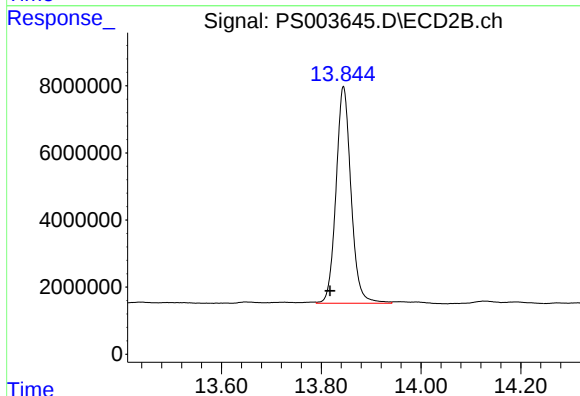


#11 2,4,5-TP (SILVEX)

R.T.: 13.845 min
Delta R.T.: 0.027 min
Response: 134778968
Conc: 52.93 ng/ml

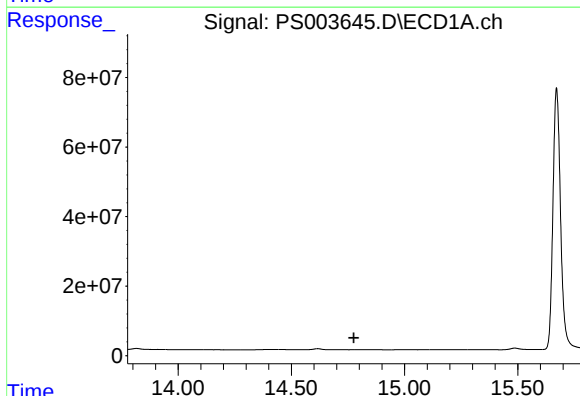


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

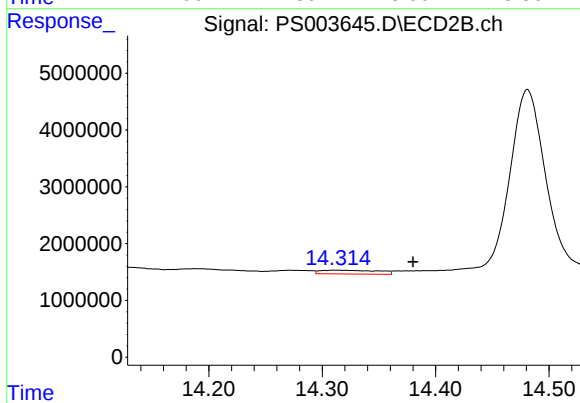

#12 2,4,5-T


R.T.: 14.313 min
Delta R.T.: -0.067 min
Response: 2347860
Conc: 1.16 ng/ml

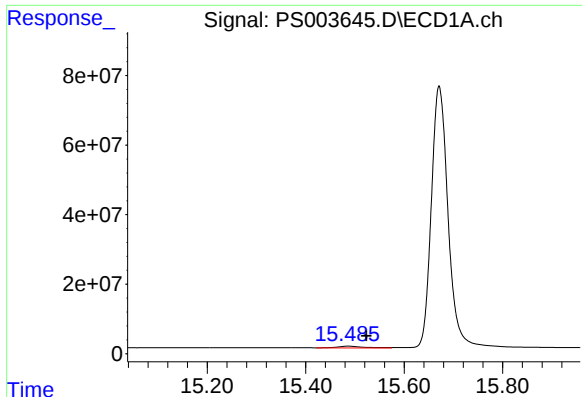

#13 2,4-DB


R.T.: 15.486 min
Delta R.T.: -0.037 min
Response: 18599076
Conc: 78.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

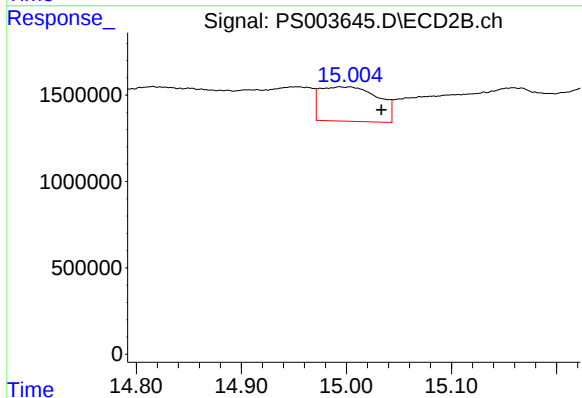


#13 2,4-DB

R.T.: 14.995 min
Delta R.T.: -0.039 min
Response: 7614484
Conc: 29.82 ng/ml

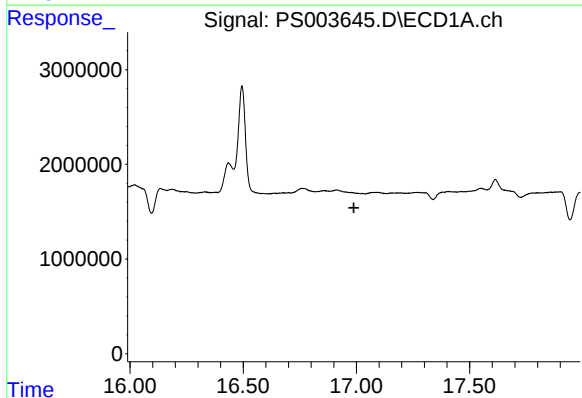


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

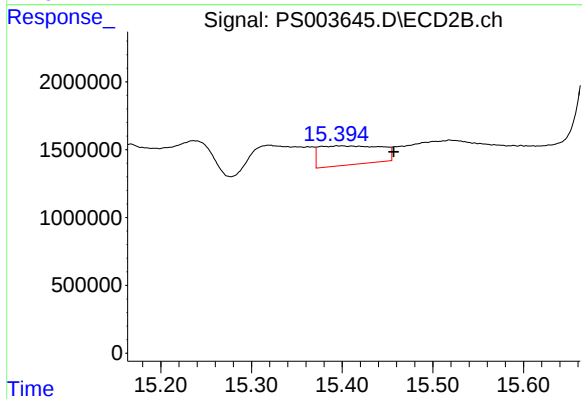

#14 DINOSEB


R.T.: 15.398 min
Delta R.T.: -0.059 min
Response: 6594057
Conc: 3.69 ng/ml

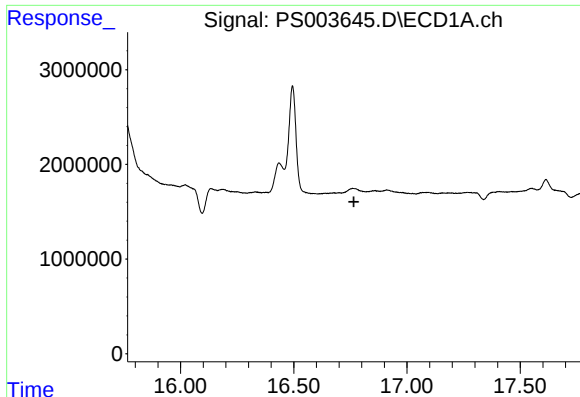

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

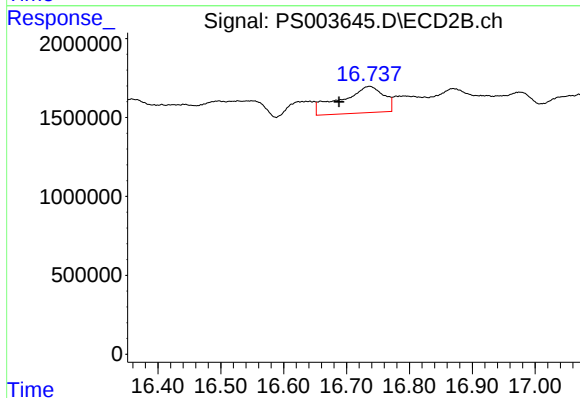


#15 Picloram

R.T.: 16.736 min
Delta R.T.: 0.048 min
Response: 8006065
Conc: 3.15 ng/ml

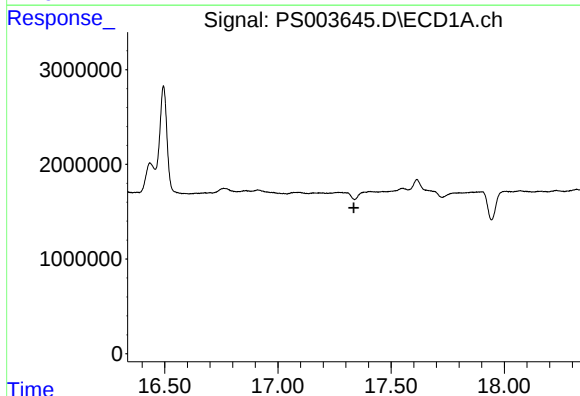

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

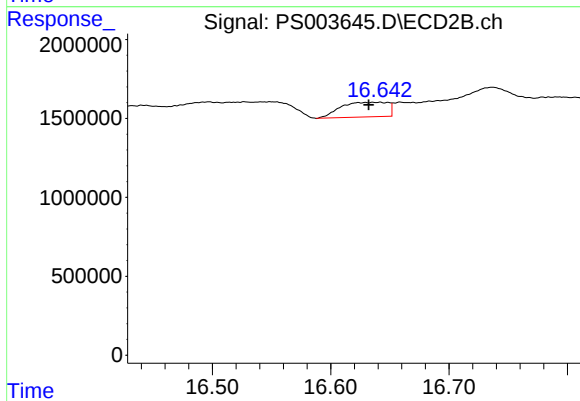

#16 DCPA

R.T.: 16.639 min
Delta R.T.: 0.007 min
Response: 2587208
Conc: 0.83 ng/ml