

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
 Data File : PS003646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2019 04:04
 Operator : EI\SJ
 Sample : K1943-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 13:50:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.283	10.778	124.0E6	117.4E6	282.393	250.108
Target Compounds							
1) T	Dalapon	2.792	2.283	34988124	57315652	53.833	90.520 #
2) T	3,5-DICHL...	0.000	8.940	0	3359436	N.D.	5.441 #
3) T	4-Nitroph...	0.000	9.945	0	4957565	N.D.	22.050 #
5) T	DICAMBA	0.000	11.016	0	6905072	N.D.	4.133 #
6) T	MCP	11.954	11.313	2494433	70452	1.900	0.060 #
9) T	2,4-D	0.000	12.636	0	1114702	N.D.	2.124 #
11) T	2,4,5-TP ...	0.000	13.792	0	324190	N.D.	0.127 #
12) T	2,4,5-T	0.000	14.321	0	1150468	N.D.	0.570 #
13) T	2,4-DB	0.000	15.010	0	6194885	N.D.	24.260 #
14) T	DINOSEB	0.000	15.405	0	4747108	N.D.	2.660 #
15) T	Picloram	0.000	16.715	0	5374383	N.D.	2.117 #
16) T	DCPA	0.000	16.643	0	3242133	N.D.	1.042 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032019\
Data File : PS003646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2019 04:04
Operator : EI\SJ
Sample : K1943-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 13:50:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

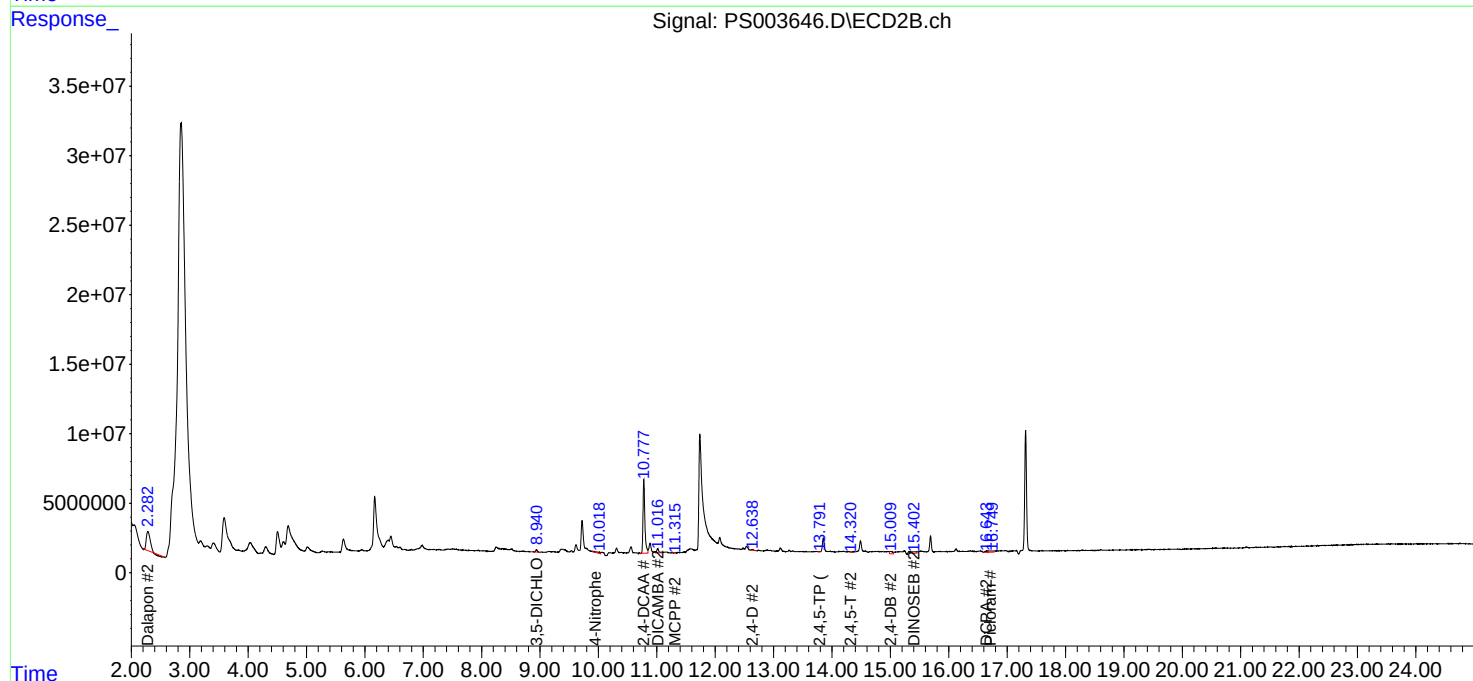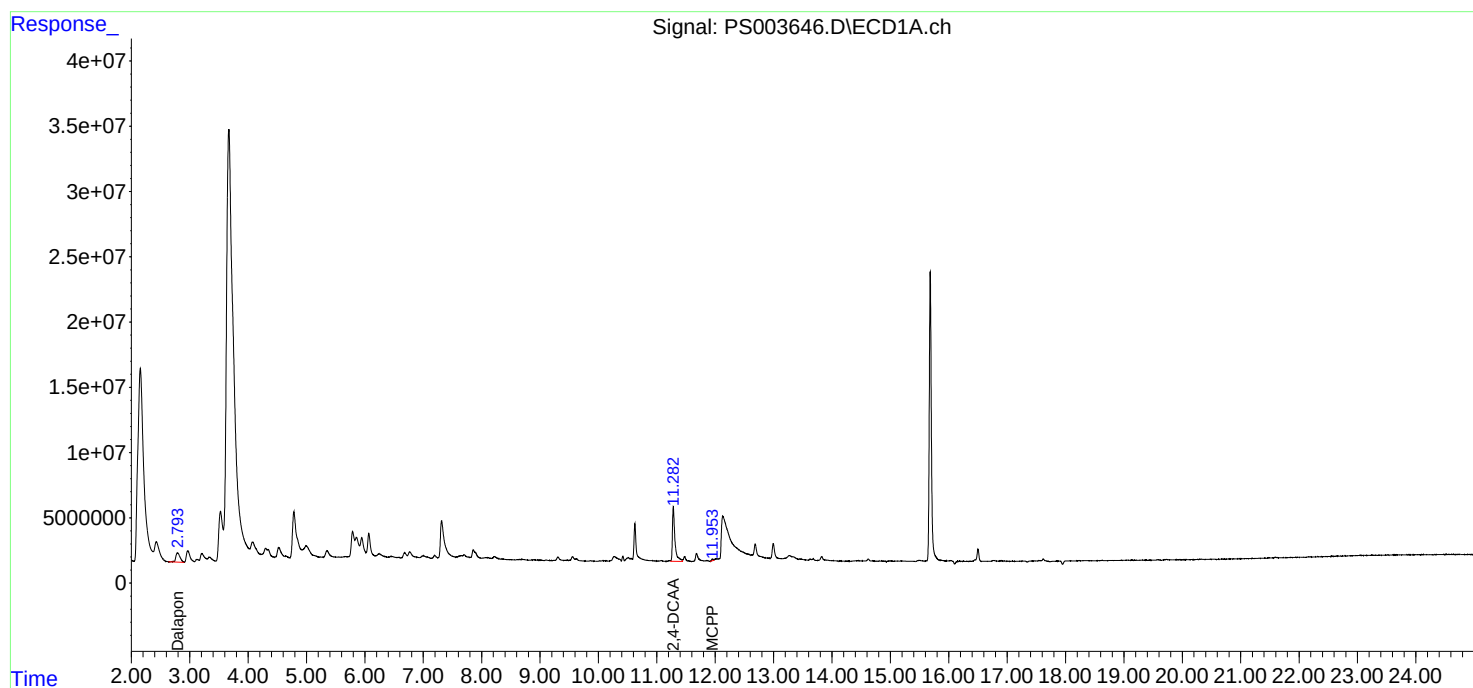


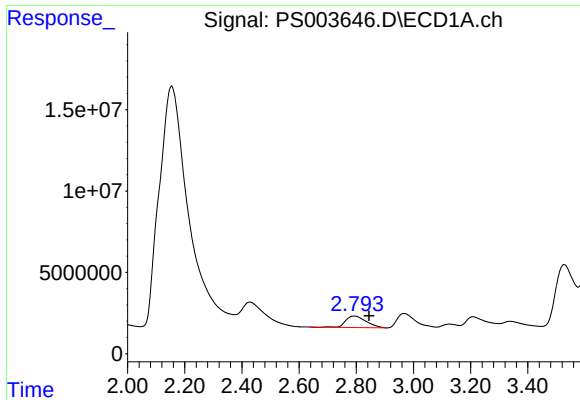

#1 Dalapon


R.T.: 2.792 min
Delta R.T.: -0.052 min
Response: 34988124
Conc: 53.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

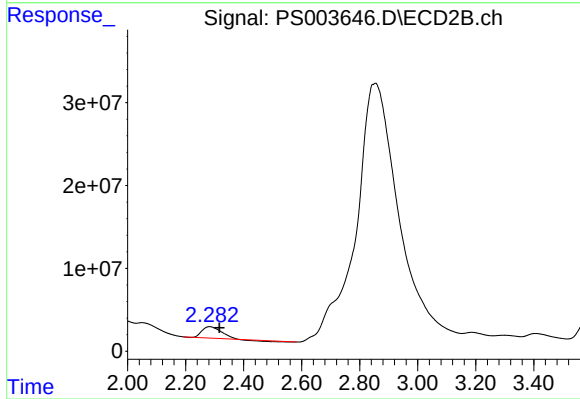


#1 Dalapon

R.T.: 2.283 min
Delta R.T.: -0.034 min
Response: 57315652
Conc: 90.52 ng/ml

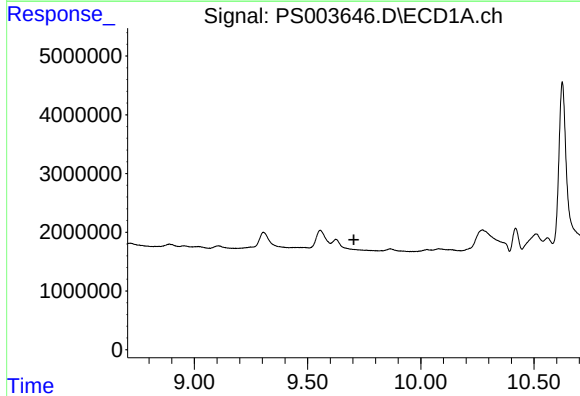


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

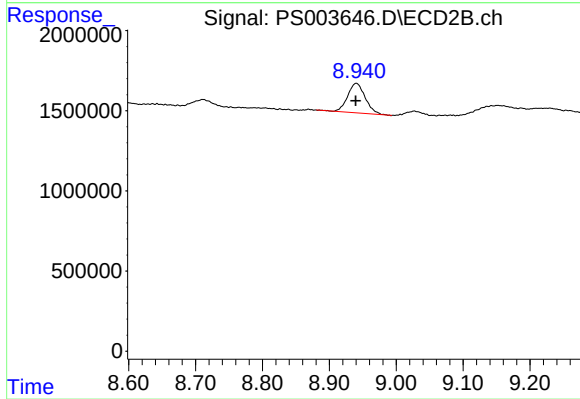

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.940 min
Delta R.T.: 0.000 min
Response: 3359436
Conc: 5.44 ng/ml

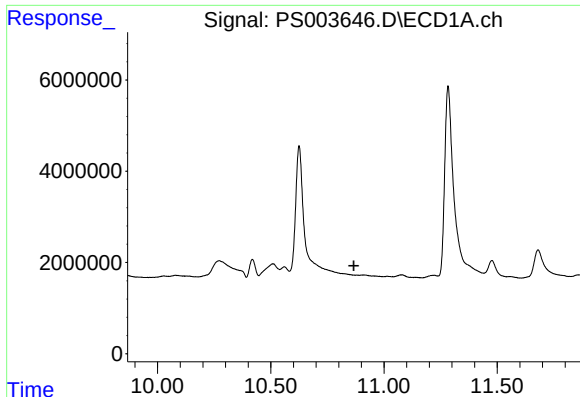

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

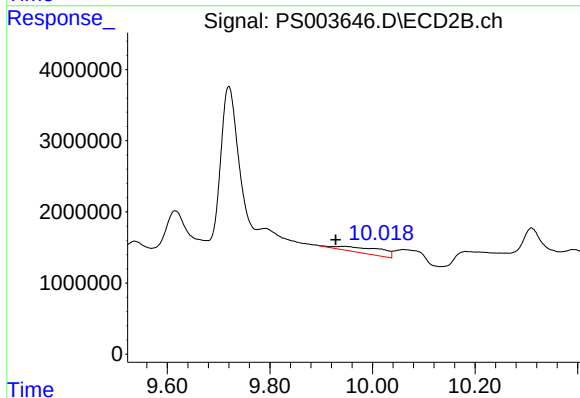


#3 4-Nitrophenol

R.T.: 9.945 min
Delta R.T.: 0.016 min
Response: 4957565
Conc: 22.05 ng/ml

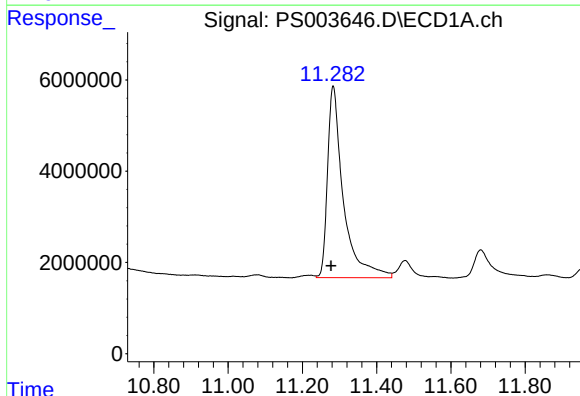


#4 2,4-DCAA

R.T.: 11.283 min
Delta R.T.: 0.005 min
Response: 123977615
Conc: 282.39 ng/ml

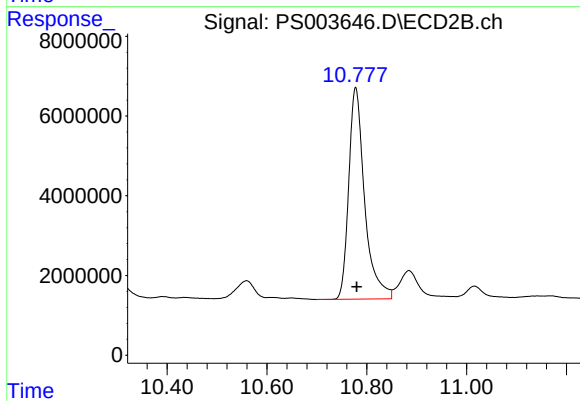

#4 2,4-DCAA


R.T.: 10.778 min
Delta R.T.: -0.002 min
Response: 117443062
Conc: 250.11 ng/ml

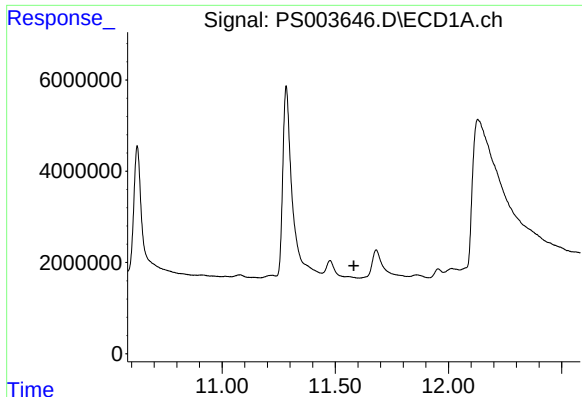

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

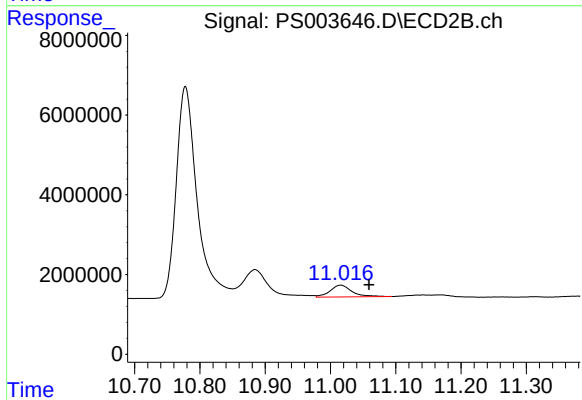


#5 DICAMBA

R.T.: 11.016 min
Delta R.T.: -0.044 min
Response: 6905072
Conc: 4.13 ng/ml

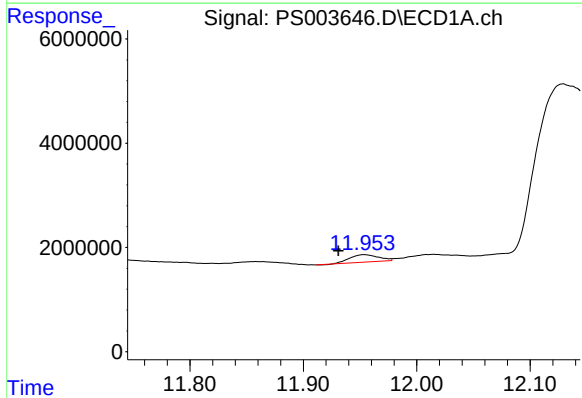


#6 MCP

R.T.: 11.954 min
Delta R.T.: 0.023 min
Response: 2494433
Conc: 1.90 ug/ml

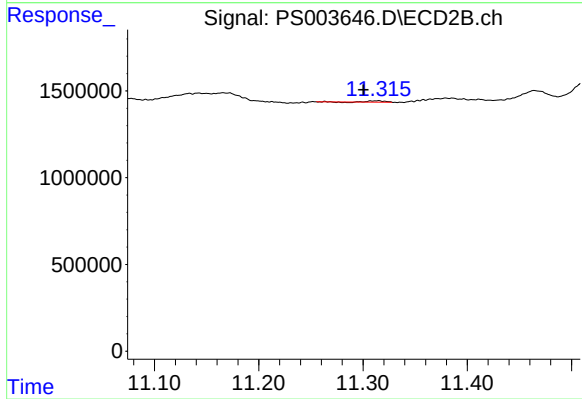

#6 MCP


R.T.: 11.313 min
Delta R.T.: 0.012 min
Response: 70452
Conc: 0.06 ug/ml

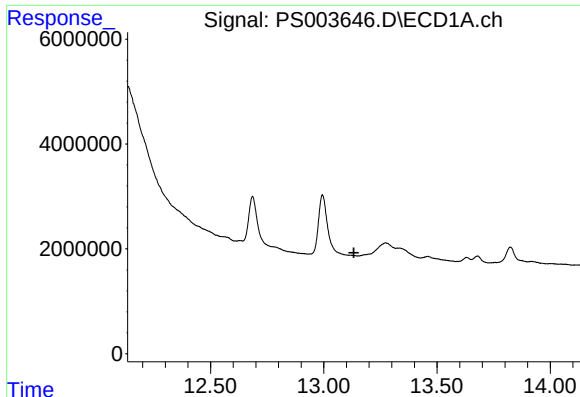

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

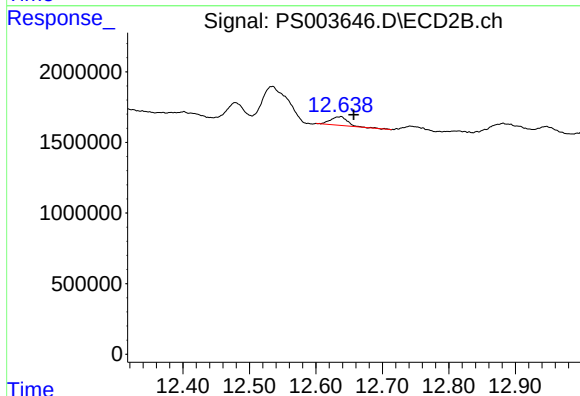


#9 2,4-D

R.T.: 12.636 min
Delta R.T.: -0.021 min
Response: 1114702
Conc: 2.12 ng/ml

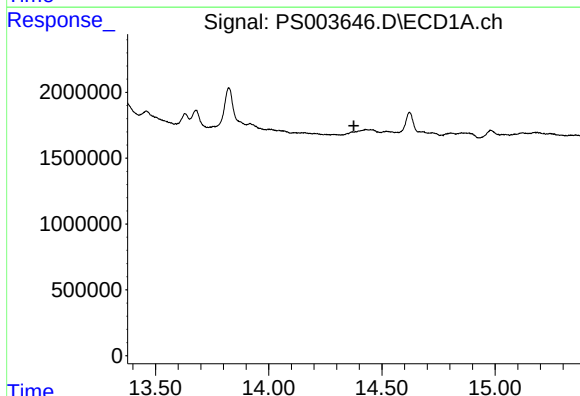


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

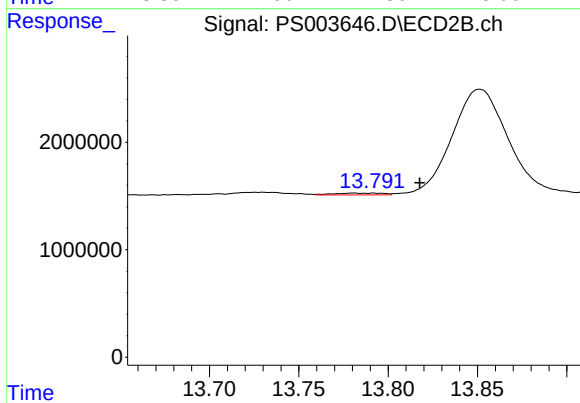

#11 2,4,5-TP (SILVEX)


R.T.: 13.792 min
Delta R.T.: -0.026 min
Response: 324190
Conc: 0.13 ng/ml

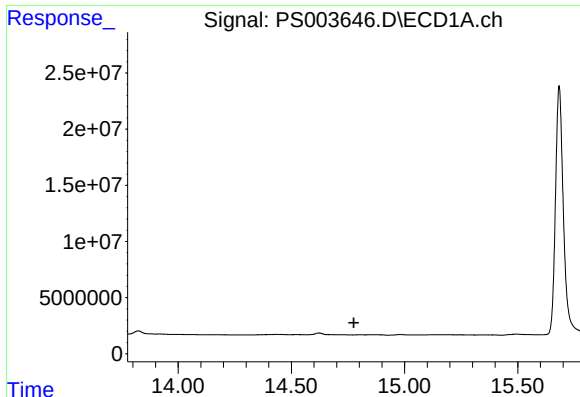

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

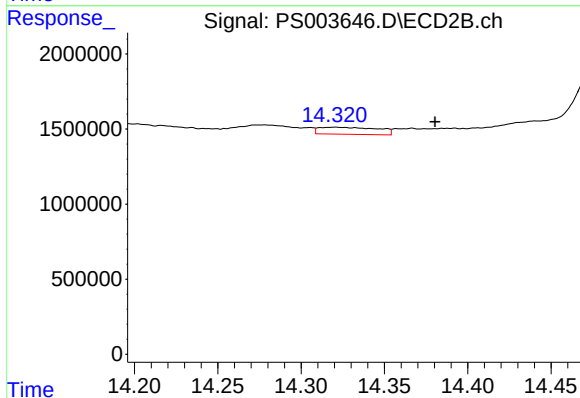


#12 2,4,5-T

R.T.: 14.321 min
Delta R.T.: -0.060 min
Response: 1150468
Conc: 0.57 ng/ml

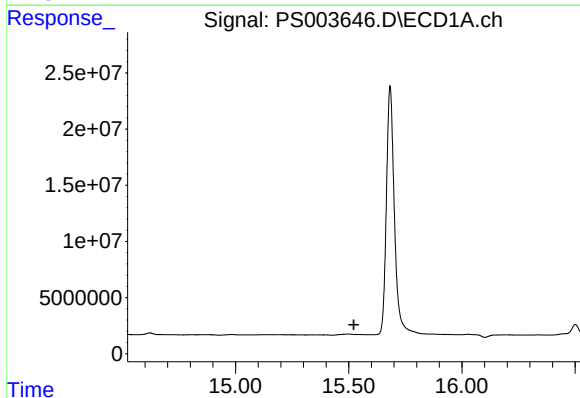


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

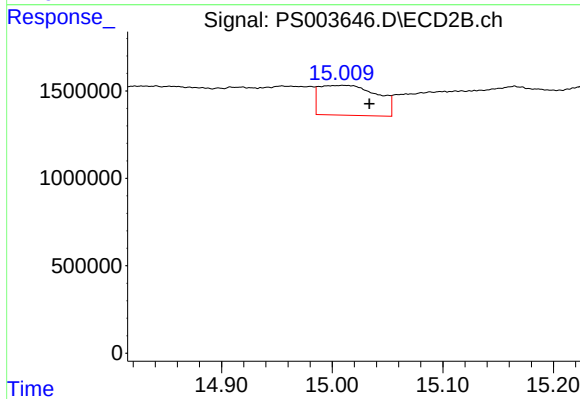

#13 2,4-DB


R.T.: 15.010 min
Delta R.T.: -0.023 min
Response: 6194885
Conc: 24.26 ng/ml

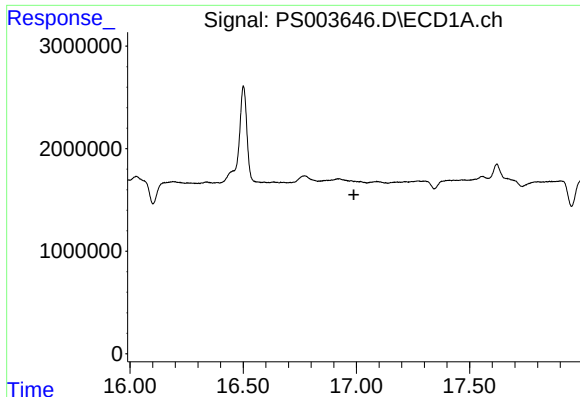

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

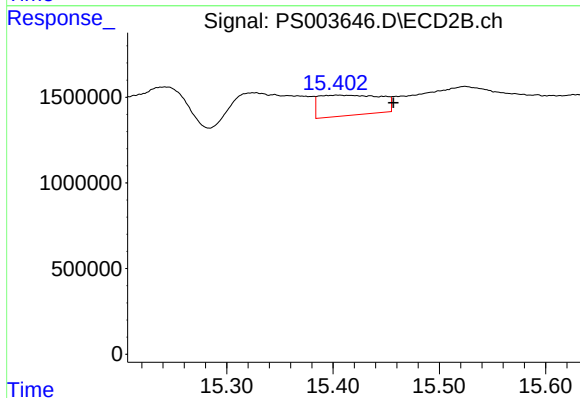


#14 DINOSEB

R.T.: 15.405 min
Delta R.T.: -0.052 min
Response: 4747108
Conc: 2.66 ng/ml

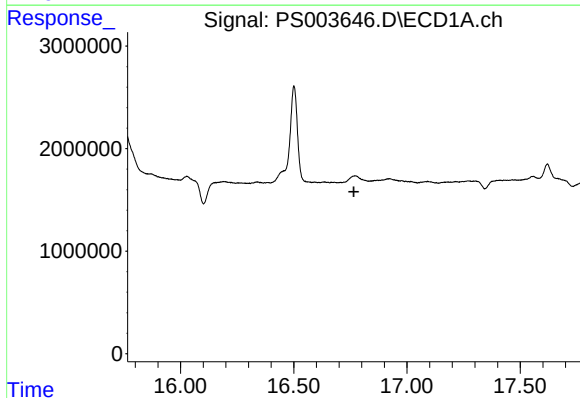


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

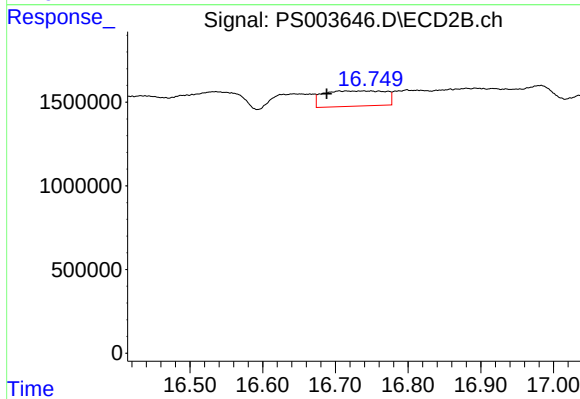

#15 Picloram


R.T.: 16.715 min
Delta R.T.: 0.027 min
Response: 5374383
Conc: 2.12 ng/ml

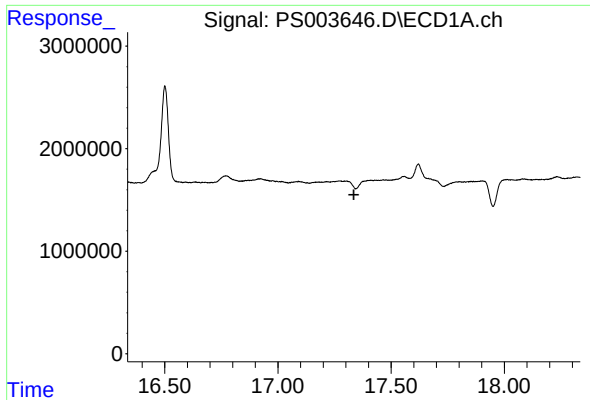

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

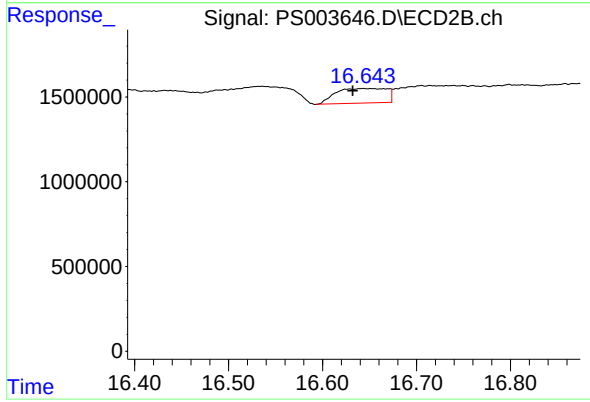

#16 DCPA

R.T.: 16.643 min
Delta R.T.: 0.011 min
Response: 3242133
Conc: 1.04 ng/ml