

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032020\
 Data File : PS009377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2020 16:31
 Operator : DD\AJ
 Sample : PB127711BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 16:49:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.243	6.933	299.9E6	293.8E6	542.164	534.956
Target Compounds							
1) T	Dalapon	3.004	2.587	19764632	89303635	25.345	113.421 #
2) T	3,5-DICHL...	0.000	6.110	0	42072485	N.D.	51.730
6) T	MCP	7.598	0.000	6526245	0	2.652	N.D. #
7) T	MCPA	7.794	0.000	69667870	0	22.874	N.D. #
8) T	DICHLORPROP	0.000	7.753	0	24956507	N.D.	44.981
11) T	2,4,5-TP ...	0.000	8.787	0	28364992	N.D.	9.515
12) T	2,4,5-T	9.453	9.252	23006517	35703496	9.044	12.094 #
14) T	DINOSEB	11.190	10.048	18140025	18496795	8.874	8.421
15) T	Picloram	11.038	11.022	109.6E6	169.2E6	36.120	41.561
16) T	DCPA	0.000	11.022	0	169.2E6	N.D.	43.698



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032020\
Data File : PS009377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2020 16:31
Operator : DD\AJ
Sample : PB127711BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 16:49:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

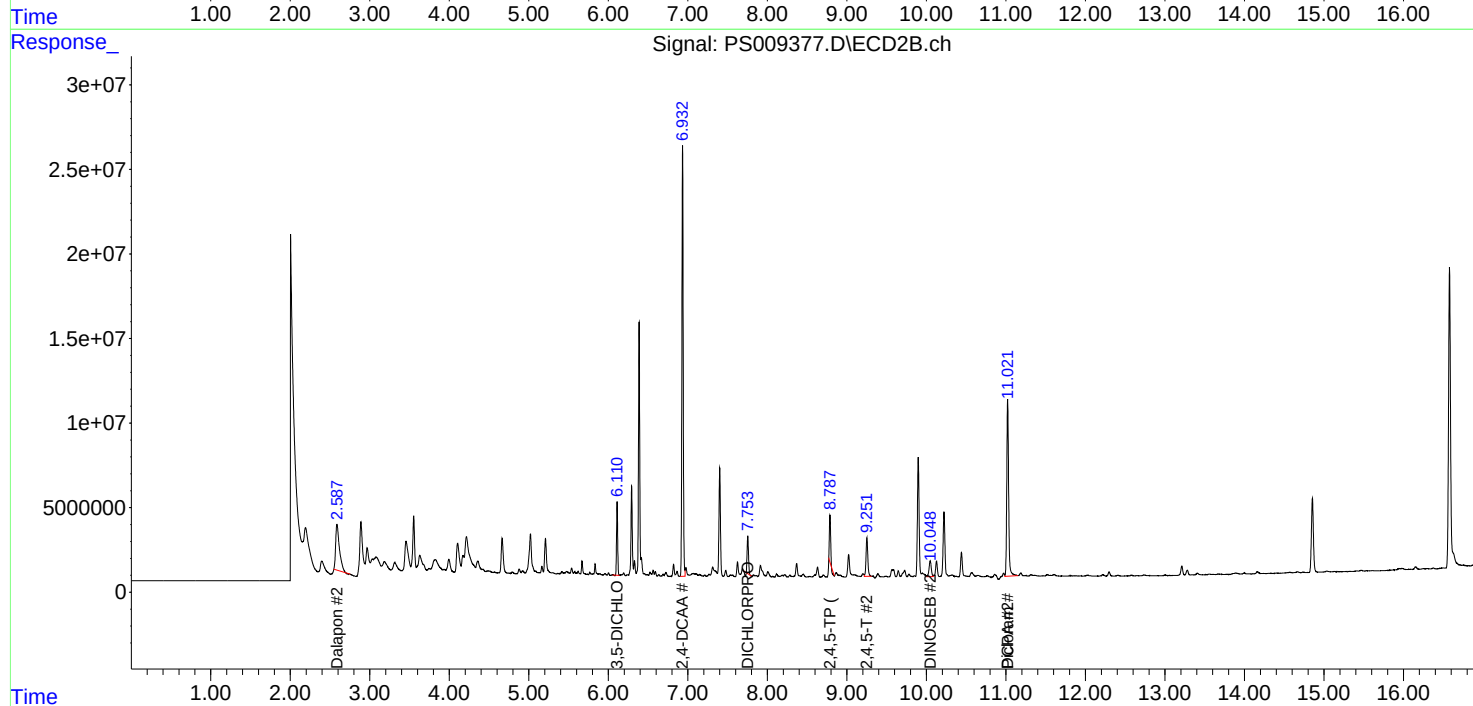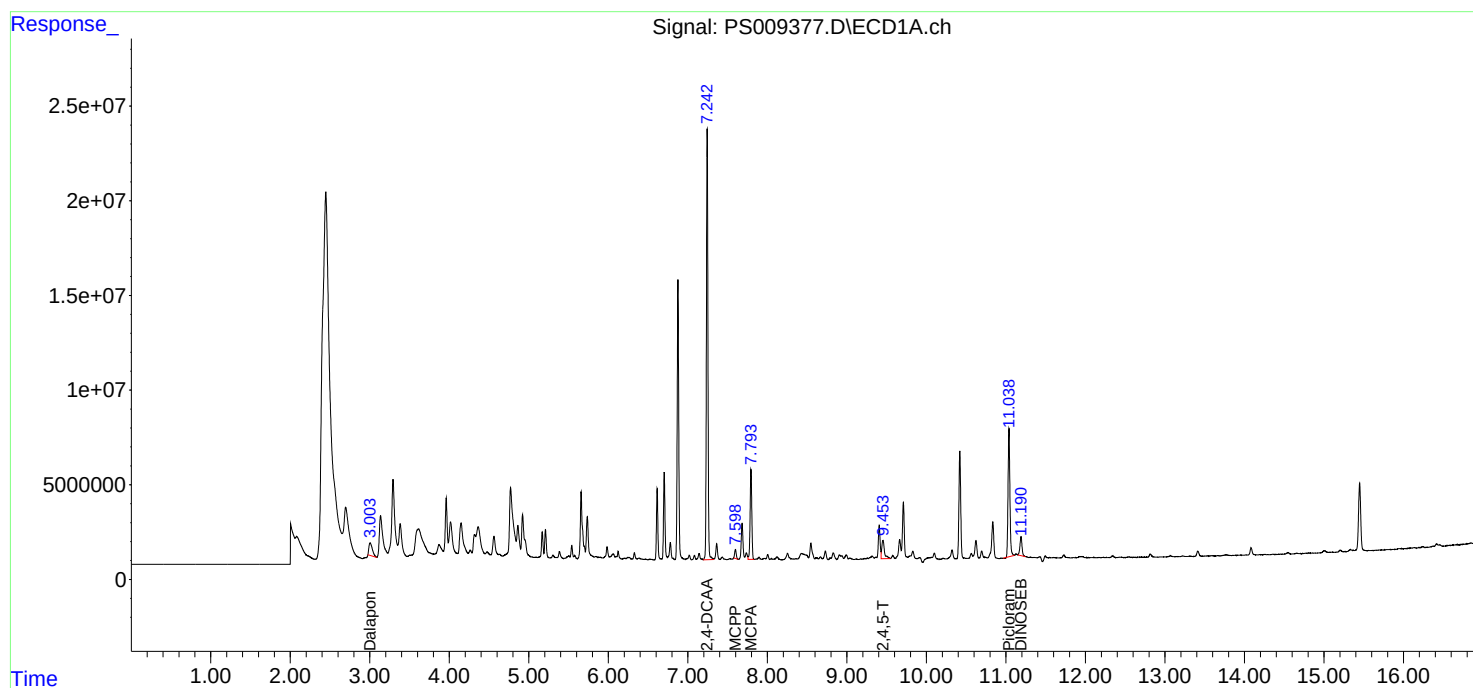


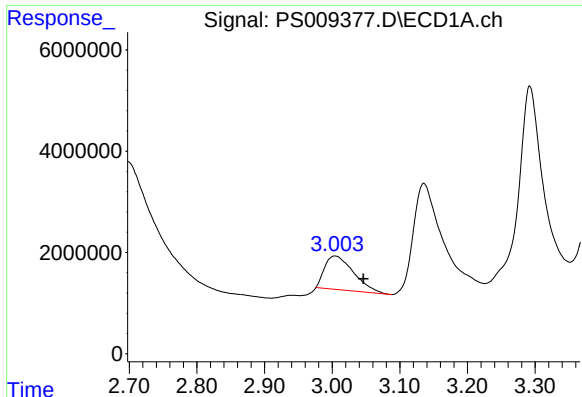

#1 Dalapon


R.T.: 3.004 min
Delta R.T.: -0.042 min
Response: 19764632
Conc: 25.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

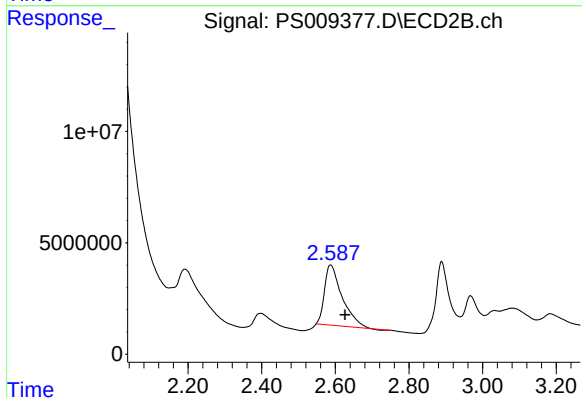


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.039 min
Response: 89303635
Conc: 113.42 ng/ml

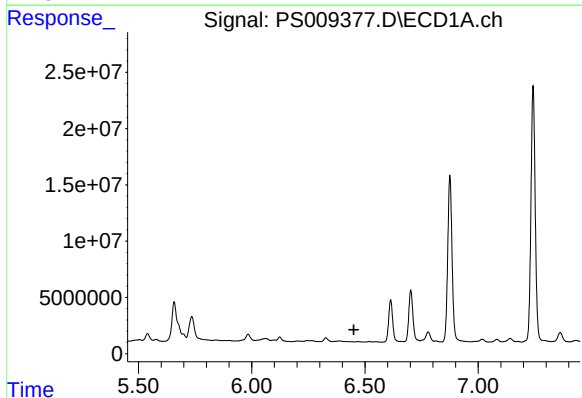


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

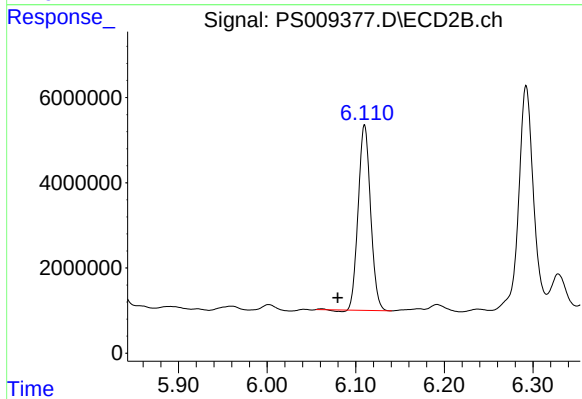

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 42072485
Conc: 51.73 ng/ml

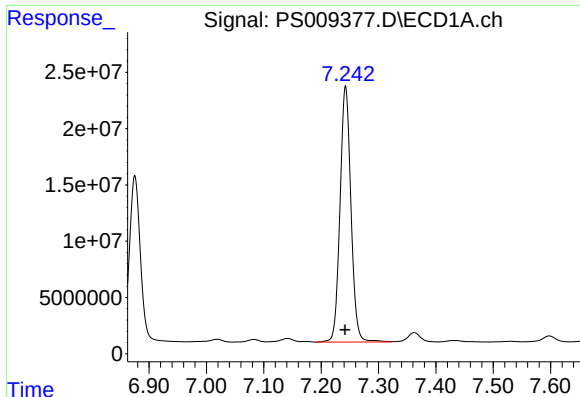

#4 2,4-DCAA


R.T.: 7.243 min
Delta R.T.: 0.000 min
Response: 299908786
Conc: 542.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

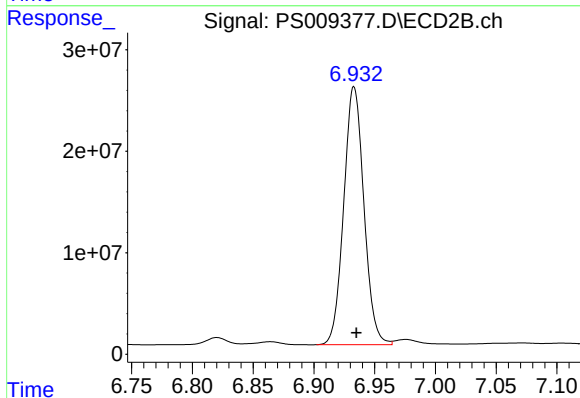


#4 2,4-DCAA

R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 293796690
Conc: 534.96 ng/ml

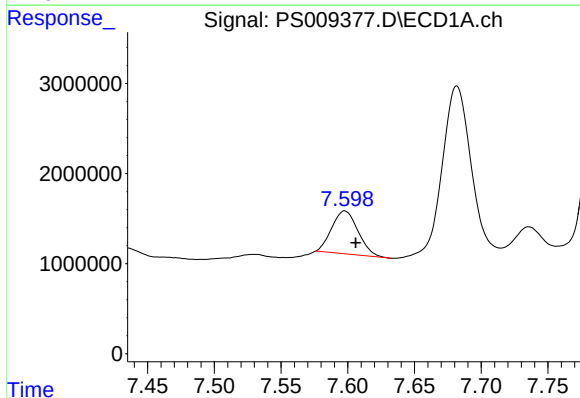


#6 MCP

R.T.: 7.598 min
Delta R.T.: -0.008 min
Response: 6526245
Conc: 2.65 ug/ml

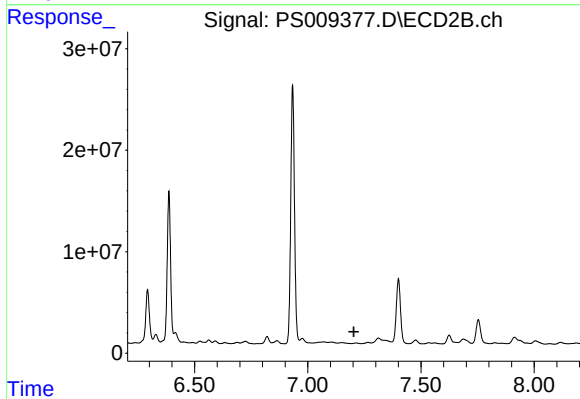

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

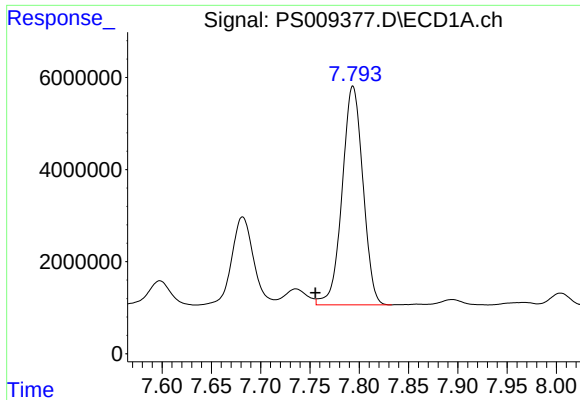

#7 MCPA


R.T.: 7.794 min
Delta R.T.: 0.038 min
Response: 69667870
Conc: 22.87 ug/ml

Instrument :
ECD_S
ClientSampleId :

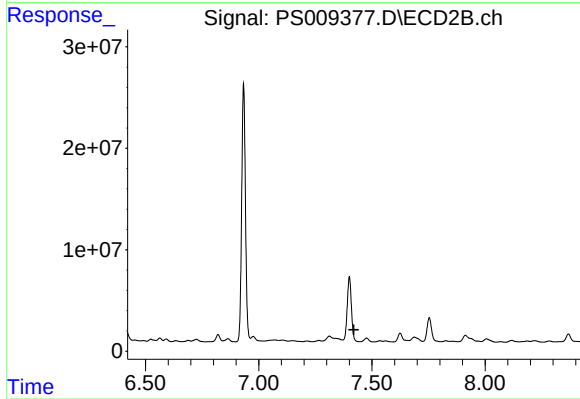


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.420 min
Response: 0
Conc: N.D.

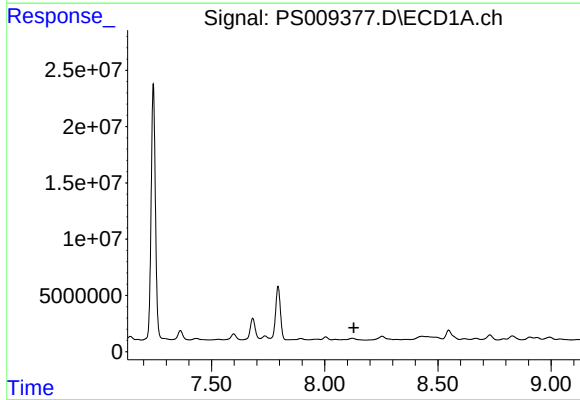


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

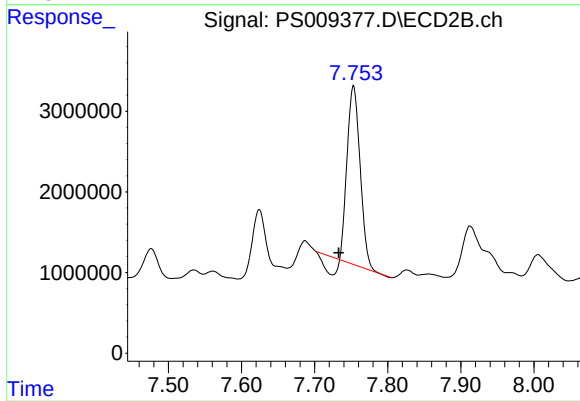

#8 DICHLORPROP


R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 24956507
Conc: 44.98 ng/ml

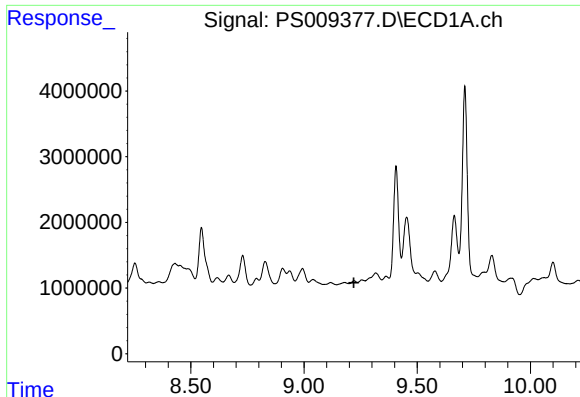

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

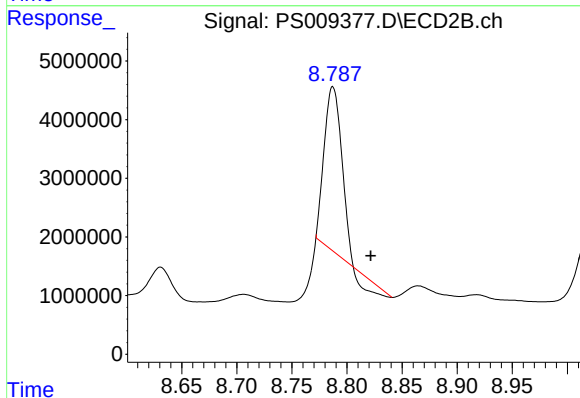


#11 2,4,5-TP (SILVEX)

R.T.: 8.787 min
Delta R.T.: -0.034 min
Response: 28364992
Conc: 9.51 ng/ml

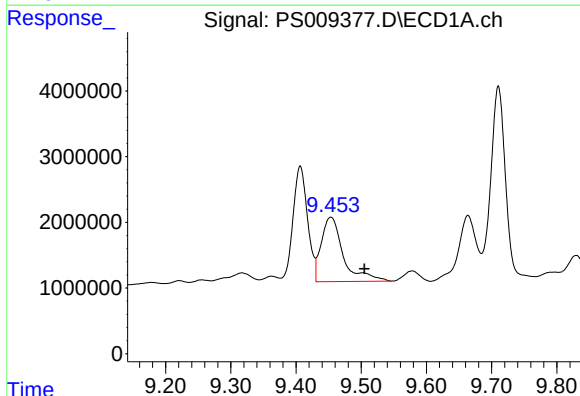


#12 2,4,5-T

R.T.: 9.453 min
Delta R.T.: -0.052 min
Response: 23006517
Conc: 9.04 ng/ml

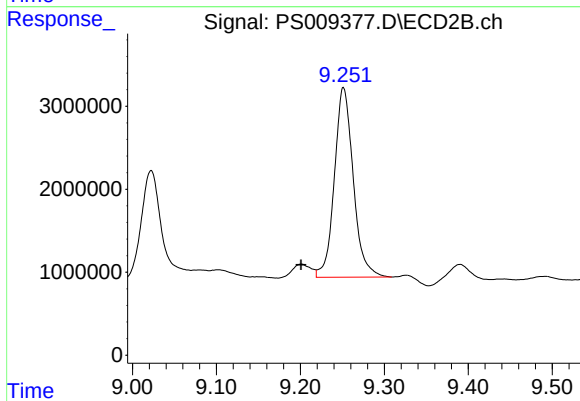

#12 2,4,5-T


R.T.: 9.252 min
Delta R.T.: 0.051 min
Response: 35703496
Conc: 12.09 ng/ml

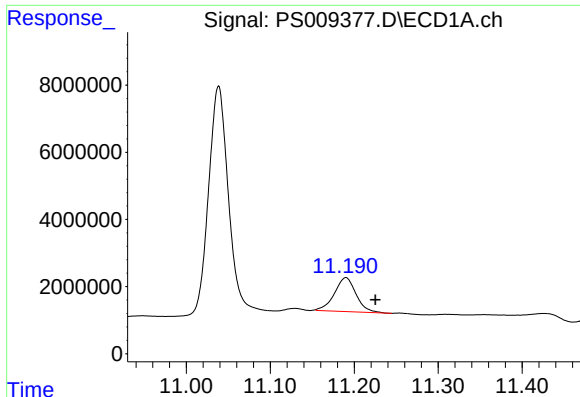

#14 DINOSEB


R.T.: 11.190 min
Delta R.T.: -0.035 min
Response: 18140025
Conc: 8.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

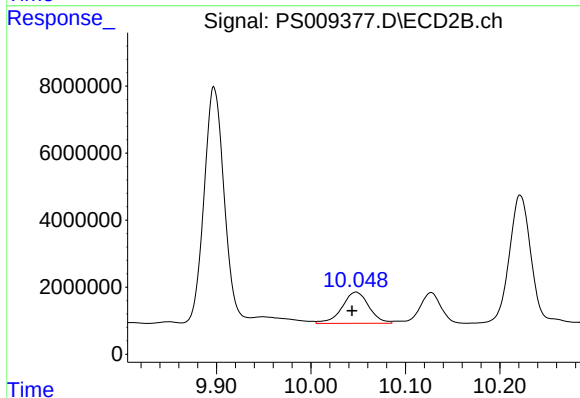


#14 DINOSEB

R.T.: 10.048 min
Delta R.T.: 0.004 min
Response: 18496795
Conc: 8.42 ng/ml

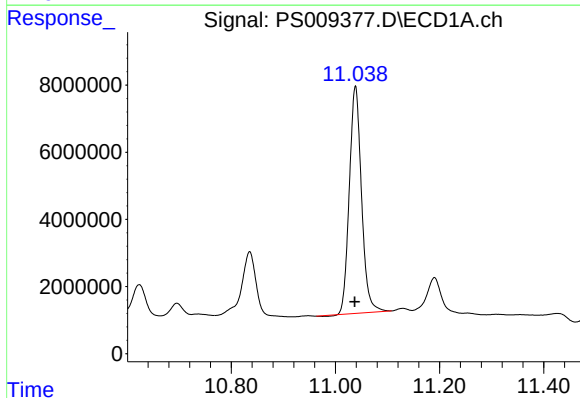


#15 Picloram

R.T.: 11.038 min
Delta R.T.: 0.000 min
Response: 109622909
Conc: 36.12 ng/ml

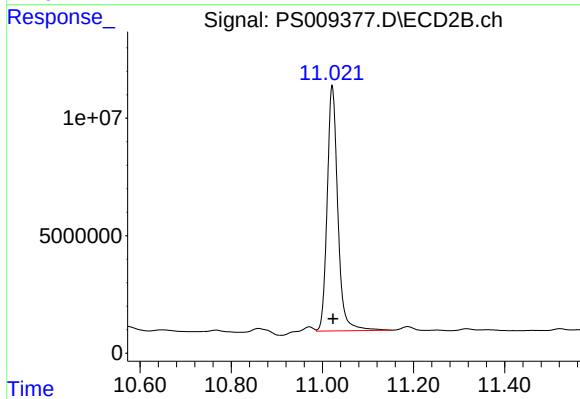

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.002 min
Response: 169242693
Conc: 41.56 ng/ml

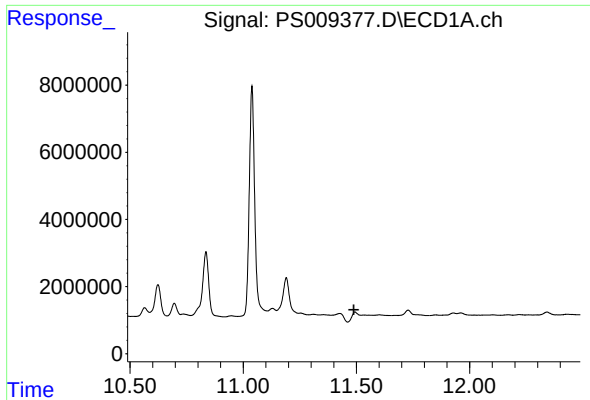

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

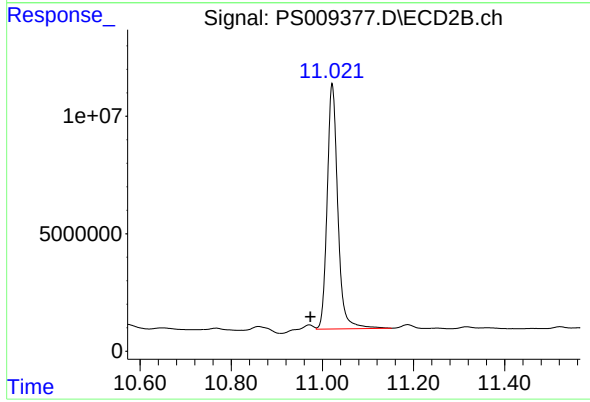

#16 DCPA

R.T.: 11.022 min
Delta R.T.: 0.048 min
Response: 169242693
Conc: 43.70 ng/ml