

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032020\
 Data File : PS009379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2020 17:16
 Operator : DD\AJ
 Sample : PB127711TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 17:33:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	300.1E6	255.2E6	542.558	464.716
Target Compounds							
1) T	Dalapon	3.006	2.588	36828103	79755113	47.226	101.294 #
2) T	3,5-DICHL...	0.000	6.109	0	56884319	N.D.	69.942
3) T	4-Nitroph...	7.117	0.000	18866844	0	79.036	N.D. #
8) T	DICHLORPROP	0.000	7.753	0	35252619	N.D.	63.539
10) T	Pentachlo...	0.000	8.457	0	7117562	N.D.	<MDL
12) T	2,4,5-T	9.446	0.000	56807673	0	22.331	N.D. #
14) T	DINOSEB	11.190	10.050	20078909	1513974	9.823	<MDL #
15) T	Picloram	11.037	11.023	9089682	9650076	2.995	2.370
16) T	DCPA	0.000	11.023	0	9650076	N.D.	2.492



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032020\
Data File : PS009379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2020 17:16
Operator : DD\AJ
Sample : PB127711TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 17:33:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

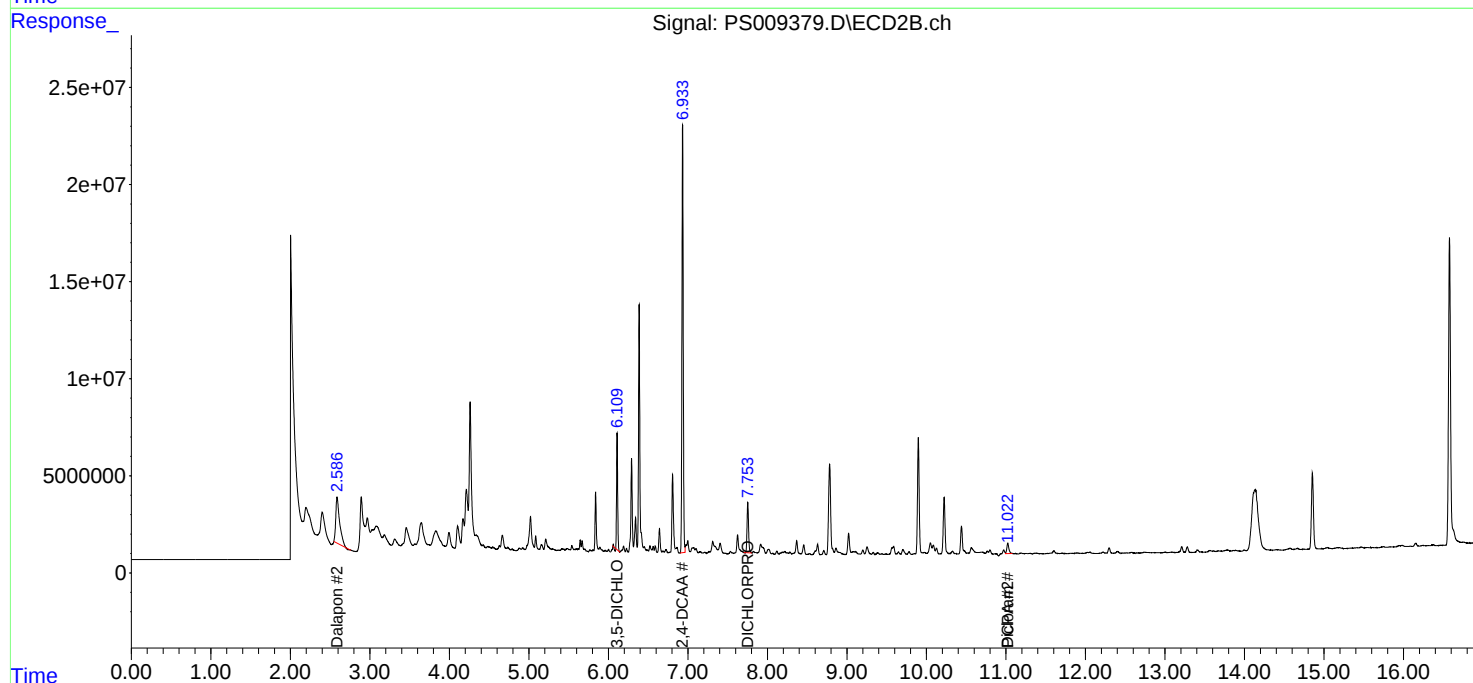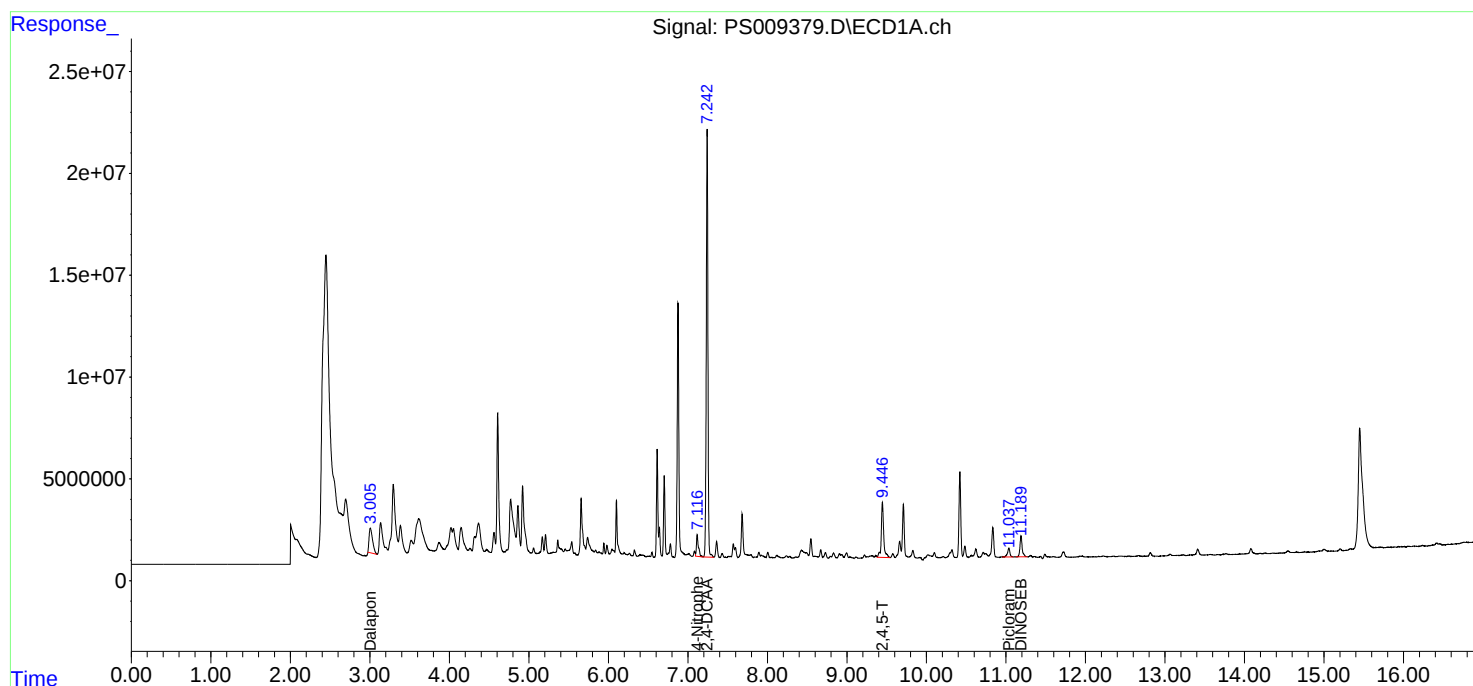


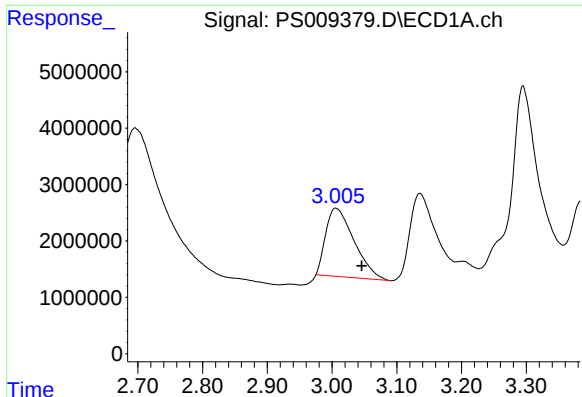

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 36828103
Conc: 47.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

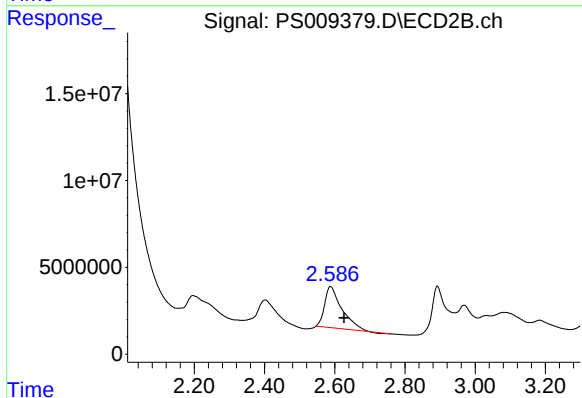


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.039 min
Response: 79755113
Conc: 101.29 ng/ml

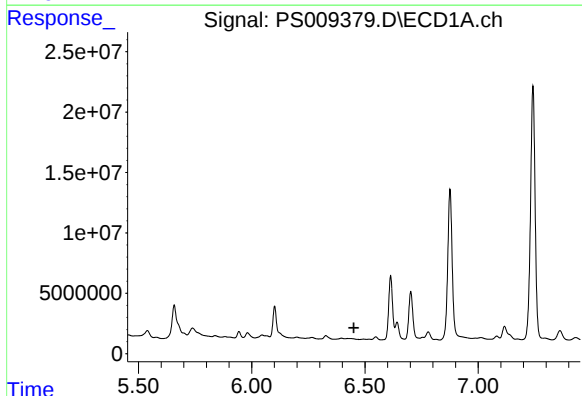


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

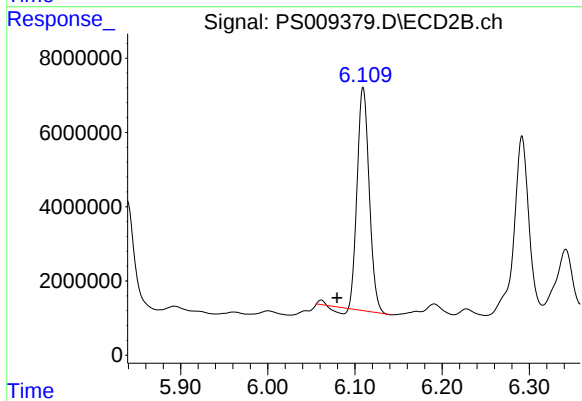

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.030 min
Response: 56884319
Conc: 69.94 ng/ml

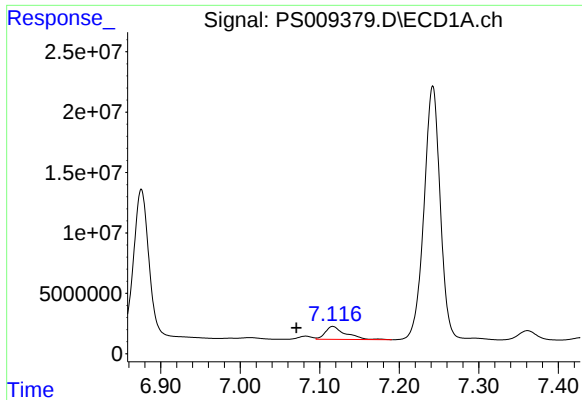

#3 4-Nitrophenol


R.T.: 7.117 min
Delta R.T.: 0.046 min
Response: 18866844
Conc: 79.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

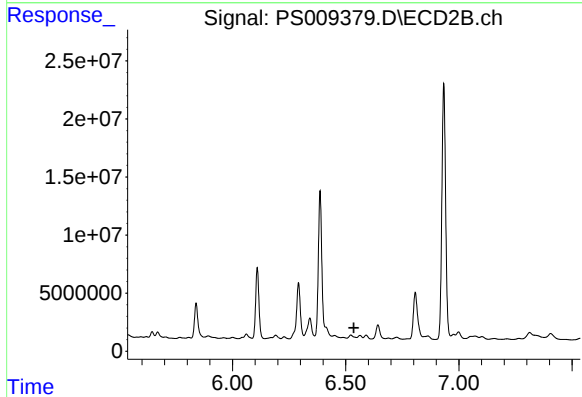


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.536 min
Response: 0
Conc: N.D.

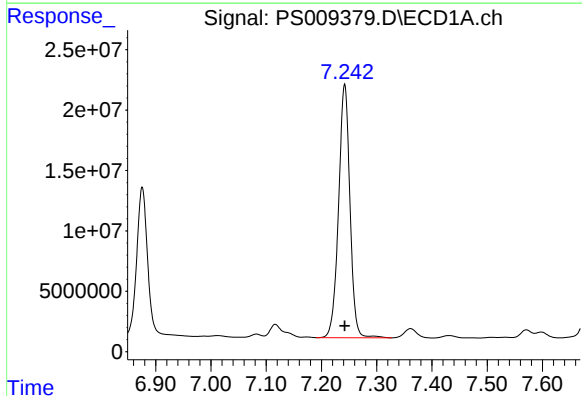


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 300126791
Conc: 542.56 ng/ml

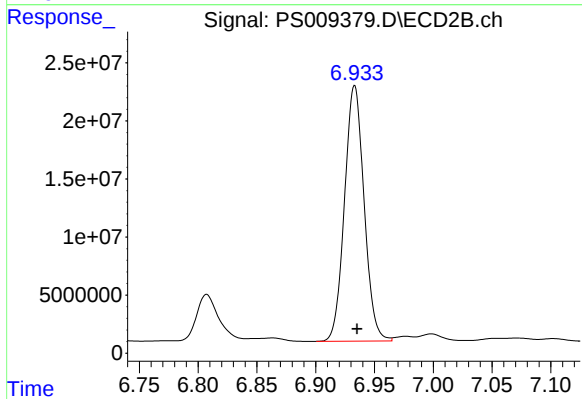

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 255220697
Conc: 464.72 ng/ml

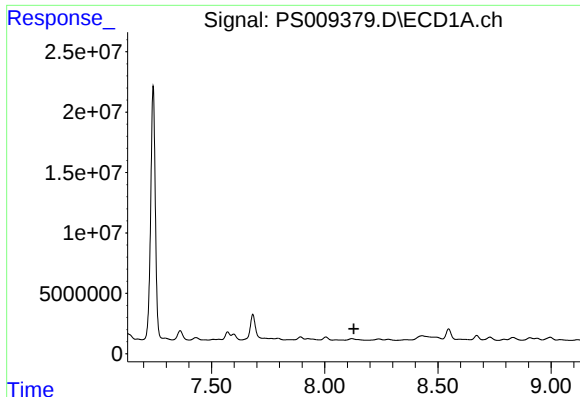

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

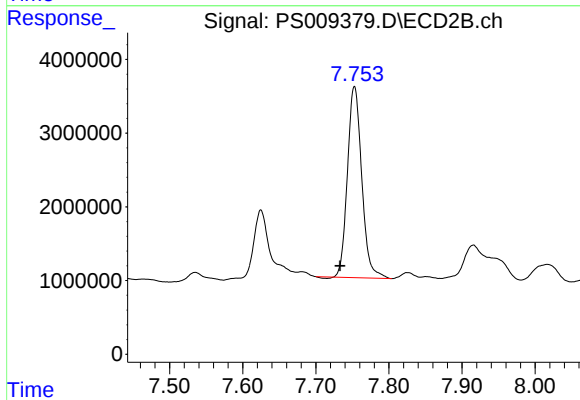


#8 DICHLORPROP

R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 35252619
Conc: 63.54 ng/ml

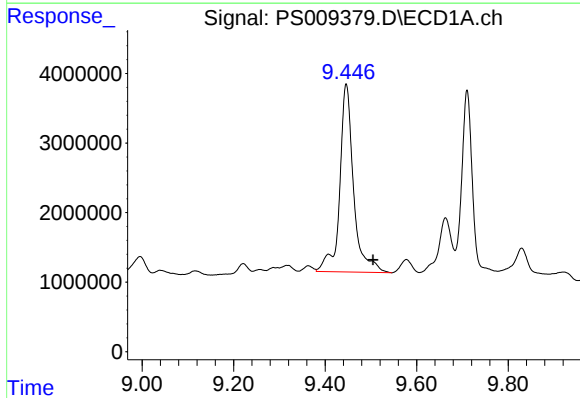


#12 2,4,5-T

R.T.: 9.446 min
Delta R.T.: -0.059 min
Response: 56807673
Conc: 22.33 ng/ml

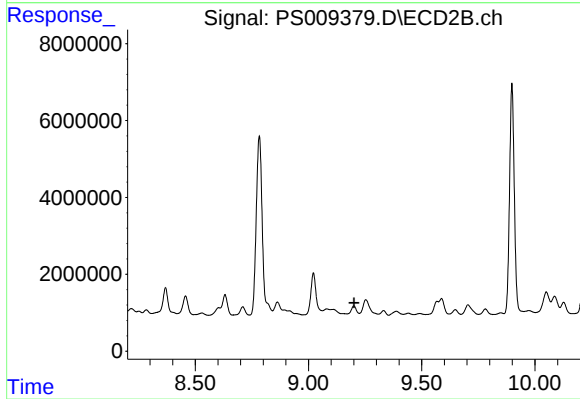

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

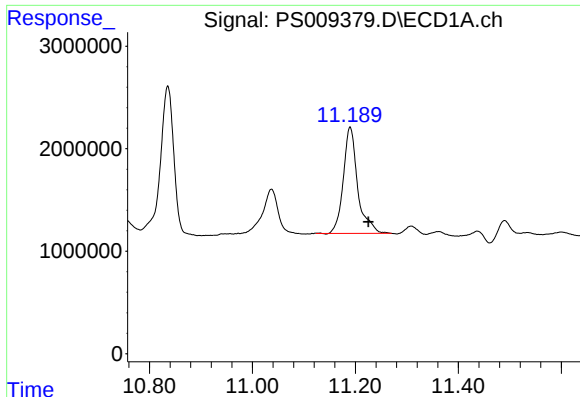

#14 DINOSEB


R.T.: 11.190 min
Delta R.T.: -0.035 min
Response: 20078909
Conc: 9.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

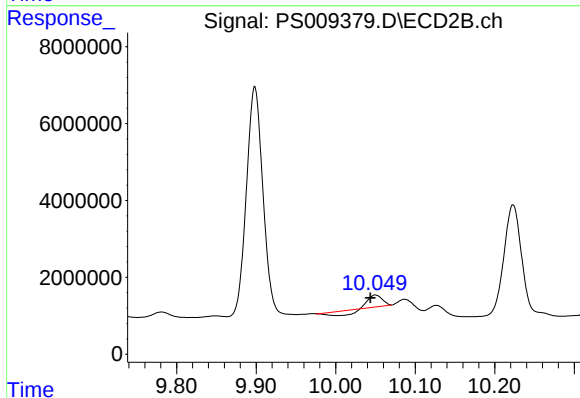


#14 DINOSEB

R.T.: 10.050 min
Delta R.T.: 0.007 min
Response: 1513974
Conc: N.D.

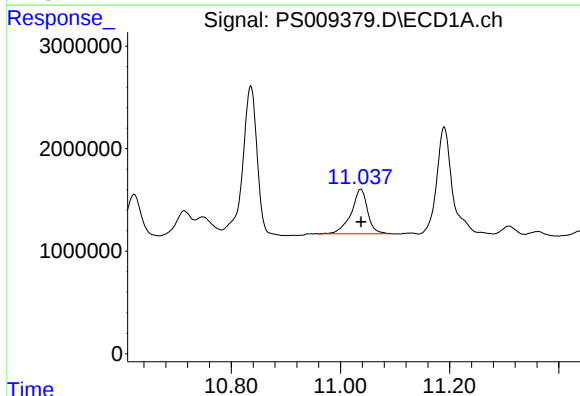


#15 Picloram

R.T.: 11.037 min
Delta R.T.: 0.000 min
Response: 9089682
Conc: 3.00 ng/ml

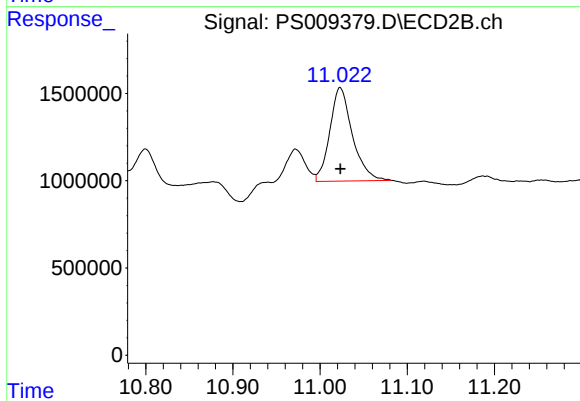

#15 Picloram


R.T.: 11.023 min
Delta R.T.: 0.000 min
Response: 9650076
Conc: 2.37 ng/ml

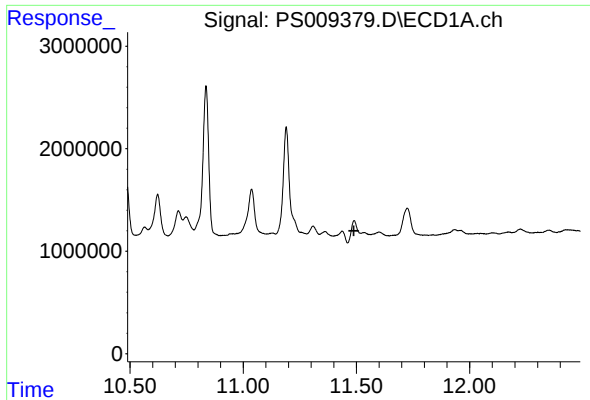

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

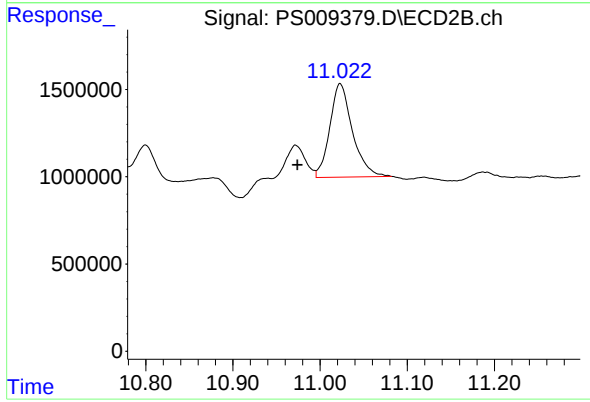

#16 DCPA

R.T.: 11.023 min
Delta R.T.: 0.049 min
Response: 9650076
Conc: 2.49 ng/ml