

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032020\
 Data File : PS009383.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2020 18:48
 Operator : DD\AJ
 Sample : L1965-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 22:53:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	311.1E6	260.2E6	562.307	473.707
Target Compounds							
1) T	Dalapon	3.006	2.590	21603577	88415927	27.703	112.294 #
2) T	3,5-DICHL...	0.000	6.110	0	62440671	N.D.	76.774
3) T	4-Nitroph...	7.116	0.000	21900160	0	91.743	N.D. #
8) T	DICHLORPROP	0.000	7.753	0	39438240	N.D.	71.083
10) T	Pentachlo...	0.000	8.456	0	7083952	N.D.	<MDL
12) T	2,4,5-T	9.447	0.000	57685341	0	22.676	N.D. #
14) T	DINOSEB	11.189	10.053	20522312	3721494	10.040	1.694 #
15) T	Picloram	0.000	11.022	0	8455094	N.D.	2.076
16) T	DCPA	0.000	11.022	0	8455094	N.D.	2.183



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032020\
Data File : PS009383.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2020 18:48
Operator : DD\AJ
Sample : L1965-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 22:53:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

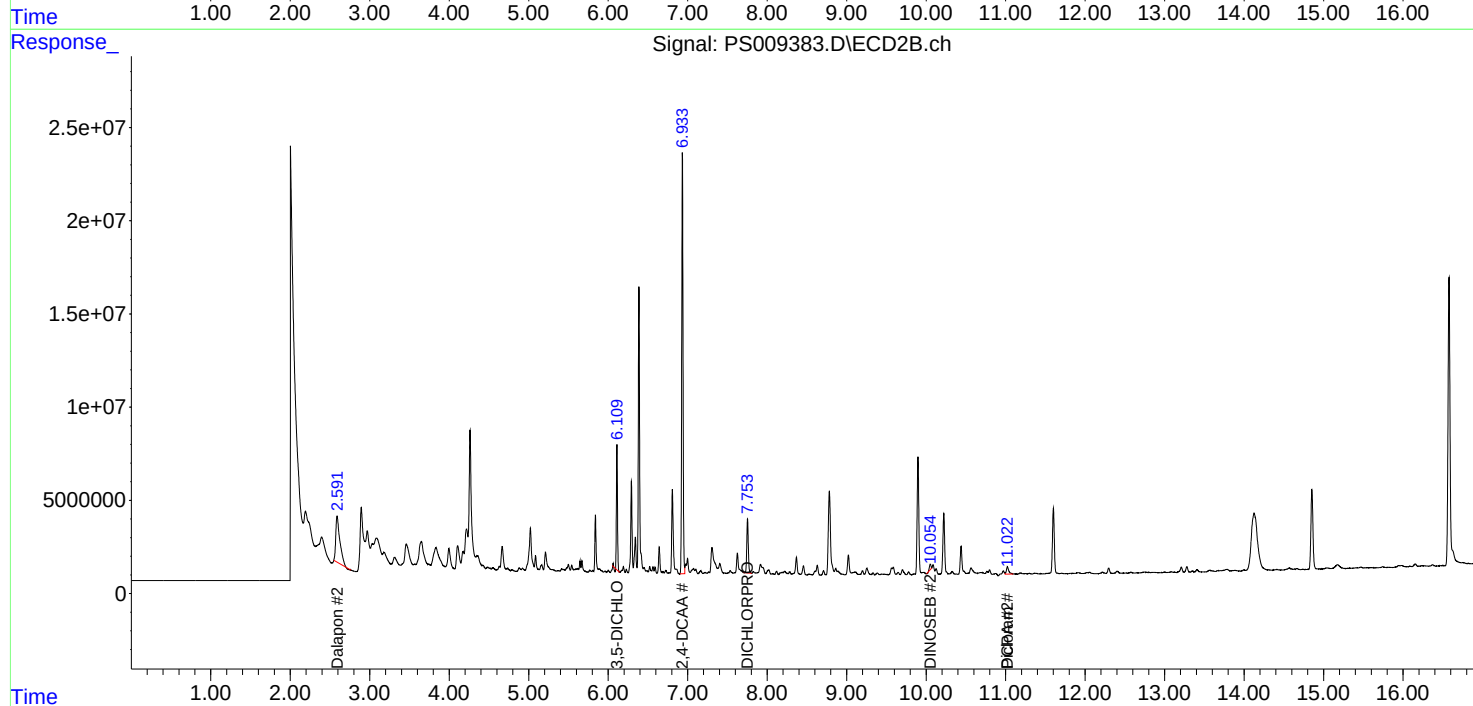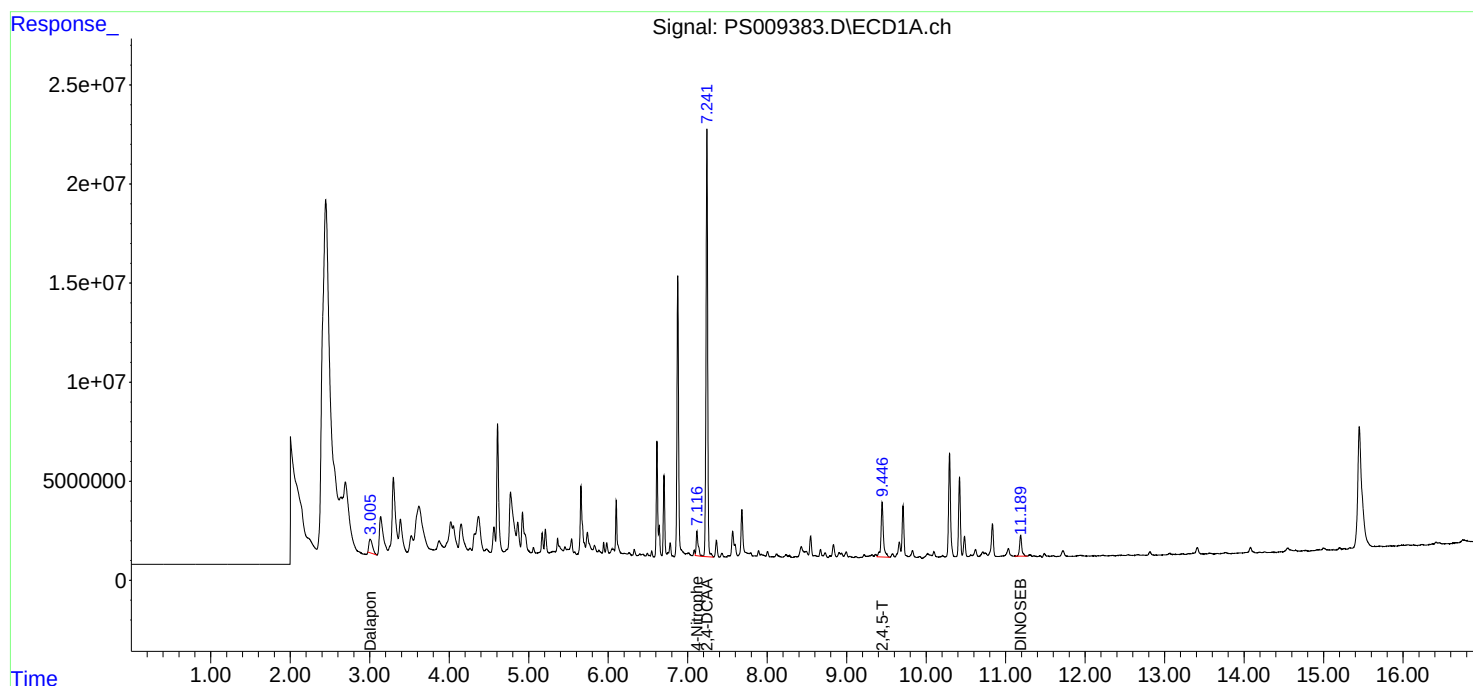


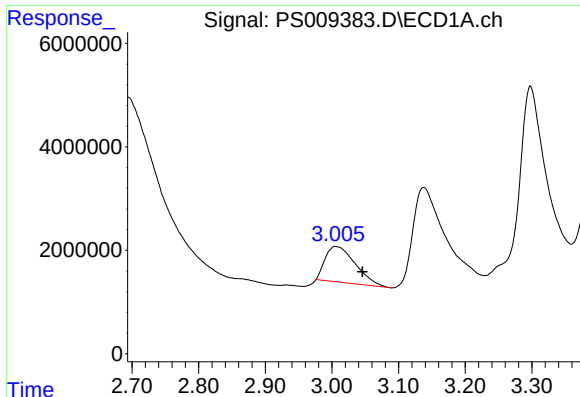

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 21603577
Conc: 27.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

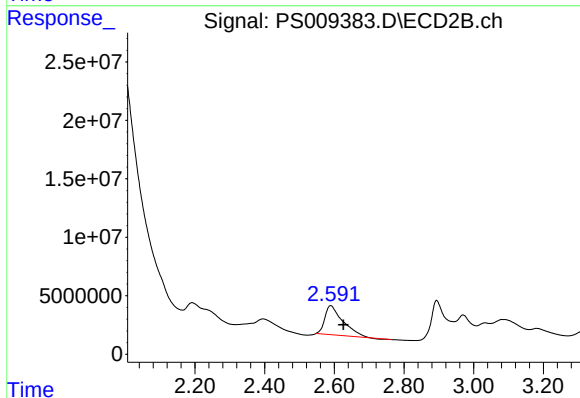


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.037 min
Response: 88415927
Conc: 112.29 ng/ml

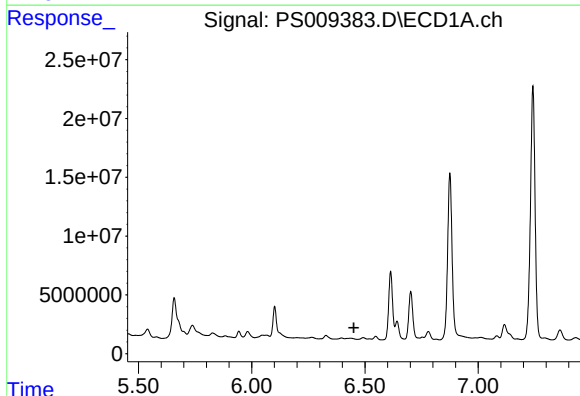


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

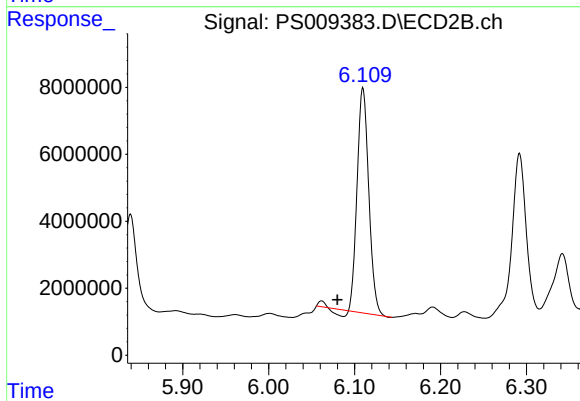

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 62440671
Conc: 76.77 ng/ml

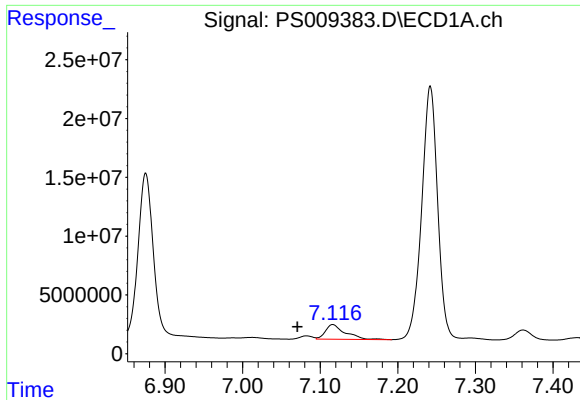

#3 4-Nitrophenol


R.T.: 7.116 min
Delta R.T.: 0.046 min
Response: 21900160
Conc: 91.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

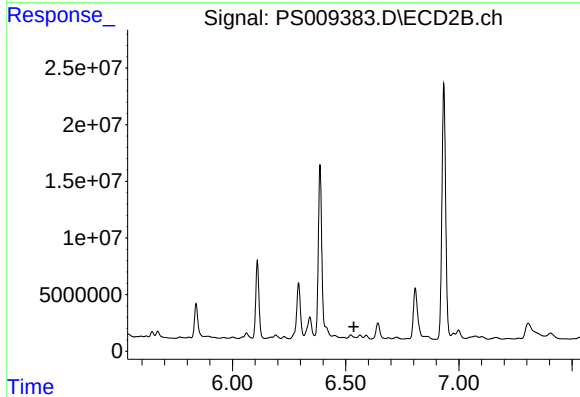


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.536 min
Response: 0
Conc: N.D.

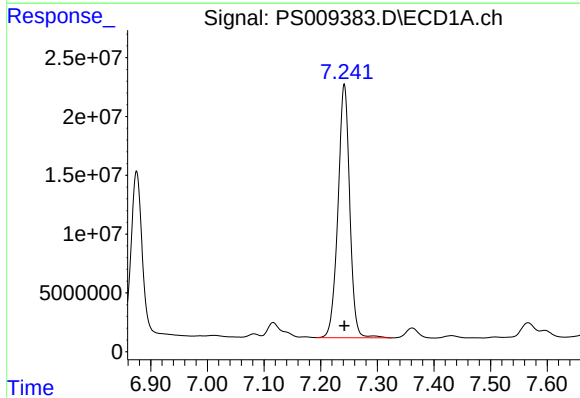


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 311051283
Conc: 562.31 ng/ml

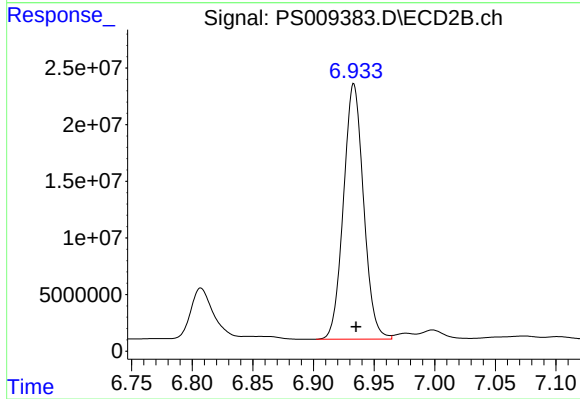

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 260158586
Conc: 473.71 ng/ml

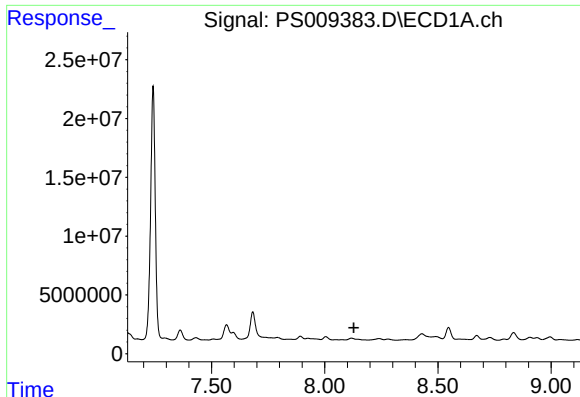

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

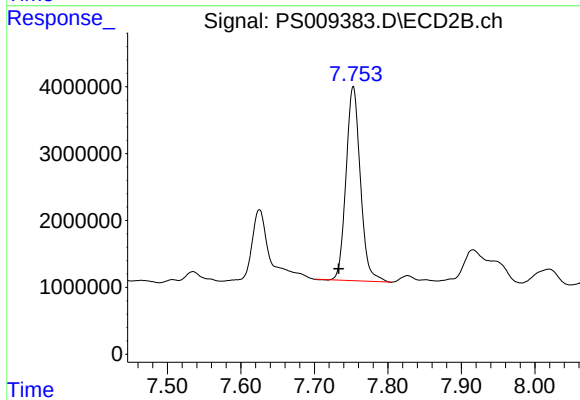


#8 DICHLORPROP

R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 39438240
Conc: 71.08 ng/ml

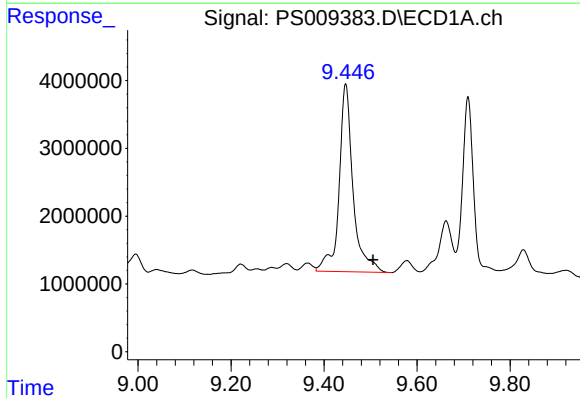


#12 2,4,5-T

R.T.: 9.447 min
Delta R.T.: -0.058 min
Response: 57685341
Conc: 22.68 ng/ml

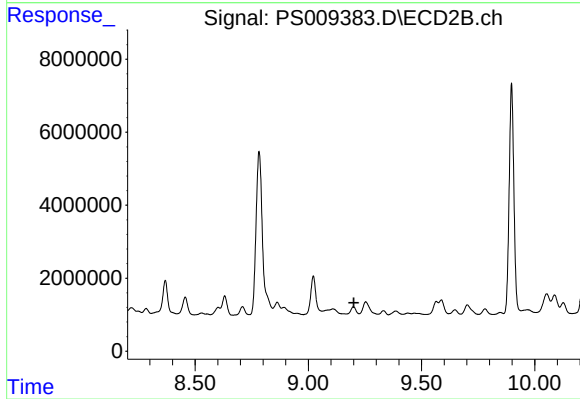

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

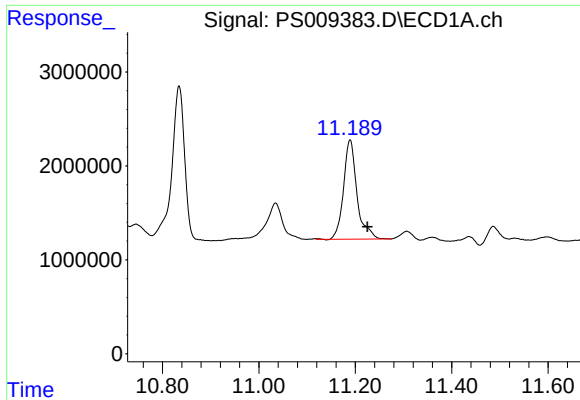

#14 DINOSEB


R.T.: 11.189 min
Delta R.T.: -0.036 min
Response: 20522312
Conc: 10.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

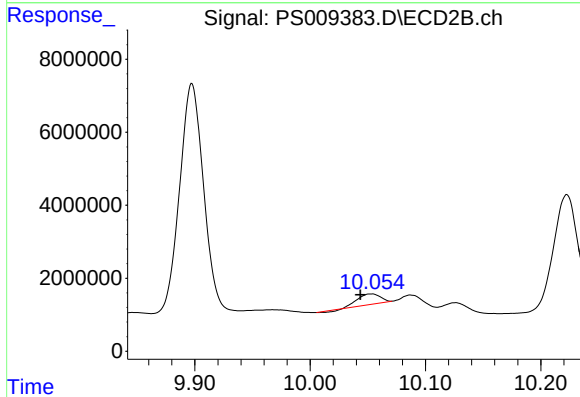


#14 DINOSEB

R.T.: 10.053 min
Delta R.T.: 0.009 min
Response: 3721494
Conc: 1.69 ng/ml

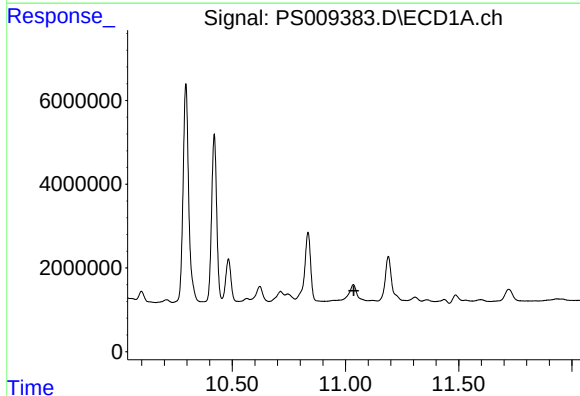


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

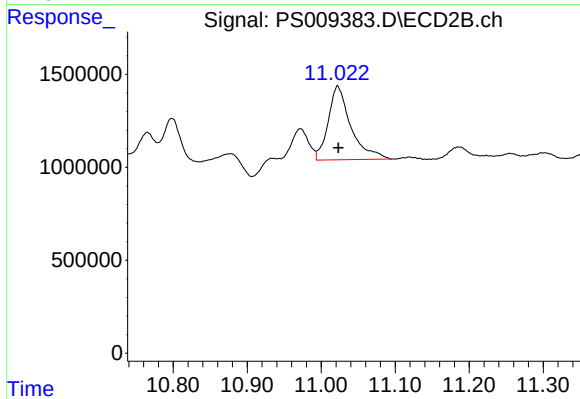

#15 Picloram


R.T.: 11.022 min
Delta R.T.: 0.000 min
Response: 8455094
Conc: 2.08 ng/ml

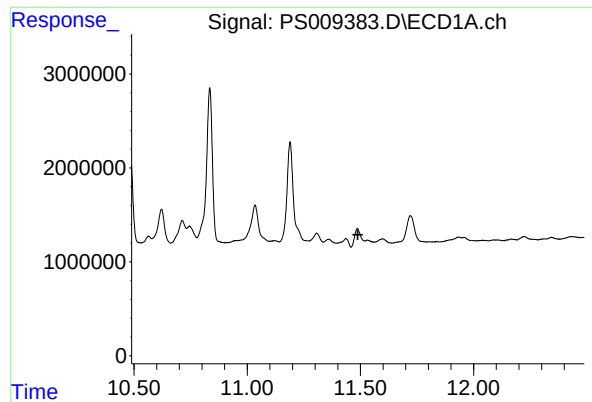

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

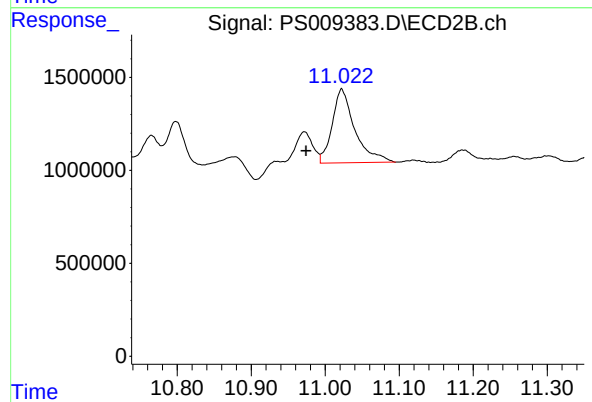

#16 DCPA

R.T.: 11.022 min
Delta R.T.: 0.048 min
Response: 8455094
Conc: 2.18 ng/ml