

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
 Data File : PS003649.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2019 09:02
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 01:31:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.767	0	149835	N.D.	0.319 #
Target Compounds							
3) T	4-Nitroph...	0.000	9.998	0	124455	N.D.	0.554 #
6) T	MCP	0.000	11.276	0	51373	N.D.	0.044 #
7) T	MCPA	0.000	11.659	0	618775	N.D.	0.359 #
8) T	DICHLORPROP	0.000	12.218	0	247847	N.D.	0.600 #
10) T	Pentachlo...	0.000	13.214	0	52459	N.D.	0.008 #
11) T	2,4,5-TP ...	0.000	13.878	0	353777	N.D.	0.139 #
12) T	2,4,5-T	0.000	14.333	0	93502	N.D.	0.046 #
13) T	2,4-DB	0.000	14.971	0	185236	N.D.	0.725 #
14) T	DINOSEB	0.000	15.428	0	491604	N.D.	0.275 #
15) T	Picloram	0.000	16.665	0	434831	N.D.	0.171 #
16) T	DCPA	0.000	16.626	0	1299027	N.D.	0.418 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
Data File : PS003649.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2019 09:02
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 01:31:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

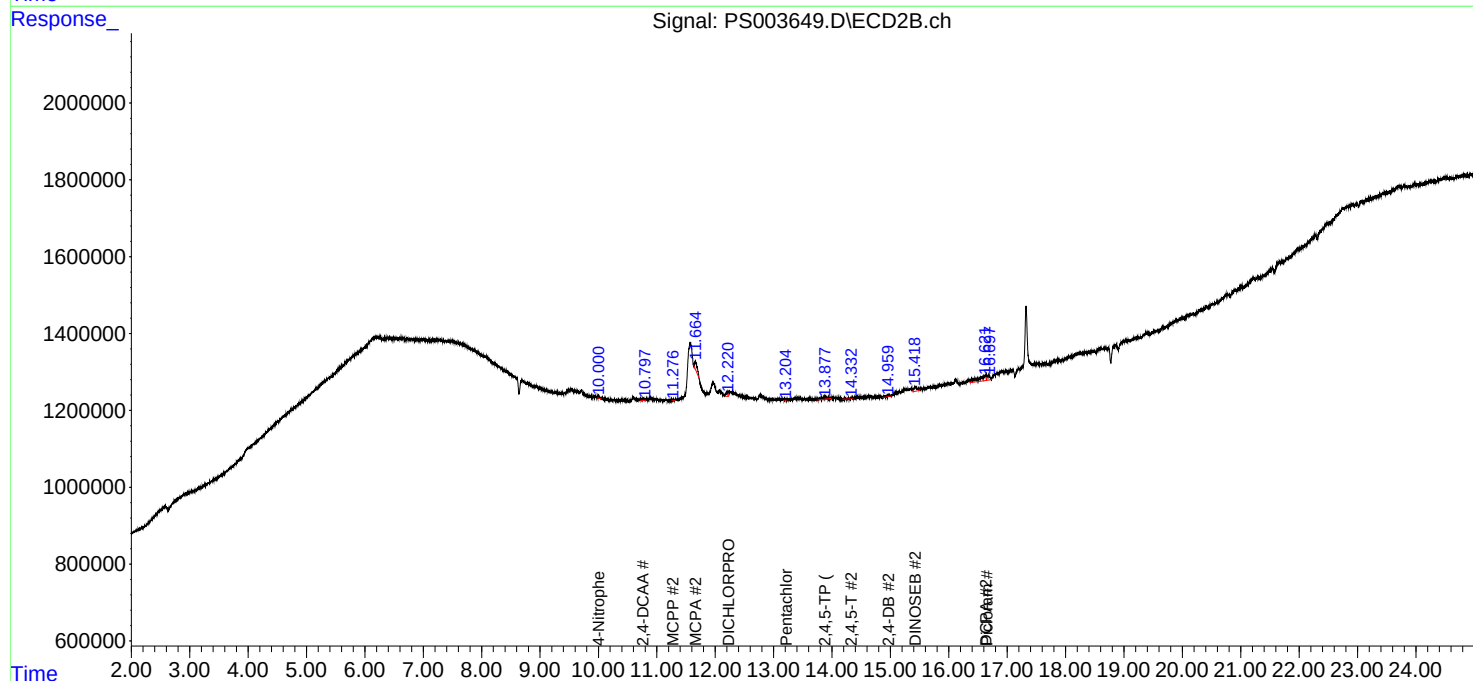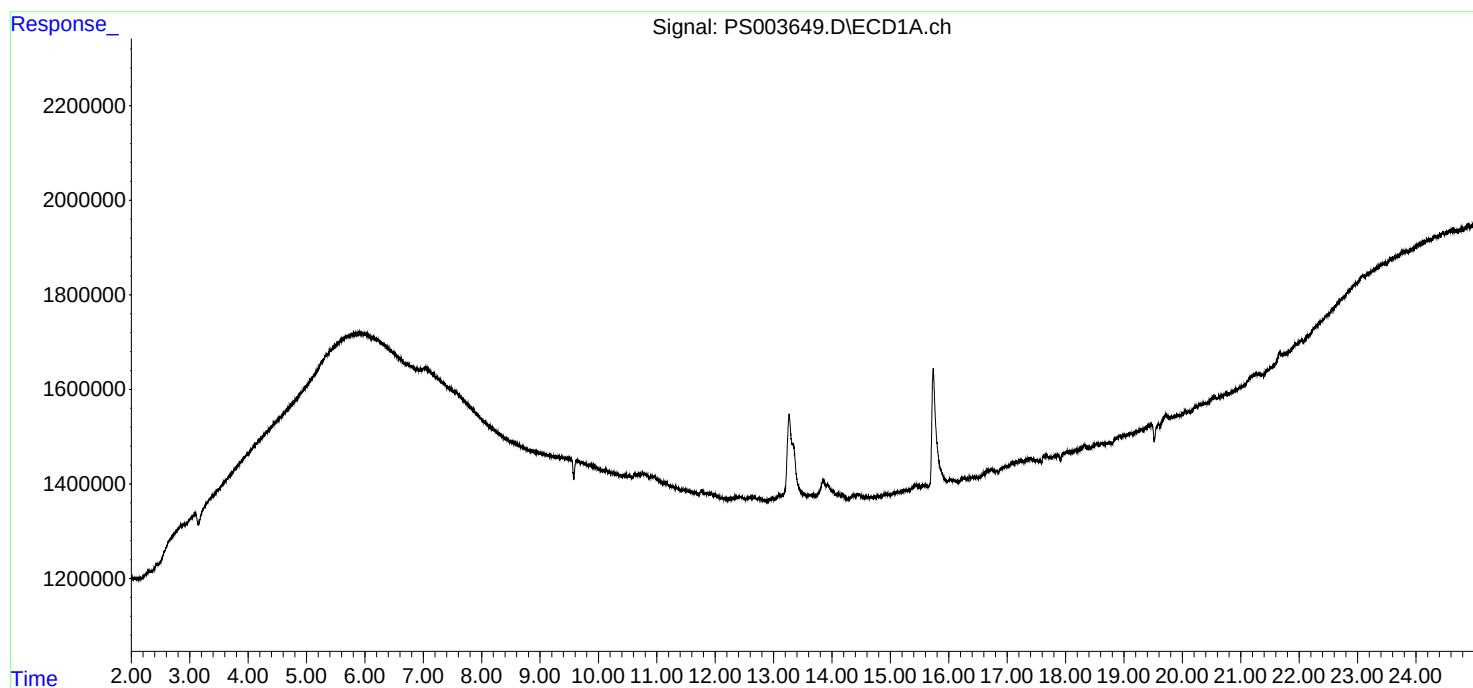


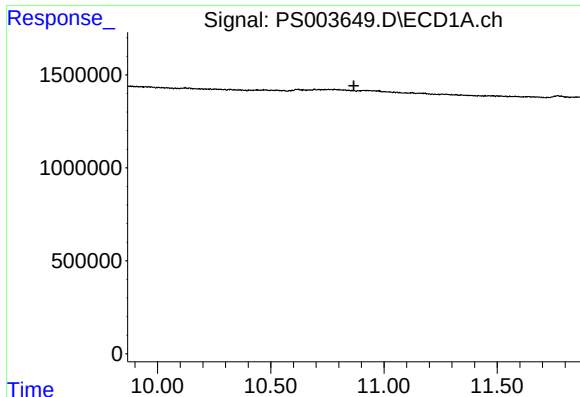

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

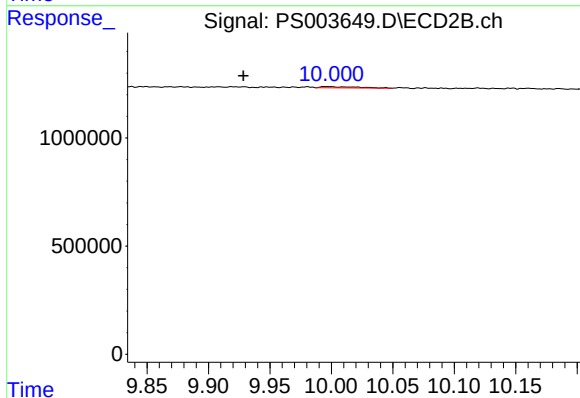


#3 4-Nitrophenol

R.T.: 9.998 min
Delta R.T.: 0.069 min
Response: 124455
Conc: 0.55 ng/ml

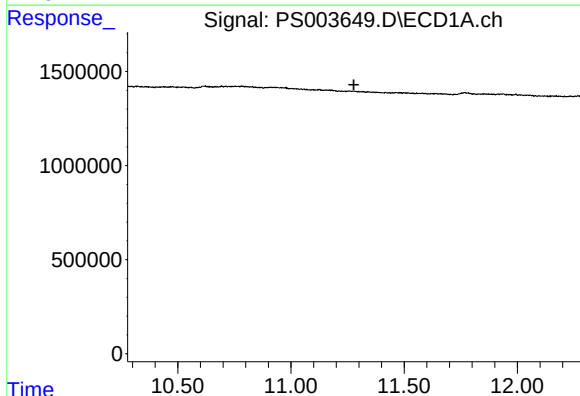


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.278 min
Response: 0
Conc: N.D.

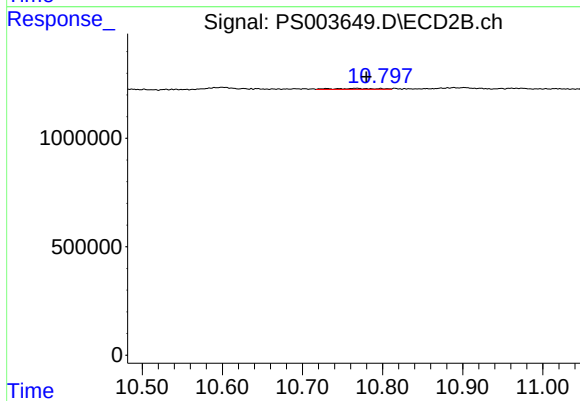

#4 2,4-DCAA


R.T.: 10.767 min
Delta R.T.: -0.013 min
Response: 149835
Conc: 0.32 ng/ml

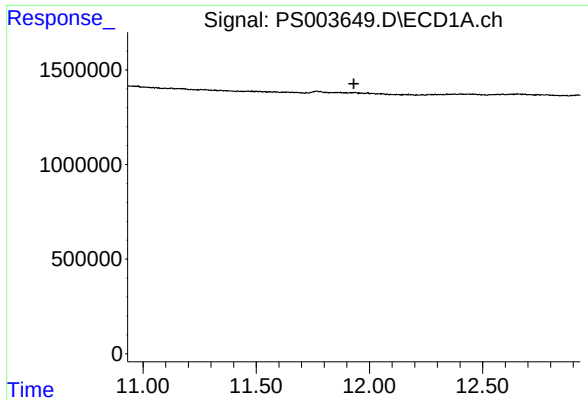

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

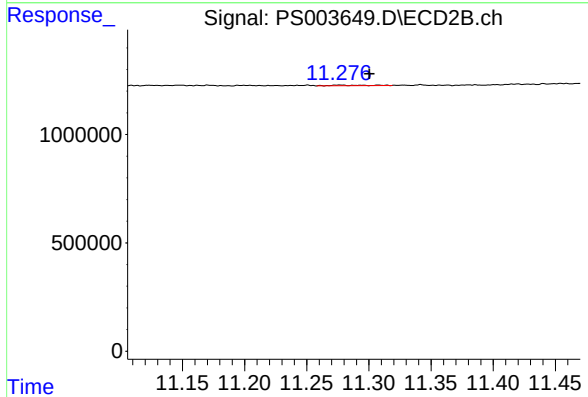


#6 MCPP

R.T.: 11.276 min
Delta R.T.: -0.024 min
Response: 51373
Conc: 0.04 ug/ml

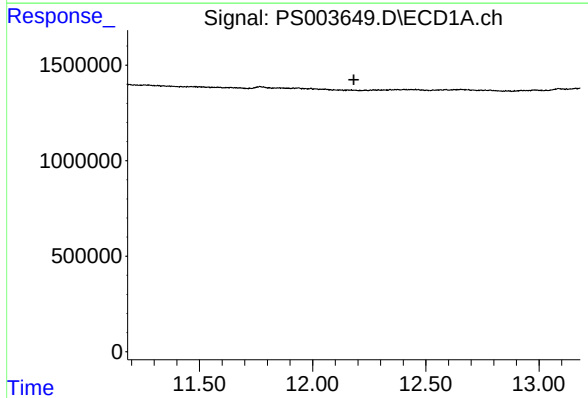


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

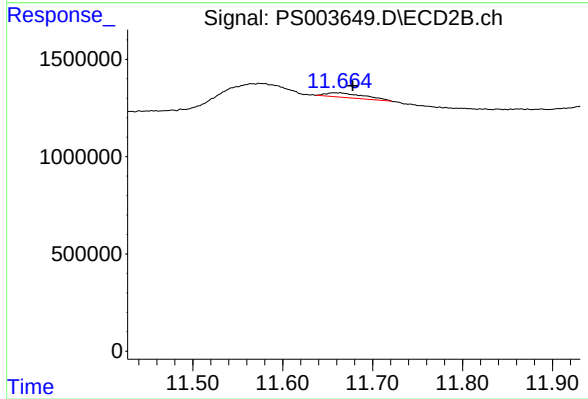

#7 MCPA


R.T.: 11.659 min
Delta R.T.: -0.018 min
Response: 618775
Conc: 0.36 ug/ml

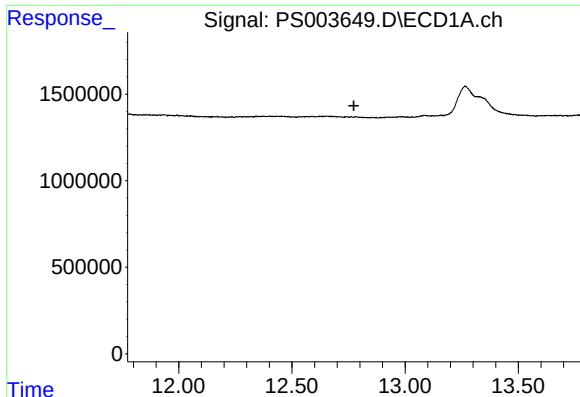

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

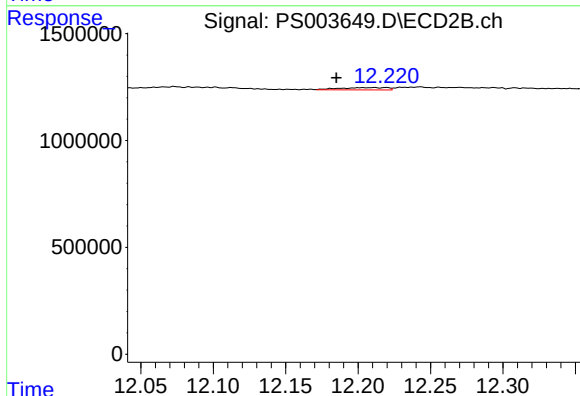


#8 DICHLORPROP

R.T.: 12.218 min
Delta R.T.: 0.033 min
Response: 247847
Conc: 0.60 ng/ml

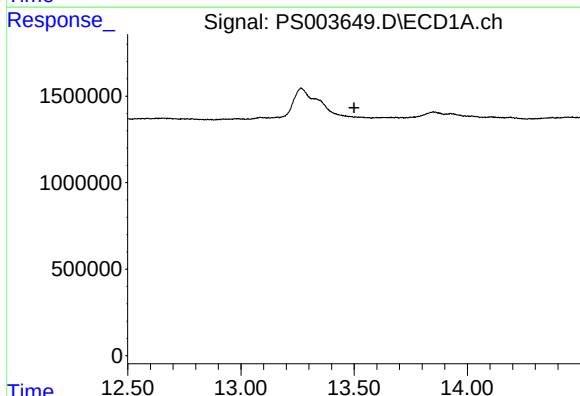


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

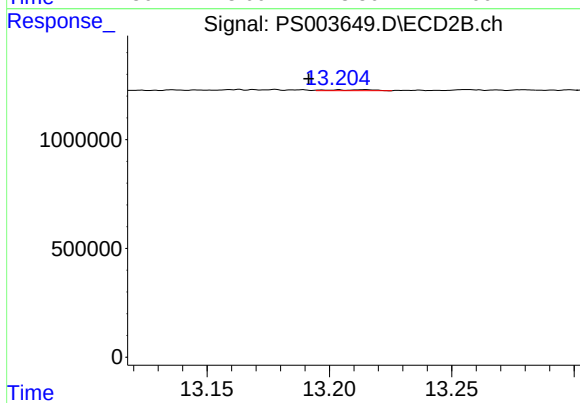

#10 Pentachlorophenol


R.T.: 13.214 min
Delta R.T.: 0.023 min
Response: 52459
Conc: 0.01 ng/ml

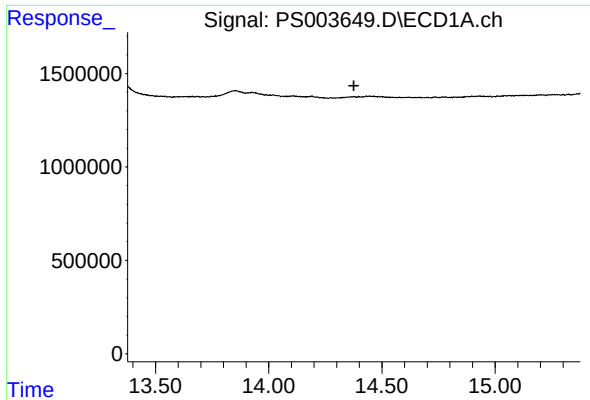

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

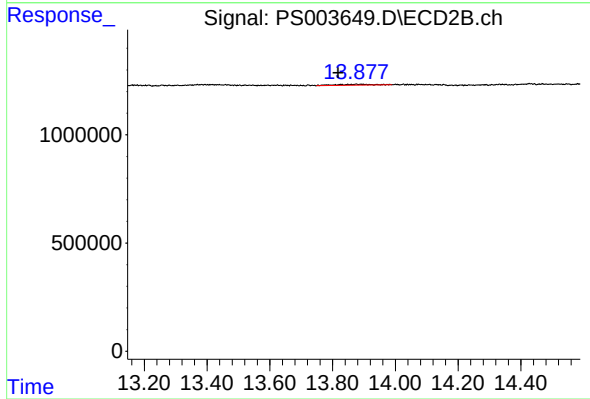


#11 2,4,5-TP (SILVEX)

R.T.: 13.878 min
Delta R.T.: 0.060 min
Response: 353777
Conc: 0.14 ng/ml

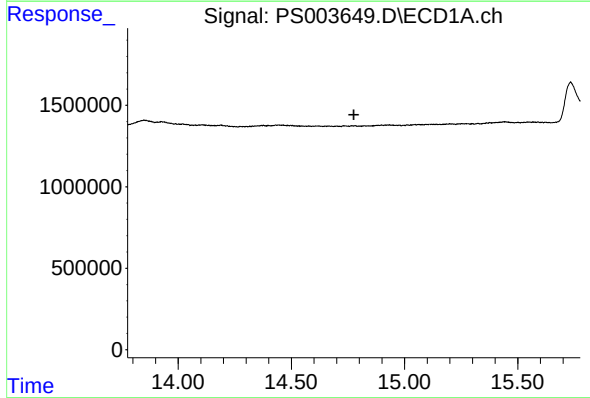


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

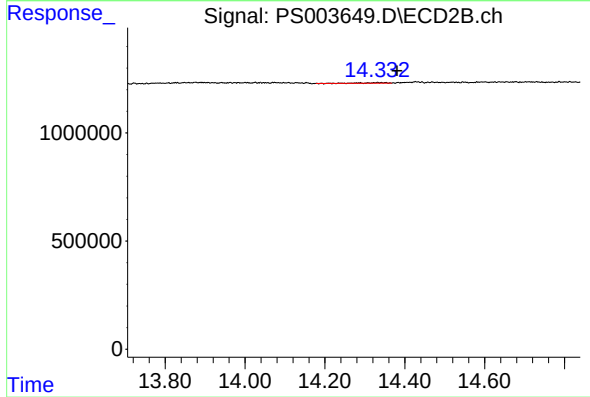

#12 2,4,5-T


R.T.: 14.333 min
Delta R.T.: -0.048 min
Response: 93502
Conc: 0.05 ng/ml

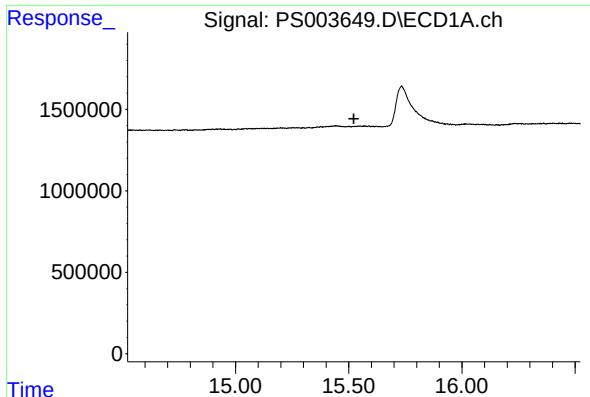

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

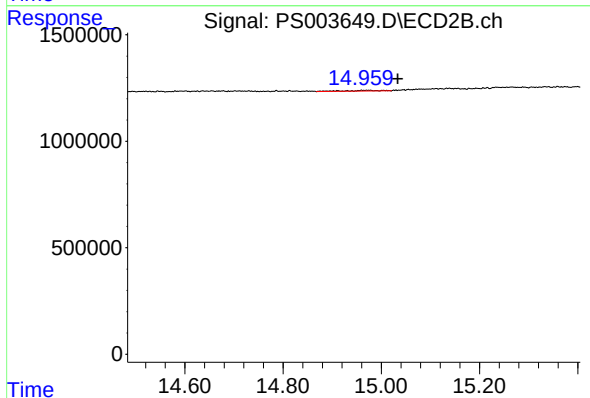


#13 2,4-DB

R.T.: 14.971 min
Delta R.T.: -0.063 min
Response: 185236
Conc: 0.73 ng/ml

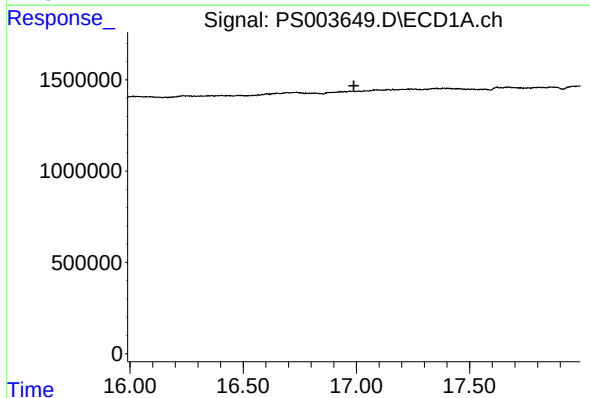


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

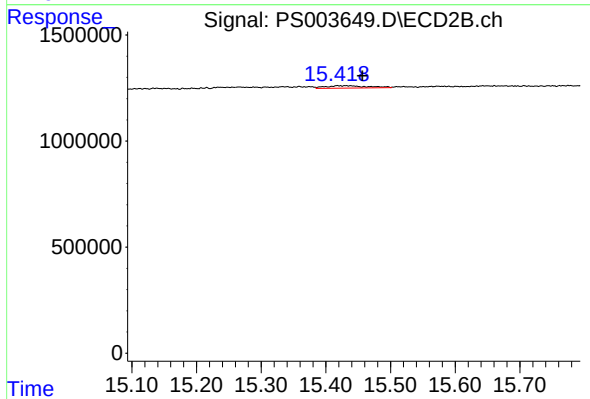

#14 DINOSEB


R.T.: 15.428 min
Delta R.T.: -0.028 min
Response: 491604
Conc: 0.28 ng/ml

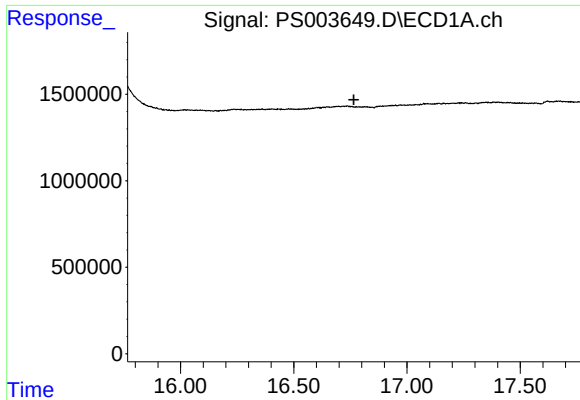

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

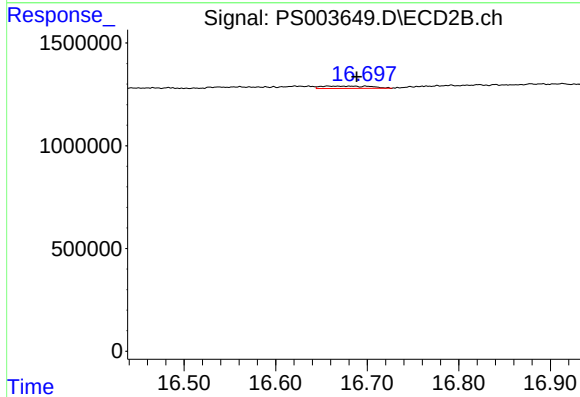


#15 Picloram

R.T.: 16.665 min
Delta R.T.: -0.024 min
Response: 434831
Conc: 0.17 ng/ml

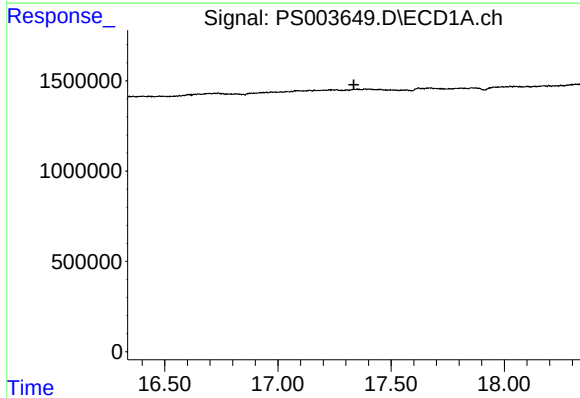

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

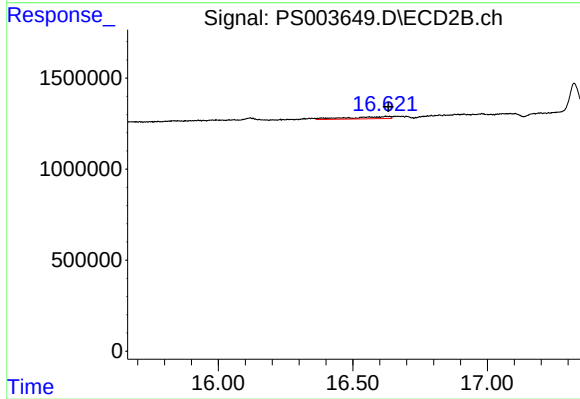

#16 DCPA

R.T.: 16.626 min
Delta R.T.: -0.006 min
Response: 1299027
Conc: 0.42 ng/ml