

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
 Data File : PS003662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2019 17:48
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 01:35:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.268	10.770	230.4E6	217.5E6	524.818	463.172
Target Compounds							
2) T	3,5-DICHL...	0.000	8.995	0	140075	N.D.	0.227 #
3) T	4-Nitroph...	0.000	9.938	0	81669	N.D.	0.363 #
7) T	MCPA	0.000	11.662	0	128211	N.D.	0.074 #
8) T	DICHLORPROP	0.000	12.116	0	3091432	N.D.	7.481 #
10) T	Pentachlo...	0.000	13.180	0	593265	N.D.	0.090 #
11) T	2,4,5-TP ...	0.000	13.827	0	177164	N.D.	0.070 #
13) T	2,4-DB	0.000	15.009	0	5592051	N.D.	21.899 #
14) T	DINOSEB	0.000	15.502	0	2252992	N.D.	1.262 #
15) T	Picloram	0.000	16.693	0	1272839	N.D.	0.501 #
16) T	DCPA	17.325	16.619	38077363	2054835	11.555	0.661 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
Data File : PS003662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2019 17:48
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 01:35:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

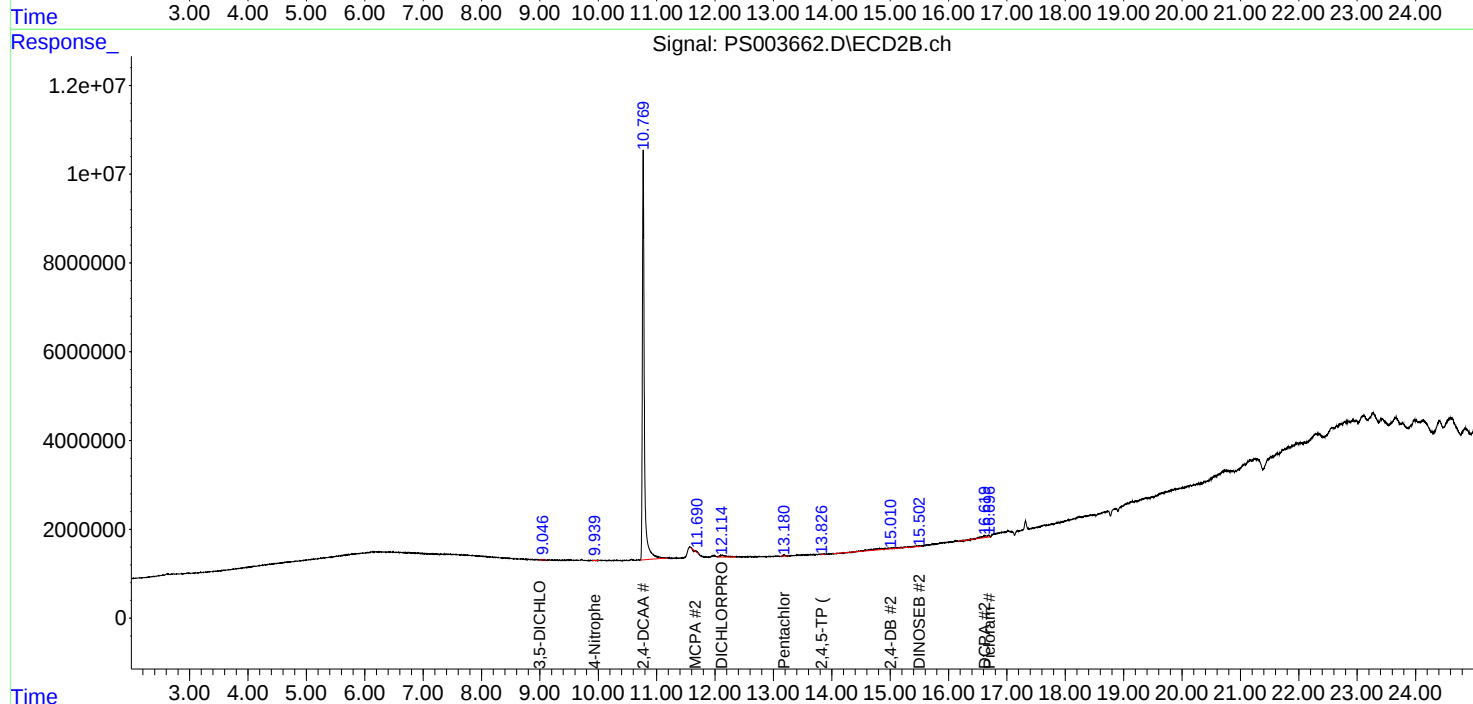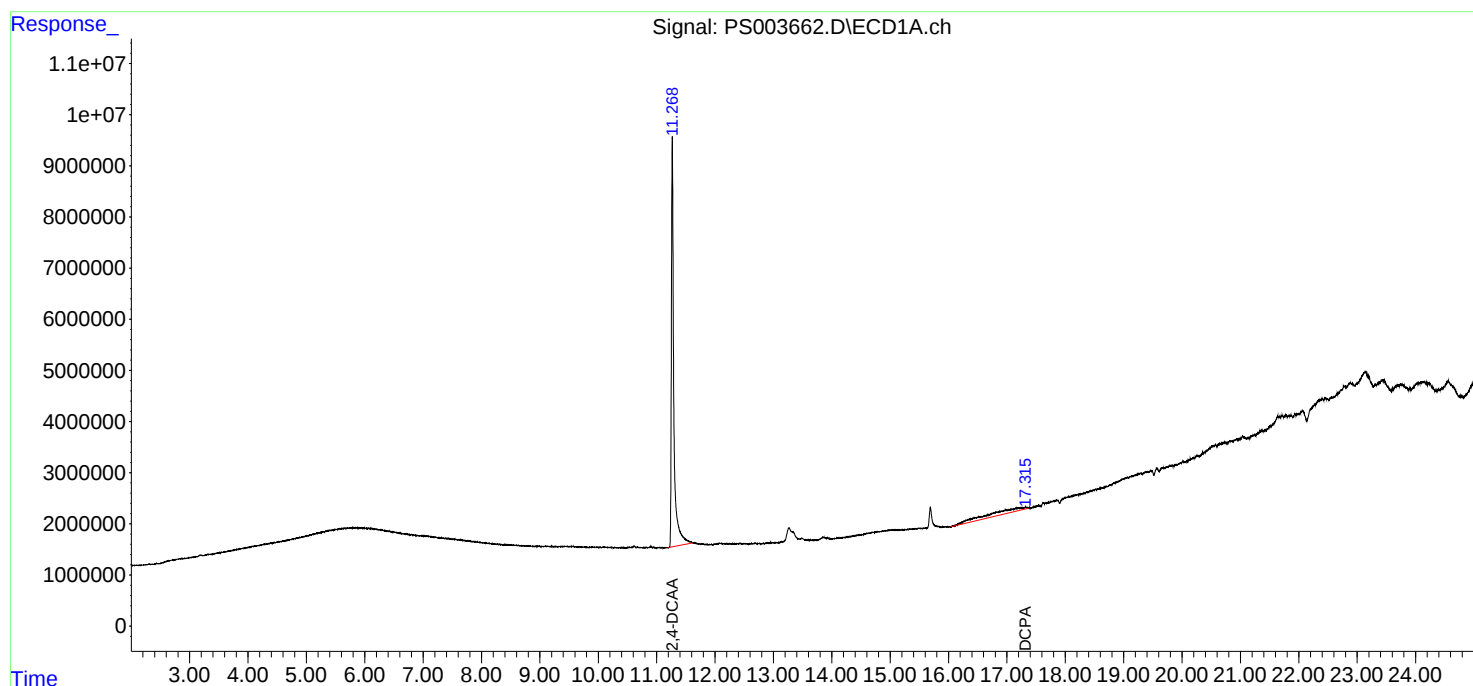


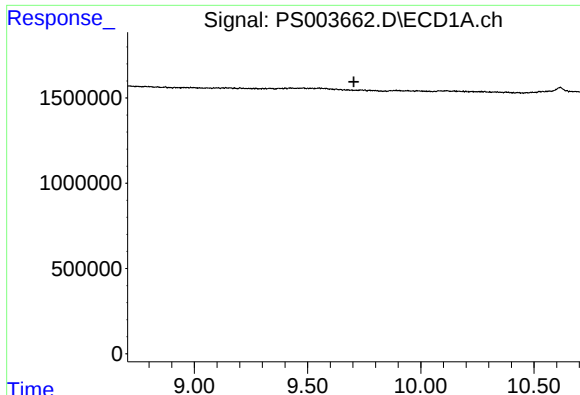

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

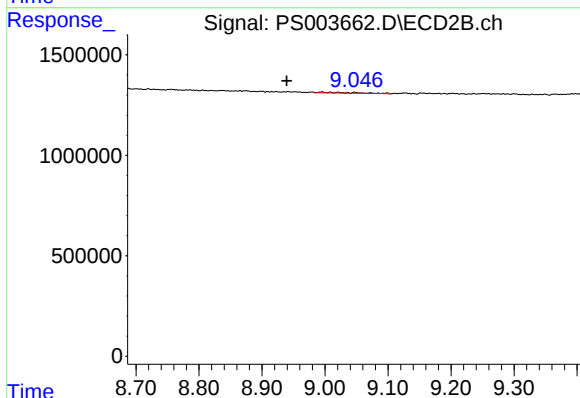


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.995 min
Delta R.T.: 0.056 min
Response: 140075
Conc: 0.23 ng/ml

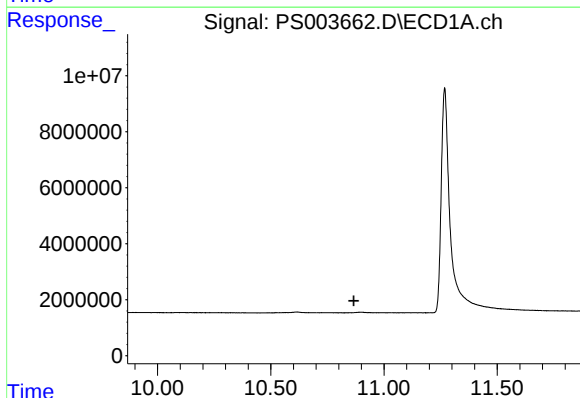


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

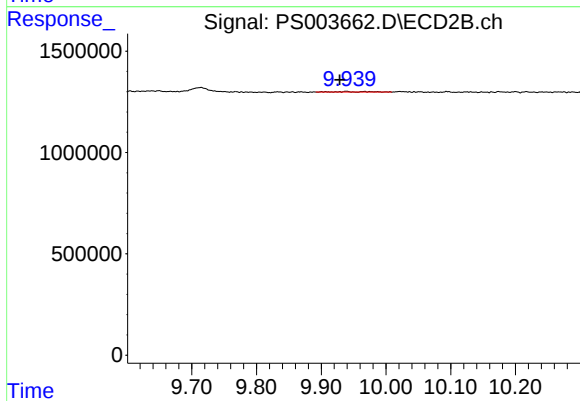

#3 4-Nitrophenol


R.T.: 9.938 min
Delta R.T.: 0.010 min
Response: 81669
Conc: 0.36 ng/ml

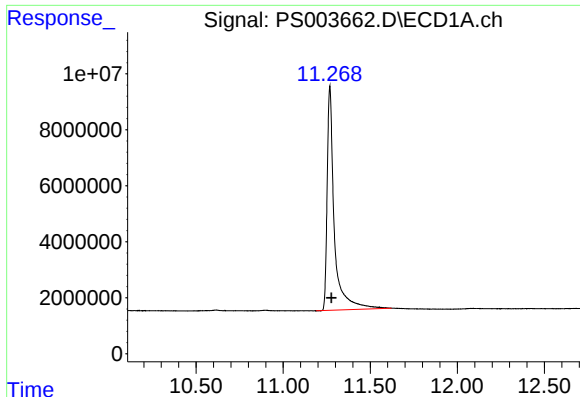

#4 2,4-DCAA


R.T.: 11.268 min
Delta R.T.: -0.010 min
Response: 230408084
Conc: 524.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

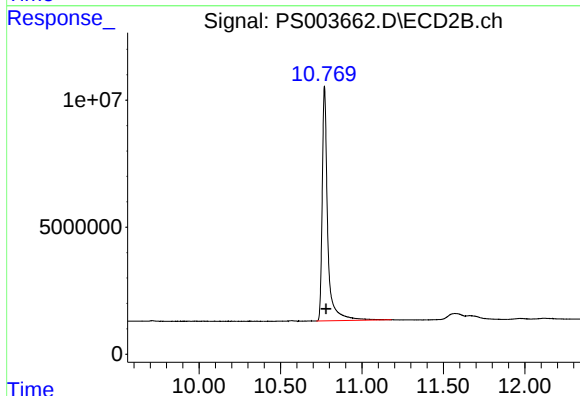


#4 2,4-DCAA

R.T.: 10.770 min
Delta R.T.: -0.010 min
Response: 217491301
Conc: 463.17 ng/ml

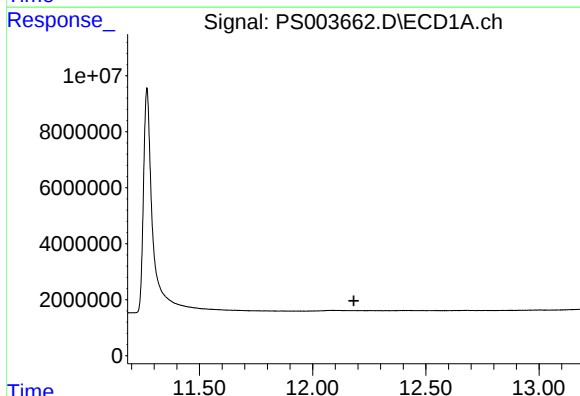


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

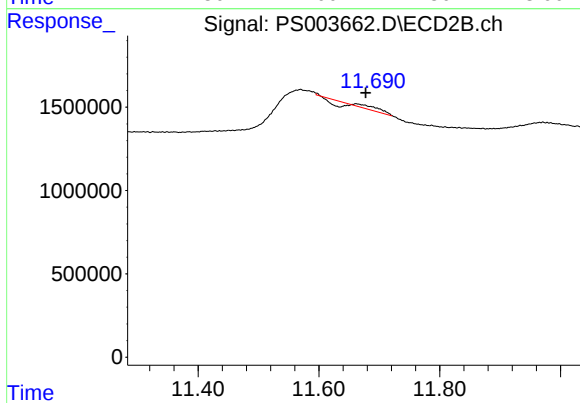

#7 MCPA


R.T.: 11.662 min
Delta R.T.: -0.015 min
Response: 128211
Conc: 0.07 ug/ml

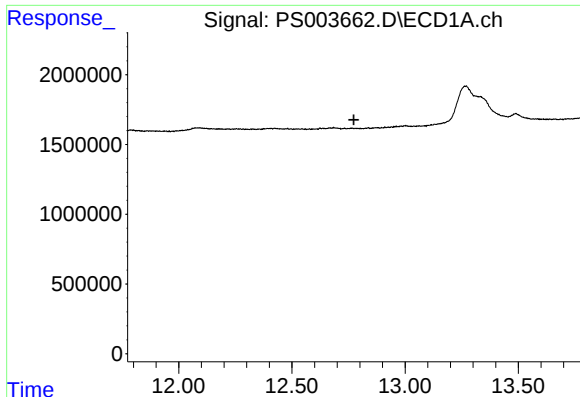

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

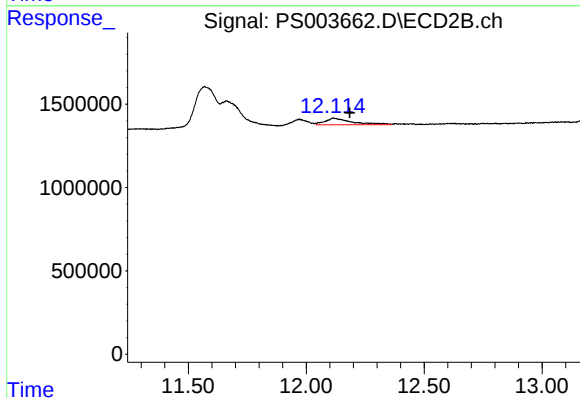


#8 DICHLORPROP

R.T.: 12.116 min
Delta R.T.: -0.069 min
Response: 3091432
Conc: 7.48 ng/ml

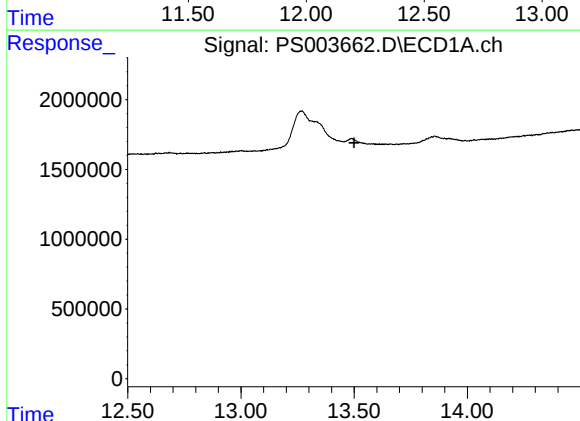


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

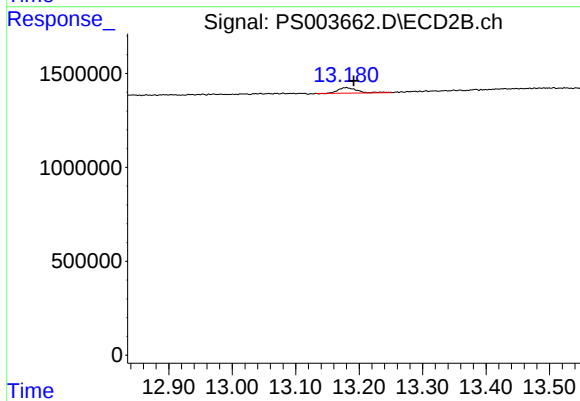

#10 Pentachlorophenol


R.T.: 13.180 min
Delta R.T.: -0.011 min
Response: 593265
Conc: 0.09 ng/ml

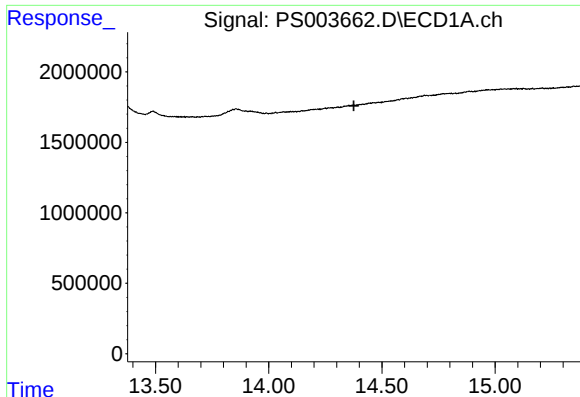

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

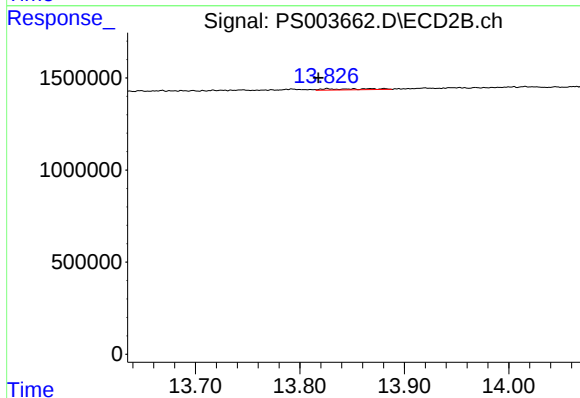


#11 2,4,5-TP (SILVEX)

R.T.: 13.827 min
Delta R.T.: 0.009 min
Response: 177164
Conc: 0.07 ng/ml

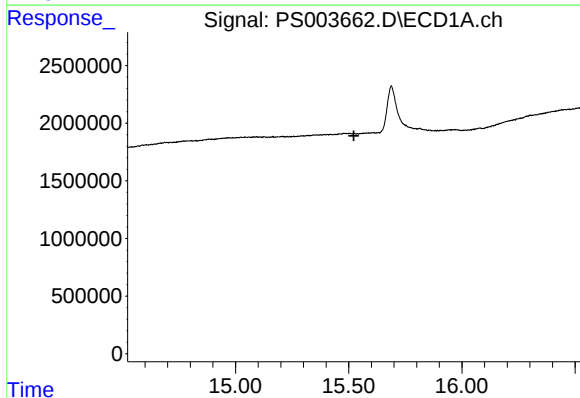


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

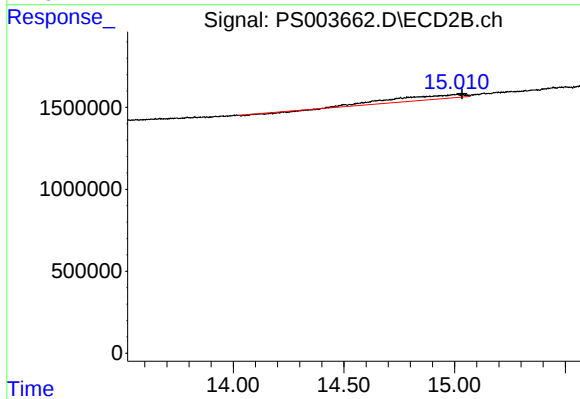

#13 2,4-DB


R.T.: 15.009 min
Delta R.T.: -0.024 min
Response: 5592051
Conc: 21.90 ng/ml

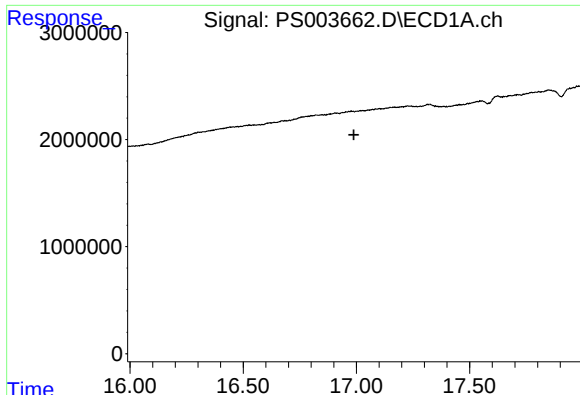

#14 DINoseb


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

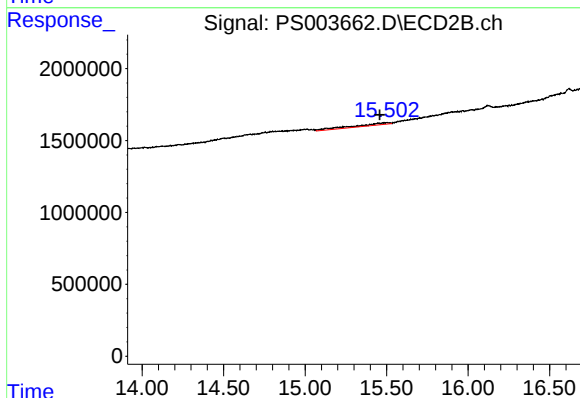


#14 DINoseb

R.T.: 15.502 min
Delta R.T.: 0.046 min
Response: 2252992
Conc: 1.26 ng/ml

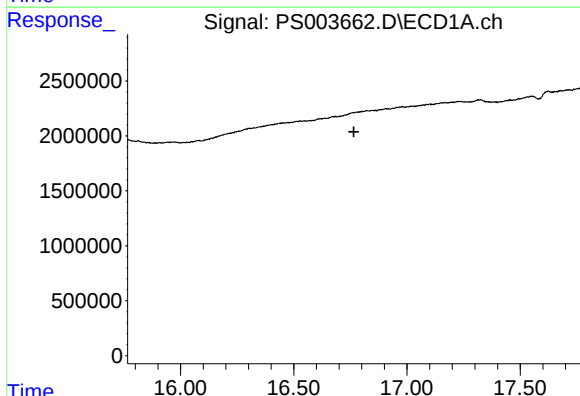


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

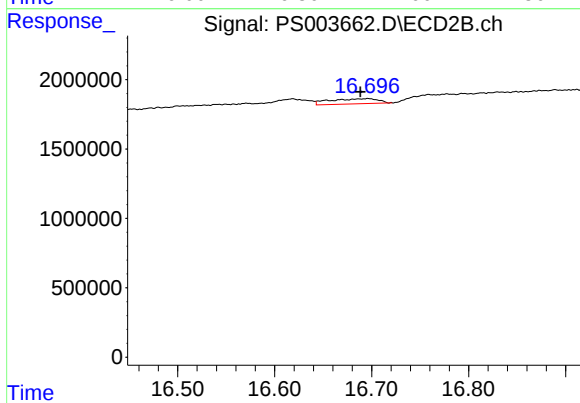

#15 Picloram


R.T.: 16.693 min
Delta R.T.: 0.005 min
Response: 1272839
Conc: 0.50 ng/ml

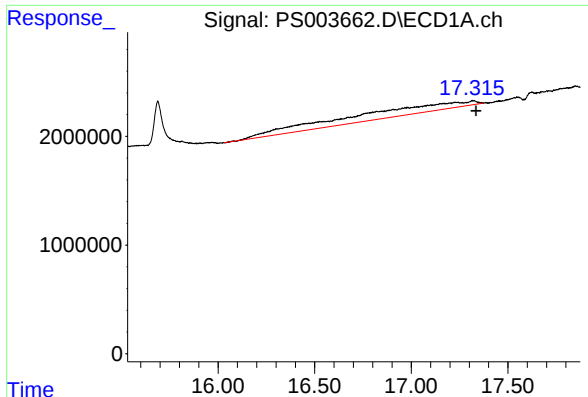

#16 DCPA

R.T.: 17.325 min
Delta R.T.: -0.010 min
Response: 38077363
Conc: 11.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

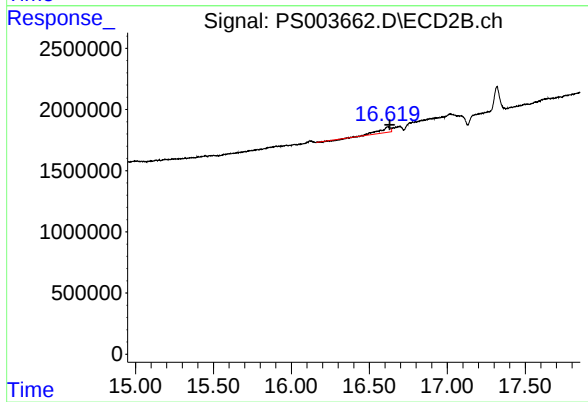

#16 DCPA

R.T.: 16.619 min
Delta R.T.: -0.013 min
Response: 2054835
Conc: 0.66 ng/ml