

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
 Data File : PS003674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 00:03
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 01:39:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.263	10.767	242.4E6	227.4E6	552.204	484.304
Target Compounds							
2) T	3,5-DICHL...	0.000	8.980	0	35730	N.D.	0.058 #
3) T	4-Nitroph...	0.000	9.975	0	170241	N.D.	0.757 #
7) T	MCPA	0.000	11.660	0	1001961	N.D.	0.581 #
9) T	2,4-D	0.000	12.665	0	30361	N.D.	0.058 #
10) T	Pentachlo...	0.000	13.177	0	851867	N.D.	0.129 #
11) T	2,4,5-TP ...	0.000	13.849	0	247499	N.D.	0.097 #
12) T	2,4,5-T	0.000	14.419	0	3912629	N.D.	1.940 #
13) T	2,4-DB	0.000	14.972	0	3428799	N.D.	13.427 #
14) T	DINOSEB	0.000	15.498	0	1003490	N.D.	0.562 #
15) T	Picloram	0.000	16.691	0	2765978	N.D.	1.090 #
16) T	DCPA	17.319	16.619	99340221	2404496	30.147	0.773 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
Data File : PS003674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 00:03
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 01:39:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

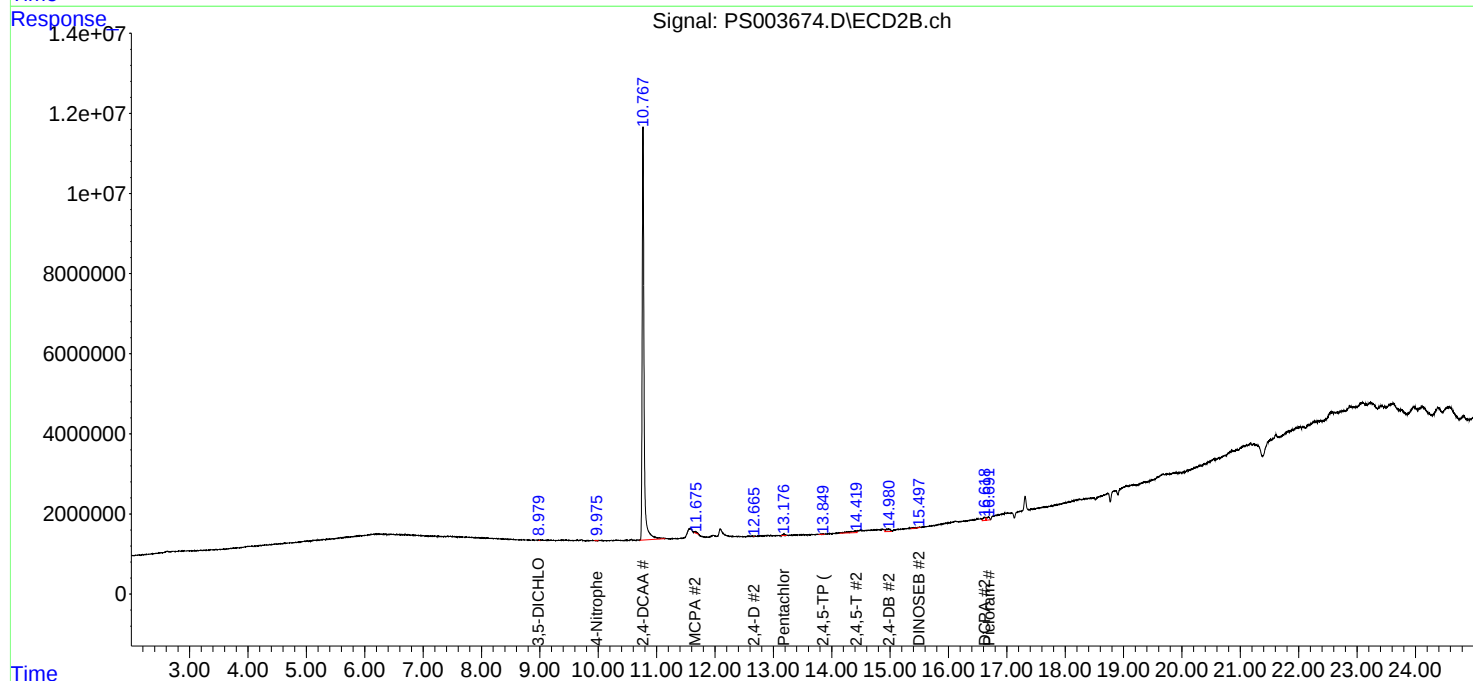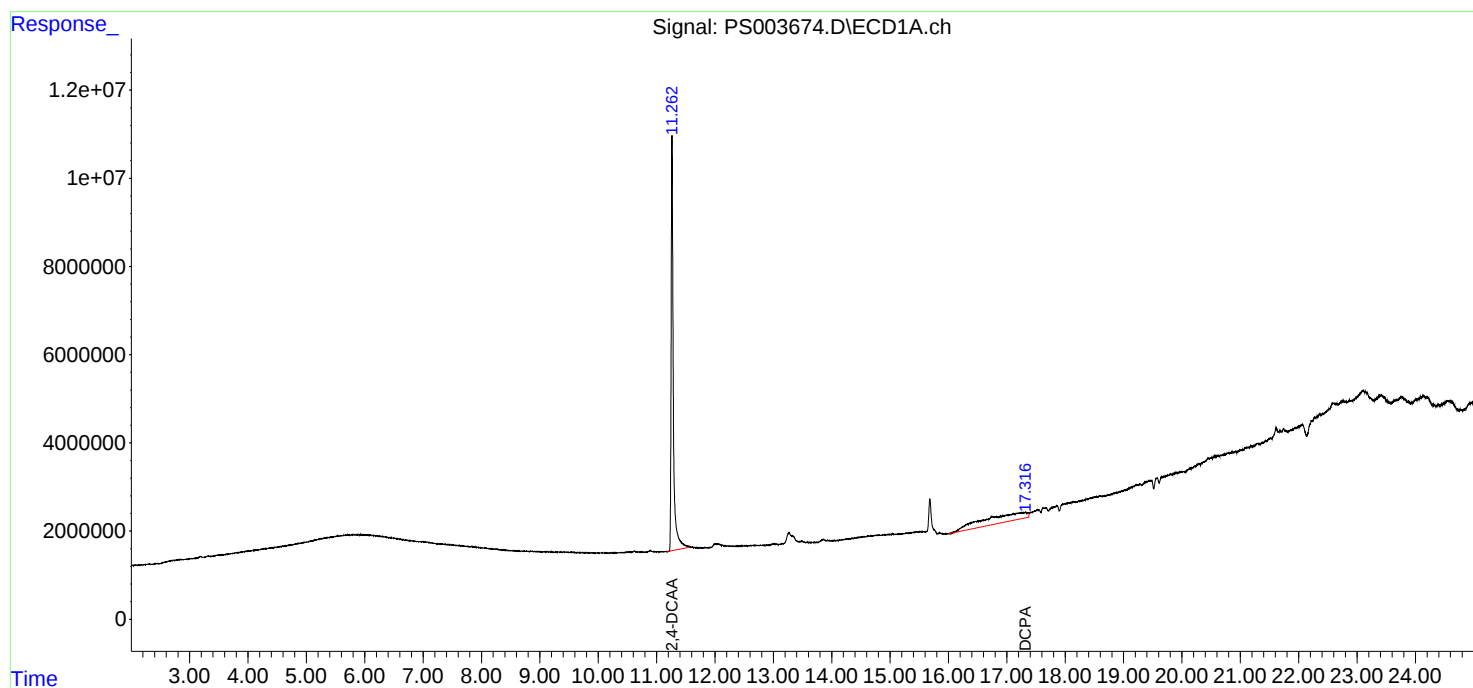


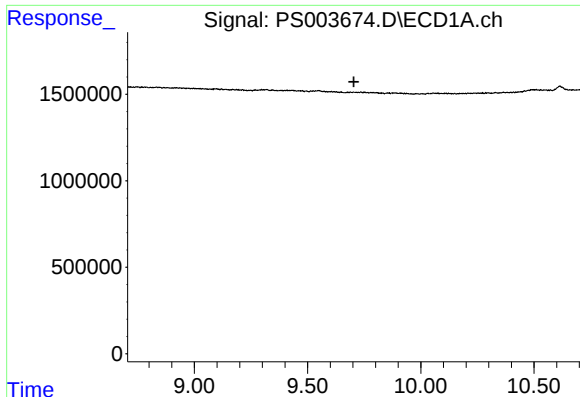

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

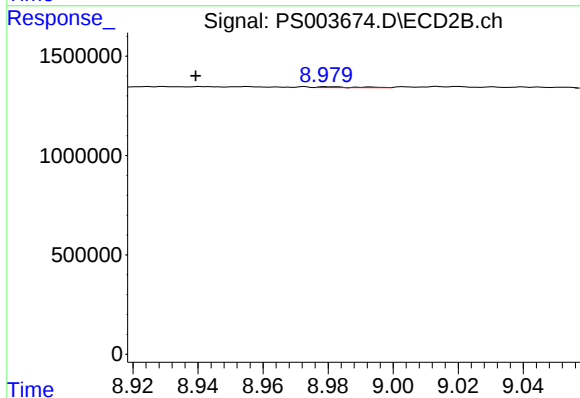


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.980 min
Delta R.T.: 0.041 min
Response: 35730
Conc: 0.06 ng/ml

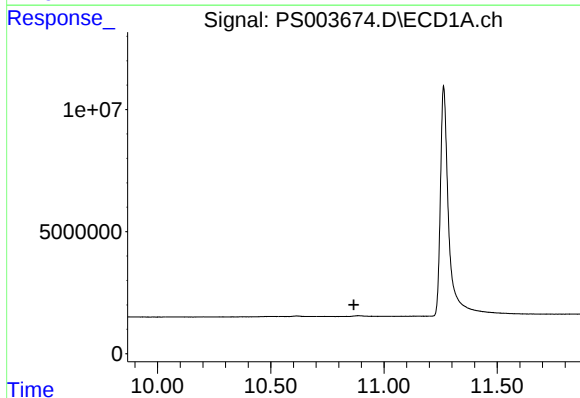


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

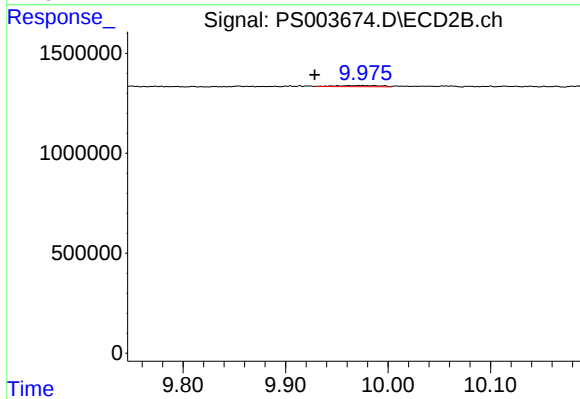

#3 4-Nitrophenol


R.T.: 9.975 min
Delta R.T.: 0.047 min
Response: 170241
Conc: 0.76 ng/ml

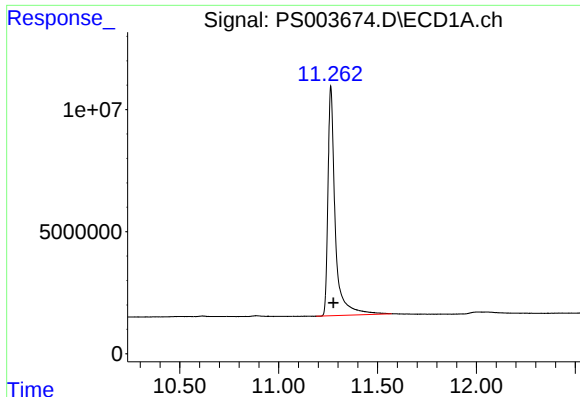

#4 2,4-DCAA


R.T.: 11.263 min
Delta R.T.: -0.014 min
Response: 242430975
Conc: 552.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

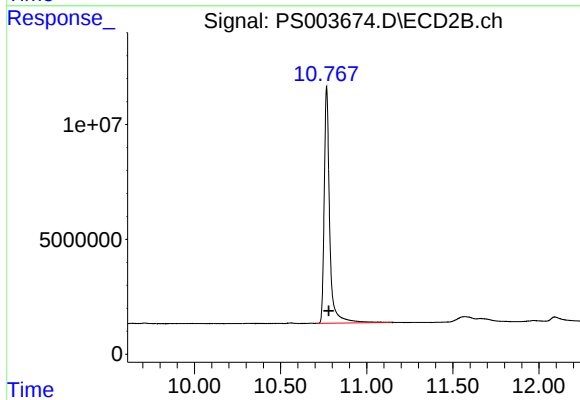


#4 2,4-DCAA

R.T.: 10.767 min
Delta R.T.: -0.013 min
Response: 227414331
Conc: 484.30 ng/ml

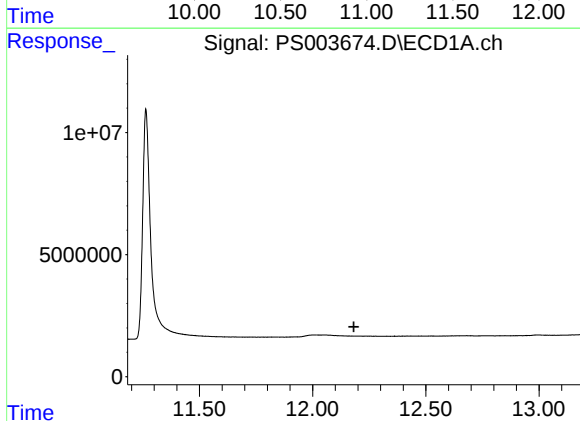


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

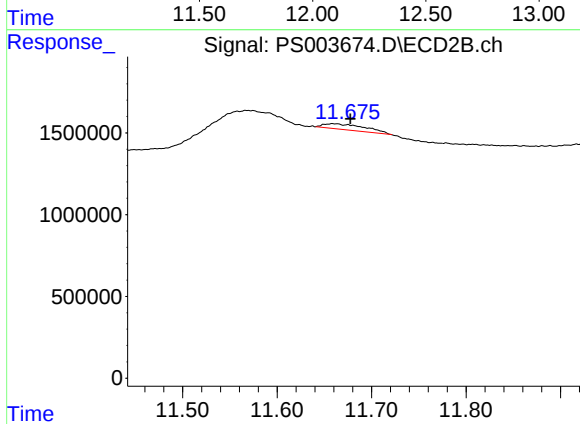

#7 MCPA


R.T.: 11.660 min
Delta R.T.: -0.018 min
Response: 1001961
Conc: 0.58 ug/ml

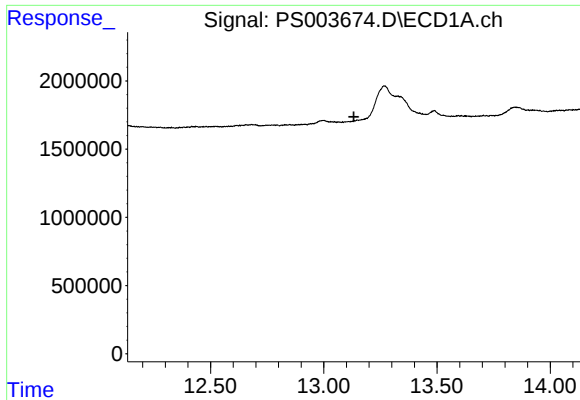

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

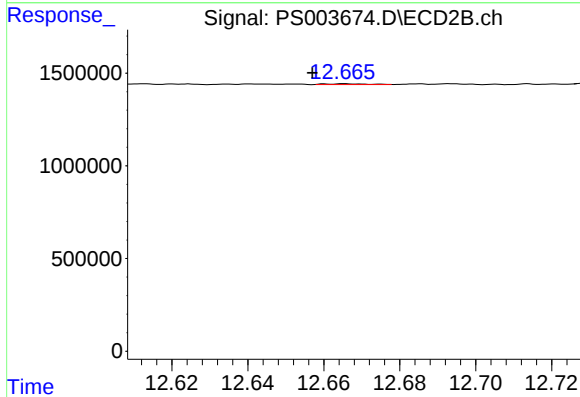


#9 2,4-D

R.T.: 12.665 min
Delta R.T.: 0.008 min
Response: 30361
Conc: 0.06 ng/ml

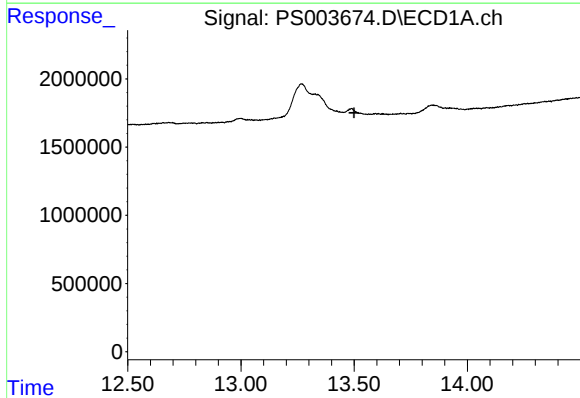


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

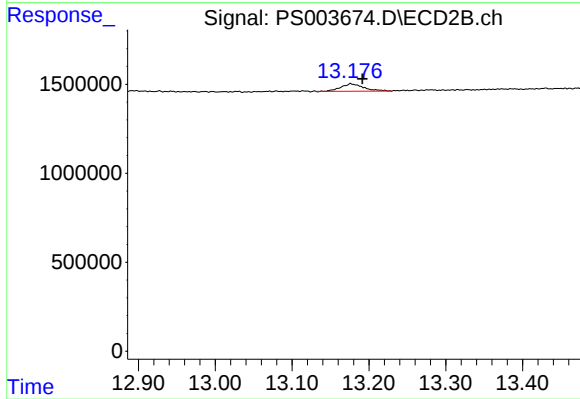

#10 Pentachlorophenol


R.T.: 13.177 min
Delta R.T.: -0.015 min
Response: 851867
Conc: 0.13 ng/ml

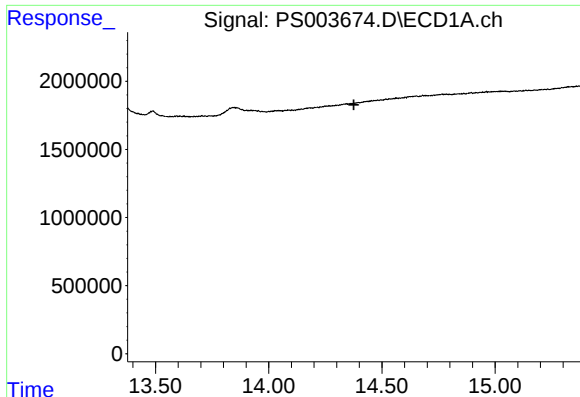

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

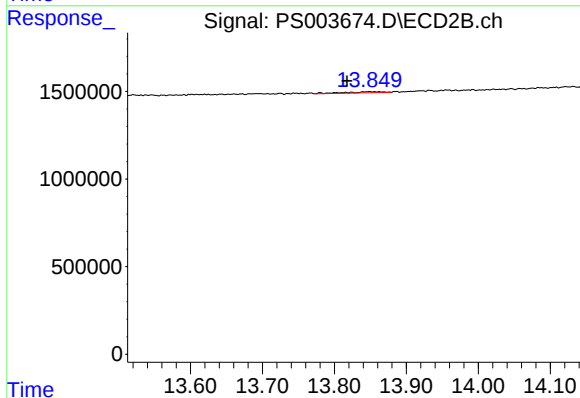


#11 2,4,5-TP (SILVEX)

R.T.: 13.849 min
Delta R.T.: 0.031 min
Response: 247499
Conc: 0.10 ng/ml

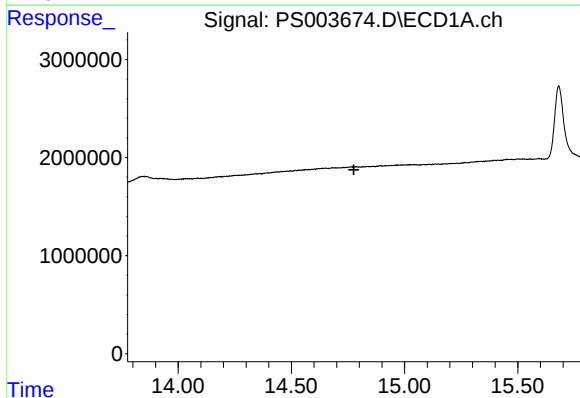


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

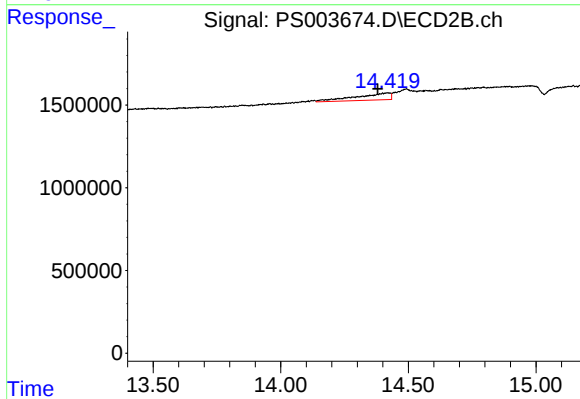

#12 2,4,5-T


R.T.: 14.419 min
Delta R.T.: 0.039 min
Response: 3912629
Conc: 1.94 ng/ml

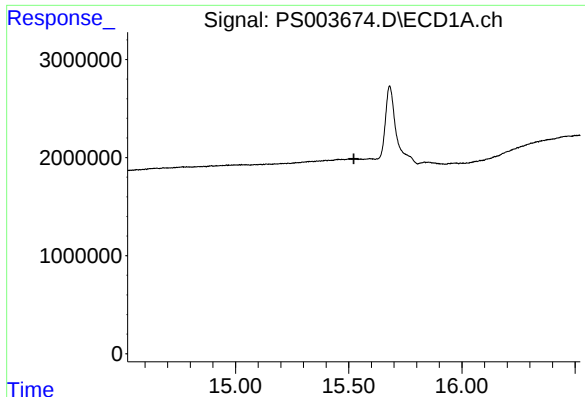

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

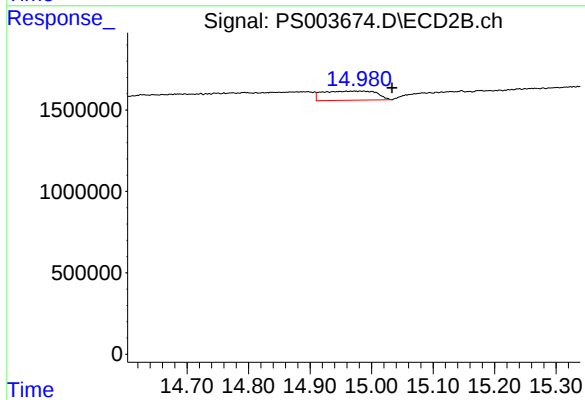


#13 2,4-DB

R.T.: 14.972 min
Delta R.T.: -0.062 min
Response: 3428799
Conc: 13.43 ng/ml

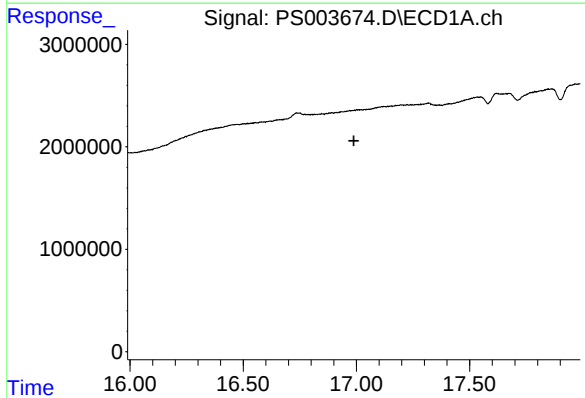


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

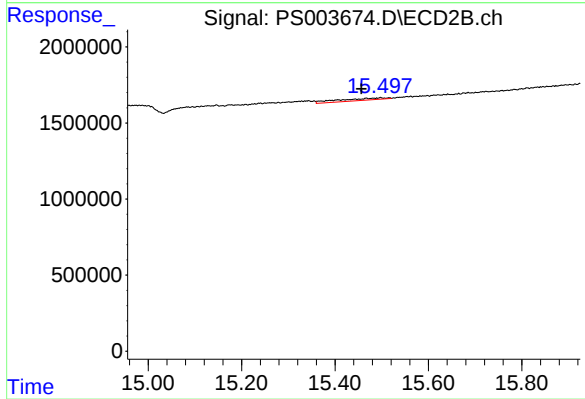

#14 DINOSEB


R.T.: 15.498 min
Delta R.T.: 0.041 min
Response: 1003490
Conc: 0.56 ng/ml

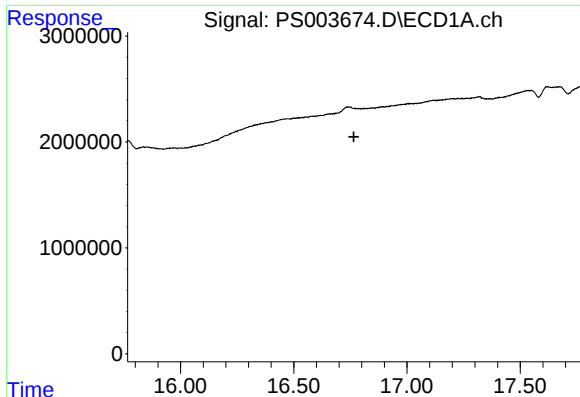

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

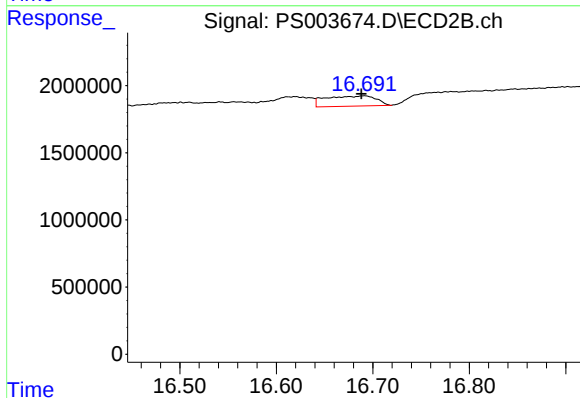


#15 Picloram

R.T.: 16.691 min
Delta R.T.: 0.002 min
Response: 2765978
Conc: 1.09 ng/ml

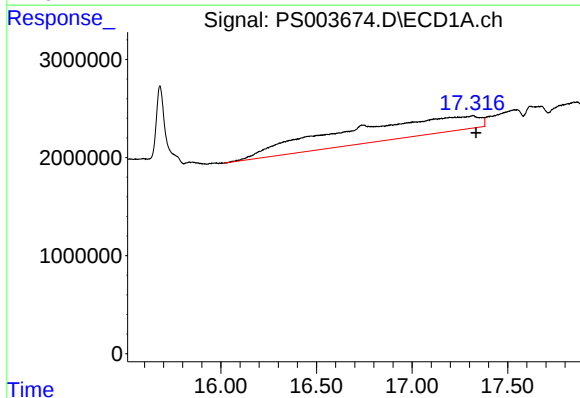

#16 DCPA

R.T.: 17.319 min
Delta R.T.: -0.017 min
Response: 99340221
Conc: 30.15 ng/ml

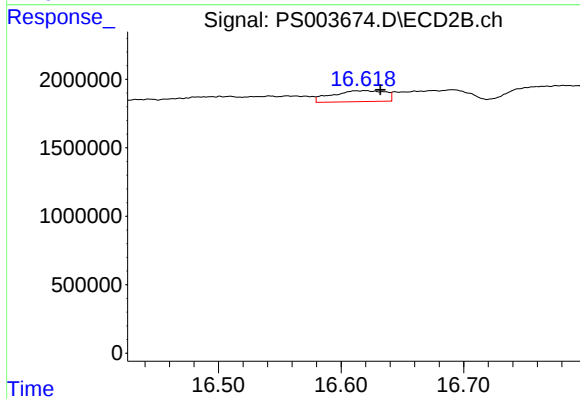

#16 DCPA

R.T.: 16.619 min
Delta R.T.: -0.013 min
Response: 2404496
Conc: 0.77 ng/ml