

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
 Data File : PS003680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 03:10
 Operator : EI\SJ
 Sample : K1943-11RE
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 03:46:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.286	10.772	104.7E6	102.2E6	238.497	217.568
Target Compounds							
1) T	Dalapon	2.803	2.278	31493233	45206483	48.455	71.395 #
2) T	3,5-DICHL...	0.000	8.936	0	4556358	N.D.	7.379 #
5) T	DICAMBA	0.000	11.009	0	11618611	N.D.	6.954 #
6) T	MCP	11.943	0.000	374.0E6	0	284.897	N.D. #
9) T	2,4-D	0.000	12.633	0	582635	N.D.	1.110 #
10) T	Pentachlo...	13.470	13.257	3391436	4046536	0.480	0.614 #
11) T	2,4,5-TP ...	0.000	13.845	0	2567193	N.D.	1.008 #
12) T	2,4,5-T	0.000	14.344	0	6445727	N.D.	3.196 #
13) T	2,4-DB	0.000	14.996	0	5474533	N.D.	21.439 #
14) T	DINOSEB	0.000	15.510	0	6845370	N.D.	3.835 #
15) T	Picloram	16.740	16.722	37619871	15903310	15.285	6.266 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
Data File : PS003680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 03:10
Operator : EI\SJ
Sample : K1943-11RE
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 03:46:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

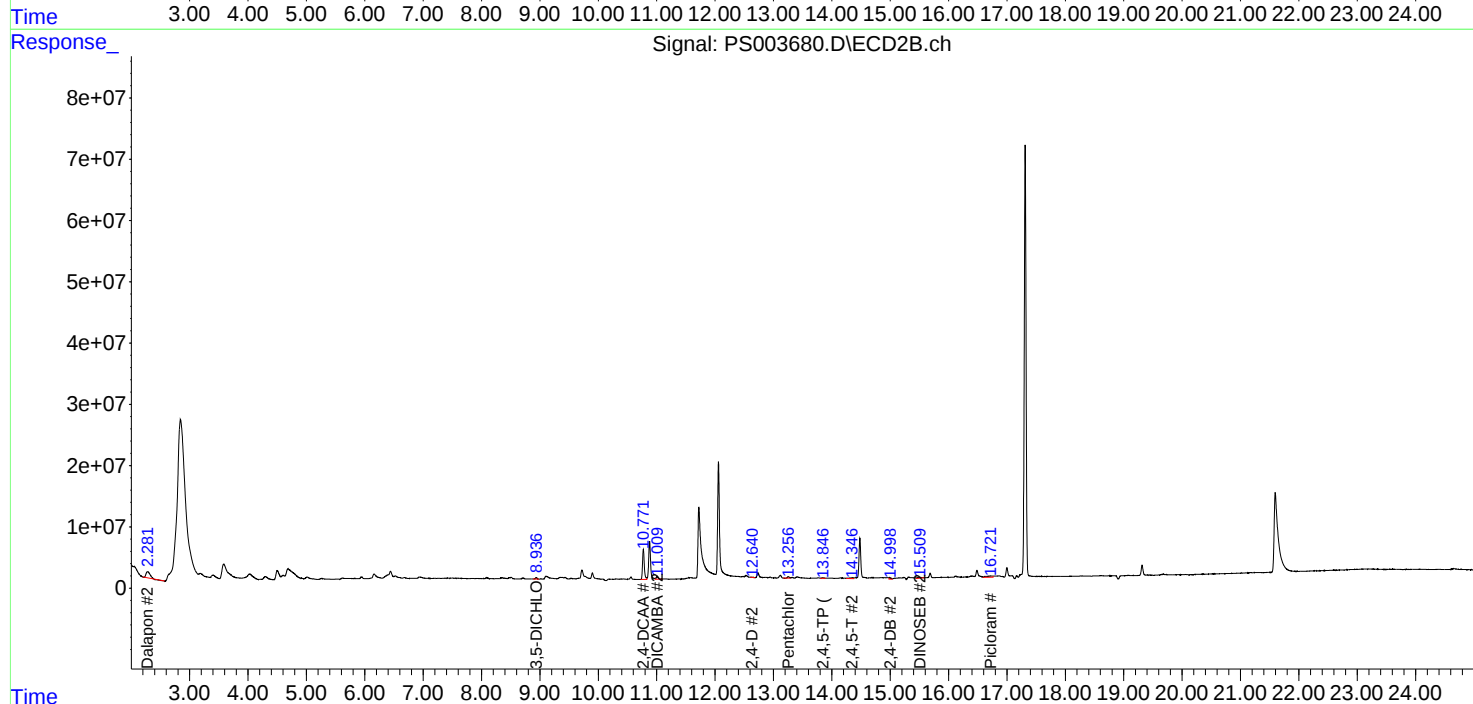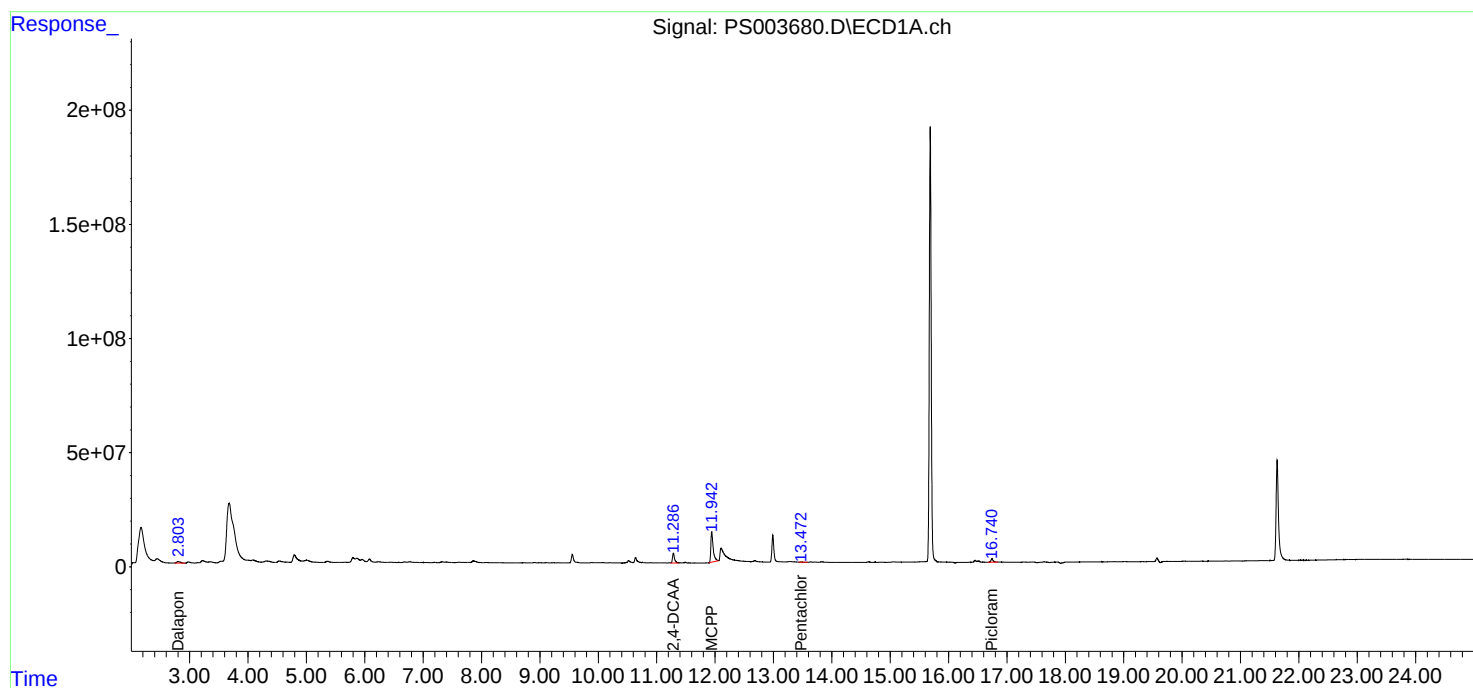


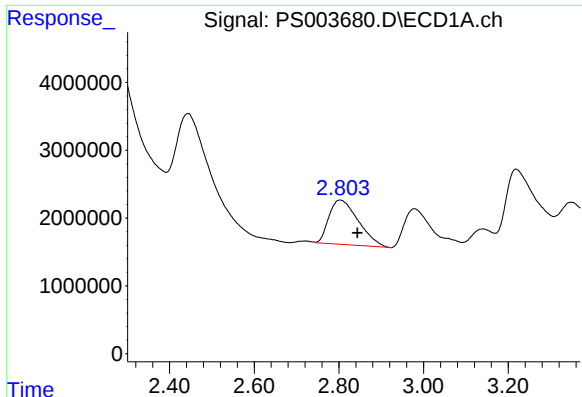

#1 Dalapon


R.T.: 2.803 min
Delta R.T.: -0.041 min
Response: 31493233
Conc: 48.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

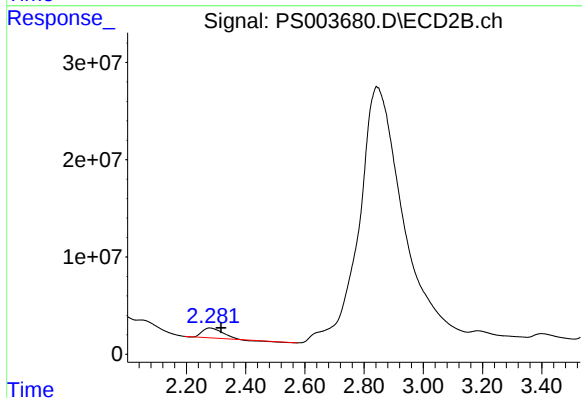


#1 Dalapon

R.T.: 2.278 min
Delta R.T.: -0.038 min
Response: 45206483
Conc: 71.40 ng/ml

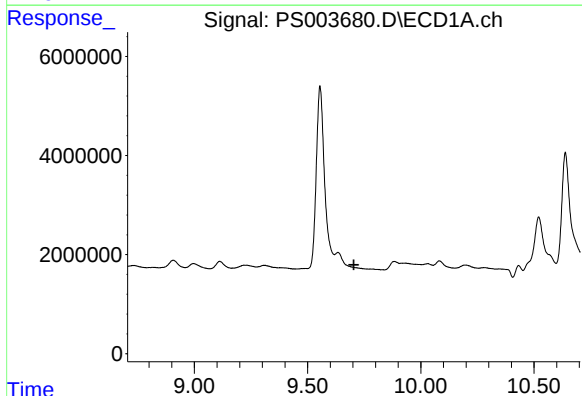


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

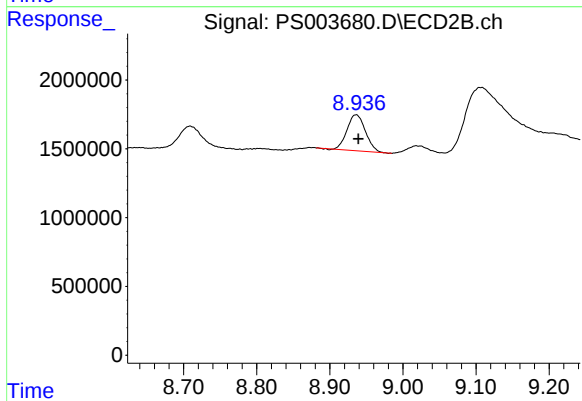

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.936 min
Delta R.T.: -0.003 min
Response: 4556358
Conc: 7.38 ng/ml

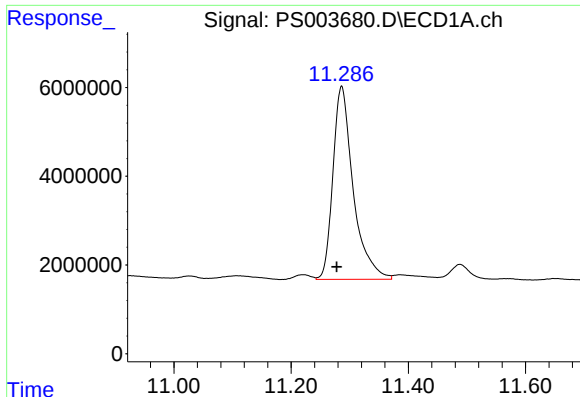

#4 2,4-DCAA


R.T.: 11.286 min
Delta R.T.: 0.008 min
Response: 104706021
Conc: 238.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

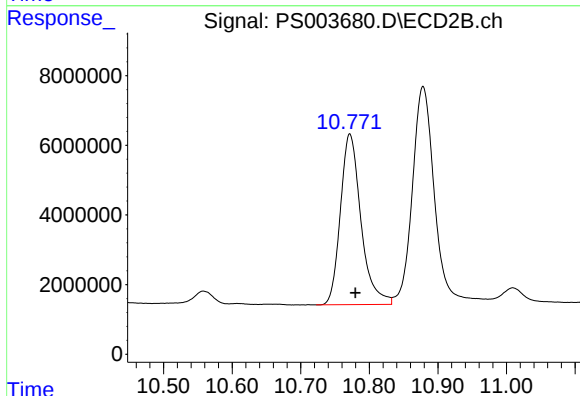


#4 2,4-DCAA

R.T.: 10.772 min
Delta R.T.: -0.008 min
Response: 102163273
Conc: 217.57 ng/ml

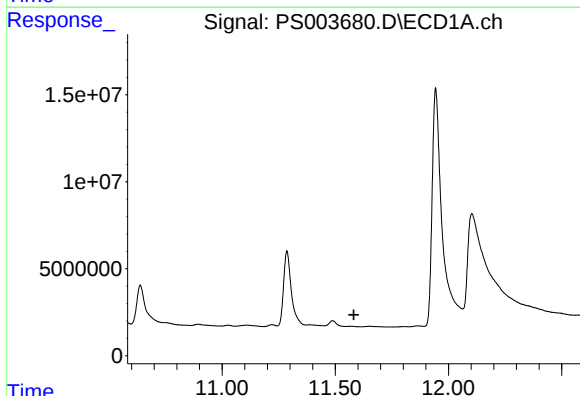


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

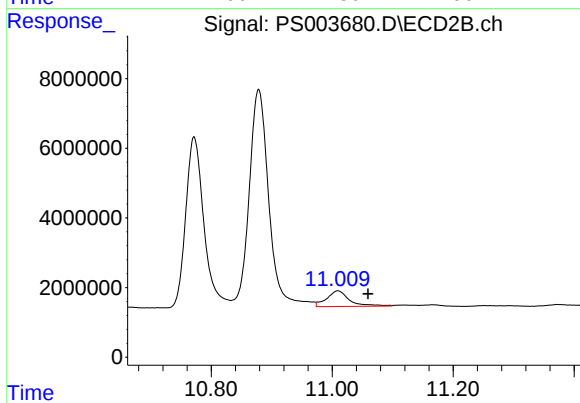

#5 DICAMBA


R.T.: 11.009 min
Delta R.T.: -0.050 min
Response: 11618611
Conc: 6.95 ng/ml

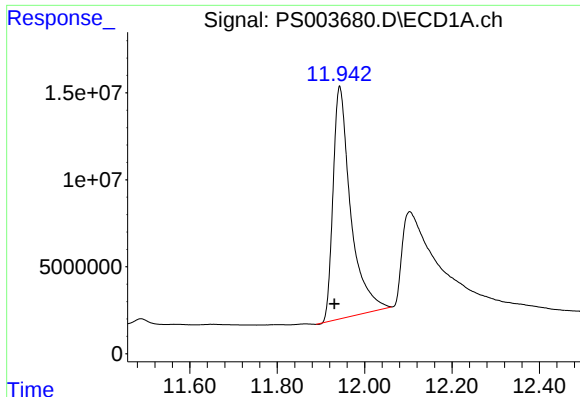

#6 MCP


R.T.: 11.943 min
Delta R.T.: 0.012 min
Response: 374043194
Conc: 284.90 ug/ml

Instrument :
ECD_S
ClientSampleId :

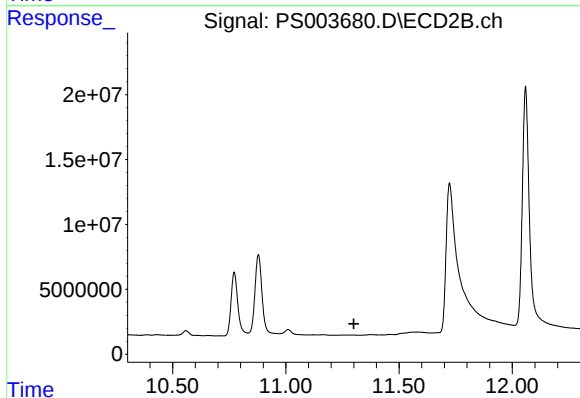


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.300 min
Response: 0
Conc: N.D.

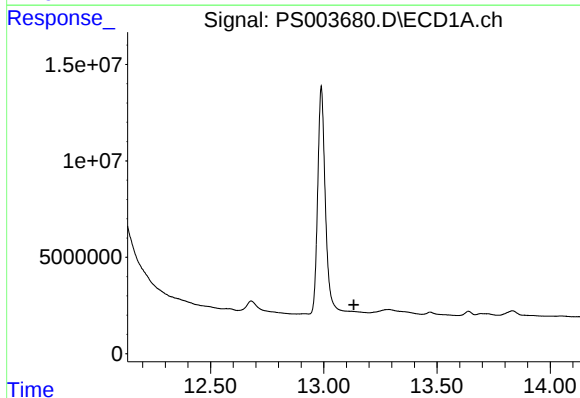


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

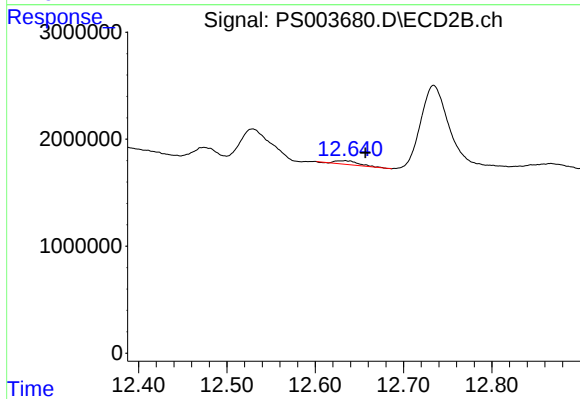

#9 2,4-D


R.T.: 12.633 min
Delta R.T.: -0.024 min
Response: 582635
Conc: 1.11 ng/ml

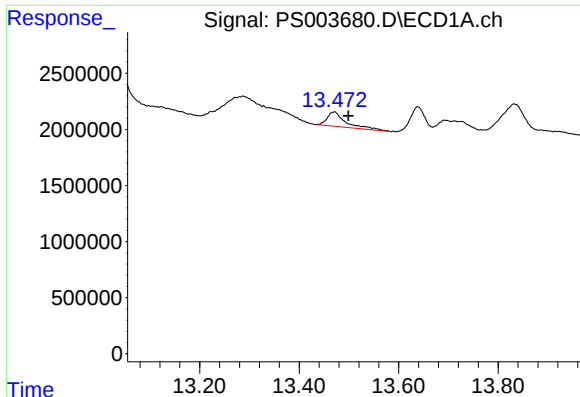

#10 Pentachlorophenol


R.T.: 13.470 min
Delta R.T.: -0.029 min
Response: 3391436
Conc: 0.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

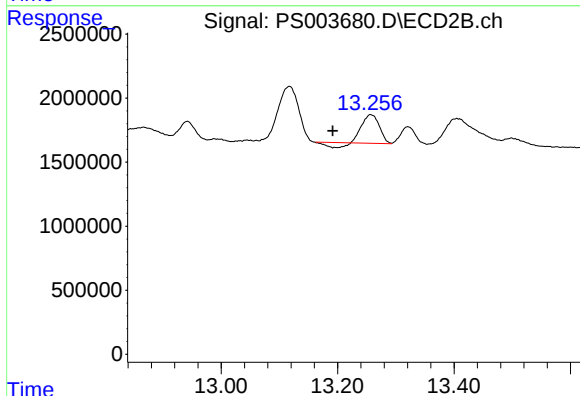


#10 Pentachlorophenol

R.T.: 13.257 min
Delta R.T.: 0.066 min
Response: 4046536
Conc: 0.61 ng/ml

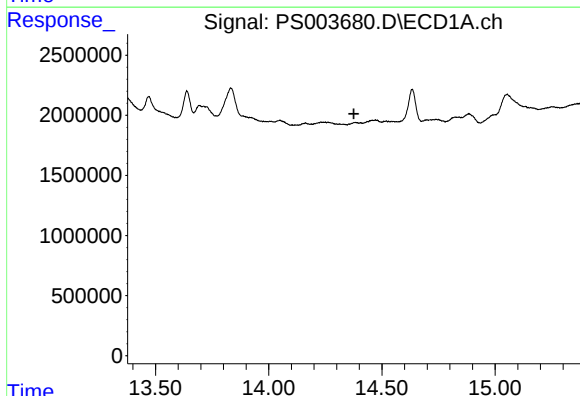


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

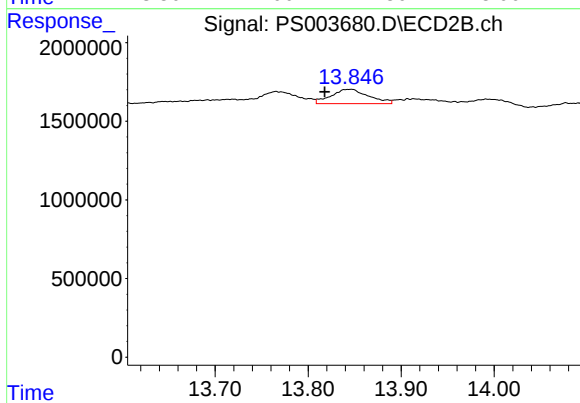

#11 2,4,5-TP (SILVEX)


R.T.: 13.845 min
Delta R.T.: 0.027 min
Response: 2567193
Conc: 1.01 ng/ml

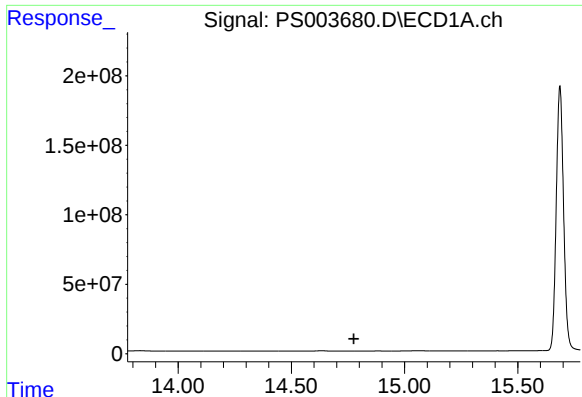

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

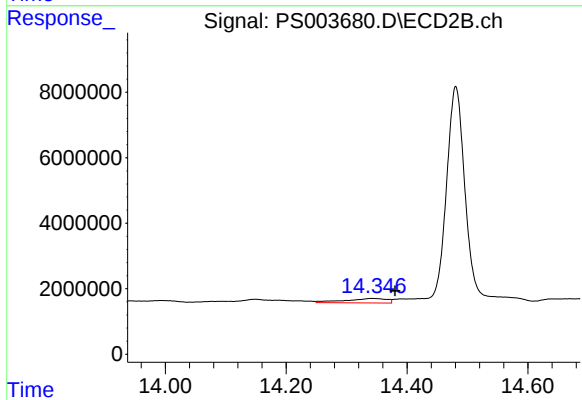


#12 2,4,5-T

R.T.: 14.344 min
Delta R.T.: -0.036 min
Response: 6445727
Conc: 3.20 ng/ml

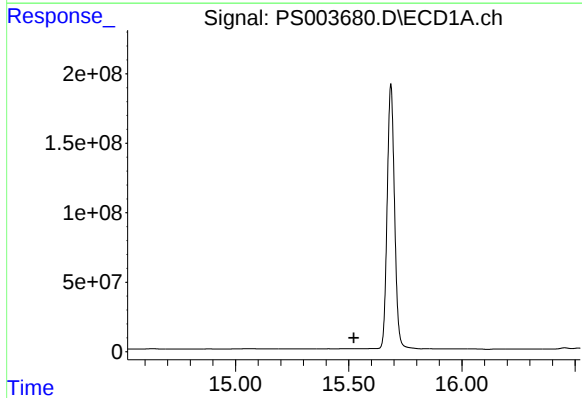


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

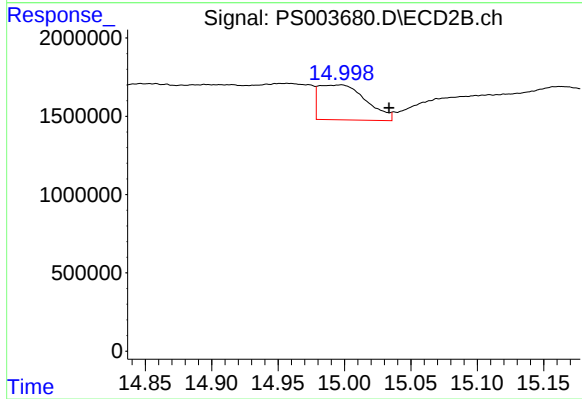

#13 2,4-DB


R.T.: 14.996 min
Delta R.T.: -0.037 min
Response: 5474533
Conc: 21.44 ng/ml

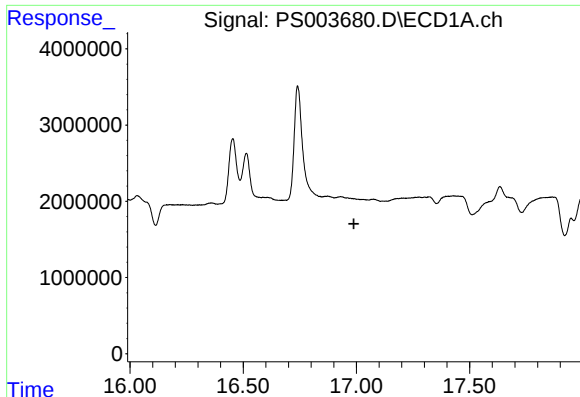

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

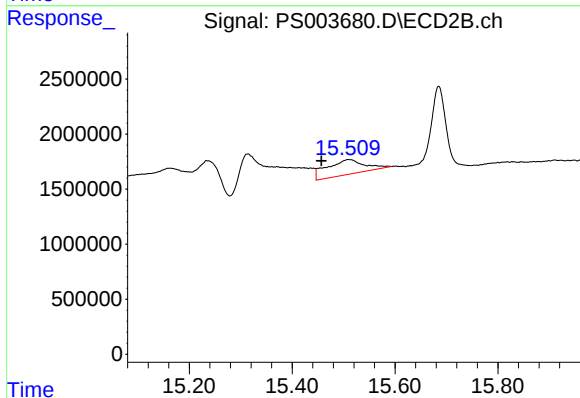


#14 DINOSEB

R.T.: 15.510 min
Delta R.T.: 0.053 min
Response: 6845370
Conc: 3.84 ng/ml

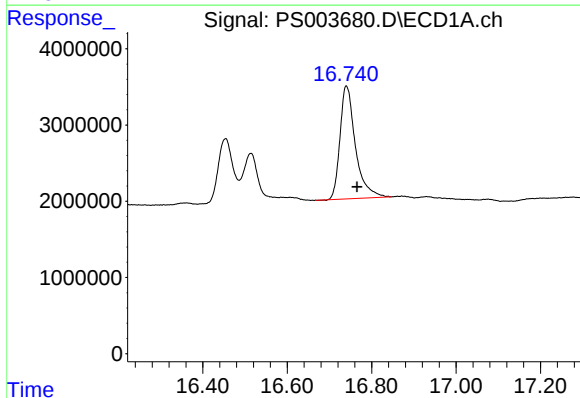

#15 Picloram

R.T.: 16.740 min
Delta R.T.: -0.025 min
Response: 37619871
Conc: 15.28 ng/ml

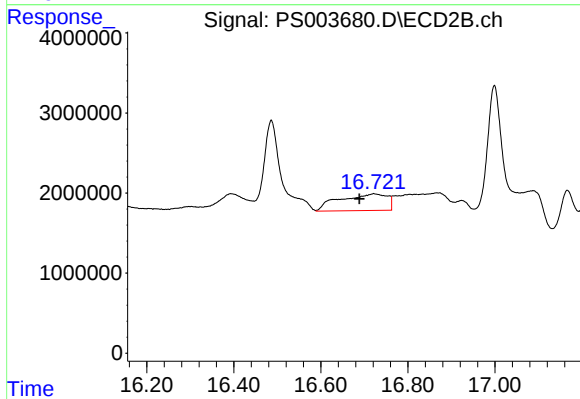

#15 Picloram

R.T.: 16.722 min
Delta R.T.: 0.034 min
Response: 15903310
Conc: 6.27 ng/ml