

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
 Data File : PS003681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 03:41
 Operator : EI\SJ
 Sample : K1943-12
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 06:40:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.268	10.771	433.7E6	403.5E6	987.760	859.223
Target Compounds							
1) T	Dalapon	2.789	2.277	24965178	19938618	38.411	31.489
2) T	3,5-DICHL...	0.000	8.938	0	3436568	N.D.	5.566 #
5) T	DICAMBA	0.000	11.012	0	7697983	N.D.	4.608 #
6) T	MCP	11.957	0.000	37308842	0	28.417	N.D. #
9) T	2,4-D	0.000	12.636	0	810361	N.D.	1.544 #
11) T	2,4,5-TP ...	0.000	13.846	0	1169573	N.D.	0.459 #
12) T	2,4,5-T	0.000	14.352	0	3912451	N.D.	1.940 #
14) T	DINOSEB	0.000	15.509	0	6849261	N.D.	3.837 #
15) T	Picloram	0.000	16.721	0	19495941	N.D.	7.681 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
Data File : PS003681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 03:41
Operator : EI\SJ
Sample : K1943-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 06:40:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

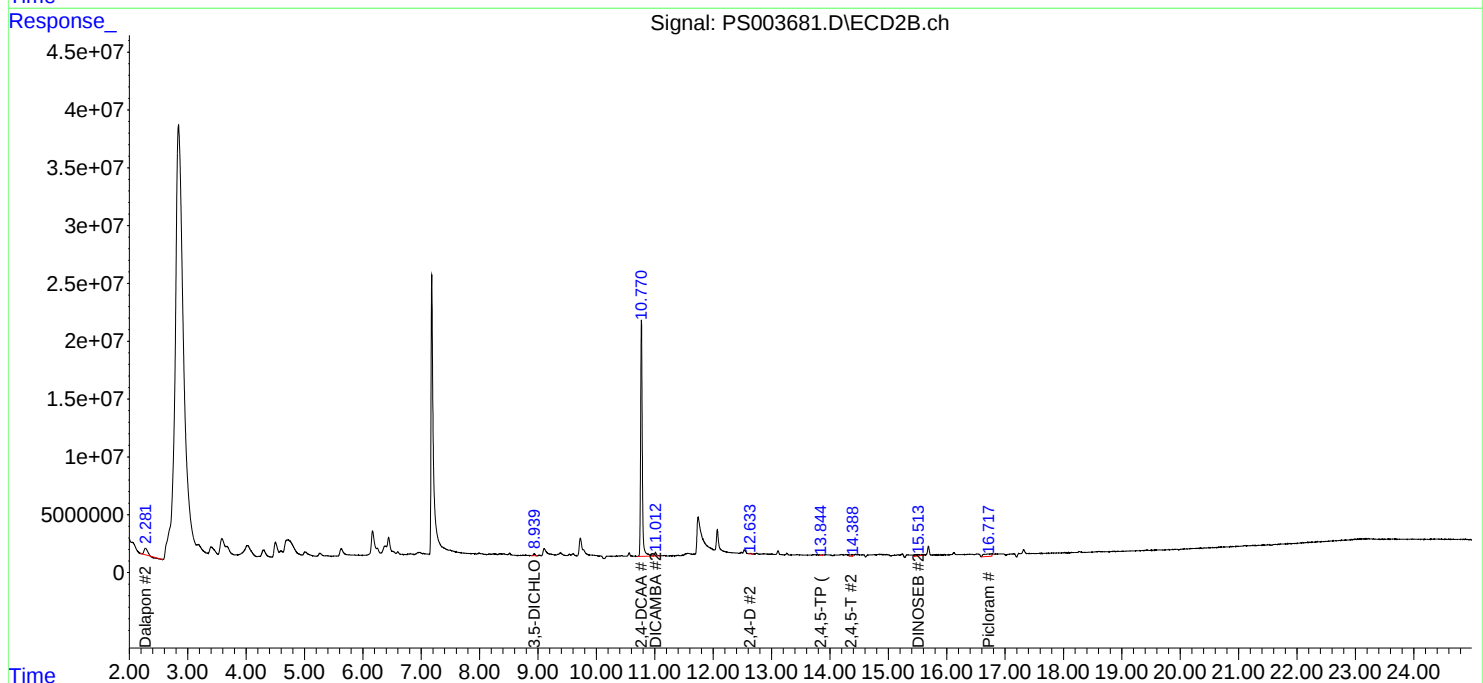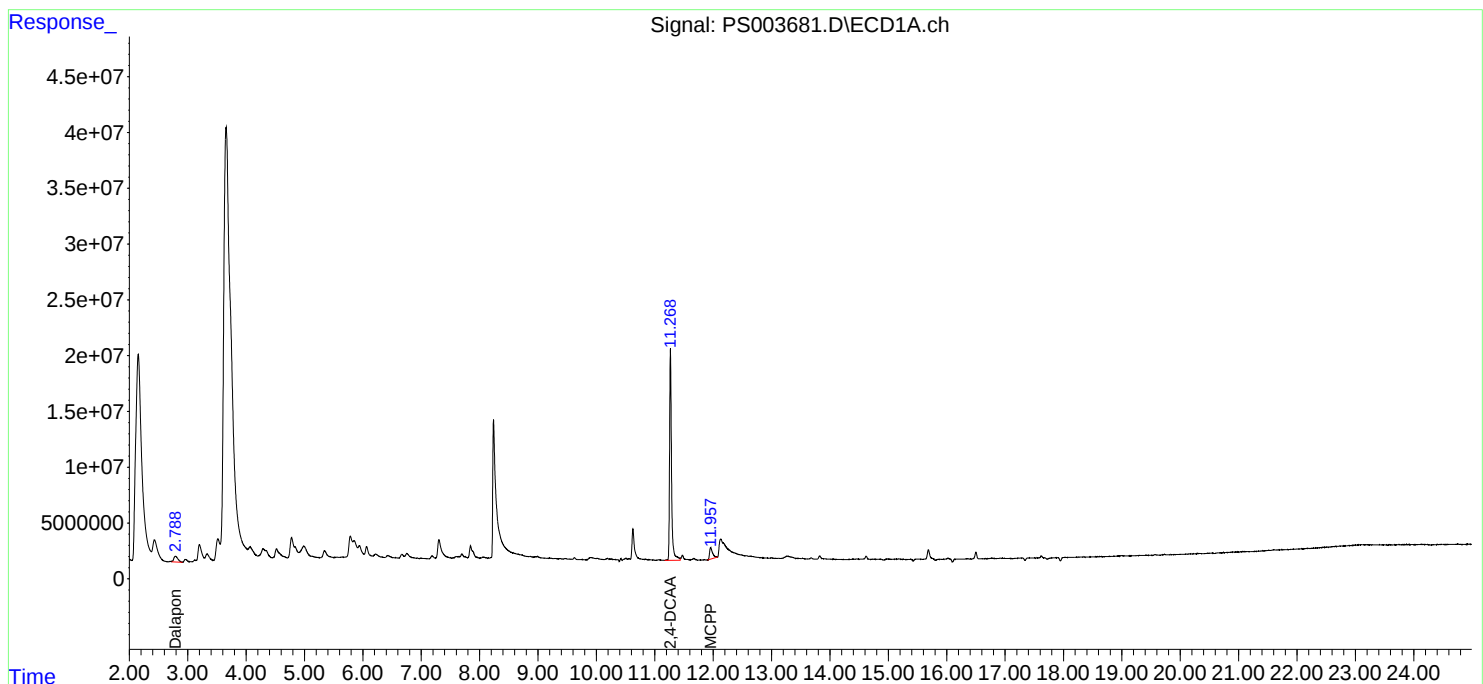


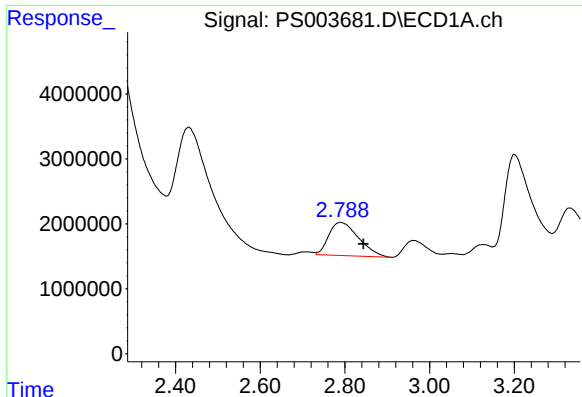

#1 Dalapon


R.T.: 2.789 min
Delta R.T.: -0.055 min
Response: 24965178
Conc: 38.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

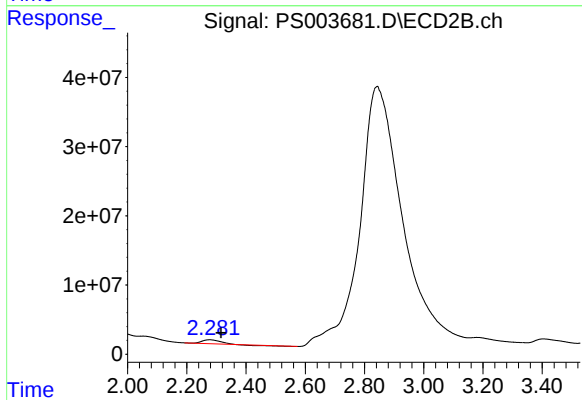


#1 Dalapon

R.T.: 2.277 min
Delta R.T.: -0.039 min
Response: 19938618
Conc: 31.49 ng/ml

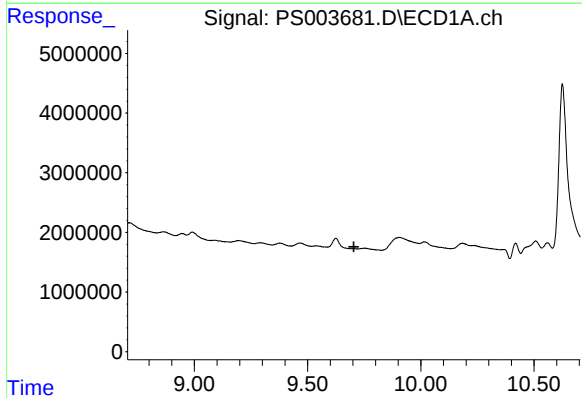


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

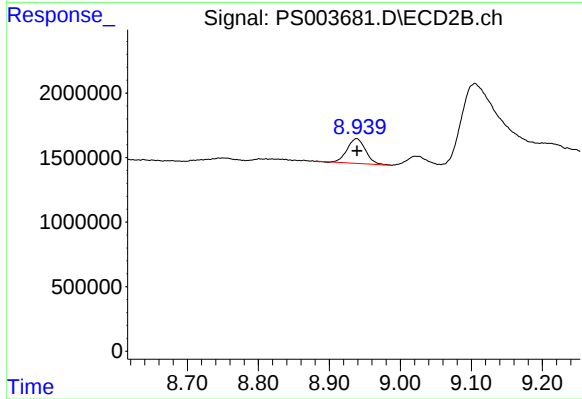

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.938 min
Delta R.T.: -0.001 min
Response: 3436568
Conc: 5.57 ng/ml

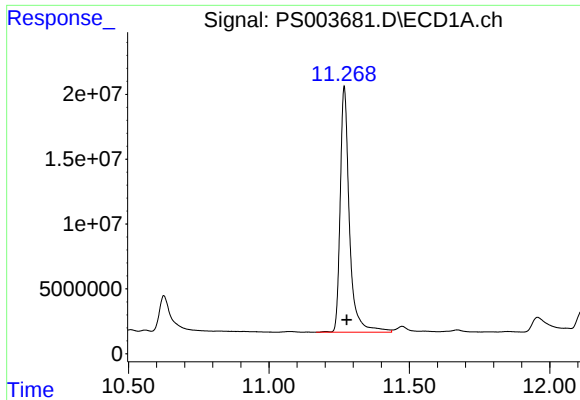

#4 2,4-DCAA


R.T.: 11.268 min
Delta R.T.: -0.009 min
Response: 433650884
Conc: 987.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

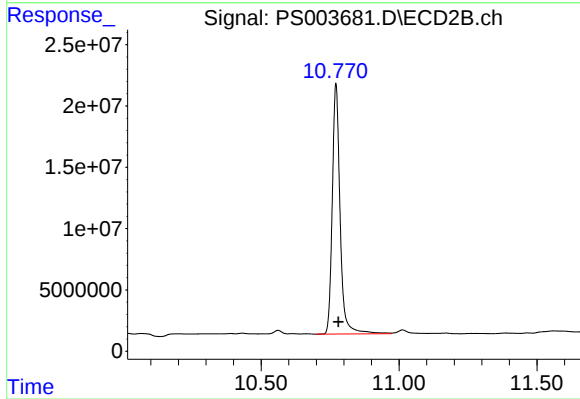


#4 2,4-DCAA

R.T.: 10.771 min
Delta R.T.: -0.009 min
Response: 403464809
Conc: 859.22 ng/ml

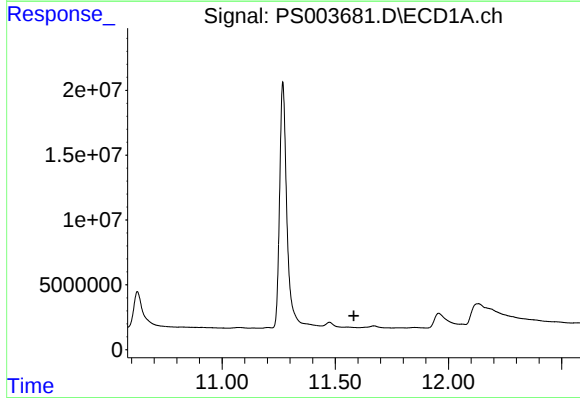


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

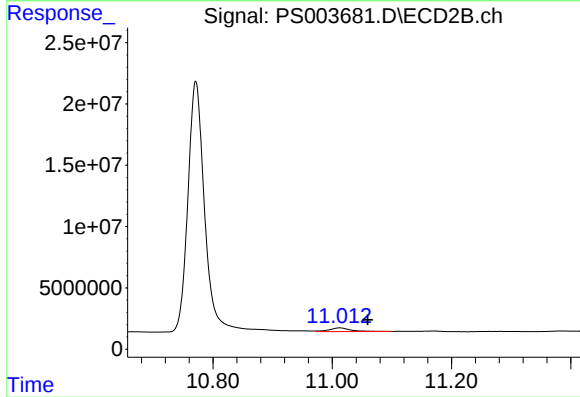

#5 DICAMBA


R.T.: 11.012 min
Delta R.T.: -0.047 min
Response: 7697983
Conc: 4.61 ng/ml

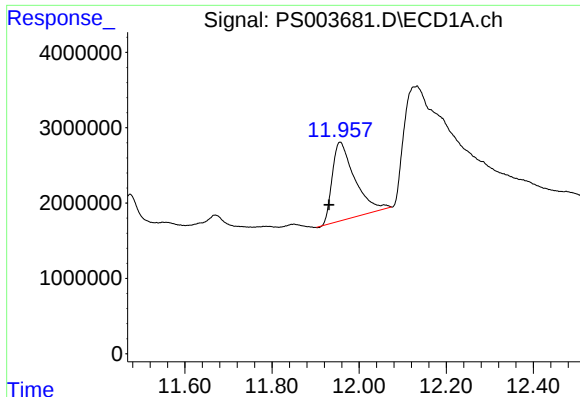

#6 MCP


R.T.: 11.957 min
Delta R.T.: 0.026 min
Response: 37308842
Conc: 28.42 ug/ml

Instrument :
ECD_S
ClientSampleId :

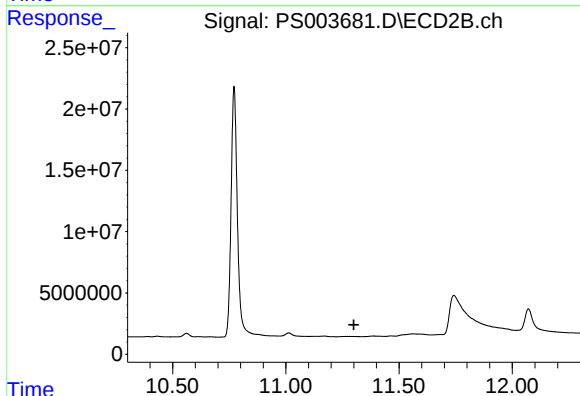


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.300 min
Response: 0
Conc: N.D.

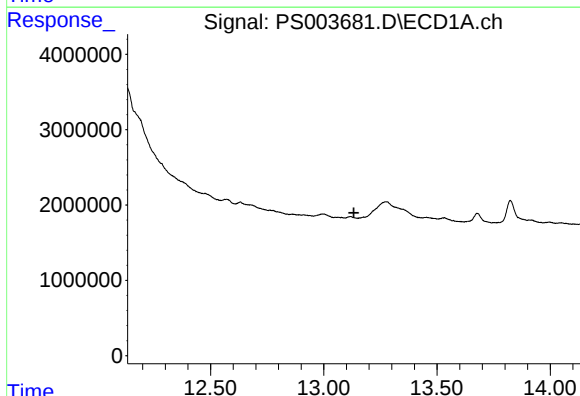


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

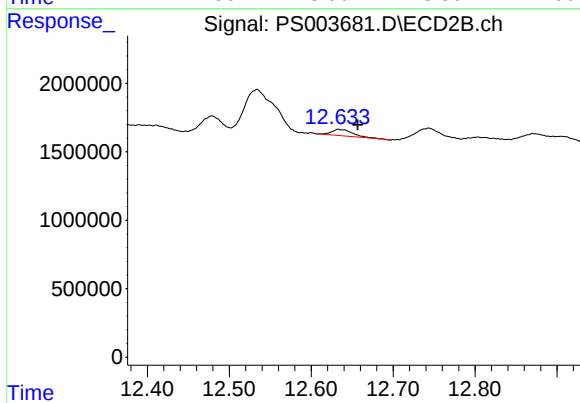

#9 2,4-D


R.T.: 12.636 min
Delta R.T.: -0.021 min
Response: 810361
Conc: 1.54 ng/ml

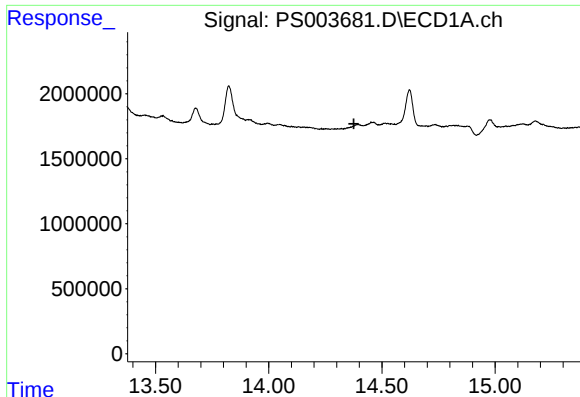

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

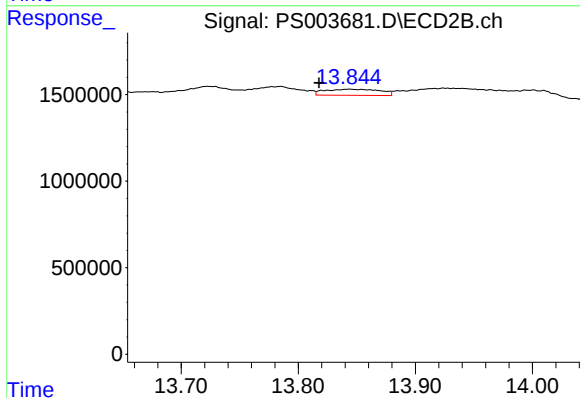


#11 2,4,5-TP (SILVEX)

R.T.: 13.846 min
Delta R.T.: 0.029 min
Response: 1169573
Conc: 0.46 ng/ml

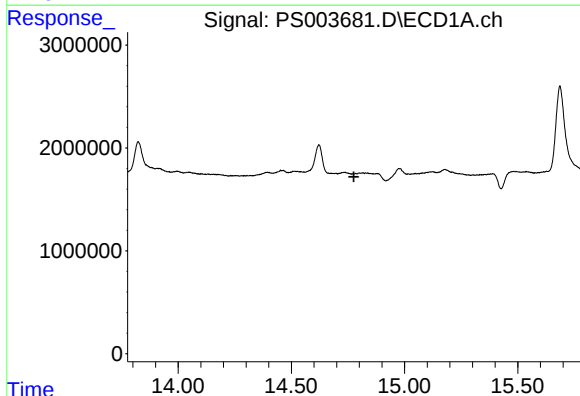


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

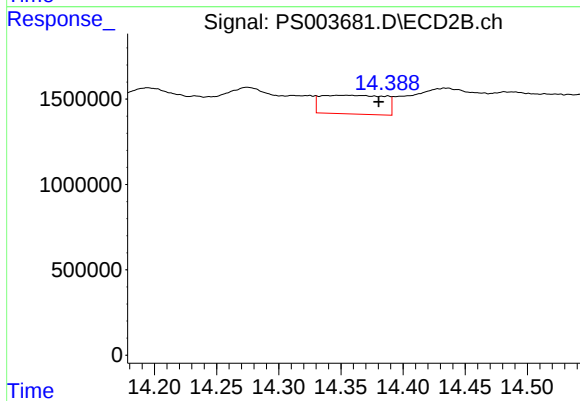

#12 2,4,5-T


R.T.: 14.352 min
Delta R.T.: -0.028 min
Response: 3912451
Conc: 1.94 ng/ml

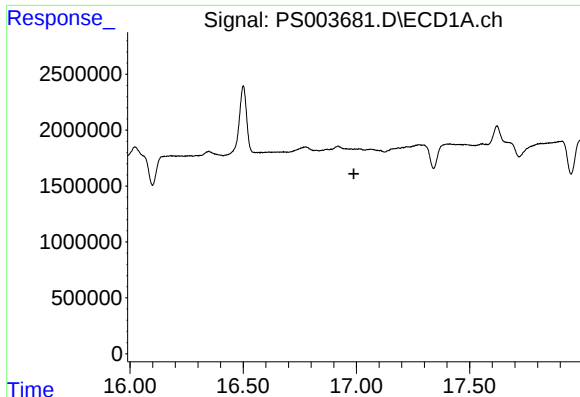

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

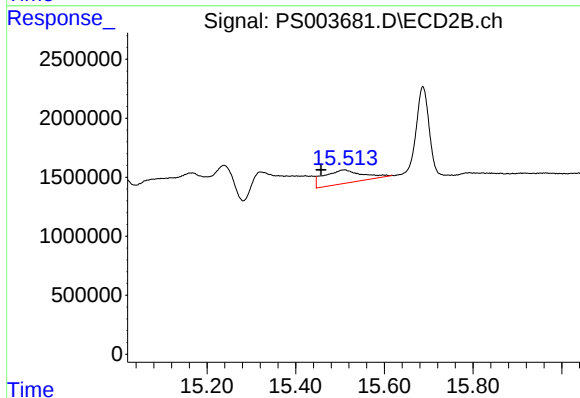


#14 DINOSEB

R.T.: 15.509 min
Delta R.T.: 0.052 min
Response: 6849261
Conc: 3.84 ng/ml

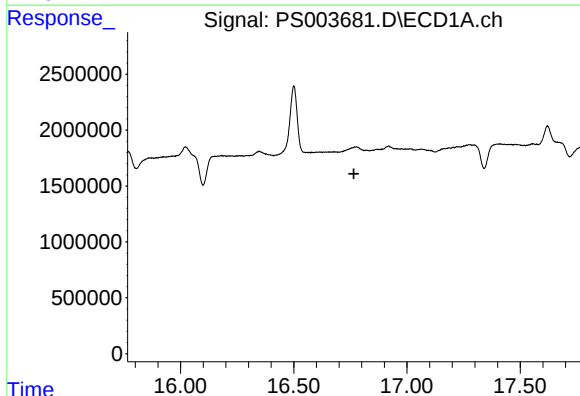

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

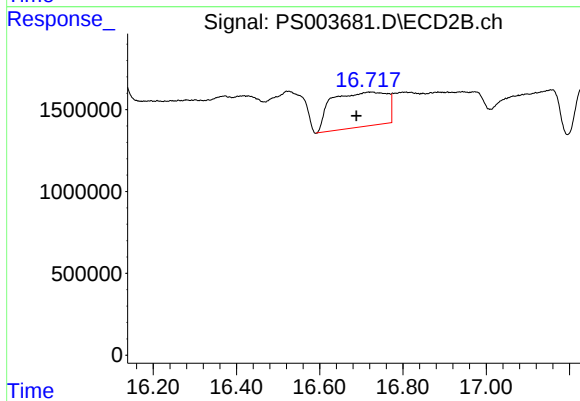

#15 Picloram

R.T.: 16.721 min
Delta R.T.: 0.033 min
Response: 19495941
Conc: 7.68 ng/ml