

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
 Data File : PS003686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 06:18
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 07:25:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.271	10.772	248.1E6	234.4E6	565.110	499.095
Target Compounds							
3) T	4-Nitroph...	0.000	9.983	0	59987	N.D.	0.267 #
7) T	MCPA	0.000	11.663	0	811785	N.D.	0.471 #
8) T	DICHLORPROP	0.000	12.119	0	7465810	N.D.	18.066 #
10) T	Pentachlo...	0.000	13.184	0	925358	N.D.	0.141 #
11) T	2,4,5-TP ...	0.000	13.827	0	117186	N.D.	0.046 #
12) T	2,4,5-T	0.000	14.433	0	699781	N.D.	0.347 #
14) T	DINOSEB	0.000	15.459	0	467512	N.D.	0.262 #
15) T	Picloram	16.752	16.681	7524976	4235890	3.057	1.669 #
16) T	DCPA	0.000	16.620	0	8772276	N.D.	2.820 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032119\
Data File : PS003686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 06:18
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 07:25:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

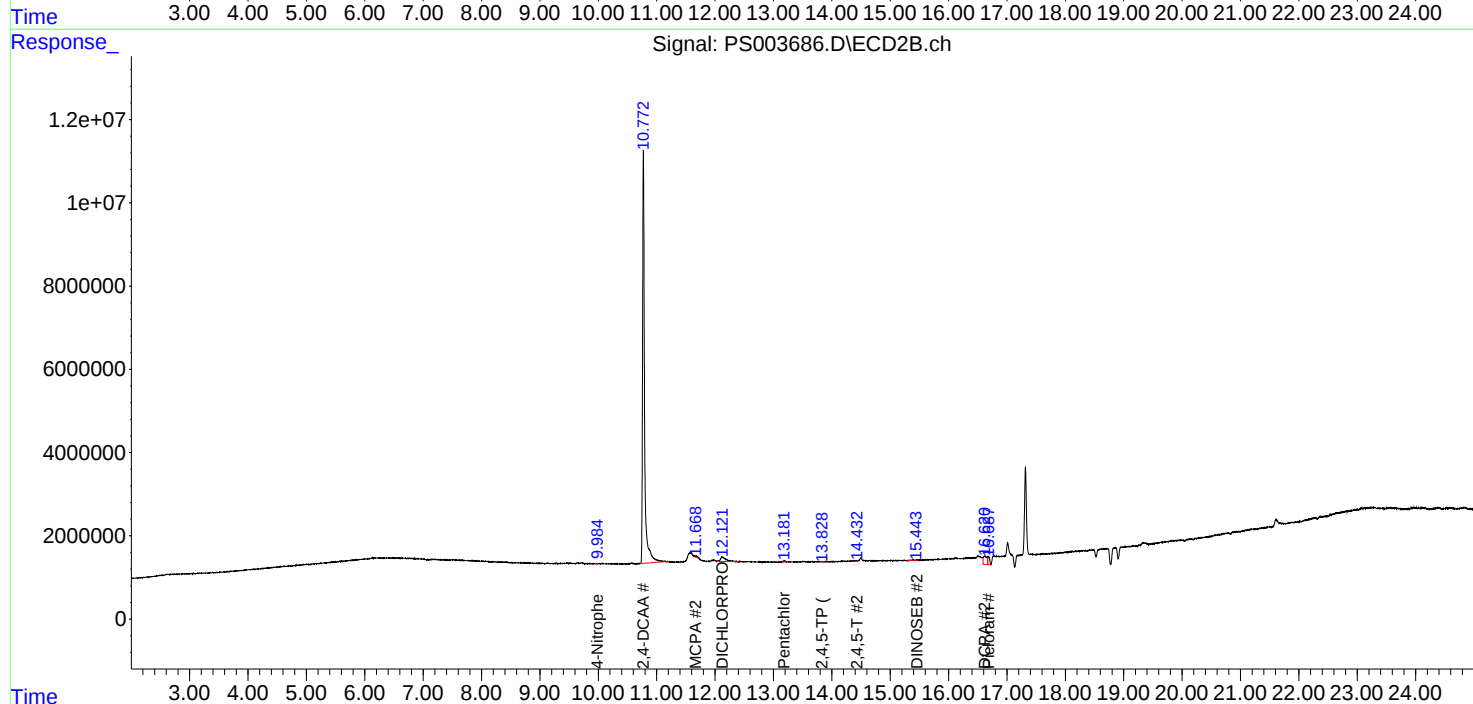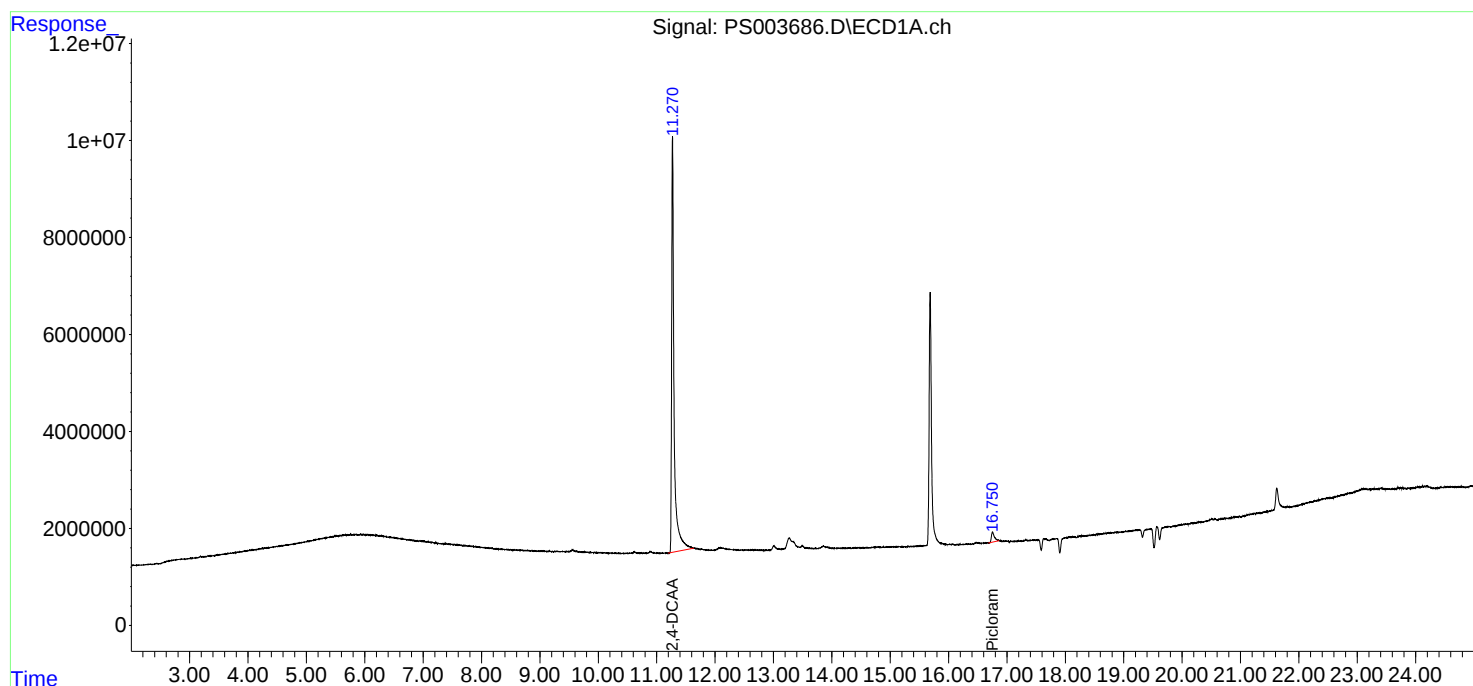


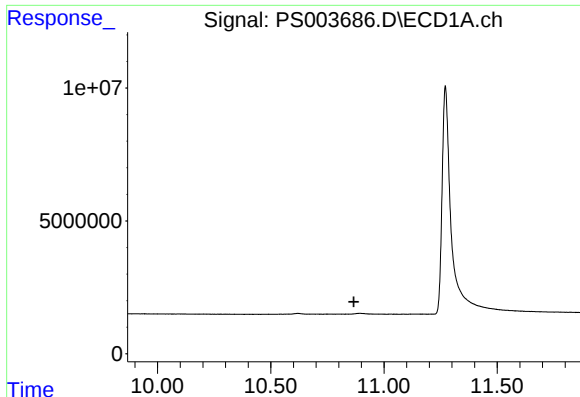

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

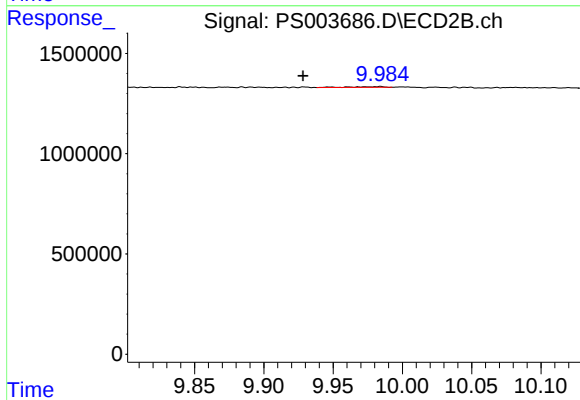


#3 4-Nitrophenol

R.T.: 9.983 min
Delta R.T.: 0.055 min
Response: 59987
Conc: 0.27 ng/ml

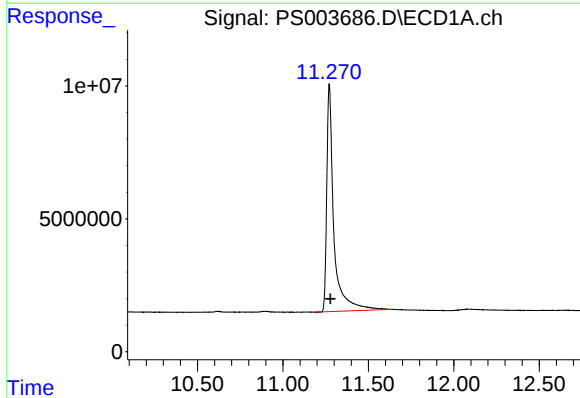


#4 2,4-DCAA

R.T.: 11.271 min
Delta R.T.: -0.007 min
Response: 248097343
Conc: 565.11 ng/ml

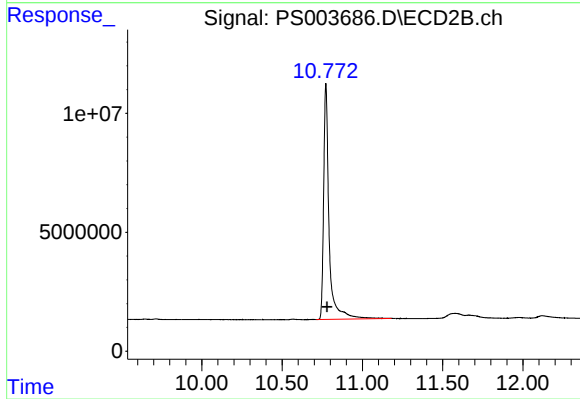

#4 2,4-DCAA


R.T.: 10.772 min
Delta R.T.: -0.007 min
Response: 234359809
Conc: 499.10 ng/ml

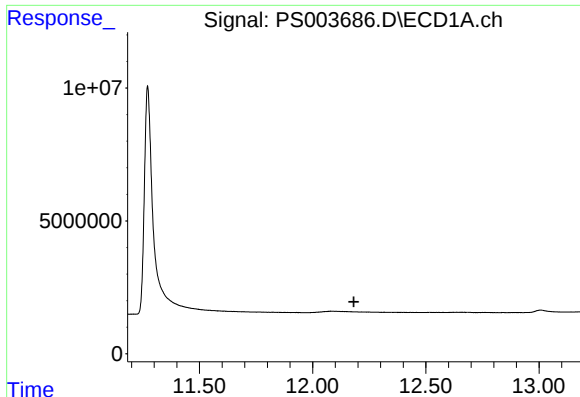

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

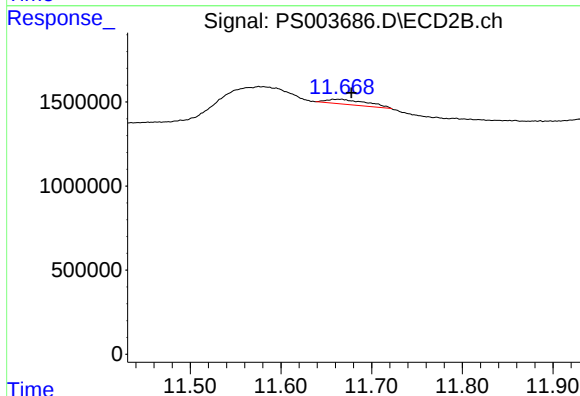


#7 MCPA

R.T.: 11.663 min
Delta R.T.: -0.014 min
Response: 811785
Conc: 0.47 ug/ml

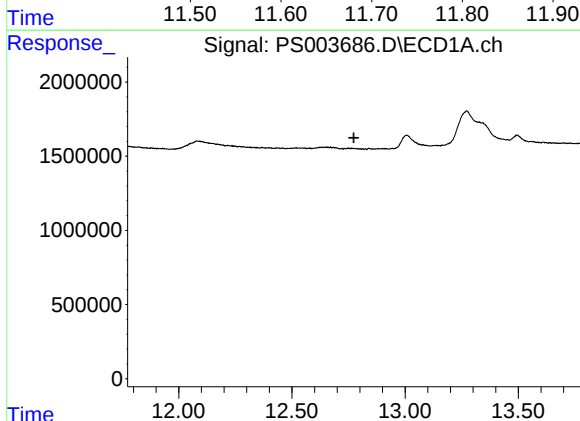


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

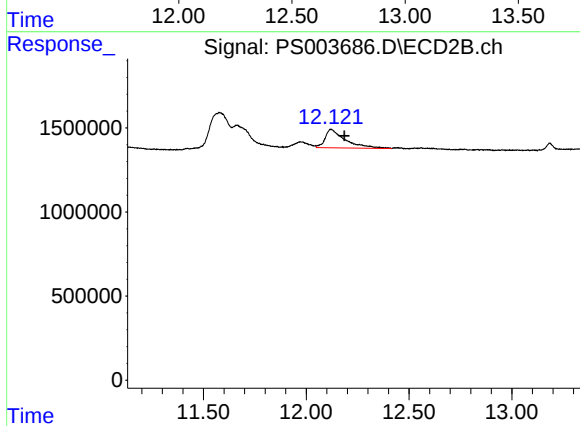

#8 DICHLORPROP


R.T.: 12.119 min
Delta R.T.: -0.066 min
Response: 7465810
Conc: 18.07 ng/ml

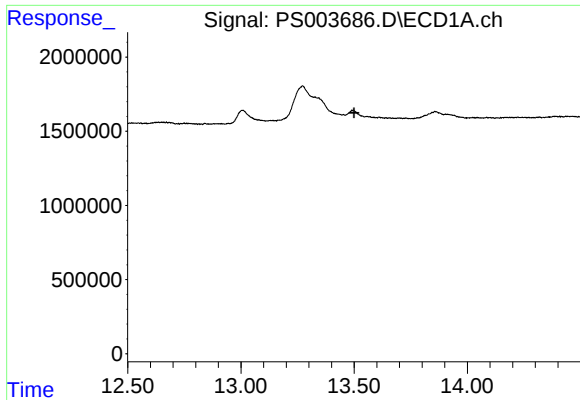

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

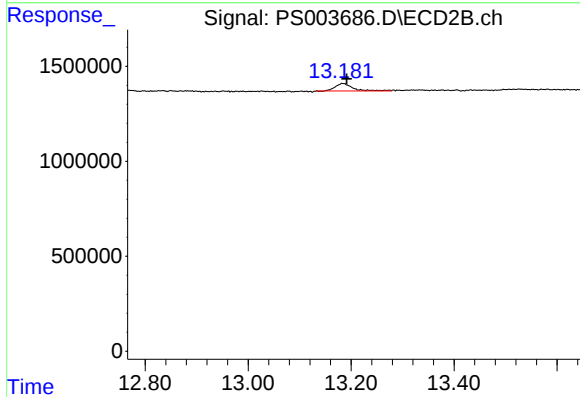


#10 Pentachlorophenol

R.T.: 13.184 min
Delta R.T.: -0.008 min
Response: 925358
Conc: 0.14 ng/ml

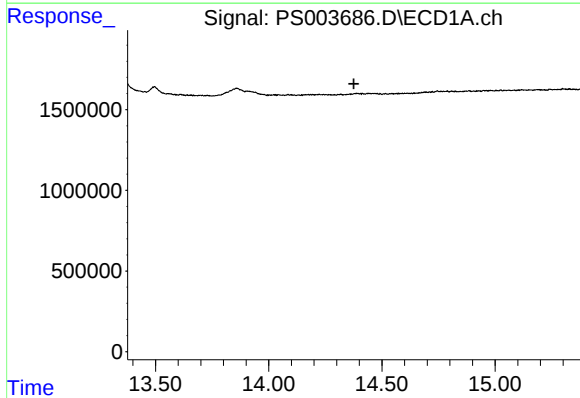


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

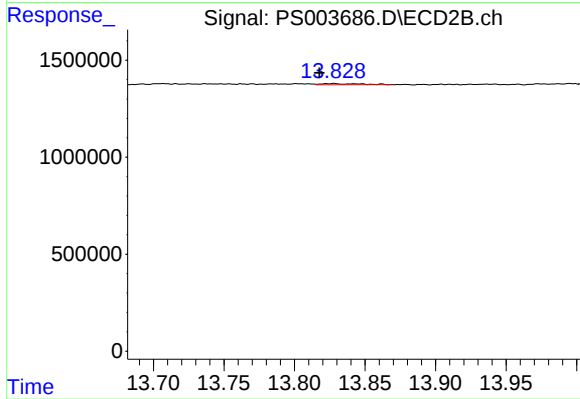

#11 2,4,5-TP (SILVEX)


R.T.: 13.827 min
Delta R.T.: 0.009 min
Response: 117186
Conc: 0.05 ng/ml

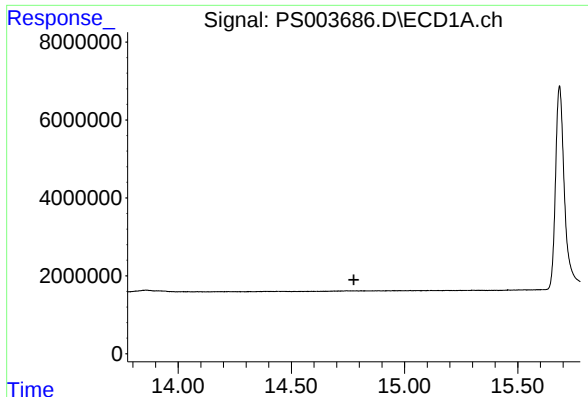

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

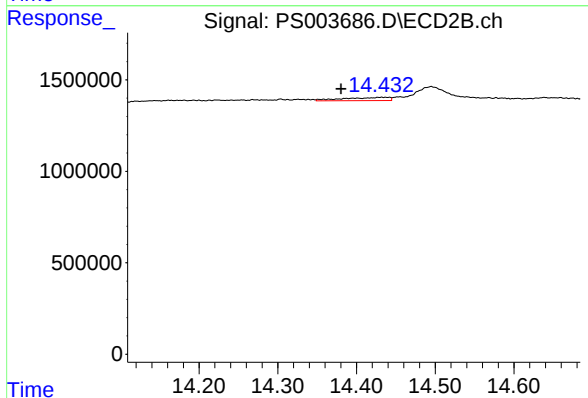


#12 2,4,5-T

R.T.: 14.433 min
Delta R.T.: 0.052 min
Response: 699781
Conc: 0.35 ng/ml

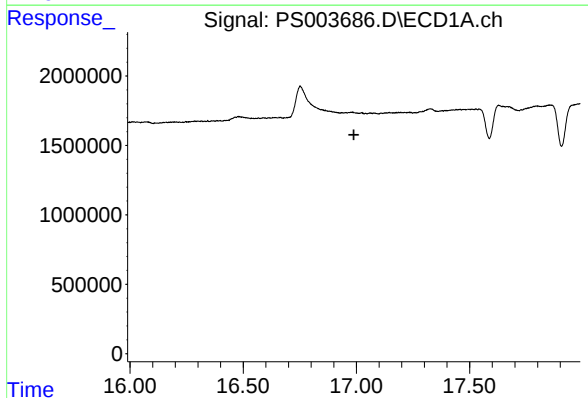


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

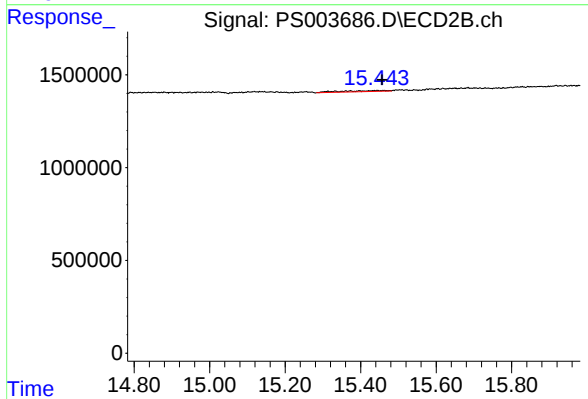

#14 DINOSEB


R.T.: 15.459 min
Delta R.T.: 0.002 min
Response: 467512
Conc: 0.26 ng/ml

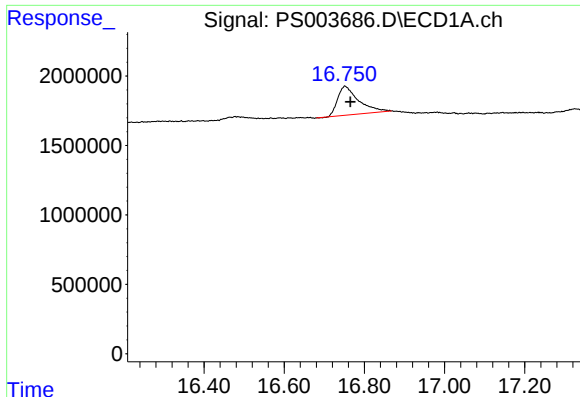

#15 Picloram


R.T.: 16.752 min
Delta R.T.: -0.014 min
Response: 7524976
Conc: 3.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

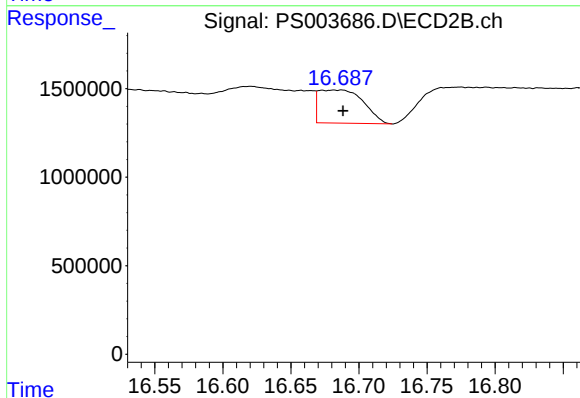


#15 Picloram

R.T.: 16.681 min
Delta R.T.: -0.008 min
Response: 4235890
Conc: 1.67 ng/ml

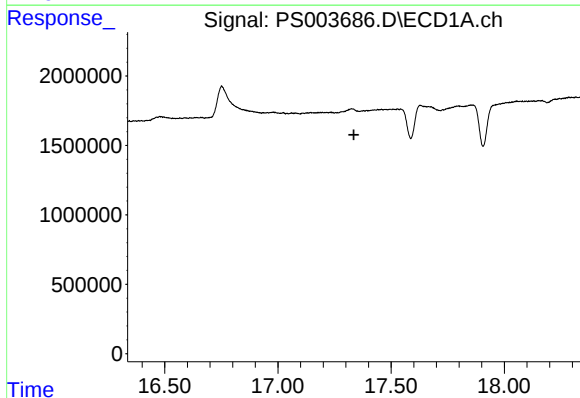

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

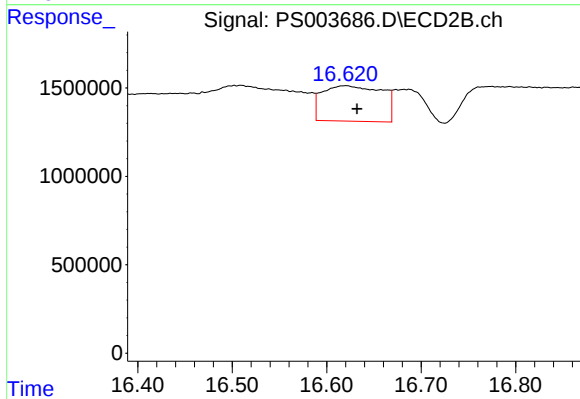

#16 DCPA

R.T.: 16.620 min
Delta R.T.: -0.012 min
Response: 8772276
Conc: 2.82 ng/ml