

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032122\
 Data File : PS018636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2022 09:17
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 15:46:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.479	0.000	101.4E6	0	26.301	N.D. #
5) T	DICAMBA	0.000	7.035f	0	21535994	N.D.	7.230
6) T	MCP	0.000	7.035f	0	21535994	N.D.	8.797
8) T	DICHLORPROP	0.000	7.621	0	5528339	N.D.	6.984
9) T	2,4-D	8.416f	0.000	55099369	0	16.444	N.D. #
10) T	Pentachlo...	8.667	0.000	5541892	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.642f	0	2405860	N.D.	<MDL
12) T	2,4,5-T	0.000	9.110f	0	2127816	N.D.	<MDL
14) T	DINOSEB	11.249	0.000	5817830	0	<MDL	N.D. #
15) T	Picloram	11.006	10.876	141.8E6	6703794	6.898	1.261 #
16) T	DCPA	0.000	10.876f	0	6703794	N.D.	1.275



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032122\
Data File : PS018636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2022 09:17
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 15:46:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

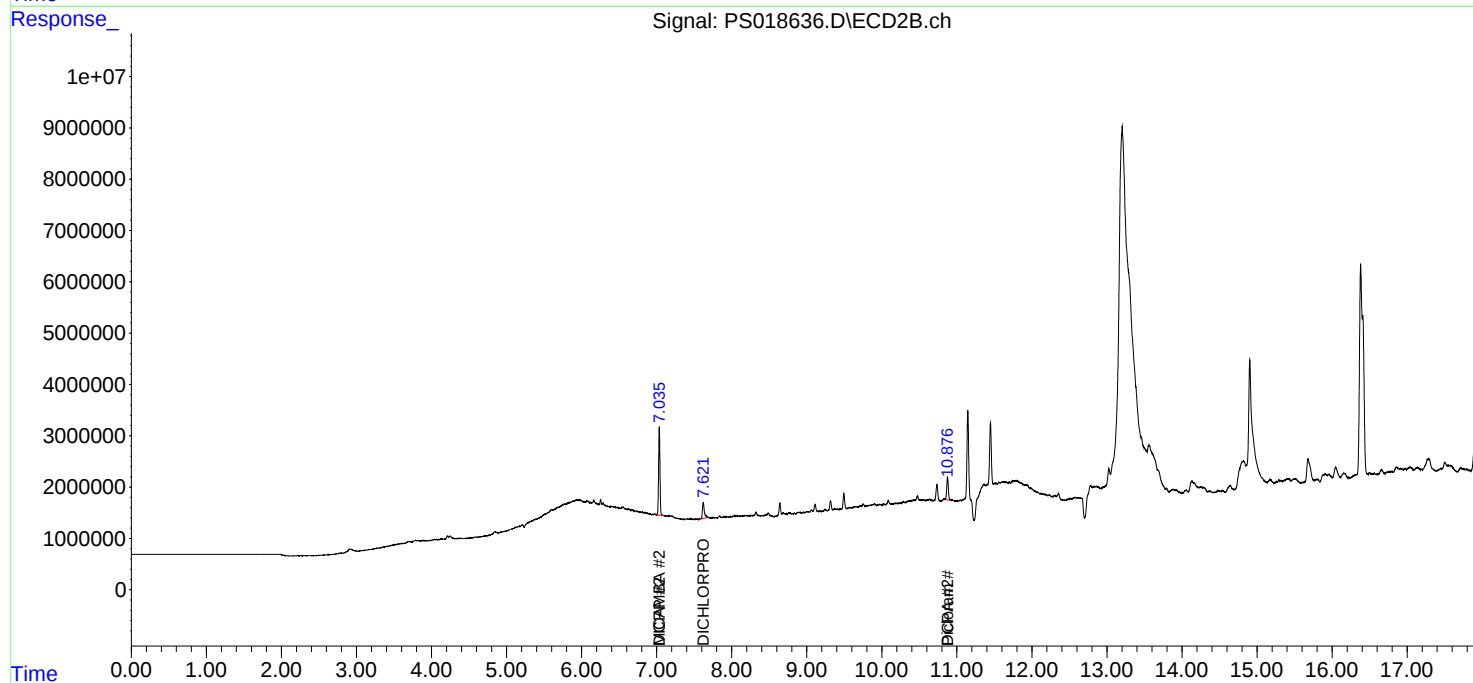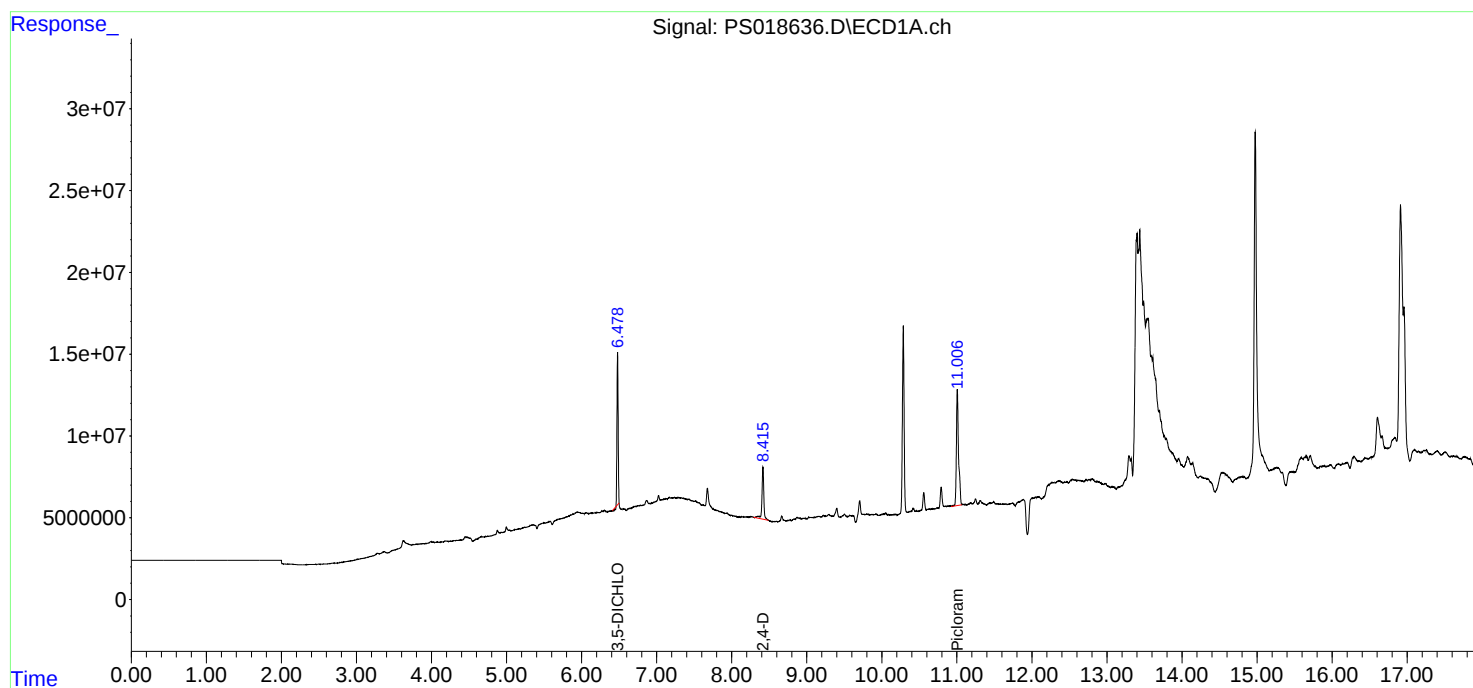


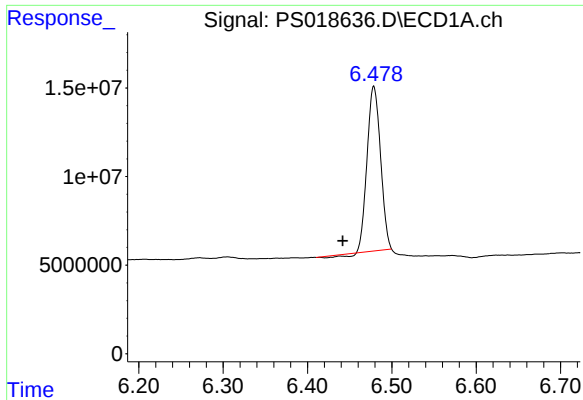

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.479 min
Delta R.T.: 0.037 min
Response: 101350989
Conc: 26.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

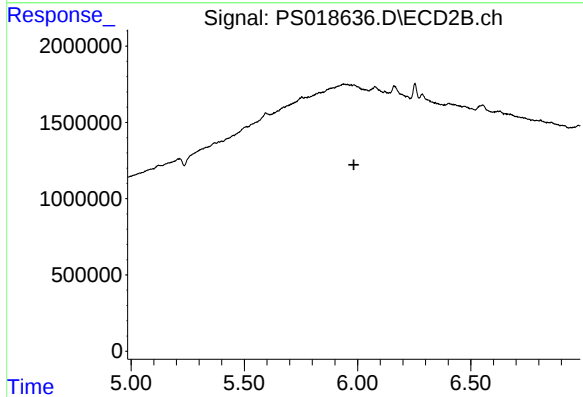


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.984 min
Response: 0
Conc: N.D.

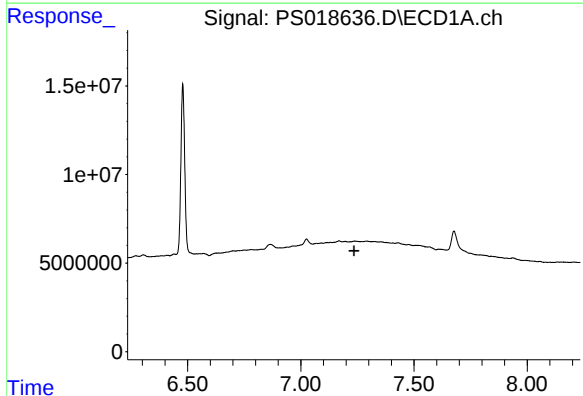


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.235 min
Response: 0
Conc: N.D.

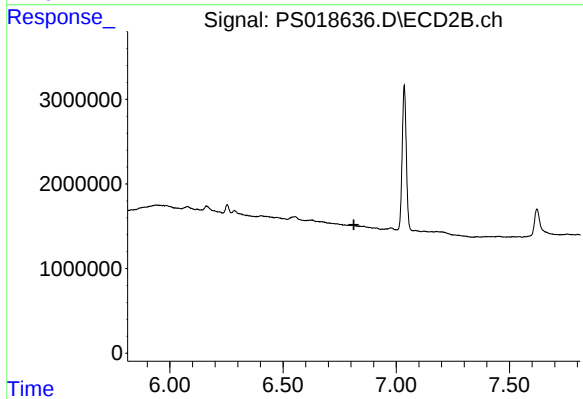

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.813 min
Response: 0
Conc: N.D.

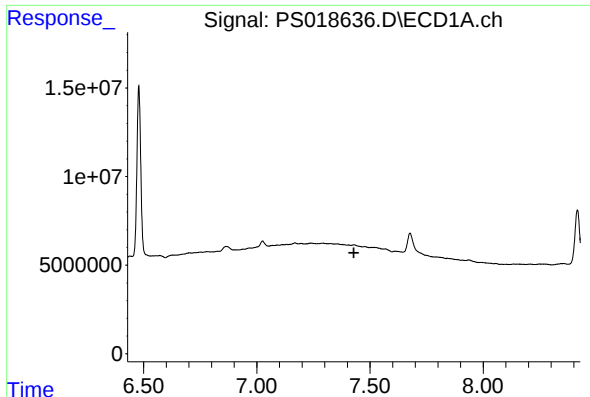

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.429 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

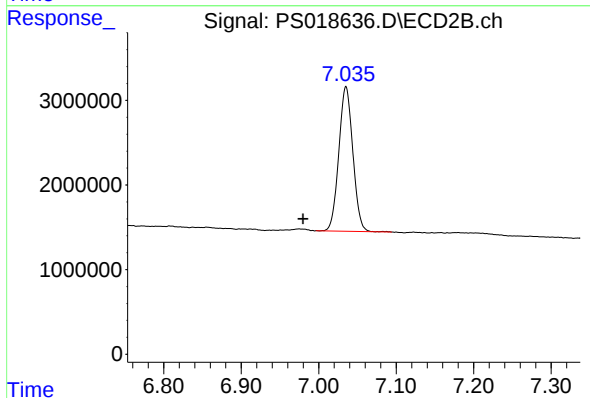


#5 DICAMBA

R.T.: 7.035 min
Delta R.T.: 0.055 min
Response: 21535994
Conc: 7.23 ng/ml

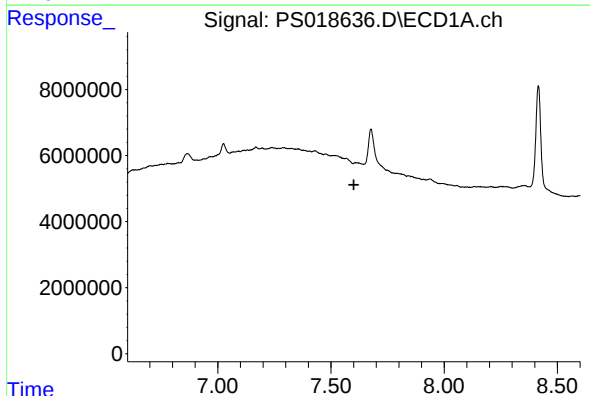


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.601 min
Response: 0
Conc: N.D.

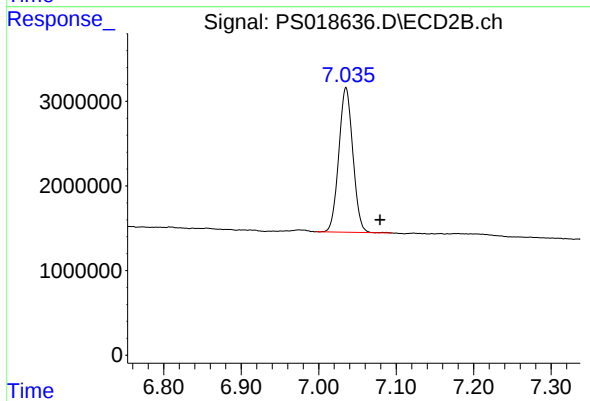

#6 MCP


R.T.: 7.035 min
Delta R.T.: -0.044 min
Response: 21535994
Conc: 8.80 ug/ml

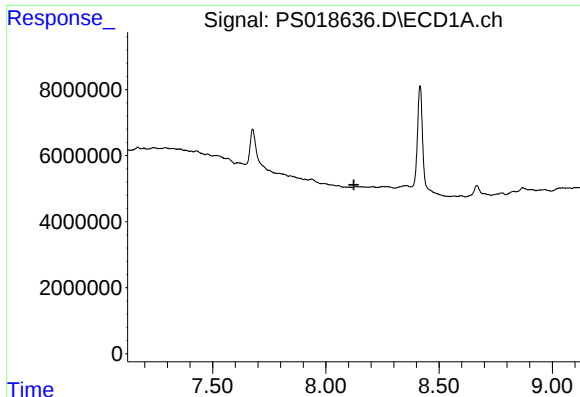

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

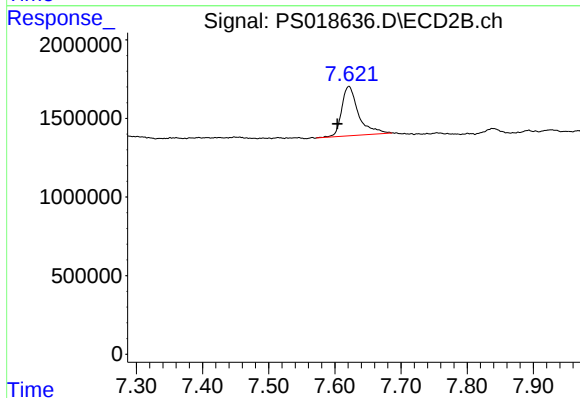


#8 DICHLORPROP

R.T.: 7.621 min
Delta R.T.: 0.017 min
Response: 5528339
Conc: 6.98 ng/ml

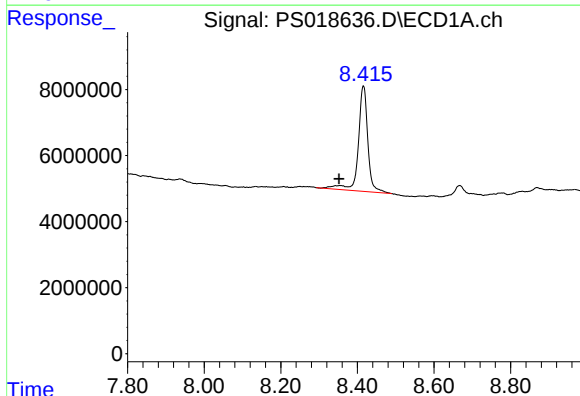


#9 2,4-D

R.T.: 8.416 min
Delta R.T.: 0.064 min
Response: 55099369
Conc: 16.44 ng/ml

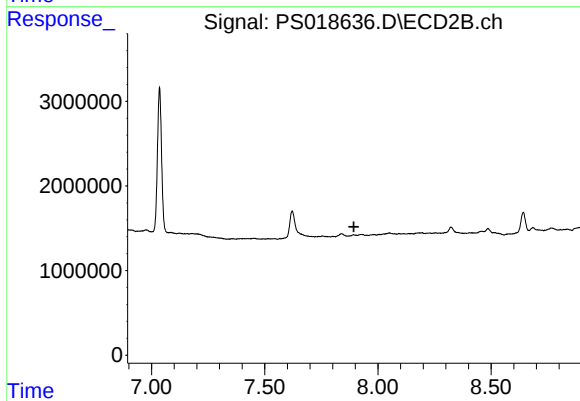

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

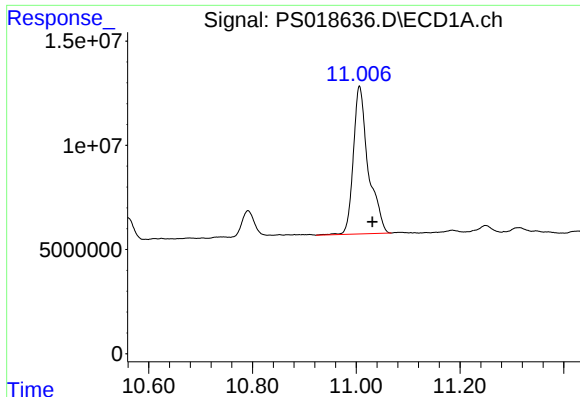

#15 Picloram


R.T.: 11.006 min
Delta R.T.: -0.025 min
Response: 141798071
Conc: 6.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

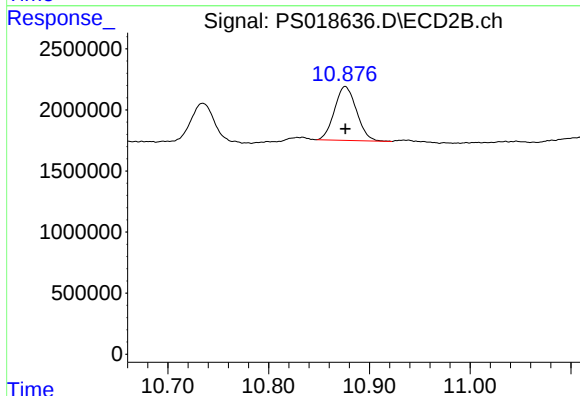


#15 Picloram

R.T.: 10.876 min
Delta R.T.: 0.000 min
Response: 6703794
Conc: 1.26 ng/ml

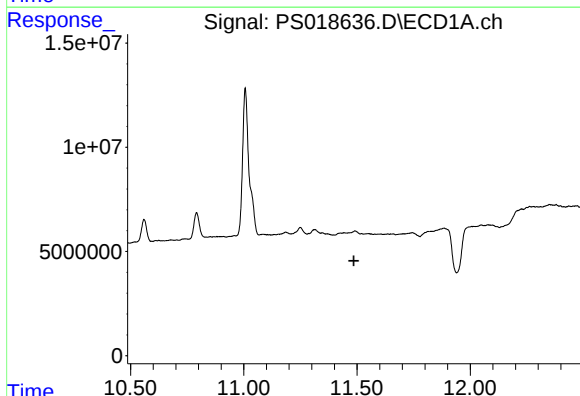

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.486 min
Response: 0
Conc: N.D.

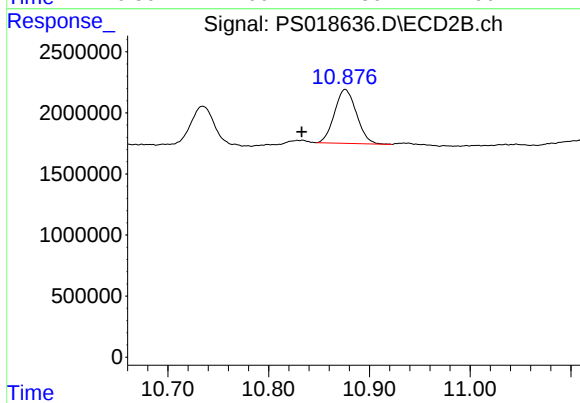

#16 DCPA

R.T.: 10.876 min
Delta R.T.: 0.043 min
Response: 6703794
Conc: 1.27 ng/ml