

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032122\
 Data File : PS018644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2022 15:28
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 16:15:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.810	1490.1E6	419.1E6	523.598	595.611
Target Compounds							
3) T	4-Nitroph...	7.121f	0.000	1979846	0	1.149	N.D. #
8) T	DICHLORPROP	0.000	7.624	0	11781166	N.D.	14.882
11) T	2,4,5-TP ...	9.169f	8.641f	97394241	14636201	6.404	3.355 #
12) T	2,4,5-T	9.495	0.000	5788938	0	<MDL	N.D. #
13) T	2,4-DB	10.006f	0.000	55842	0	<MDL	N.D. #
14) T	DINOSEB	11.178f	0.000	6465211	0	<MDL	N.D. #
15) T	Picloram	11.030	10.874	36646476	8325563	1.783	1.566
16) T	DCPA	0.000	10.874f	0	8325563	N.D.	1.583



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032122\
Data File : PS018644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2022 15:28
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 16:15:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

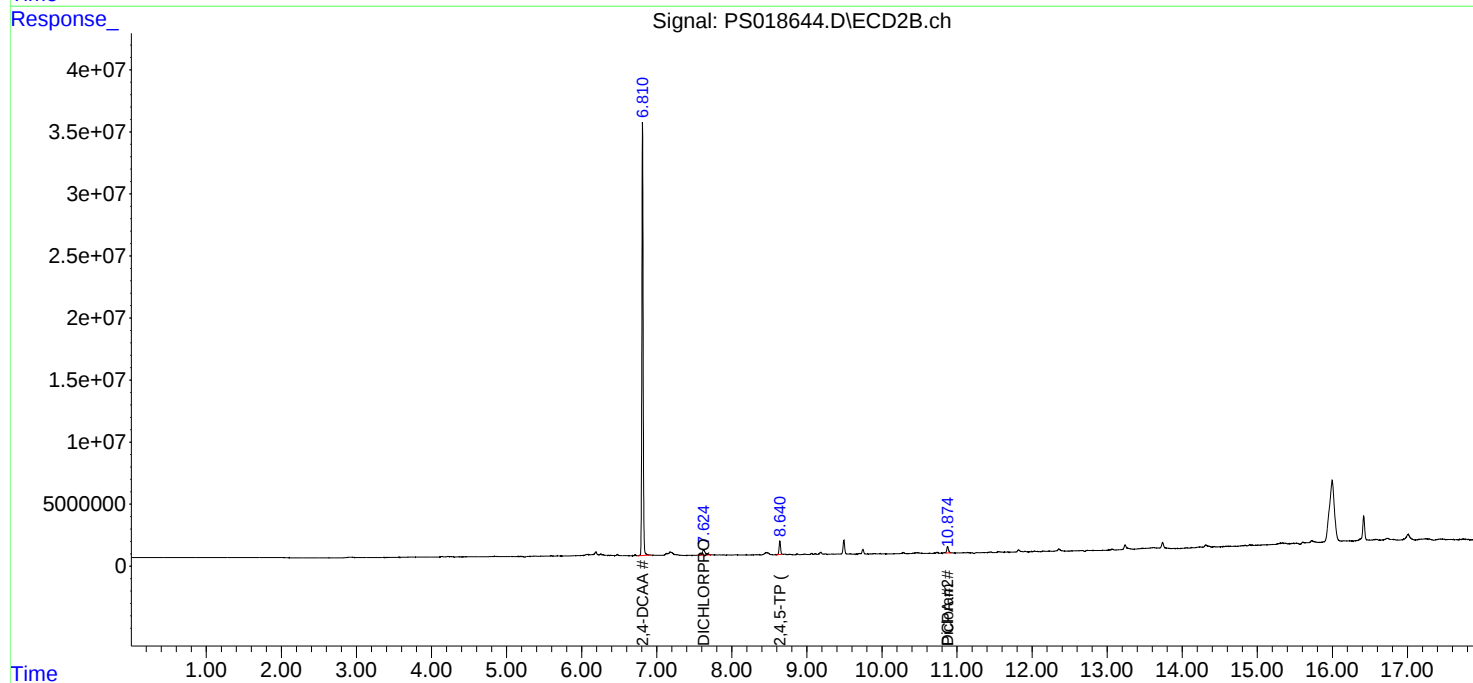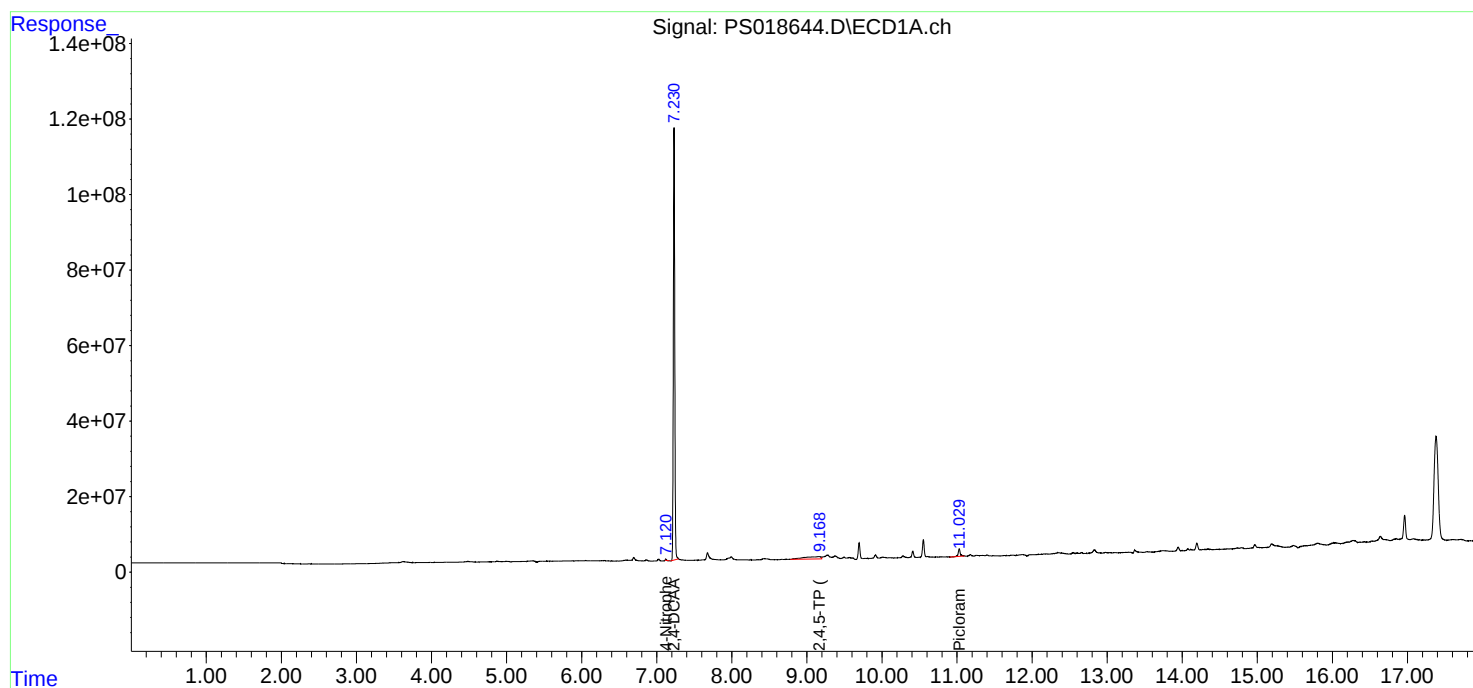


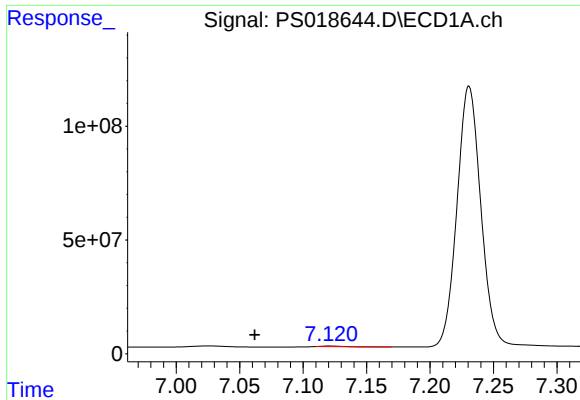

#3 4-Nitrophenol


R.T.: 7.121 min
Delta R.T.: 0.059 min
Response: 1979846
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

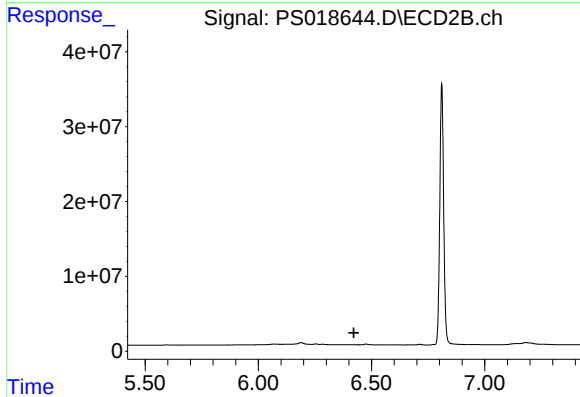


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

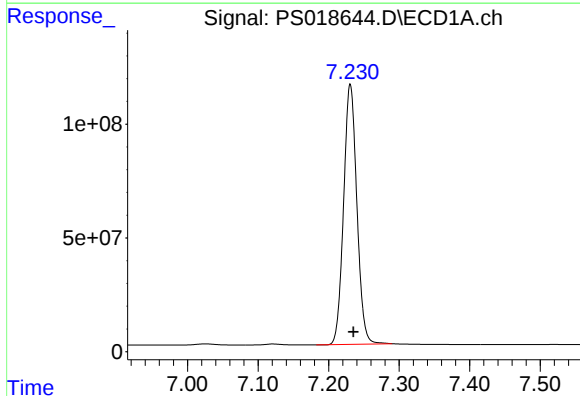


#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: -0.004 min
Response: 1490115852
Conc: 523.60 ng/ml

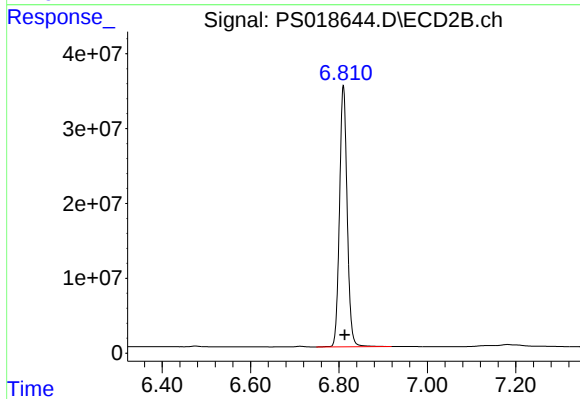

#4 2,4-DCAA


R.T.: 6.810 min
Delta R.T.: -0.003 min
Response: 419104773
Conc: 595.61 ng/ml

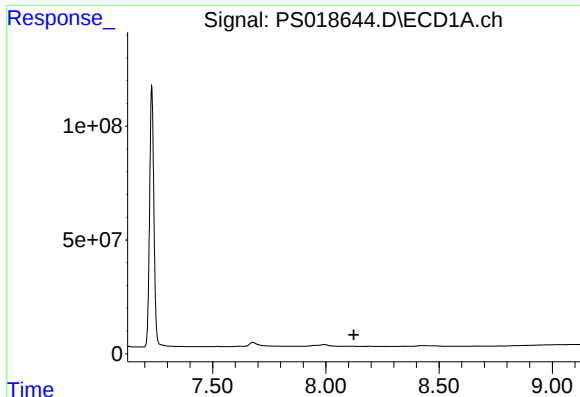

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

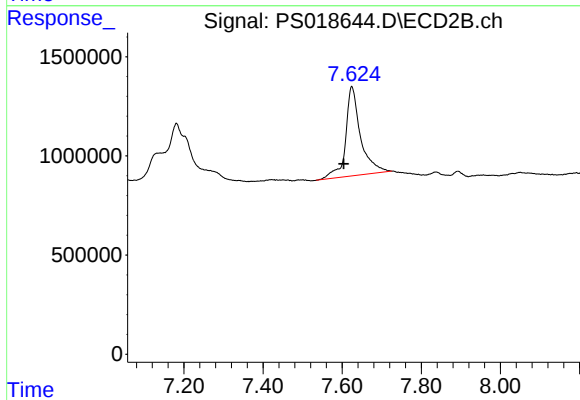


#8 DICHLORPROP

R.T.: 7.624 min
Delta R.T.: 0.020 min
Response: 11781166
Conc: 14.88 ng/ml

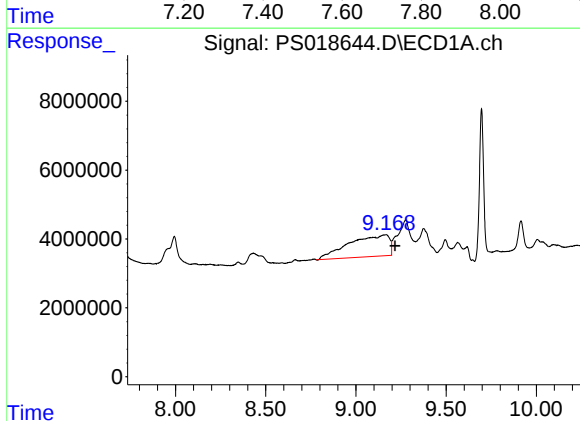


#11 2,4,5-TP (SILVEX)

R.T.: 9.169 min
Delta R.T.: -0.049 min
Response: 97394241
Conc: 6.40 ng/ml

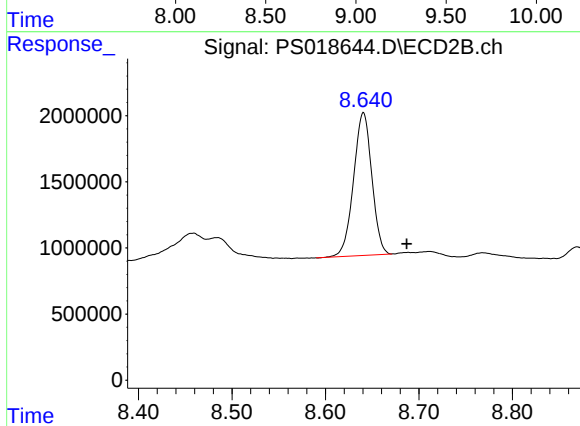

#11 2,4,5-TP (SILVEX)


R.T.: 8.641 min
Delta R.T.: -0.046 min
Response: 14636201
Conc: 3.36 ng/ml

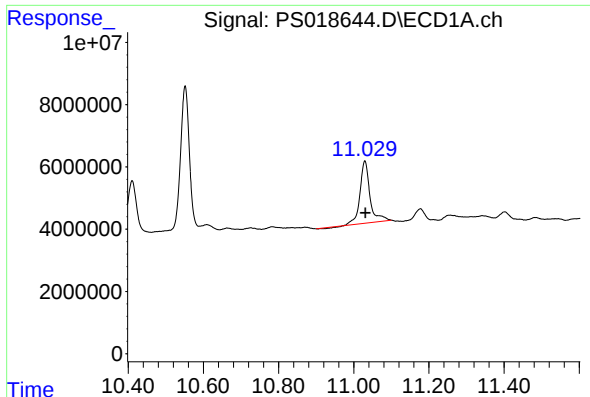

#15 Picloram


R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 36646476
Conc: 1.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

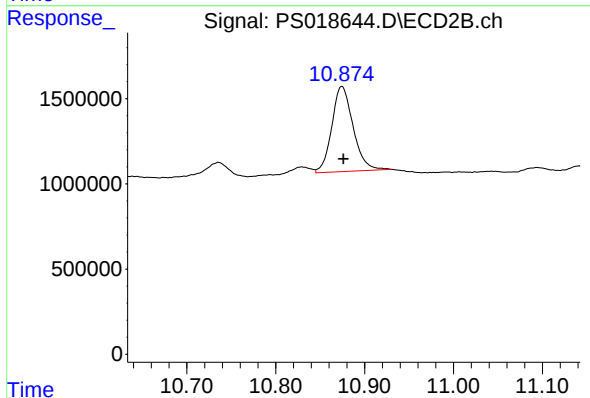


#15 Picloram

R.T.: 10.874 min
Delta R.T.: -0.002 min
Response: 8325563
Conc: 1.57 ng/ml

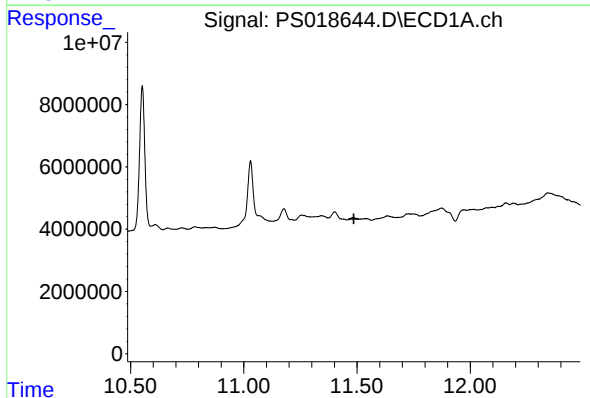

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.486 min
Response: 0
Conc: N.D.

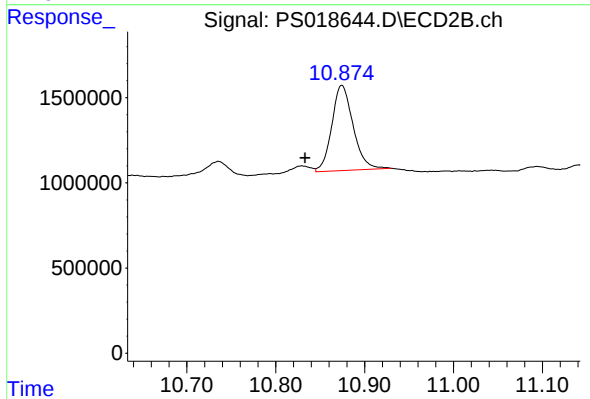

#16 DCPA

R.T.: 10.874 min
Delta R.T.: 0.041 min
Response: 8325563
Conc: 1.58 ng/ml