

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032122\
 Data File : PS018654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2022 20:20
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 01:39:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.810	1513.6E6	425.8E6	531.848	605.157
Target Compounds							
3) T	4-Nitroph...	7.024	6.475f	-317827	1382078	N.D.	3.402
8) T	DICHLORPROP	0.000	7.623	0	14259191	N.D.	18.013
9) T	2,4-D	8.414f	0.000	3245390	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.277f	8.640f	19643359	13064172	1.292	2.995 #
12) T	2,4,5-T	9.494	9.060	10872285	2038087	<MDL	<MDL #
13) T	2,4-DB	10.005f	0.000	110607	0	<MDL	N.D. #
14) T	DINOSEB	11.177f	0.000	2252873	0	<MDL	N.D. #
15) T	Picloram	11.029	10.875	101.9E6	25173396	4.956	4.735
16) T	DCPA	0.000	10.875f	0	25173396	N.D.	4.786



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032122\
Data File : PS018654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2022 20:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 01:39:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

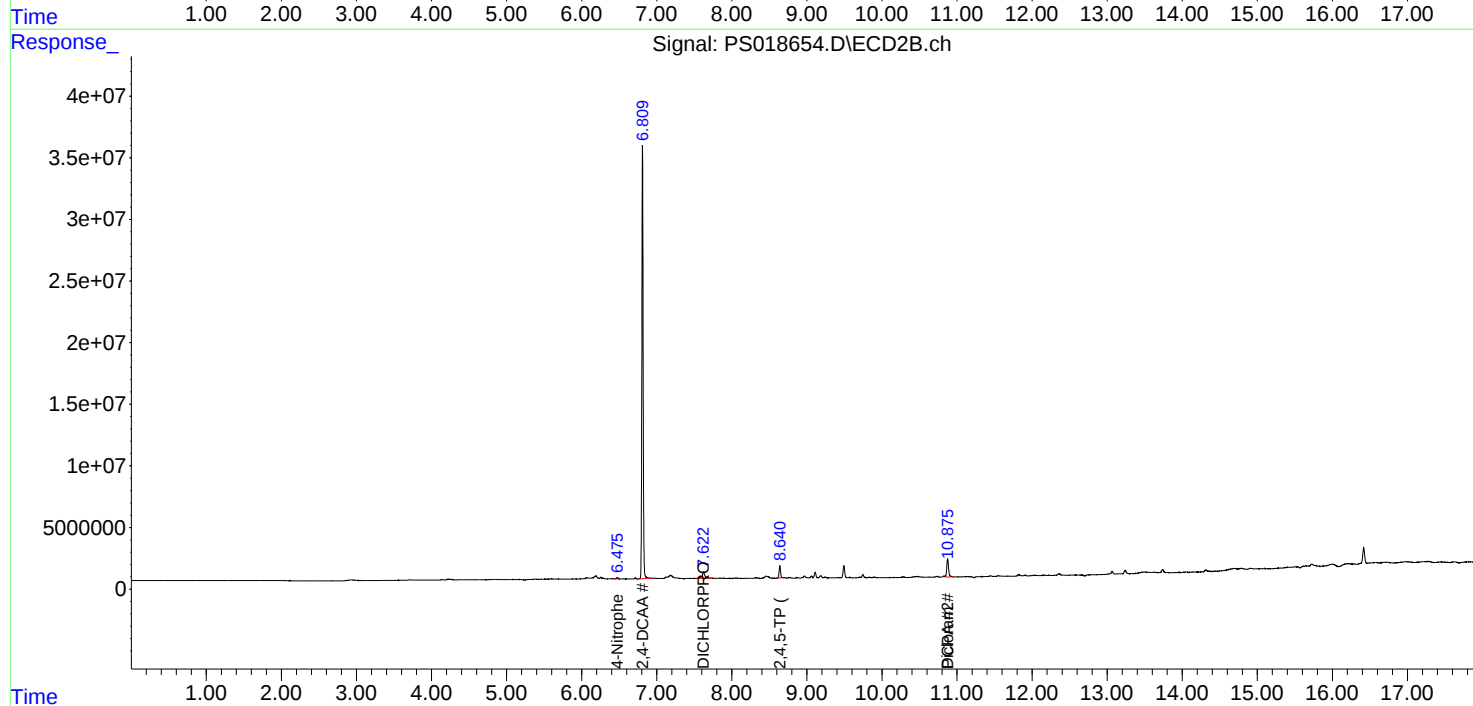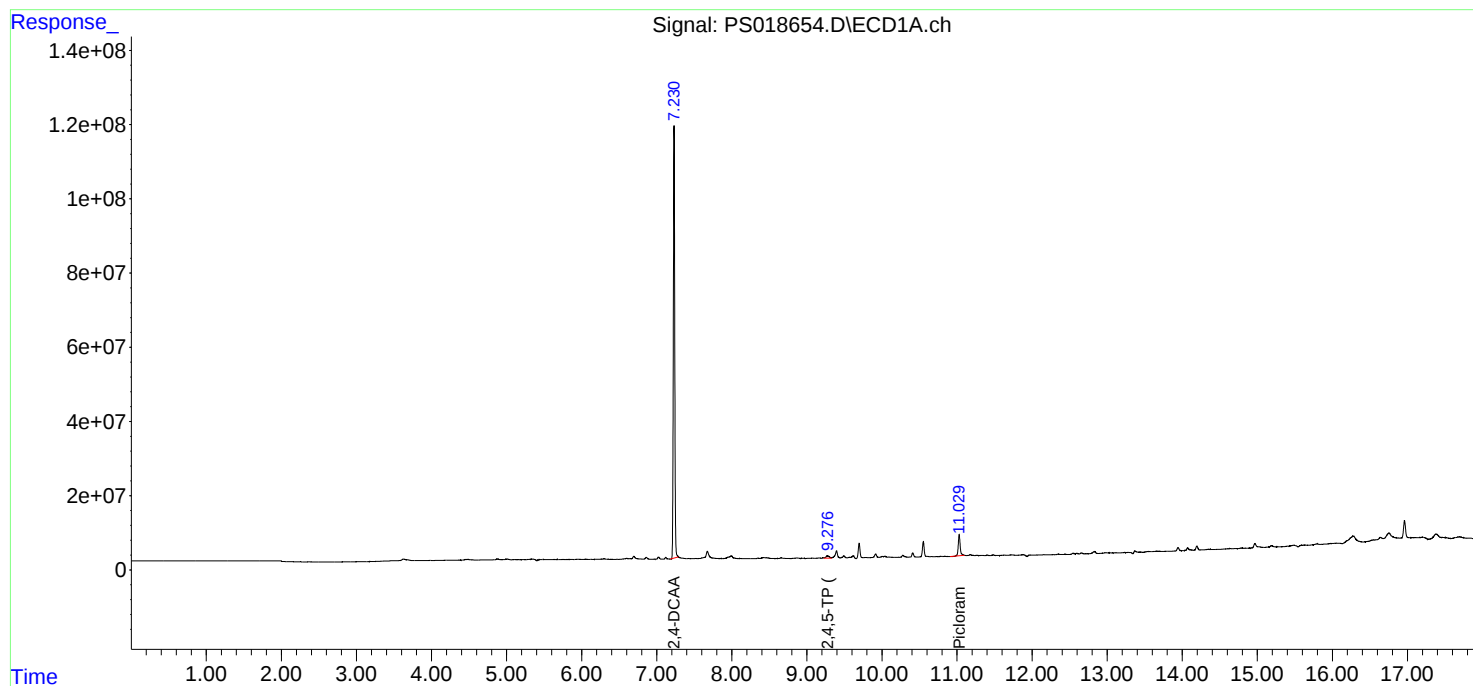


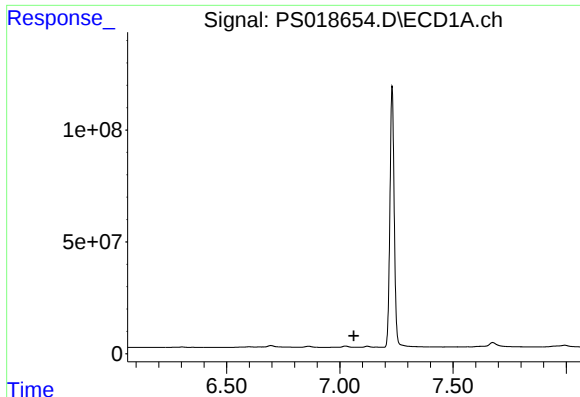

#3 4-Nitrophenol


R.T.: 7.024 min
Delta R.T.: -0.038 min
Response: -317827
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

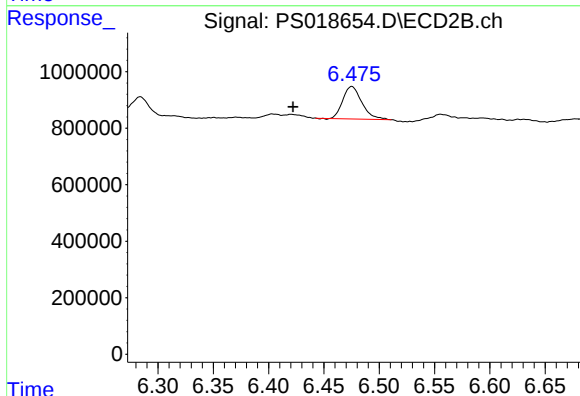


#3 4-Nitrophenol

R.T.: 6.475 min
Delta R.T.: 0.053 min
Response: 1382078
Conc: 3.40 ng/ml

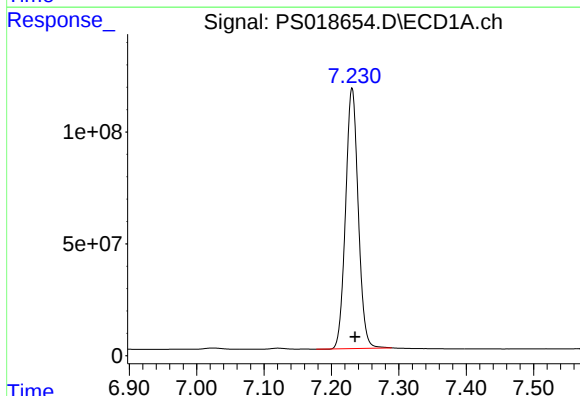


#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: -0.004 min
Response: 1513593734
Conc: 531.85 ng/ml

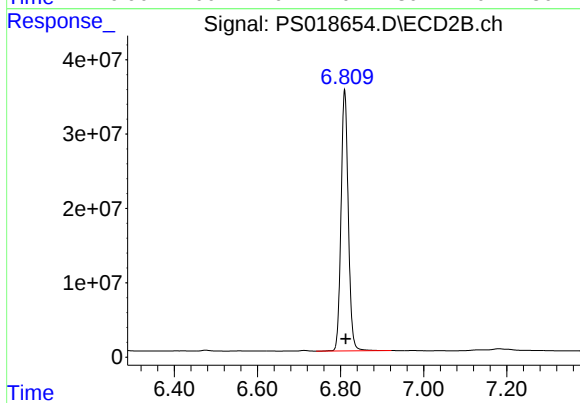

#4 2,4-DCAA


R.T.: 6.810 min
Delta R.T.: -0.003 min
Response: 425821510
Conc: 605.16 ng/ml

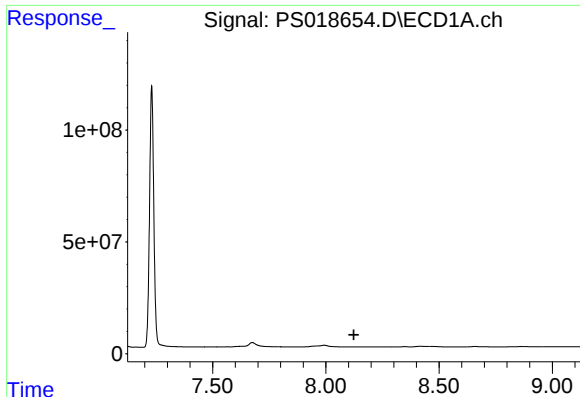

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

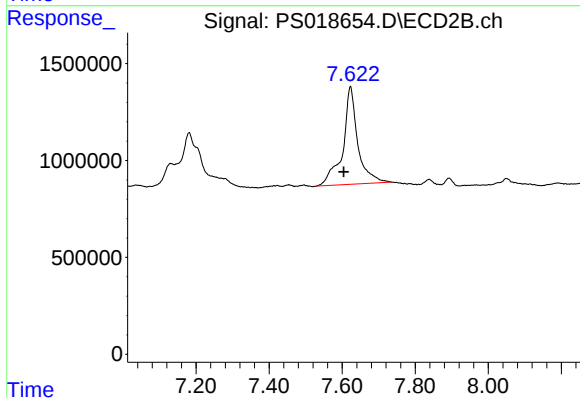


#8 DICHLORPROP

R.T.: 7.623 min
Delta R.T.: 0.019 min
Response: 14259191
Conc: 18.01 ng/ml

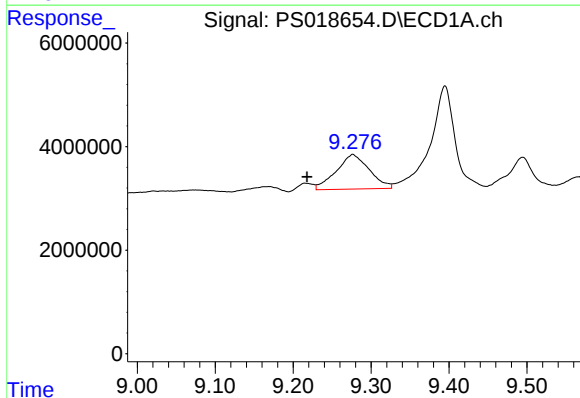


#11 2,4,5-TP (SILVEX)

R.T.: 9.277 min
Delta R.T.: 0.059 min
Response: 19643359
Conc: 1.29 ng/ml

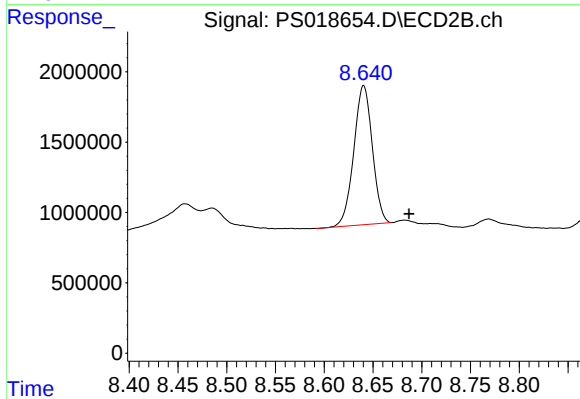

#11 2,4,5-TP (SILVEX)


R.T.: 8.640 min
Delta R.T.: -0.047 min
Response: 13064172
Conc: 2.99 ng/ml

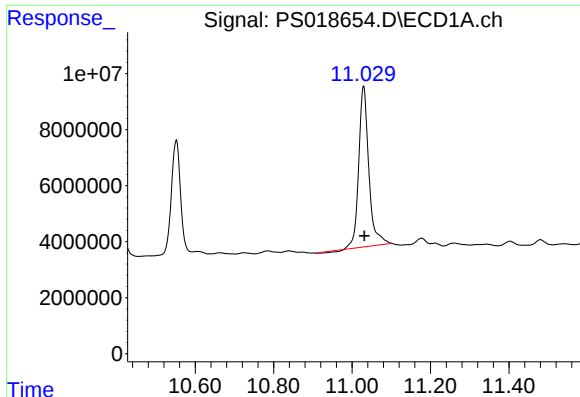

#15 Picloram


R.T.: 11.029 min
Delta R.T.: -0.002 min
Response: 101866992
Conc: 4.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

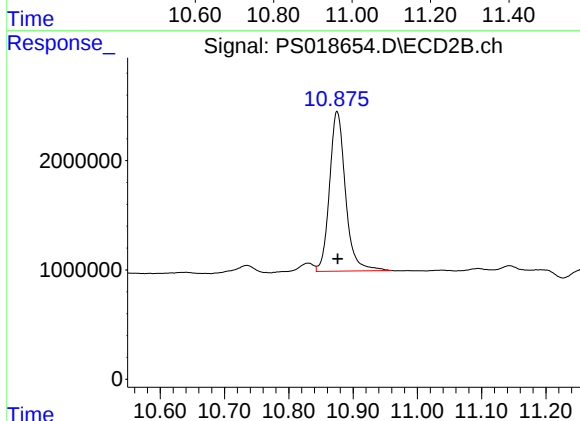


#15 Picloram

R.T.: 10.875 min
Delta R.T.: 0.000 min
Response: 25173396
Conc: 4.74 ng/ml

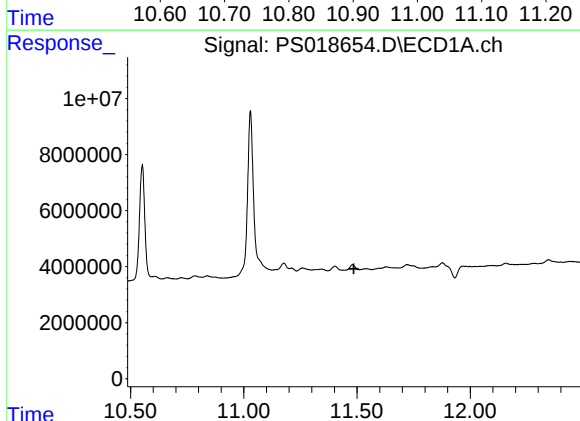

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.486 min
Response: 0
Conc: N.D.

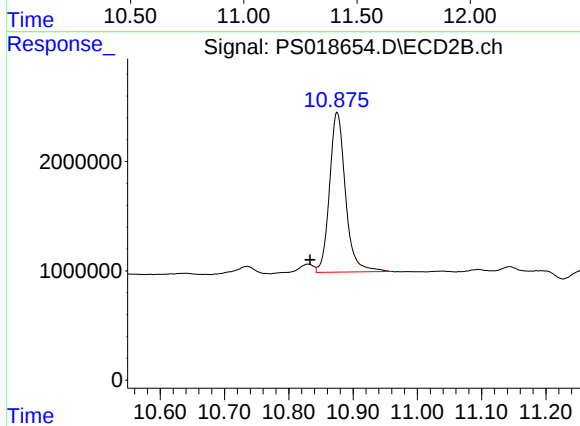

#16 DCPA

R.T.: 10.875 min
Delta R.T.: 0.042 min
Response: 25173396
Conc: 4.79 ng/ml