

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032125\
 Data File : PS029496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2025 17:45
 Operator : AR\AJ
 Sample : Q1592-01MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 23:26:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032025.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 21 04:46:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.150	7.616	159.1E6	9823809	38.460	11.298 #
Target Compounds							
1) T	Dalapon	2.577	2.633	753.3E6	199.1E6	134.294	98.672 #
2) T	3,5-DICHL...	6.336	6.565	175.7E6	36619739	30.198	27.469
3) T	4-Nitroph...	6.953	7.119	151.9E6	70414150	80.532	97.816
5) T	DICAMBA	7.332	7.772	587.7E6	138.8E6	32.775	27.073
6) T	MCPD	7.509	7.903	3586856	7448142	<MDL	3.223 #
7) T	MCPA	7.657	8.138	63180268	7000677	3.665	2.333 #
8) T	DICHLORPROP	8.033	8.509	202.3E6	74674680	43.808	61.700 #
9) T	2,4-D	8.266	8.798	189.5E6	62670583	41.894	52.192
10) T	Pentachlo...	8.553	9.308	3386.4E6	1046.5E6	60.340	45.124 #
11) T	2,4,5-TP ...	9.127	9.683	858.5E6	330.9E6	34.746	36.826
12) T	2,4,5-T	9.421	10.097	842.5E6	228.8E6	33.823	29.355
13) T	2,4-DB	9.993	10.652f	495.1E6	59922022	135.440	79.631 #
14) T	DINOSEB	11.181	11.031	363.7E6	115.5E6	20.896	20.012
15) T	Picloram	11.004	12.099	1102.4E6	294.8E6	36.594	25.975 #
16) T	DCPA	11.475	12.099	2182.9E6	294.8E6	72.872	24.656 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032125\
Data File : PS029496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2025 17:45
Operator : AR\AJ
Sample : Q1592-01MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 23:26:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032025.M
Quant Title : 8080.M
QLast Update : Fri Mar 21 04:46:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

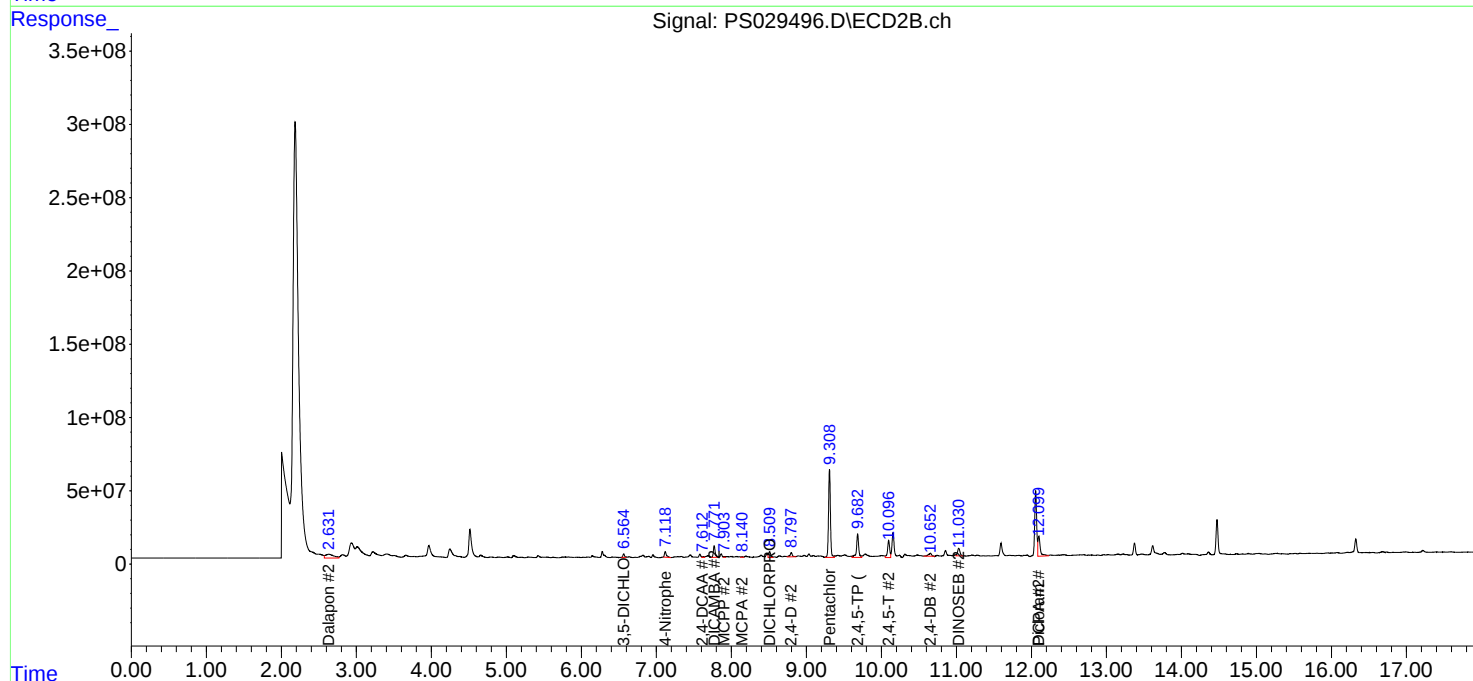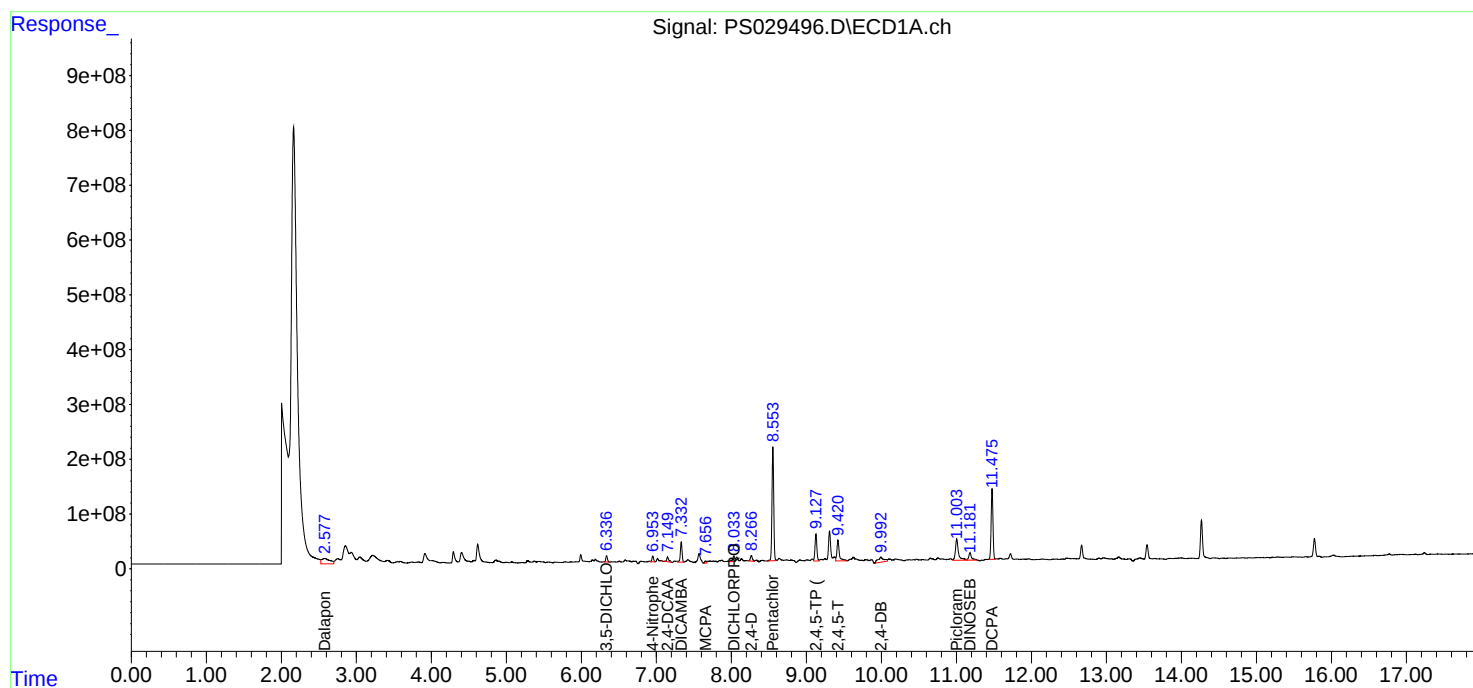


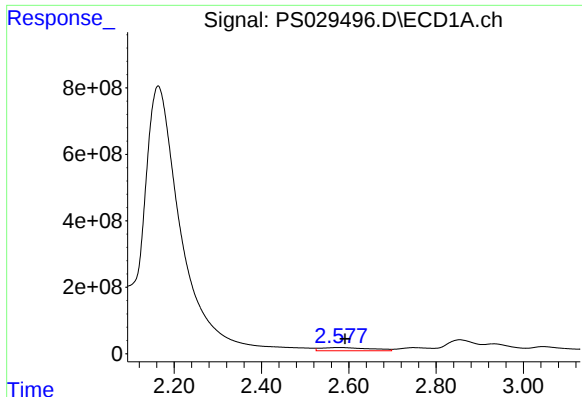

#1 Dalapon


R.T.: 2.577 min
Delta R.T.: -0.014 min
Response: 753322412
Conc: 134.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

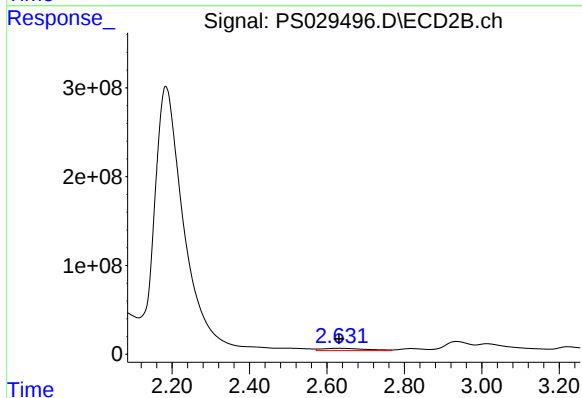


#1 Dalapon

R.T.: 2.633 min
Delta R.T.: 0.001 min
Response: 199145541
Conc: 98.67 ng/ml

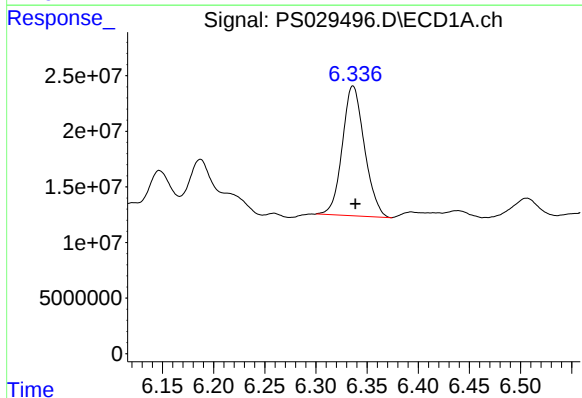


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.336 min
Delta R.T.: -0.002 min
Response: 175701513
Conc: 30.20 ng/ml

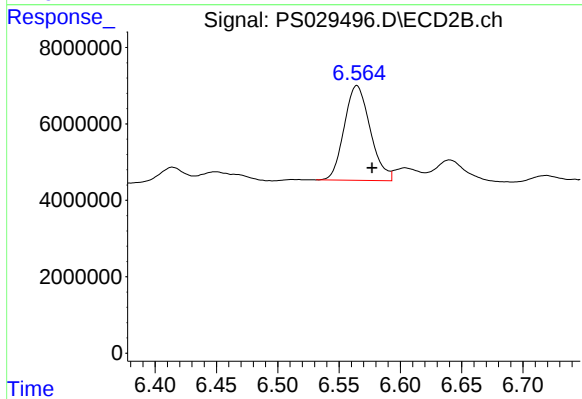

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.565 min
Delta R.T.: -0.012 min
Response: 36619739
Conc: 27.47 ng/ml

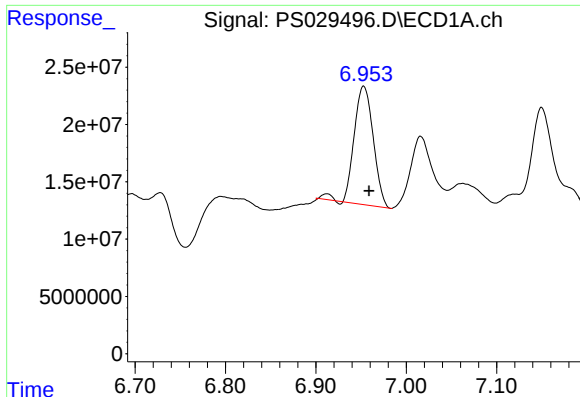

#3 4-Nitrophenol


R.T.: 6.953 min
Delta R.T.: -0.006 min
Response: 151867264
Conc: 80.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

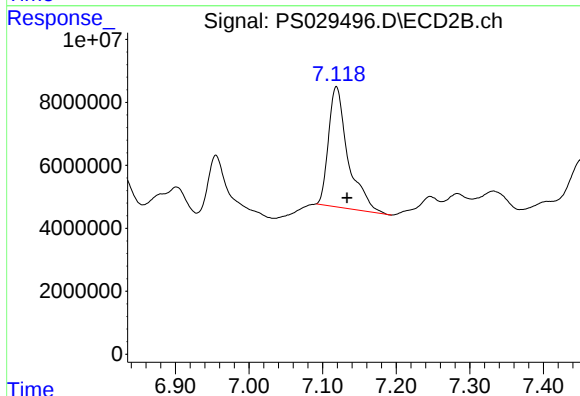


#3 4-Nitrophenol

R.T.: 7.119 min
Delta R.T.: -0.015 min
Response: 70414150
Conc: 97.82 ng/ml

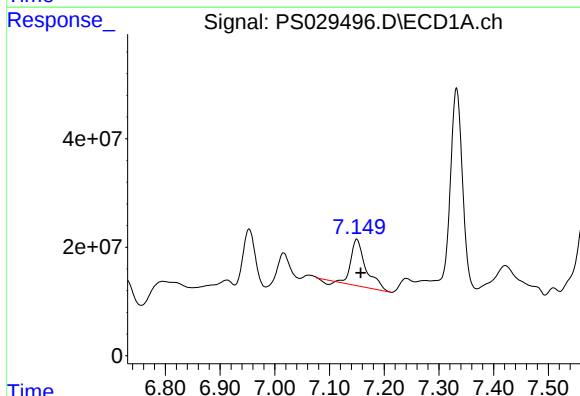


#4 2,4-DCAA

R.T.: 7.150 min
Delta R.T.: -0.007 min
Response: 159147703
Conc: 38.46 ng/ml

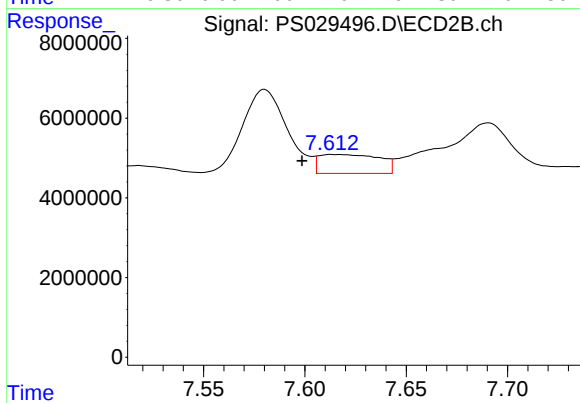

#4 2,4-DCAA


R.T.: 7.616 min
Delta R.T.: 0.017 min
Response: 9823809
Conc: 11.30 ng/ml

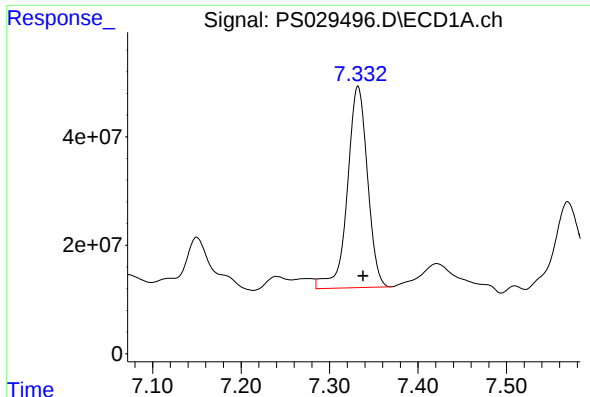

#5 DICAMBA


R.T.: 7.332 min
Delta R.T.: -0.006 min
Response: 587742143
Conc: 32.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

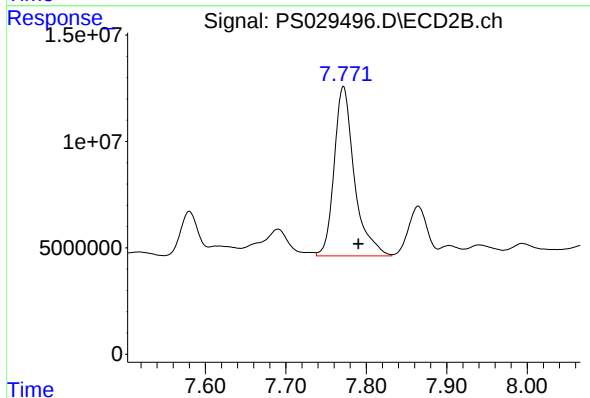


#5 DICAMBA

R.T.: 7.772 min
Delta R.T.: -0.019 min
Response: 138763201
Conc: 27.07 ng/ml

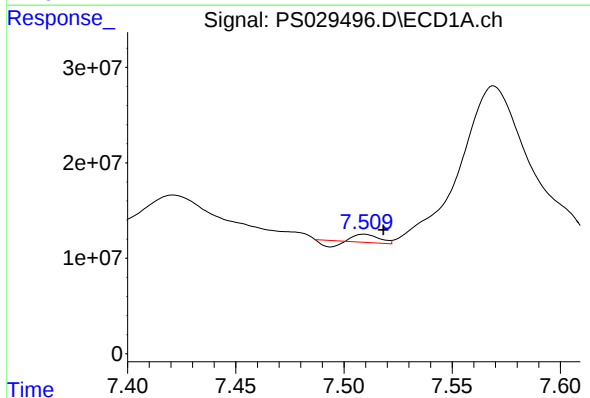


#6 MCP

R.T.: 7.509 min
Delta R.T.: -0.009 min
Response: 3586856
Conc: N.D.

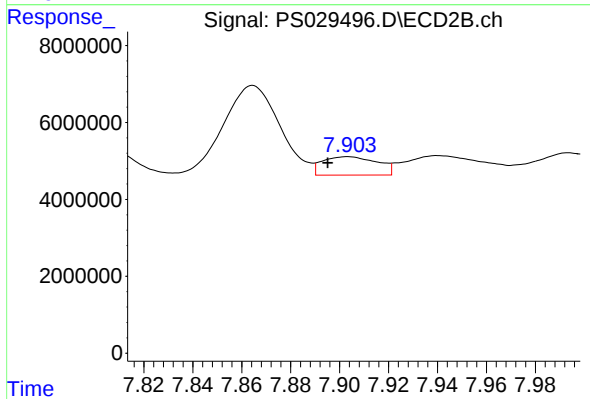

#6 MCP


R.T.: 7.903 min
Delta R.T.: 0.008 min
Response: 7448142
Conc: 3.22 ug/ml

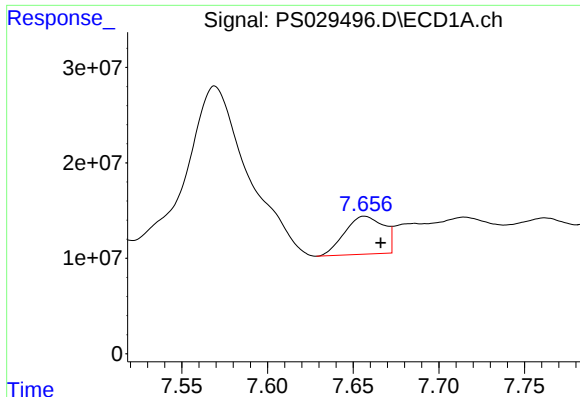

#7 MCPA


R.T.: 7.657 min
Delta R.T.: -0.009 min
Response: 63180268
Conc: 3.67 ug/ml

Instrument :
ECD_S
ClientSampleId :

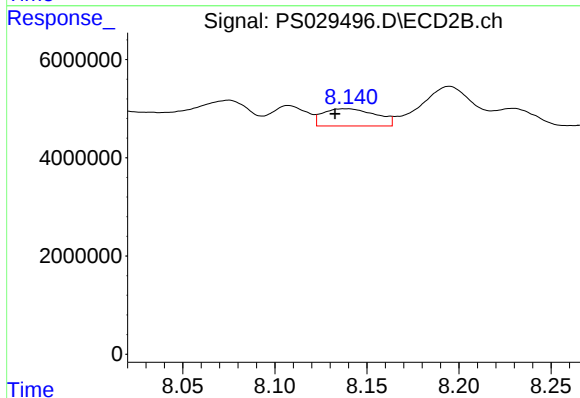


#7 MCPA

R.T.: 8.138 min
Delta R.T.: 0.006 min
Response: 7000677
Conc: 2.33 ug/ml

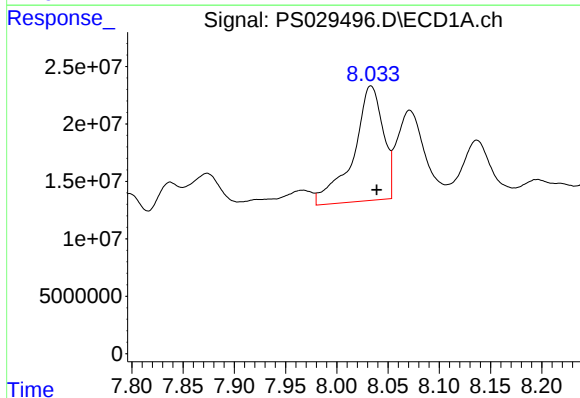


#8 DICHLORPROP

R.T.: 8.033 min
Delta R.T.: -0.005 min
Response: 202288009
Conc: 43.81 ng/ml

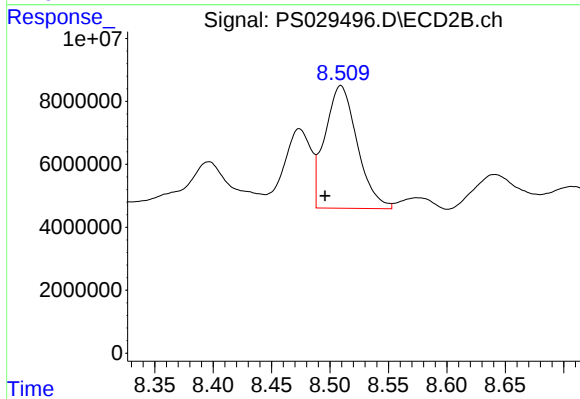

#8 DICHLORPROP


R.T.: 8.509 min
Delta R.T.: 0.013 min
Response: 74674680
Conc: 61.70 ng/ml

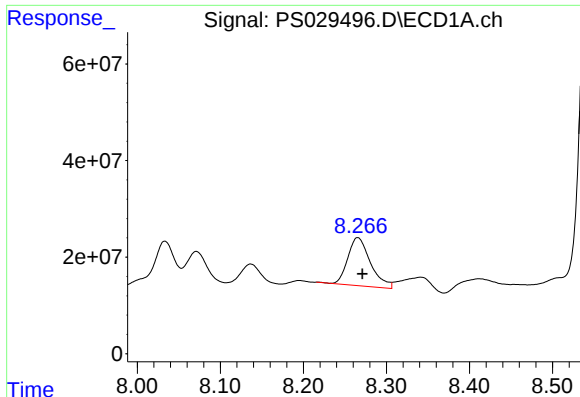

#9 2,4-D


R.T.: 8.266 min
Delta R.T.: -0.005 min
Response: 189508463
Conc: 41.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

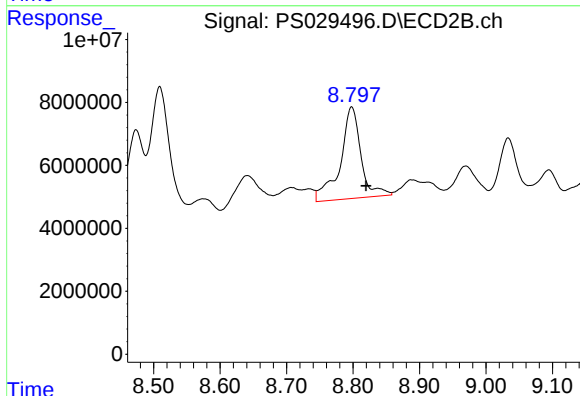


#9 2,4-D

R.T.: 8.798 min
Delta R.T.: -0.022 min
Response: 62670583
Conc: 52.19 ng/ml

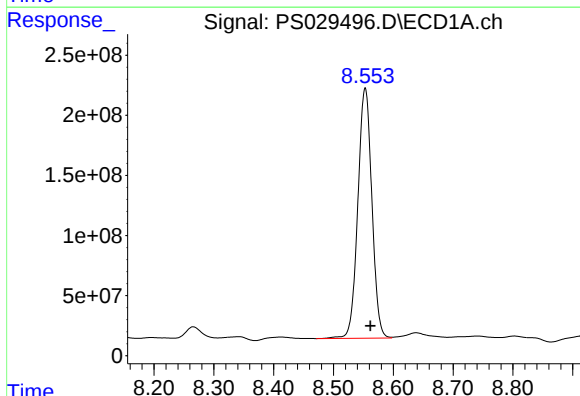


#10 Pentachlorophenol

R.T.: 8.553 min
Delta R.T.: -0.009 min
Response: 3386404699
Conc: 60.34 ng/ml

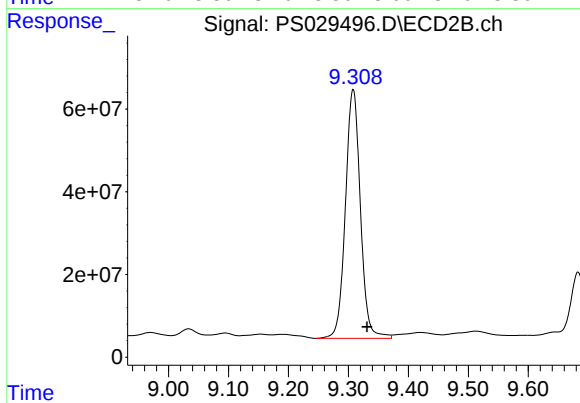

#10 Pentachlorophenol


R.T.: 9.308 min
Delta R.T.: -0.023 min
Response: 1046536098
Conc: 45.12 ng/ml

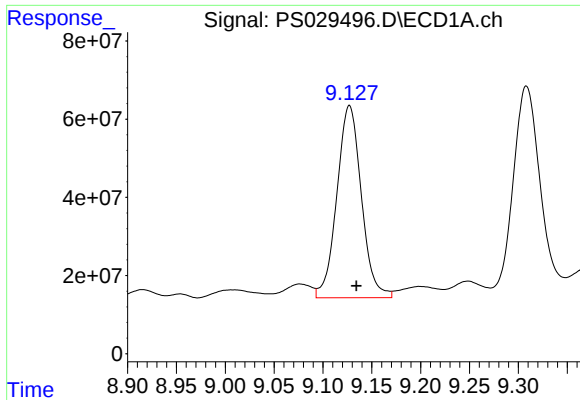

#11 2,4,5-TP (SILVEX)


R.T.: 9.127 min
Delta R.T.: -0.007 min
Response: 858489604
Conc: 34.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

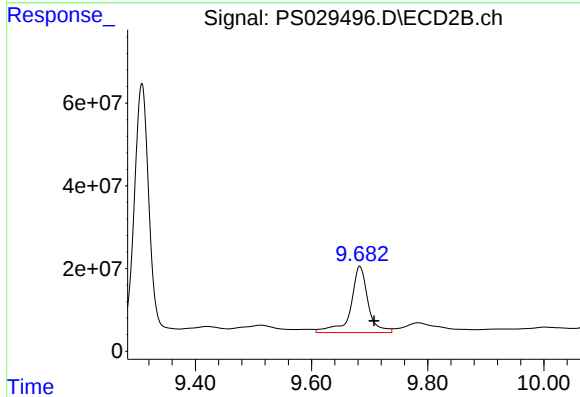


#11 2,4,5-TP (SILVEX)

R.T.: 9.683 min
Delta R.T.: -0.024 min
Response: 330856105
Conc: 36.83 ng/ml

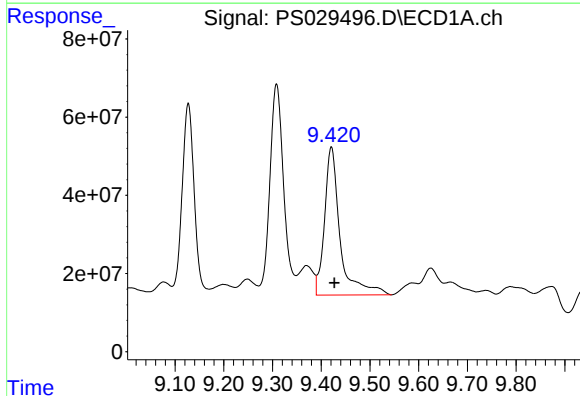


#12 2,4,5-T

R.T.: 9.421 min
Delta R.T.: -0.006 min
Response: 842460208
Conc: 33.82 ng/ml

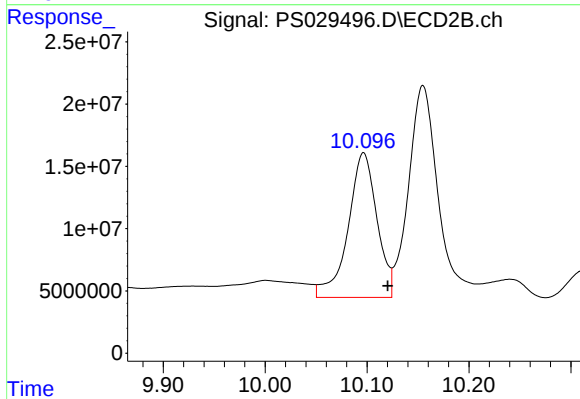

#12 2,4,5-T


R.T.: 10.097 min
Delta R.T.: -0.024 min
Response: 228807082
Conc: 29.35 ng/ml

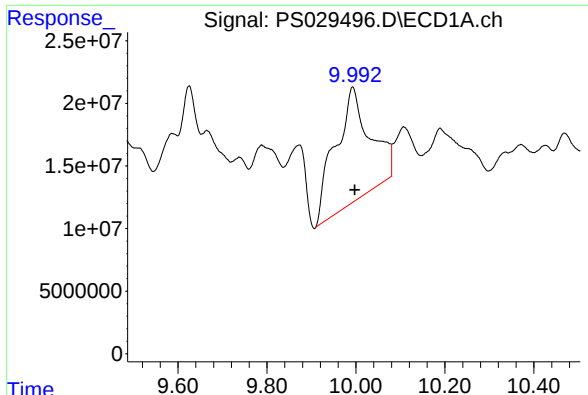

#13 2,4-DB


R.T.: 9.993 min
Delta R.T.: -0.004 min
Response: 495093533
Conc: 135.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

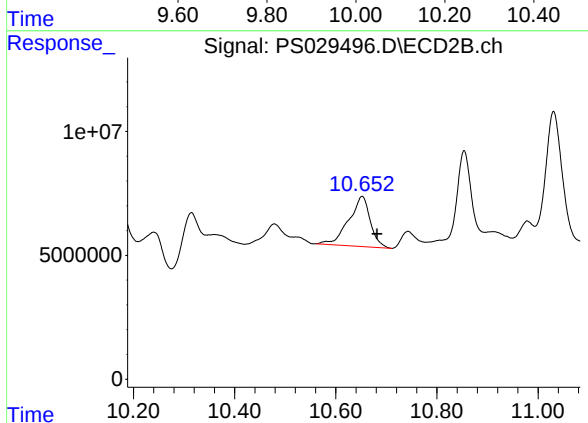


#13 2,4-DB

R.T.: 10.652 min
Delta R.T.: -0.029 min
Response: 59922022
Conc: 79.63 ng/ml

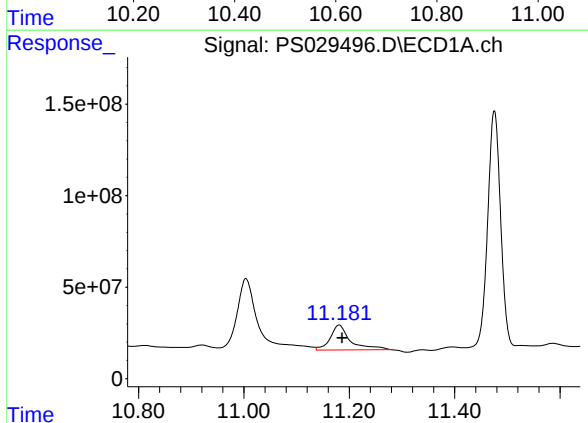


#14 DINOSEB

R.T.: 11.181 min
Delta R.T.: -0.006 min
Response: 363744305
Conc: 20.90 ng/ml

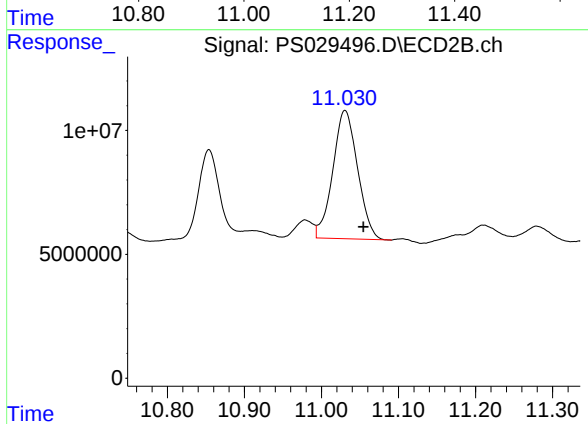

#14 DINOSEB


R.T.: 11.031 min
Delta R.T.: -0.024 min
Response: 115506748
Conc: 20.01 ng/ml

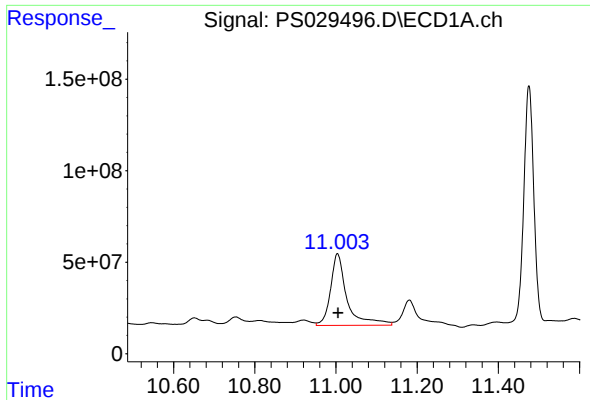

#15 Picloram


R.T.: 11.004 min
Delta R.T.: -0.002 min
Response: 1102374702
Conc: 36.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

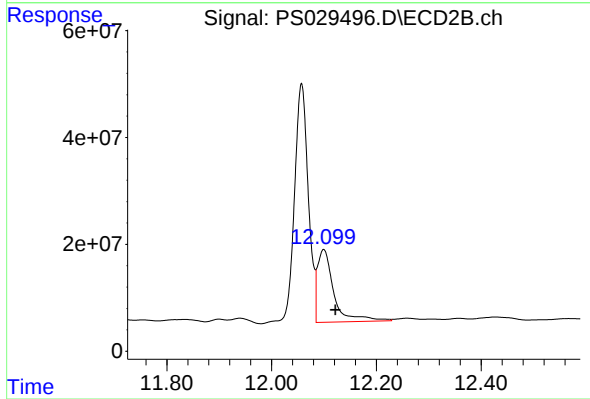


#15 Picloram

R.T.: 12.099 min
Delta R.T.: -0.022 min
Response: 294791565
Conc: 25.98 ng/ml

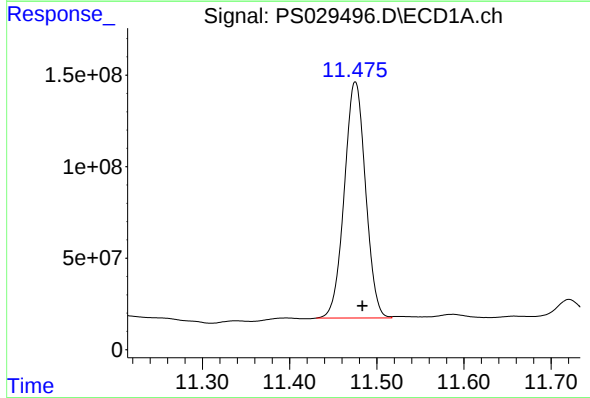

#16 DCPA

R.T.: 11.475 min
Delta R.T.: -0.008 min
Response: 2182940295
Conc: 72.87 ng/ml

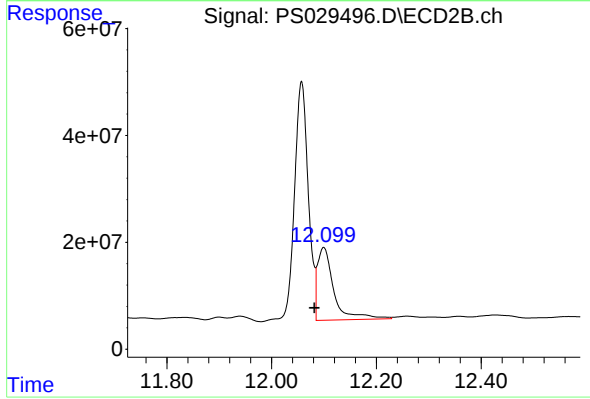

#16 DCPA

R.T.: 12.099 min
Delta R.T.: 0.018 min
Response: 294791565
Conc: 24.66 ng/ml