

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032219\
 Data File : PS003688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 08:33
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 15:39:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.786	0	17554129	N.D.	37.383 #
Target Compounds							
5) T	DICAMBA	0.000	11.122	0	497736	N.D.	0.298 #
6) T	MCPD	0.000	11.351	0	36234	N.D.	0.031 #
9) T	2,4-D	0.000	12.652	0	61093	N.D.	0.116 #
10) T	Pentachlo...	0.000	13.179	0	223024	N.D.	0.034 #
11) T	2,4,5-TP ...	0.000	13.807	0	313028	N.D.	0.123 #
12) T	2,4,5-T	0.000	14.397	0	1589262	N.D.	0.788 #
13) T	2,4-DB	0.000	15.046	0	46017	N.D.	0.180 #
14) T	DINOSEB	0.000	15.450	0	601957	N.D.	0.337 #
15) T	Picloram	16.756	16.687	8893511	5839787	3.613	2.301 #
16) T	DCPA	0.000	16.636	0	1605865	N.D.	0.516 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032219\
Data File : PS003688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 08:33
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 15:39:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

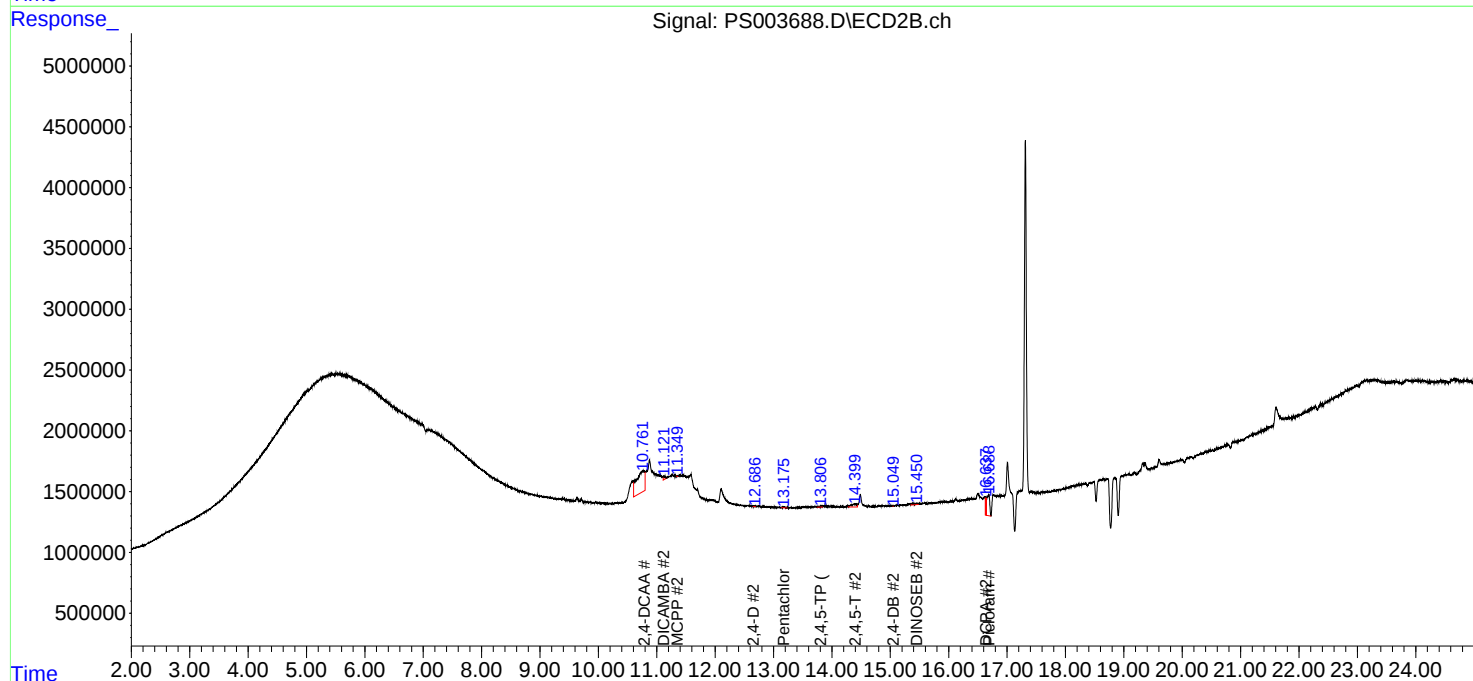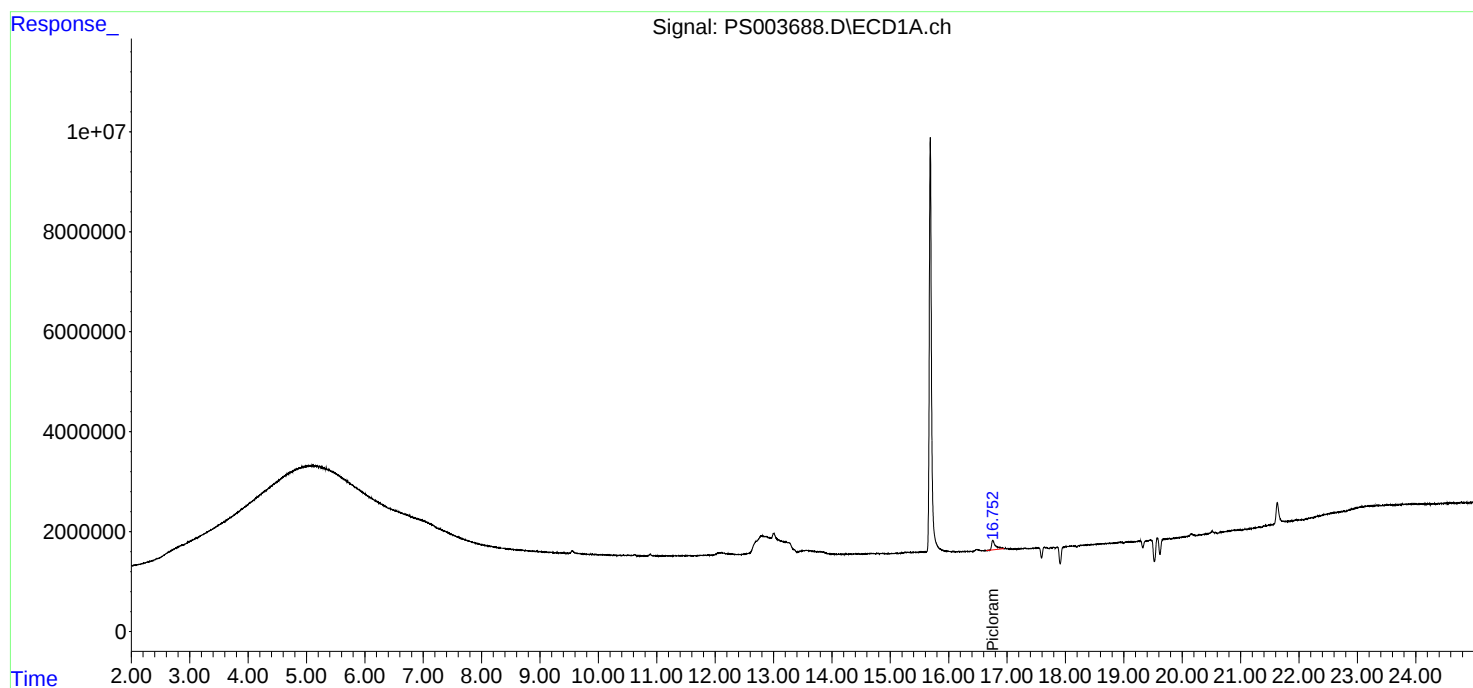


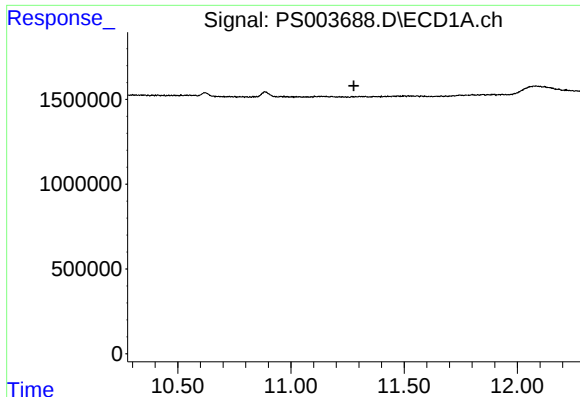

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

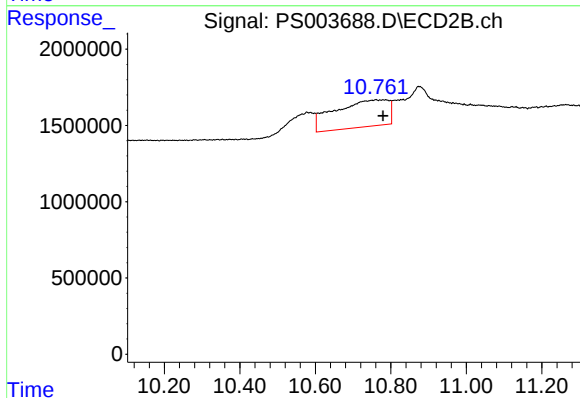


#4 2,4-DCAA

R.T.: 10.786 min
Delta R.T.: 0.007 min
Response: 17554129
Conc: 37.38 ng/ml

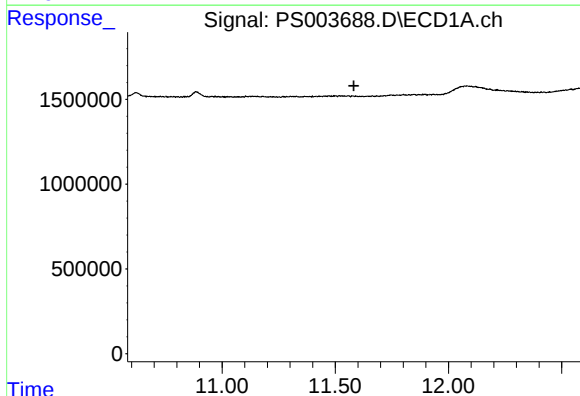


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

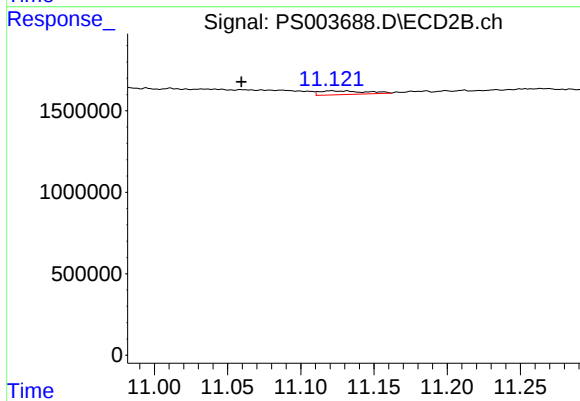

#5 DICAMBA


R.T.: 11.122 min
Delta R.T.: 0.062 min
Response: 497736
Conc: 0.30 ng/ml

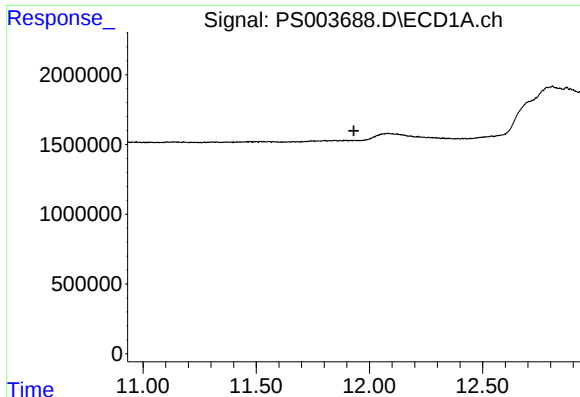

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

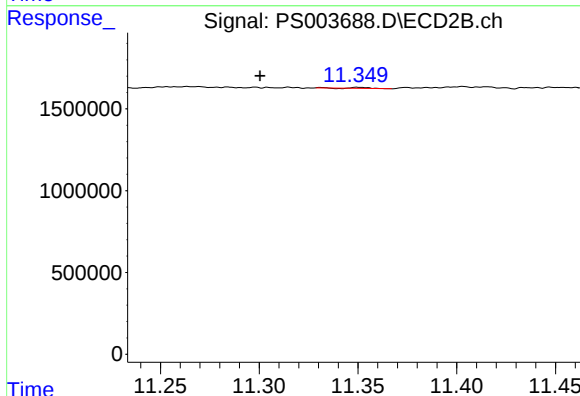


#6 MCPP

R.T.: 11.351 min
Delta R.T.: 0.050 min
Response: 36234
Conc: 0.03 ug/ml

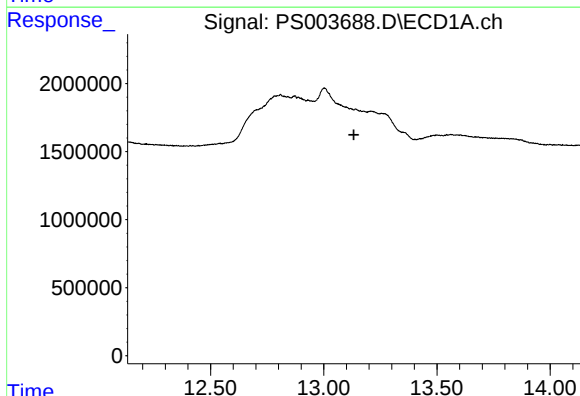


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

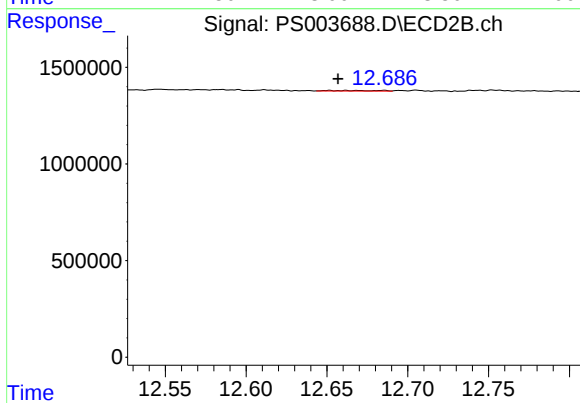

#9 2,4-D


R.T.: 12.652 min
Delta R.T.: -0.005 min
Response: 61093
Conc: 0.12 ng/ml

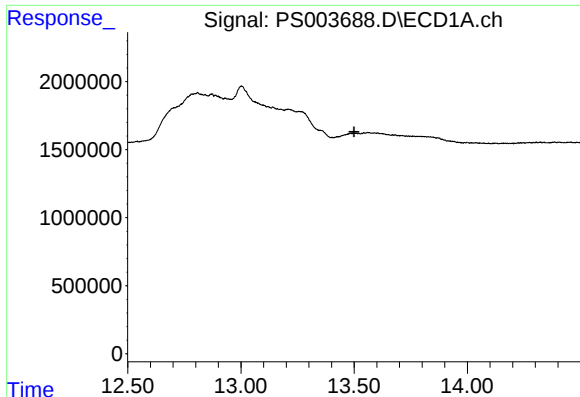

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

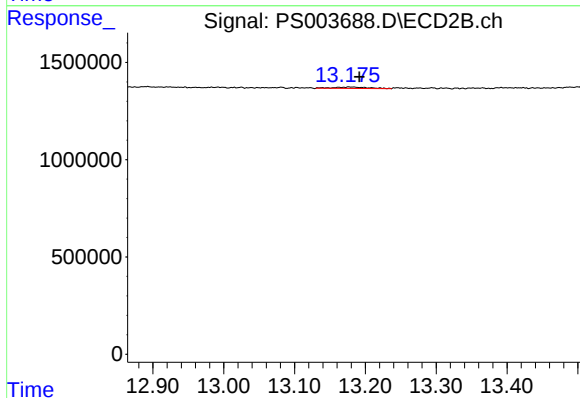


#10 Pentachlorophenol

R.T.: 13.179 min
Delta R.T.: -0.013 min
Response: 223024
Conc: 0.03 ng/ml

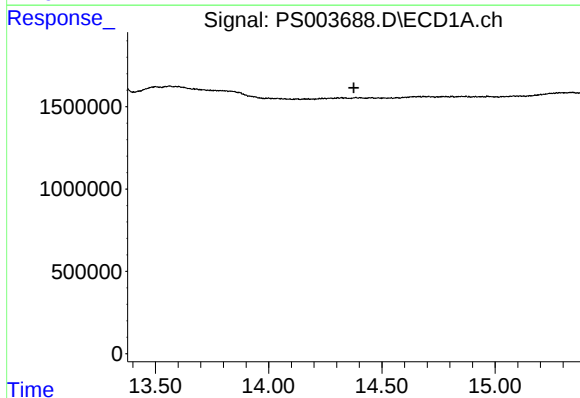


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

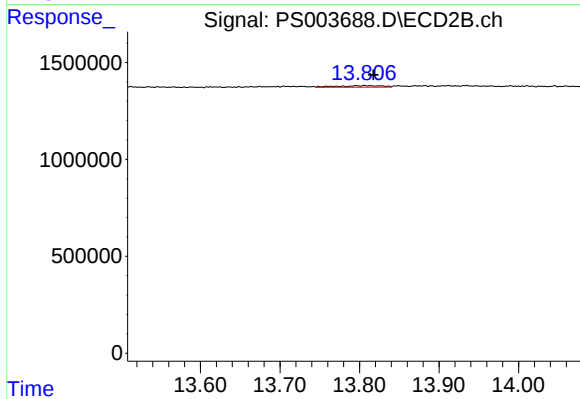

#11 2,4,5-TP (SILVEX)


R.T.: 13.807 min
Delta R.T.: -0.010 min
Response: 313028
Conc: 0.12 ng/ml

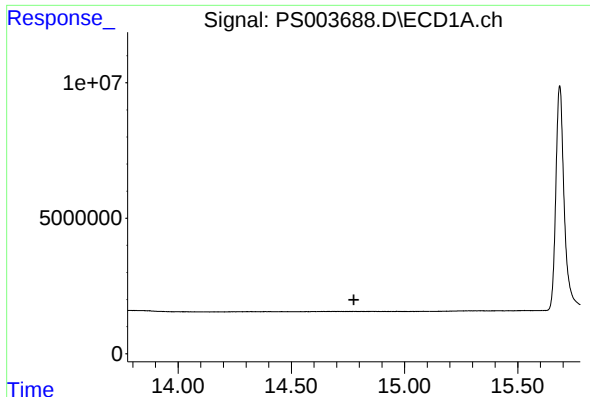

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

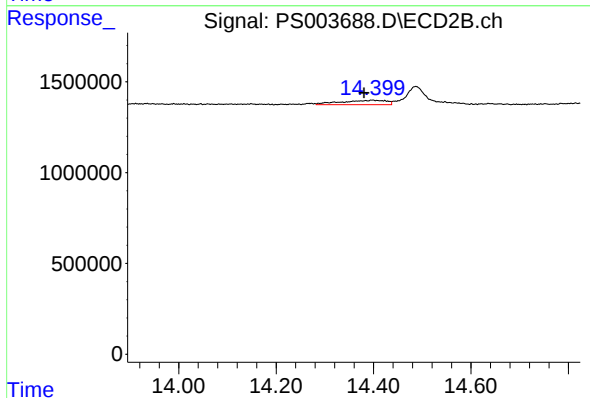


#12 2,4,5-T

R.T.: 14.397 min
Delta R.T.: 0.017 min
Response: 1589262
Conc: 0.79 ng/ml

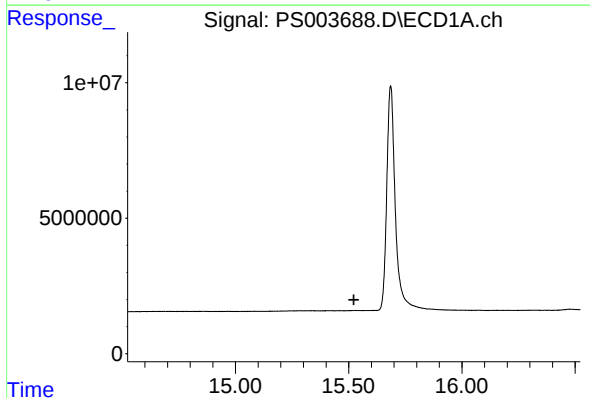


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

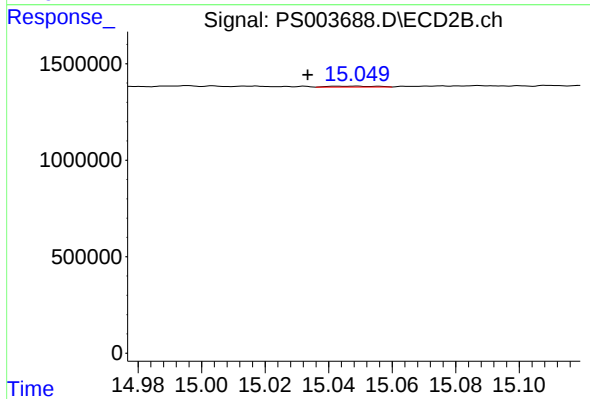

#13 2,4-DB


R.T.: 15.046 min
Delta R.T.: 0.013 min
Response: 46017
Conc: 0.18 ng/ml

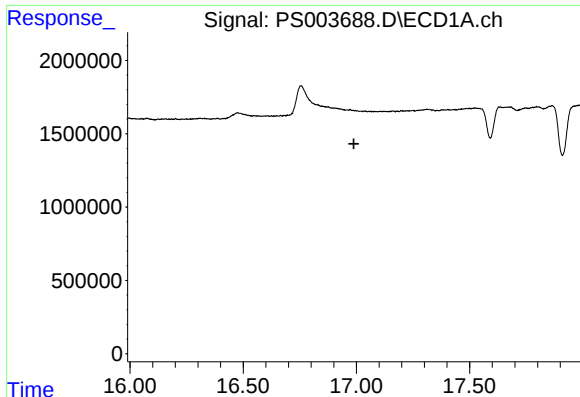

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

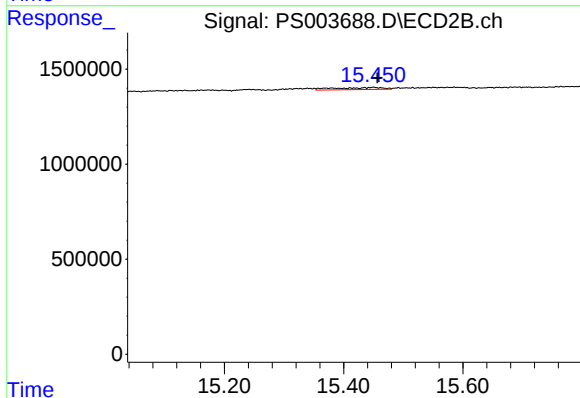


#14 DINOSEB

R.T.: 15.450 min
Delta R.T.: -0.007 min
Response: 601957
Conc: 0.34 ng/ml

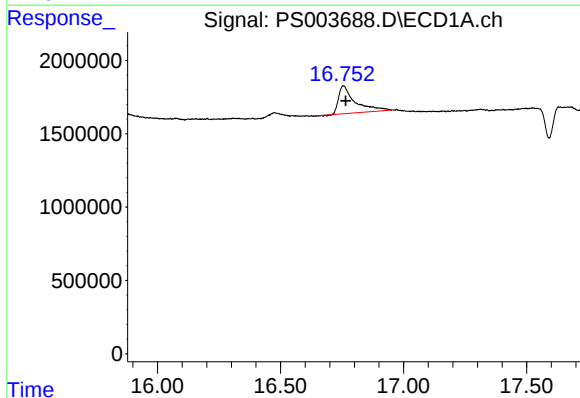


#15 Picloram

R.T.: 16.756 min
Delta R.T.: -0.010 min
Response: 8893511
Conc: 3.61 ng/ml

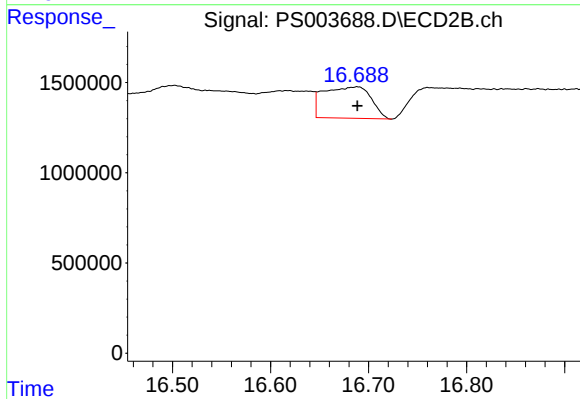

#15 Picloram


R.T.: 16.687 min
Delta R.T.: 0.000 min
Response: 5839787
Conc: 2.30 ng/ml

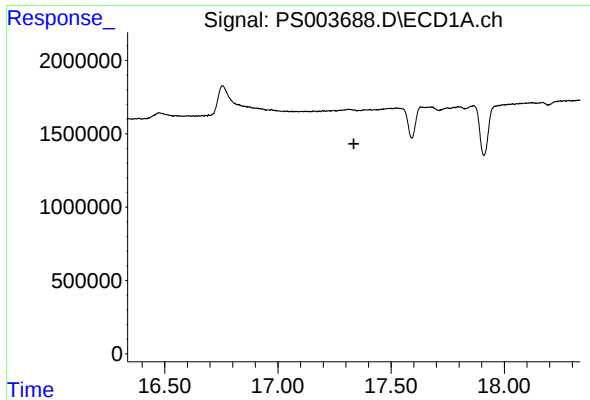

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

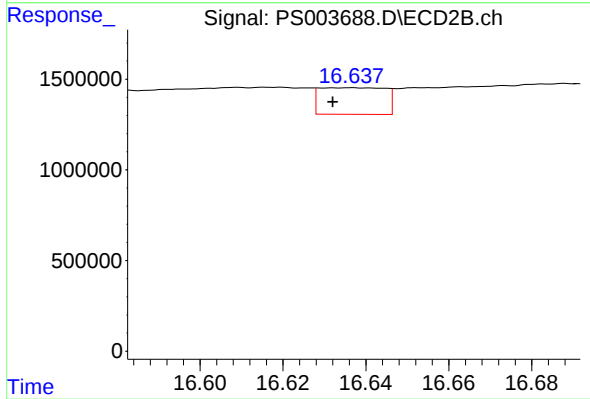

#16 DCPA

R.T.: 16.636 min
Delta R.T.: 0.004 min
Response: 1605865
Conc: 0.52 ng/ml