

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032219\
 Data File : PS003689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 09:04
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 15:40:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.289	10.789	251.3E6	217.6E6	572.329	463.382
Target Compounds							
7) T	MCPA	0.000	11.680	0	332914	N.D.	0.193 #
8) T	DICHLORPROP	0.000	12.135	0	13051556	N.D.	31.583 #
10) T	Pentachlo...	0.000	13.198	0	649722	N.D.	0.099 #
11) T	2,4,5-TP ...	0.000	13.797	0	189514	N.D.	0.074 #
12) T	2,4,5-T	0.000	14.388	0	96904	N.D.	0.048 #
13) T	2,4-DB	0.000	14.987	0	1160350	N.D.	4.544 #
14) T	DINOSEB	0.000	15.463	0	1198170	N.D.	0.671 #
15) T	Picloram	16.758	16.638	27794453	19689376	11.293	7.757 #
16) T	DCPA	0.000	16.638	0	19689376	N.D.	6.330 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032219\
Data File : PS003689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 09:04
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 15:40:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

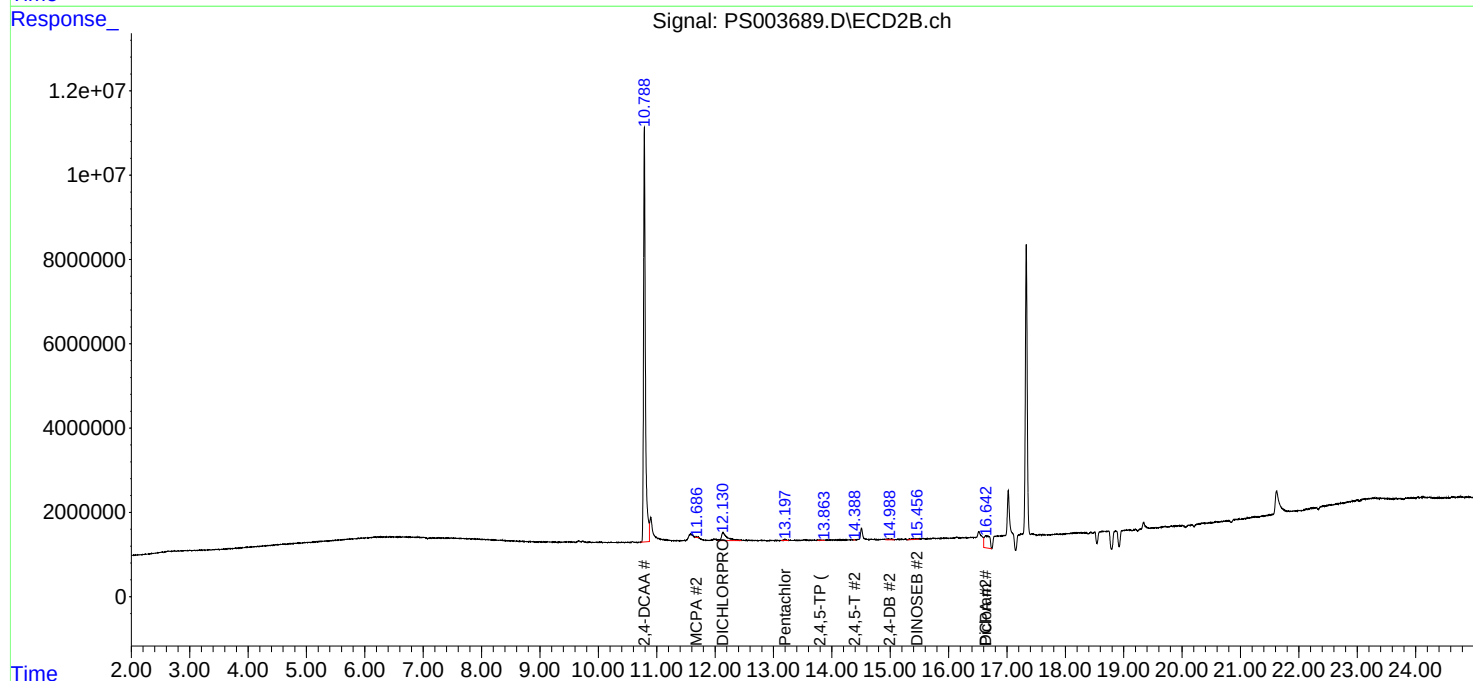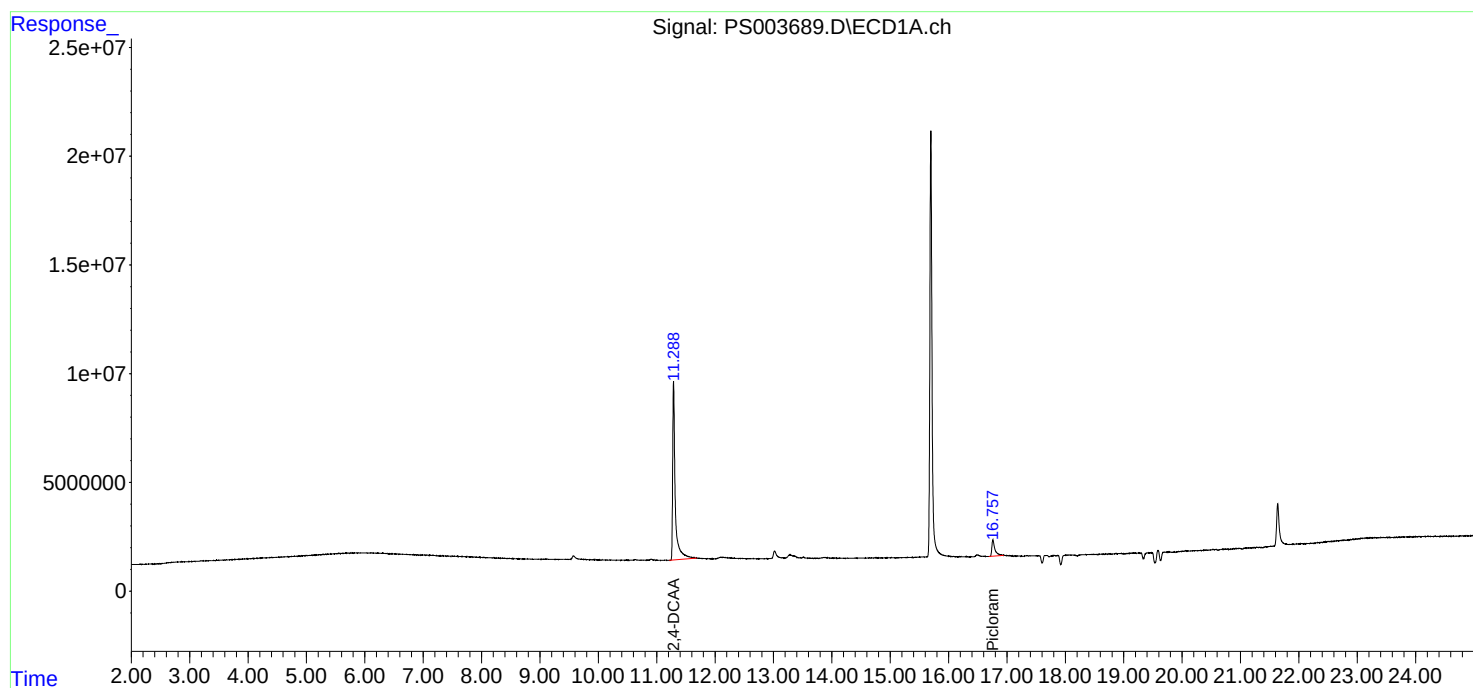


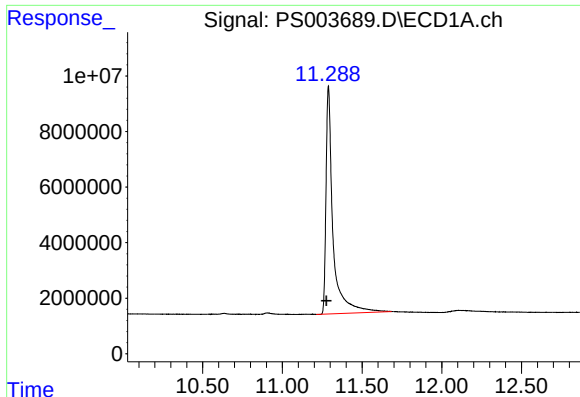

#4 2,4-DCAA


R.T.: 11.289 min
Delta R.T.: 0.011 min
Response: 251266488
Conc: 572.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

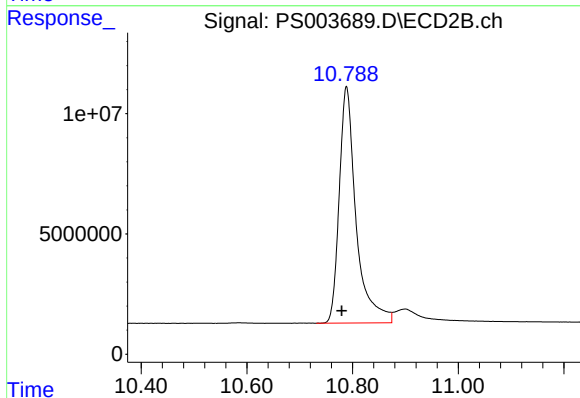


#4 2,4-DCAA

R.T.: 10.789 min
Delta R.T.: 0.009 min
Response: 217589787
Conc: 463.38 ng/ml

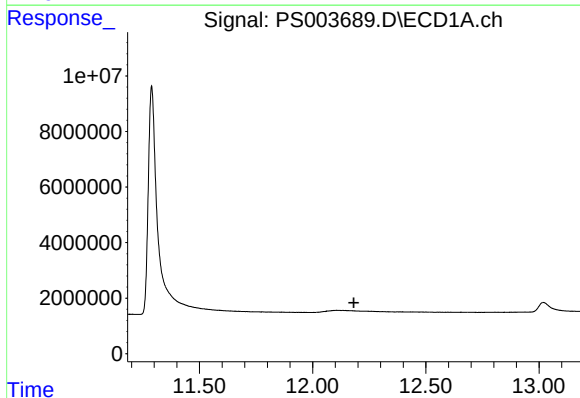


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

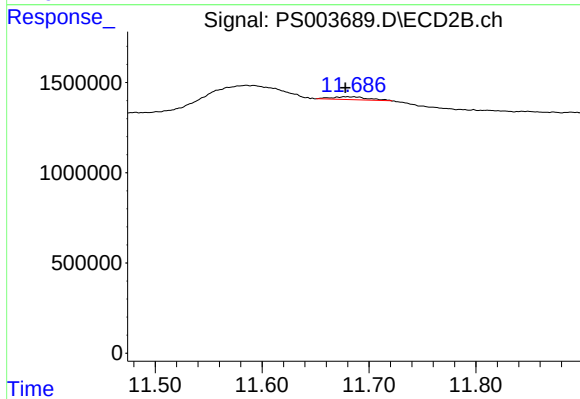

#7 MCPA


R.T.: 11.680 min
Delta R.T.: 0.002 min
Response: 332914
Conc: 0.19 ug/ml

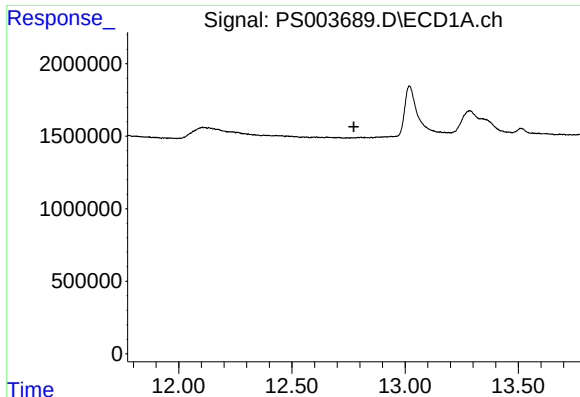

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

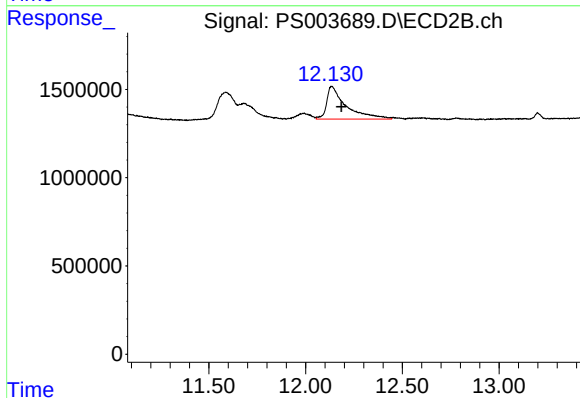


#8 DICHLORPROP

R.T.: 12.135 min
Delta R.T.: -0.050 min
Response: 13051556
Conc: 31.58 ng/ml

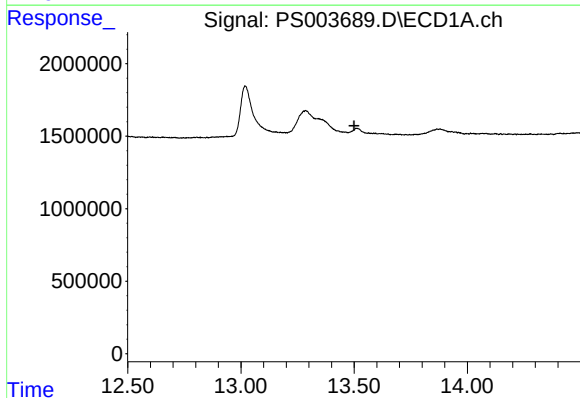


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

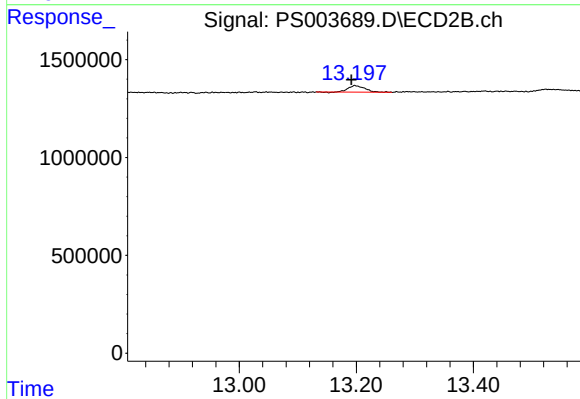

#10 Pentachlorophenol


R.T.: 13.198 min
Delta R.T.: 0.007 min
Response: 649722
Conc: 0.10 ng/ml

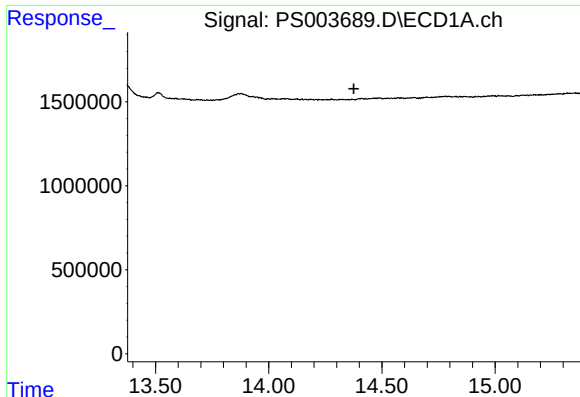

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

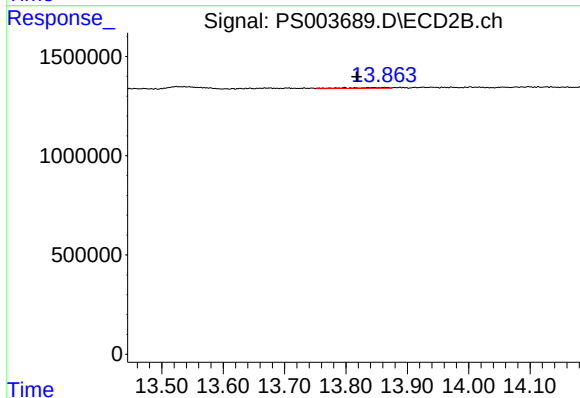


#11 2,4,5-TP (SILVEX)

R.T.: 13.797 min
Delta R.T.: -0.020 min
Response: 189514
Conc: 0.07 ng/ml

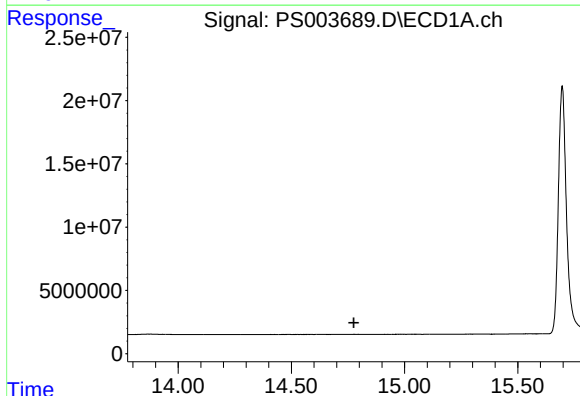


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

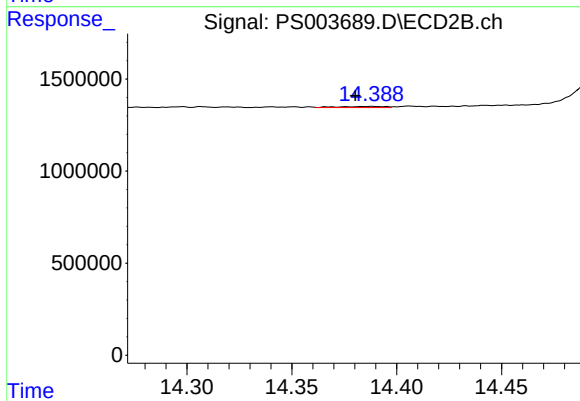

#12 2,4,5-T


R.T.: 14.388 min
Delta R.T.: 0.008 min
Response: 96904
Conc: 0.05 ng/ml

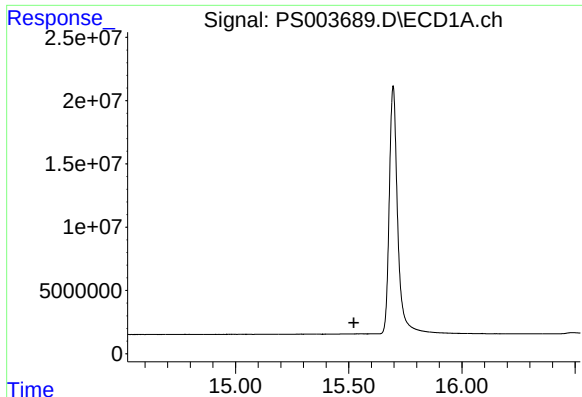

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

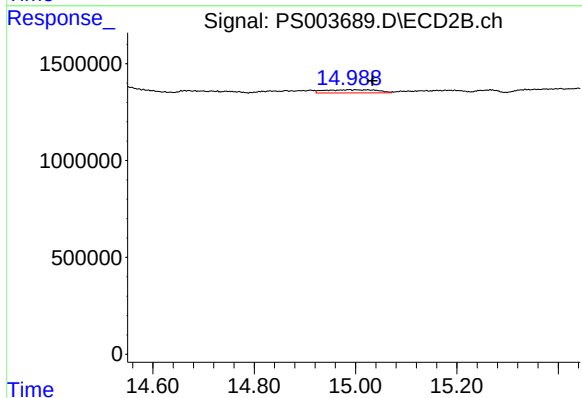


#13 2,4-DB

R.T.: 14.987 min
Delta R.T.: -0.046 min
Response: 1160350
Conc: 4.54 ng/ml

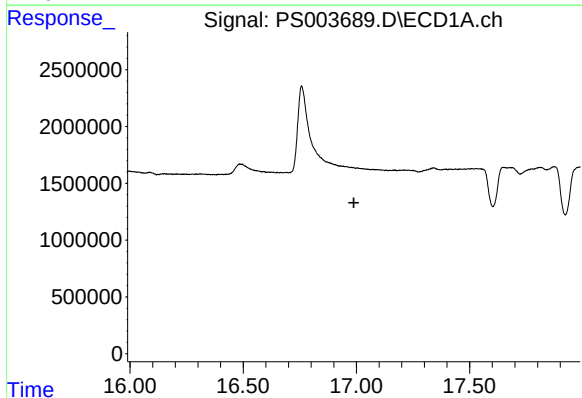


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

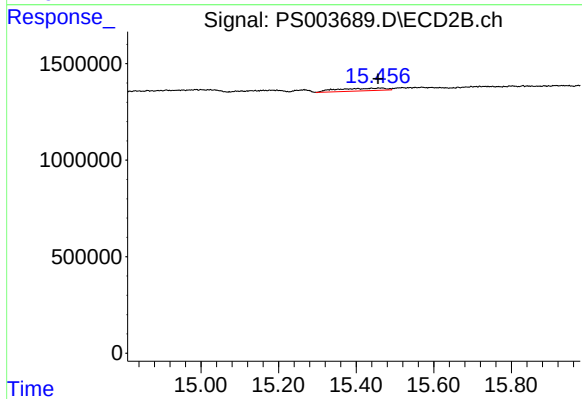

#14 DINOSEB


R.T.: 15.463 min
Delta R.T.: 0.006 min
Response: 1198170
Conc: 0.67 ng/ml

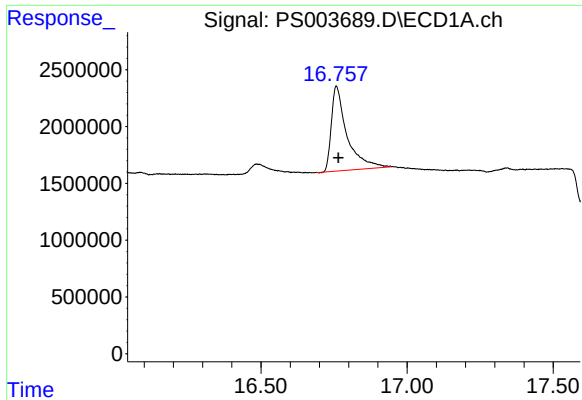

#15 Picloram


R.T.: 16.758 min
Delta R.T.: -0.008 min
Response: 27794453
Conc: 11.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

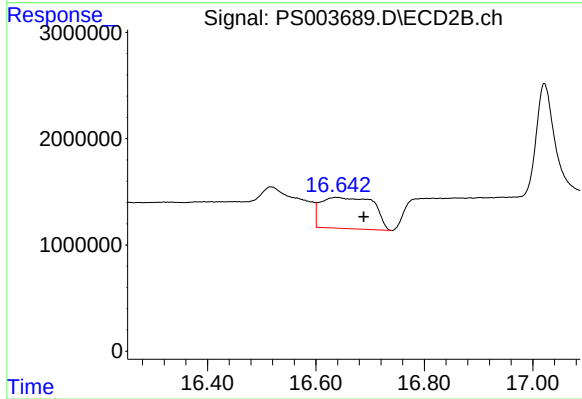


#15 Picloram

R.T.: 16.638 min
Delta R.T.: -0.050 min
Response: 19689376
Conc: 7.76 ng/ml

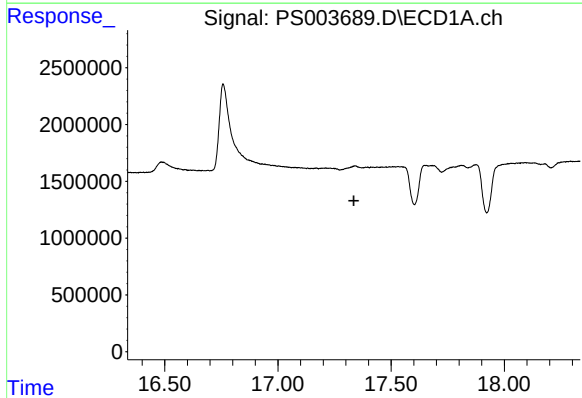

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

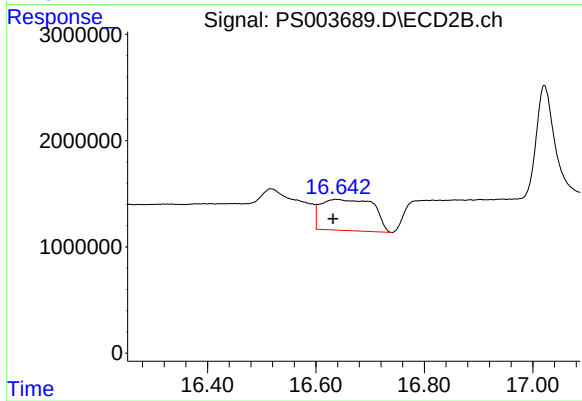

#16 DCPA

R.T.: 16.638 min
Delta R.T.: 0.006 min
Response: 19689376
Conc: 6.33 ng/ml