

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032219\
 Data File : PS003701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 17:15
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 00:56:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.272	10.774	255.9E6	225.8E6	582.946	480.872
Target Compounds							
2) T	3,5-DICHL...	0.000	8.956	0	101747	N.D.	0.165 #
3) T	4-Nitroph...	0.000	9.975	0	476455	N.D.	2.119 #
7) T	MCPA	0.000	11.664	0	716533	N.D.	0.415 #
9) T	2,4-D	0.000	12.688	0	17367	N.D.	0.033 #
10) T	Pentachlo...	0.000	13.185	0	869573	N.D.	0.132 #
11) T	2,4,5-TP ...	0.000	13.842	0	195306	N.D.	0.077 #
12) T	2,4,5-T	0.000	14.326	0	38216	N.D.	0.019 #
13) T	2,4-DB	0.000	15.002	0	603036	N.D.	2.362 #
14) T	DINOSEB	0.000	15.444	0	2382070	N.D.	1.335 #
15) T	Picloram	16.737	16.678	32582955	9661418	13.238	3.807 #
16) T	DCPA	0.000	16.624	0	15391912	N.D.	4.949 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032219\
Data File : PS003701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 17:15
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 00:56:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

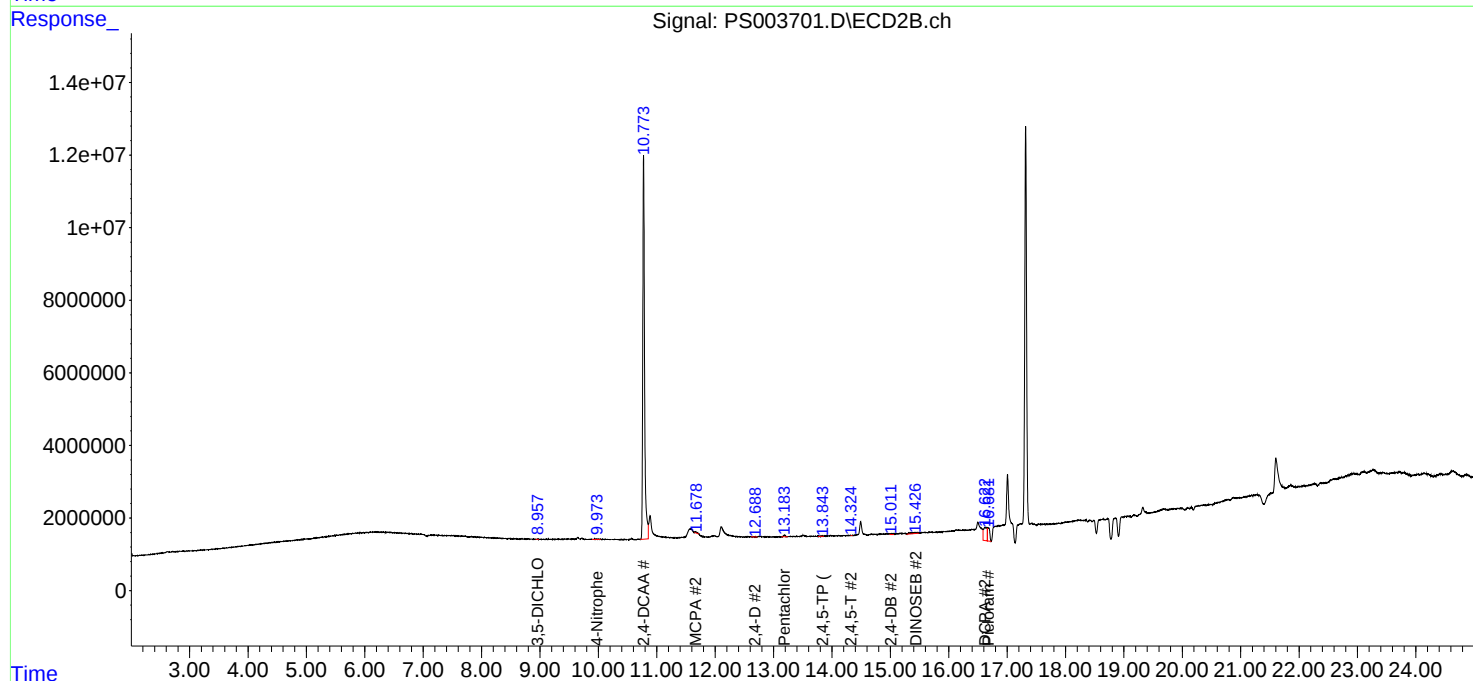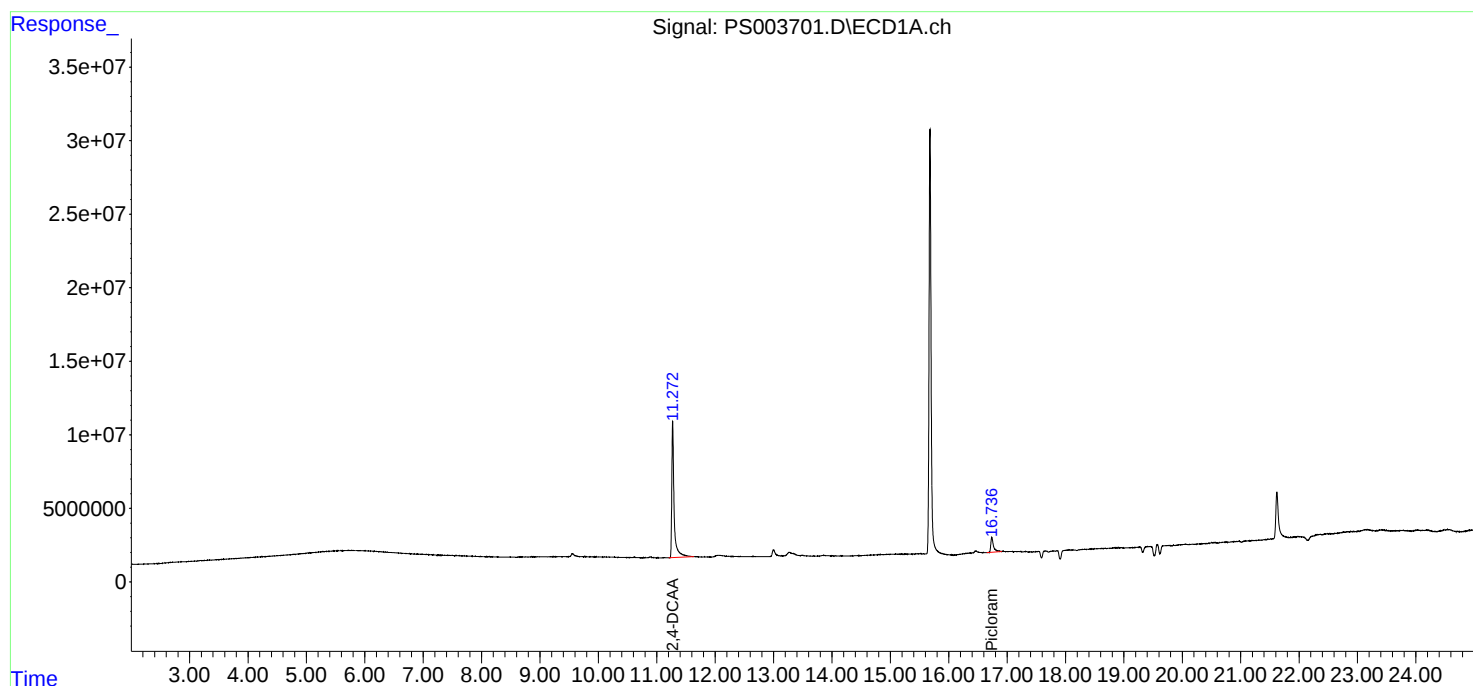


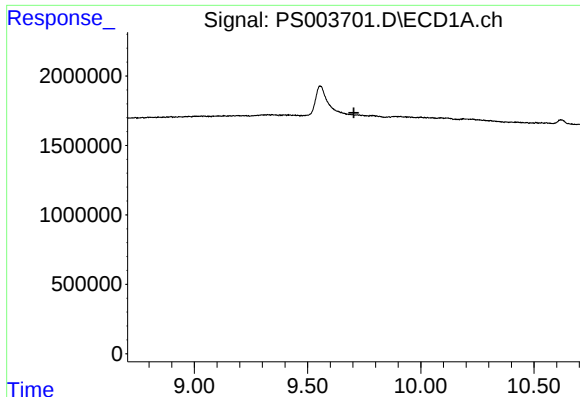

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

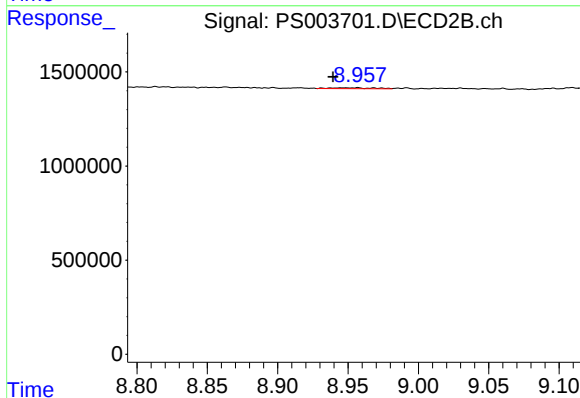


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.956 min
Delta R.T.: 0.016 min
Response: 101747
Conc: 0.16 ng/ml

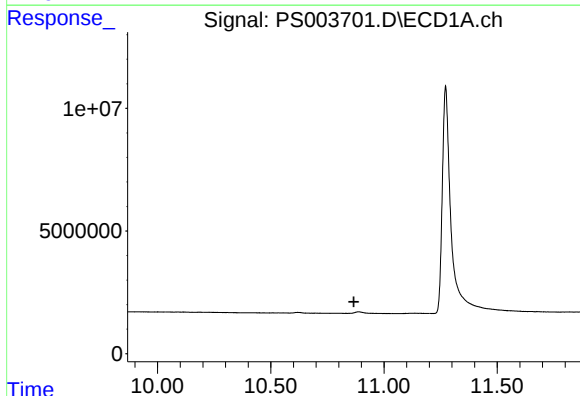


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

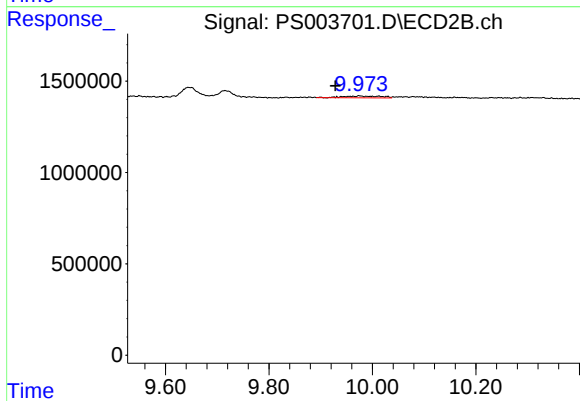

#3 4-Nitrophenol


R.T.: 9.975 min
Delta R.T.: 0.047 min
Response: 476455
Conc: 2.12 ng/ml

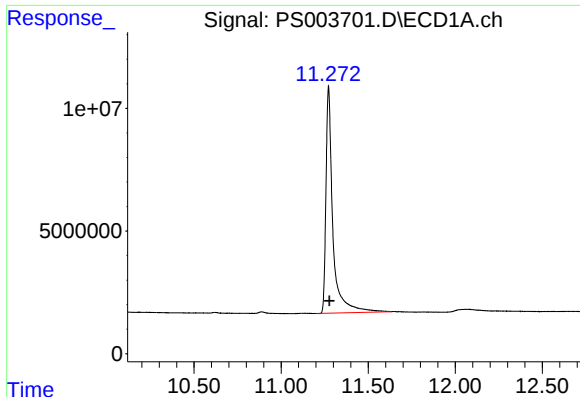

#4 2,4-DCAA


R.T.: 11.272 min
Delta R.T.: -0.006 min
Response: 255927670
Conc: 582.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

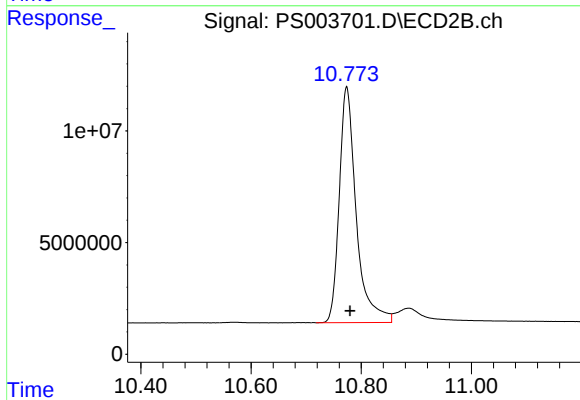


#4 2,4-DCAA

R.T.: 10.774 min
Delta R.T.: -0.006 min
Response: 225802677
Conc: 480.87 ng/ml

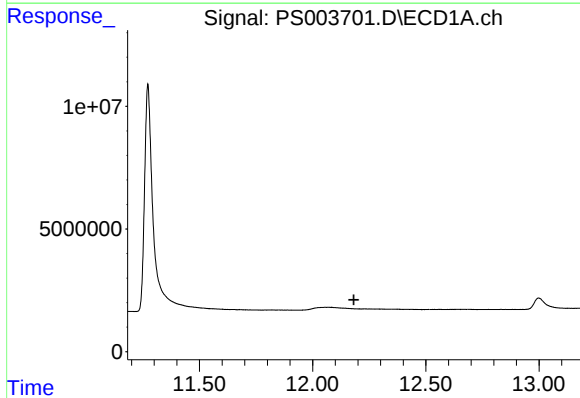


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

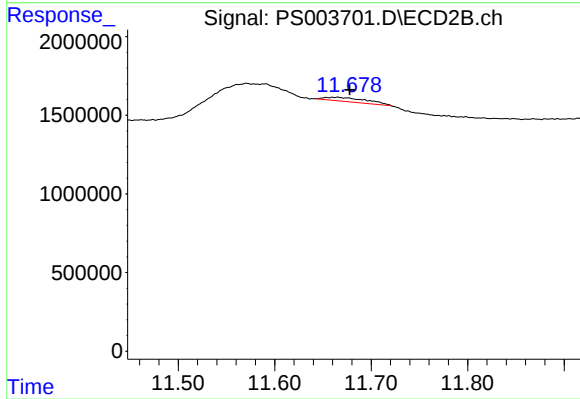

#7 MCPA


R.T.: 11.664 min
Delta R.T.: -0.014 min
Response: 716533
Conc: 0.42 ug/ml

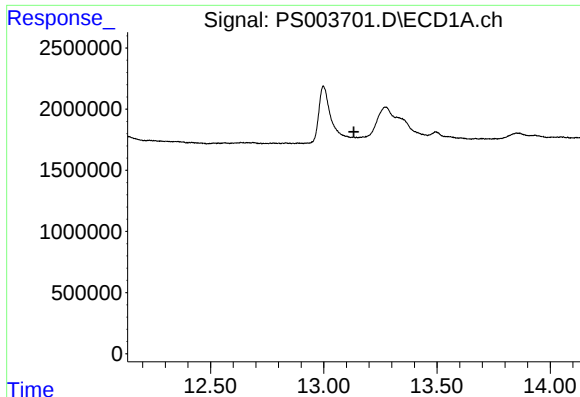

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

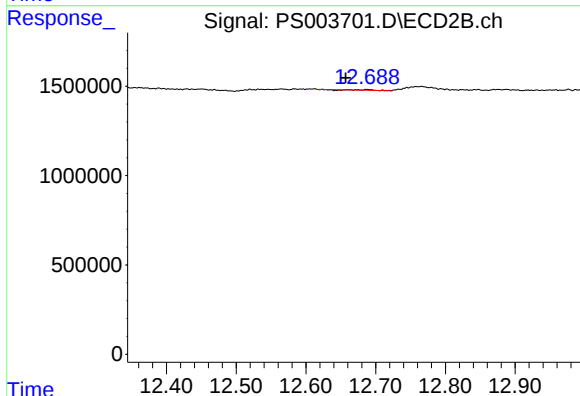


#9 2,4-D

R.T.: 12.688 min
Delta R.T.: 0.031 min
Response: 17367
Conc: 0.03 ng/ml

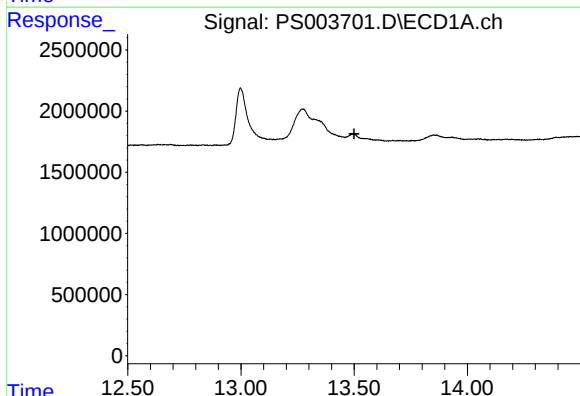


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

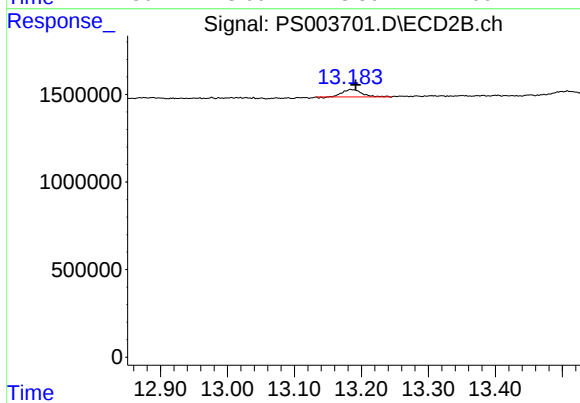

#10 Pentachlorophenol


R.T.: 13.185 min
Delta R.T.: -0.006 min
Response: 869573
Conc: 0.13 ng/ml

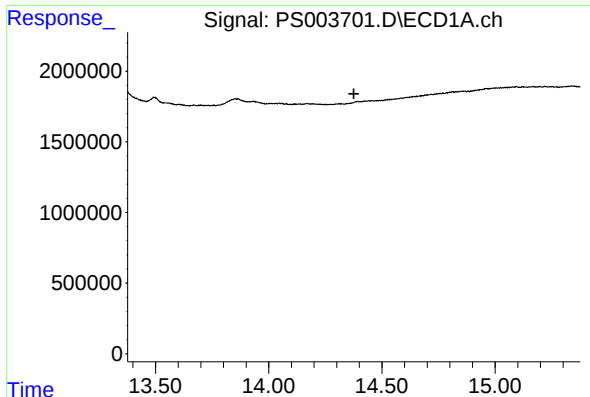

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

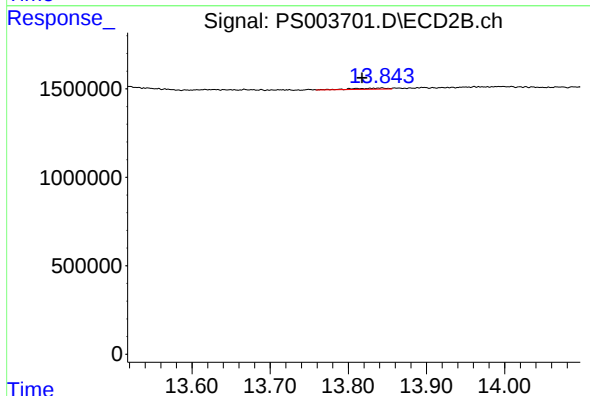


#11 2,4,5-TP (SILVEX)

R.T.: 13.842 min
Delta R.T.: 0.024 min
Response: 195306
Conc: 0.08 ng/ml

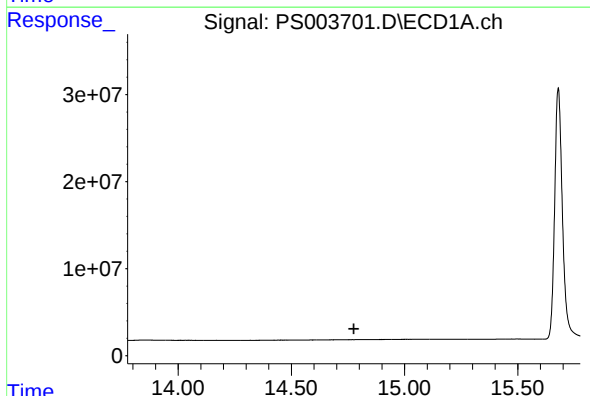


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

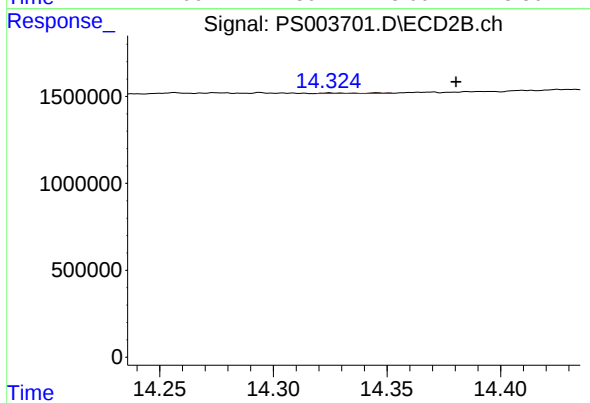

#12 2,4,5-T


R.T.: 14.326 min
Delta R.T.: -0.054 min
Response: 38216
Conc: 0.02 ng/ml

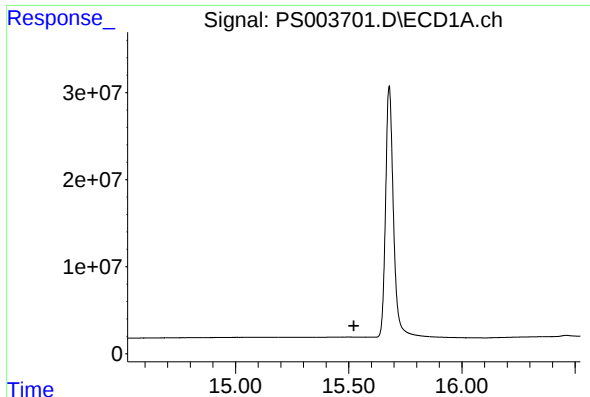

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

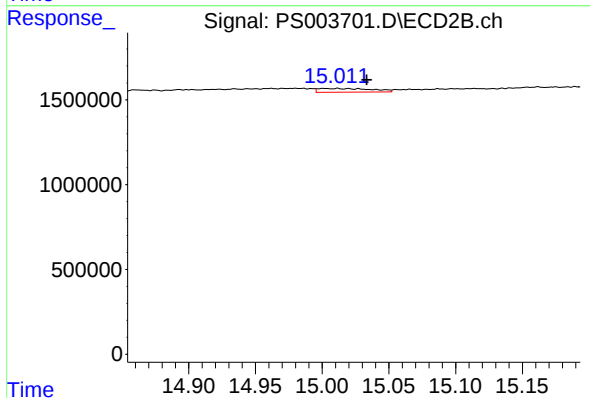


#13 2,4-DB

R.T.: 15.002 min
Delta R.T.: -0.031 min
Response: 603036
Conc: 2.36 ng/ml

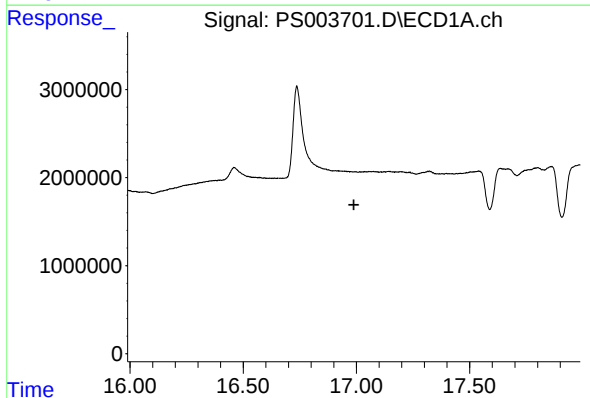


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

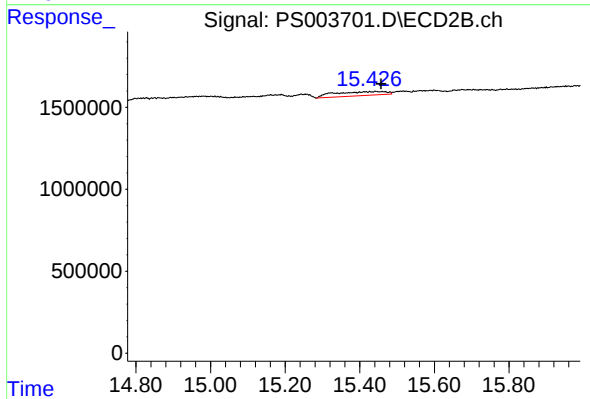

#14 DINOSEB


R.T.: 15.444 min
Delta R.T.: -0.013 min
Response: 2382070
Conc: 1.33 ng/ml

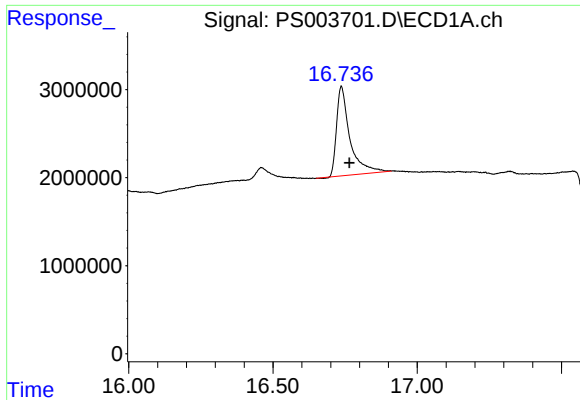

#15 Picloram


R.T.: 16.737 min
Delta R.T.: -0.028 min
Response: 32582955
Conc: 13.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

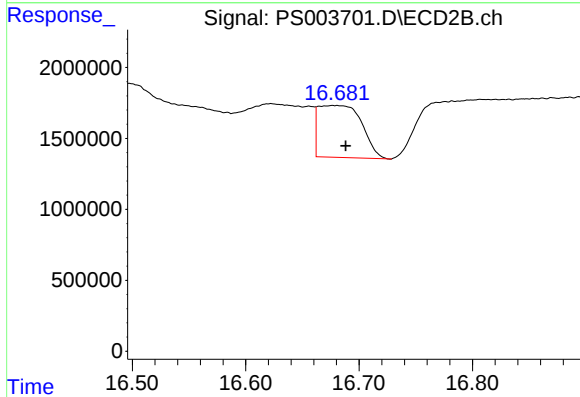


#15 Picloram

R.T.: 16.678 min
Delta R.T.: -0.011 min
Response: 9661418
Conc: 3.81 ng/ml

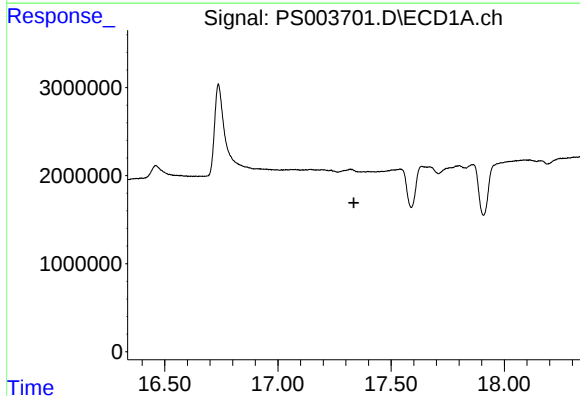

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

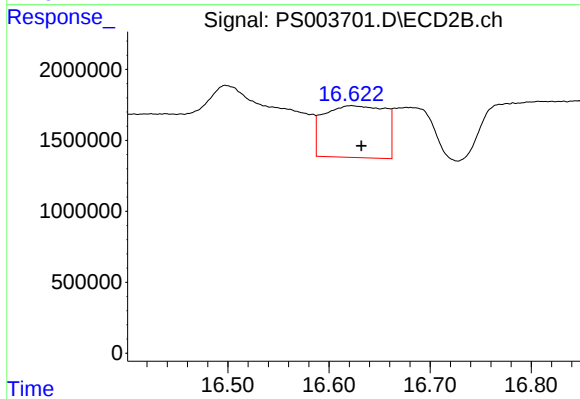

#16 DCPA

R.T.: 16.624 min
Delta R.T.: -0.008 min
Response: 15391912
Conc: 4.95 ng/ml