

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032219\
 Data File : PS003707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 20:23
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 00:58:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.267	10.768	255.7E6	225.4E6	582.474	479.964
Target Compounds							
2) T	3,5-DICHL...	0.000	8.945	0	95592	N.D.	0.155 #
3) T	4-Nitroph...	0.000	9.961	0	72363	N.D.	0.322 #
7) T	MCPA	0.000	11.653	0	782655	N.D.	0.454 #
10) T	Pentachlo...	0.000	13.180	0	973769	N.D.	0.148 #
11) T	2,4,5-TP ...	0.000	13.817	0	437997	N.D.	0.172 #
12) T	2,4,5-T	0.000	14.314	0	110788	N.D.	0.055 #
13) T	2,4-DB	0.000	14.970	0	1468855	N.D.	5.752 #
14) T	DINOSEB	0.000	15.446	0	1276491	N.D.	0.715 #
15) T	Picloram	16.735	16.670	35181409	9547908	14.294	3.762 #
16) T	DCPA	0.000	16.617	0	12989012	N.D.	4.176 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032219\
Data File : PS003707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 20:23
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 00:58:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

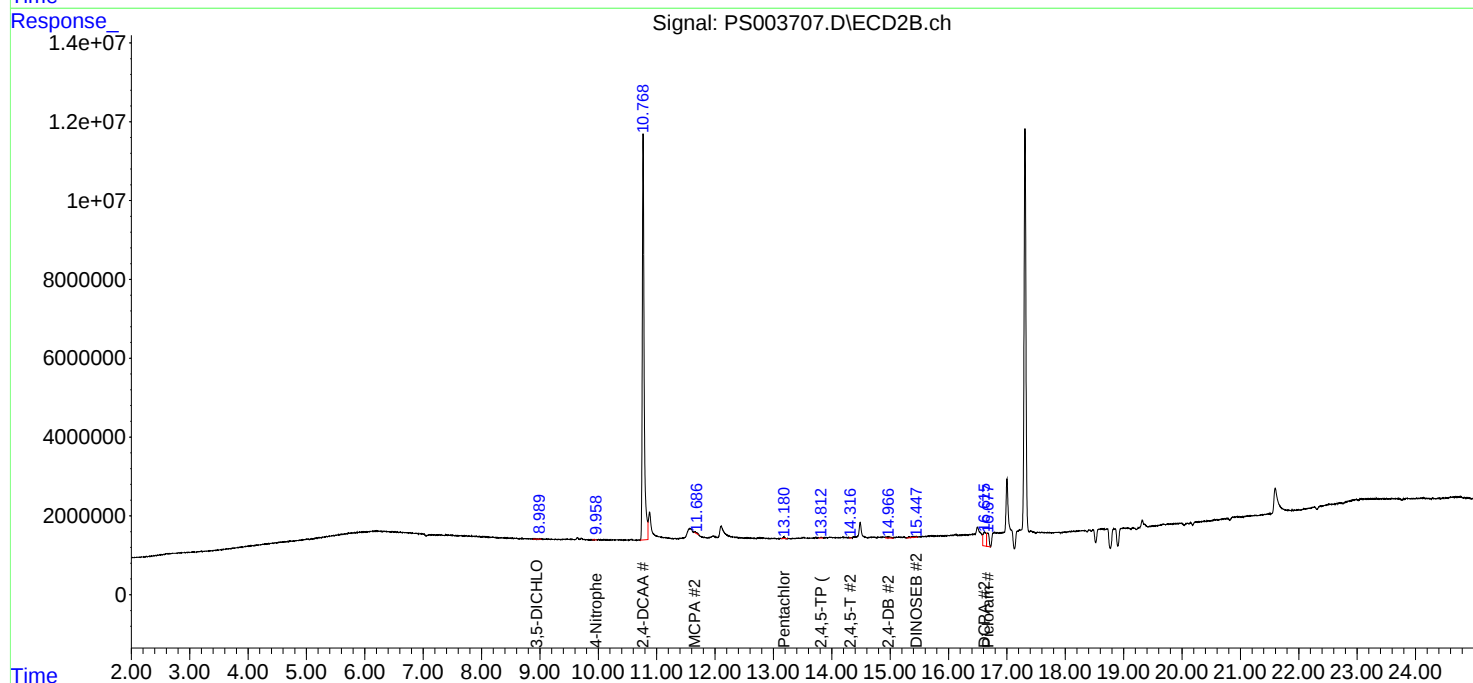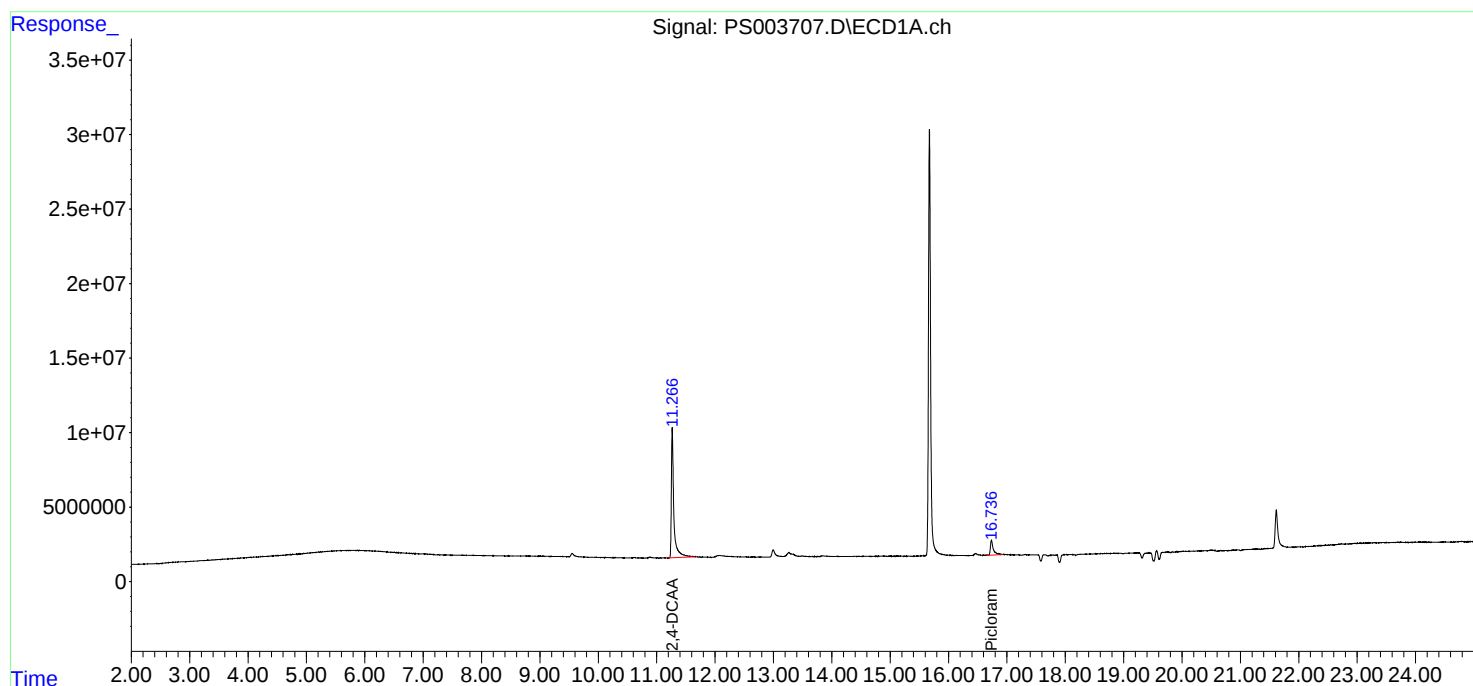


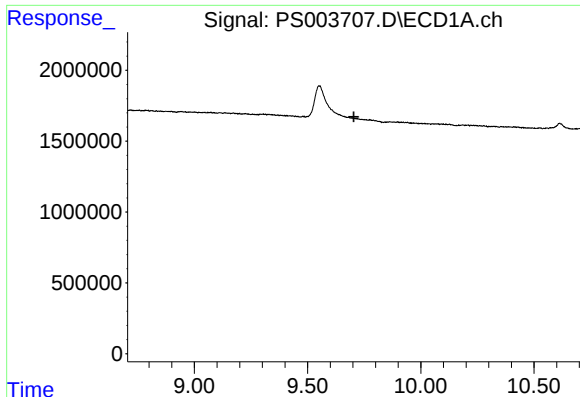

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

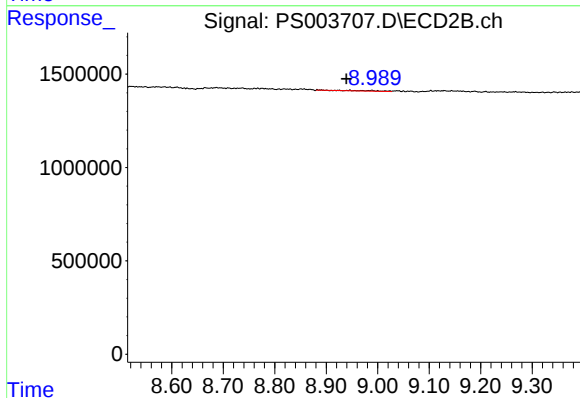


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.945 min
Delta R.T.: 0.006 min
Response: 95592
Conc: 0.15 ng/ml

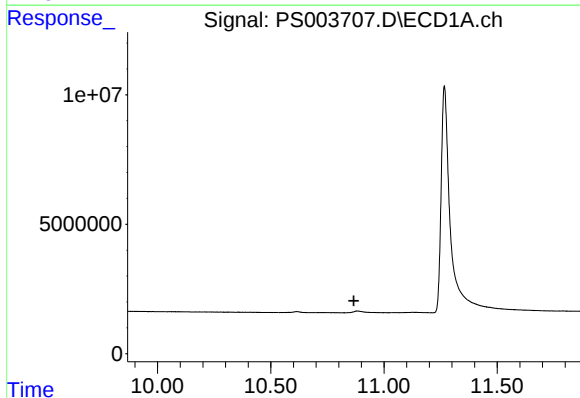


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

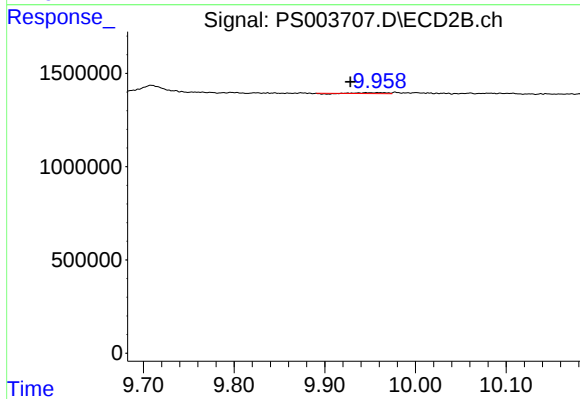

#3 4-Nitrophenol


R.T.: 9.961 min
Delta R.T.: 0.033 min
Response: 72363
Conc: 0.32 ng/ml

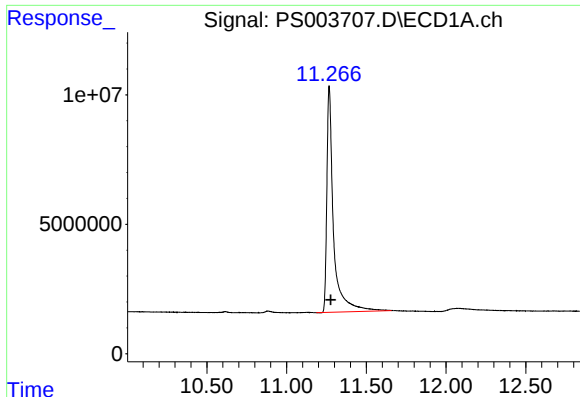

#4 2,4-DCAA


R.T.: 11.267 min
Delta R.T.: -0.011 min
Response: 255720243
Conc: 582.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

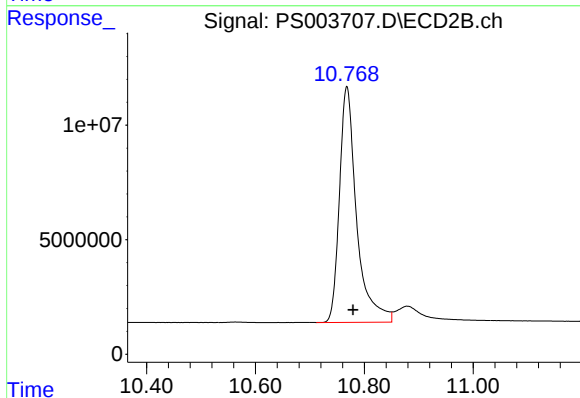


#4 2,4-DCAA

R.T.: 10.768 min
Delta R.T.: -0.012 min
Response: 225376074
Conc: 479.96 ng/ml

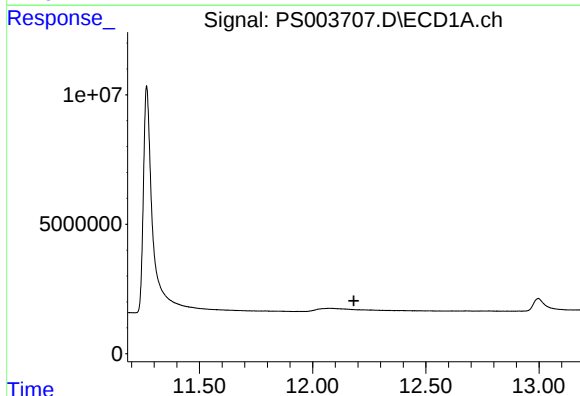


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

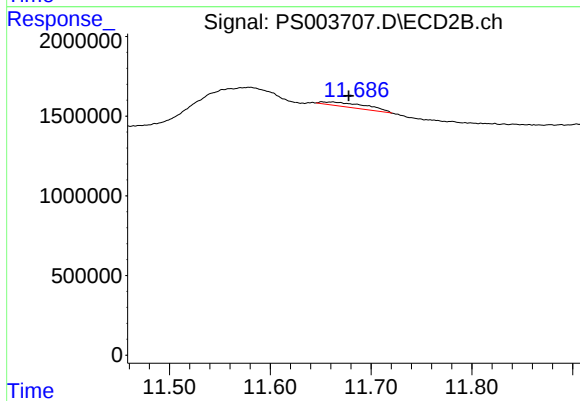

#7 MCPA


R.T.: 11.653 min
Delta R.T.: -0.025 min
Response: 782655
Conc: 0.45 ug/ml

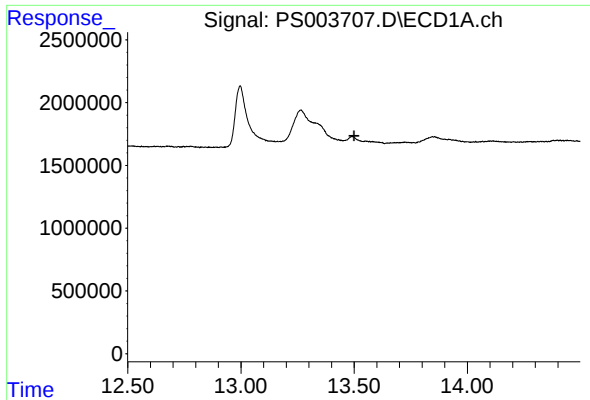

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

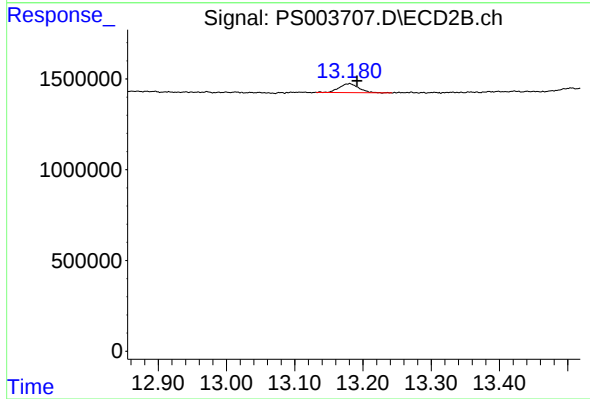


#10 Pentachlorophenol

R.T.: 13.180 min
Delta R.T.: -0.012 min
Response: 973769
Conc: 0.15 ng/ml

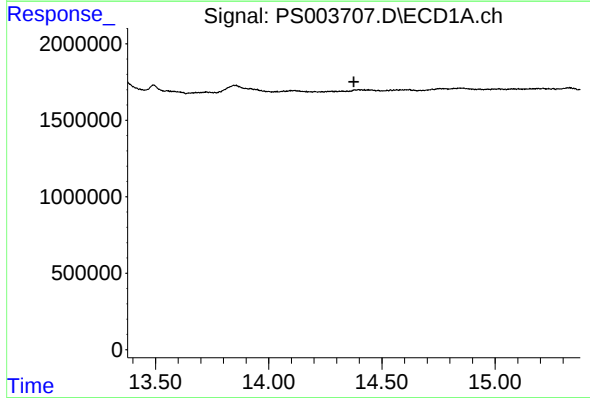


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

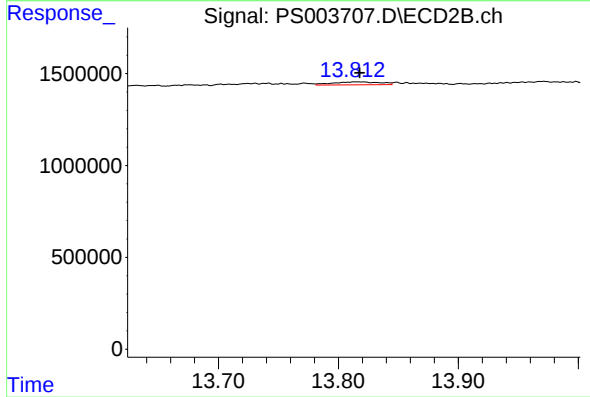

#11 2,4,5-TP (SILVEX)


R.T.: 13.817 min
Delta R.T.: 0.000 min
Response: 437997
Conc: 0.17 ng/ml

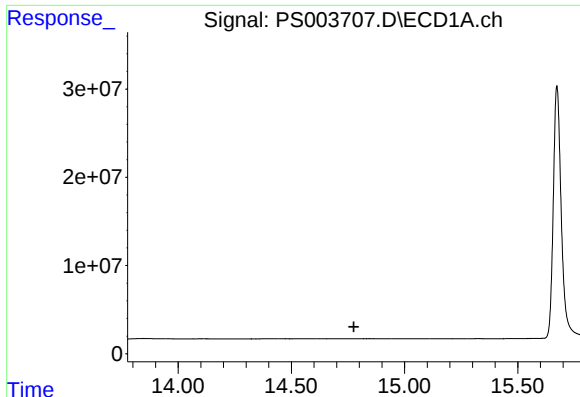

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

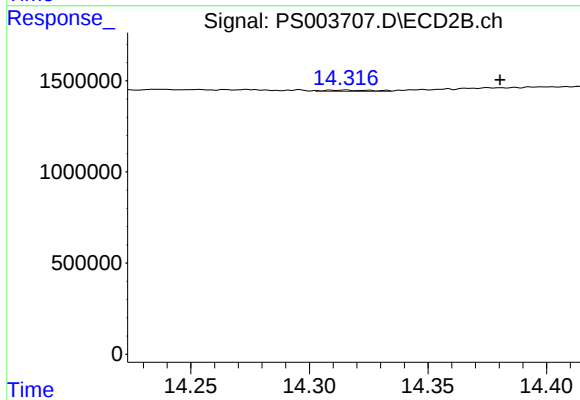


#12 2,4,5-T

R.T.: 14.314 min
Delta R.T.: -0.067 min
Response: 110788
Conc: 0.05 ng/ml

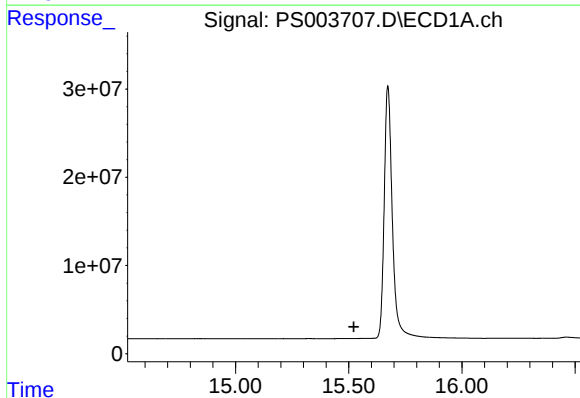


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

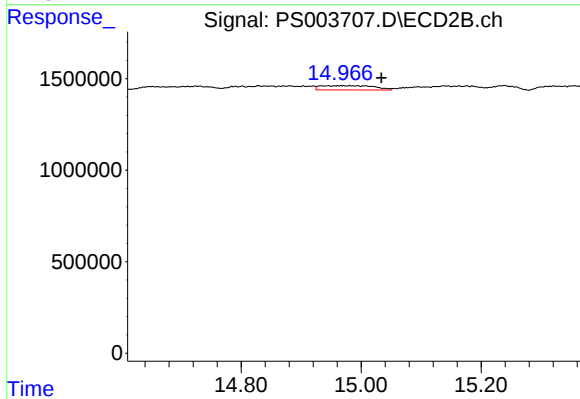

#13 2,4-DB


R.T.: 14.970 min
Delta R.T.: -0.063 min
Response: 1468855
Conc: 5.75 ng/ml

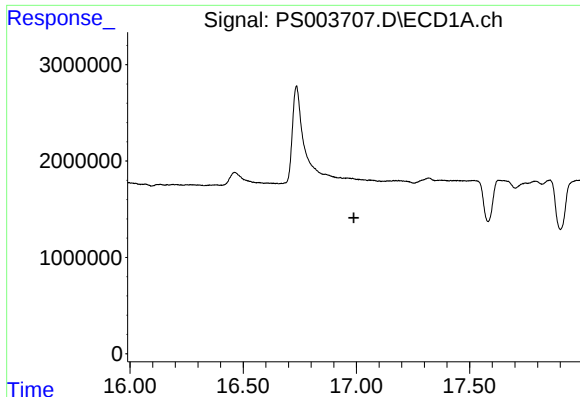

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

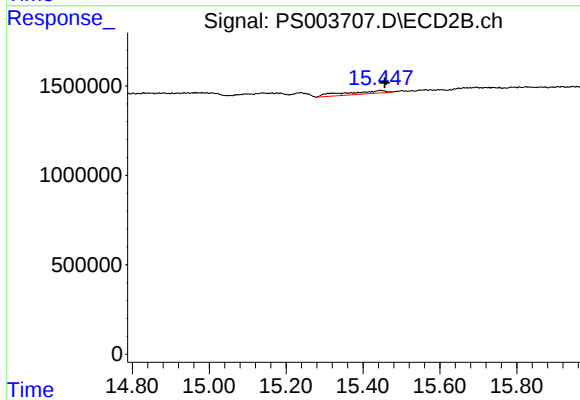


#14 DINOSEB

R.T.: 15.446 min
Delta R.T.: -0.011 min
Response: 1276491
Conc: 0.72 ng/ml

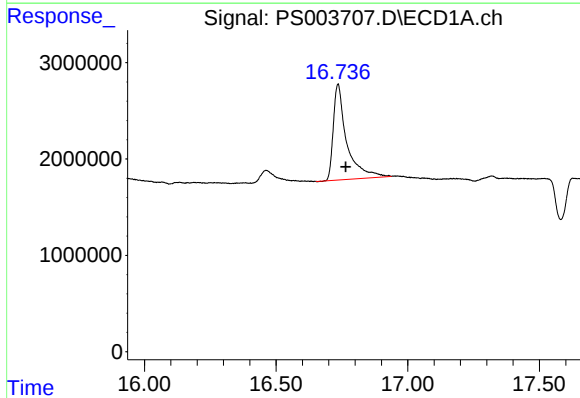


#15 Picloram

R.T.: 16.735 min
Delta R.T.: -0.030 min
Response: 35181409
Conc: 14.29 ng/ml

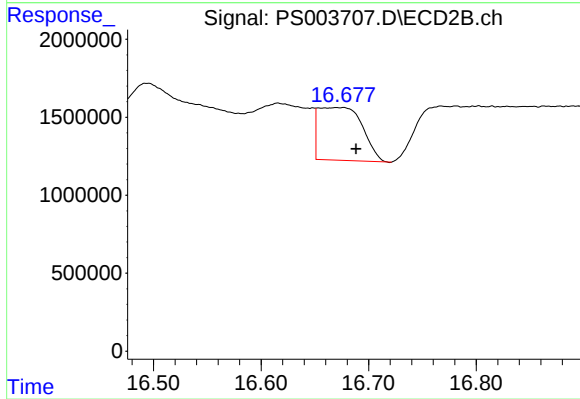

#15 Picloram


R.T.: 16.670 min
Delta R.T.: -0.018 min
Response: 9547908
Conc: 3.76 ng/ml

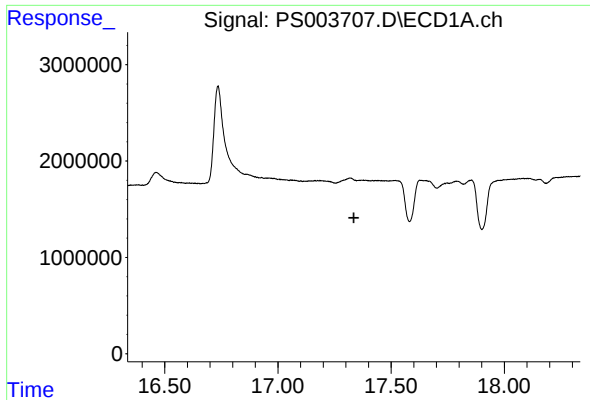

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

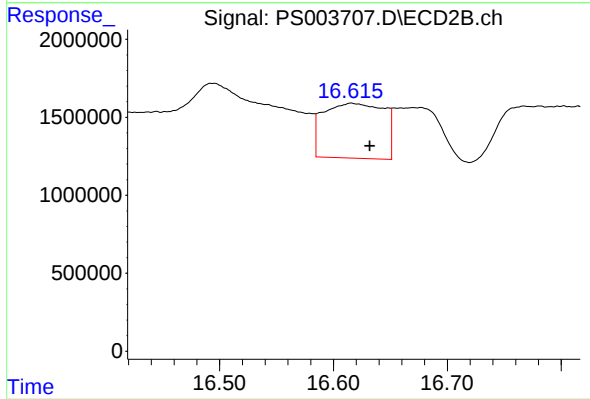

#16 DCPA

R.T.: 16.617 min
Delta R.T.: -0.015 min
Response: 12989012
Conc: 4.18 ng/ml