

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
 Data File : PS018665.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 08:54
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:11:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.478	0.000	304.9E6	0	79.127	N.D. #
5) T	DICAMBA	0.000	7.035f	0	65721506	N.D.	22.065
6) T	MCP	0.000	7.035f	0	65721506	N.D.	26.846
8) T	DICHLORPROP	0.000	7.622	0	16597561	N.D.	20.967
9) T	2,4-D	8.413f	0.000	164.3E6	0	49.039	N.D. #
10) T	Pentachlo...	8.668	0.000	8601594	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.640f	0	2156326	N.D.	<MDL
12) T	2,4,5-T	0.000	9.110f	0	4358572	N.D.	1.052
15) T	Picloram	11.004	10.875	342.8E6	12006646	16.676	2.259 #
16) T	DCPA	0.000	10.875f	0	12006646	N.D.	2.283



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
Data File : PS018665.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 08:54
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:11:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

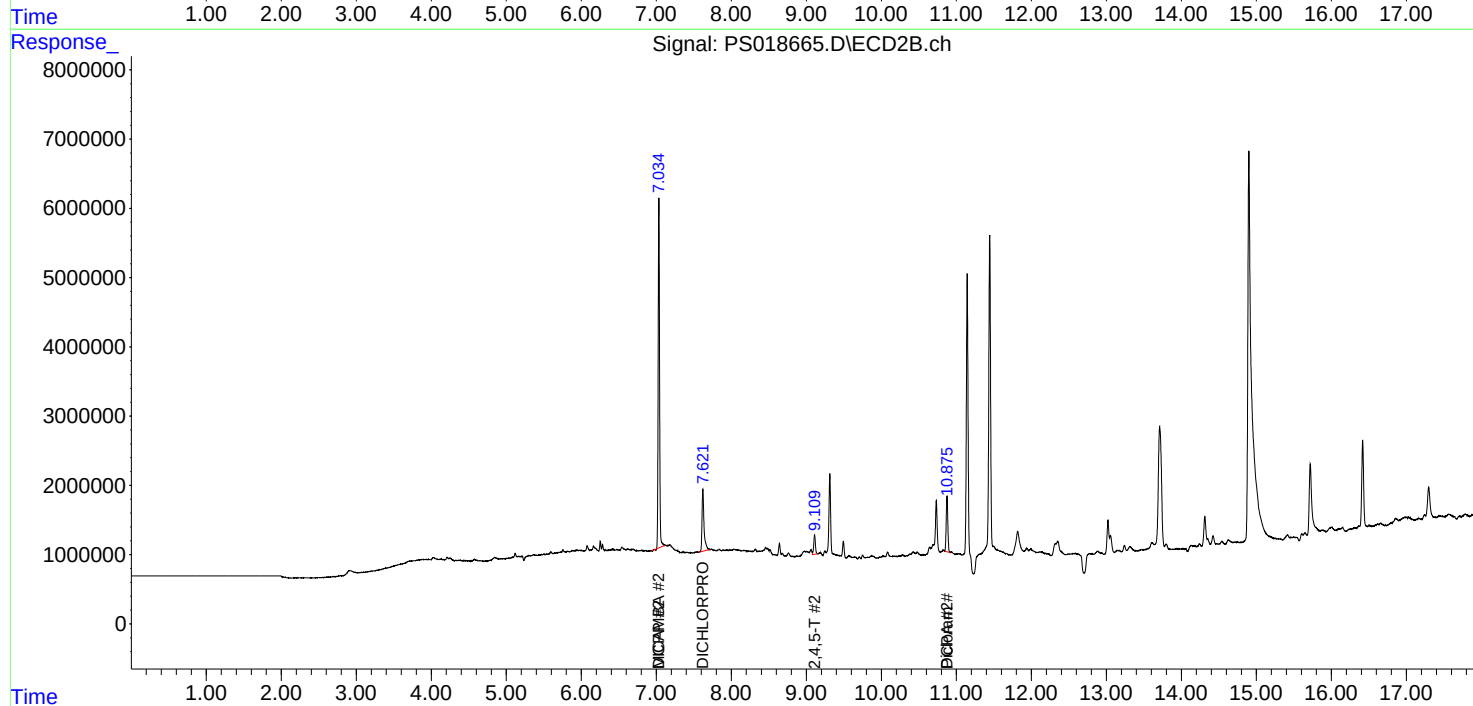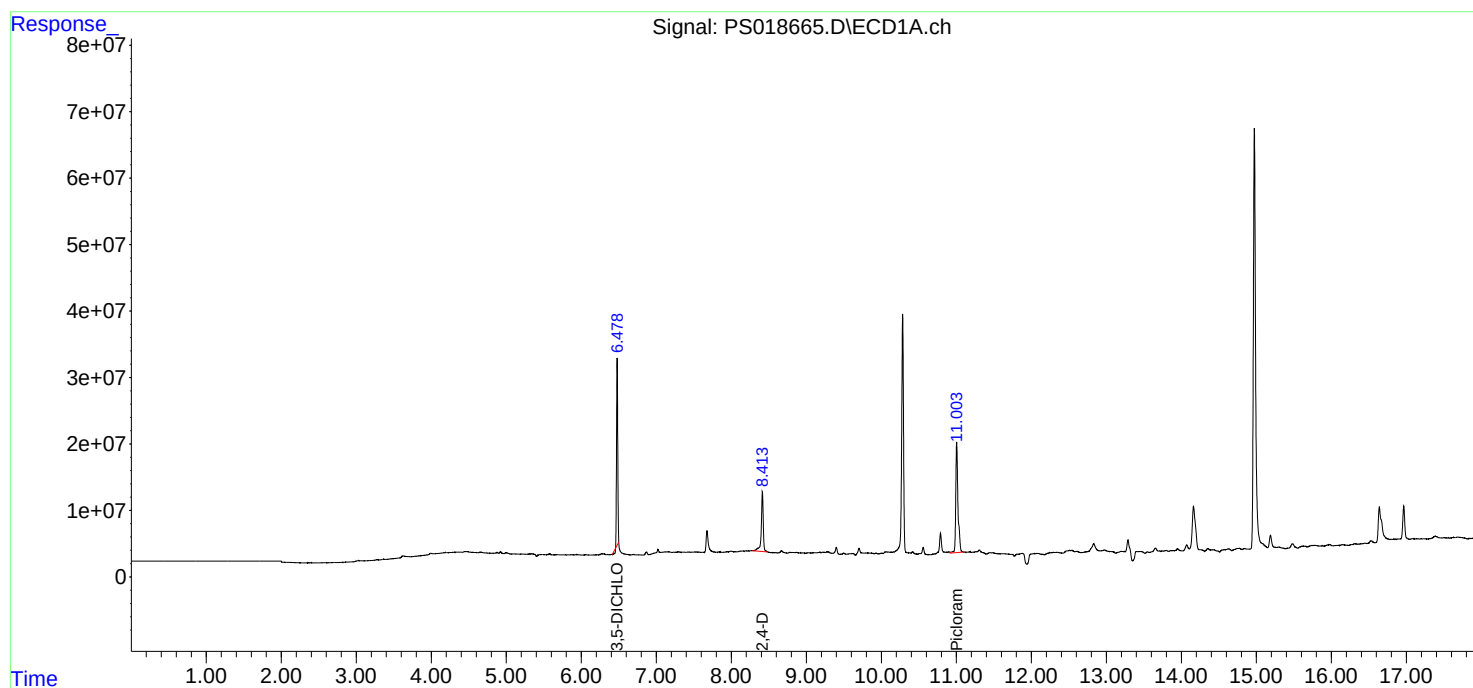


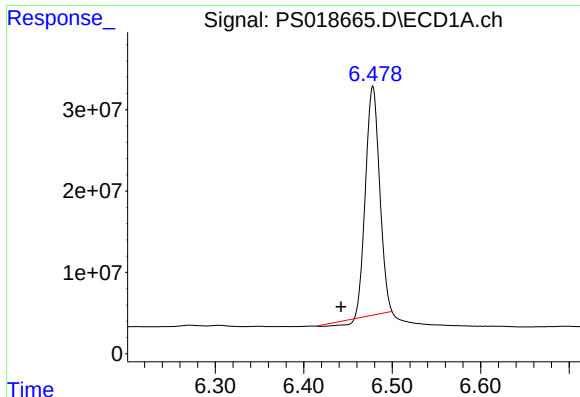

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.478 min
Delta R.T.: 0.036 min
Response: 304919203
Conc: 79.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

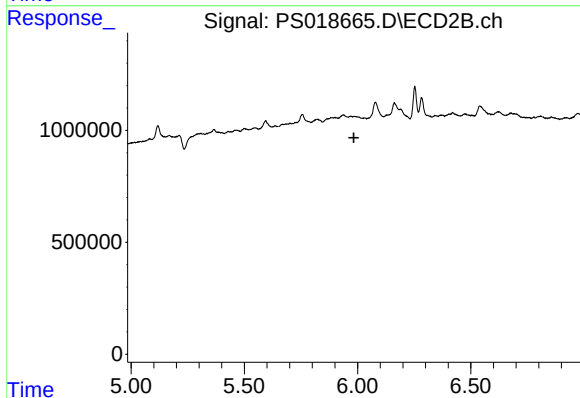


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.984 min
Response: 0
Conc: N.D.

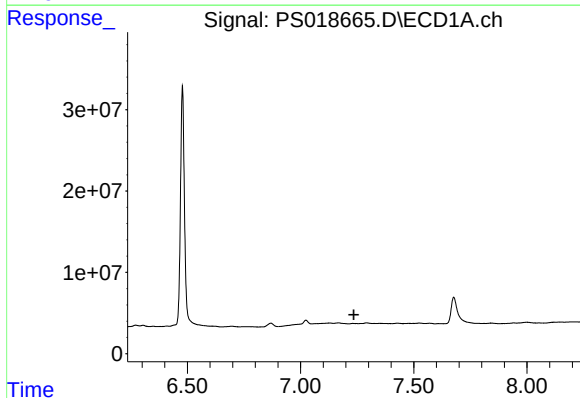


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.235 min
Response: 0
Conc: N.D.

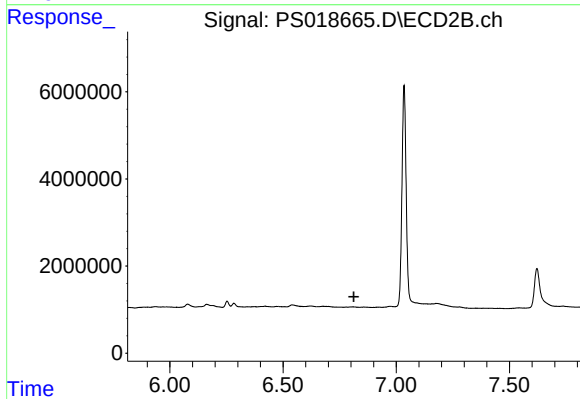

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.813 min
Response: 0
Conc: N.D.

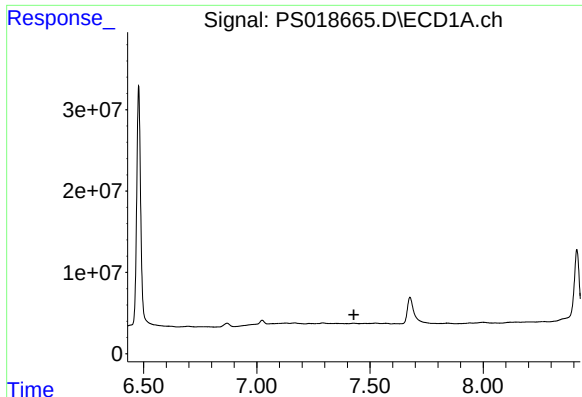

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.429 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

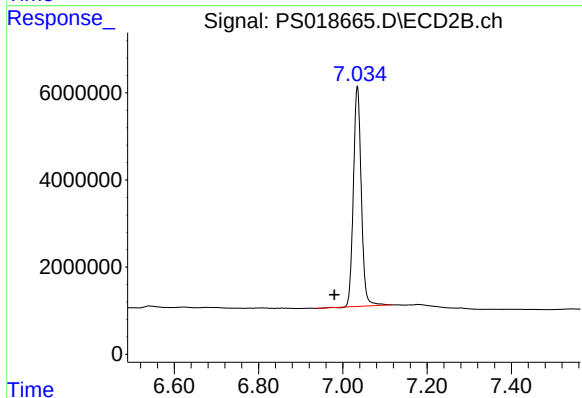


#5 DICAMBA

R.T.: 7.035 min
Delta R.T.: 0.055 min
Response: 65721506
Conc: 22.06 ng/ml

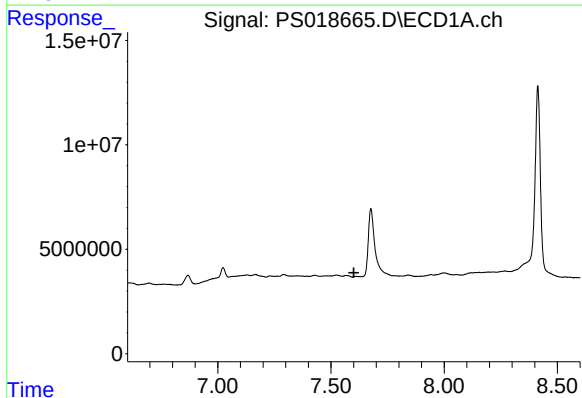


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.601 min
Response: 0
Conc: N.D.

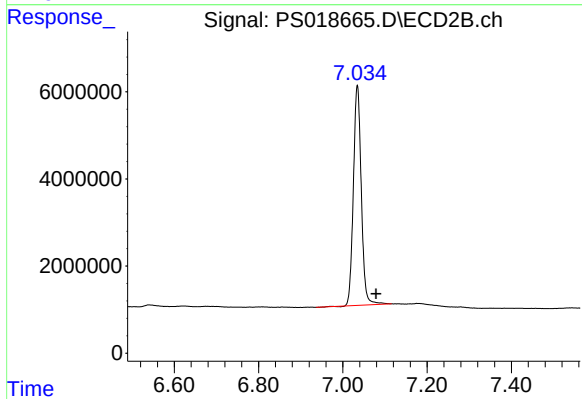

#6 MCP


R.T.: 7.035 min
Delta R.T.: -0.044 min
Response: 65721506
Conc: 26.85 ug/ml

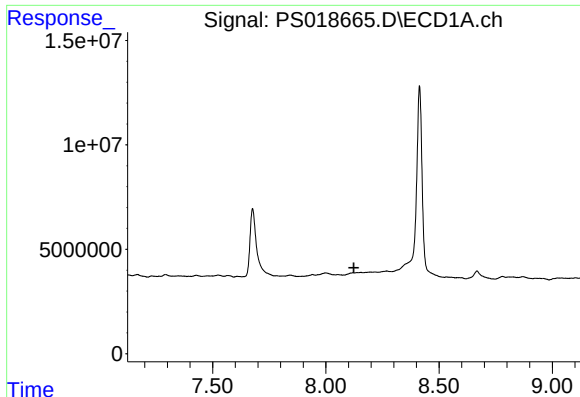

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

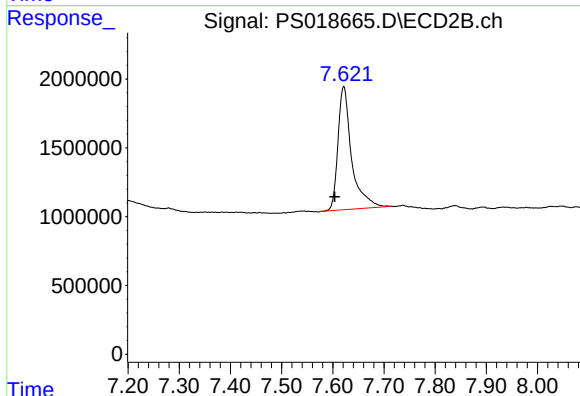


#8 DICHLORPROP

R.T.: 7.622 min
Delta R.T.: 0.018 min
Response: 16597561
Conc: 20.97 ng/ml

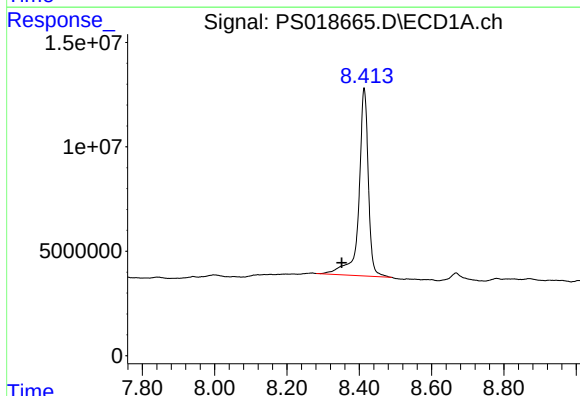


#9 2,4-D

R.T.: 8.413 min
Delta R.T.: 0.061 min
Response: 164311151
Conc: 49.04 ng/ml

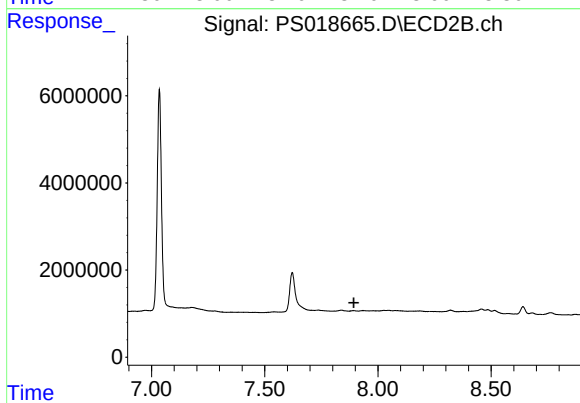

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

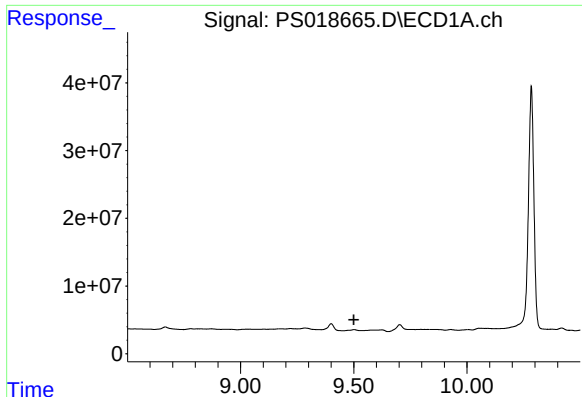

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

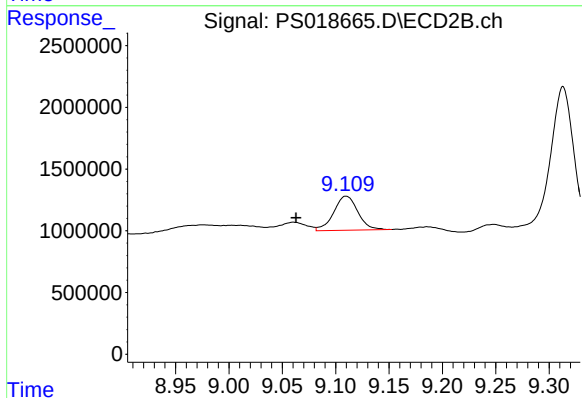


#12 2,4,5-T

R.T.: 9.110 min
Delta R.T.: 0.047 min
Response: 4358572
Conc: 1.05 ng/ml

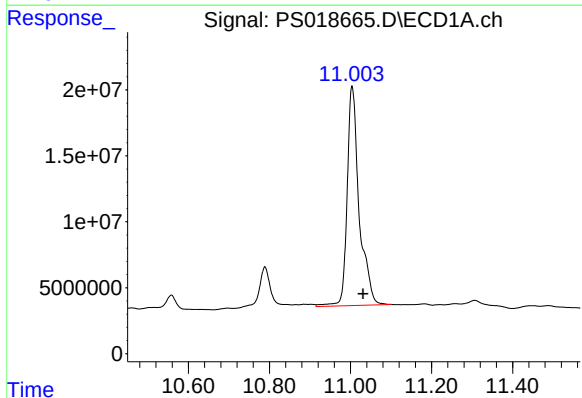


#15 Picloram

R.T.: 11.004 min
Delta R.T.: -0.027 min
Response: 342797218
Conc: 16.68 ng/ml

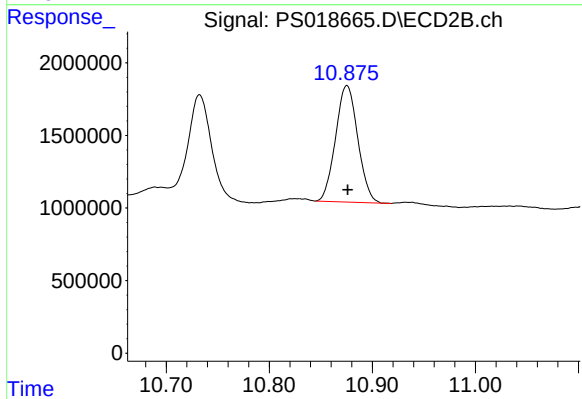

#15 Picloram


R.T.: 10.875 min
Delta R.T.: 0.000 min
Response: 12006646
Conc: 2.26 ng/ml

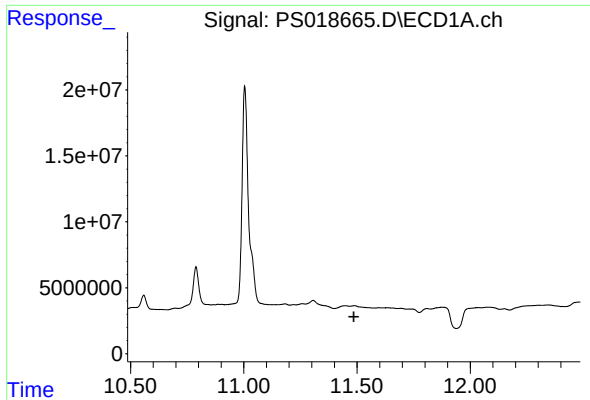

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

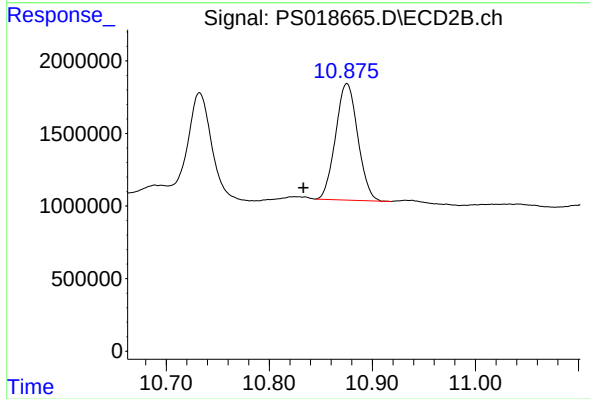

#16 DCPA

R.T.: 10.875 min
Delta R.T.: 0.042 min
Response: 12006646
Conc: 2.28 ng/ml