

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
 Data File : PS018670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 11:21
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:12:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.809	1582.4E6	447.2E6	556.022	635.509
Target Compounds							
3) T	4-Nitroph...	7.022	0.000	21835	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.620	0	7021437	N.D.	8.870
11) T	2,4,5-TP ...	9.168f	8.640f	104.5E6	11954942	6.874	2.741 #
12) T	2,4,5-T	9.495	9.110f	5331240	1349395	<MDL	<MDL #
13) T	2,4-DB	10.005f	0.000	275794	0	<MDL	N.D. #
14) T	DINOSEB	11.176f	0.000	6061302	0	<MDL	N.D. #
15) T	Picloram	11.030	10.876	30921412	6626684	1.504	1.247
16) T	DCPA	0.000	10.876f	0	6626684	N.D.	1.260


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
Data File : PS018670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 11:21
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:12:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

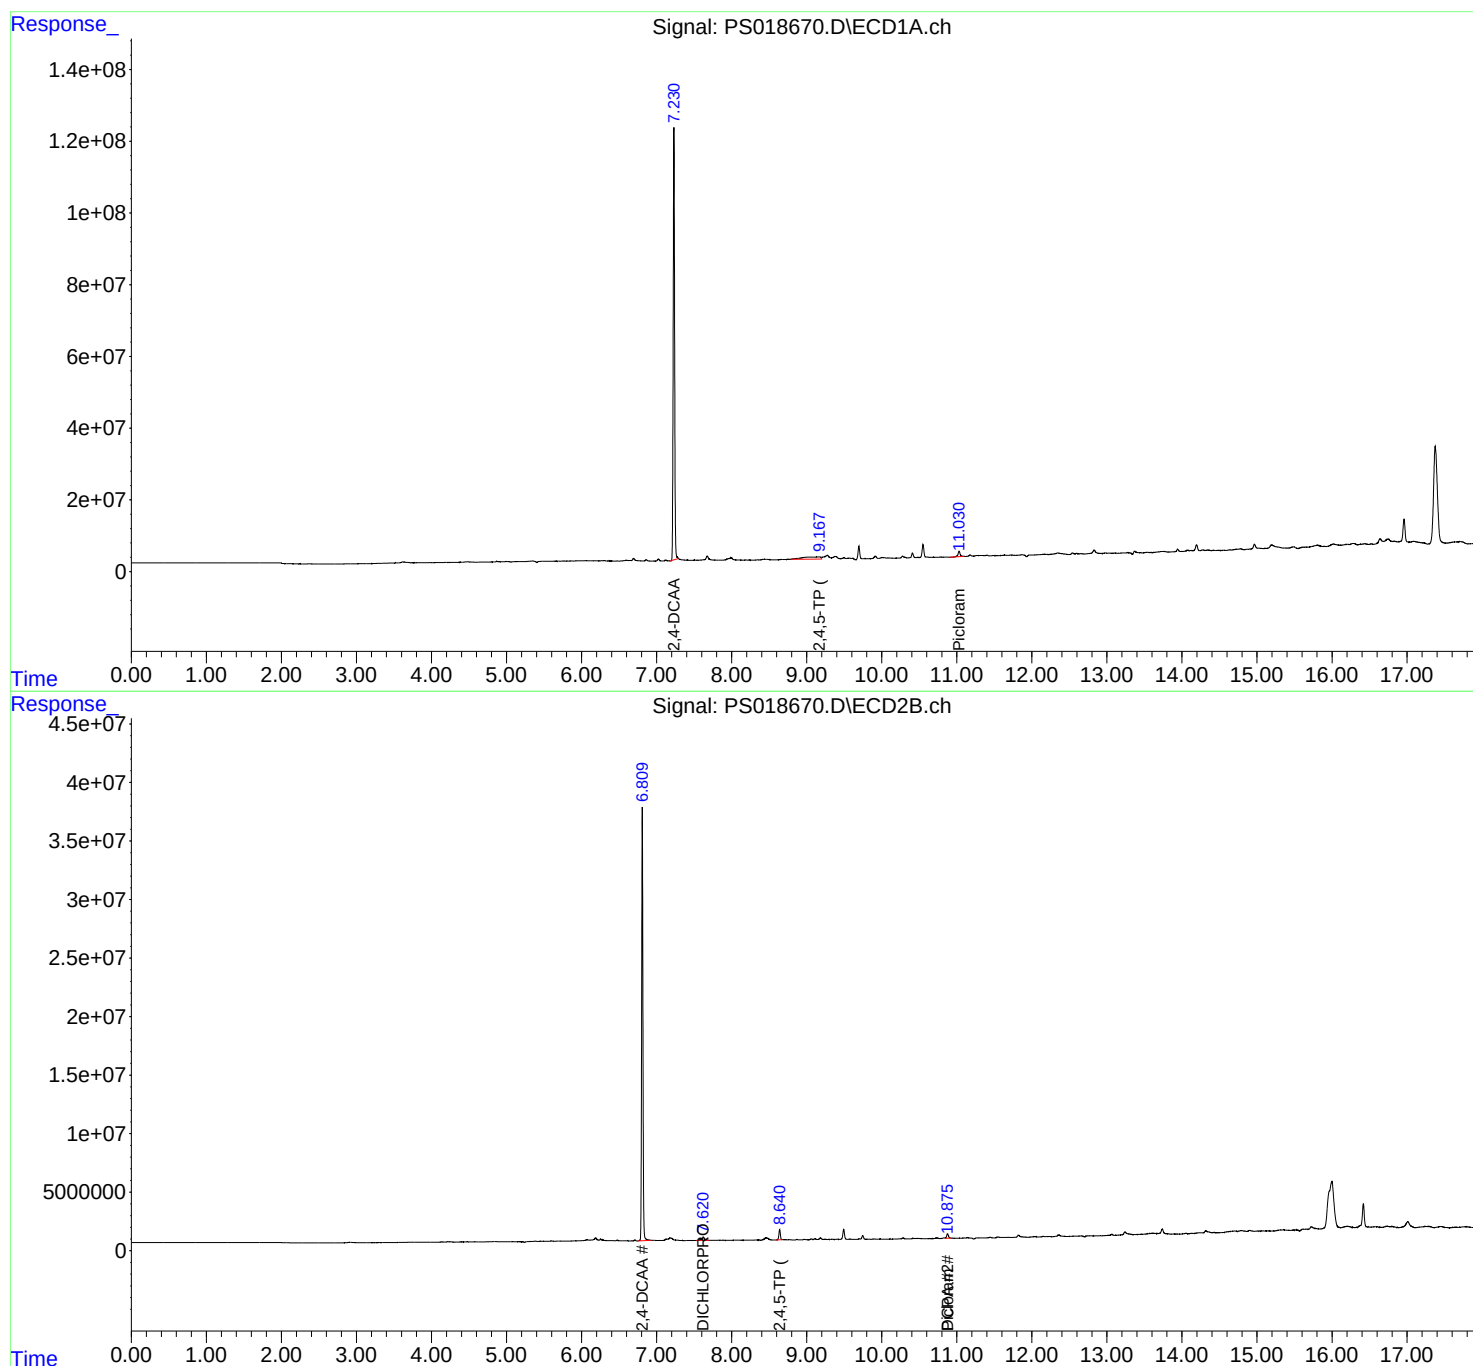


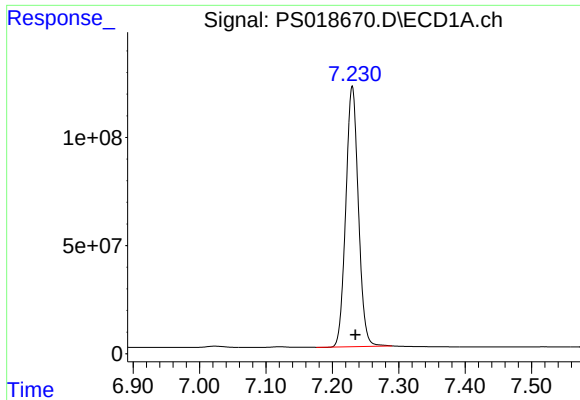

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: -0.005 min
Response: 1582391272
Conc: 556.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

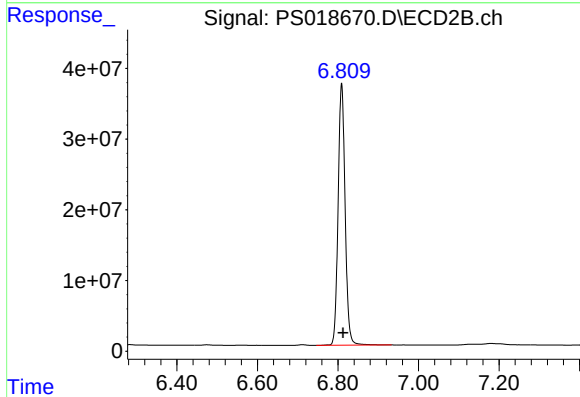


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.004 min
Response: 447179425
Conc: 635.51 ng/ml

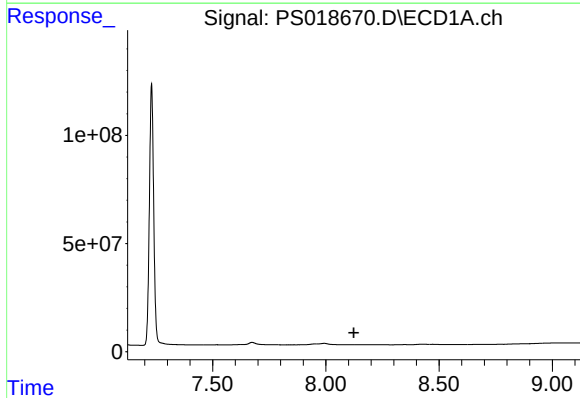


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.124 min
Response: 0
Conc: N.D.

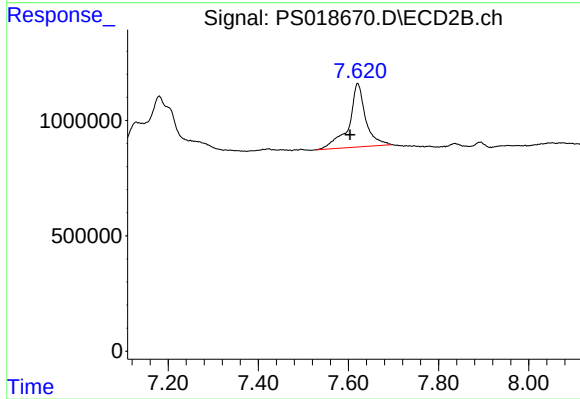

#8 DICHLORPROP


R.T.: 7.620 min
Delta R.T.: 0.016 min
Response: 7021437
Conc: 8.87 ng/ml

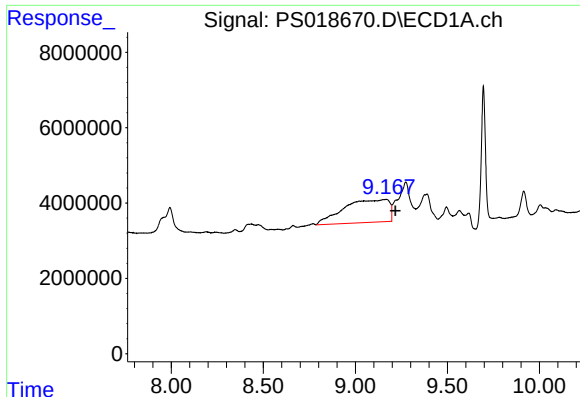

#11 2,4,5-TP (SILVEX)


R.T.: 9.168 min
Delta R.T.: -0.050 min
Response: 104539856
Conc: 6.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

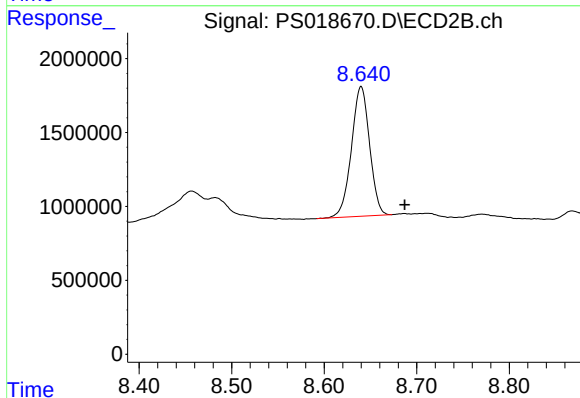


#11 2,4,5-TP (SILVEX)

R.T.: 8.640 min
Delta R.T.: -0.047 min
Response: 11954942
Conc: 2.74 ng/ml

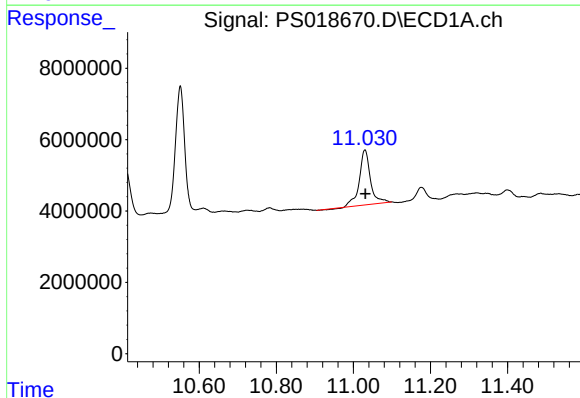


#15 Picloram

R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 30921412
Conc: 1.50 ng/ml

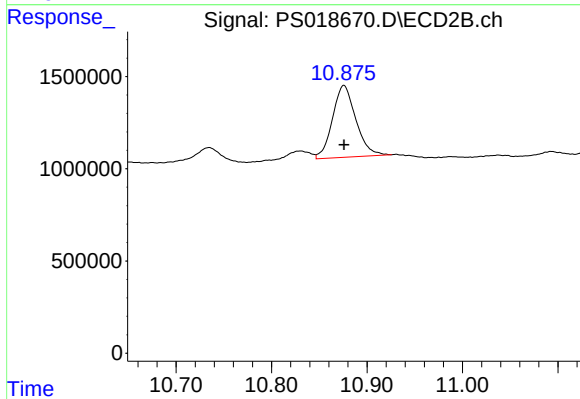

#15 Picloram


R.T.: 10.876 min
Delta R.T.: 0.000 min
Response: 6626684
Conc: 1.25 ng/ml

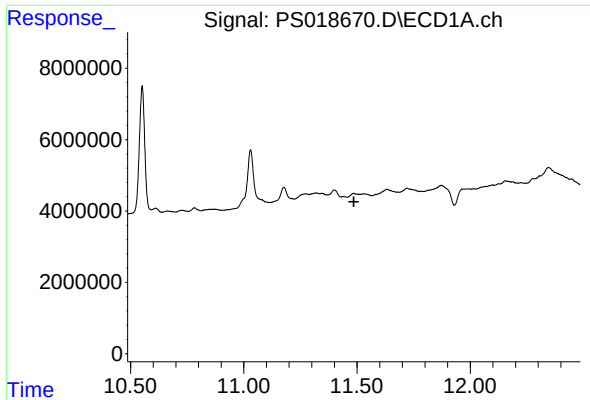

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

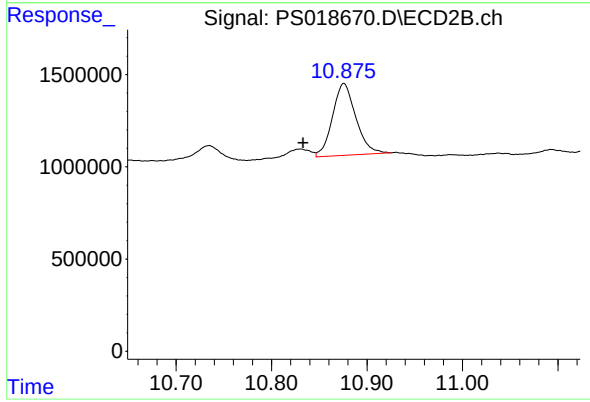

#16 DCPA

R.T.: 10.876 min
Delta R.T.: 0.043 min
Response: 6626684
Conc: 1.26 ng/ml