

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
 Data File : PS018681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 16:13
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:16:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.809	1651.2E6	466.8E6	580.200	663.443
Target Compounds							
3) T	4-Nitroph...	7.021f	6.474f	-3117233	4160128	N.D.	10.240
5) T	DICAMBA	7.484f	0.000	7447144	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.623	0	26074181	N.D.	32.938
9) T	2,4-D	8.409f	0.000	3779256	0	1.128	N.D. #
11) T	2,4,5-TP ...	9.167f	8.705	29260684	3968924	1.924	<MDL #
12) T	2,4,5-T	9.493	9.109f	3936141	1572957	<MDL	<MDL #
14) T	DINOSEB	11.179	0.000	663389	0	<MDL	N.D. #
15) T	Picloram	11.025	10.878	41822679	44997649	2.035	8.464 #
16) T	DCPA	11.536f	10.878f	5099699	44997649	<MDL	8.556 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
Data File : PS018681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 16:13
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:16:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

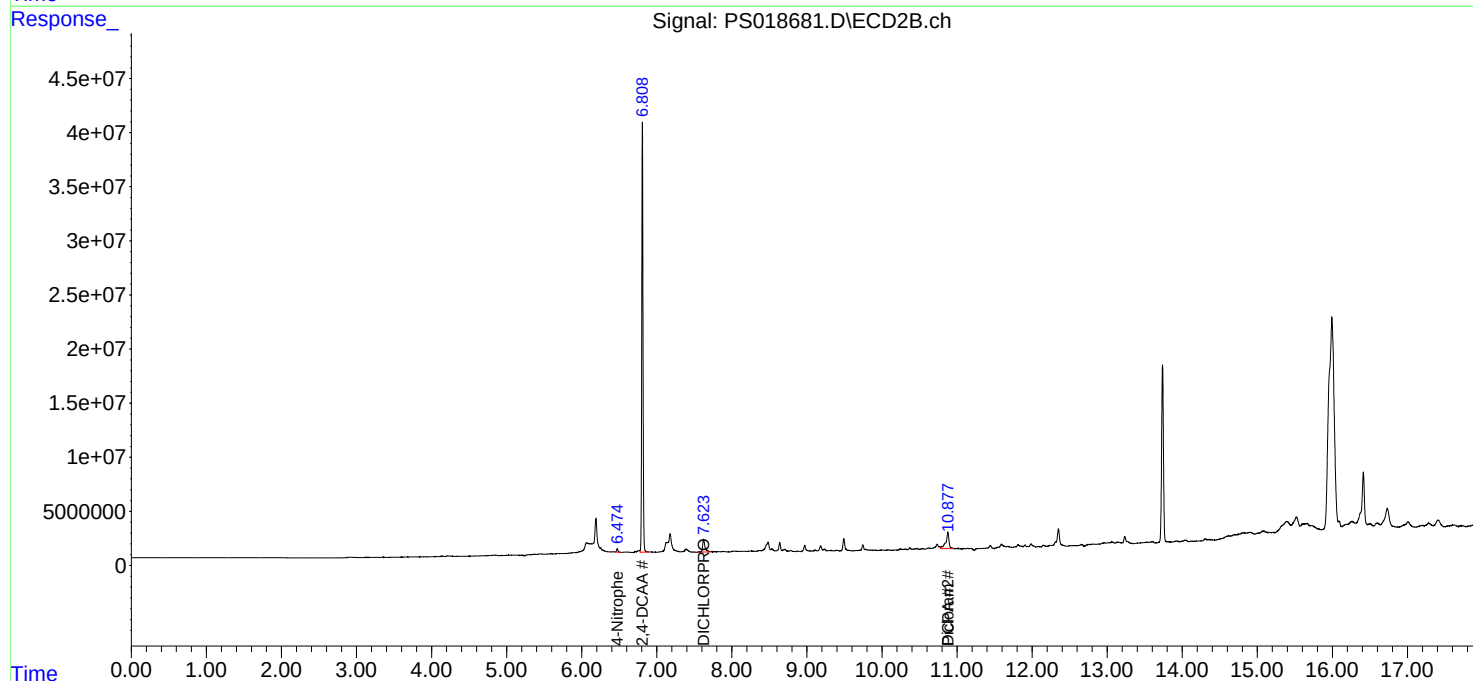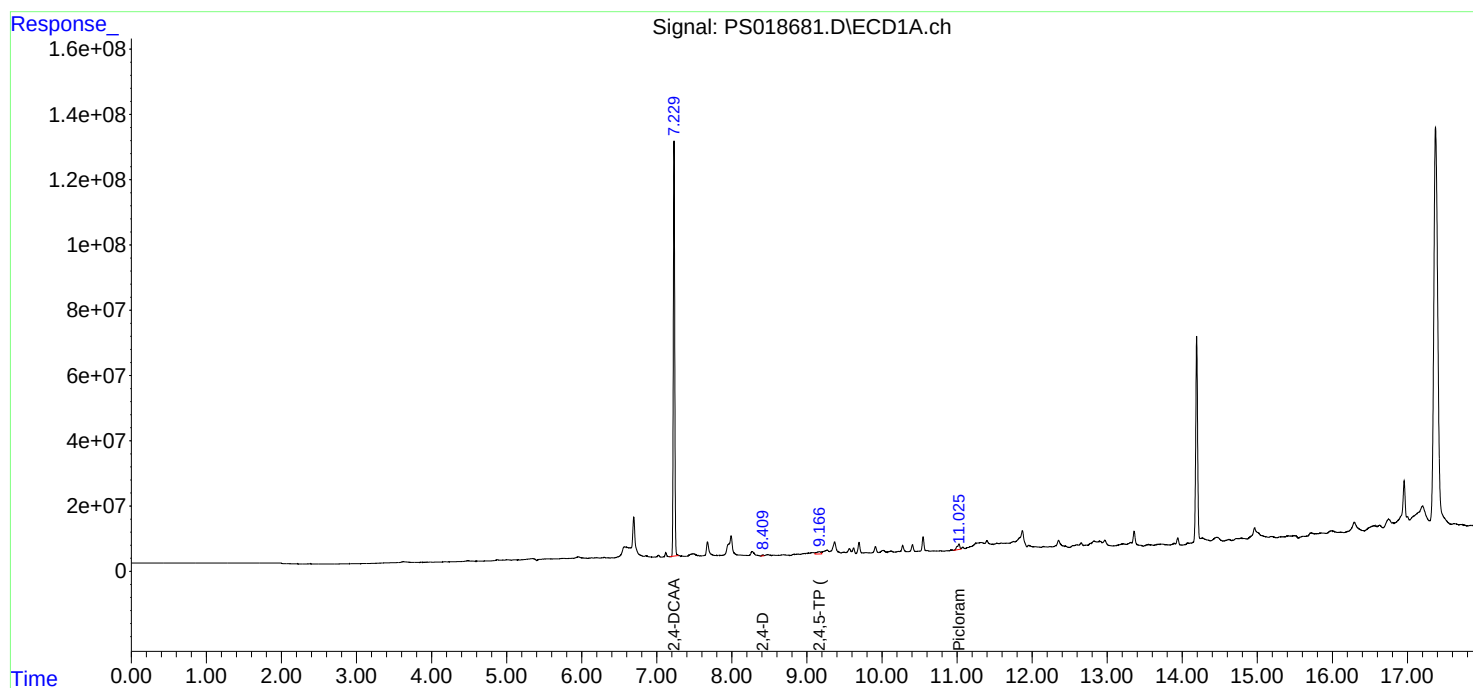


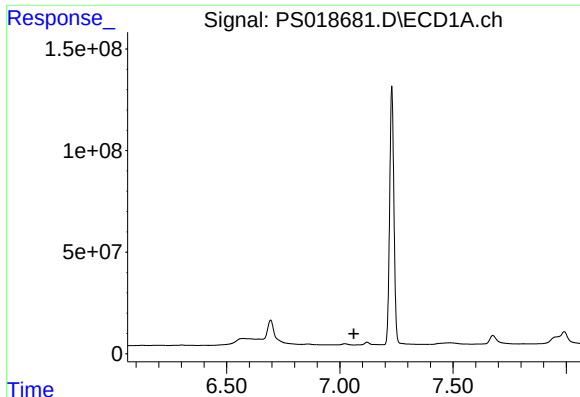

#3 4-Nitrophenol


R.T.: 7.021 min
Delta R.T.: -0.041 min
Response: -3117233
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

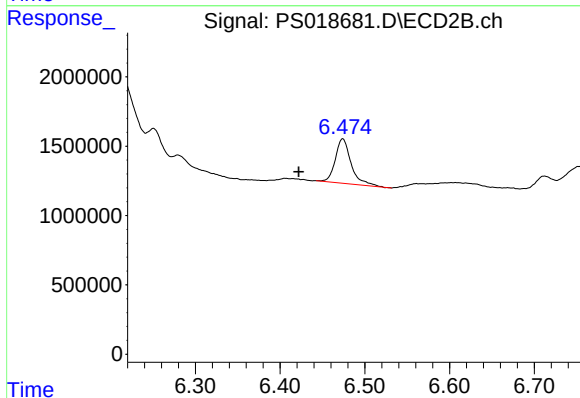


#3 4-Nitrophenol

R.T.: 6.474 min
Delta R.T.: 0.052 min
Response: 4160128
Conc: 10.24 ng/ml

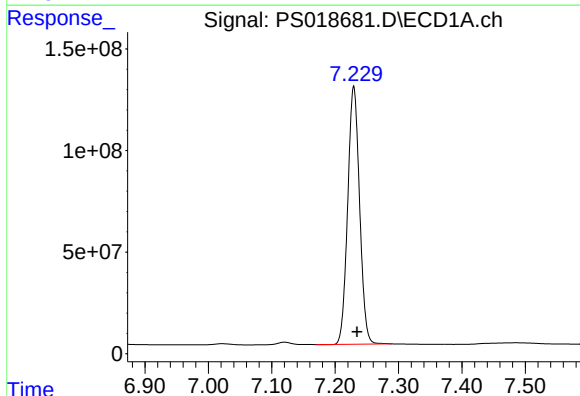


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: -0.006 min
Response: 1651199305
Conc: 580.20 ng/ml

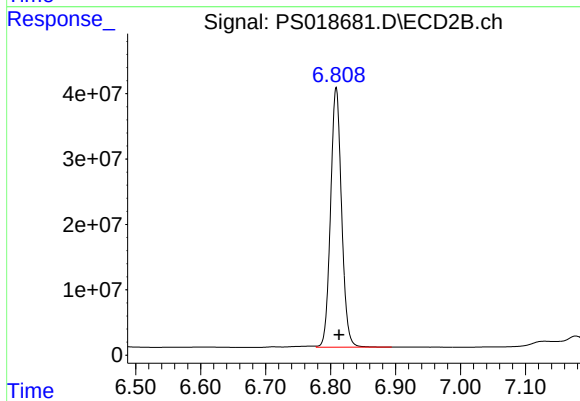

#4 2,4-DCAA


R.T.: 6.809 min
Delta R.T.: -0.004 min
Response: 466835109
Conc: 663.44 ng/ml

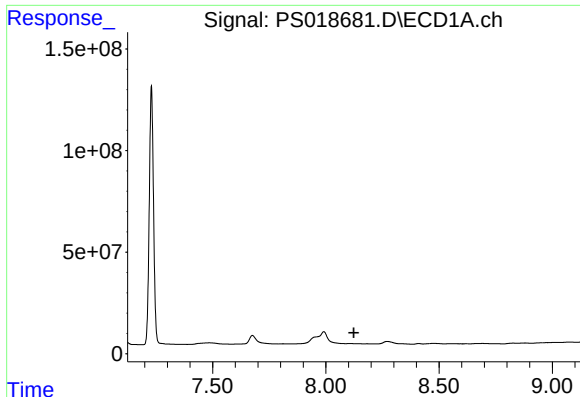

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

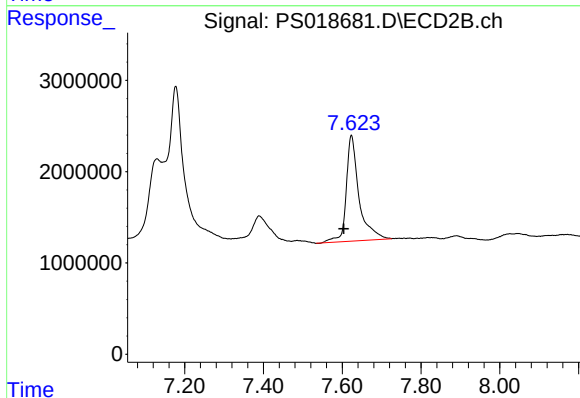


#8 DICHLORPROP

R.T.: 7.623 min
Delta R.T.: 0.019 min
Response: 26074181
Conc: 32.94 ng/ml

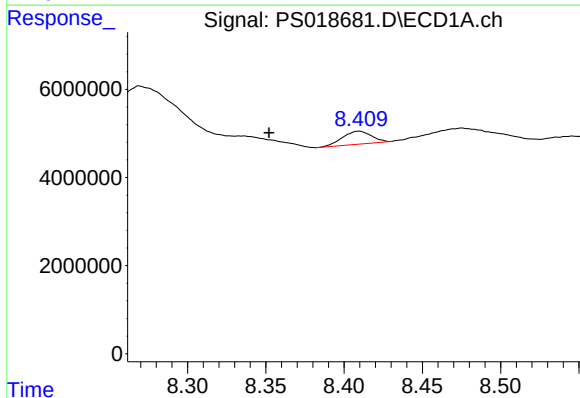


#9 2,4-D

R.T.: 8.409 min
Delta R.T.: 0.057 min
Response: 3779256
Conc: 1.13 ng/ml

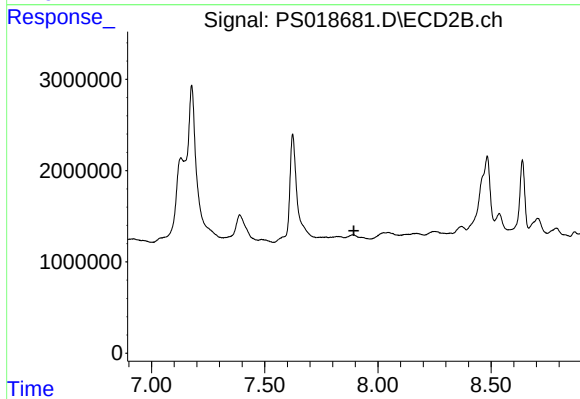

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

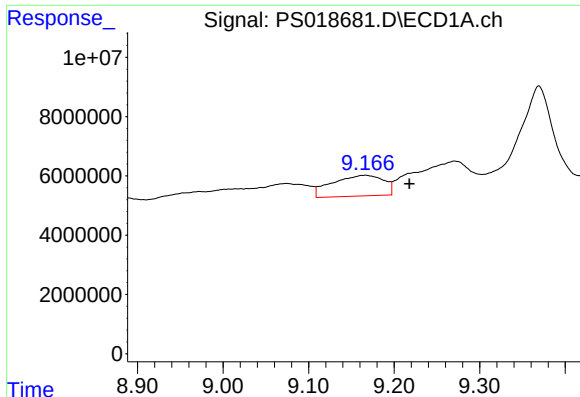

#11 2,4,5-TP (SILVEX)


R.T.: 9.167 min
Delta R.T.: -0.051 min
Response: 29260684
Conc: 1.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

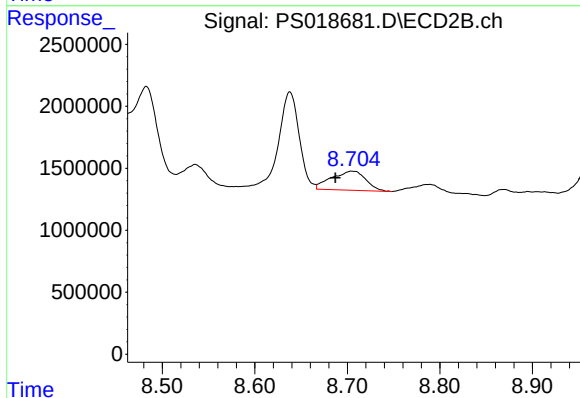


#11 2,4,5-TP (SILVEX)

R.T.: 8.705 min
Delta R.T.: 0.018 min
Response: 3968924
Conc: N.D.

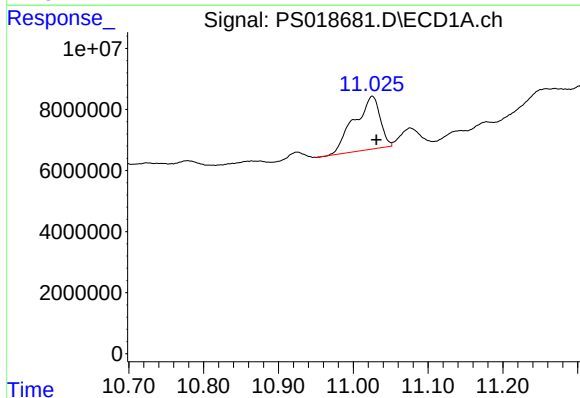


#15 Picloram

R.T.: 11.025 min
Delta R.T.: -0.006 min
Response: 41822679
Conc: 2.03 ng/ml

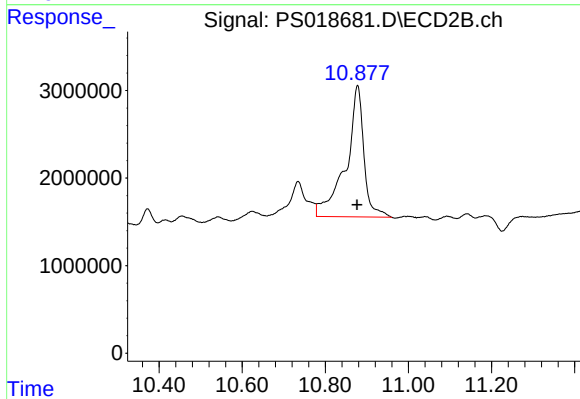

#15 Picloram


R.T.: 10.878 min
Delta R.T.: 0.002 min
Response: 44997649
Conc: 8.46 ng/ml

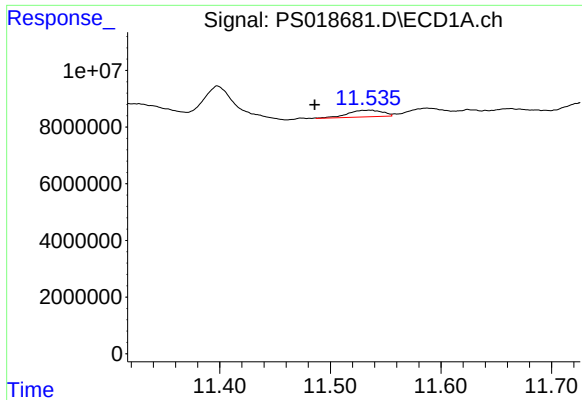

#16 DCPA

R.T.: 11.536 min
Delta R.T.: 0.050 min
Response: 5099699
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

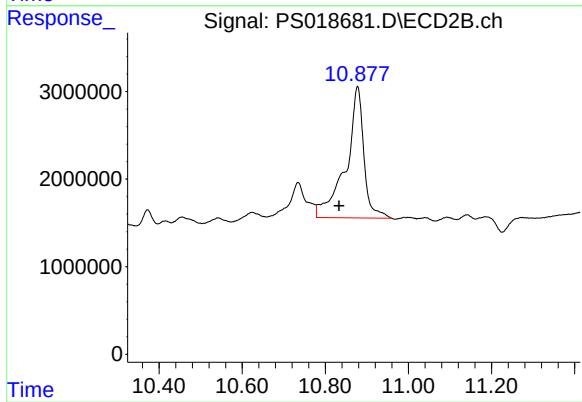

#16 DCPA

R.T.: 10.878 min
Delta R.T.: 0.045 min
Response: 44997649
Conc: 8.56 ng/ml