

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
 Data File : PS018693.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 22:58
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:20:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.809	1688.6E6	481.4E6	593.325	684.139
Target Compounds							
3) T	4-Nitroph...	7.021f	6.474f	2551000	4679299	1.480	11.518 #
5) T	DICAMBA	7.477f	0.000	6509803	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.622	0	23675047	N.D.	29.907
9) T	2,4-D	8.407f	0.000	3489366	0	1.041	N.D. #
11) T	2,4,5-TP ...	9.167f	8.707	42653382	4576269	2.805	1.049 #
12) T	2,4,5-T	9.564f	0.000	13939862	0	<MDL	N.D. #
14) T	DINOSEB	11.248	0.000	12328282	0	1.153	N.D. #
15) T	Picloram	11.024	10.878	21621490	43872182	1.052	8.253 #
16) T	DCPA	11.534f	10.792f	110.3E6	2472209	6.167	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
Data File : PS018693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 22:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:20:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

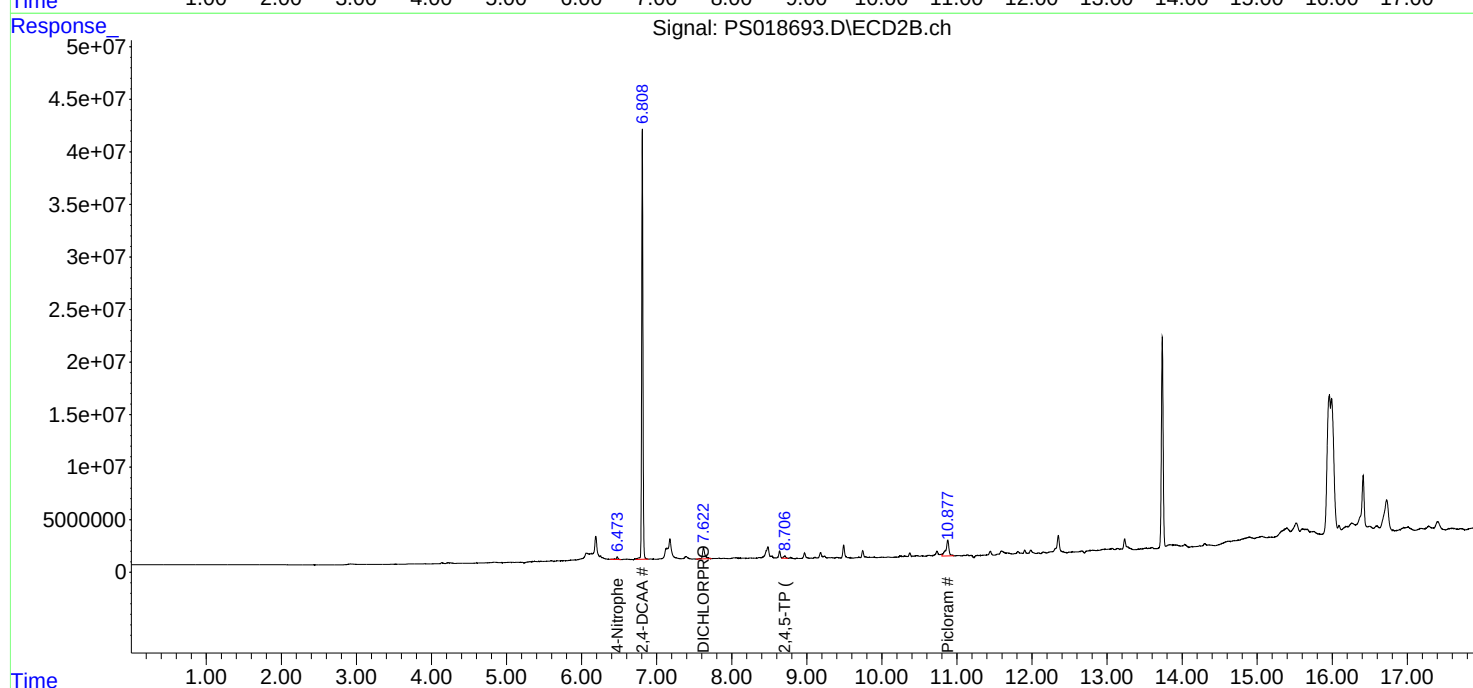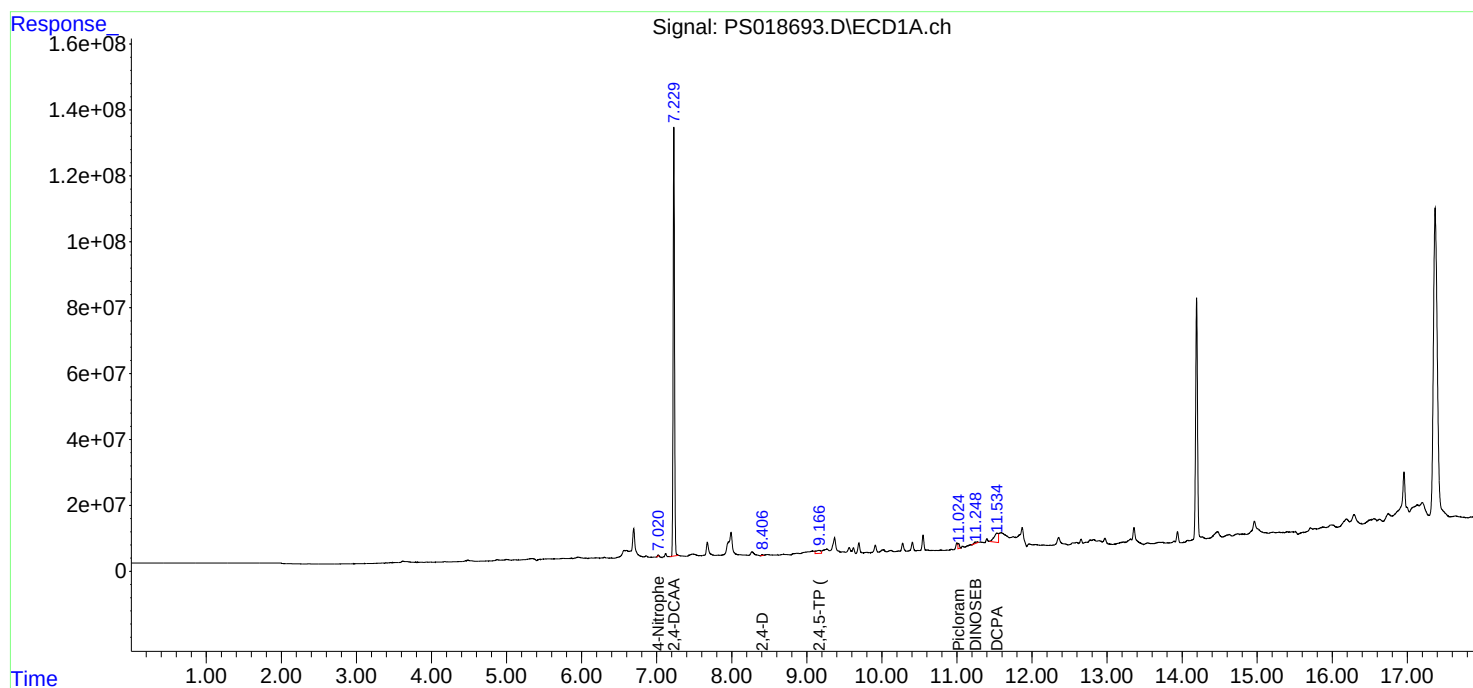


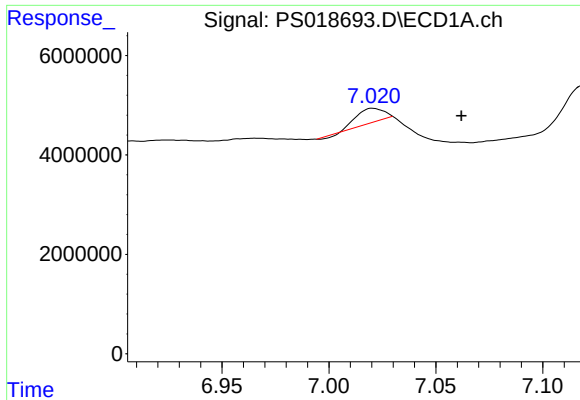

#3 4-Nitrophenol


R.T.: 7.021 min
Delta R.T.: -0.041 min
Response: 2551000
Conc: 1.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

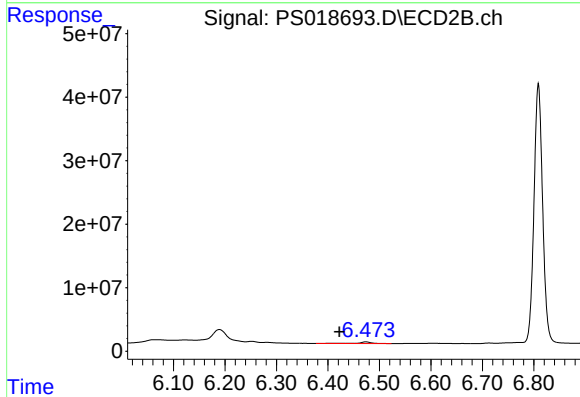


#3 4-Nitrophenol

R.T.: 6.474 min
Delta R.T.: 0.052 min
Response: 4679299
Conc: 11.52 ng/ml

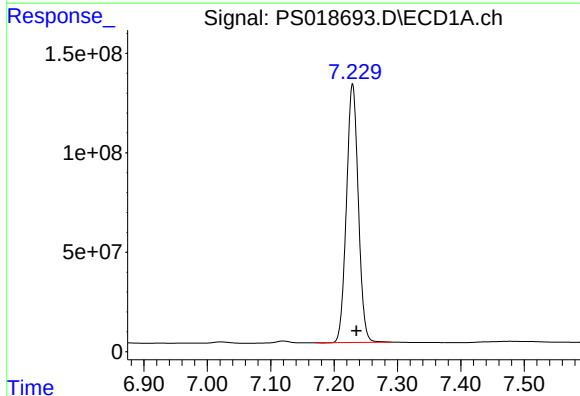


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: -0.006 min
Response: 1688554393
Conc: 593.33 ng/ml

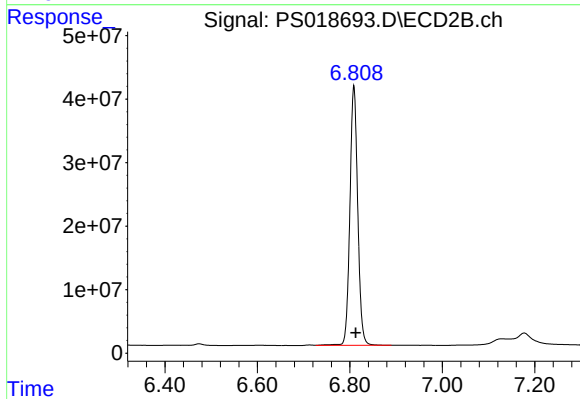

#4 2,4-DCAA


R.T.: 6.809 min
Delta R.T.: -0.004 min
Response: 481397587
Conc: 684.14 ng/ml

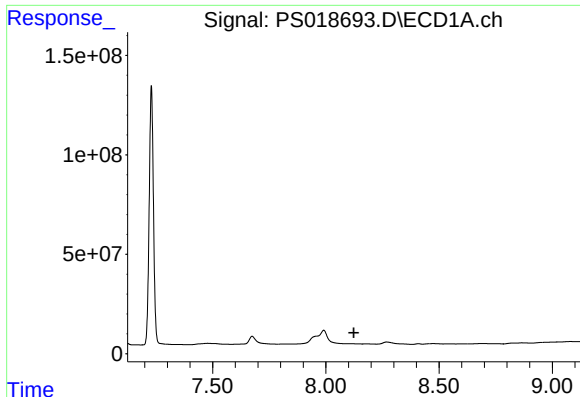

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

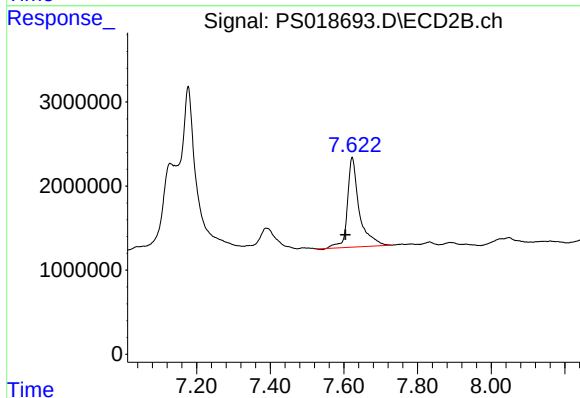


#8 DICHLORPROP

R.T.: 7.622 min
Delta R.T.: 0.018 min
Response: 23675047
Conc: 29.91 ng/ml

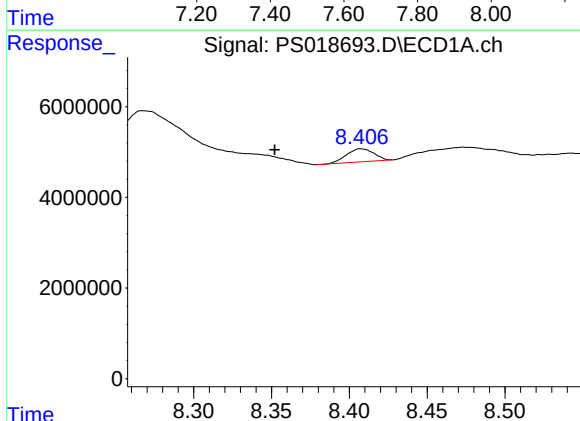


#9 2,4-D

R.T.: 8.407 min
Delta R.T.: 0.055 min
Response: 3489366
Conc: 1.04 ng/ml

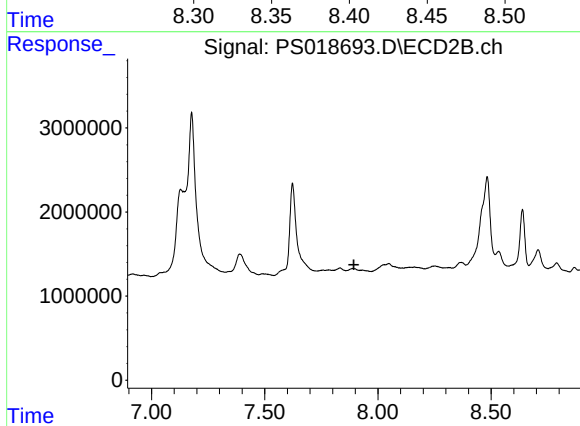

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

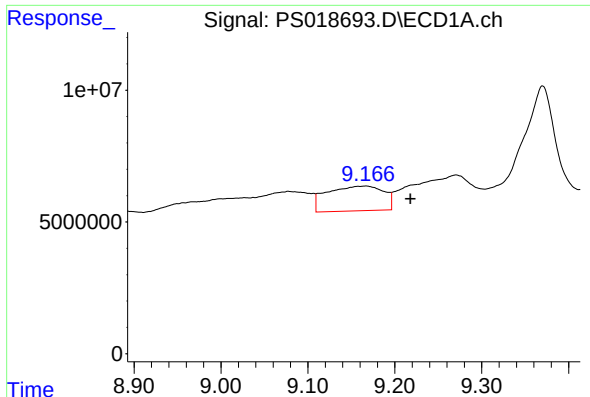

#11 2,4,5-TP (SILVEX)


R.T.: 9.167 min
Delta R.T.: -0.051 min
Response: 42653382
Conc: 2.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

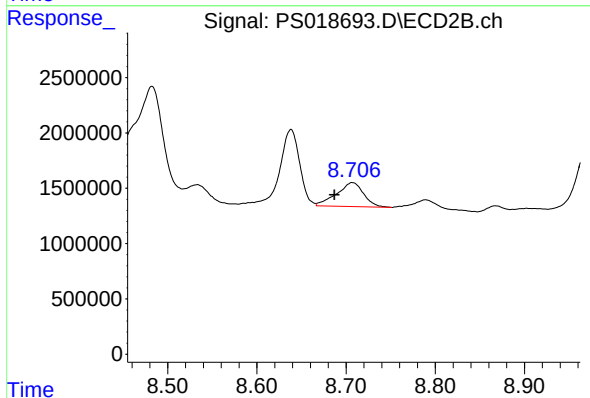


#11 2,4,5-TP (SILVEX)

R.T.: 8.707 min
Delta R.T.: 0.020 min
Response: 4576269
Conc: 1.05 ng/ml

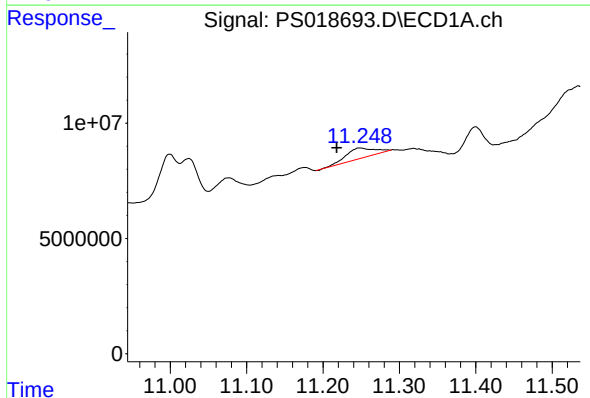


#14 DINOSEB

R.T.: 11.248 min
Delta R.T.: 0.030 min
Response: 12328282
Conc: 1.15 ng/ml

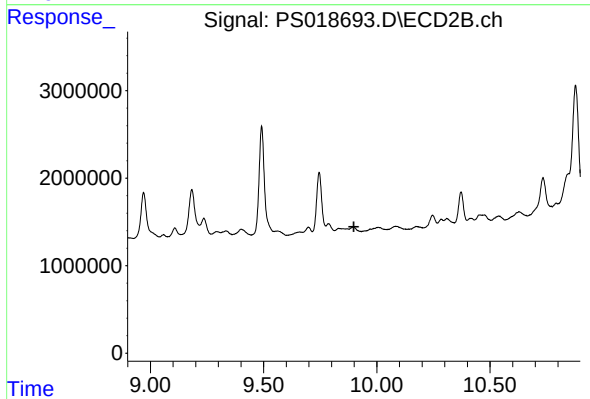

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.899 min
Response: 0
Conc: N.D.

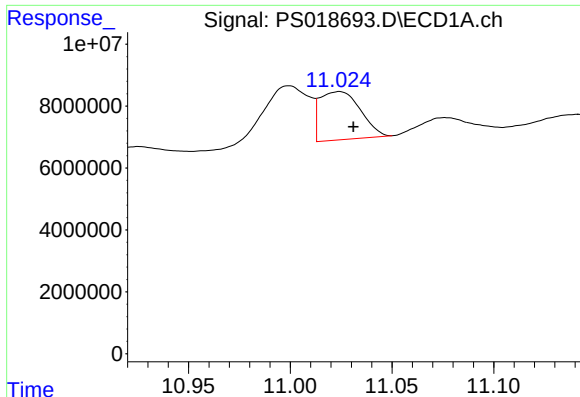

#15 Picloram


R.T.: 11.024 min
Delta R.T.: -0.007 min
Response: 21621490
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

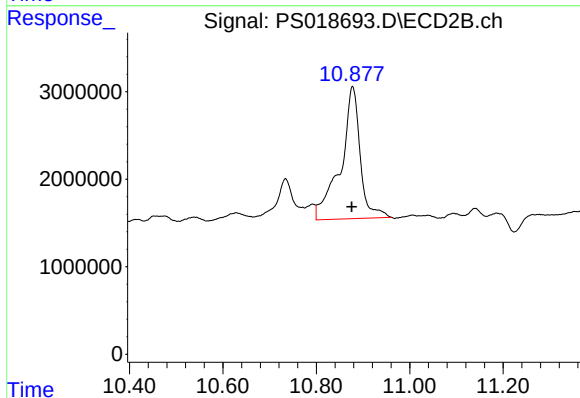


#15 Picloram

R.T.: 10.878 min
Delta R.T.: 0.002 min
Response: 43872182
Conc: 8.25 ng/ml

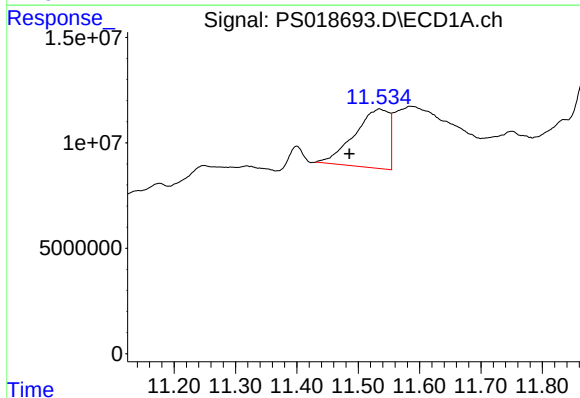

#16 DCPA

R.T.: 11.534 min
Delta R.T.: 0.048 min
Response: 110338517
Conc: 6.17 ng/ml

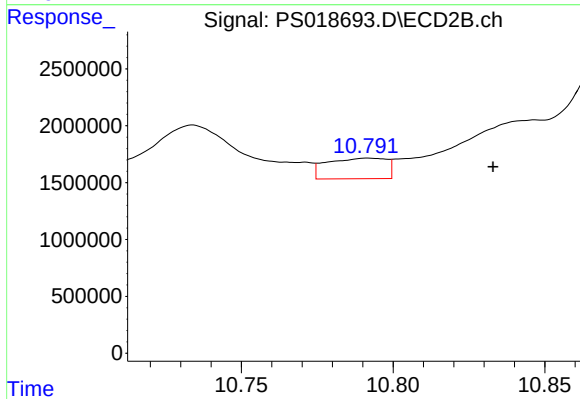

#16 DCPA

R.T.: 10.792 min
Delta R.T.: -0.041 min
Response: 2472209
Conc: N.D.