

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
 Data File : PS018703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 04:32
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 05:21:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.809	1718.7E6	492.6E6	603.930	700.037
Target Compounds							
8) T	DICHLORPROP	0.000	7.622	0	13876063	N.D.	17.529
9) T	2,4-D	8.411f	0.000	1639250	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.271f	8.638f	19668587	8656573	1.293	1.985 #
12) T	2,4,5-T	9.493	0.000	5242046	0	<MDL	N.D. #
15) T	Picloram	11.028	10.877	32916163	9685276	1.601	1.822
16) T	DCPA	0.000	10.877f	0	9685276	N.D.	1.842



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
Data File : PS018703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 04:32
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 05:21:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

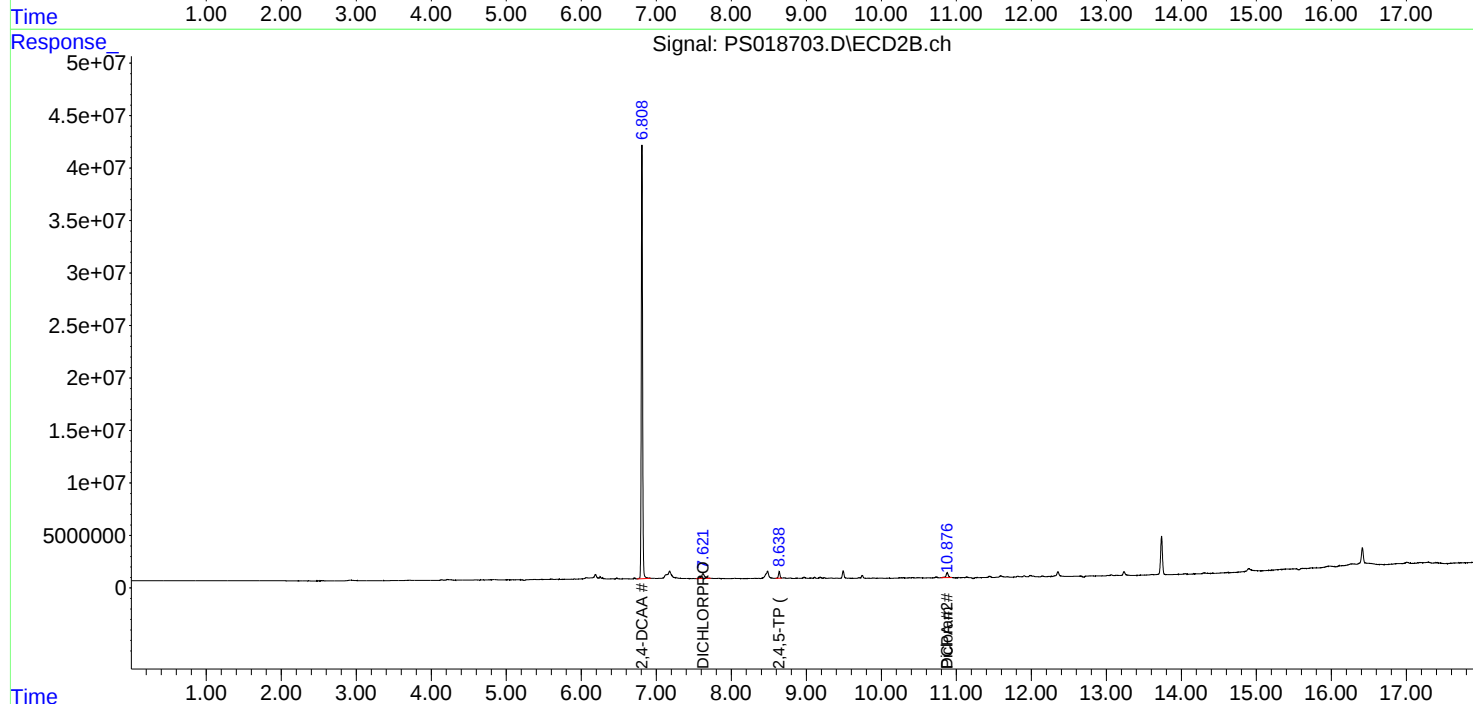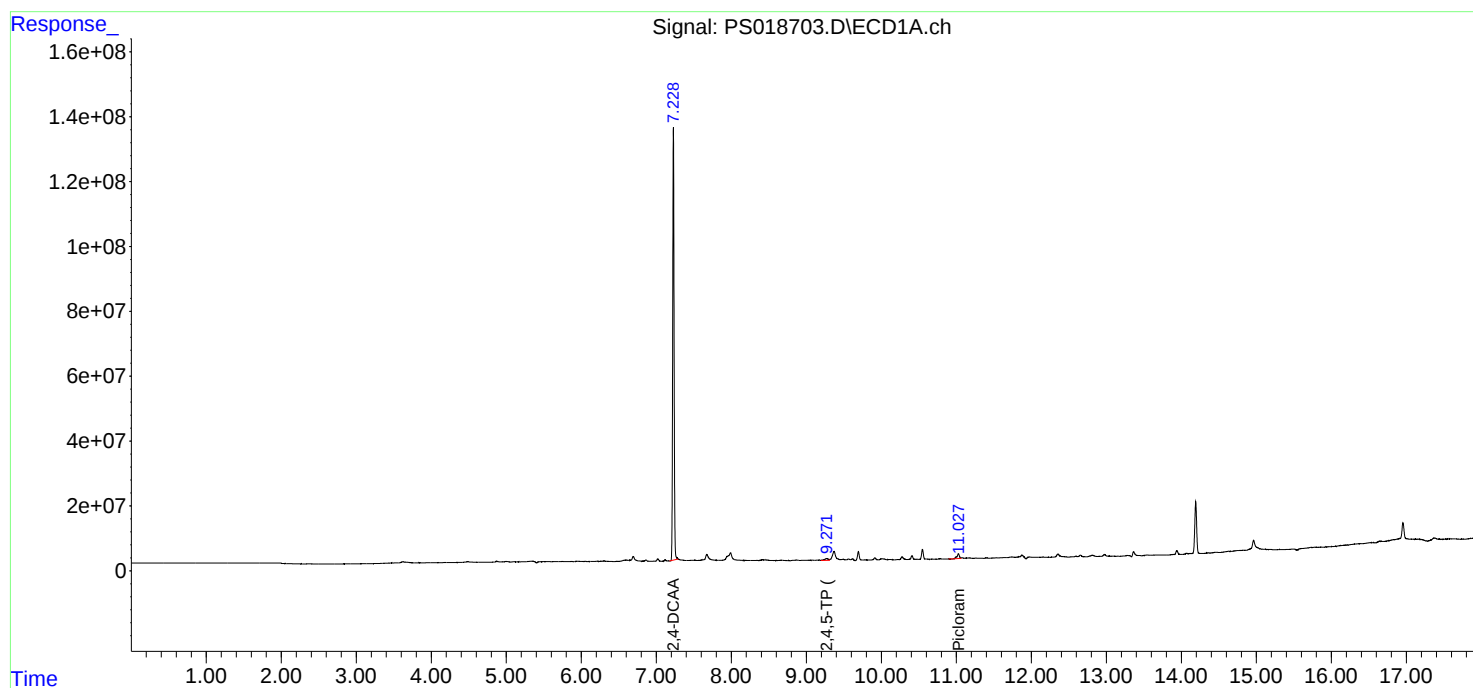


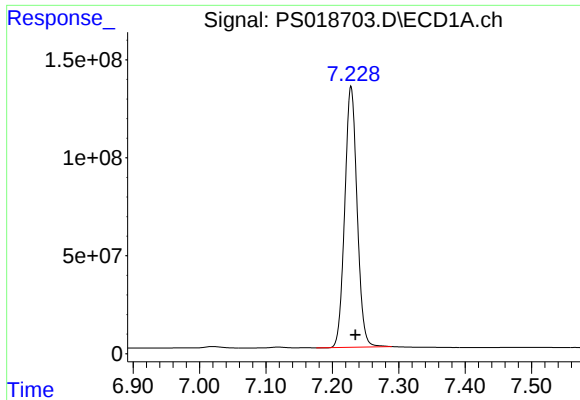

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: -0.007 min
Response: 1718734518
Conc: 603.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

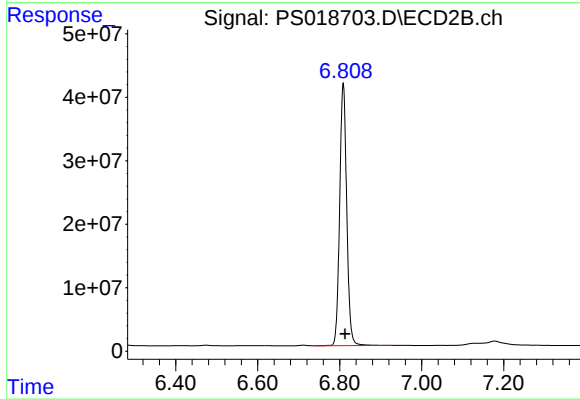


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.004 min
Response: 492584245
Conc: 700.04 ng/ml

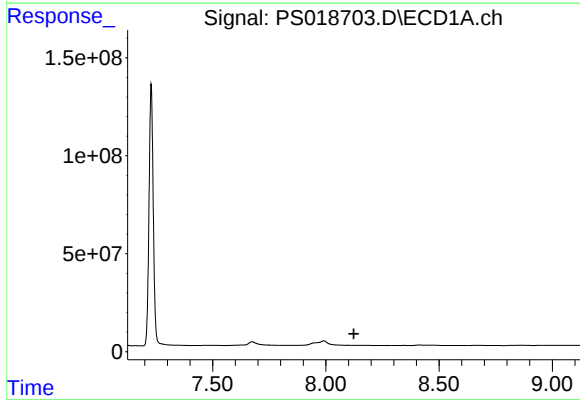


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.124 min
Response: 0
Conc: N.D.

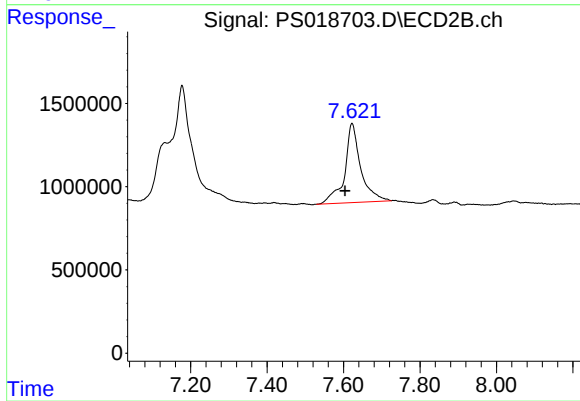

#8 DICHLORPROP


R.T.: 7.622 min
Delta R.T.: 0.018 min
Response: 13876063
Conc: 17.53 ng/ml

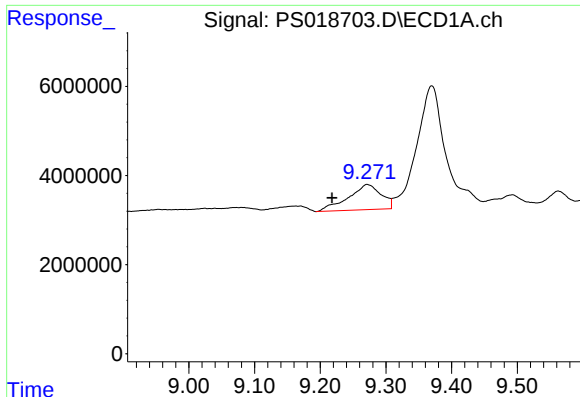

#11 2,4,5-TP (SILVEX)


R.T.: 9.271 min
Delta R.T.: 0.053 min
Response: 19668587
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

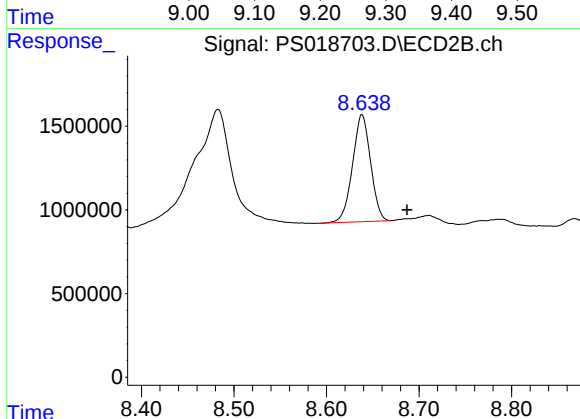


#11 2,4,5-TP (SILVEX)

R.T.: 8.638 min
Delta R.T.: -0.049 min
Response: 8656573
Conc: 1.98 ng/ml

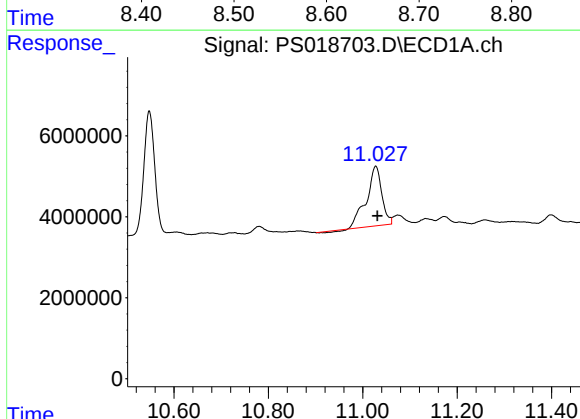


#15 Picloram

R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 32916163
Conc: 1.60 ng/ml

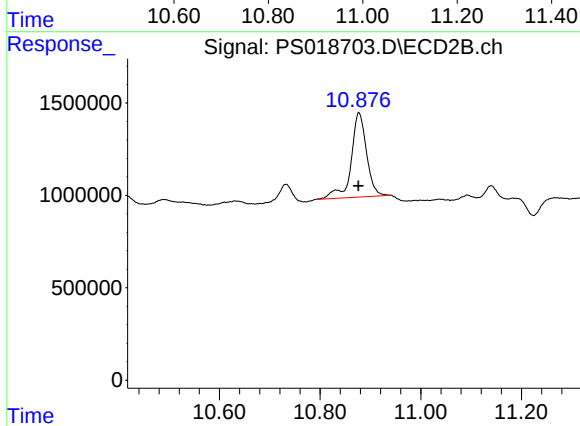

#15 Picloram


R.T.: 10.877 min
Delta R.T.: 0.001 min
Response: 9685276
Conc: 1.82 ng/ml

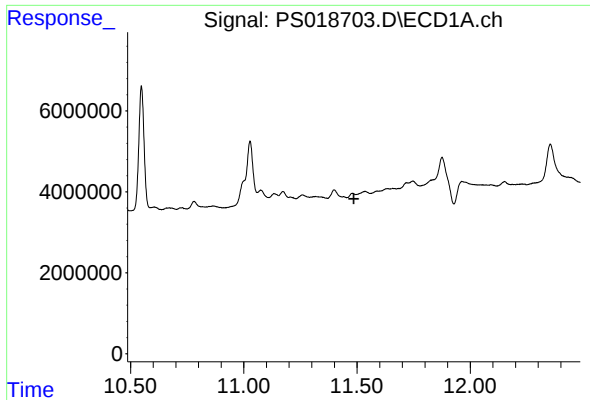

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

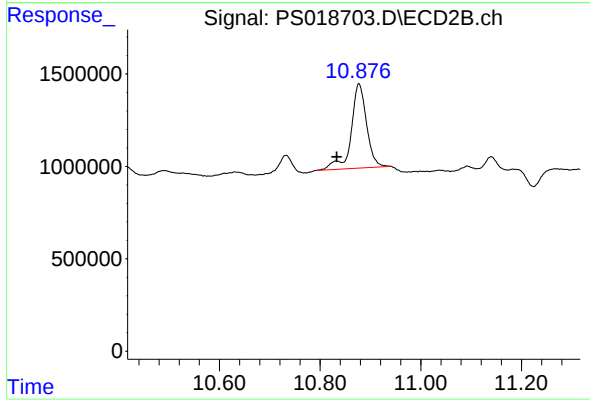

#16 DCPA

R.T.: 10.877 min
Delta R.T.: 0.044 min
Response: 9685276
Conc: 1.84 ng/ml