

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
 Data File : PS018715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 11:17
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 14:09:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.808	1795.5E6	518.3E6	630.891	736.599
Target Compounds							
3) T	4-Nitroph...	7.019f	6.473f	-3838142	2695041	N.D.	6.634
8) T	DICHLORPROP	0.000	7.623	0	44053413	N.D.	55.650
9) T	2,4-D	8.407f	0.000	1400810	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.270f	8.637f	58663442	9416527	3.857	2.159 #
12) T	2,4,5-T	9.489	9.108f	3828681	1486321	<MDL	<MDL #
14) T	DINOSEB	11.253	0.000	11012715	0	1.030	N.D. #
15) T	Picloram	11.024	10.878	24187979	32283378	1.177	6.073 #
16) T	DCPA	0.000	10.878f	0	32283378	N.D.	6.138



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
Data File : PS018715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 11:17
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 14:09:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

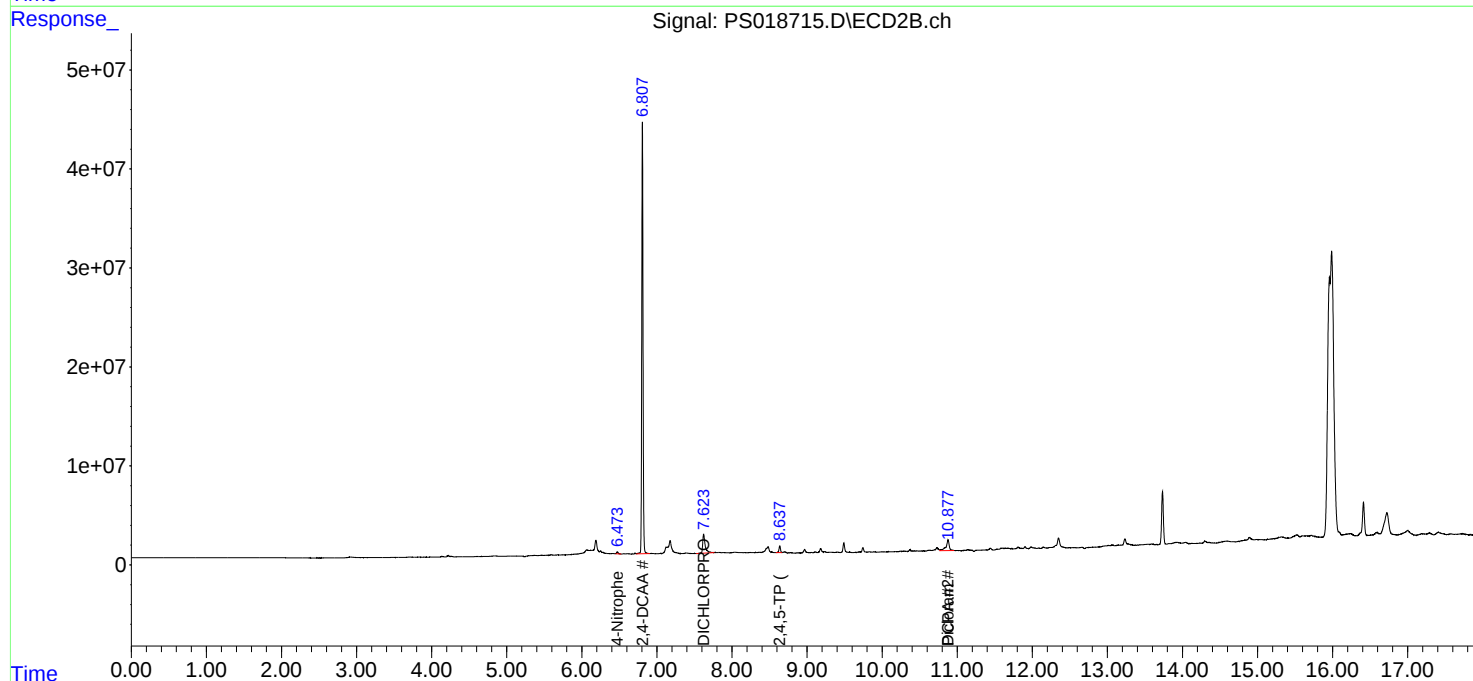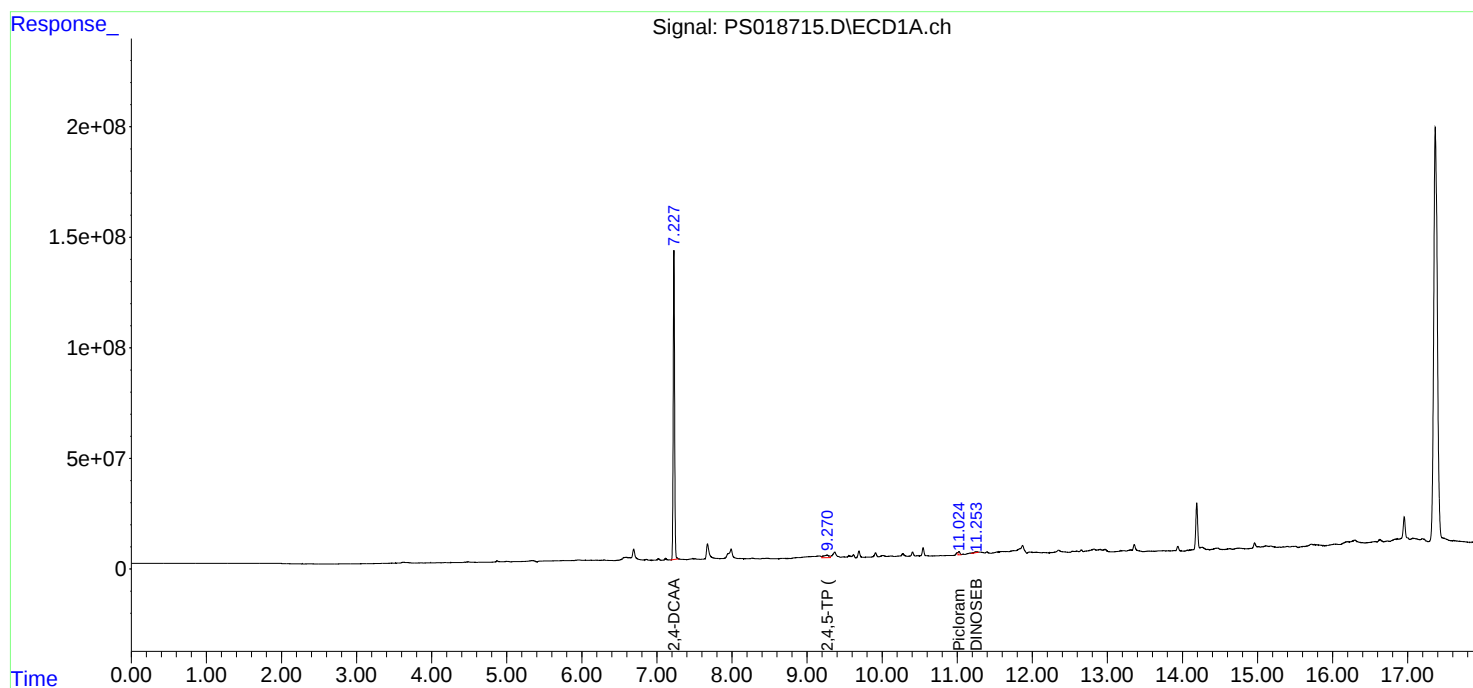


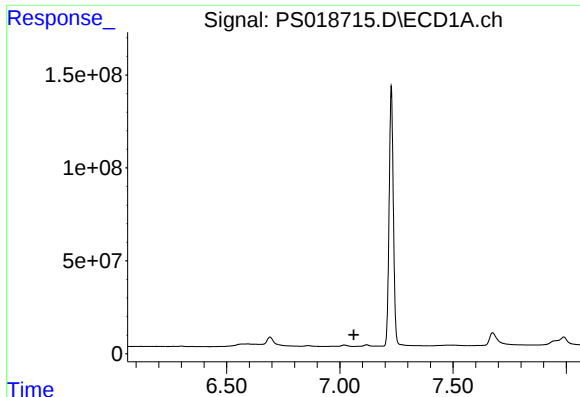

#3 4-Nitrophenol


R.T.: 7.019 min
Delta R.T.: -0.043 min
Response: -3838142
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

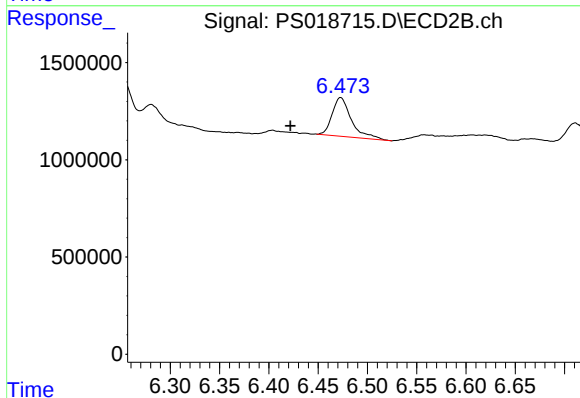


#3 4-Nitrophenol

R.T.: 6.473 min
Delta R.T.: 0.051 min
Response: 2695041
Conc: 6.63 ng/ml

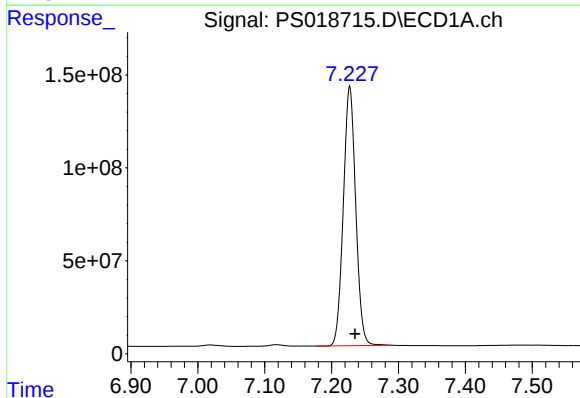


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: -0.008 min
Response: 1795463841
Conc: 630.89 ng/ml

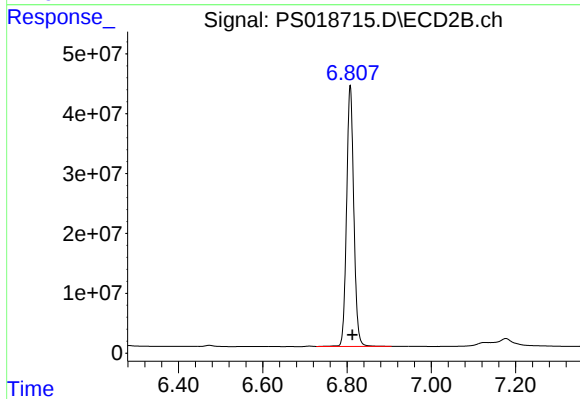

#4 2,4-DCAA


R.T.: 6.808 min
Delta R.T.: -0.005 min
Response: 518311374
Conc: 736.60 ng/ml

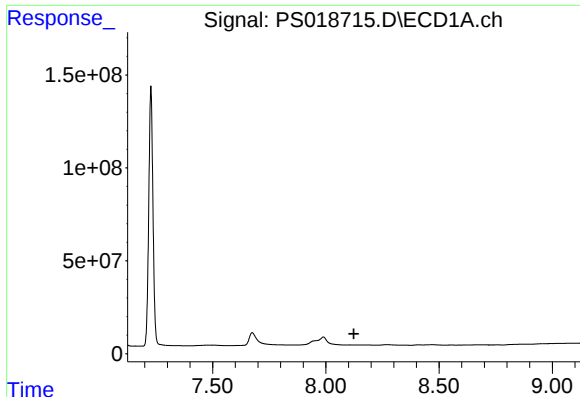

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

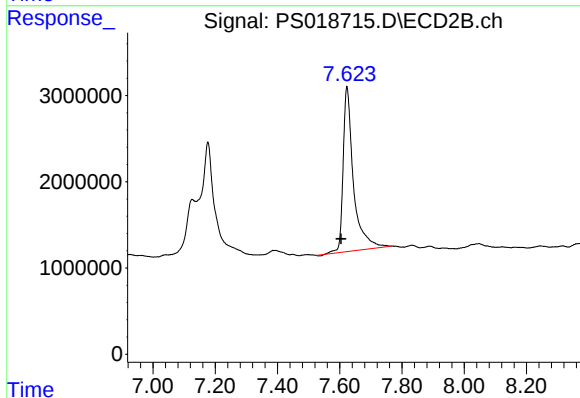


#8 DICHLORPROP

R.T.: 7.623 min
Delta R.T.: 0.019 min
Response: 44053413
Conc: 55.65 ng/ml

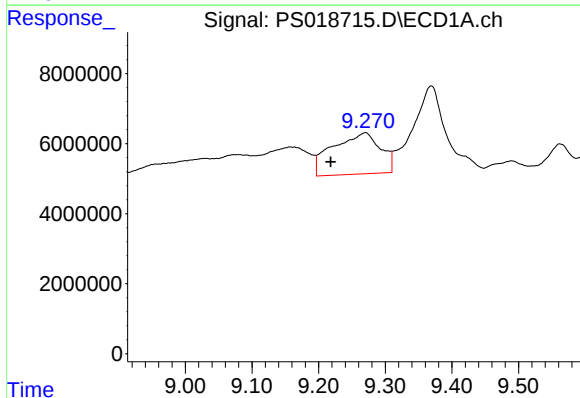


#11 2,4,5-TP (SILVEX)

R.T.: 9.270 min
Delta R.T.: 0.052 min
Response: 58663442
Conc: 3.86 ng/ml

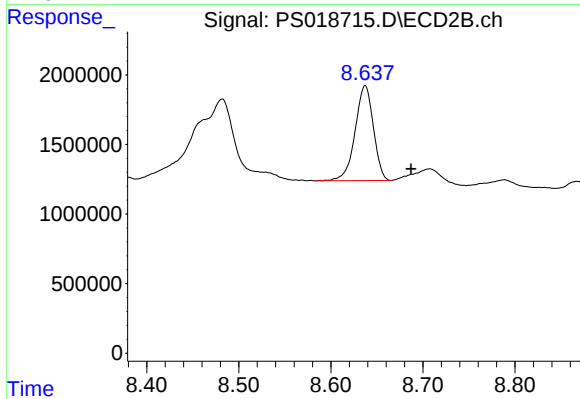

#11 2,4,5-TP (SILVEX)


R.T.: 8.637 min
Delta R.T.: -0.050 min
Response: 9416527
Conc: 2.16 ng/ml

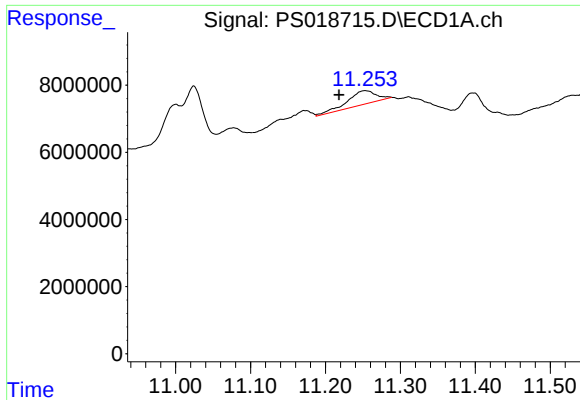

#14 DINoseb


R.T.: 11.253 min
Delta R.T.: 0.035 min
Response: 11012715
Conc: 1.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

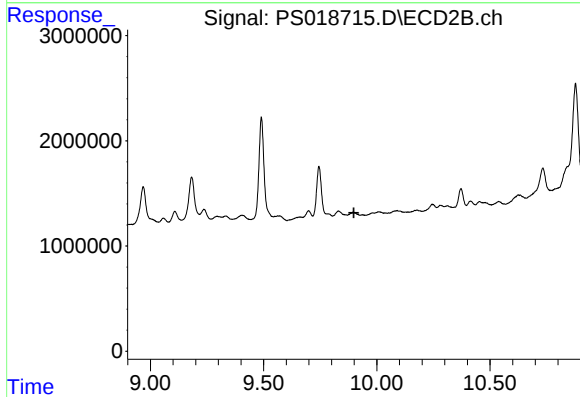


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.899 min
Response: 0
Conc: N.D.

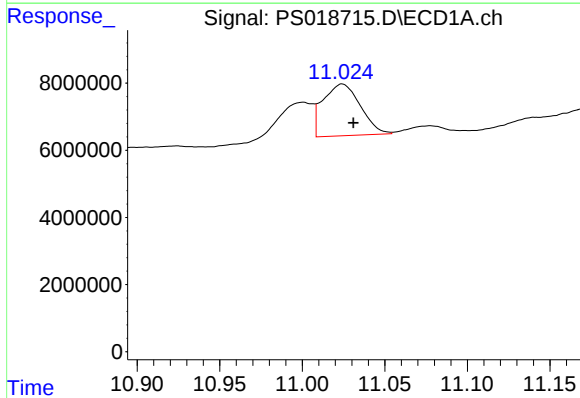


#15 Picloram

R.T.: 11.024 min
Delta R.T.: -0.007 min
Response: 24187979
Conc: 1.18 ng/ml

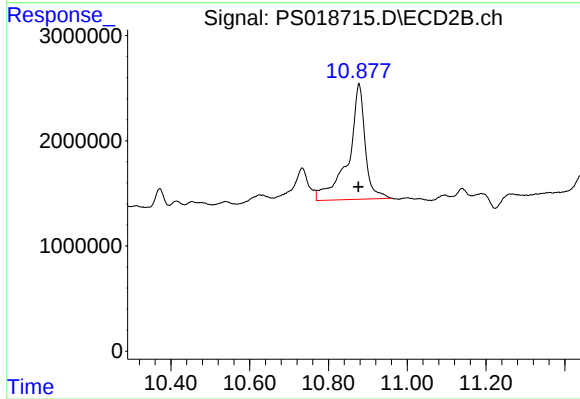

#15 Picloram


R.T.: 10.878 min
Delta R.T.: 0.002 min
Response: 32283378
Conc: 6.07 ng/ml

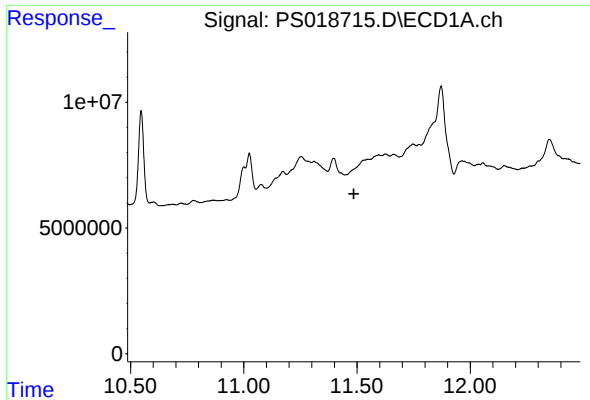

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

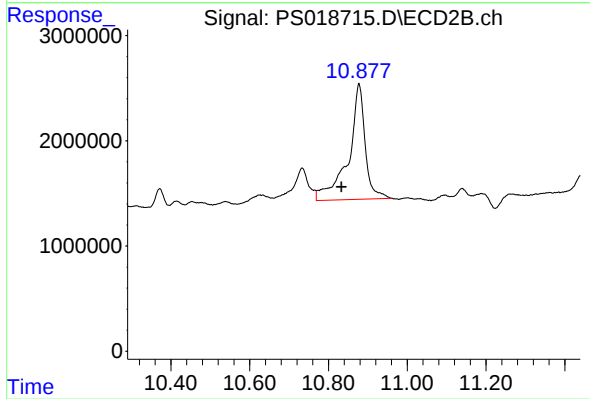

#16 DCPA

R.T.: 10.878 min
Delta R.T.: 0.045 min
Response: 32283378
Conc: 6.14 ng/ml