

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
 Data File : PS018719.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 13:39
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 14:10:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.808	1826.6E6	530.0E6	641.824	753.207
Target Compounds							
3) T	4-Nitroph...	7.019f	6.474f	4087133	3517698	2.372	8.658 #
5) T	DICAMBA	7.494f	0.000	9213188	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.621	0	18630580	N.D.	23.535
9) T	2,4-D	8.408f	0.000	2976571	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.268f	8.706	50325165	4374053	3.309	1.003 #
12) T	2,4,5-T	9.491	9.109f	4105240	1395338	<MDL	<MDL #
14) T	DINOSEB	11.257	0.000	15453129	0	1.445	N.D. #
15) T	Picloram	11.023	10.878	22381626	33029572	1.089	6.213 #
16) T	DCPA	11.529f	10.878f	42615392	33029572	2.382	6.280 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032222\
Data File : PS018719.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 13:39
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 14:10:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

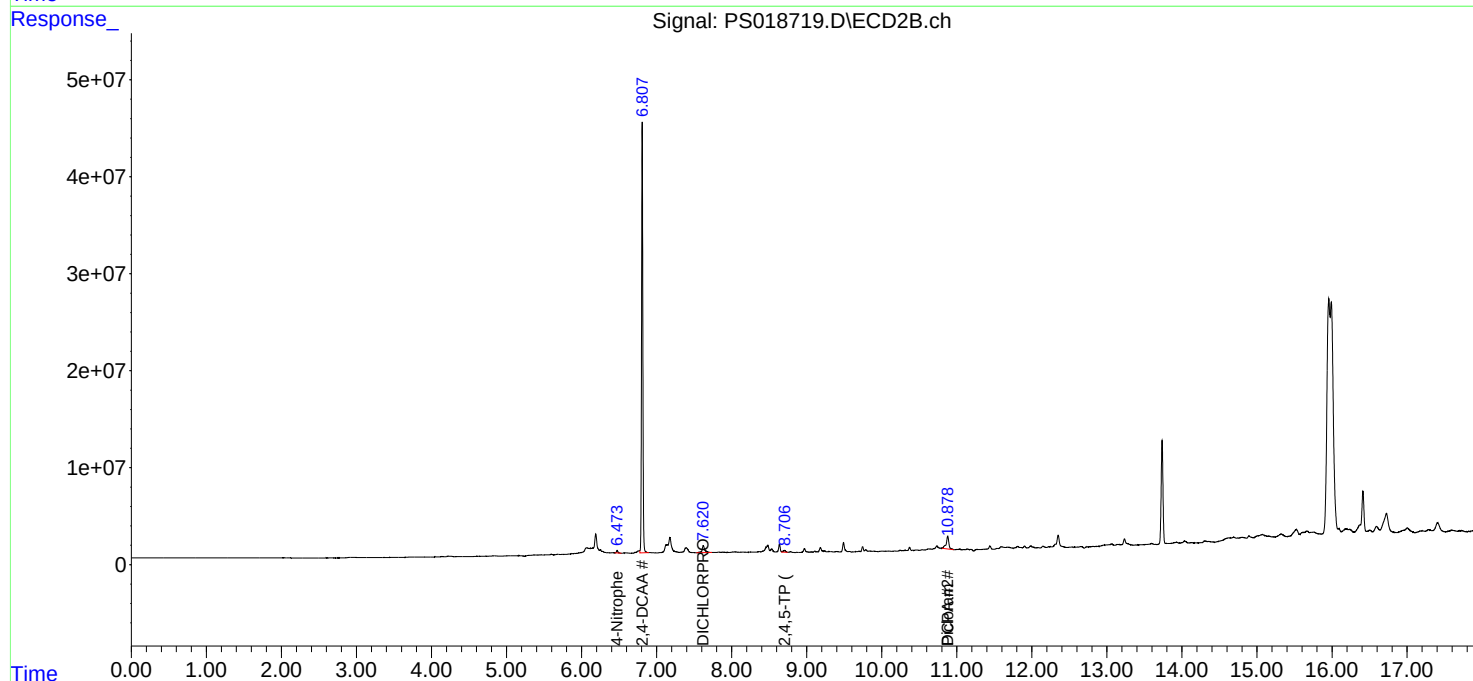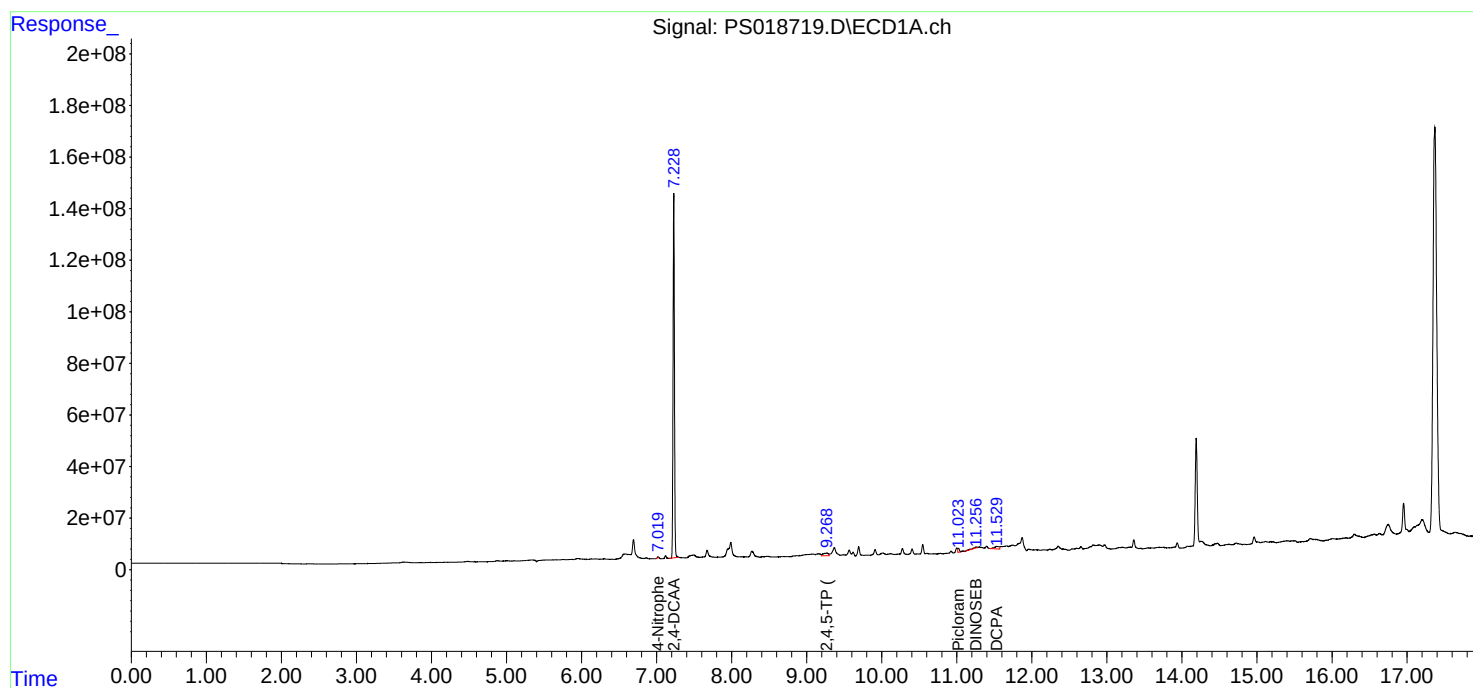


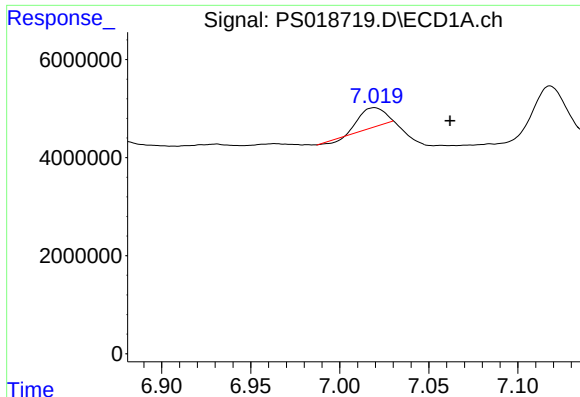

#3 4-Nitrophenol


R.T.: 7.019 min
Delta R.T.: -0.043 min
Response: 4087133
Conc: 2.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

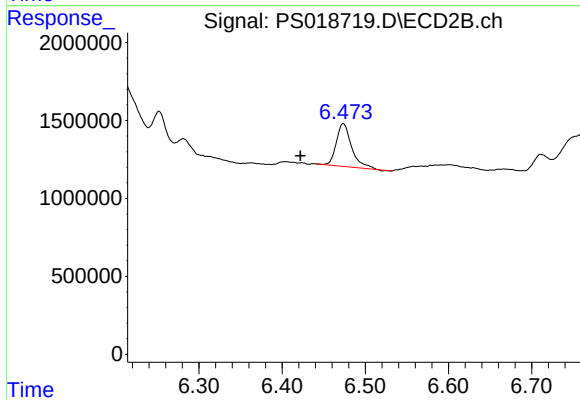


#3 4-Nitrophenol

R.T.: 6.474 min
Delta R.T.: 0.052 min
Response: 3517698
Conc: 8.66 ng/ml

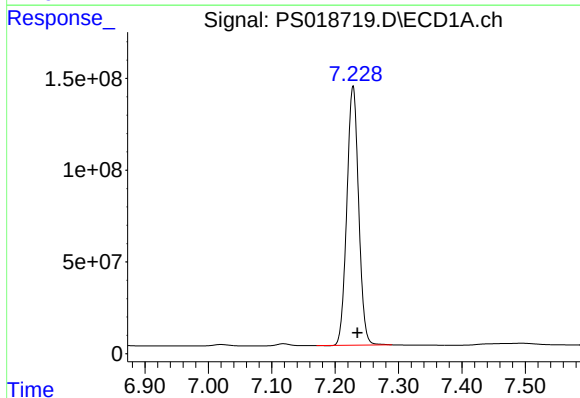


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.007 min
Response: 1826576762
Conc: 641.82 ng/ml

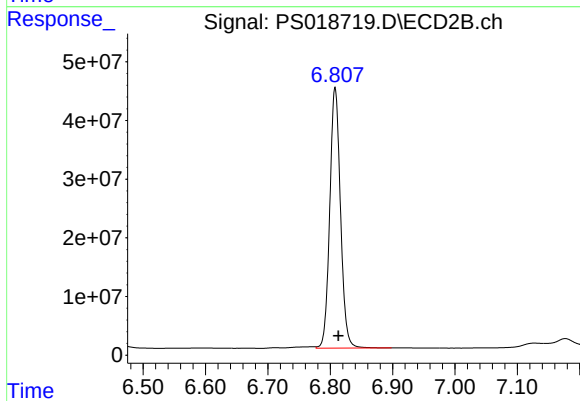

#4 2,4-DCAA


R.T.: 6.808 min
Delta R.T.: -0.005 min
Response: 529997833
Conc: 753.21 ng/ml

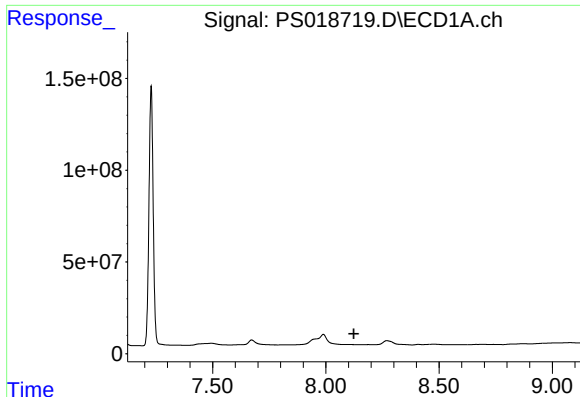

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

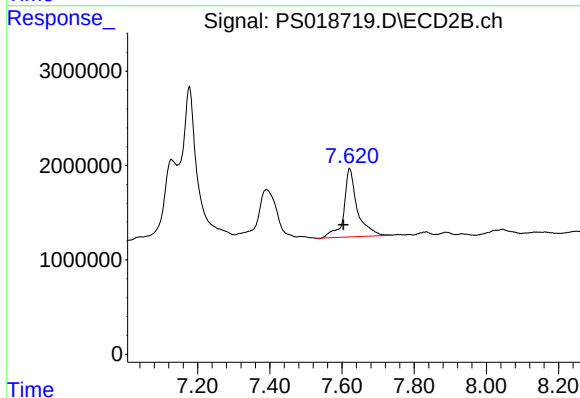


#8 DICHLORPROP

R.T.: 7.621 min
Delta R.T.: 0.017 min
Response: 18630580
Conc: 23.53 ng/ml

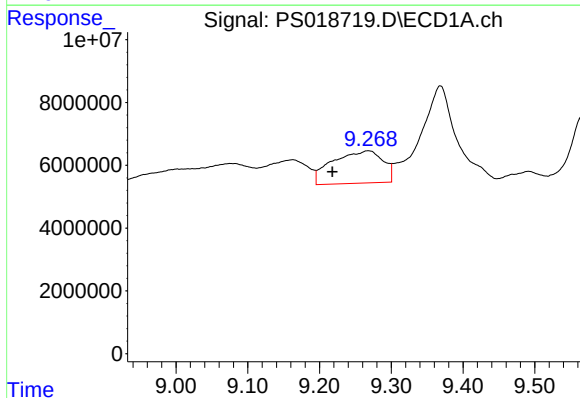


#11 2,4,5-TP (SILVEX)

R.T.: 9.268 min
Delta R.T.: 0.050 min
Response: 50325165
Conc: 3.31 ng/ml

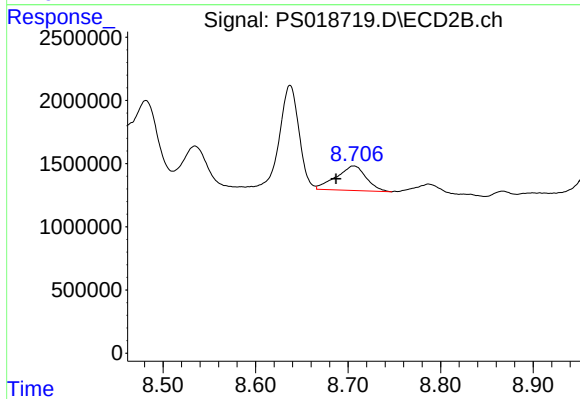

#11 2,4,5-TP (SILVEX)


R.T.: 8.706 min
Delta R.T.: 0.019 min
Response: 4374053
Conc: 1.00 ng/ml

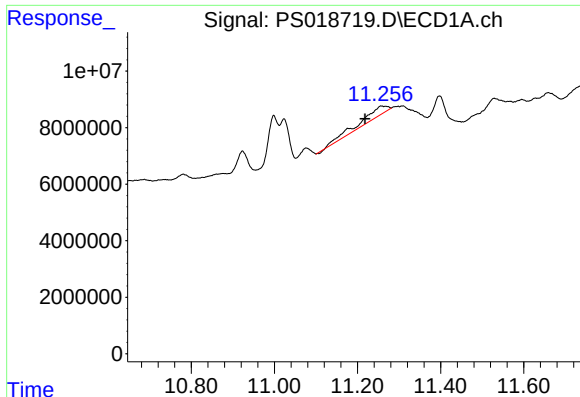

#14 DINoseb


R.T.: 11.257 min
Delta R.T.: 0.039 min
Response: 15453129
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

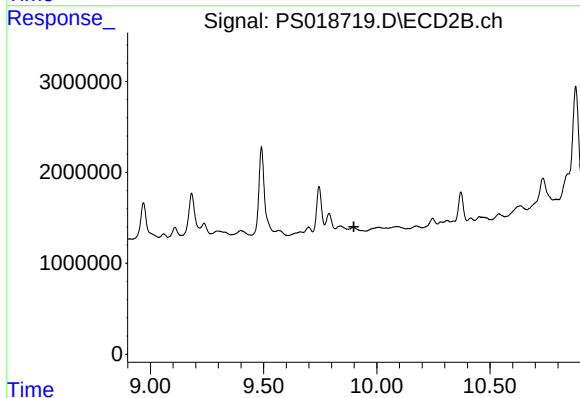


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.899 min
Response: 0
Conc: N.D.

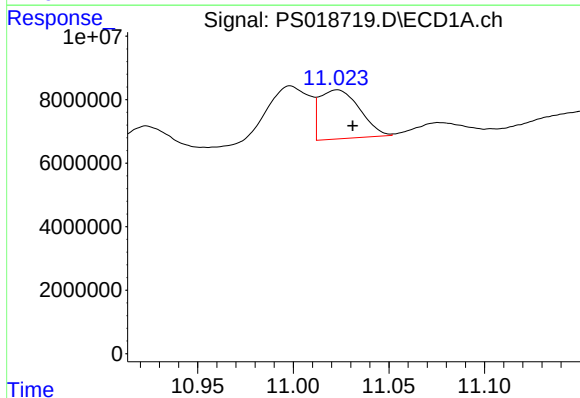


#15 Picloram

R.T.: 11.023 min
Delta R.T.: -0.008 min
Response: 22381626
Conc: 1.09 ng/ml

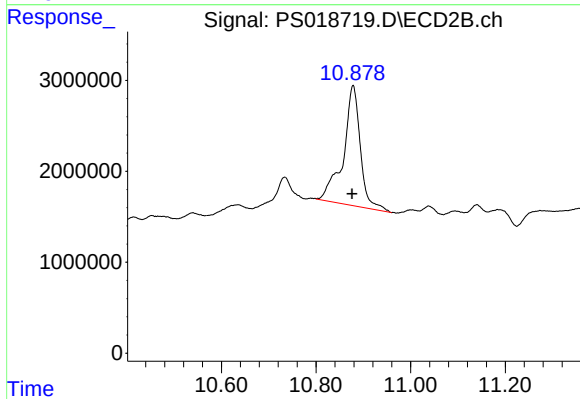

#15 Picloram


R.T.: 10.878 min
Delta R.T.: 0.002 min
Response: 33029572
Conc: 6.21 ng/ml

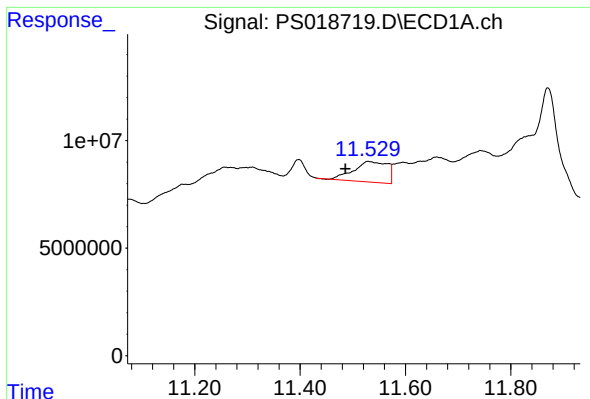

#16 DCPA

R.T.: 11.529 min
Delta R.T.: 0.043 min
Response: 42615392
Conc: 2.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

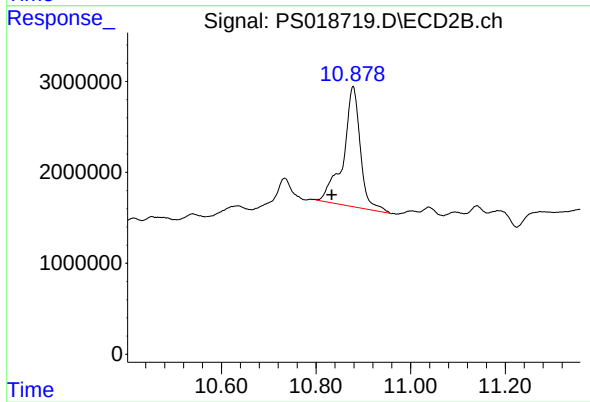

#16 DCPA

R.T.: 10.878 min
Delta R.T.: 0.045 min
Response: 33029572
Conc: 6.28 ng/ml