

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032223\
 Data File : PS022462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2023 18:48
 Operator : AR\AJ
 Sample : 02001-07MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 21:17:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.294	6.717	1072.5E6	856.4E6	438.749	415.796
Target Compounds							
2) T	3,5-DICHL...	5.677	5.919	1126.2E6	1025.9E6	302.465	321.699
3) T	4-Nitroph...	6.135	6.342	737.9E6	577.7E6	538.521	411.488
5) T	DICAMBA	6.432	6.876	3436.2E6	3221.0E6	334.254	326.512
6) T	MCP	6.581	6.973	252.1E6	240.7E6	33.163	30.923
7) T	MCPA	6.704	7.181	366.3E6	379.7E6	35.098	36.137
8) T	DICHLORPROP	7.016	7.523	842.8E6	9894.5E6	318.013	3973.676 #
9) T	2,4-D	7.216	7.786	1099.1E6	1103.6E6	335.207	373.033
10) T	Pentachlo...	7.439	8.205	6648.1E6	6014.7E6	188.945	183.238
11) T	2,4,5-TP ...	7.966	8.568	5074.5E6	3884.1E6	339.487	285.141
12) T	2,4,5-T	8.224	8.948	4855.6E6	4054.9E6	295.691	322.334
13) T	2,4-DB	8.741	9.458	17625.9E6	5277.1E6	5845.504	3142.459 #
14) T	DINOSEB	9.717f	9.772	83117.4E6	840.3E6	6413.497	87.607 #
15) T	Picloram	9.615	10.742	4513.9E6	8023.0E6	181.854	399.811 #
16) T	DCPA	10.037	10.696	8055.3E6	9687.5E6	390.533	610.725 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032223\
Data File : PS022462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2023 18:48
Operator : AR\AJ
Sample : 02001-07MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 21:17:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

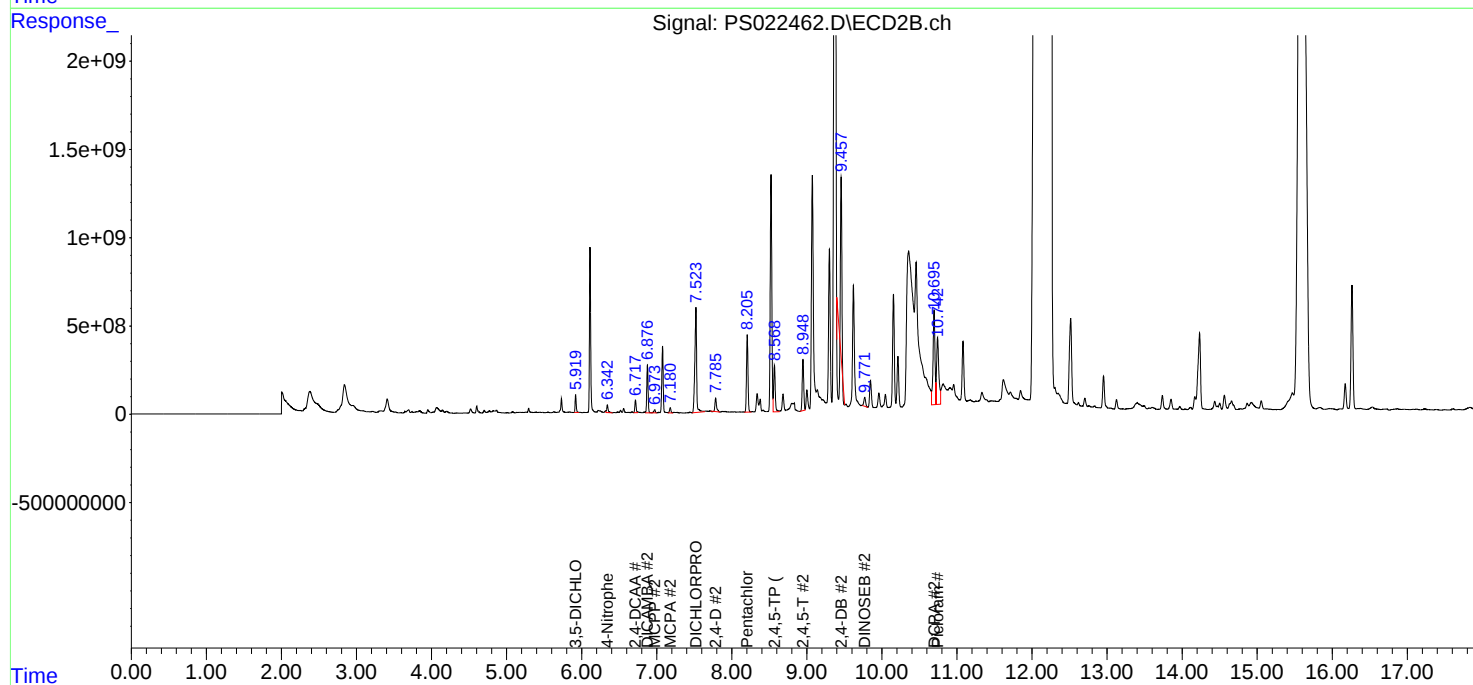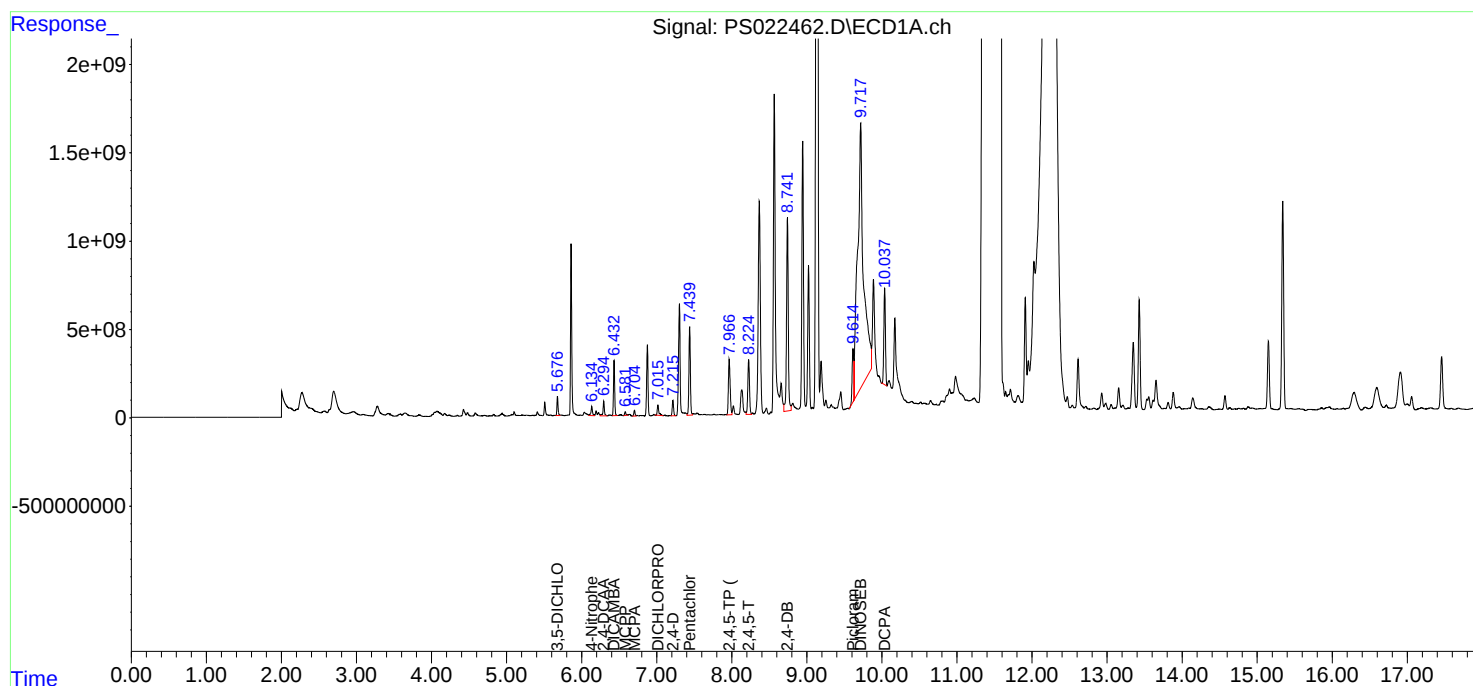


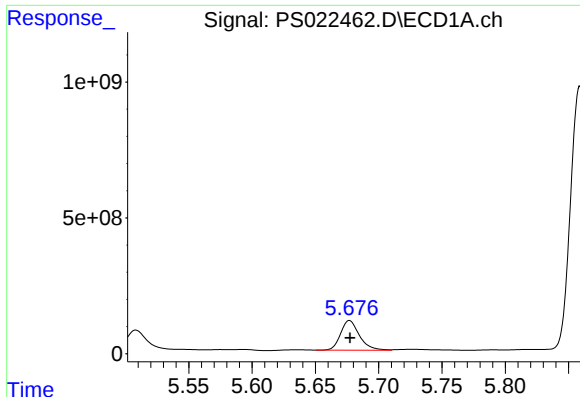

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.677 min
Delta R.T.: 0.000 min
Response: 1126176923
Conc: 302.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

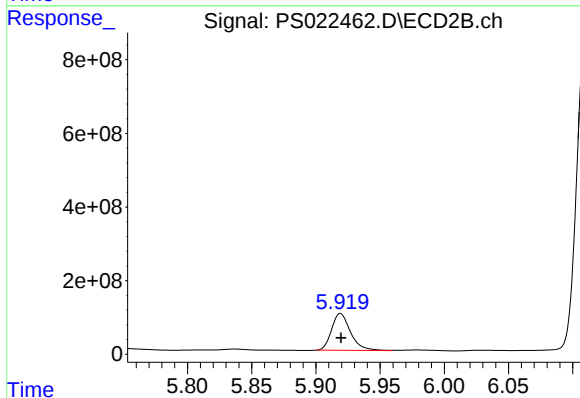


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.919 min
Delta R.T.: 0.000 min
Response: 1025881577
Conc: 321.70 ng/ml

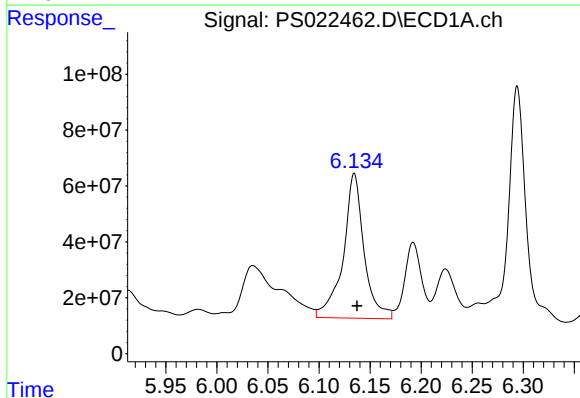


#3 4-Nitrophenol

R.T.: 6.135 min
Delta R.T.: -0.003 min
Response: 737867873
Conc: 538.52 ng/ml

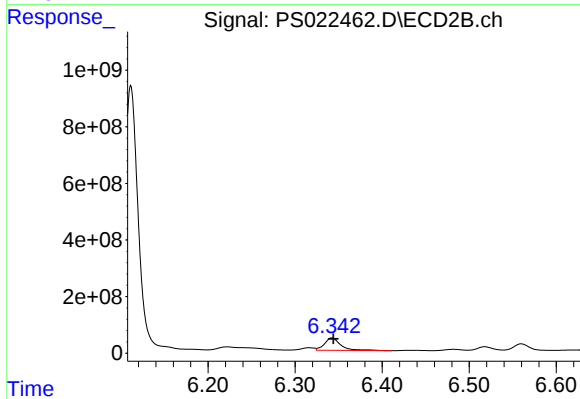

#3 4-Nitrophenol


R.T.: 6.342 min
Delta R.T.: -0.002 min
Response: 577722932
Conc: 411.49 ng/ml

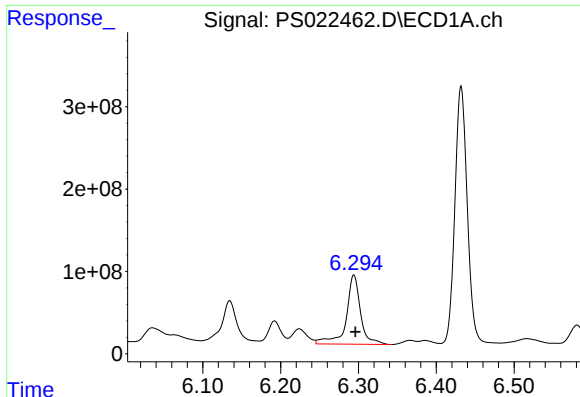

#4 2,4-DCAA


R.T.: 6.294 min
Delta R.T.: -0.002 min
Response: 1072469381
Conc: 438.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

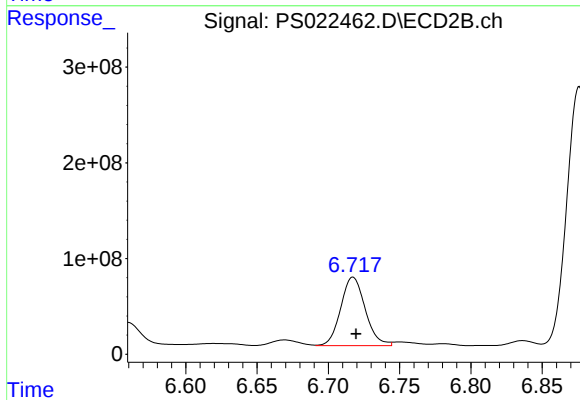


#4 2,4-DCAA

R.T.: 6.717 min
Delta R.T.: -0.002 min
Response: 856408647
Conc: 415.80 ng/ml

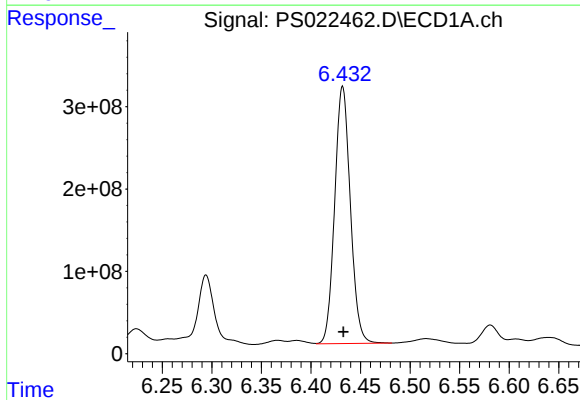


#5 DICAMBA

R.T.: 6.432 min
Delta R.T.: 0.000 min
Response: 3436214160
Conc: 334.25 ng/ml

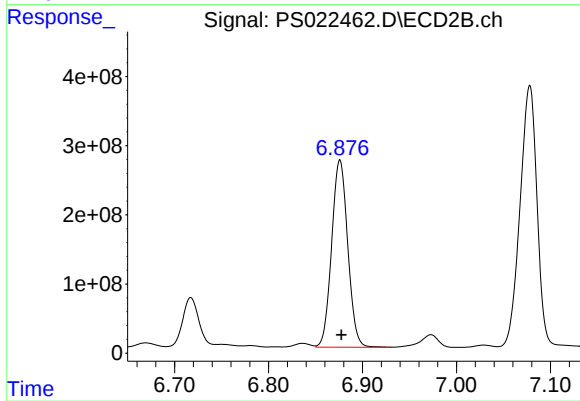

#5 DICAMBA


R.T.: 6.876 min
Delta R.T.: -0.002 min
Response: 3221036284
Conc: 326.51 ng/ml

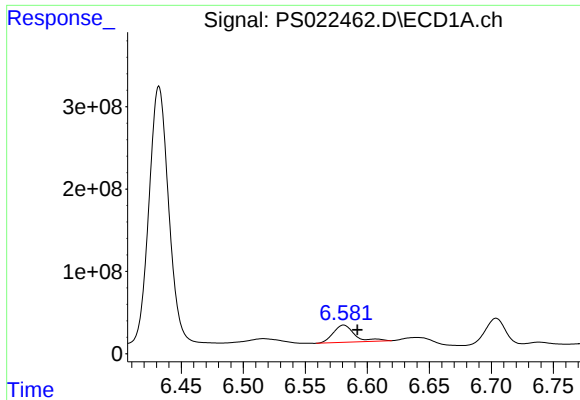

#6 MCP


R.T.: 6.581 min
Delta R.T.: -0.011 min
Response: 252113414
Conc: 33.16 ug/ml

Instrument :
ECD_S
ClientSampleId :

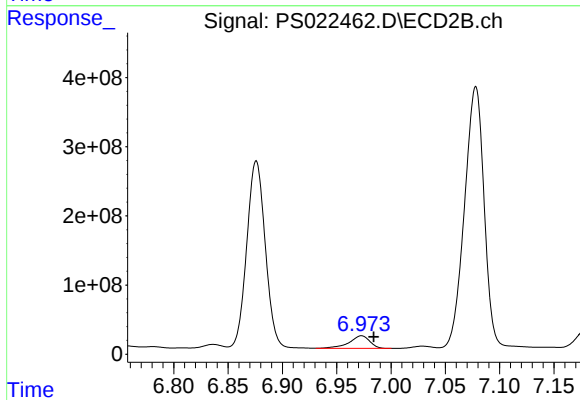


#6 MCP

R.T.: 6.973 min
Delta R.T.: -0.011 min
Response: 240715200
Conc: 30.92 ug/ml

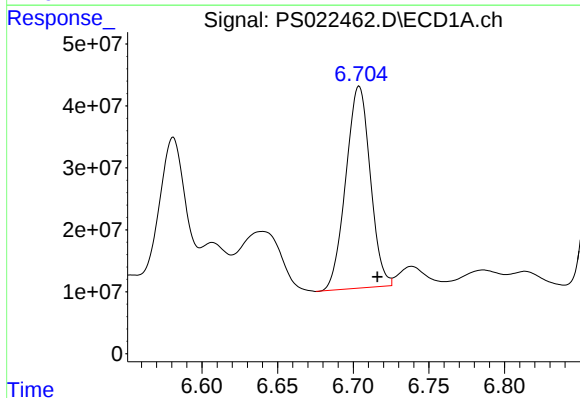


#7 MCP

R.T.: 6.704 min
Delta R.T.: -0.012 min
Response: 366323660
Conc: 35.10 ug/ml

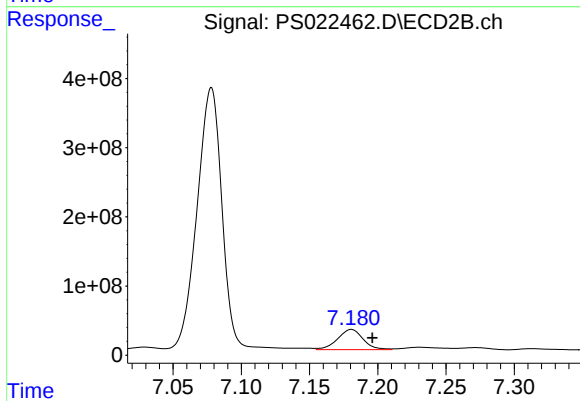

#7 MCP


R.T.: 7.181 min
Delta R.T.: -0.015 min
Response: 379663247
Conc: 36.14 ug/ml

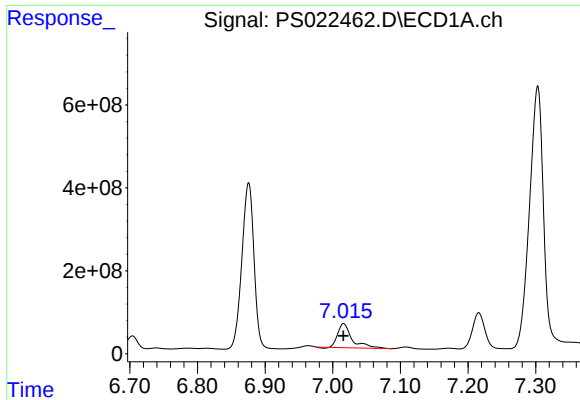

#8 DICHLORPROP


R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 842825037
Conc: 318.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

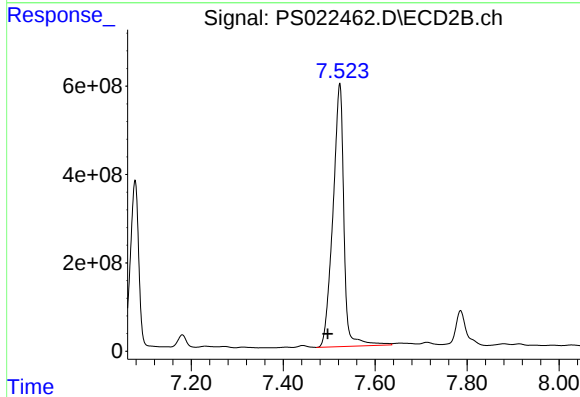


#8 DICHLORPROP

R.T.: 7.523 min
Delta R.T.: 0.026 min
Response: 9894547391
Conc: 3973.68 ng/ml

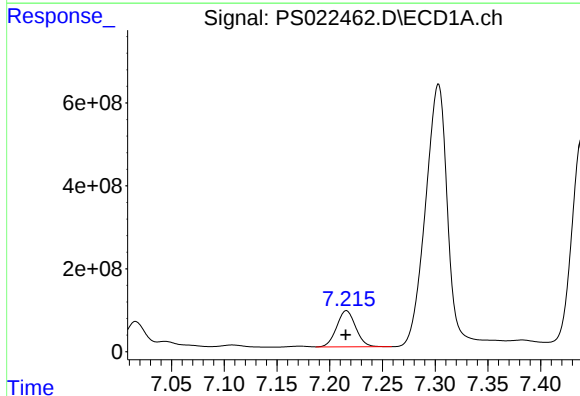


#9 2,4-D

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 1099146610
Conc: 335.21 ng/ml

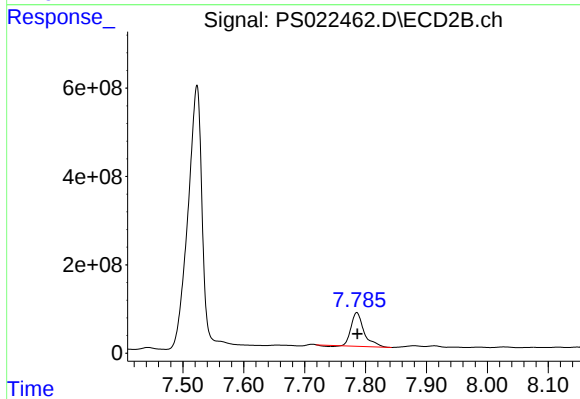

#9 2,4-D


R.T.: 7.786 min
Delta R.T.: 0.000 min
Response: 1103610624
Conc: 373.03 ng/ml

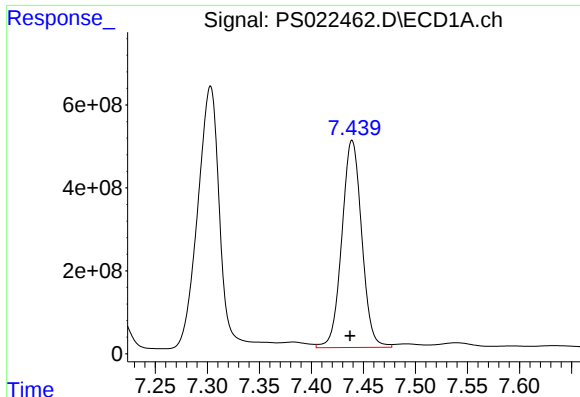

#10 Pentachlorophenol


R.T.: 7.439 min
Delta R.T.: 0.002 min
Response: 6648067296
Conc: 188.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

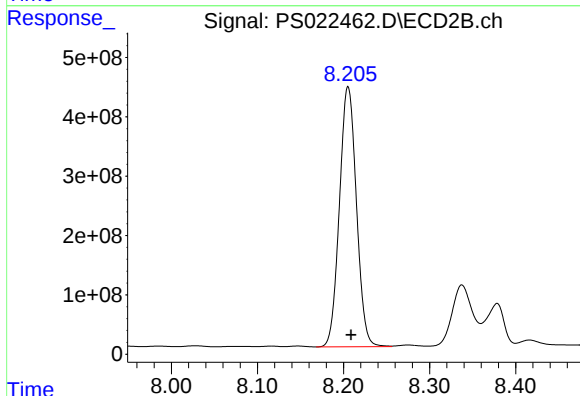


#10 Pentachlorophenol

R.T.: 8.205 min
Delta R.T.: -0.003 min
Response: 6014673712
Conc: 183.24 ng/ml

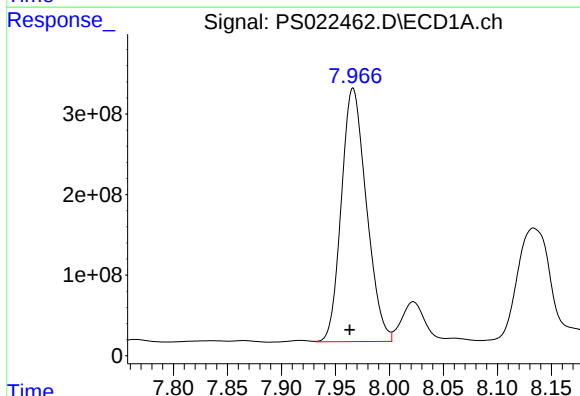


#11 2,4,5-TP (SILVEX)

R.T.: 7.966 min
Delta R.T.: 0.003 min
Response: 5074479694
Conc: 339.49 ng/ml

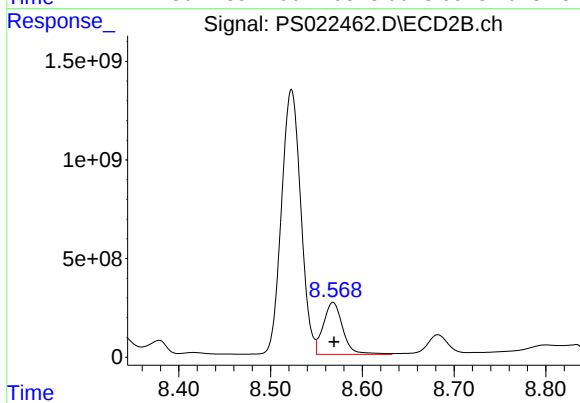

#11 2,4,5-TP (SILVEX)


R.T.: 8.568 min
Delta R.T.: -0.001 min
Response: 3884149901
Conc: 285.14 ng/ml

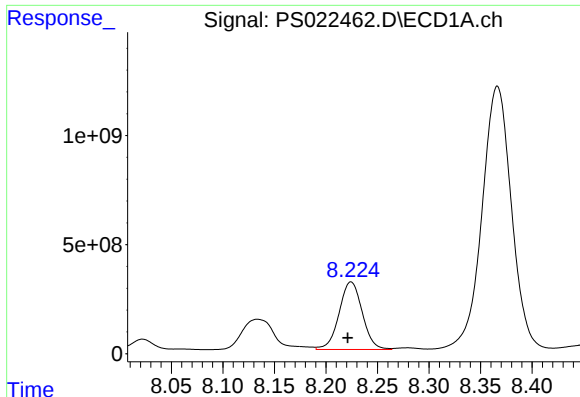

#12 2,4,5-T


R.T.: 8.224 min
Delta R.T.: 0.003 min
Response: 4855591227
Conc: 295.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

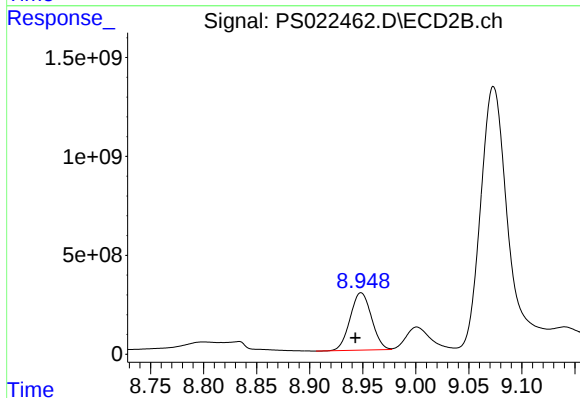


#12 2,4,5-T

R.T.: 8.948 min
Delta R.T.: 0.005 min
Response: 4054898742
Conc: 322.33 ng/ml

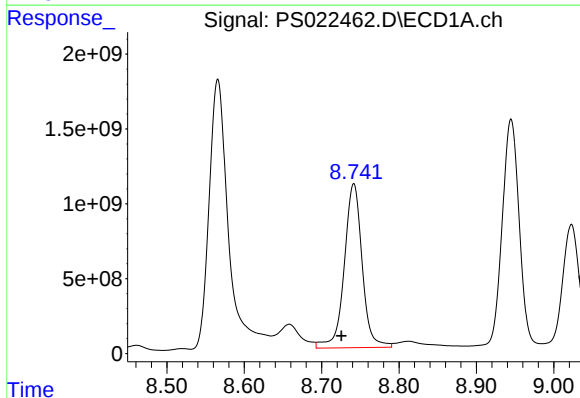


#13 2,4-DB

R.T.: 8.741 min
Delta R.T.: 0.016 min
Response: 17625903249
Conc: 5845.50 ng/ml

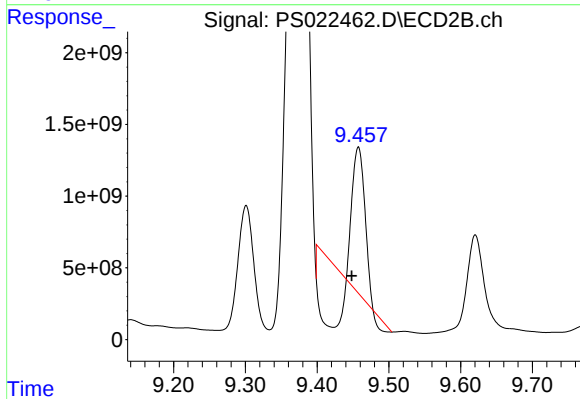

#13 2,4-DB


R.T.: 9.458 min
Delta R.T.: 0.009 min
Response: 5277129925
Conc: 3142.46 ng/ml

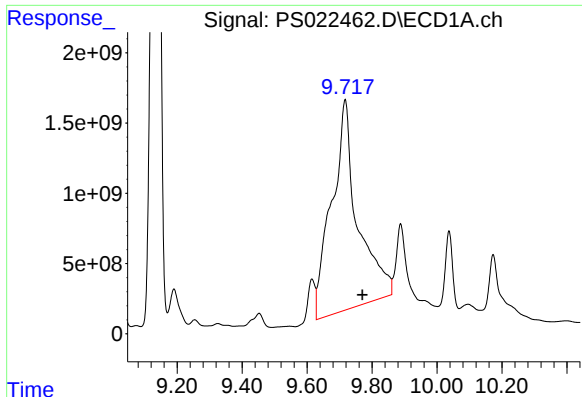

#14 DINOSEB


R.T.: 9.717 min
Delta R.T.: -0.053 min
Response: 83117374026
Conc: 6413.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

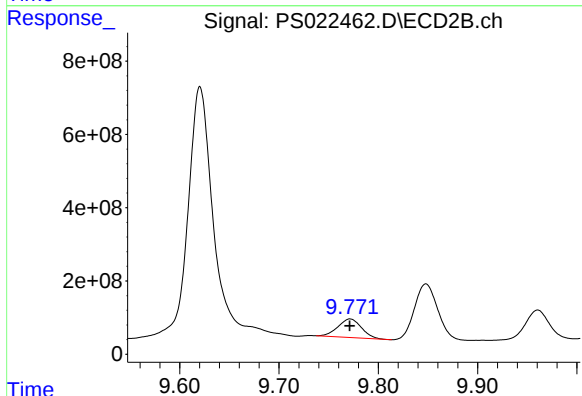


#14 DINOSEB

R.T.: 9.772 min
Delta R.T.: 0.000 min
Response: 840256212
Conc: 87.61 ng/ml

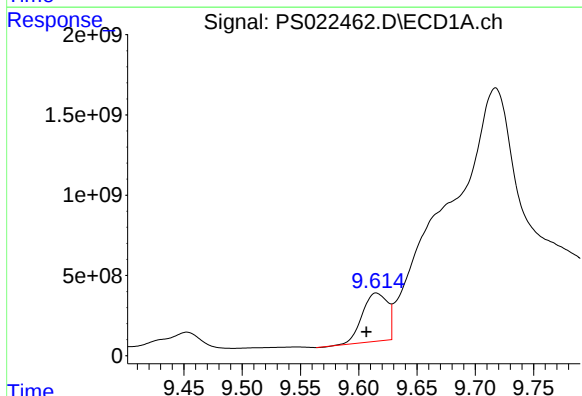


#15 Picloram

R.T.: 9.615 min
Delta R.T.: 0.009 min
Response: 4513868197
Conc: 181.85 ng/ml

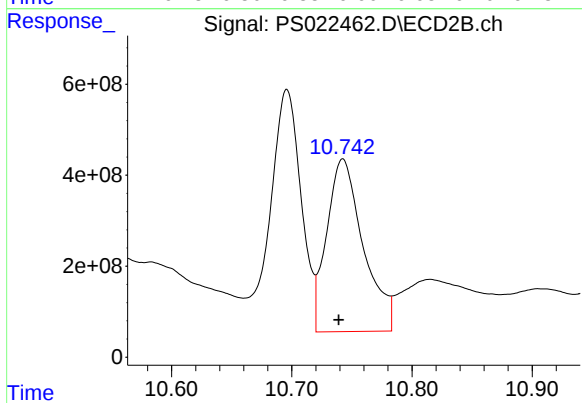

#15 Picloram

R.T.: 10.742 min
Delta R.T.: 0.003 min
Response: 8023024046
Conc: 399.81 ng/ml

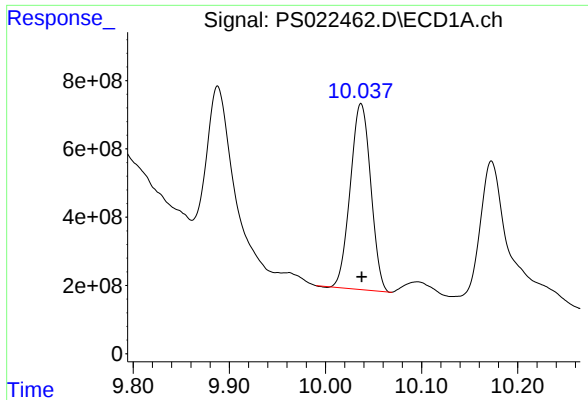

#16 DCPA


R.T.: 10.037 min

Delta R.T.: 0.000 min

Response: 8055261395

Conc: 390.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

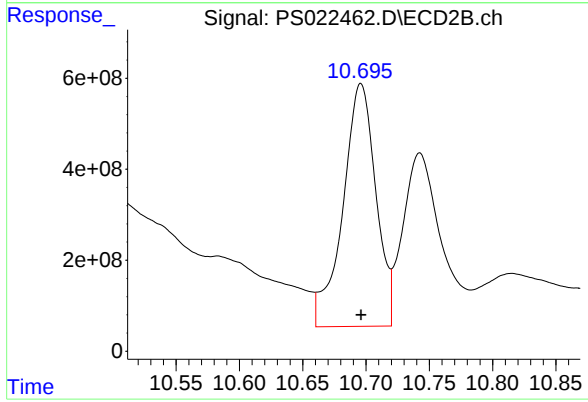

#16 DCPA

R.T.: 10.696 min

Delta R.T.: 0.000 min

Response: 9687484243

Conc: 610.72 ng/ml