

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032223\
 Data File : PS022474.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2023 00:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:58:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.295	6.718	1400.8E6	1310.5E6	573.088	636.257
Target Compounds							
1) T	Dalapon	2.433	2.509	2152854	856732	<MDL	<MDL #
3) T	4-Nitroph...	6.138	6.332	7665466	1043539	5.595	<MDL #
5) T	DICAMBA	6.432	6.924f	6567762	739.3E6	<MDL	74.938 #
6) T	MCP	6.547f	6.924f	381907	739.3E6	<MDL	94.969 #
8) T	DICHLORPROP	7.009	7.523	7493127	59180381	2.827	23.767 #
9) T	2,4-D	7.175f	7.829f	1097.9E6	2013917	334.830	<MDL #
10) T	Pentachlo...	7.438	8.207	20501226	16570428	<MDL	<MDL #
11) T	2,4,5-TP ...	7.977	8.569	23056416	8353539	1.542	<MDL #
12) T	2,4,5-T	8.239	8.953	32992671	25722271	2.009	2.045
14) T	DINOSEB	9.767	9.770	11349744	1460237	<MDL	<MDL #
15) T	Picloram	9.587	10.750	105.4E6	51991290	4.247	2.591 #
16) T	DCPA	10.035	10.701	8869863	62111280	<MDL	3.916 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032223\
Data File : PS022474.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2023 00:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:58:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

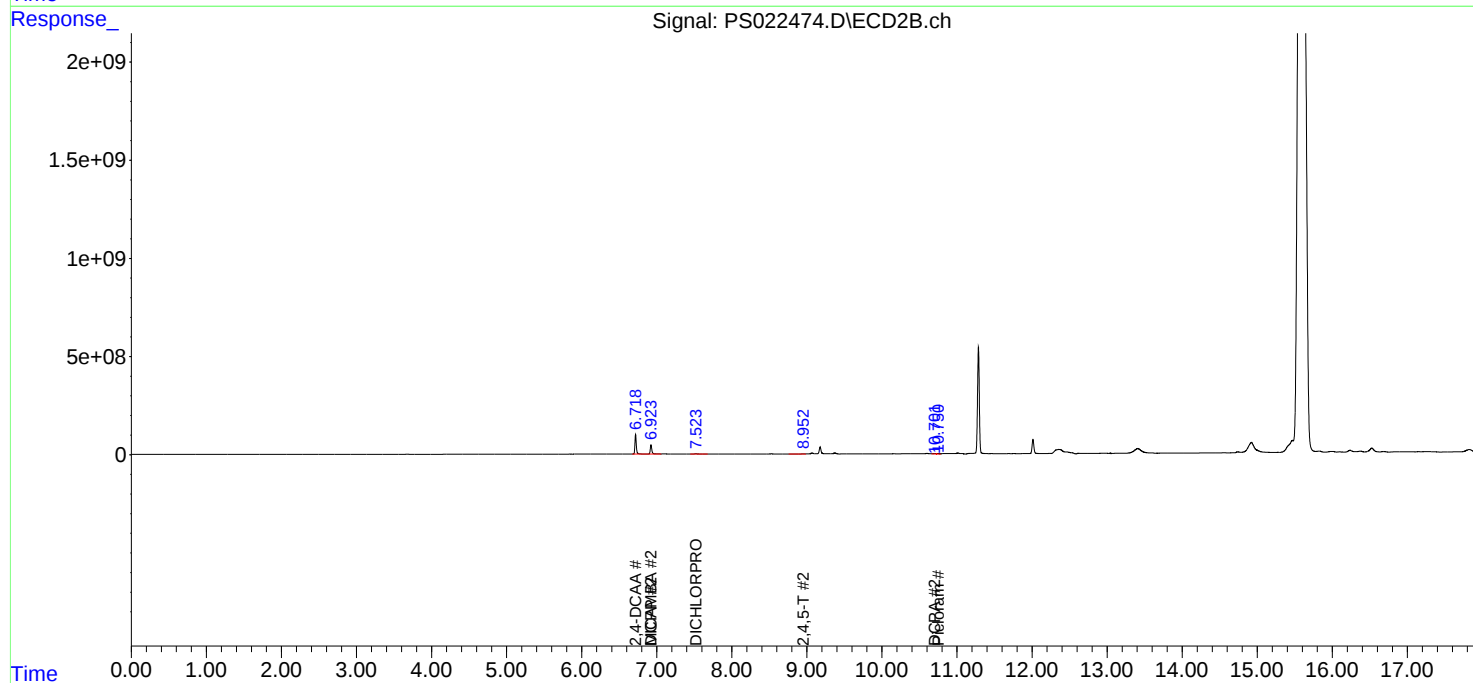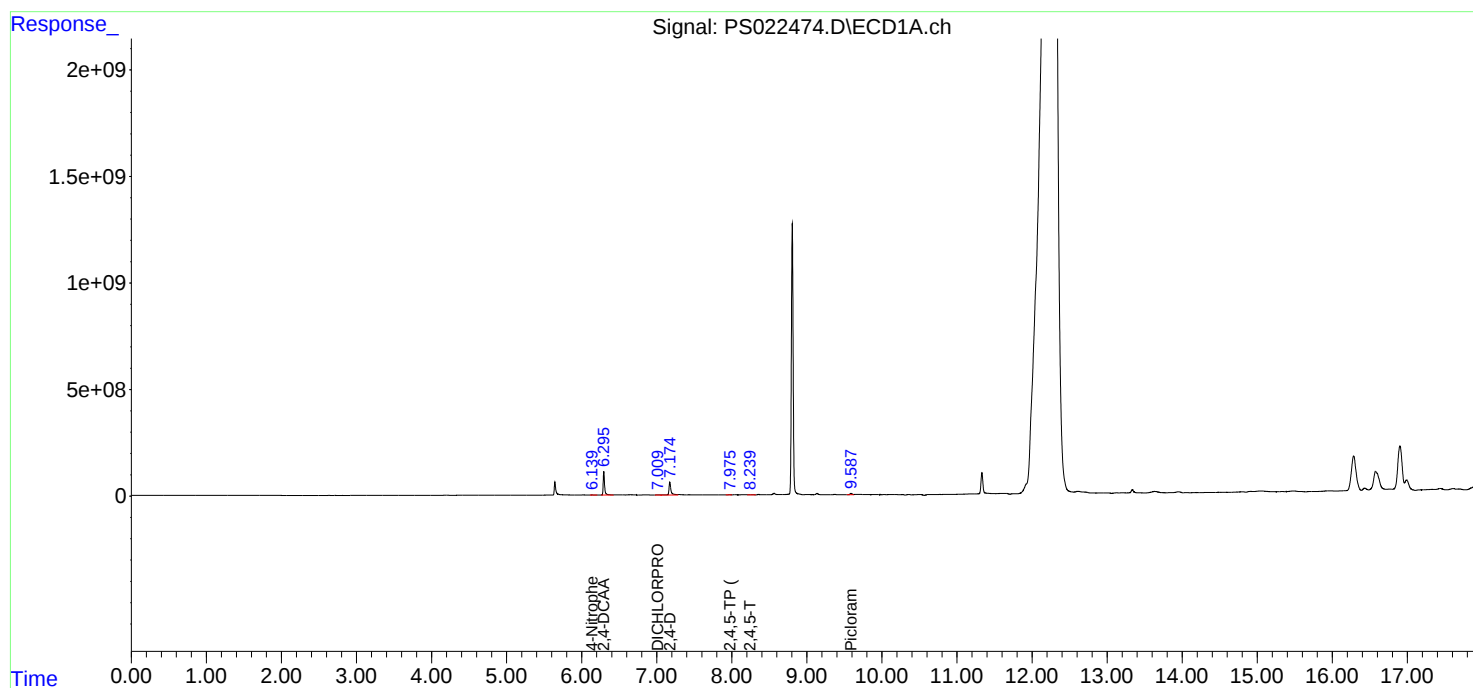


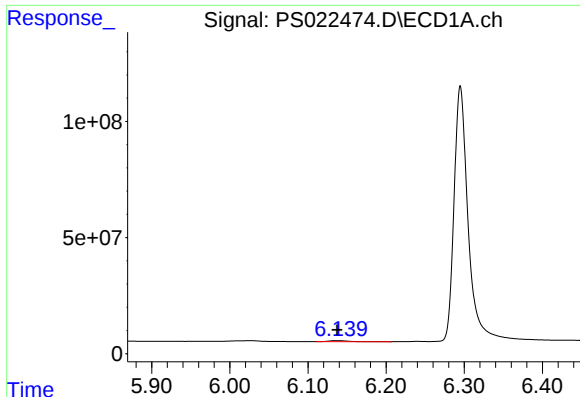

#3 4-Nitrophenol


R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 7665466
Conc: 5.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

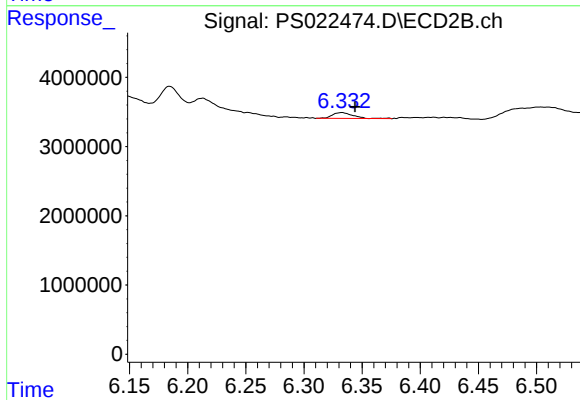


#3 4-Nitrophenol

R.T.: 6.332 min
Delta R.T.: -0.012 min
Response: 1043539
Conc: N.D.

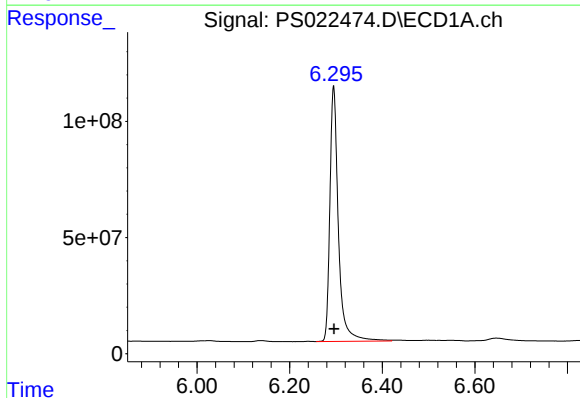


#4 2,4-DCAA

R.T.: 6.295 min
Delta R.T.: 0.000 min
Response: 1400846154
Conc: 573.09 ng/ml

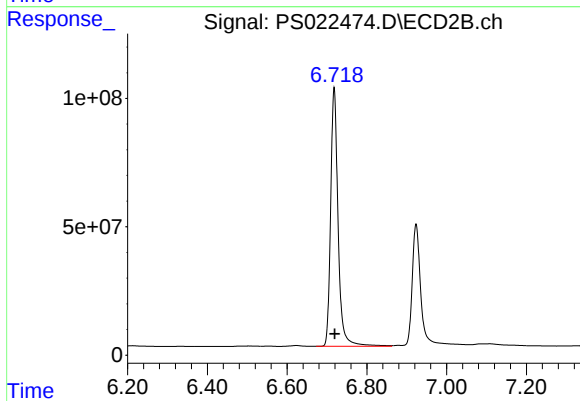

#4 2,4-DCAA


R.T.: 6.718 min
Delta R.T.: -0.001 min
Response: 1310490195
Conc: 636.26 ng/ml

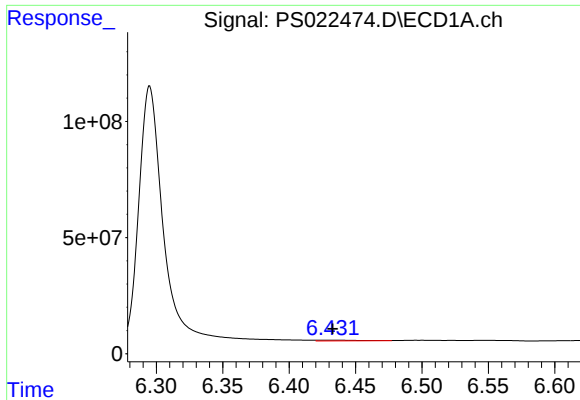

#5 DICAMBA


R.T.: 6.432 min
Delta R.T.: -0.001 min
Response: 6567762
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

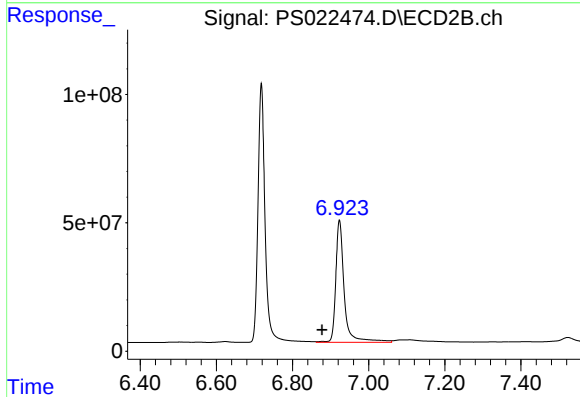


#5 DICAMBA

R.T.: 6.924 min
Delta R.T.: 0.046 min
Response: 739266192
Conc: 74.94 ng/ml

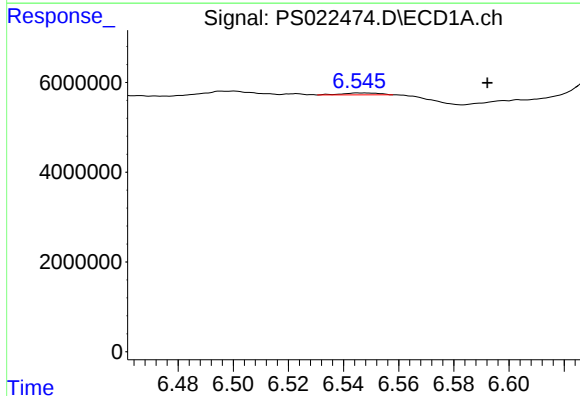


#6 MCPP

R.T.: 6.547 min
Delta R.T.: -0.045 min
Response: 381907
Conc: N.D.

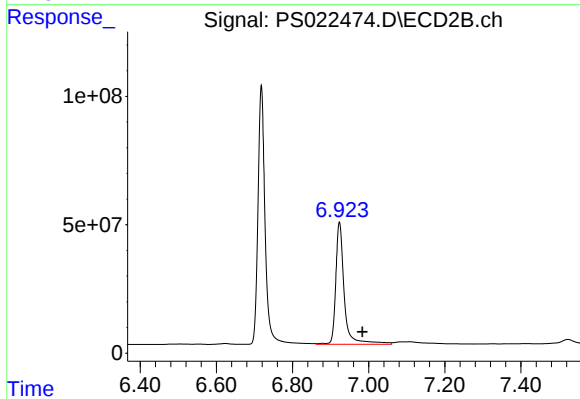

#6 MCPP


R.T.: 6.924 min
Delta R.T.: -0.061 min
Response: 739266192
Conc: 94.97 ug/ml

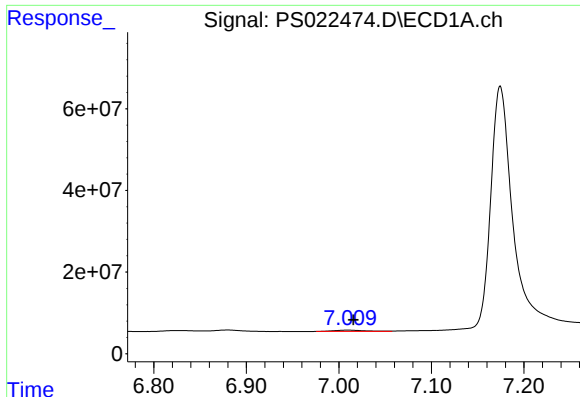

#8 DICHLORPROP


R.T.: 7.009 min
Delta R.T.: -0.006 min
Response: 7493127
Conc: 2.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

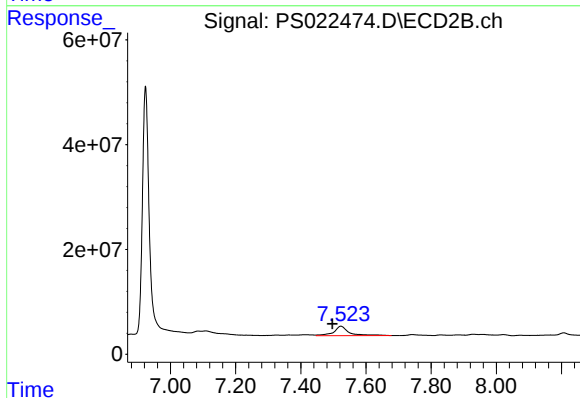


#8 DICHLORPROP

R.T.: 7.523 min
Delta R.T.: 0.026 min
Response: 59180381
Conc: 23.77 ng/ml

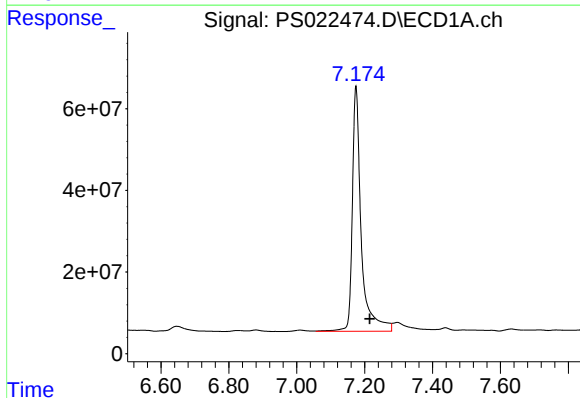


#9 2,4-D

R.T.: 7.175 min
Delta R.T.: -0.041 min
Response: 1097911518
Conc: 334.83 ng/ml

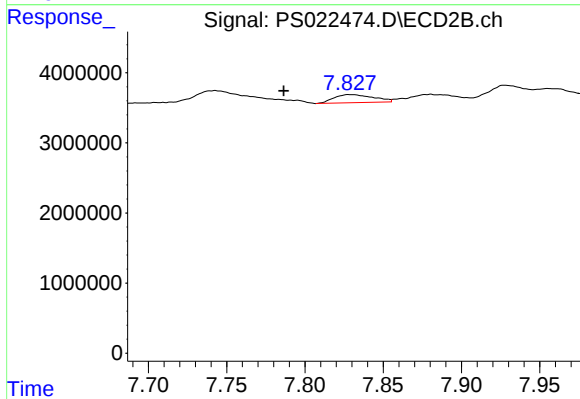

#9 2,4-D


R.T.: 7.829 min
Delta R.T.: 0.043 min
Response: 2013917
Conc: N.D.

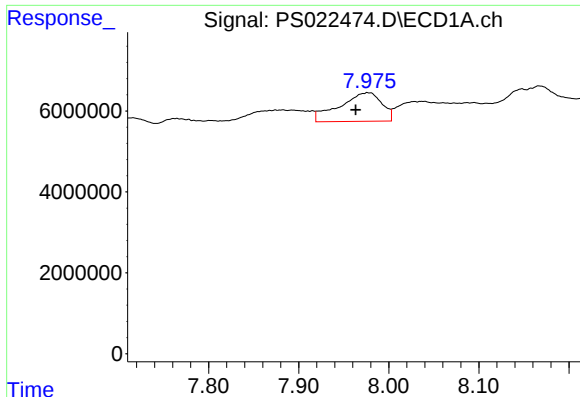

#11 2,4,5-TP (SILVEX)


R.T.: 7.977 min
Delta R.T.: 0.014 min
Response: 23056416
Conc: 1.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

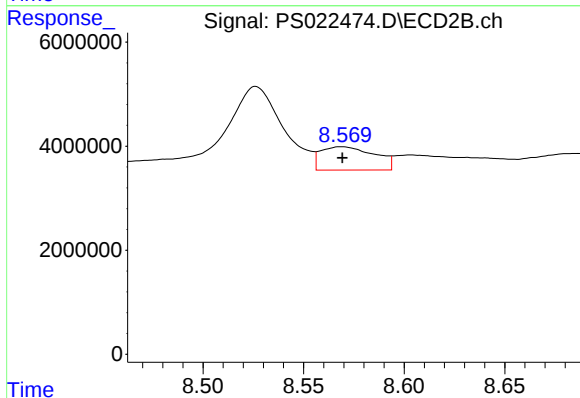


#11 2,4,5-TP (SILVEX)

R.T.: 8.569 min
Delta R.T.: 0.000 min
Response: 8353539
Conc: N.D.

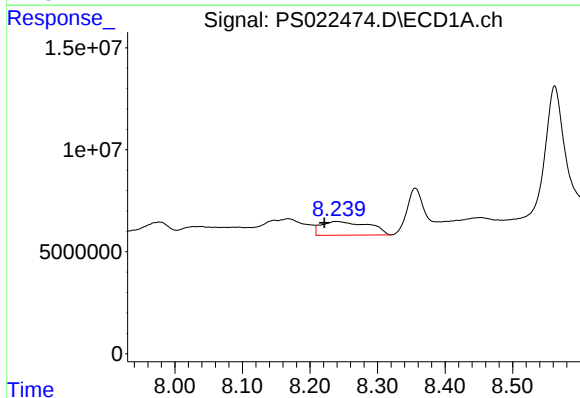


#12 2,4,5-T

R.T.: 8.239 min
Delta R.T.: 0.018 min
Response: 32992671
Conc: 2.01 ng/ml

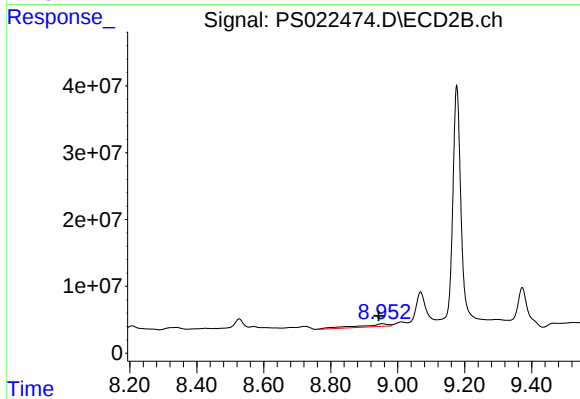

#12 2,4,5-T


R.T.: 8.953 min
Delta R.T.: 0.010 min
Response: 25722271
Conc: 2.04 ng/ml

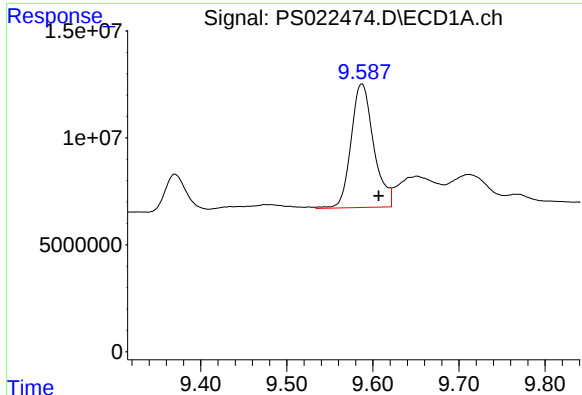

#15 Picloram


R.T.: 9.587 min
Delta R.T.: -0.020 min
Response: 105425524
Conc: 4.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

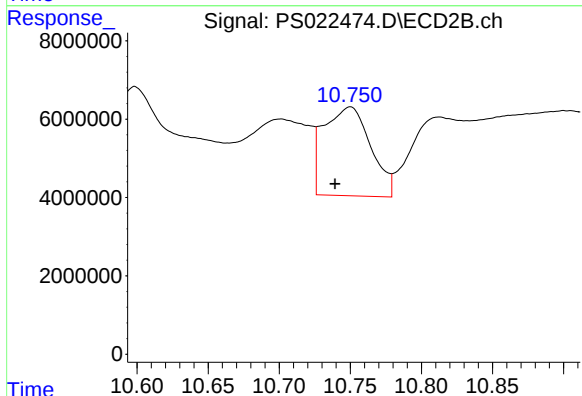


#15 Picloram

R.T.: 10.750 min
Delta R.T.: 0.010 min
Response: 51991290
Conc: 2.59 ng/ml

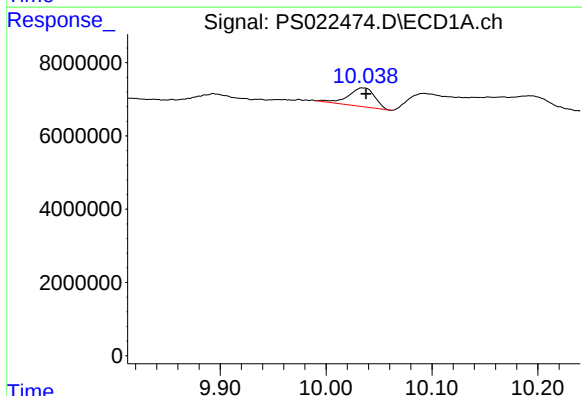

#16 DCPA

R.T.: 10.035 min
Delta R.T.: -0.003 min
Response: 8869863
Conc: N.D.

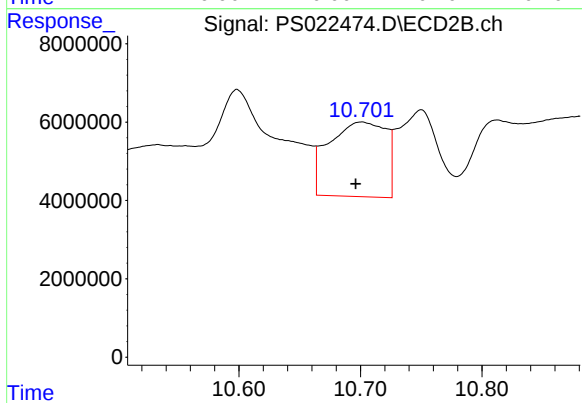

#16 DCPA

R.T.: 10.701 min
Delta R.T.: 0.005 min
Response: 62111280
Conc: 3.92 ng/ml