

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032320\
 Data File : PS009400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2020 16:34
 Operator : DD\AJ
 Sample : PB127729BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 16:59:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.932	336.4E6	331.0E6	608.097	602.757
Target Compounds							
1) T	Dalapon	3.006	2.587	22619677	105.7E6	29.006	134.247 #
2) T	3,5-DICHL...	0.000	6.109	0	50754927	N.D.	62.406
6) T	MCP	7.597	0.000	8661702	0	3.520	N.D. #
7) T	MCPA	7.793	7.399	73447101	55126844	24.115	20.428
8) T	DICHLORPROP	0.000	7.751	0	31593027	N.D.	56.943
11) T	2,4,5-TP ...	0.000	8.785	0	30764233	N.D.	10.320
12) T	2,4,5-T	9.454	9.250	22428922	26144648	8.817	8.856
14) T	DINOSEB	11.187	10.045	28414070	16769627	13.900	7.635 #
15) T	Picloram	11.036	11.020	84161985	123.5E6	27.731	30.340
16) T	DCPA	0.000	10.969	0	8527041	N.D.	2.202



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032320\
Data File : PS009400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2020 16:34
Operator : DD\AJ
Sample : PB127729BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 16:59:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

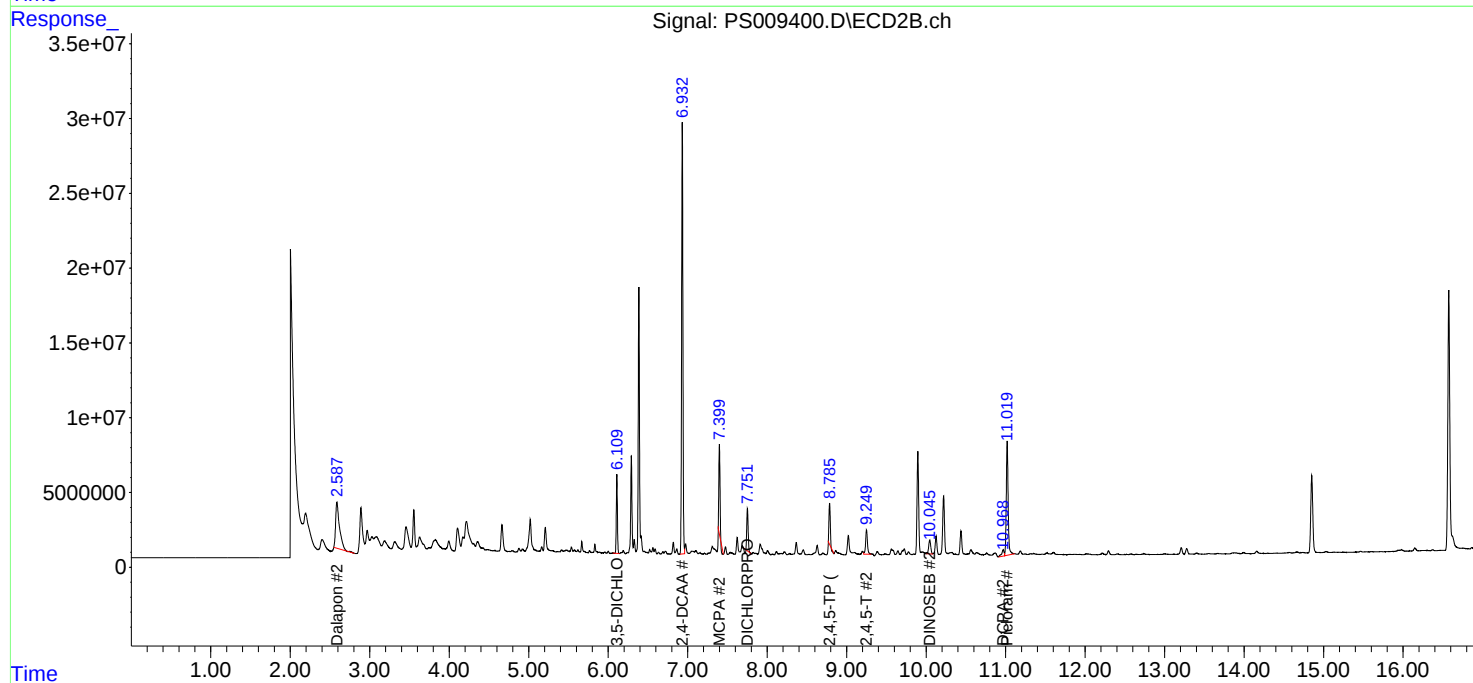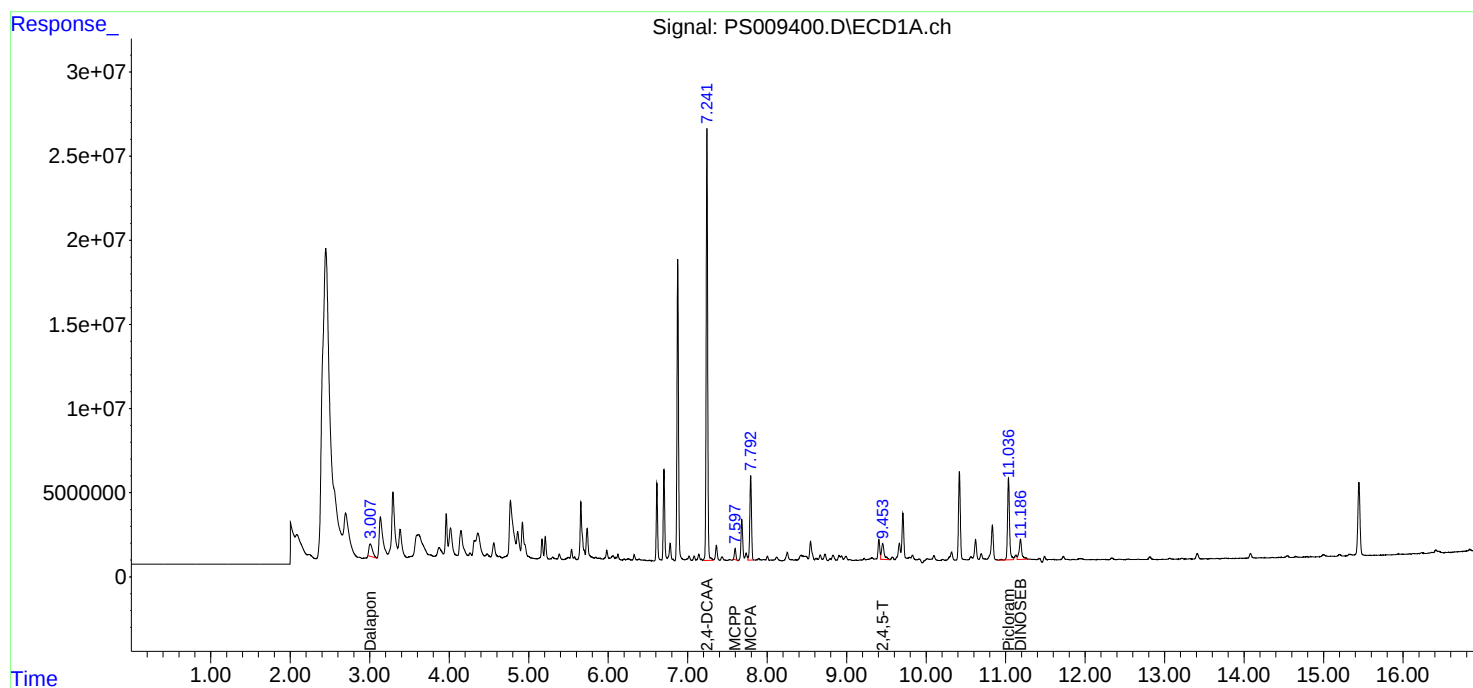


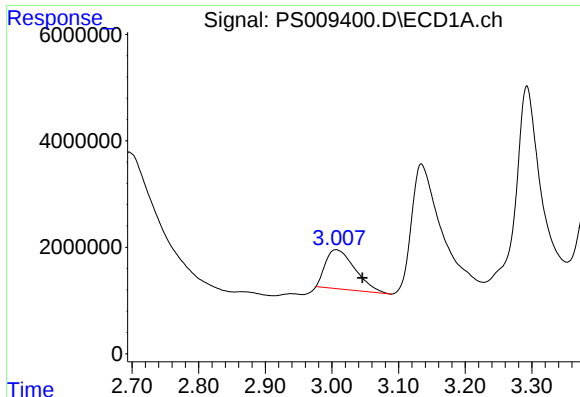

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 22619677
Conc: 29.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

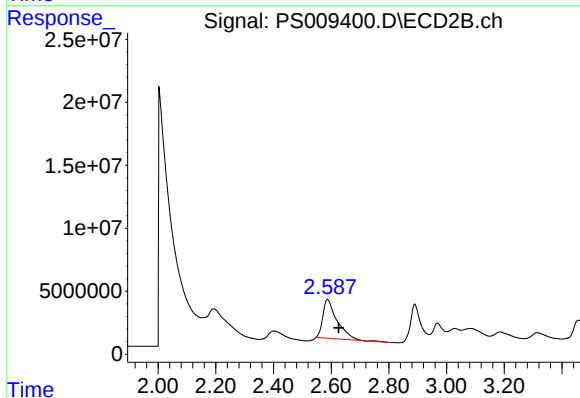


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.039 min
Response: 105701401
Conc: 134.25 ng/ml

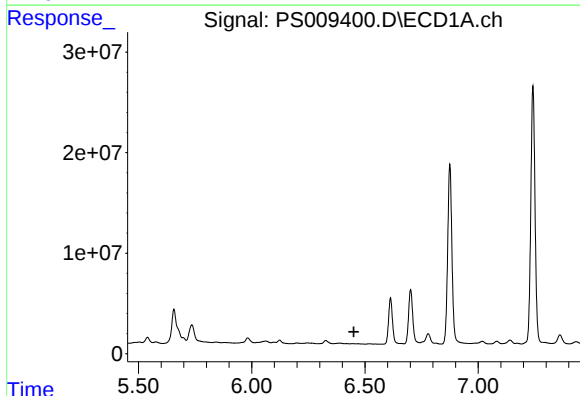


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

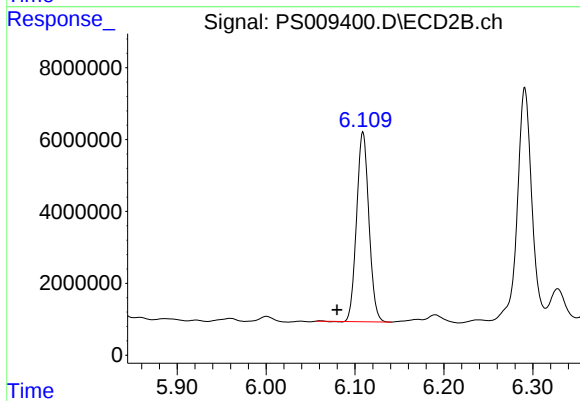

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.029 min
Response: 50754927
Conc: 62.41 ng/ml

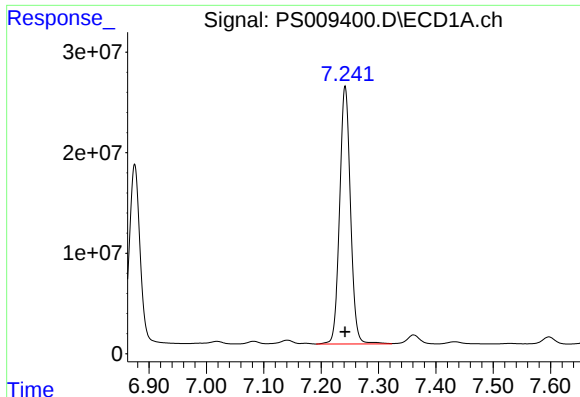

#4 2,4-DCAA


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 336381251
Conc: 608.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

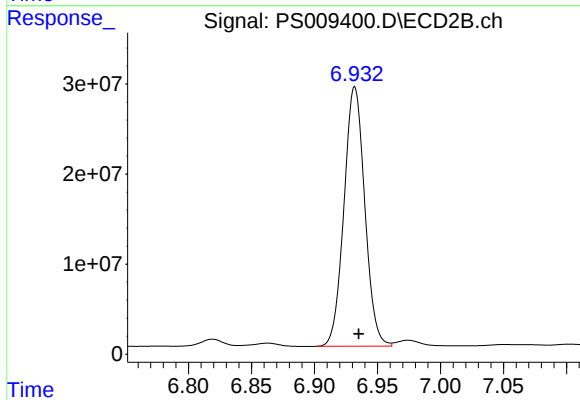


#4 2,4-DCAA

R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 331032906
Conc: 602.76 ng/ml

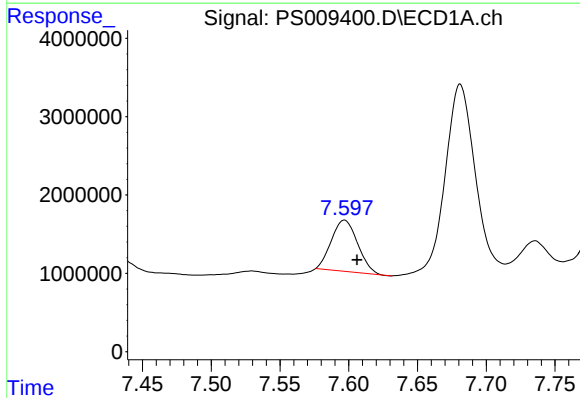


#6 MCP

R.T.: 7.597 min
Delta R.T.: -0.009 min
Response: 8661702
Conc: 3.52 ug/ml

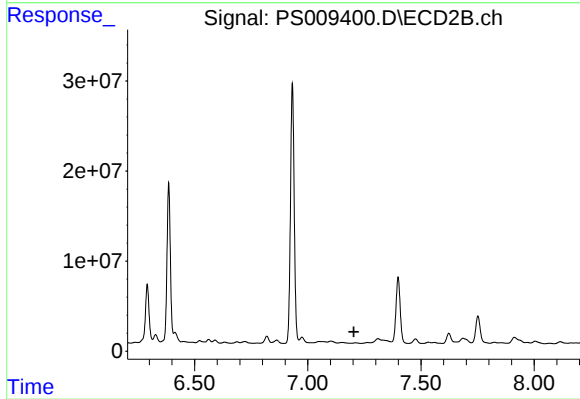

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

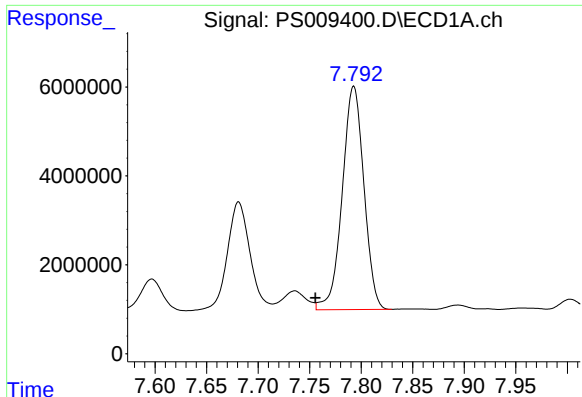

#7 MCPA


R.T.: 7.793 min
Delta R.T.: 0.037 min
Response: 73447101
Conc: 24.12 ug/ml

Instrument :
ECD_S
ClientSampleId :

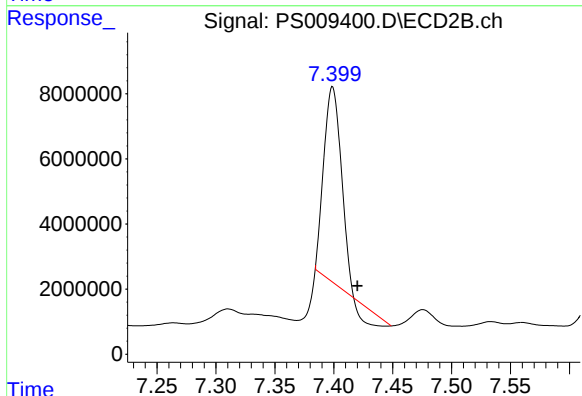


#7 MCPA

R.T.: 7.399 min
Delta R.T.: -0.021 min
Response: 55126844
Conc: 20.43 ug/ml

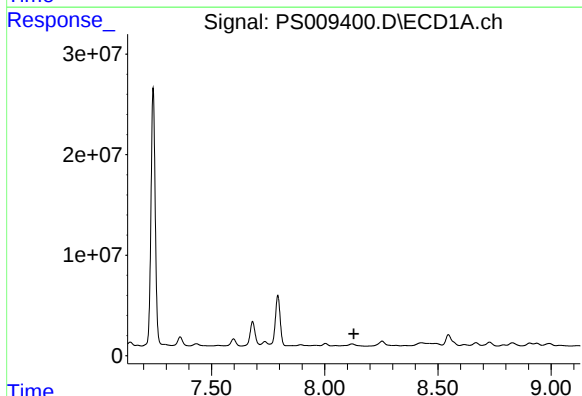


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

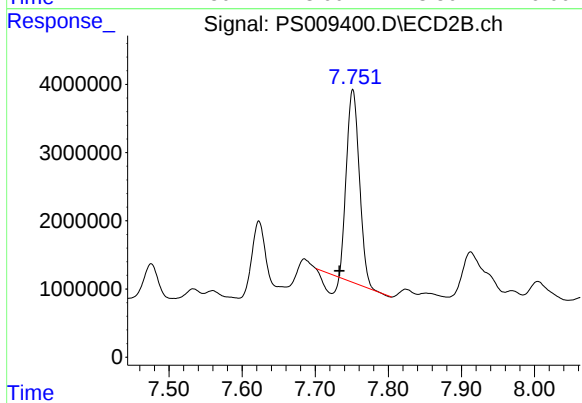

#8 DICHLORPROP


R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 31593027
Conc: 56.94 ng/ml

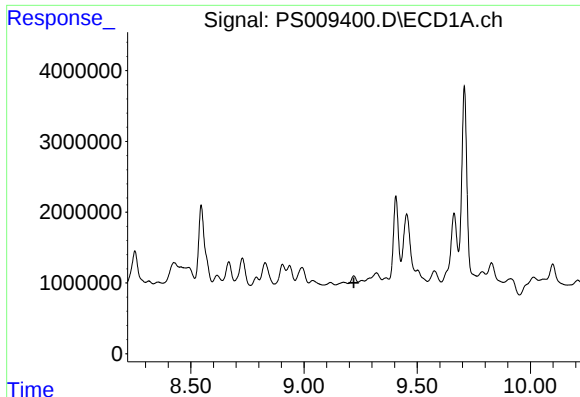

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

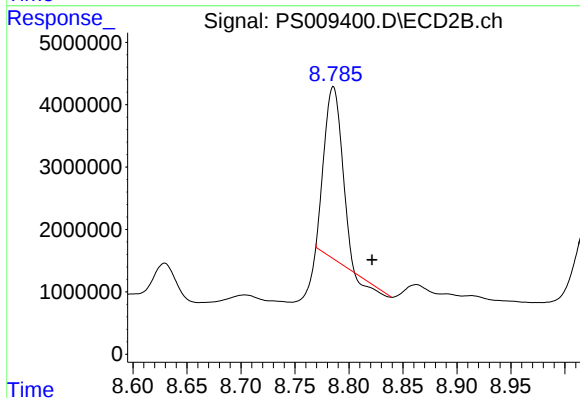


#11 2,4,5-TP (SILVEX)

R.T.: 8.785 min
Delta R.T.: -0.036 min
Response: 30764233
Conc: 10.32 ng/ml

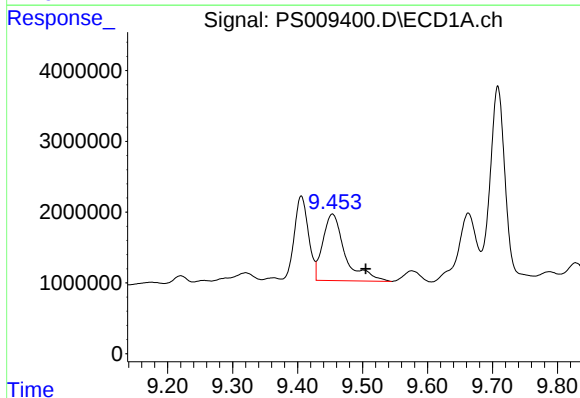


#12 2,4,5-T

R.T.: 9.454 min
Delta R.T.: -0.051 min
Response: 22428922
Conc: 8.82 ng/ml

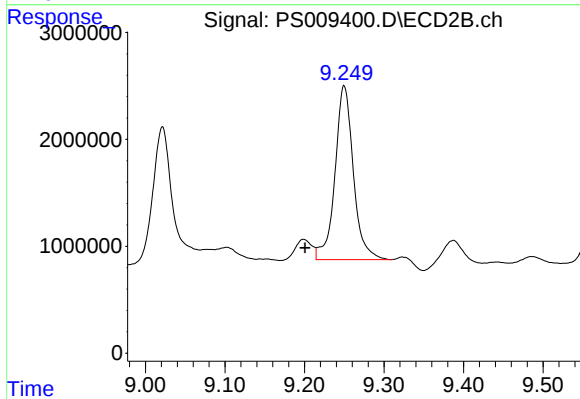

#12 2,4,5-T


R.T.: 9.250 min
Delta R.T.: 0.049 min
Response: 26144648
Conc: 8.86 ng/ml

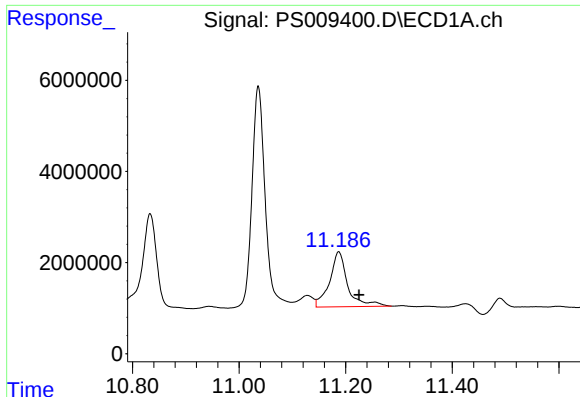

#14 DINOSEB


R.T.: 11.187 min
Delta R.T.: -0.038 min
Response: 28414070
Conc: 13.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

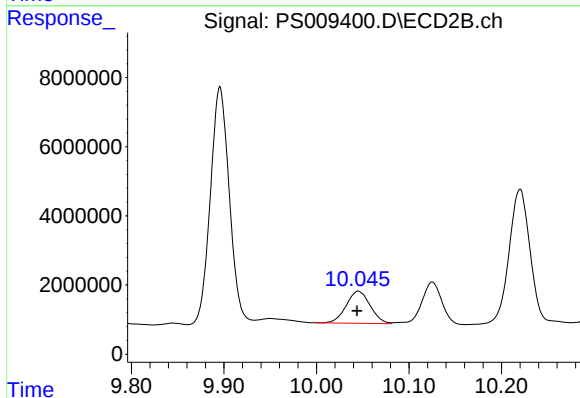


#14 DINOSEB

R.T.: 10.045 min
Delta R.T.: 0.002 min
Response: 16769627
Conc: 7.63 ng/ml

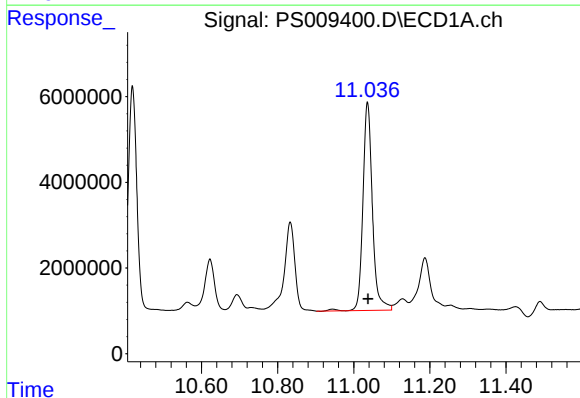


#15 Picloram

R.T.: 11.036 min
Delta R.T.: -0.001 min
Response: 84161985
Conc: 27.73 ng/ml

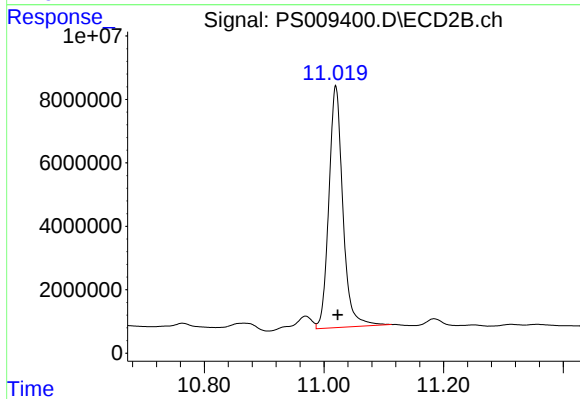

#15 Picloram


R.T.: 11.020 min
Delta R.T.: -0.004 min
Response: 123549544
Conc: 30.34 ng/ml

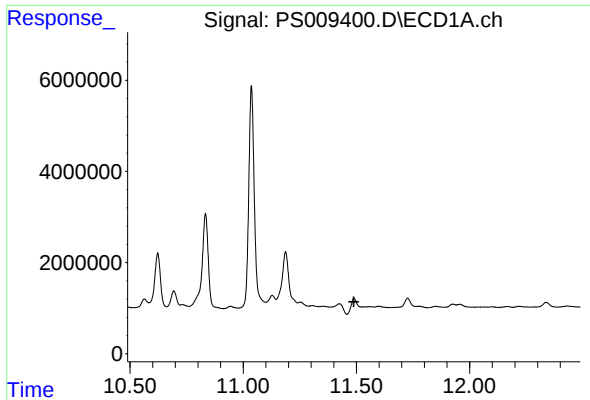

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

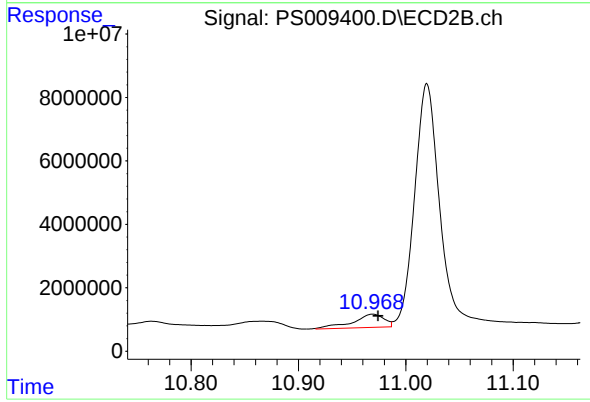

#16 DCPA

R.T.: 10.969 min
Delta R.T.: -0.005 min
Response: 8527041
Conc: 2.20 ng/ml