

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032320\
 Data File : PS009402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2020 17:20
 Operator : DD\AJ
 Sample : L1749-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 17:40:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.932	207.5E6	199.0E6	375.171	362.358
Target Compounds							
1) T	Dalapon	3.007	2.587	22397183	105.7E6	28.720	134.207 #
2) T	3,5-DICHL...	0.000	6.109	0	59426392	N.D.	73.068
6) T	MCPD	7.598	0.000	7539560	0	3.064	N.D. #
7) T	MCPA	7.734	7.399	6672117	36311686	2.191	13.456 #
8) T	DICHLORPROP	0.000	7.751	0	26675174	N.D.	48.079
11) T	2,4,5-TP ...	0.000	8.785	0	25495621	N.D.	8.552
12) T	2,4,5-T	9.451	0.000	26205390	0	10.301	N.D. #
13) T	2,4-DB	0.000	9.725	0	11004954	N.D.	28.990
14) T	DINOSEB	11.187	10.044	28425775	33532817	13.906	15.267
15) T	Picloram	11.036	11.020	16695687	27548422	5.501	6.765
16) T	DCPA	0.000	11.020	0	27548422	N.D.	7.113



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032320\
Data File : PS009402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2020 17:20
Operator : DD\AJ
Sample : L1749-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 17:40:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

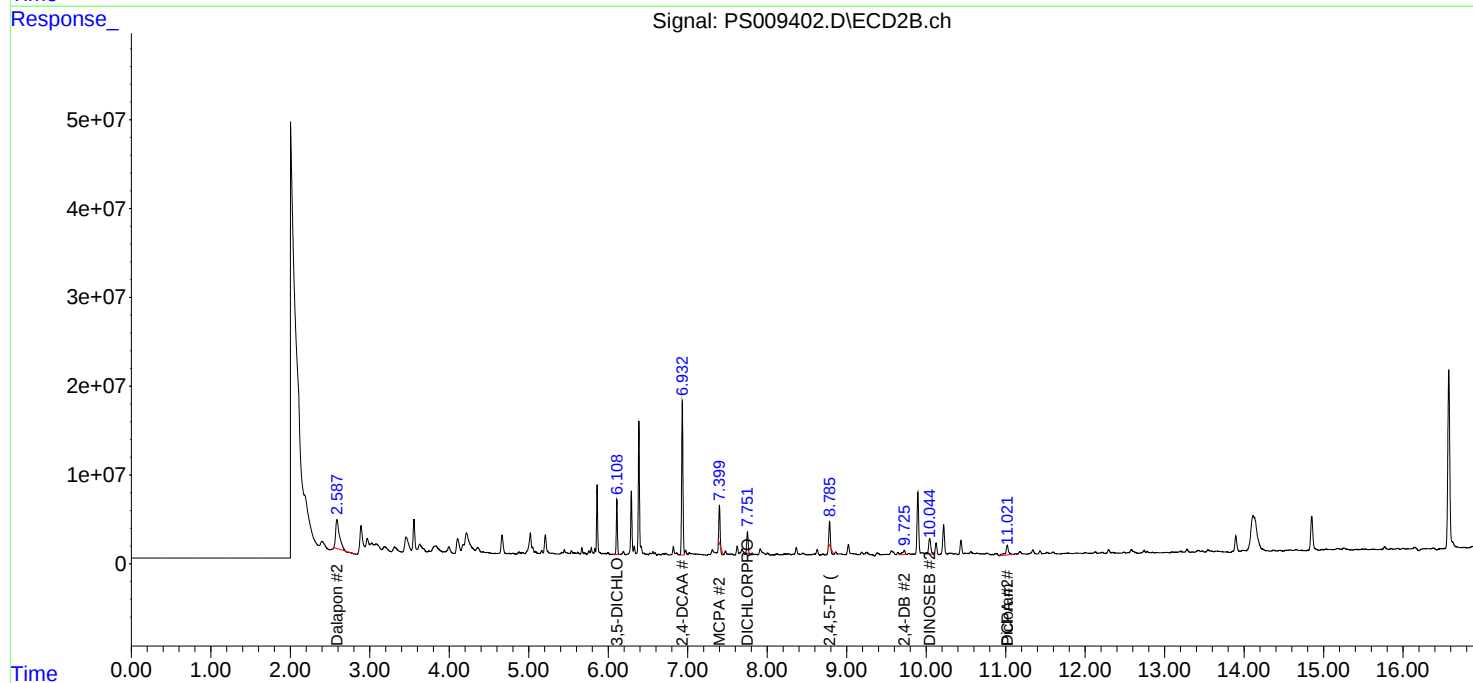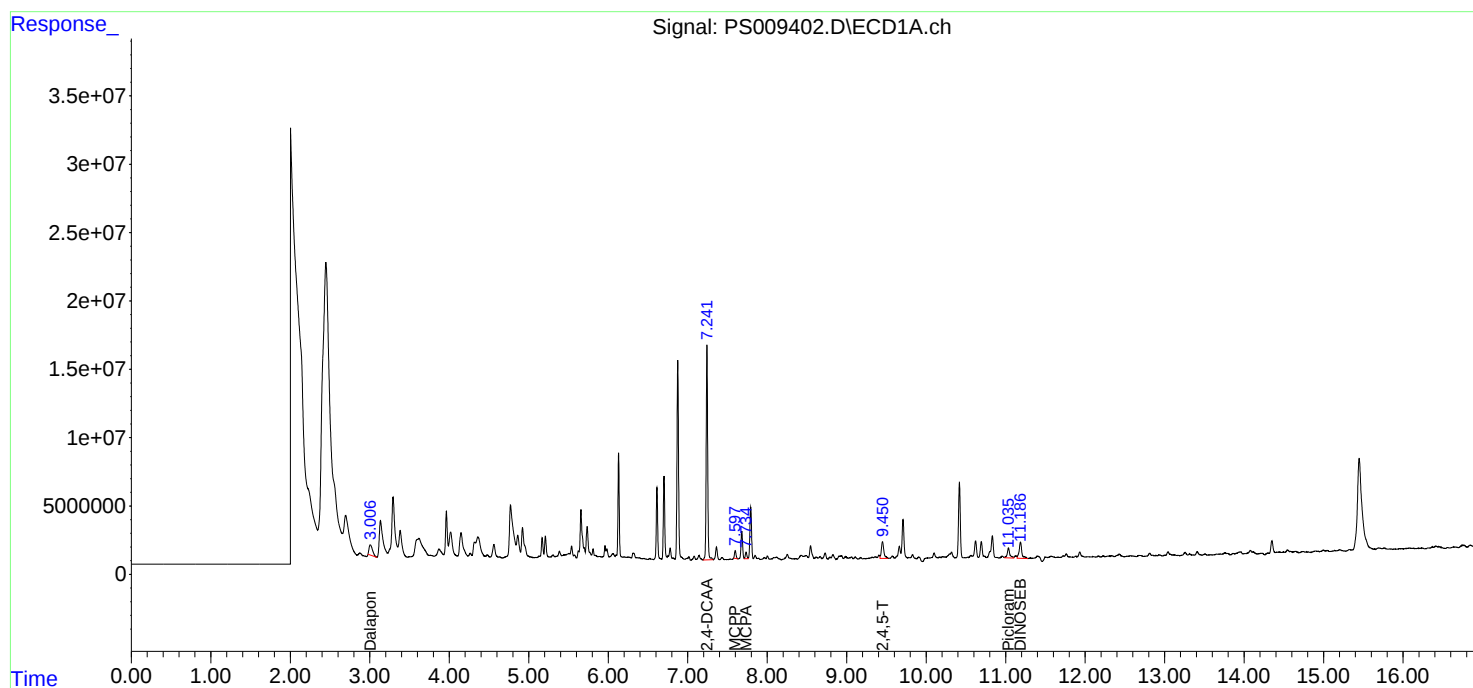


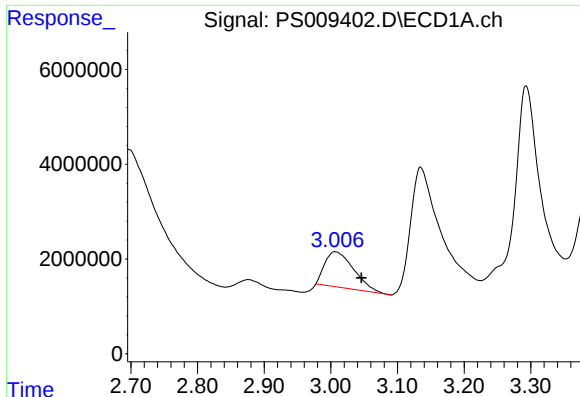

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 22397183
Conc: 28.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

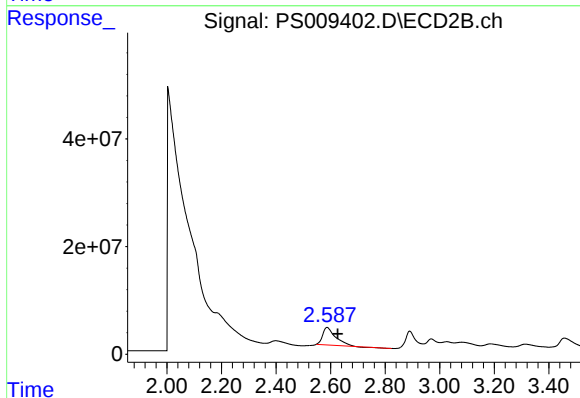


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.039 min
Response: 105669536
Conc: 134.21 ng/ml

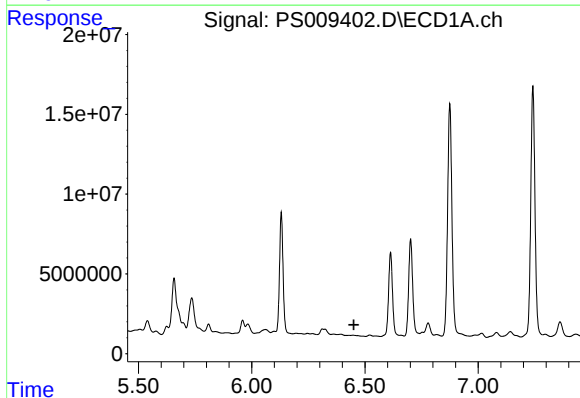


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

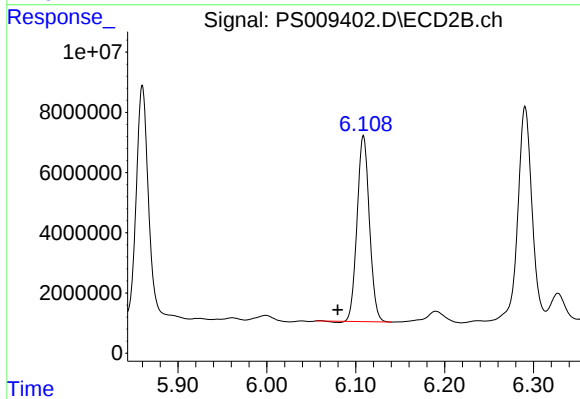

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.029 min
Response: 59426392
Conc: 73.07 ng/ml

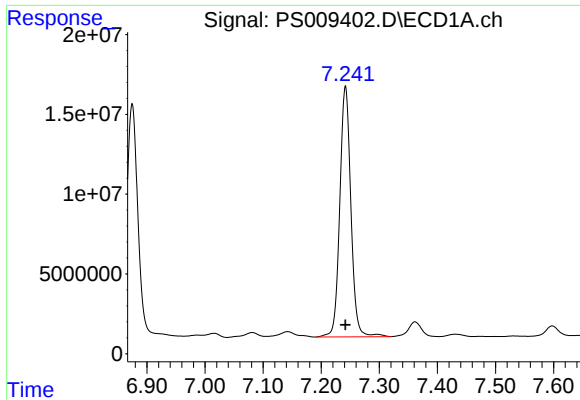

#4 2,4-DCAA


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 207533355
Conc: 375.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

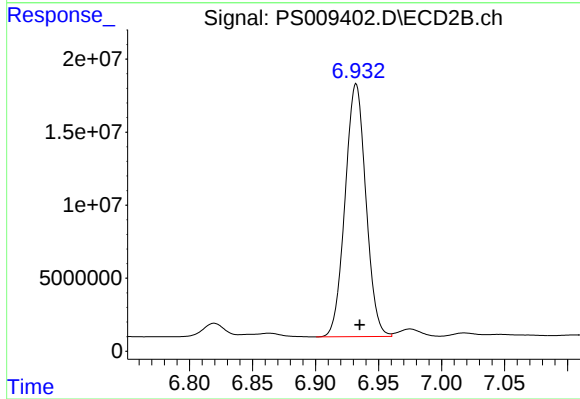


#4 2,4-DCAA

R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 199006299
Conc: 362.36 ng/ml

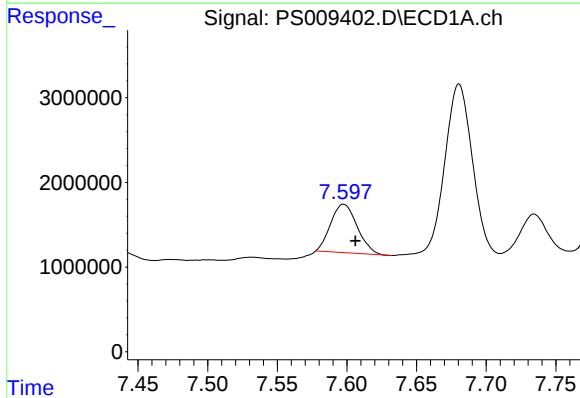


#6 MCP

R.T.: 7.598 min
Delta R.T.: -0.008 min
Response: 7539560
Conc: 3.06 ug/ml

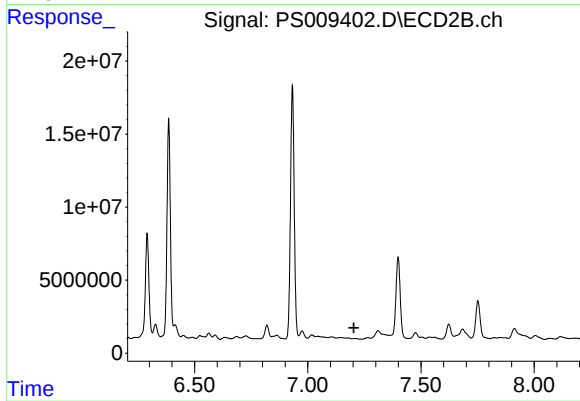

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

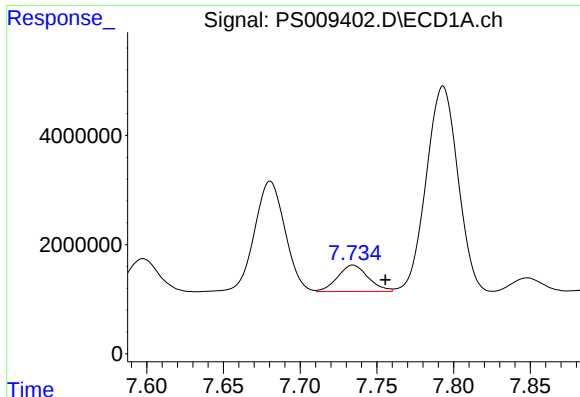

#7 MCPA


R.T.: 7.734 min
Delta R.T.: -0.021 min
Response: 6672117
Conc: 2.19 ug/ml

Instrument :
ECD_S
ClientSampleId :

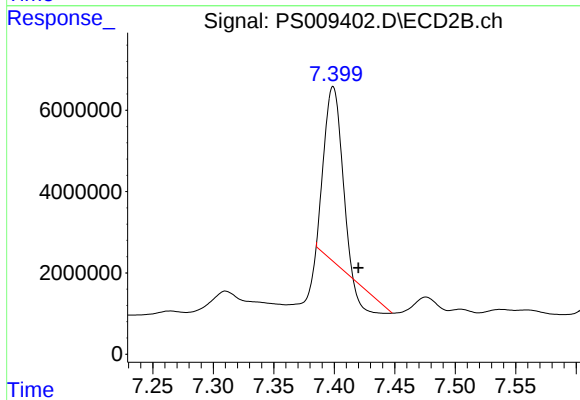


#7 MCPA

R.T.: 7.399 min
Delta R.T.: -0.021 min
Response: 36311686
Conc: 13.46 ug/ml

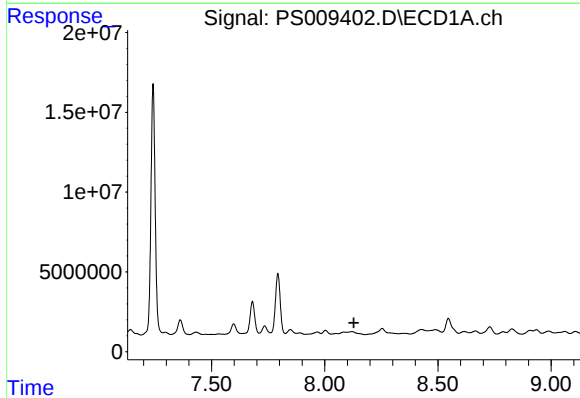


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

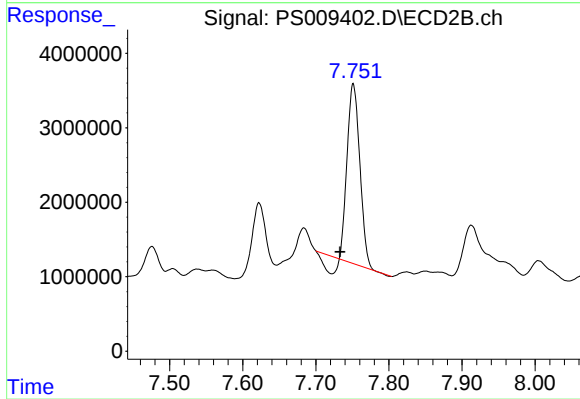

#8 DICHLORPROP


R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 26675174
Conc: 48.08 ng/ml

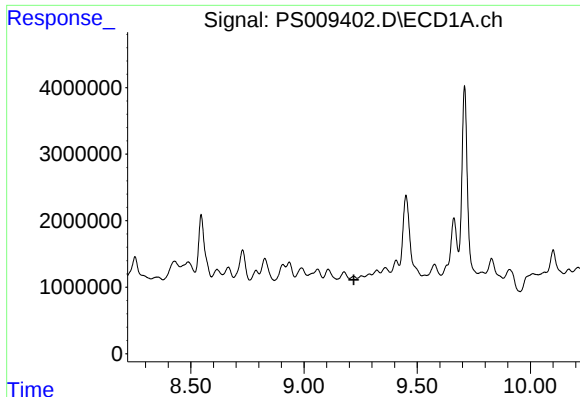

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

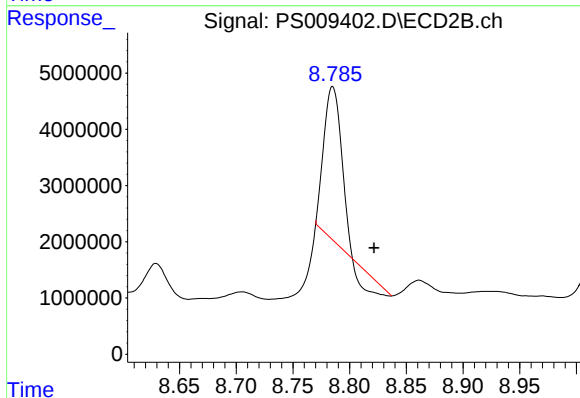


#11 2,4,5-TP (SILVEX)

R.T.: 8.785 min
Delta R.T.: -0.036 min
Response: 25495621
Conc: 8.55 ng/ml

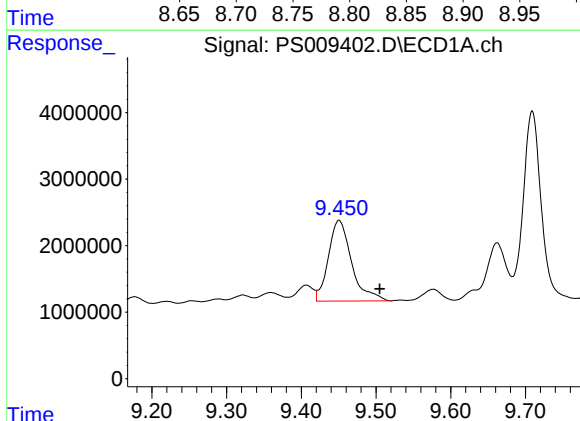


#12 2,4,5-T

R.T.: 9.451 min
Delta R.T.: -0.054 min
Response: 26205390
Conc: 10.30 ng/ml

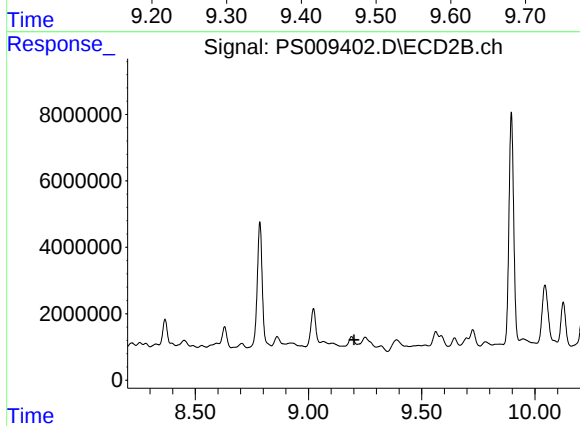

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

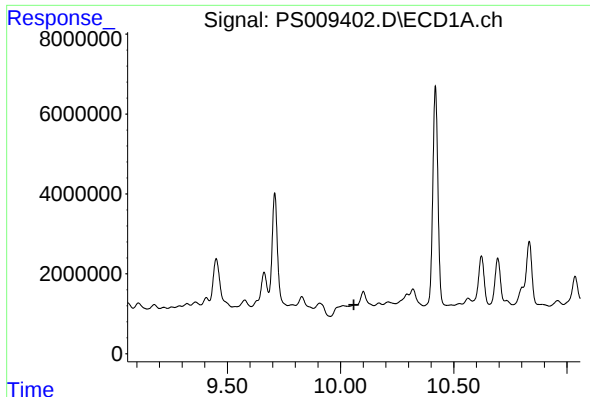

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

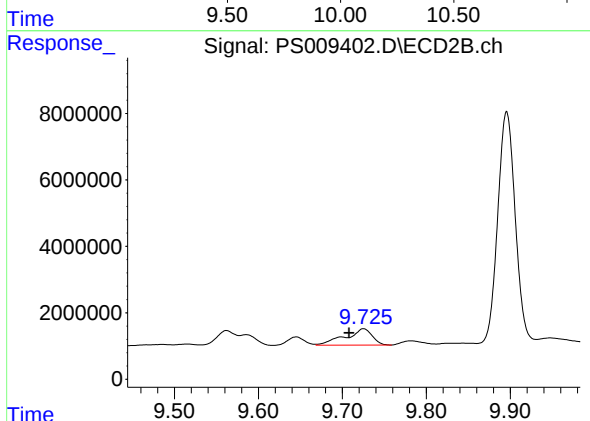


#13 2,4-DB

R.T.: 9.725 min
Delta R.T.: 0.017 min
Response: 11004954
Conc: 28.99 ng/ml

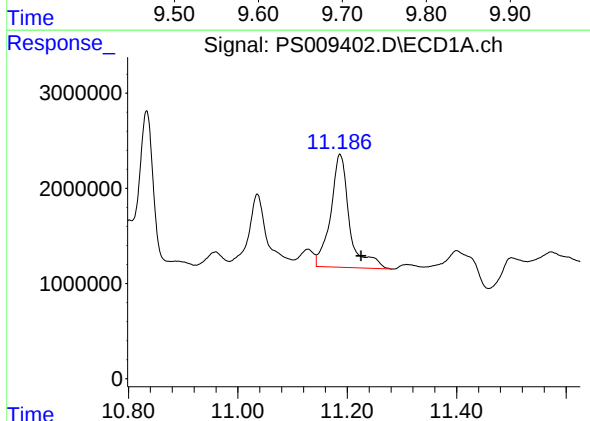


#14 DINOSEB

R.T.: 11.187 min
Delta R.T.: -0.038 min
Response: 28425775
Conc: 13.91 ng/ml

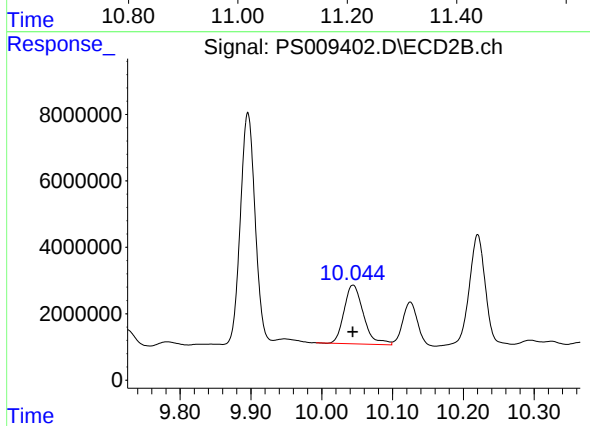

#14 DINOSEB


R.T.: 10.044 min
Delta R.T.: 0.000 min
Response: 33532817
Conc: 15.27 ng/ml

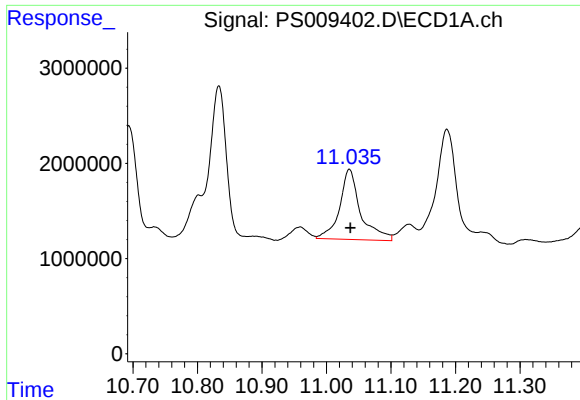

#15 Picloram


R.T.: 11.036 min
Delta R.T.: -0.002 min
Response: 16695687
Conc: 5.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

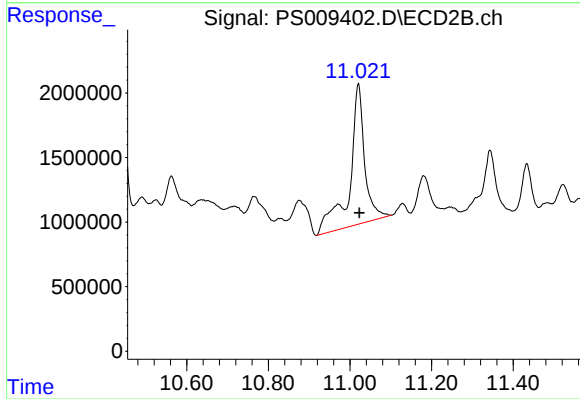


#15 Picloram

R.T.: 11.020 min
Delta R.T.: -0.003 min
Response: 27548422
Conc: 6.77 ng/ml

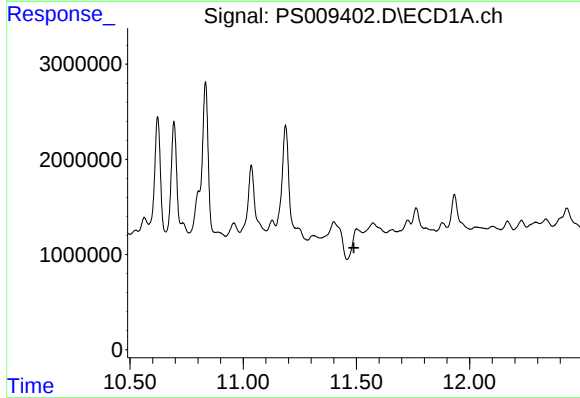

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

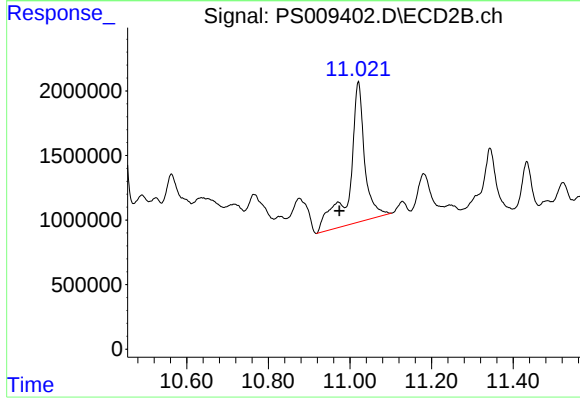

#16 DCPA

R.T.: 11.020 min
Delta R.T.: 0.046 min
Response: 27548422
Conc: 7.11 ng/ml