

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032320\
 Data File : PS009405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2020 18:29
 Operator : DD\AJ
 Sample : L1762-18
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 18:46:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.932	139.8E6	130.5E6	252.636	237.707
Target Compounds							
1) T	Dalapon	3.007	2.588	20193477	78109524	25.895	99.204 #
2) T	3,5-DICHL...	0.000	6.109	0	70489994	N.D.	86.671
6) T	MCP	7.597	0.000	8642144	0	3.512	N.D. #
7) T	MCPA	7.793	7.399	60836324	46649023	19.975	17.286
8) T	DICHLORPROP	0.000	7.751	0	28428040	N.D.	51.238
11) T	2,4,5-TP ...	0.000	8.784	0	18177669	N.D.	6.098
12) T	2,4,5-T	9.450	0.000	33764288	0	13.273	N.D. #
14) T	DINOSEB	11.186	10.043	43459866	32067444	21.261	14.599 #
15) T	Picloram	11.012	11.020	40276375	15087784	13.271	3.705 #
16) T	DCPA	0.000	11.020	0	15087784	N.D.	3.896



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032320\
Data File : PS009405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2020 18:29
Operator : DD\AJ
Sample : L1762-18
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 18:46:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

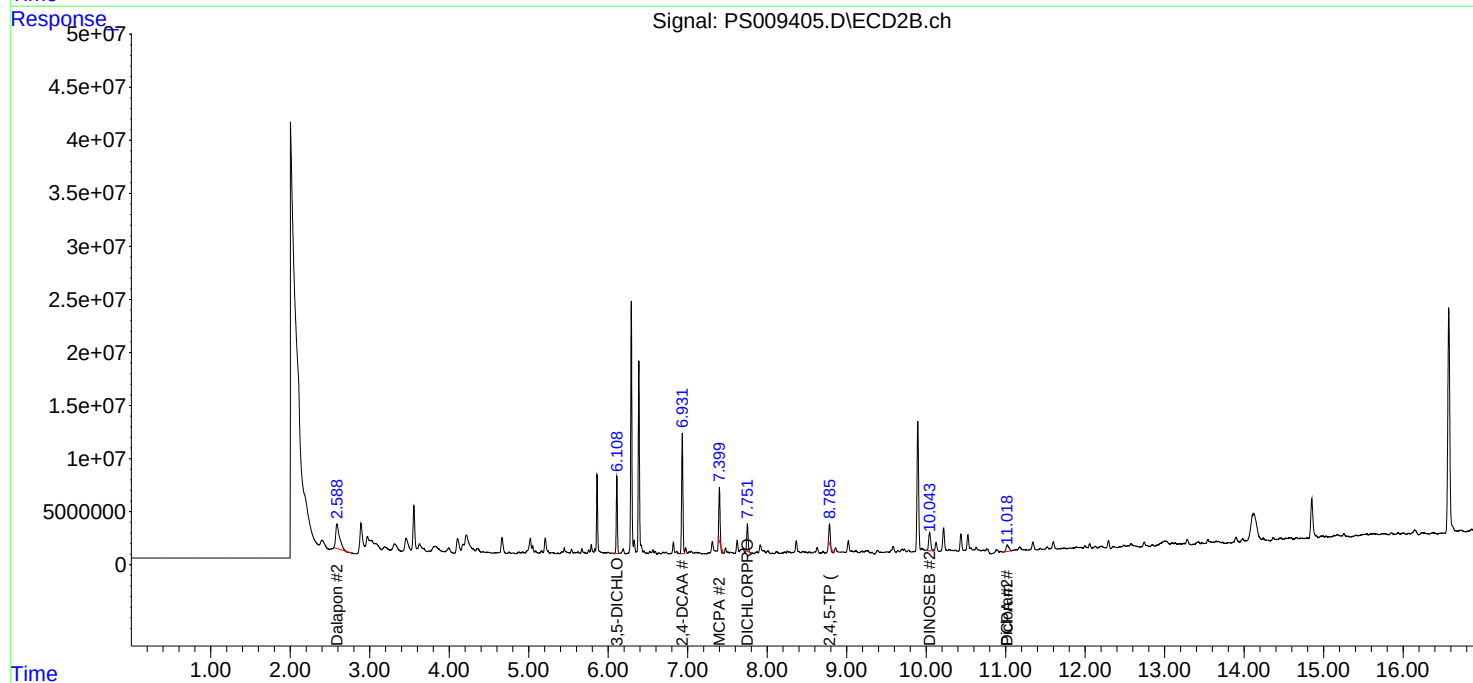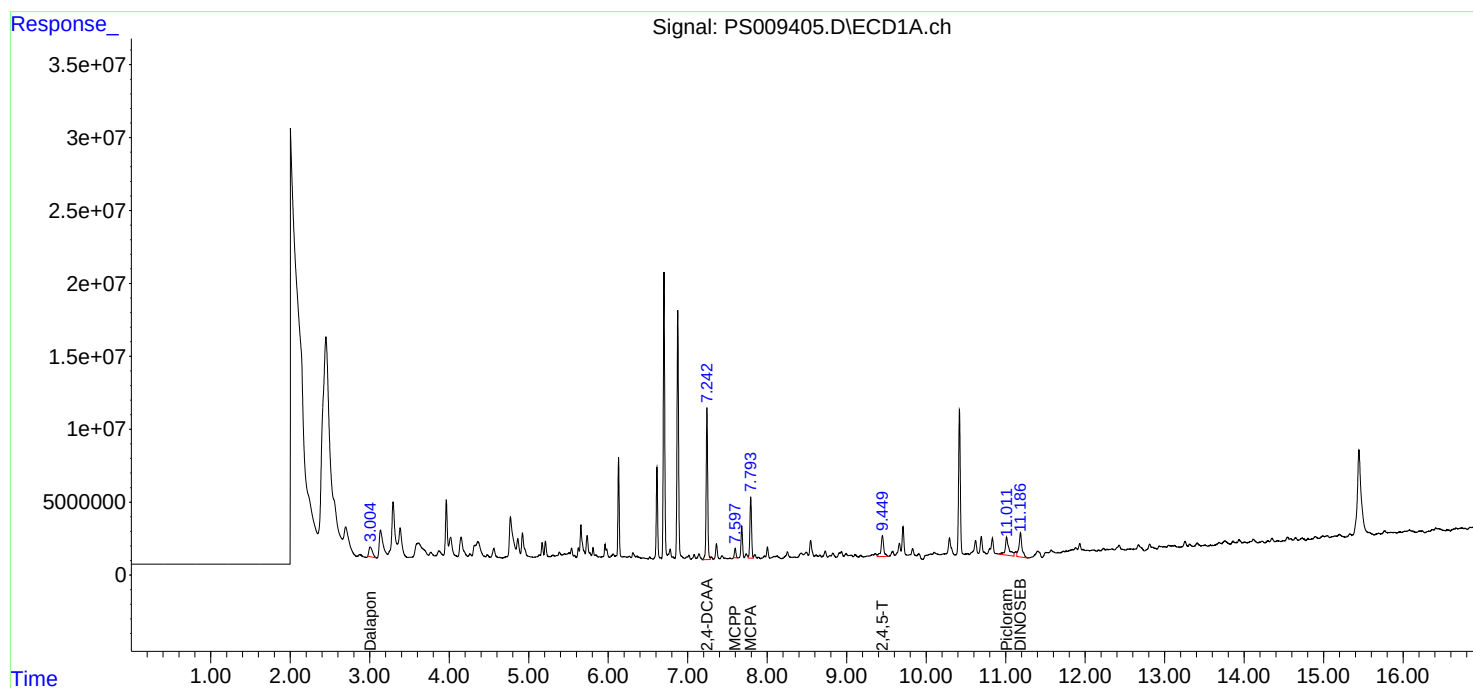


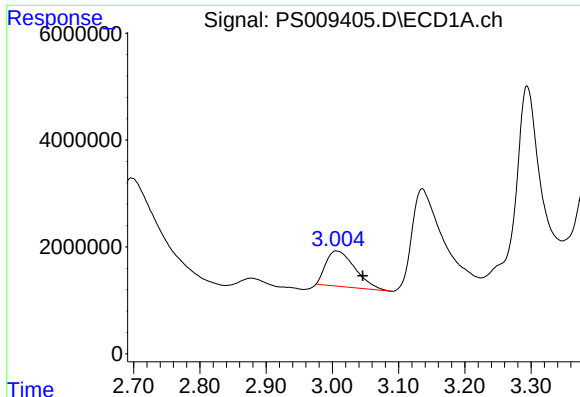

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 20193477
Conc: 25.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

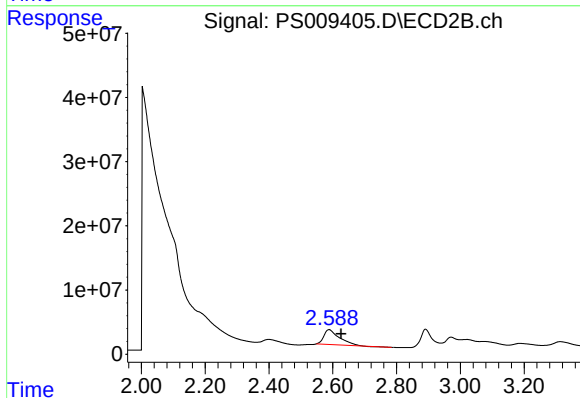


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 78109524
Conc: 99.20 ng/ml

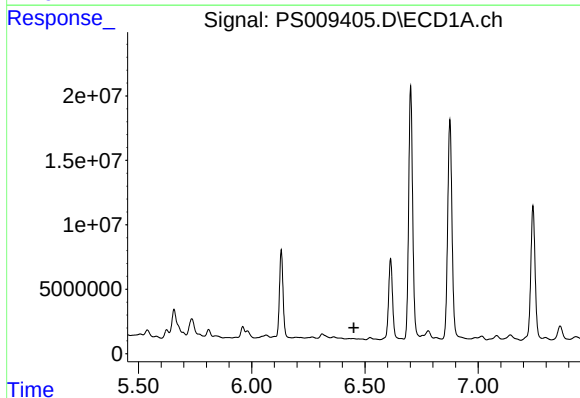


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

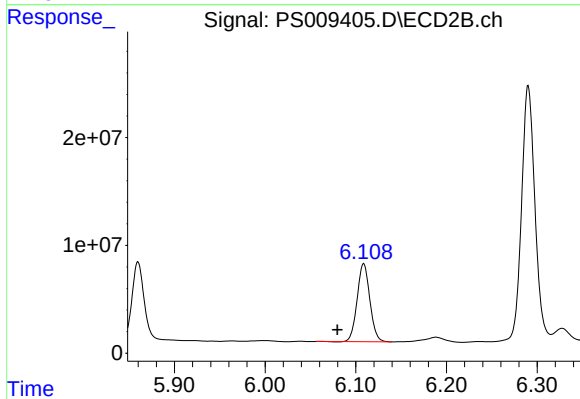

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.029 min
Response: 70489994
Conc: 86.67 ng/ml

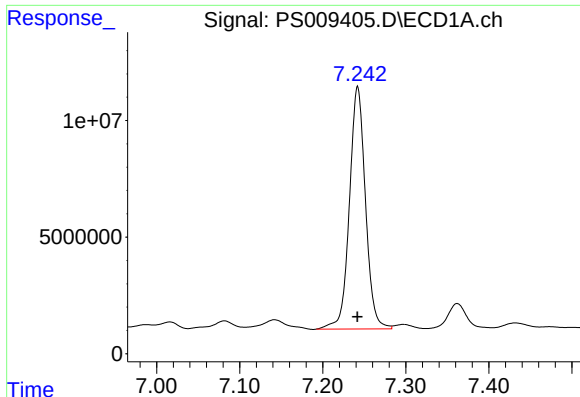

#4 2,4-DCAA


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 139750683
Conc: 252.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

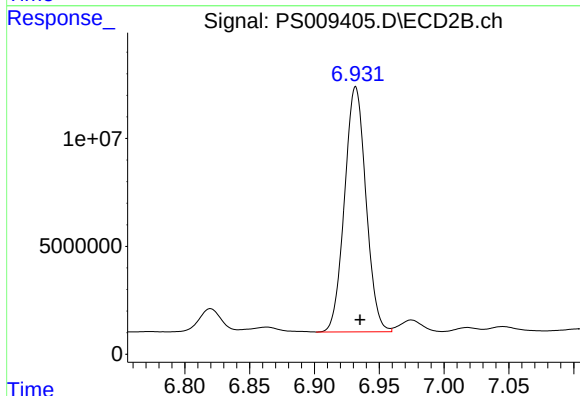


#4 2,4-DCAA

R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 130547978
Conc: 237.71 ng/ml

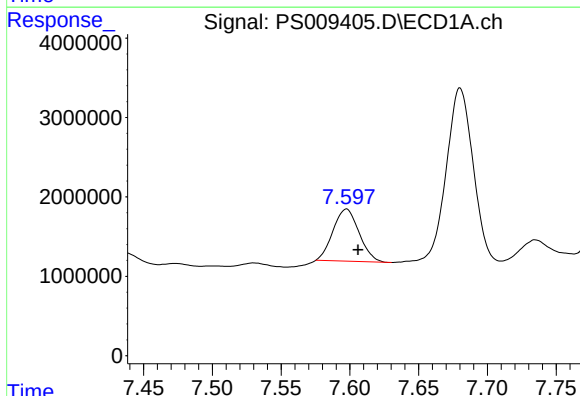


#6 MCPP

R.T.: 7.597 min
Delta R.T.: -0.009 min
Response: 8642144
Conc: 3.51 ug/ml

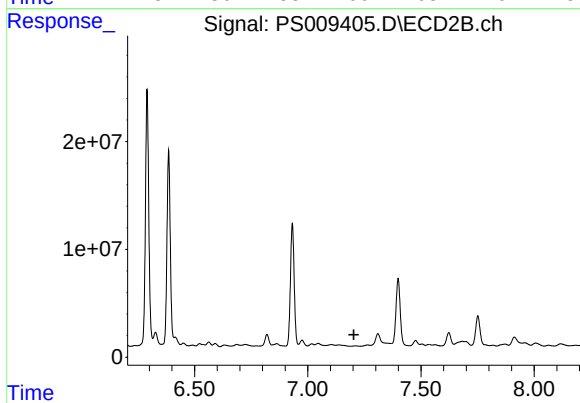

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

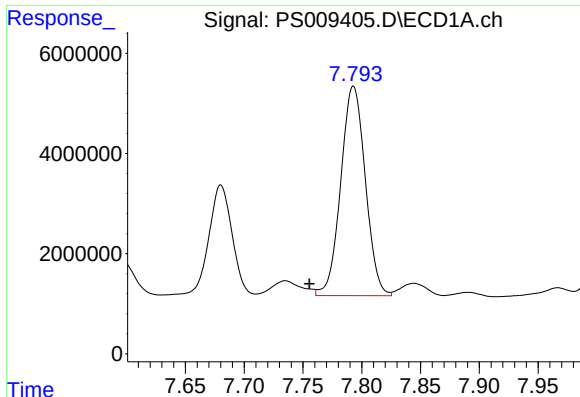

#7 MCPA


R.T.: 7.793 min
Delta R.T.: 0.037 min
Response: 60836324
Conc: 19.97 ug/ml

Instrument :
ECD_S
ClientSampleId :

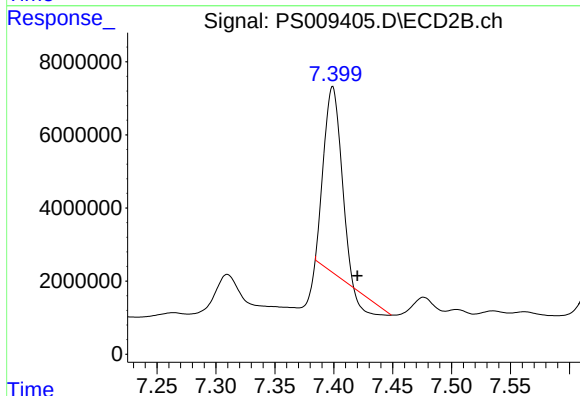


#7 MCPA

R.T.: 7.399 min
Delta R.T.: -0.021 min
Response: 46649023
Conc: 17.29 ug/ml

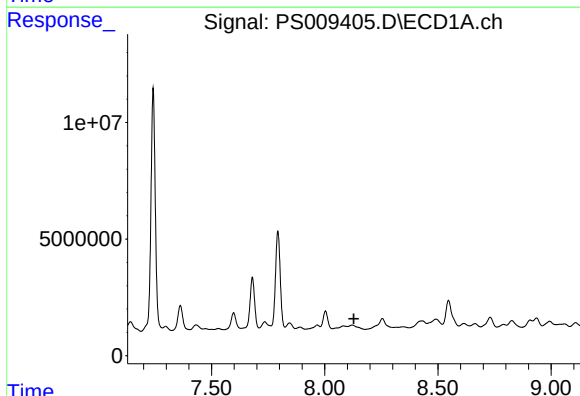


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

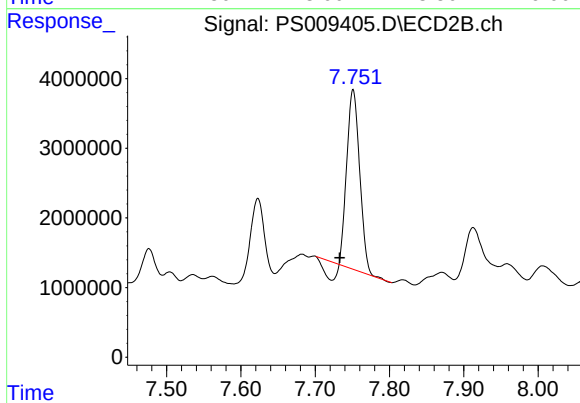

#8 DICHLORPROP


R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 28428040
Conc: 51.24 ng/ml

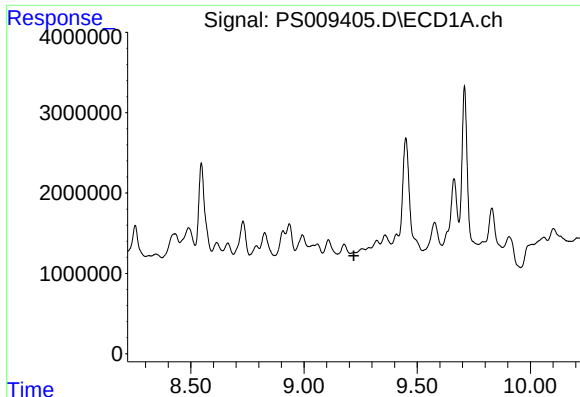

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

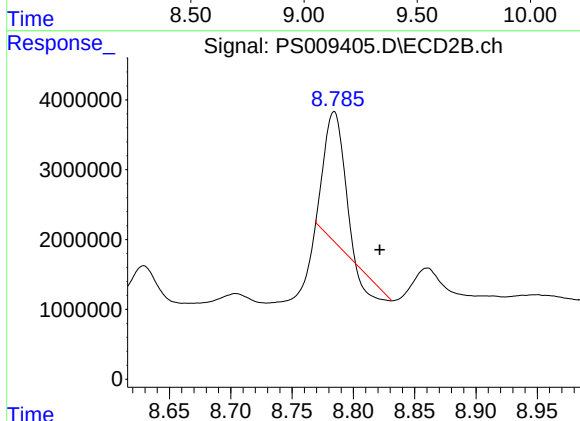


#11 2,4,5-TP (SILVEX)

R.T.: 8.784 min
Delta R.T.: -0.037 min
Response: 18177669
Conc: 6.10 ng/ml

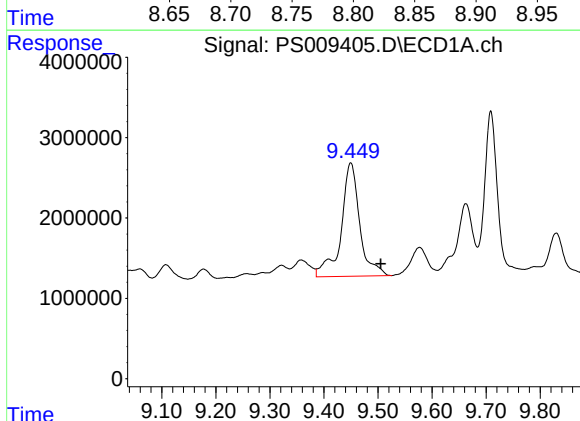


#12 2,4,5-T

R.T.: 9.450 min
Delta R.T.: -0.055 min
Response: 33764288
Conc: 13.27 ng/ml

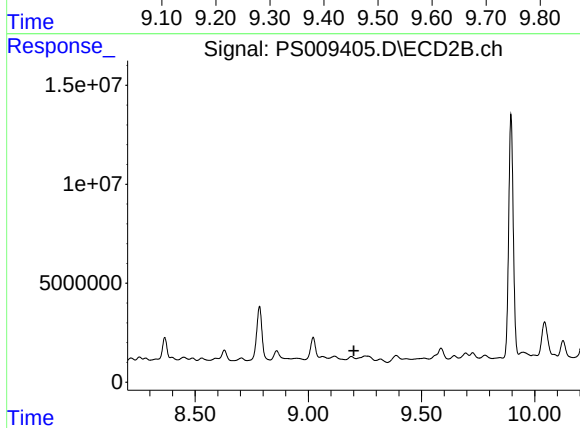

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

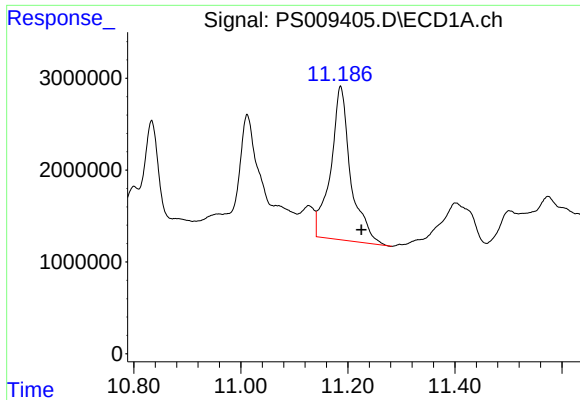

#14 DINOSEB


R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 43459866
Conc: 21.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

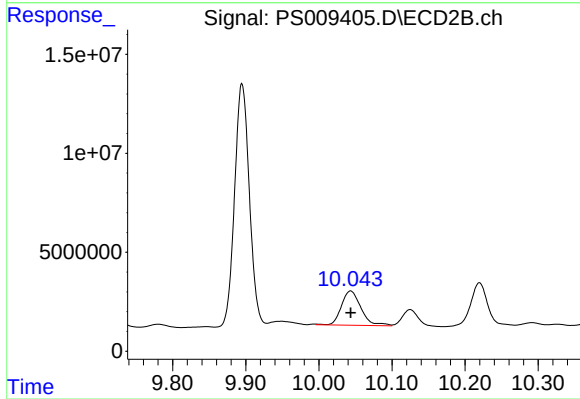


#14 DINOSEB

R.T.: 10.043 min
Delta R.T.: 0.000 min
Response: 32067444
Conc: 14.60 ng/ml

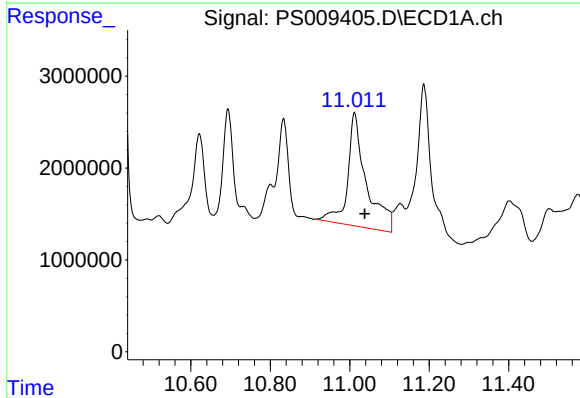


#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.025 min
Response: 40276375
Conc: 13.27 ng/ml

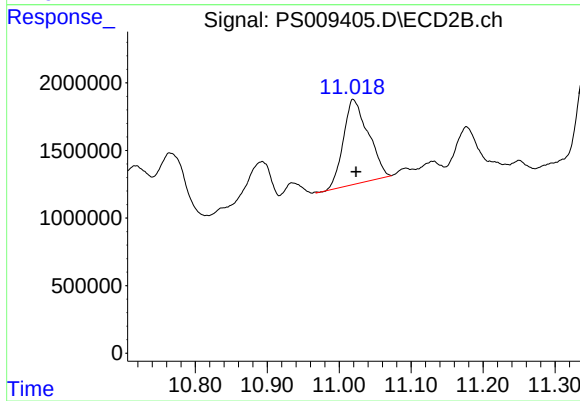

#15 Picloram


R.T.: 11.020 min
Delta R.T.: -0.003 min
Response: 15087784
Conc: 3.71 ng/ml

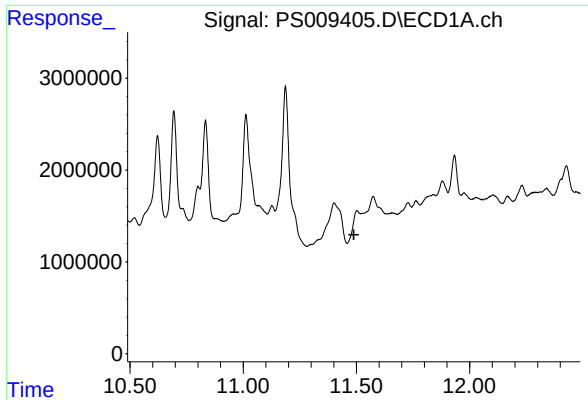

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

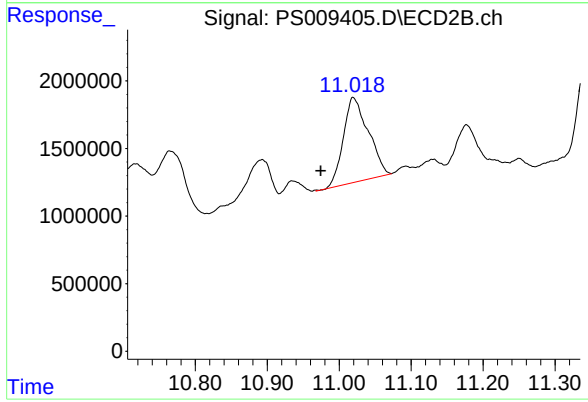

#16 DCPA

R.T.: 11.020 min
Delta R.T.: 0.046 min
Response: 15087784
Conc: 3.90 ng/ml