

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032321\
 Data File : PS014322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2021 08:32
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 12:14:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.432	0.000	52195010	0	27.036	N.D. #
3) T	4-Nitroph...	6.957f	0.000	624860	0	<MDL	N.D. #
5) T	DICAMBA	7.427f	7.120f	27878104	21191692	5.184	10.578 #
6) T	MCP	0.000	7.120	0	21191692	N.D.	12.727
7) T	MCPA	7.651	0.000	7726966	0	1.343	N.D. #
8) T	DICHLORPROP	0.000	7.735f	0	958363	N.D.	1.881
11) T	2,4,5-TP ...	9.142	0.000	8145712	0	1.057	N.D. #
13) T	2,4-DB	9.921	0.000	26907224	0	17.400	N.D. #
15) T	Picloram	10.900	10.991	41283796	3176139	3.953	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032321\
Data File : PS014322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2021 08:32
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 12:14:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

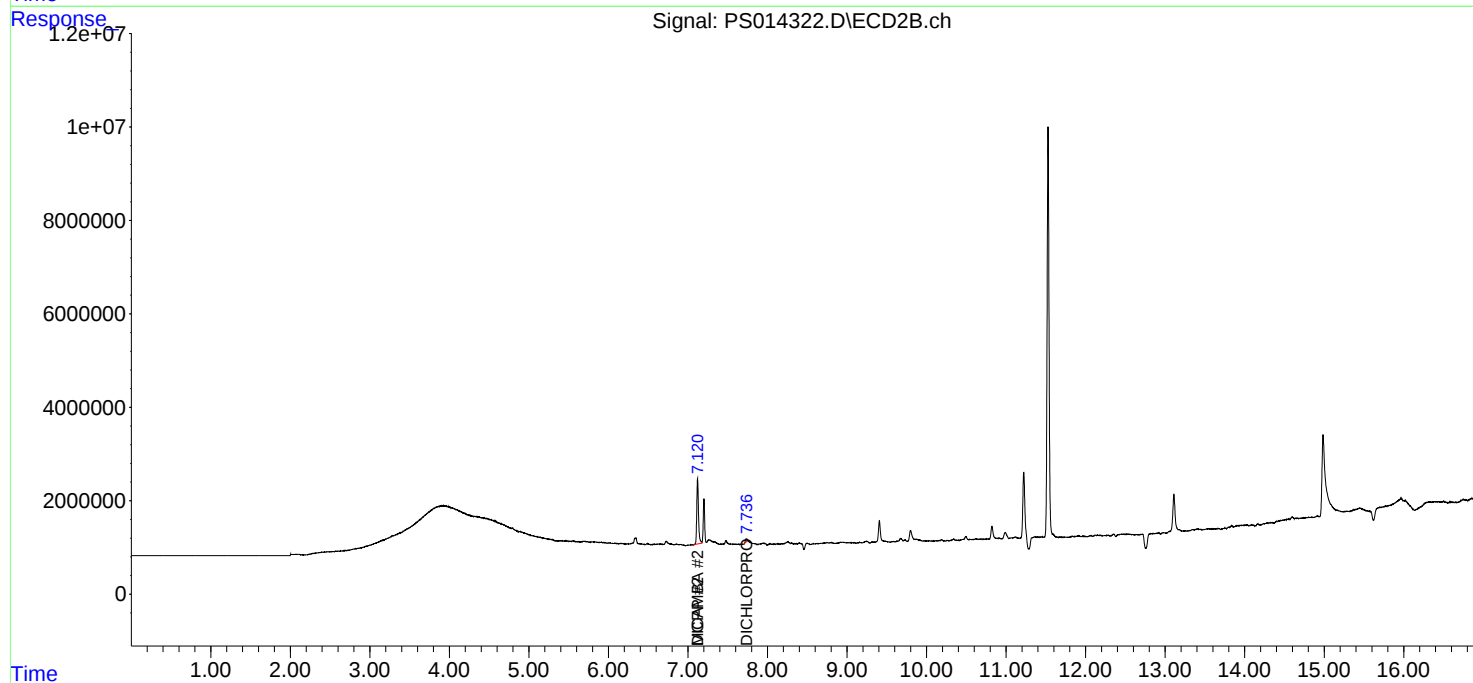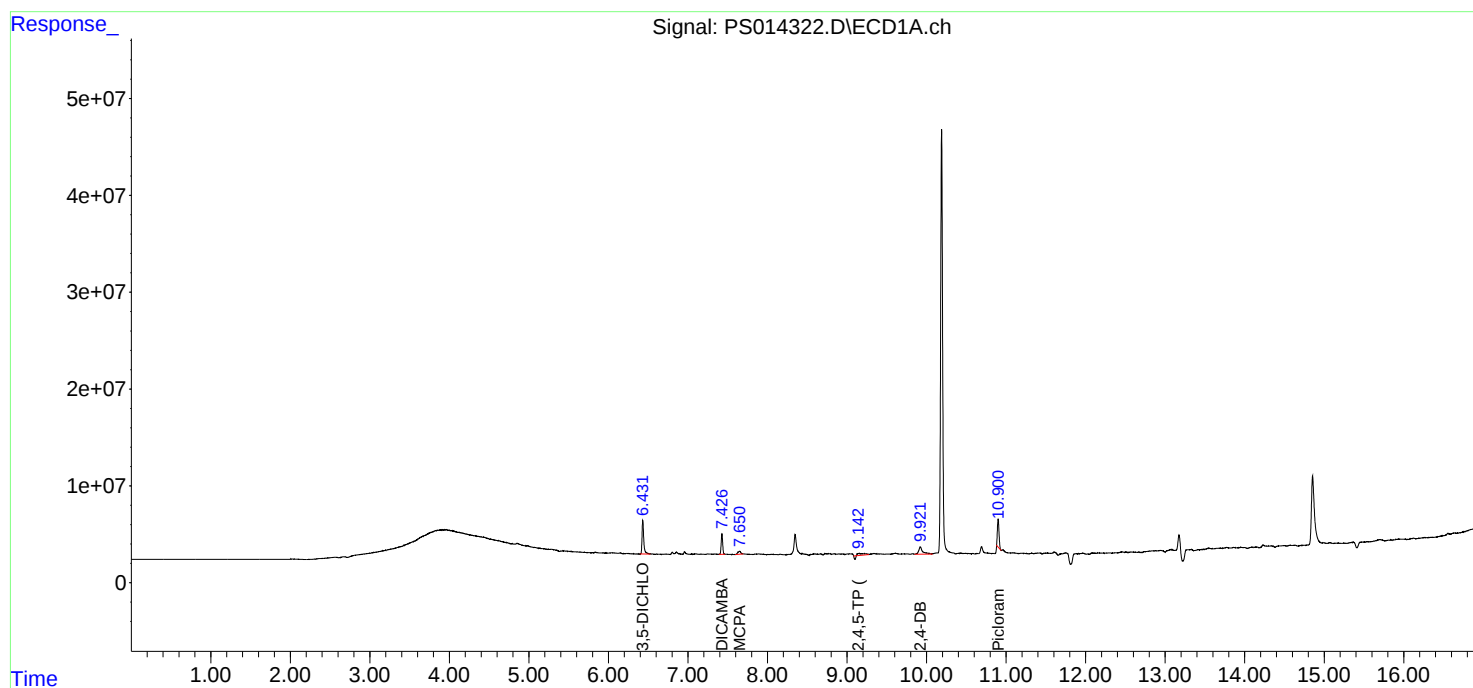


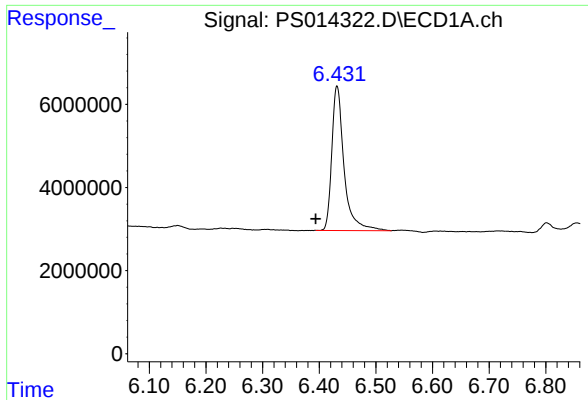

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.432 min
Delta R.T.: 0.037 min
Response: 52195010
Conc: 27.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

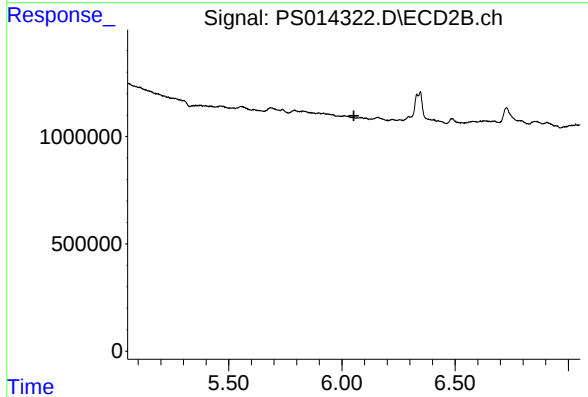


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

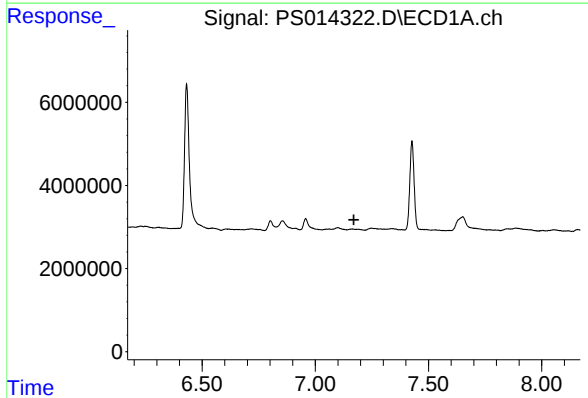


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.170 min
Response: 0
Conc: N.D.

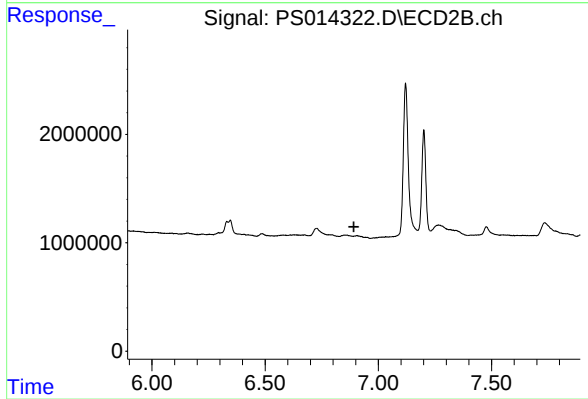

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.892 min
Response: 0
Conc: N.D.

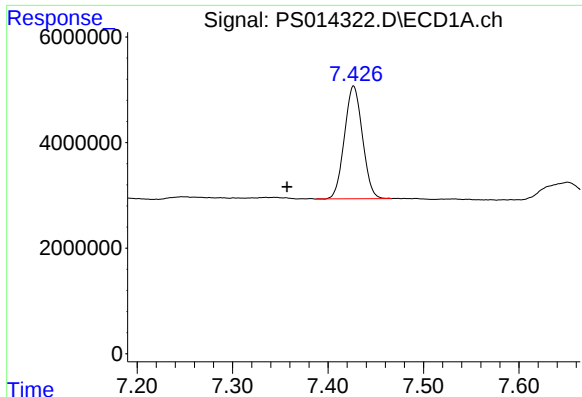

#5 DICAMBA


R.T.: 7.427 min
Delta R.T.: 0.070 min
Response: 27878104
Conc: 5.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

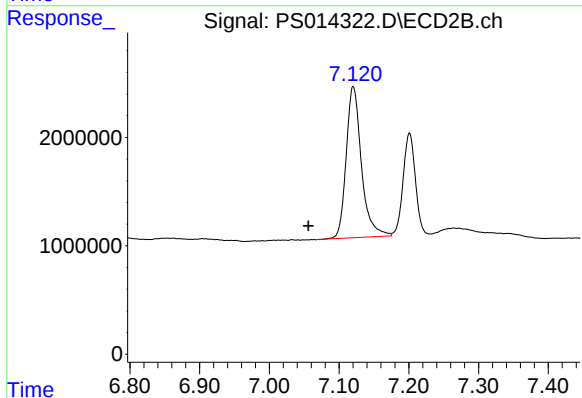


#5 DICAMBA

R.T.: 7.120 min
Delta R.T.: 0.064 min
Response: 21191692
Conc: 10.58 ng/ml

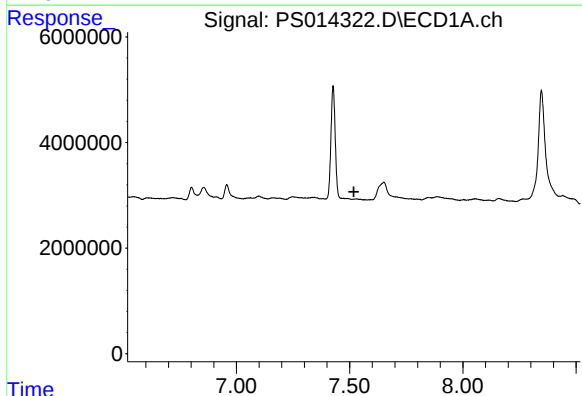


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.518 min
Response: 0
Conc: N.D.

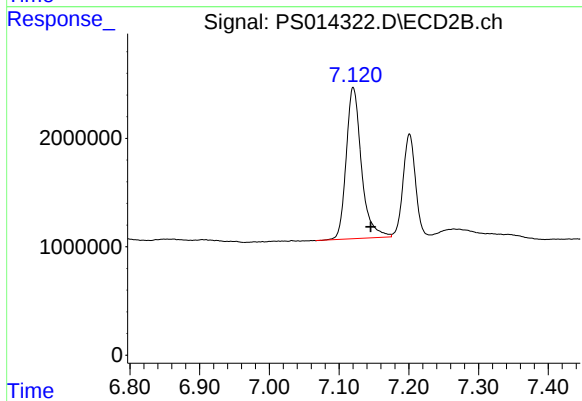

#6 MCP


R.T.: 7.120 min
Delta R.T.: -0.025 min
Response: 21191692
Conc: 12.73 ug/ml

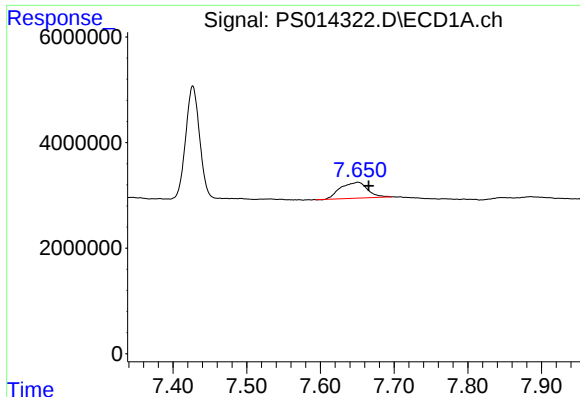

#7 MCPA


R.T.: 7.651 min
Delta R.T.: -0.015 min
Response: 7726966
Conc: 1.34 ug/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

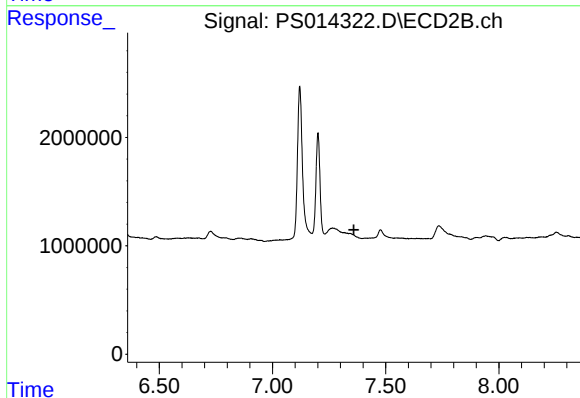


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.359 min
Response: 0
Conc: N.D.

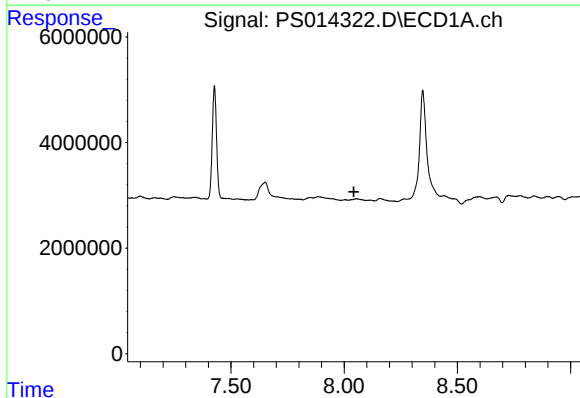


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.043 min
Response: 0
Conc: N.D.

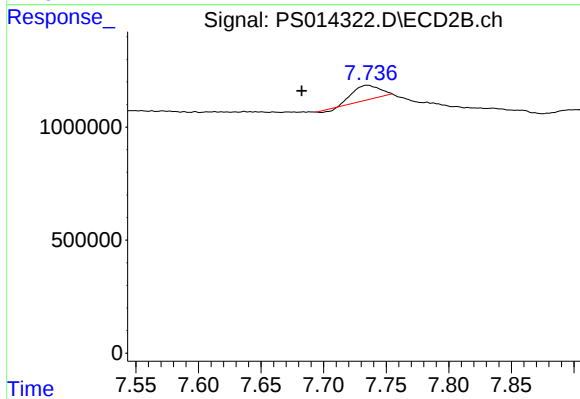

#8 DICHLORPROP


R.T.: 7.735 min
Delta R.T.: 0.052 min
Response: 958363
Conc: 1.88 ng/ml

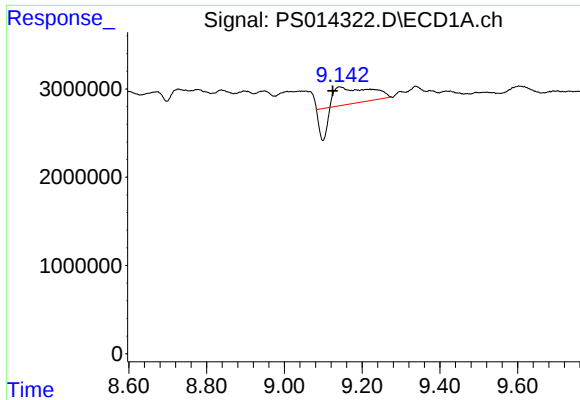

#11 2,4,5-TP (SILVEX)


R.T.: 9.142 min
Delta R.T.: 0.018 min
Response: 8145712
Conc: 1.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

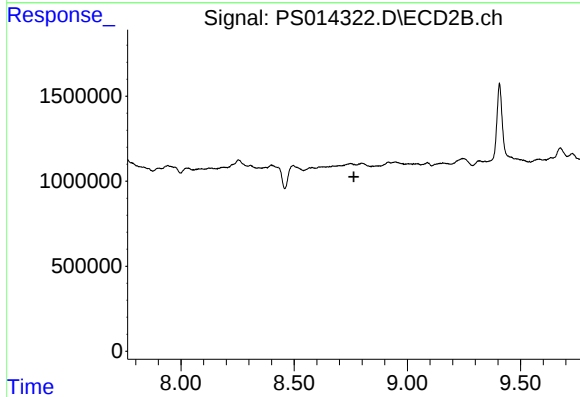


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.764 min
Response: 0
Conc: N.D.

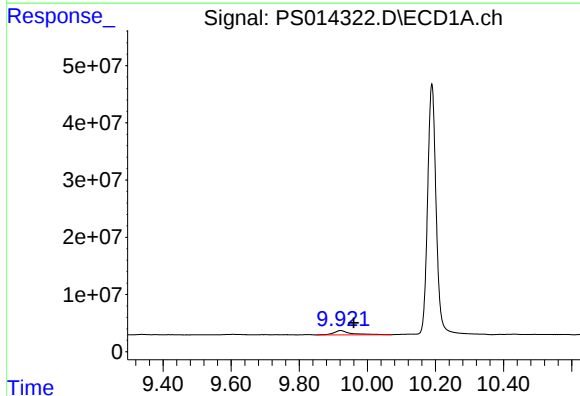


#13 2,4-DB

R.T.: 9.921 min
Delta R.T.: -0.039 min
Response: 26907224
Conc: 17.40 ng/ml

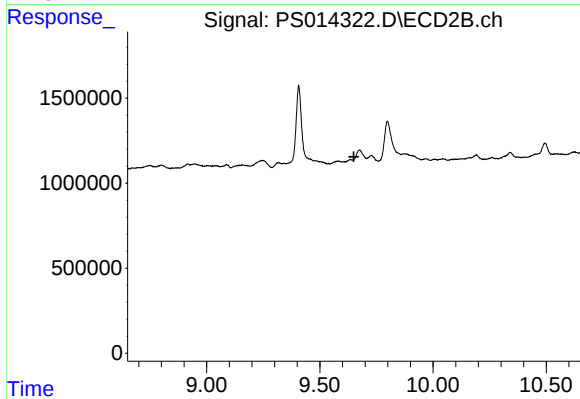

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.651 min
Response: 0
Conc: N.D.

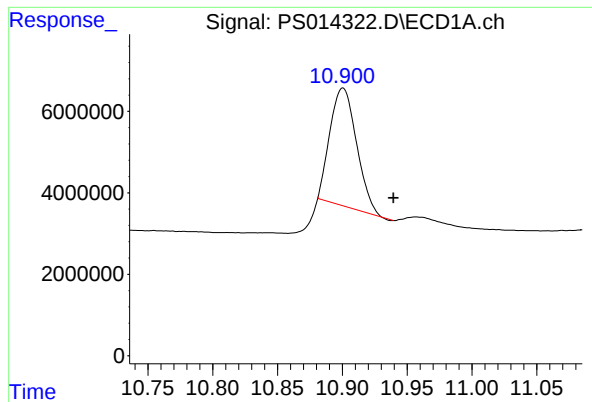

#15 Picloram

R.T.: 10.900 min
Delta R.T.: -0.039 min
Response: 41283796
Conc: 3.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

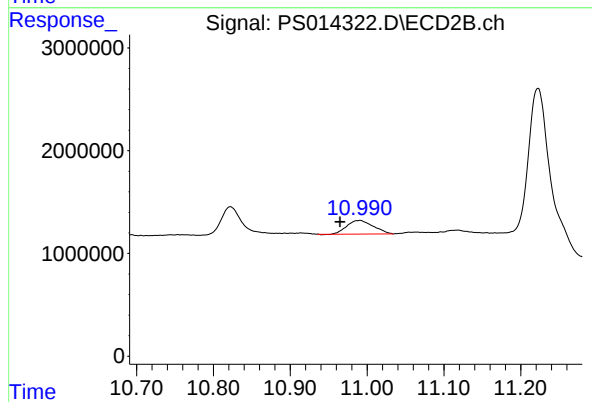

#15 Picloram

R.T.: 10.991 min
Delta R.T.: 0.026 min
Response: 3176139
Conc: N.D.