

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032322\
 Data File : PS018722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 17:21
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 02:12:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.808	1260.8E6	359.8E6	443.004	511.314
Target Compounds							
3) T	4-Nitroph...	7.119f	6.474f	635209	2298707	<MDL	5.658 #
8) T	DICHLORPROP	0.000	7.620	0	15739432	N.D.	19.883
9) T	2,4-D	8.409f	0.000	4241490	0	1.266	N.D. #
11) T	2,4,5-TP ...	9.273f	8.638f	7583059	1701246	<MDL	<MDL #
12) T	2,4,5-T	9.568f	9.109f	243861	2163976	<MDL	<MDL #
15) T	Picloram	11.031	10.876	40189493	11504876	1.955	2.164
16) T	DCPA	0.000	10.876f	0	11504876	N.D.	2.188



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032322\
Data File : PS018722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 17:21
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 02:12:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

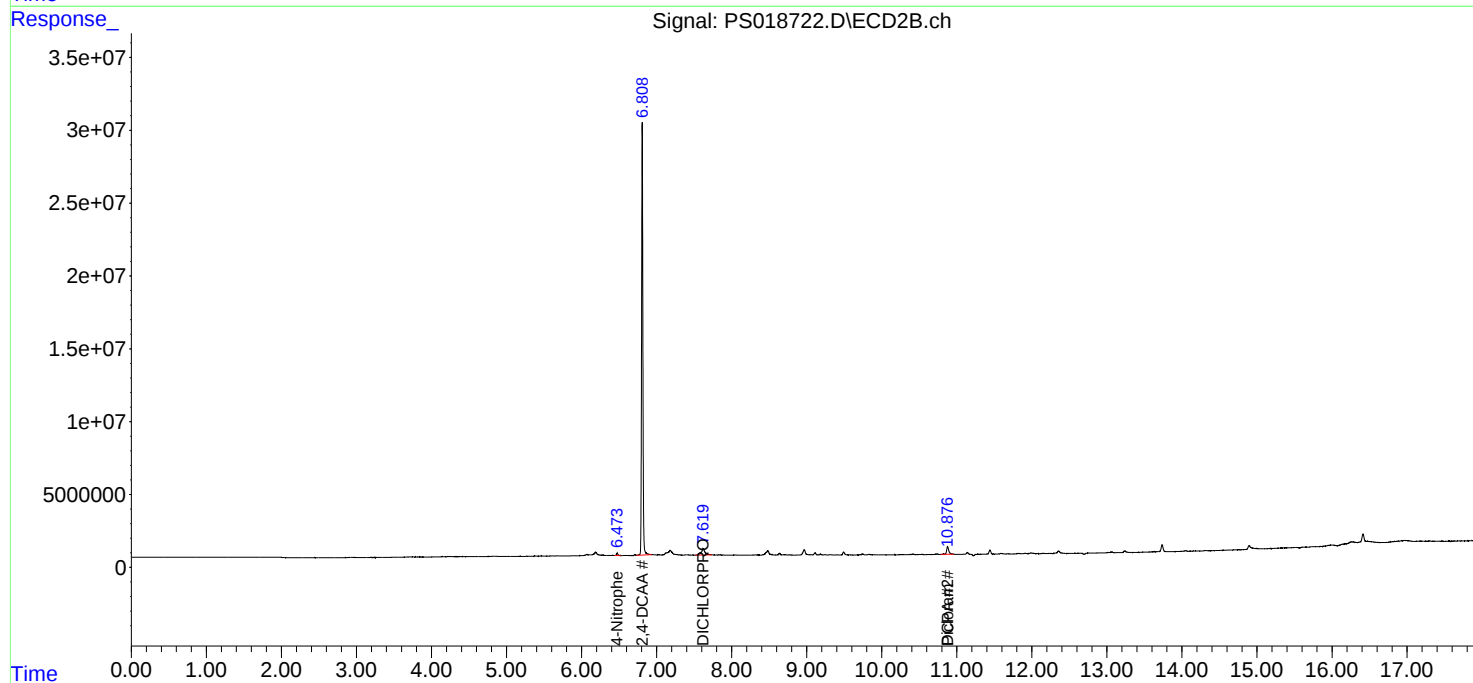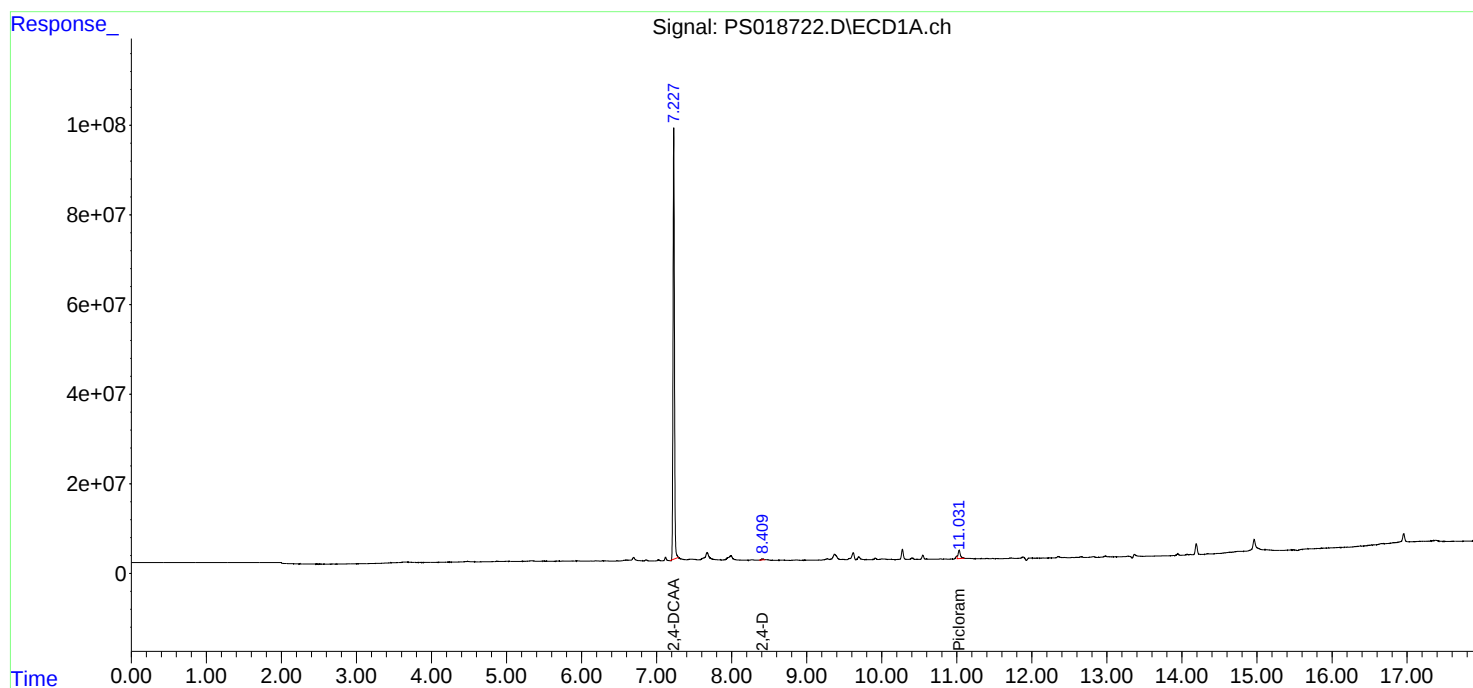


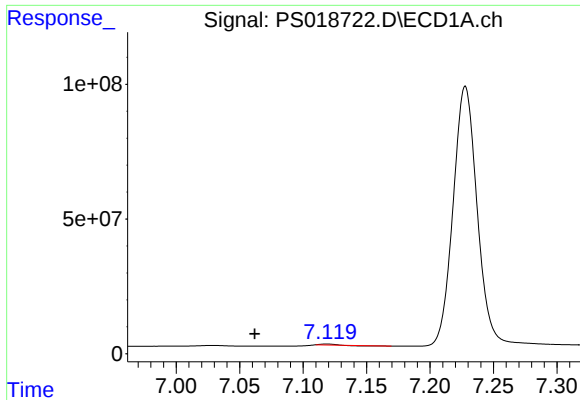

#3 4-Nitrophenol


R.T.: 7.119 min
Delta R.T.: 0.057 min
Response: 635209
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

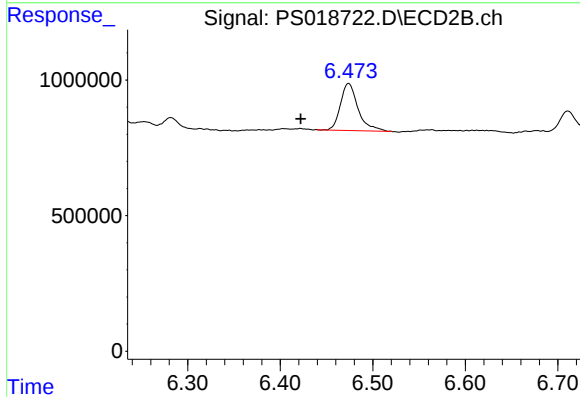


#3 4-Nitrophenol

R.T.: 6.474 min
Delta R.T.: 0.052 min
Response: 2298707
Conc: 5.66 ng/ml

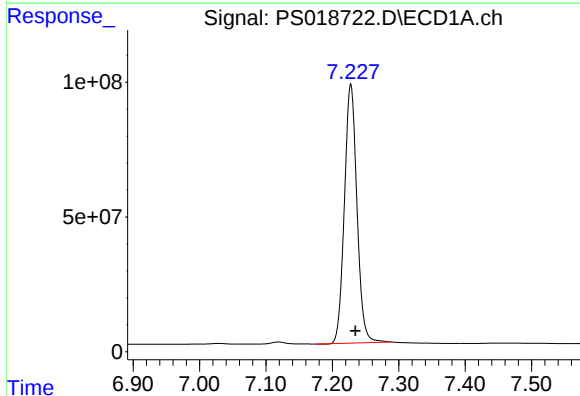


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.007 min
Response: 1260751632
Conc: 443.00 ng/ml

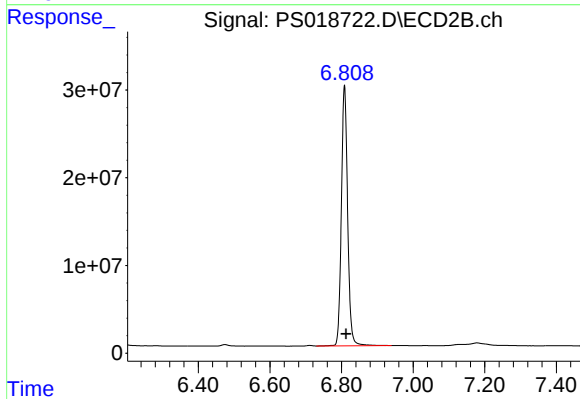

#4 2,4-DCAA


R.T.: 6.808 min
Delta R.T.: -0.005 min
Response: 359788995
Conc: 511.31 ng/ml

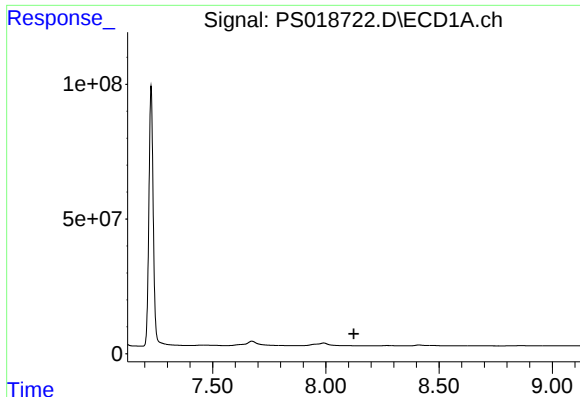

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

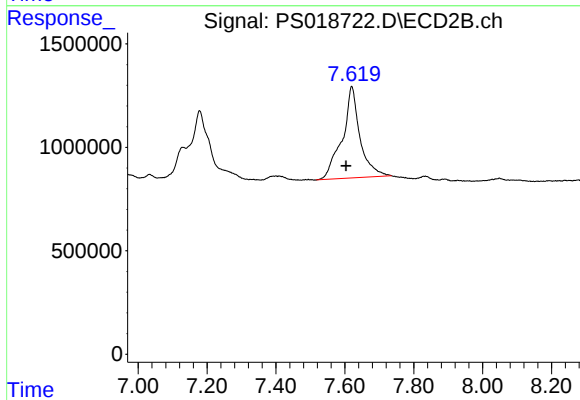


#8 DICHLORPROP

R.T.: 7.620 min
Delta R.T.: 0.016 min
Response: 15739432
Conc: 19.88 ng/ml

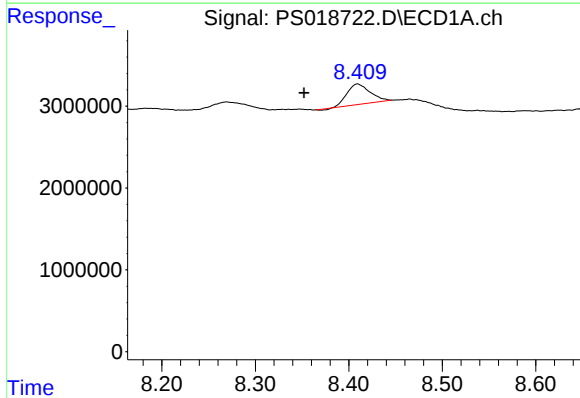


#9 2,4-D

R.T.: 8.409 min
Delta R.T.: 0.057 min
Response: 4241490
Conc: 1.27 ng/ml

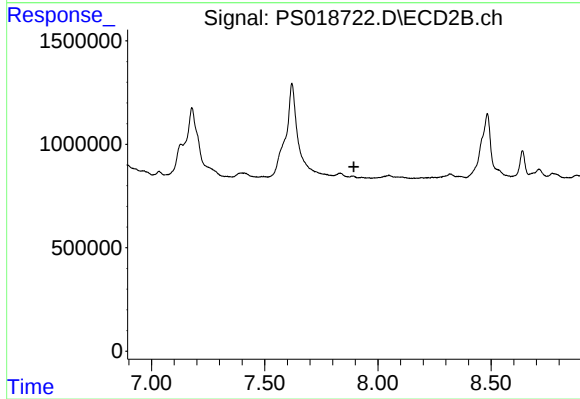

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

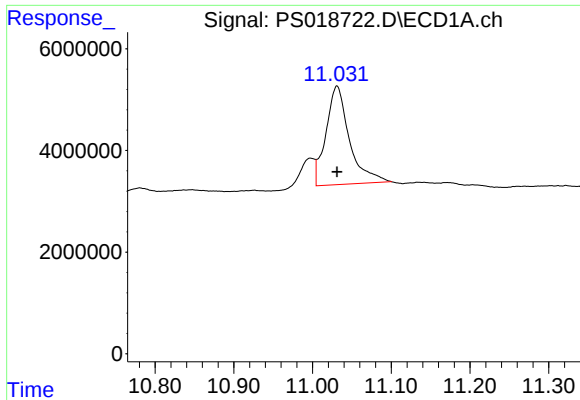

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 40189493
Conc: 1.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

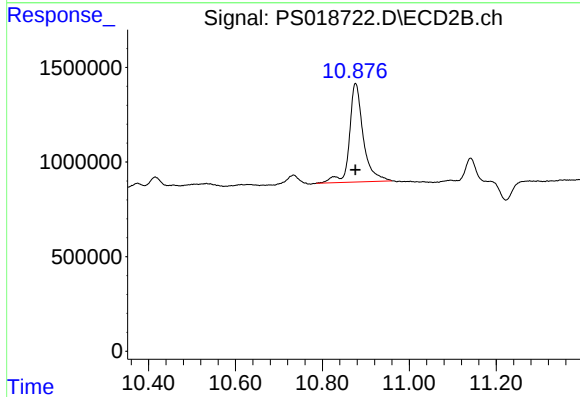


#15 Picloram

R.T.: 10.876 min
Delta R.T.: 0.000 min
Response: 11504876
Conc: 2.16 ng/ml

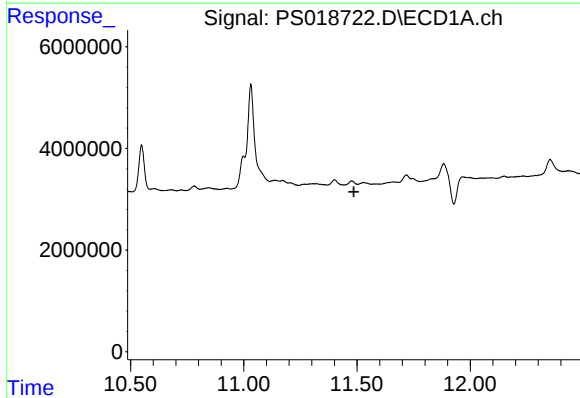

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.486 min
Response: 0
Conc: N.D.

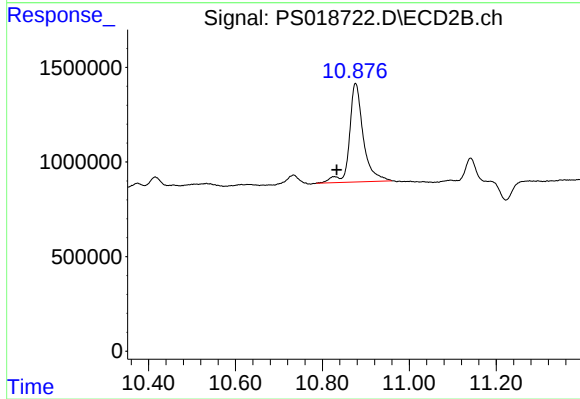

#16 DCPA

R.T.: 10.876 min
Delta R.T.: 0.043 min
Response: 11504876
Conc: 2.19 ng/ml