

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032322\
 Data File : PS018728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 19:48
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 02:14:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.808	1279.9E6	365.5E6	449.749	519.435
Target Compounds							
3) T	4-Nitroph...	7.118f	6.474f	3259454	3228104	1.892	7.946 #
5) T	DICAMBA	7.484f	0.000	7624828	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.622	0	25907071	N.D.	32.727
9) T	2,4-D	8.406f	0.000	4567335	0	1.363	N.D. #
11) T	2,4,5-TP ...	9.214	8.707	26952759	3721875	1.772	<MDL #
12) T	2,4,5-T	9.565f	9.109f	6811614	1621091	<MDL	<MDL #
14) T	DINOSEB	11.257	0.000	13969005	0	1.306	N.D. #
15) T	Picloram	11.026	10.881	14998553	27056250	<MDL	5.089 #
16) T	DCPA	0.000	10.881f	0	27056250	N.D.	5.144



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032322\
Data File : PS018728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 19:48
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 02:14:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

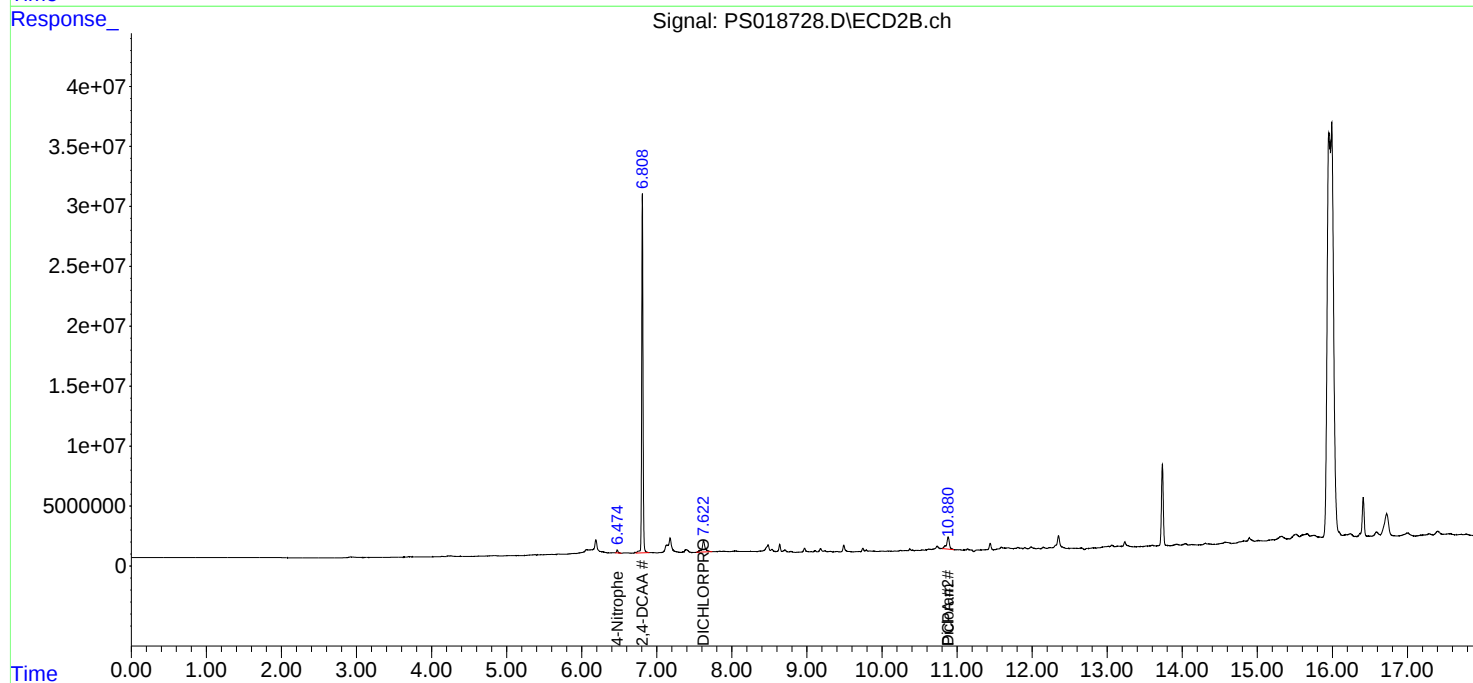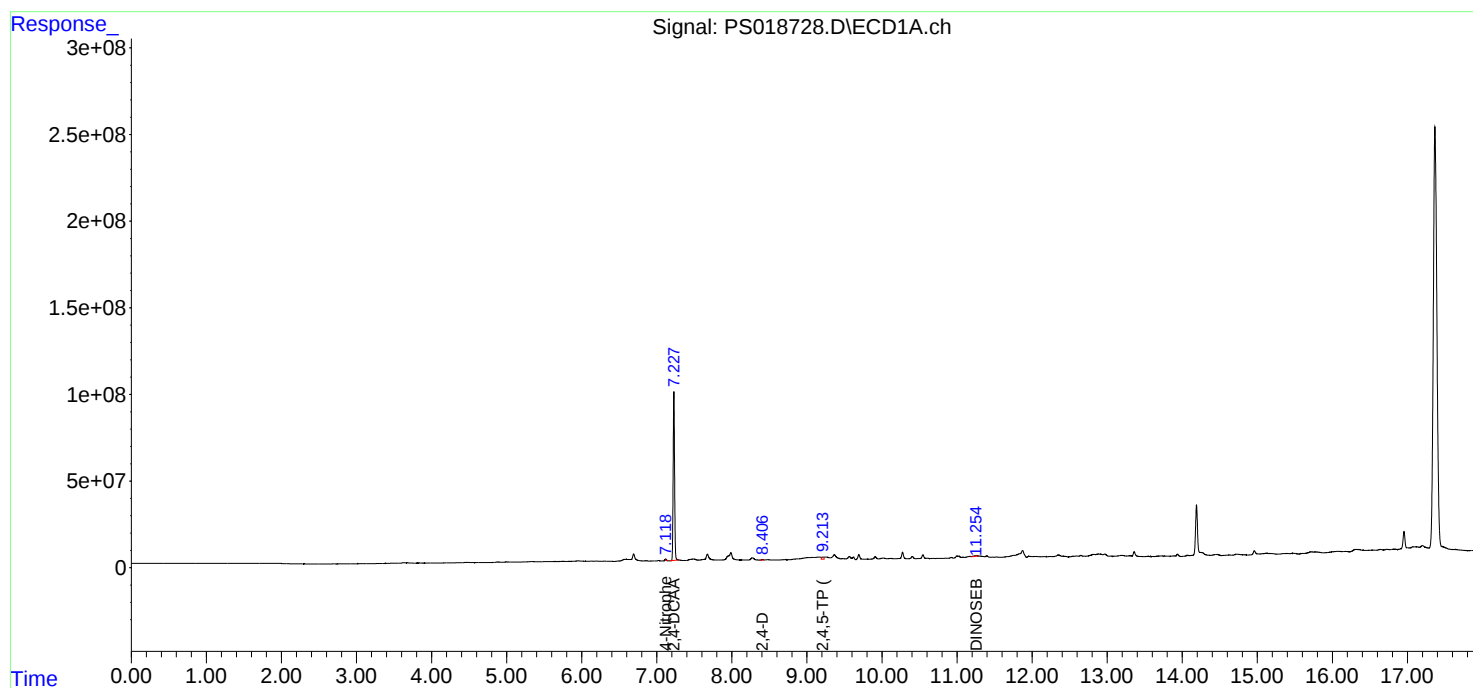


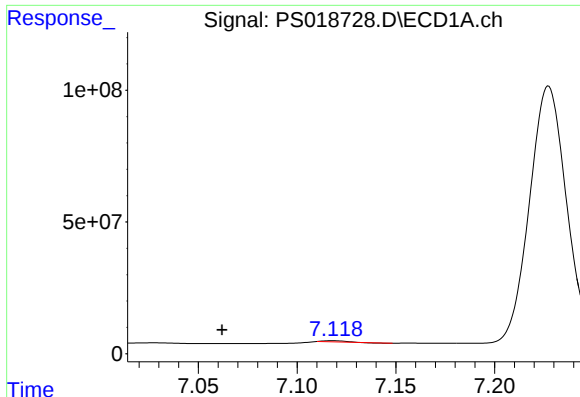

#3 4-Nitrophenol


R.T.: 7.118 min
Delta R.T.: 0.056 min
Response: 3259454
Conc: 1.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

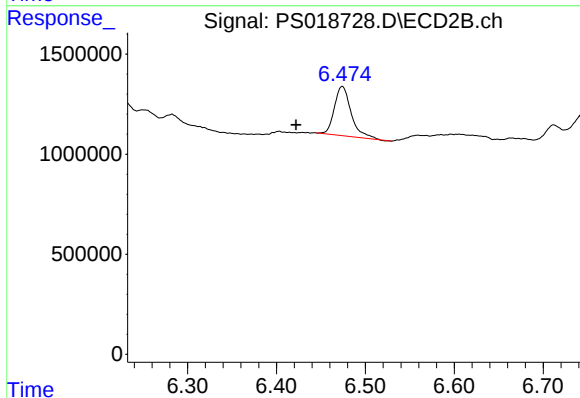


#3 4-Nitrophenol

R.T.: 6.474 min
Delta R.T.: 0.052 min
Response: 3228104
Conc: 7.95 ng/ml

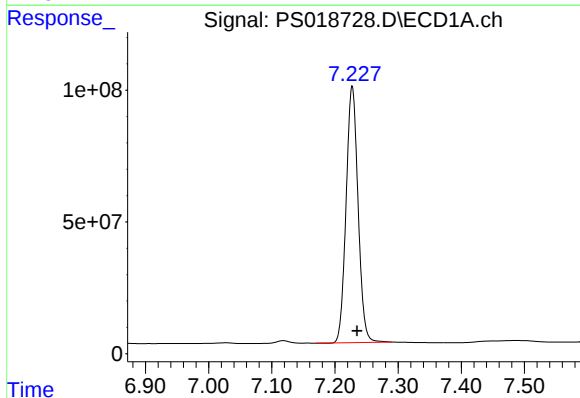


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: -0.008 min
Response: 1279948418
Conc: 449.75 ng/ml

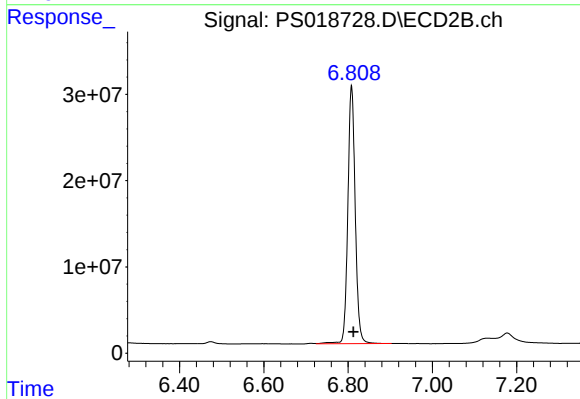

#4 2,4-DCAA


R.T.: 6.808 min
Delta R.T.: -0.005 min
Response: 365503200
Conc: 519.44 ng/ml

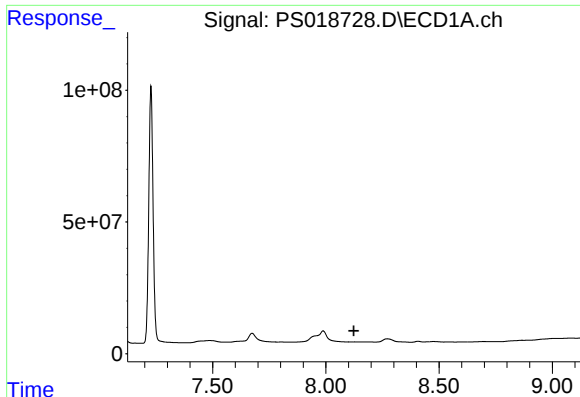

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

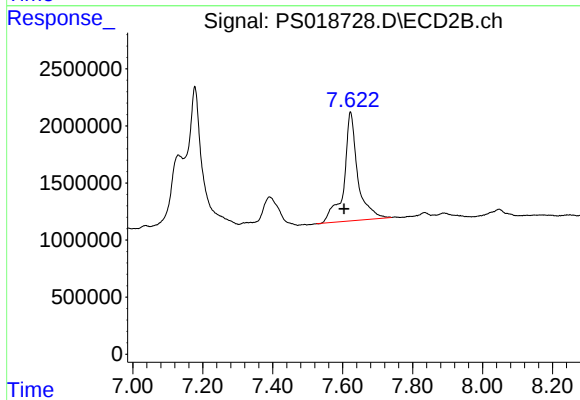


#8 DICHLORPROP

R.T.: 7.622 min
Delta R.T.: 0.018 min
Response: 25907071
Conc: 32.73 ng/ml

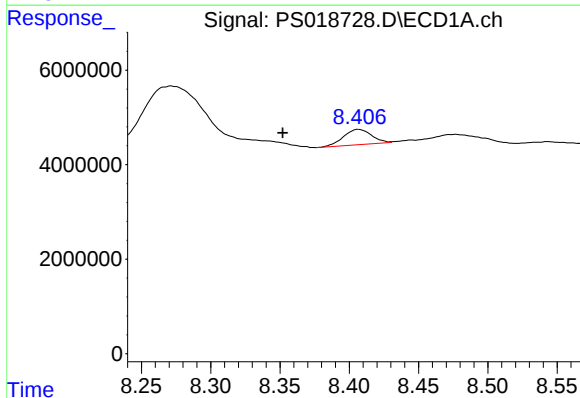


#9 2,4-D

R.T.: 8.406 min
Delta R.T.: 0.054 min
Response: 4567335
Conc: 1.36 ng/ml

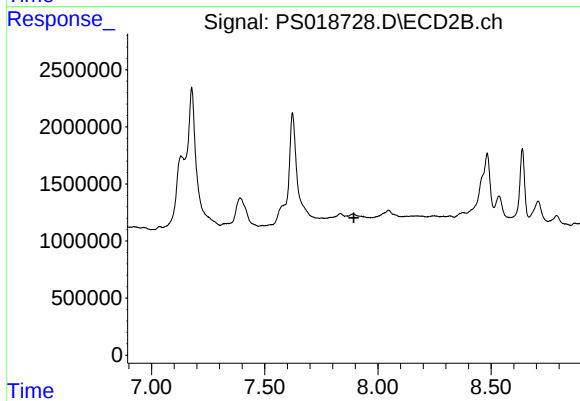

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

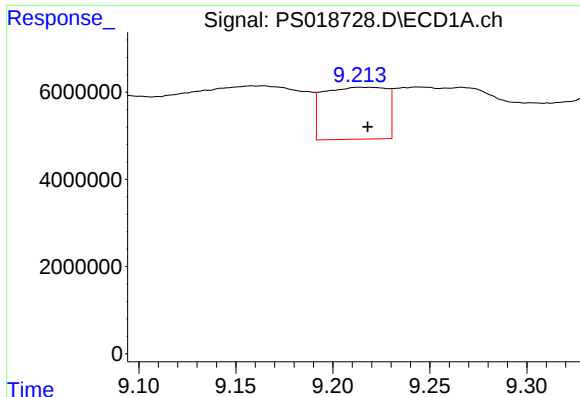

#11 2,4,5-TP (SILVEX)


R.T.: 9.214 min
Delta R.T.: -0.004 min
Response: 26952759
Conc: 1.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

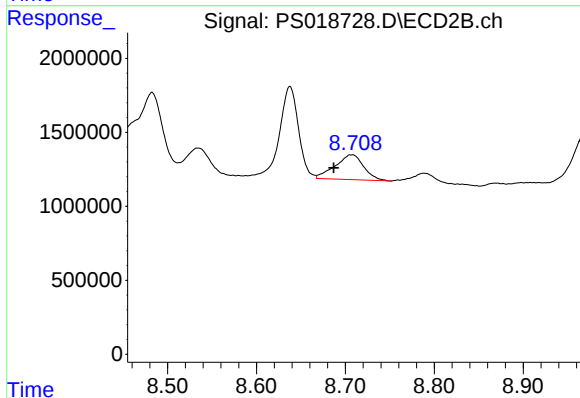


#11 2,4,5-TP (SILVEX)

R.T.: 8.707 min
Delta R.T.: 0.020 min
Response: 3721875
Conc: N.D.

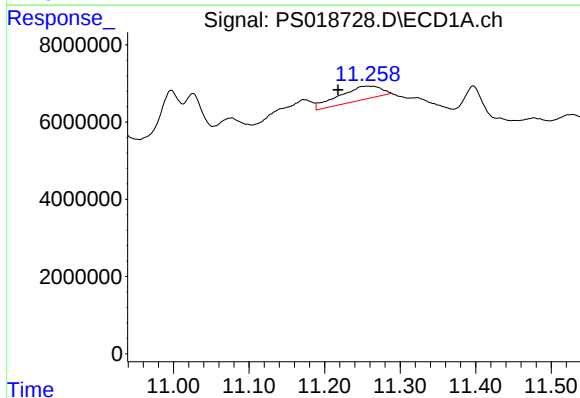


#14 DINOSEB

R.T.: 11.257 min
Delta R.T.: 0.039 min
Response: 13969005
Conc: 1.31 ng/ml

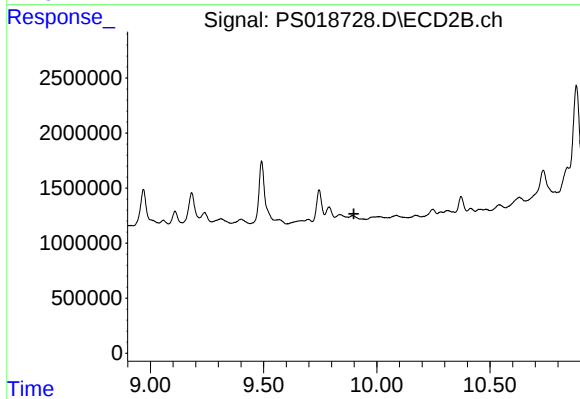

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.899 min
Response: 0
Conc: N.D.

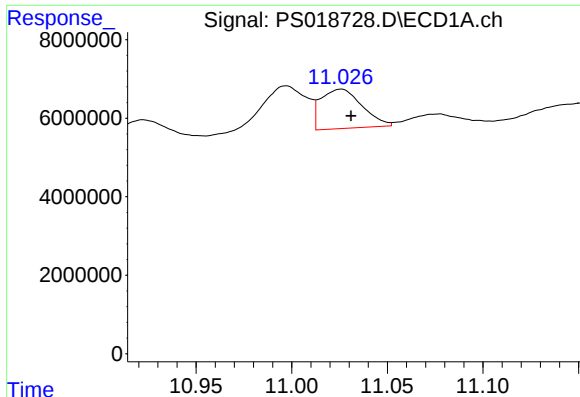

#15 Picloram


R.T.: 11.026 min
Delta R.T.: -0.005 min
Response: 14998553
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

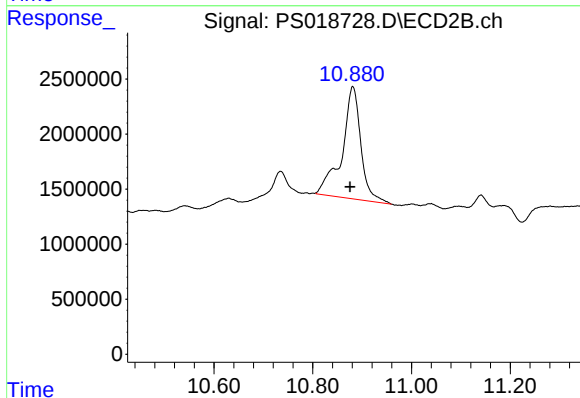


#15 Picloram

R.T.: 10.881 min
Delta R.T.: 0.005 min
Response: 27056250
Conc: 5.09 ng/ml

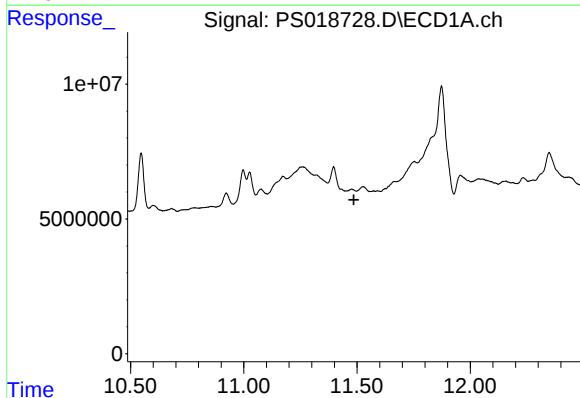

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.486 min
Response: 0
Conc: N.D.

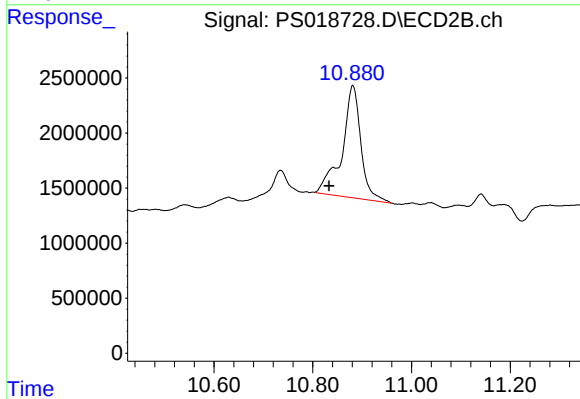

#16 DCPA

R.T.: 10.881 min
Delta R.T.: 0.048 min
Response: 27056250
Conc: 5.14 ng/ml