

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032323\
 Data File : PS022499.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2023 00:28
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 02:01:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.296	6.718	1530.4E6	1439.2E6	626.101	698.742
Target Compounds							
1) T	Dalapon	2.439	2.509	1004010	406059	<MDL	<MDL #
3) T	4-Nitroph...	6.140	0.000	6495052	0	4.740	N.D. #
5) T	DICAMBA	6.432	6.879	11001494	4990268	1.070	<MDL #
6) T	MCP	0.000	6.926f	0	786.6E6	N.D.	101.048
8) T	DICHLORPROP	7.017	7.518	6949865	35548016	2.622	14.276 #
9) T	2,4-D	7.181	7.745f	838.8E6	2192968	255.811	<MDL #
10) T	Pentachlo...	7.441	8.207	30762221	13243075	<MDL	<MDL #
11) T	2,4,5-TP ...	7.974	8.571	23455320	12868830	1.569	<MDL #
12) T	2,4,5-T	8.250	8.961	22759819	4665767	1.386	<MDL #
14) T	DINOSEB	9.768	9.772	9114095	2193754	<MDL	<MDL #
15) T	Picloram	9.592	10.754	97098072	36206085	3.912	1.804 #
16) T	DCPA	10.038	10.700	8139735	49269047	<MDL	3.106 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032323\
Data File : PS022499.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2023 00:28
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 02:01:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

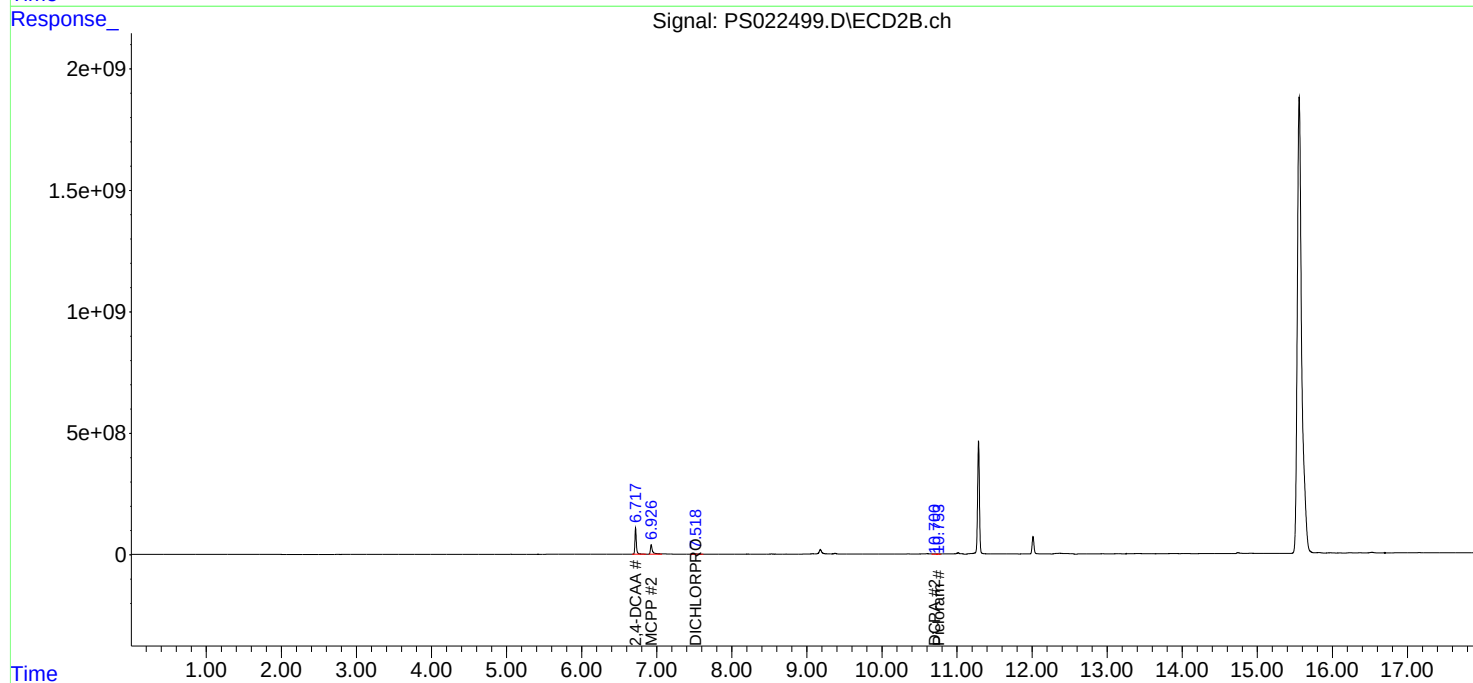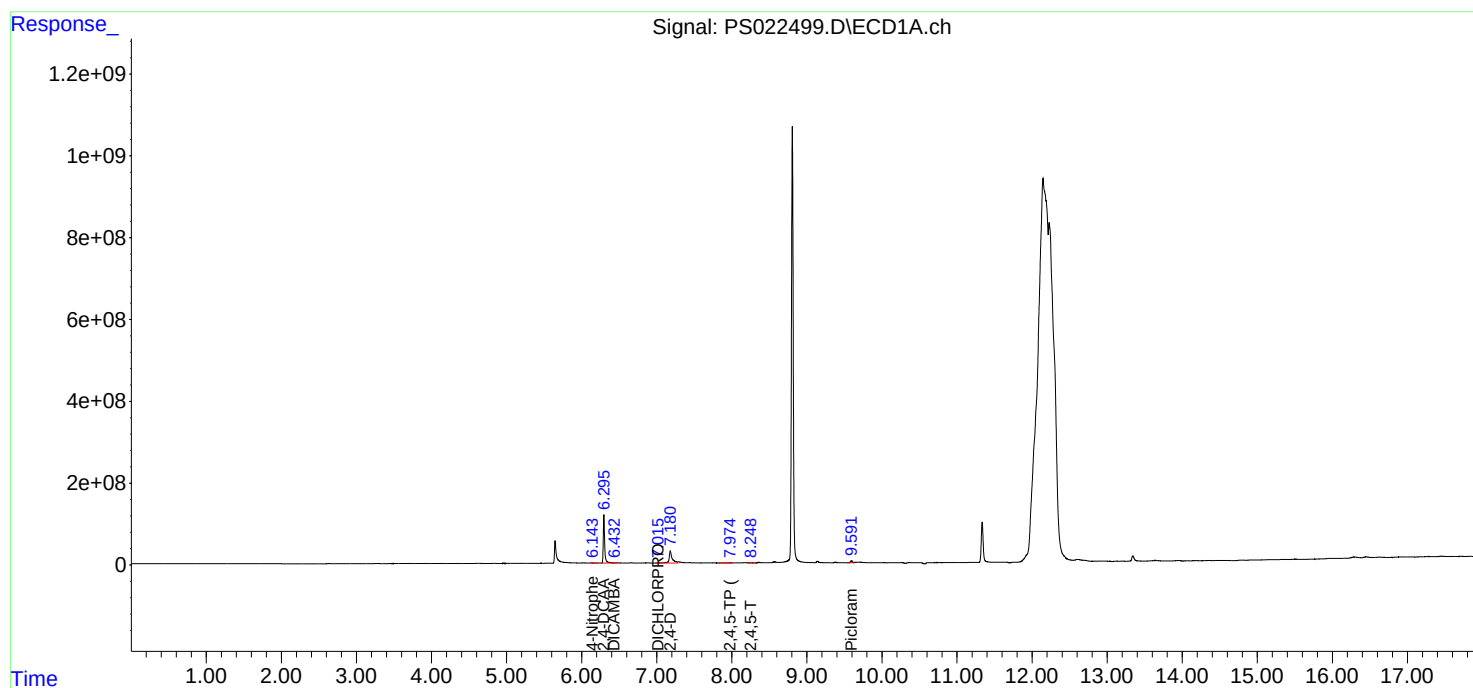


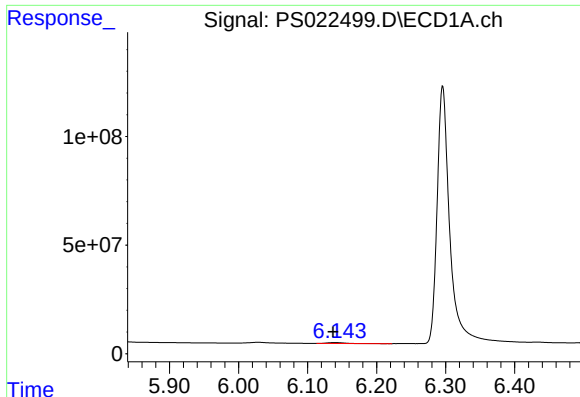

#3 4-Nitrophenol


R.T.: 6.140 min
Delta R.T.: 0.003 min
Response: 6495052
Conc: 4.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

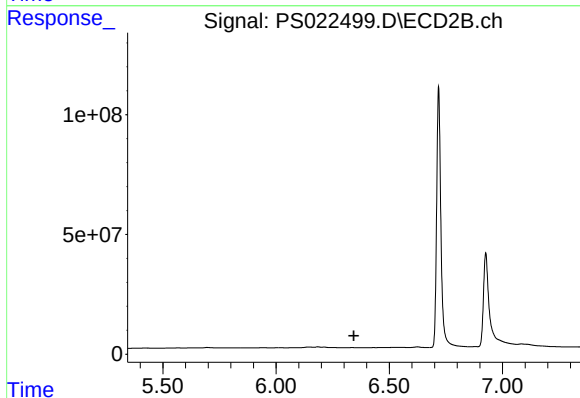


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

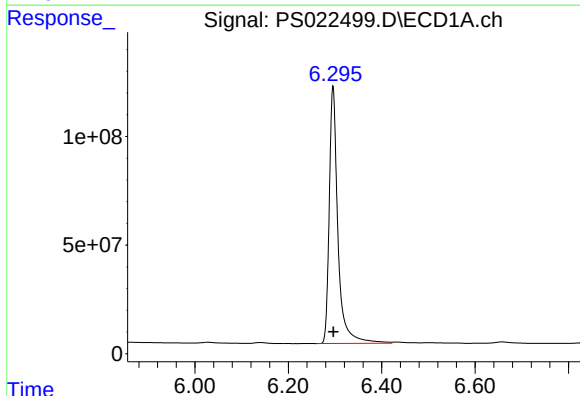


#4 2,4-DCAA

R.T.: 6.296 min
Delta R.T.: 0.000 min
Response: 1530429294
Conc: 626.10 ng/ml

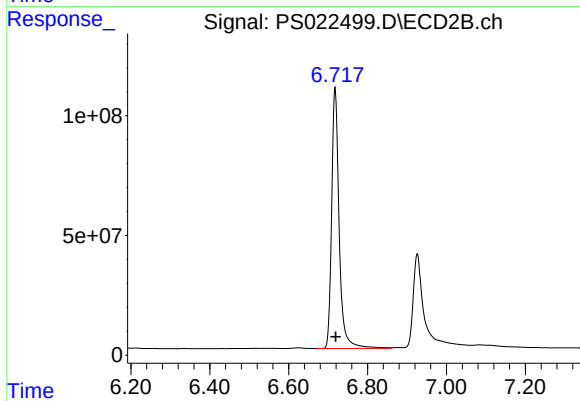

#4 2,4-DCAA


R.T.: 6.718 min
Delta R.T.: -0.002 min
Response: 1439188998
Conc: 698.74 ng/ml

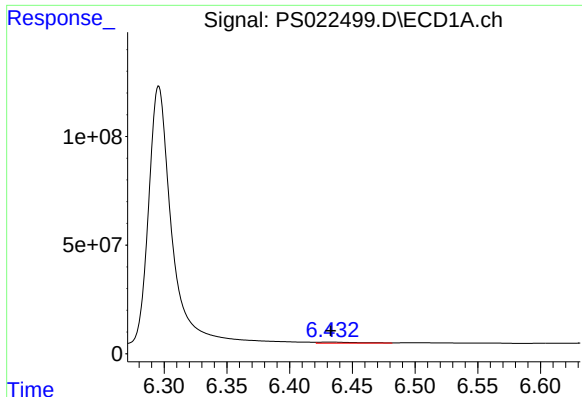

#5 DICAMBA


R.T.: 6.432 min
Delta R.T.: 0.000 min
Response: 11001494
Conc: 1.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

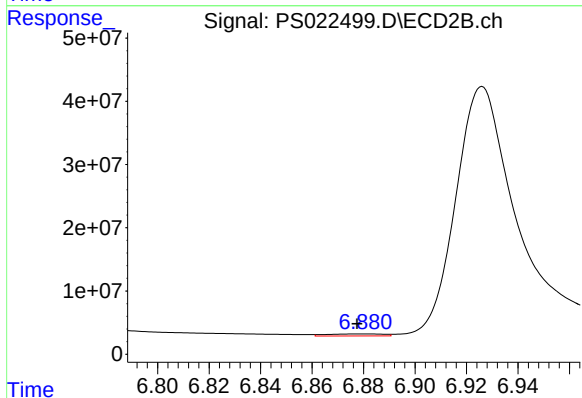


#5 DICAMBA

R.T.: 6.879 min
Delta R.T.: 0.002 min
Response: 4990268
Conc: N.D.

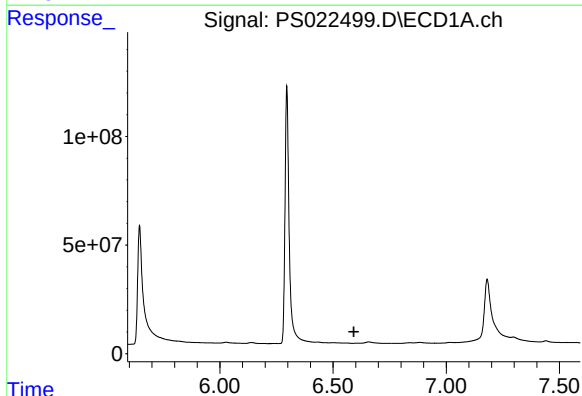


#6 MCP

R.T.: 0.000 min
Exp R.T. : 6.592 min
Response: 0
Conc: N.D.

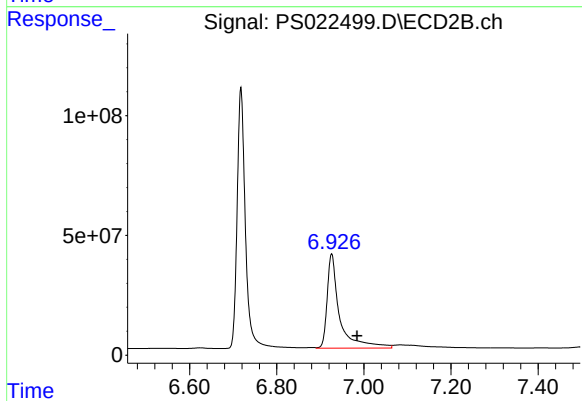

#6 MCP


R.T.: 6.926 min
Delta R.T.: -0.058 min
Response: 786587743
Conc: 101.05 ug/ml

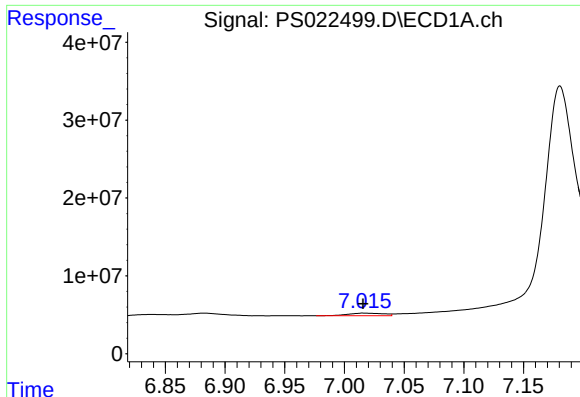

#8 DICHLORPROP


R.T.: 7.017 min
Delta R.T.: 0.001 min
Response: 6949865
Conc: 2.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

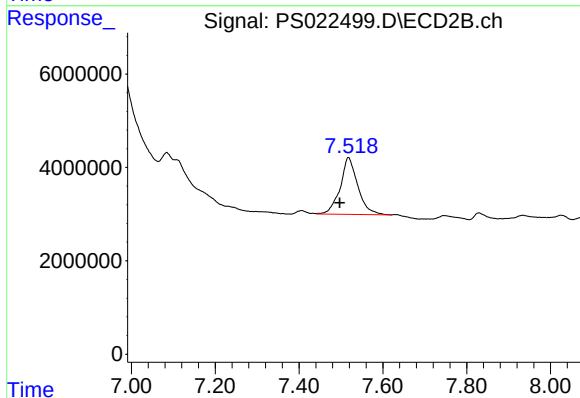


#8 DICHLORPROP

R.T.: 7.518 min
Delta R.T.: 0.021 min
Response: 35548016
Conc: 14.28 ng/ml

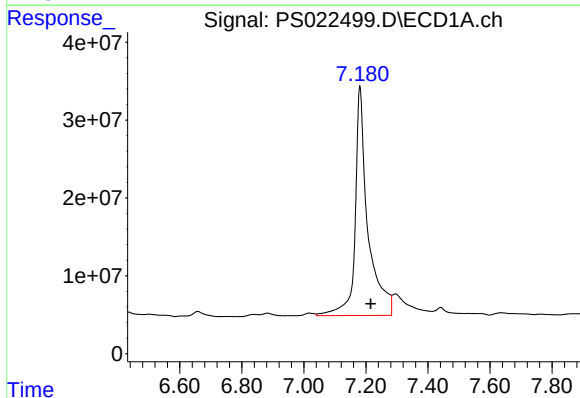


#9 2,4-D

R.T.: 7.181 min
Delta R.T.: -0.034 min
Response: 838806749
Conc: 255.81 ng/ml

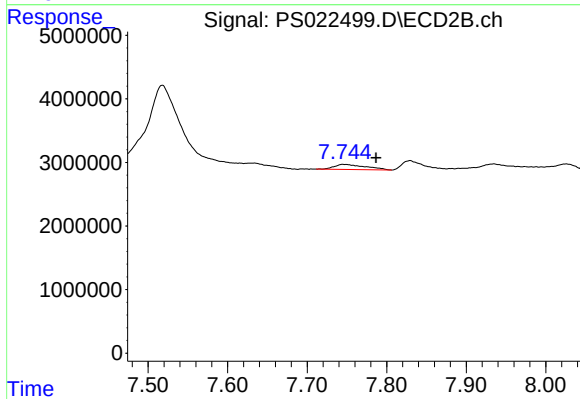

#9 2,4-D


R.T.: 7.745 min
Delta R.T.: -0.042 min
Response: 2192968
Conc: N.D.

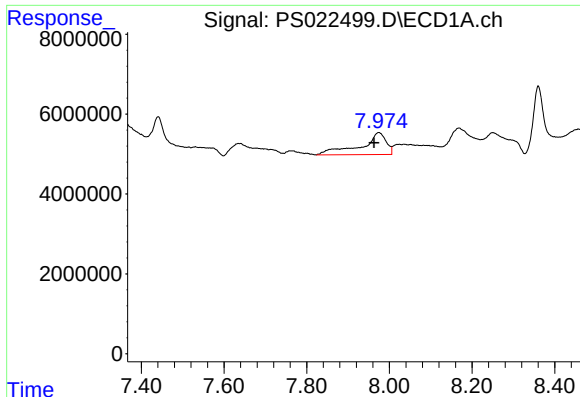

#11 2,4,5-TP (SILVEX)


R.T.: 7.974 min
Delta R.T.: 0.011 min
Response: 23455320
Conc: 1.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

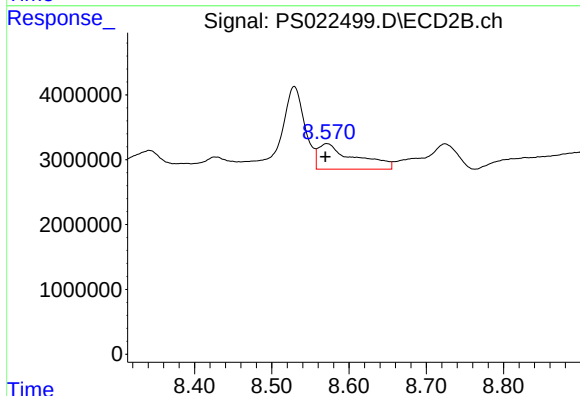


#11 2,4,5-TP (SILVEX)

R.T.: 8.571 min
Delta R.T.: 0.002 min
Response: 12868830
Conc: N.D.

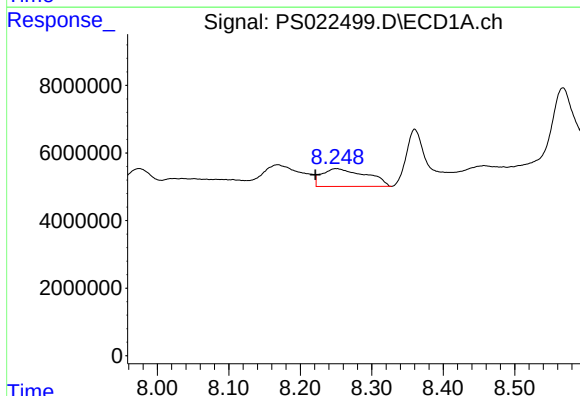


#12 2,4,5-T

R.T.: 8.250 min
Delta R.T.: 0.029 min
Response: 22759819
Conc: 1.39 ng/ml

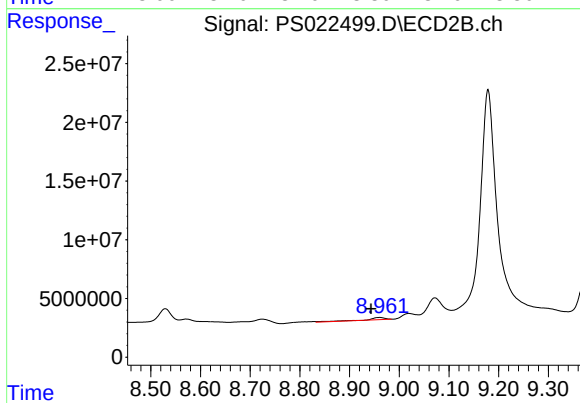

#12 2,4,5-T


R.T.: 8.961 min
Delta R.T.: 0.018 min
Response: 4665767
Conc: N.D.

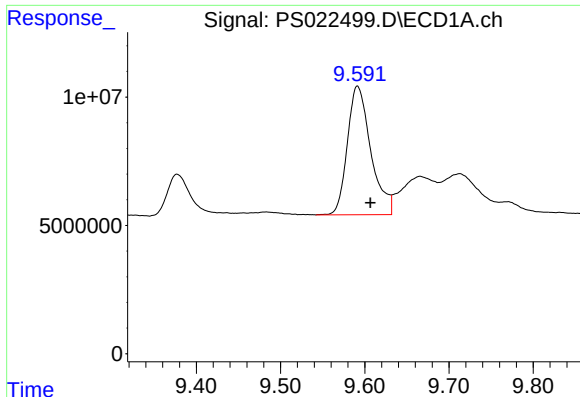

#15 Picloram


R.T.: 9.592 min
Delta R.T.: -0.015 min
Response: 97098072
Conc: 3.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

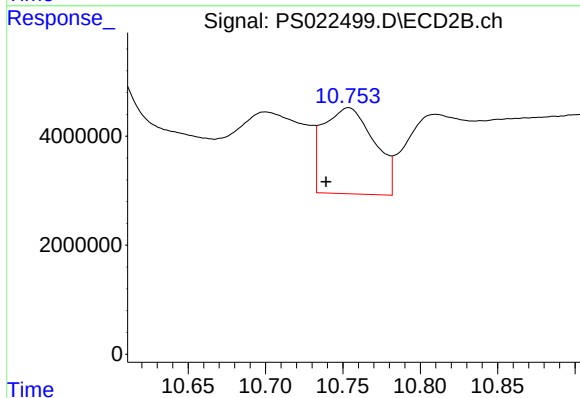


#15 Picloram

R.T.: 10.754 min
Delta R.T.: 0.014 min
Response: 36206085
Conc: 1.80 ng/ml

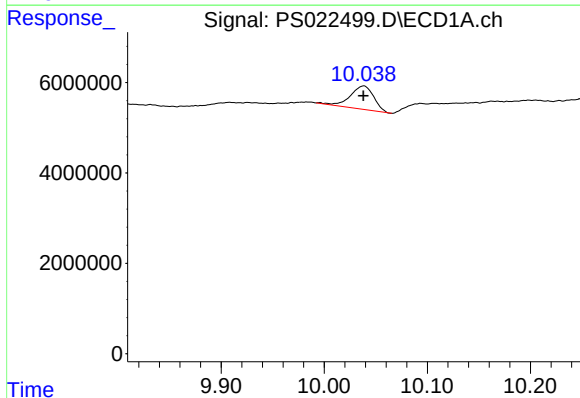

#16 DCPA

R.T.: 10.038 min
Delta R.T.: 0.000 min
Response: 8139735
Conc: N.D.

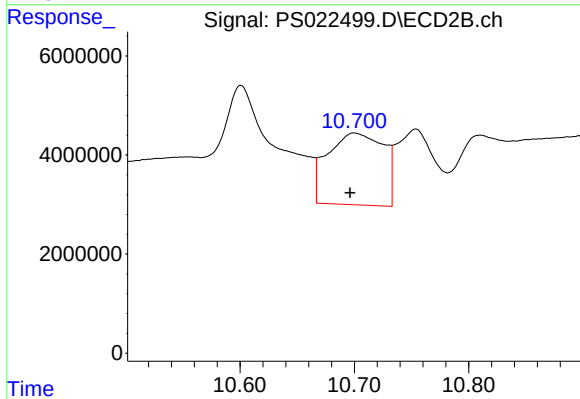

#16 DCPA

R.T.: 10.700 min
Delta R.T.: 0.004 min
Response: 49269047
Conc: 3.11 ng/ml