

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032323\
 Data File : PS022492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2023 21:37
 Operator : AR\AJ
 Sample : 02023-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-11-TEST-PIT-ON-CENTRAL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/24/2023
 Supervised By :Ankita Jodhani 03/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 01:58:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	6.301	6.716	1127.6E6	1068.8E6	461.310m	518.925
------	----------	-------	-------	----------	----------	----------	---------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032323\
Data File : PS022492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2023 21:37
Operator : AR\AJ
Sample : 02023-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-11-TEST-PIT-ON-CENTRAL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/24/2023
Supervised By : Ankita Jodhani 03/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 01:58:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

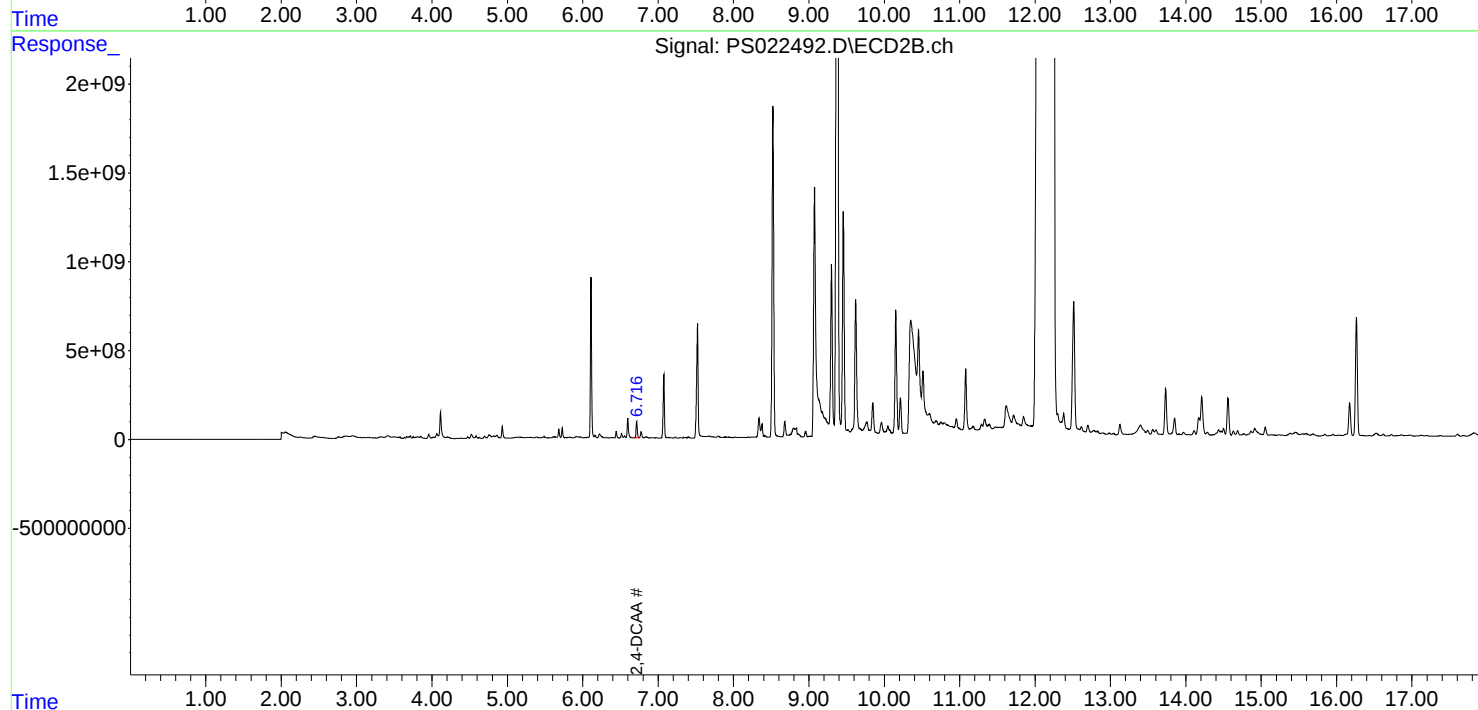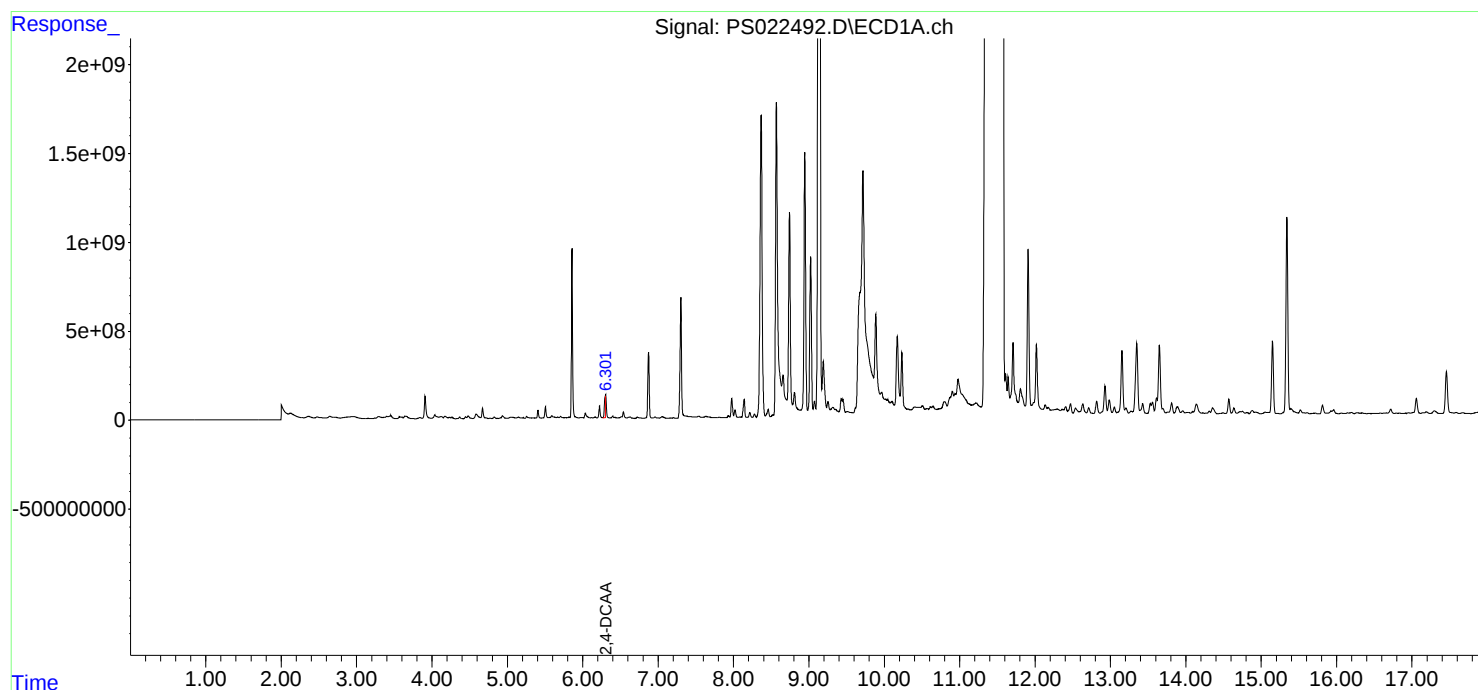

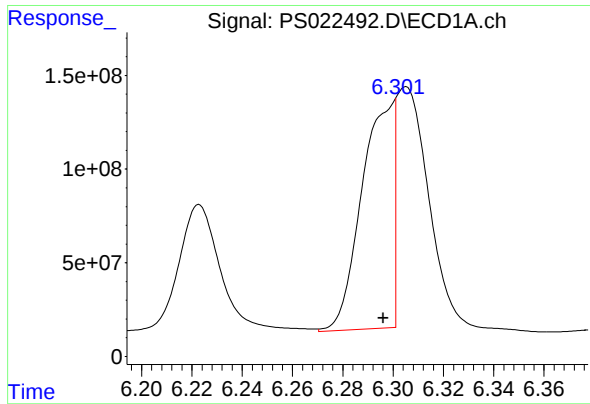


#4 2,4-DCAA

R.T.: 6.301 min
Delta R.T.: 0.005 min
Response: 1127618285
Conc: 461.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-11-TEST-PIT-ON-CENTRAL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/24/2023
Supervised By :Ankita Jodhani 03/24/2023

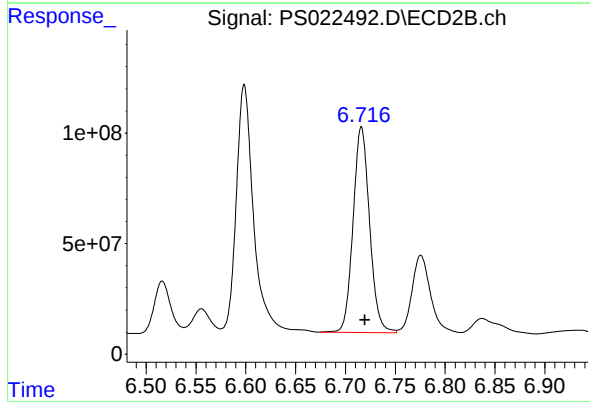

#4 2,4-DCAA

R.T.: 6.716 min
Delta R.T.: -0.003 min
Response: 1068823775
Conc: 518.93 ng/ml