

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032323\
 Data File : PS022494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2023 22:26
 Operator : AR\AJ
 Sample : 02023-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-13-TEST-PIT-ON-GRAVELLY

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/24/2023
 Supervised By :Ankita Jodhani 03/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 01:58:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	6.298	6.716	919.0E6	1048.2E6	375.971m	508.913 #
------	----------	-------	-------	---------	----------	----------	-----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032323\
Data File : PS022494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2023 22:26
Operator : AR\AJ
Sample : 02023-06
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-13-TEST-PIT-ON-GRAVELLY


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/24/2023
Supervised By : Ankita Jodhani 03/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 01:58:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

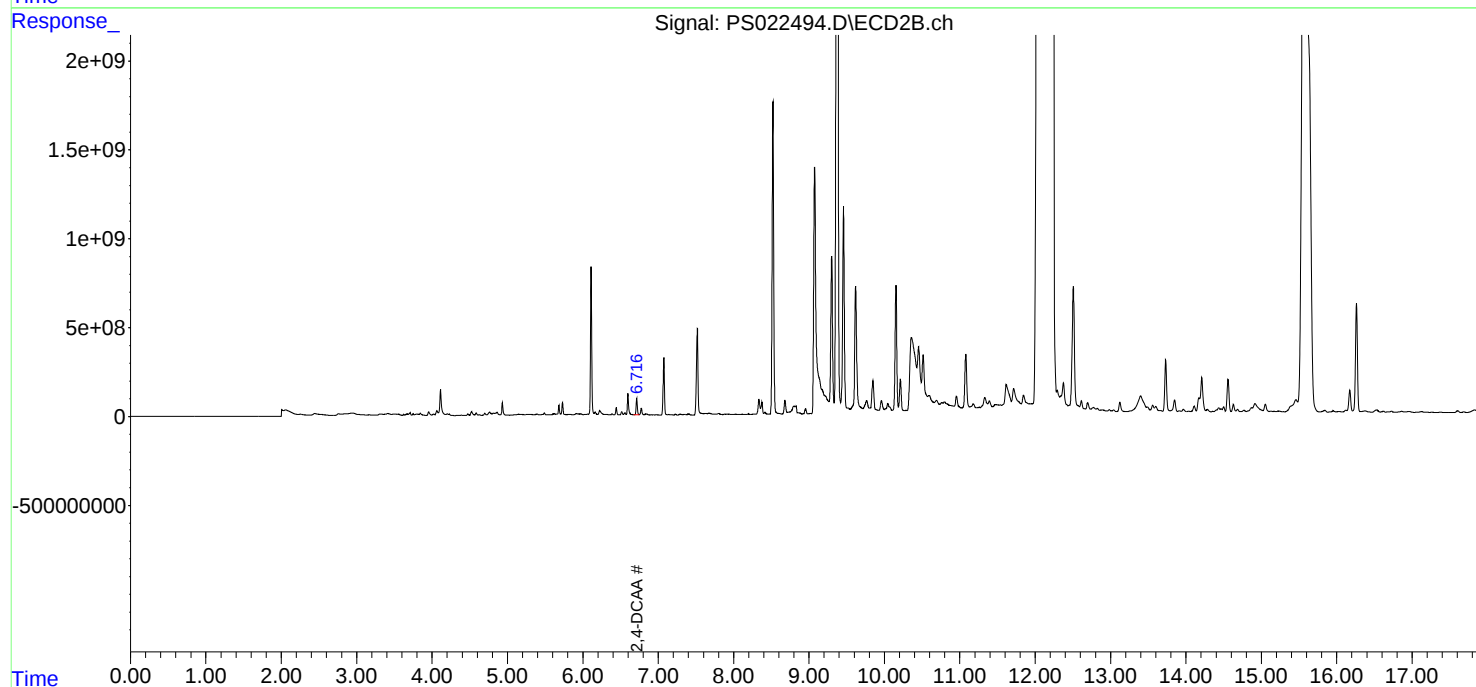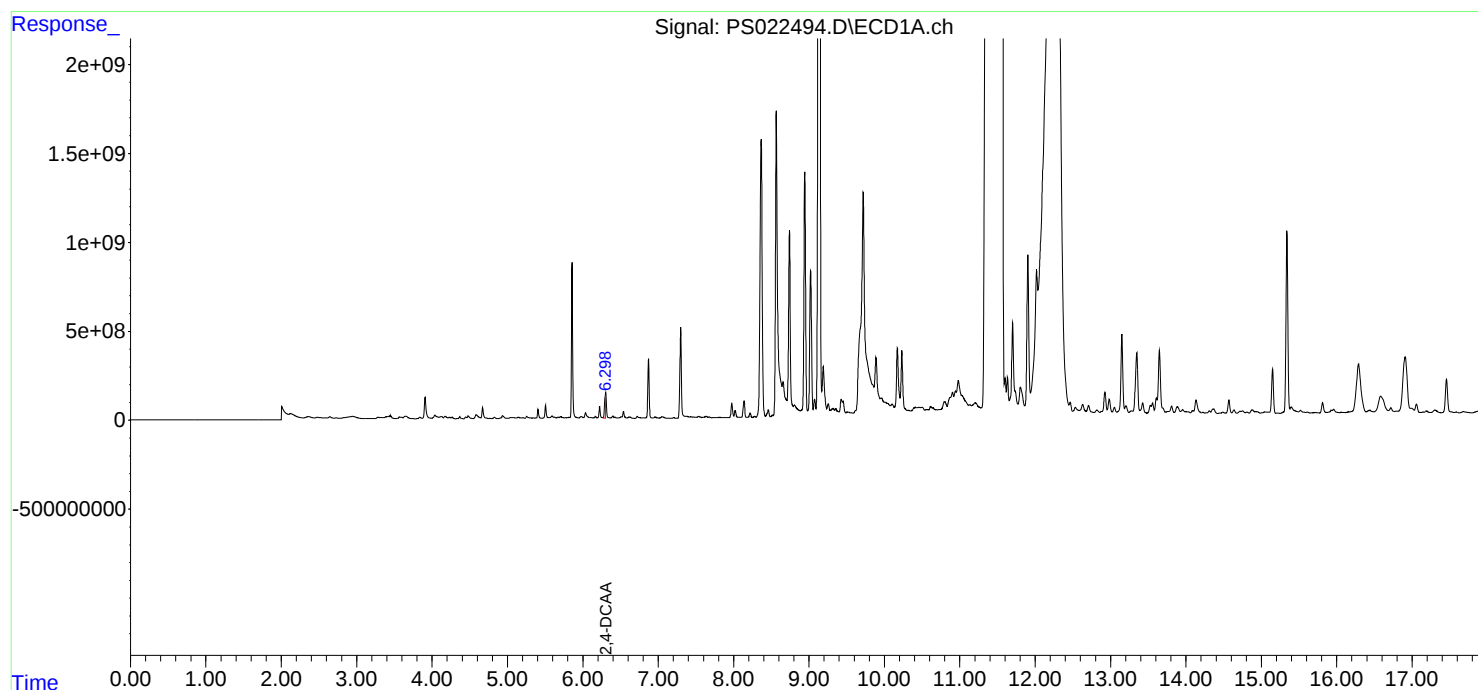

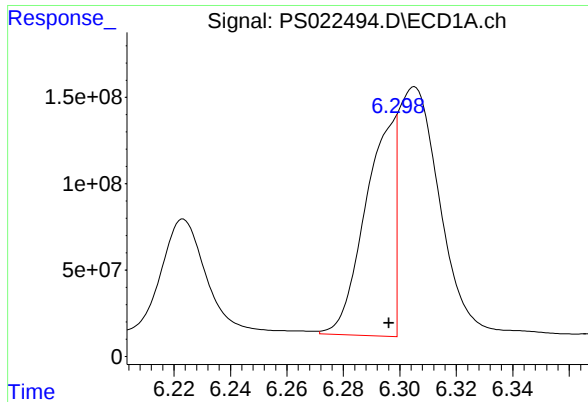


#4 2,4-DCAA

R.T.: 6.298 min
Delta R.T.: 0.002 min
Response: 919015723
Conc: 375.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-13-TEST-PIT-ON-GRAVELLY

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/24/2023
Supervised By :Ankita Jodhani 03/24/2023

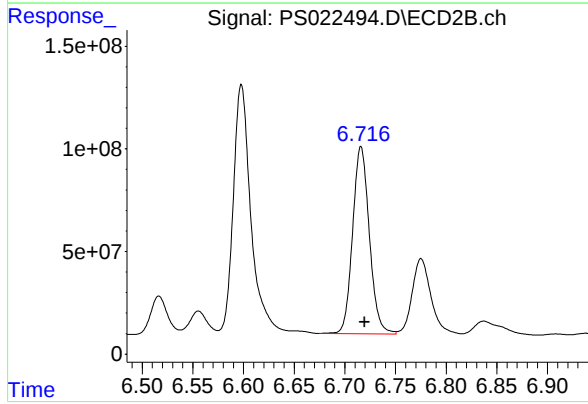

#4 2,4-DCAA

R.T.: 6.716 min
Delta R.T.: -0.003 min
Response: 1048200909
Conc: 508.91 ng/ml