

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
 Data File : PS009415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2020 17:04
 Operator : DD\AJ
 Sample : L2011-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 17:23:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.243	6.932	278.2E6	273.8E6	502.919	498.540
Target Compounds							
1) T	Dalapon	3.007	2.588	17633750	67623101	22.612	85.886 #
2) T	3,5-DICHL...	0.000	6.109	0	35756274	N.D.	43.964
6) T	MCPD	7.597	0.000	7182256	0	2.919	N.D. #
7) T	MCPA	7.793	7.477	61783532	5909513	20.286	2.190 #
8) T	DICHLORPROP	0.000	7.752	0	28520423	N.D.	51.405
12) T	2,4,5-T	9.453	0.000	19322688	0	7.596	N.D. #
14) T	DINOSEB	11.188	10.048	30605681	33363205	14.972	15.189
15) T	Picloram	11.016	11.020	20534150	17699663	6.766	4.346 #
16) T	DCPA	11.551	10.966	10411553	12854545	3.004	3.319



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
Data File : PS009415.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2020 17:04
Operator : DD\AJ
Sample : L2011-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 17:23:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

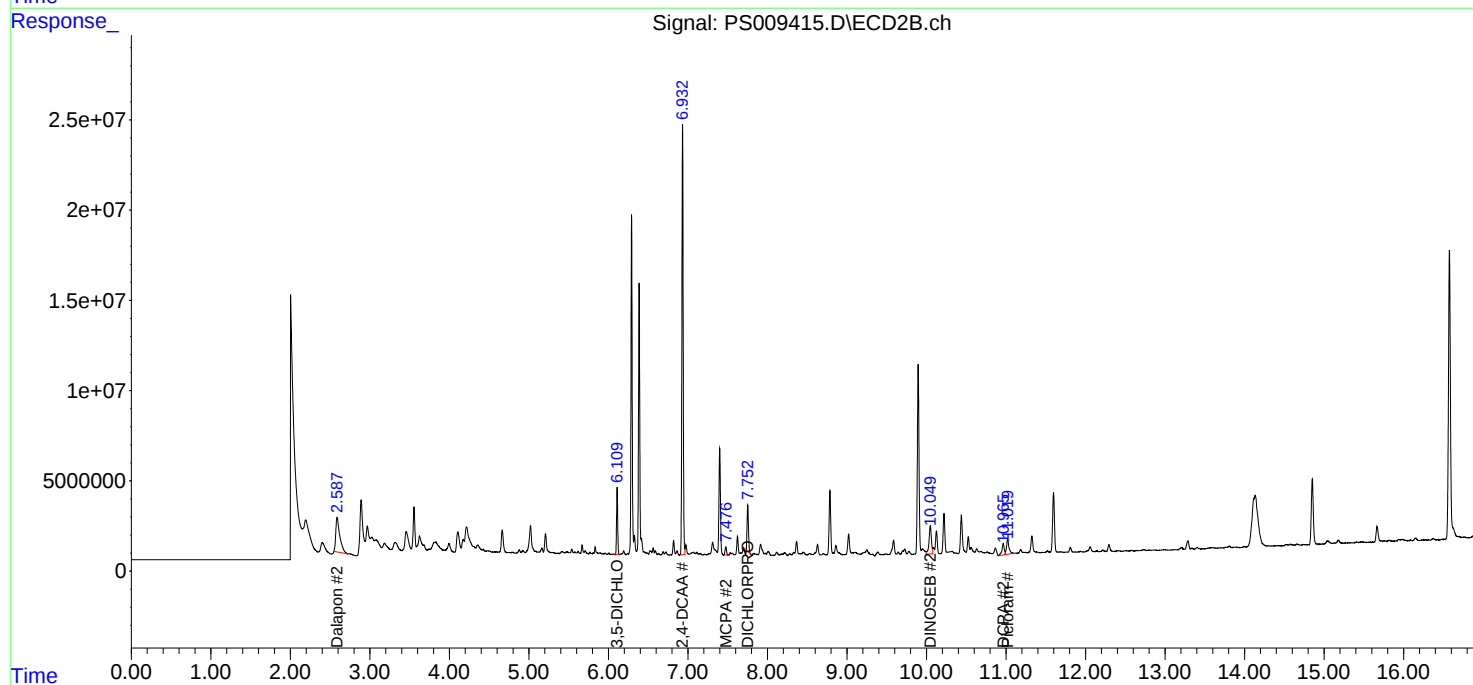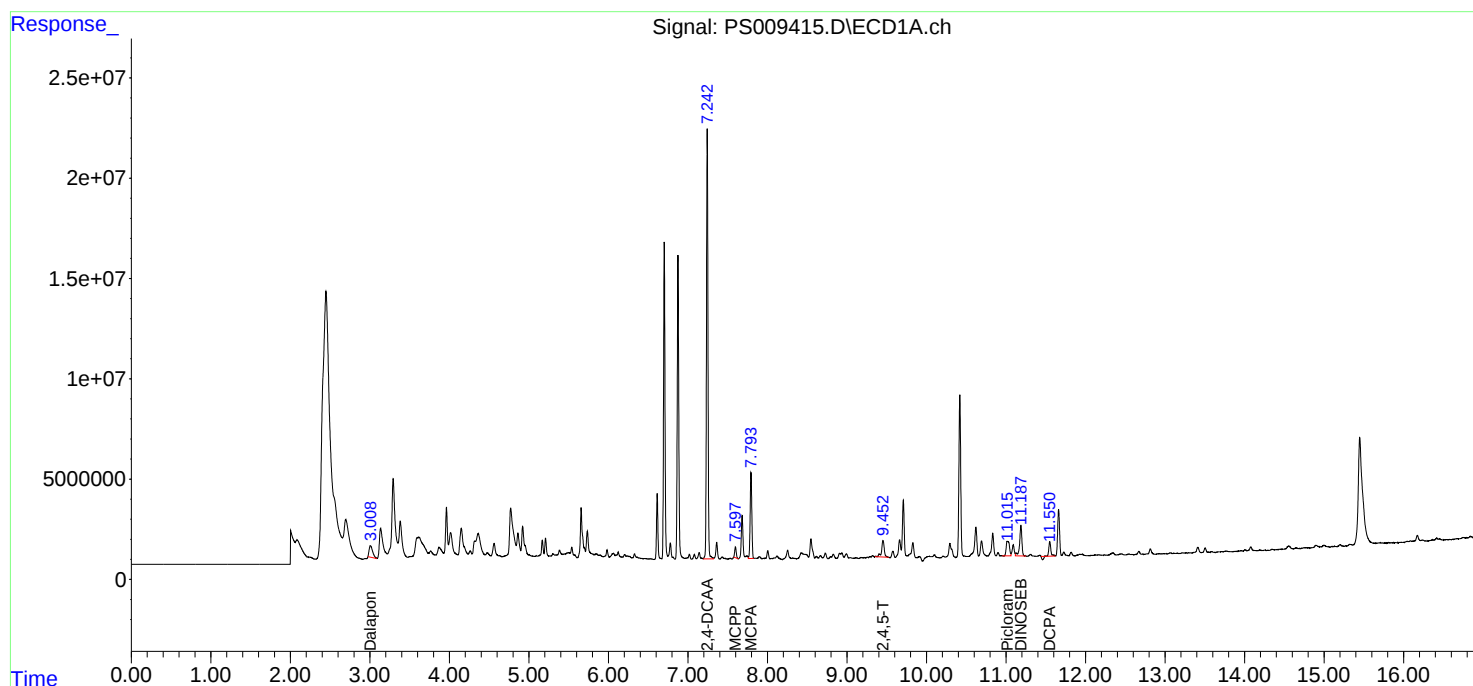


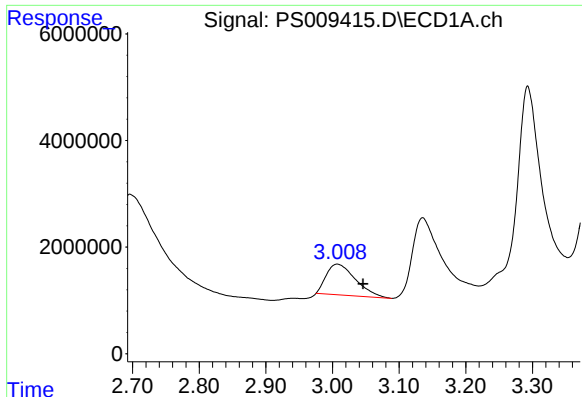

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 17633750
Conc: 22.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

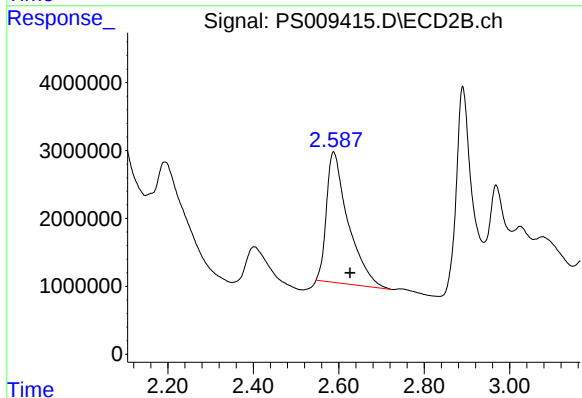


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 67623101
Conc: 85.89 ng/ml

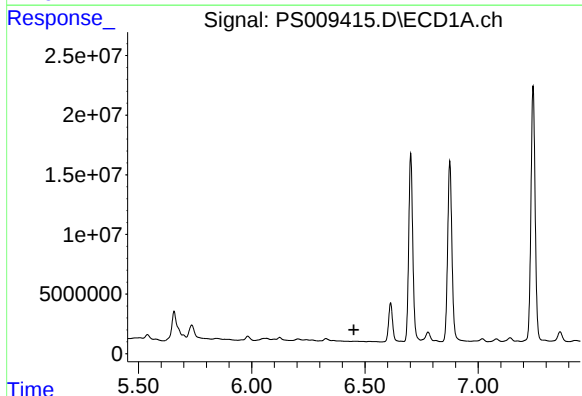


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

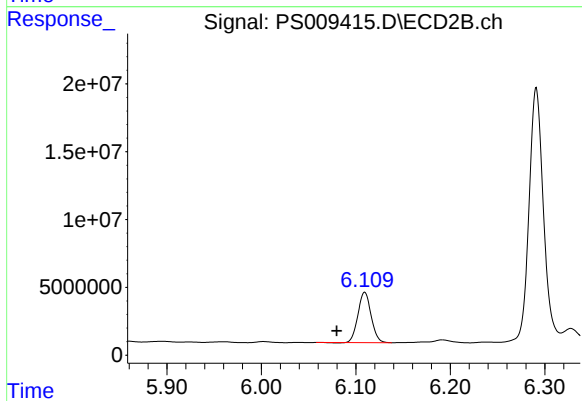

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.030 min
Response: 35756274
Conc: 43.96 ng/ml

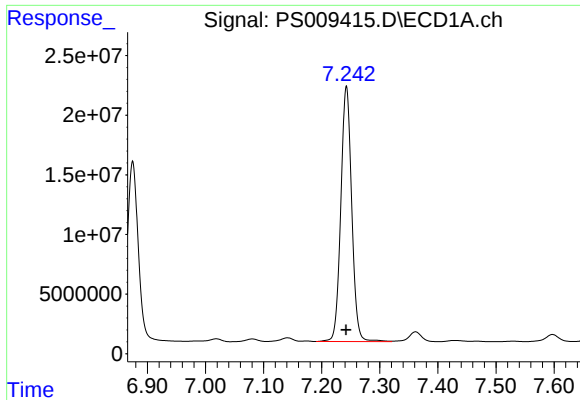

#4 2,4-DCAA


R.T.: 7.243 min
Delta R.T.: 0.000 min
Response: 278199503
Conc: 502.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

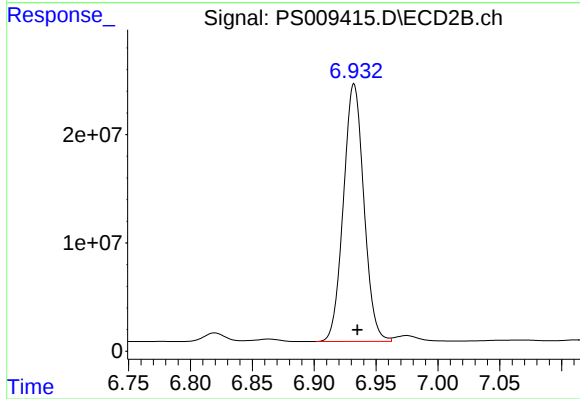


#4 2,4-DCAA

R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 273796778
Conc: 498.54 ng/ml

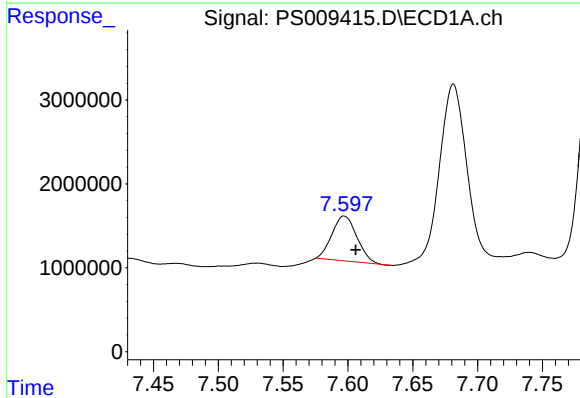


#6 MCP

R.T.: 7.597 min
Delta R.T.: -0.009 min
Response: 7182256
Conc: 2.92 ug/ml

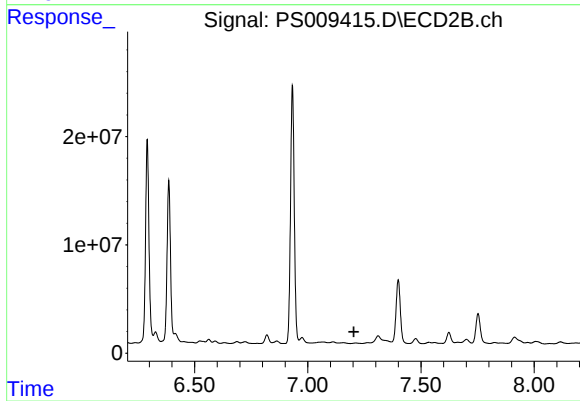

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

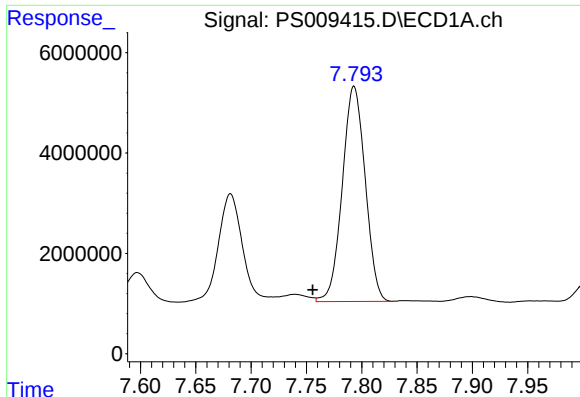

#7 MCPA


R.T.: 7.793 min
Delta R.T.: 0.038 min
Response: 61783532
Conc: 20.29 ug/ml

Instrument :
ECD_S
ClientSampleId :

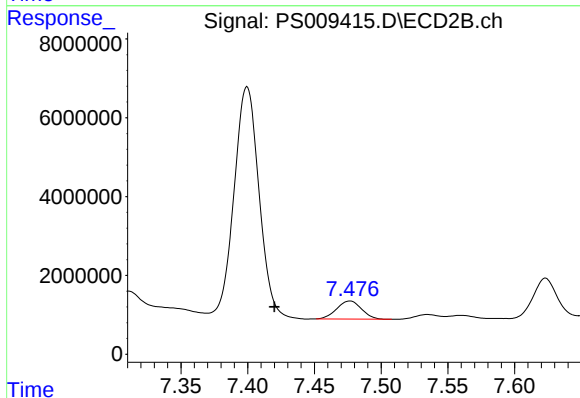


#7 MCPA

R.T.: 7.477 min
Delta R.T.: 0.056 min
Response: 5909513
Conc: 2.19 ug/ml

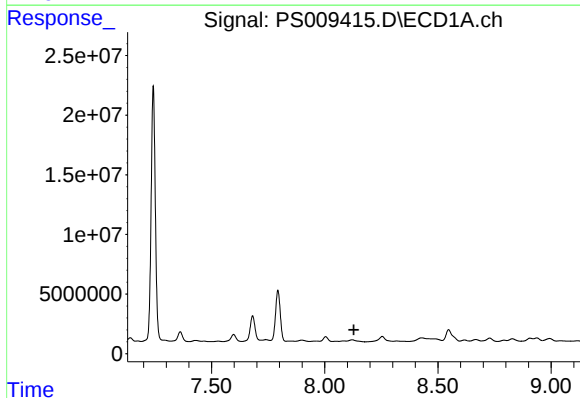


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

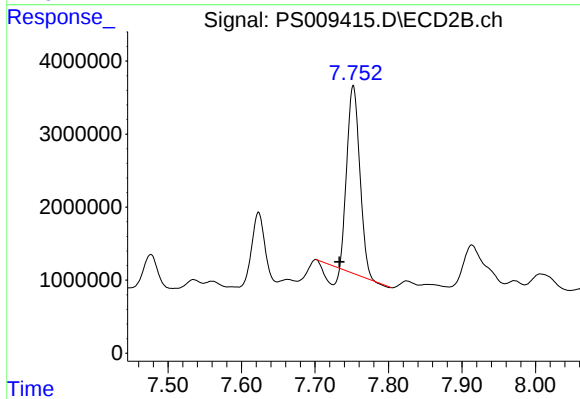

#8 DICHLORPROP


R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 28520423
Conc: 51.40 ng/ml

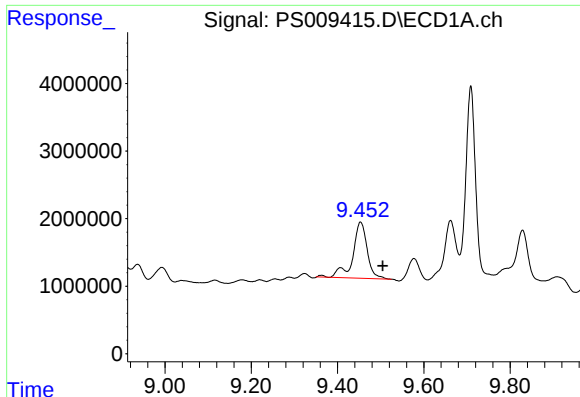

#12 2,4,5-T


R.T.: 9.453 min
Delta R.T.: -0.052 min
Response: 19322688
Conc: 7.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

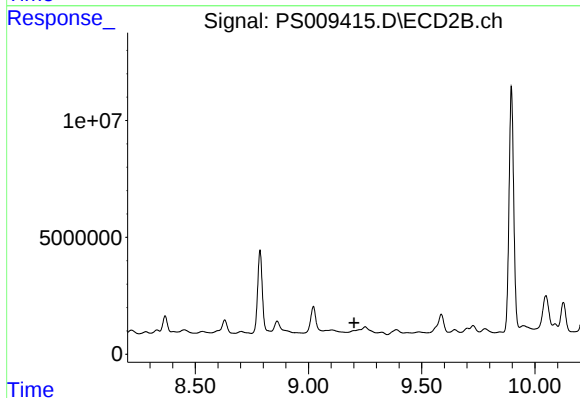


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

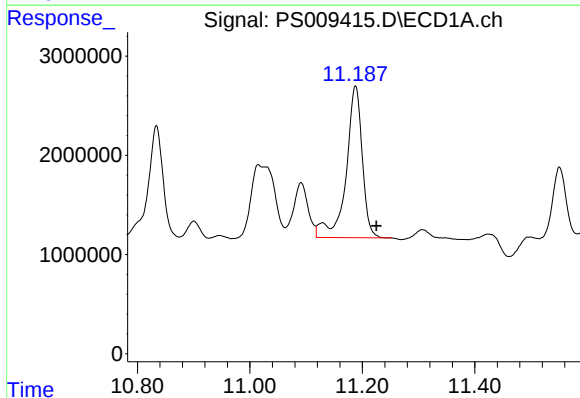


#14 DINOSEB

R.T.: 11.188 min
Delta R.T.: -0.037 min
Response: 30605681
Conc: 14.97 ng/ml

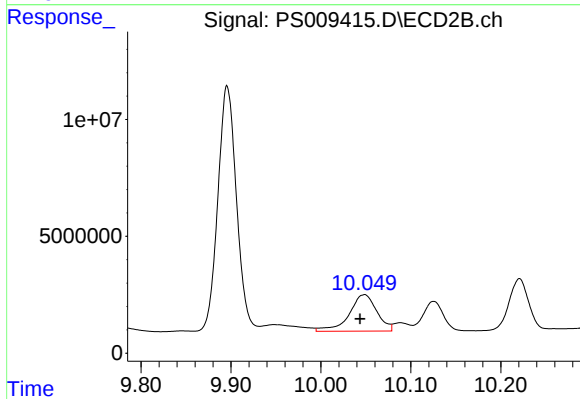

#14 DINOSEB


R.T.: 10.048 min
Delta R.T.: 0.004 min
Response: 33363205
Conc: 15.19 ng/ml

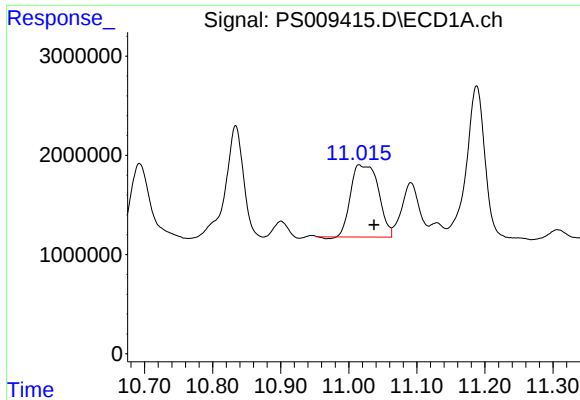

#15 Picloram


R.T.: 11.016 min
Delta R.T.: -0.021 min
Response: 20534150
Conc: 6.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

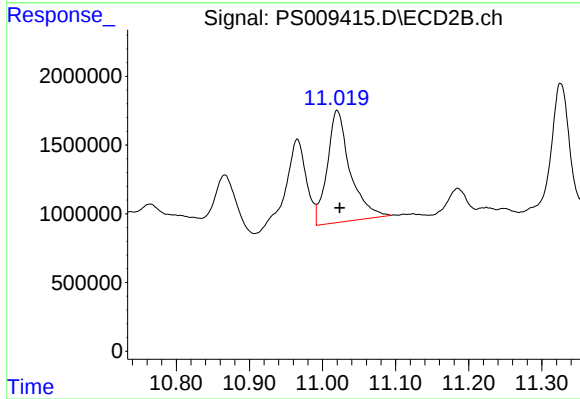


#15 Picloram

R.T.: 11.020 min
Delta R.T.: -0.003 min
Response: 17699663
Conc: 4.35 ng/ml

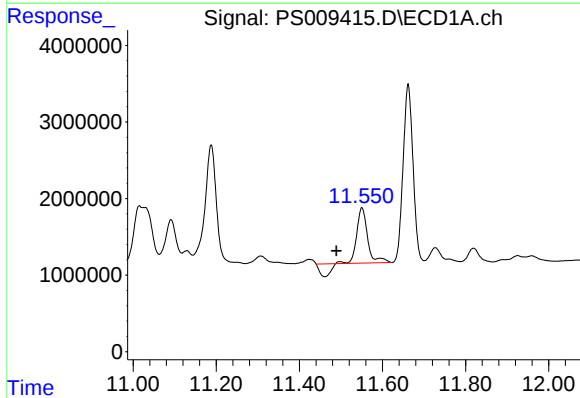

#16 DCPA

R.T.: 11.551 min
Delta R.T.: 0.062 min
Response: 10411553
Conc: 3.00 ng/ml

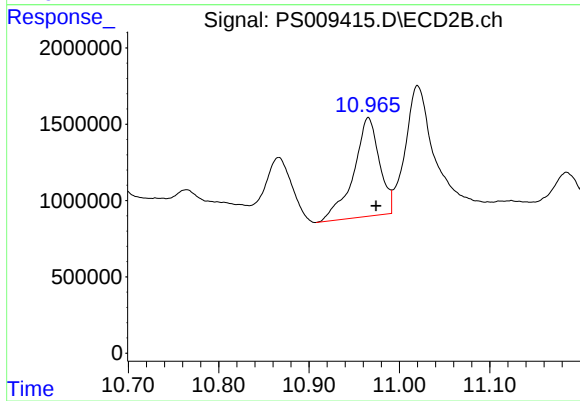

#16 DCPA

R.T.: 10.966 min
Delta R.T.: -0.009 min
Response: 12854545
Conc: 3.32 ng/ml